


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX100820\
 Data File : VX018832.D
 Acq On : 08 Oct 2020 10:19
 Operator : JC/SP
 Sample : BFB80
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB80

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Oct 09 04:43:33 2020

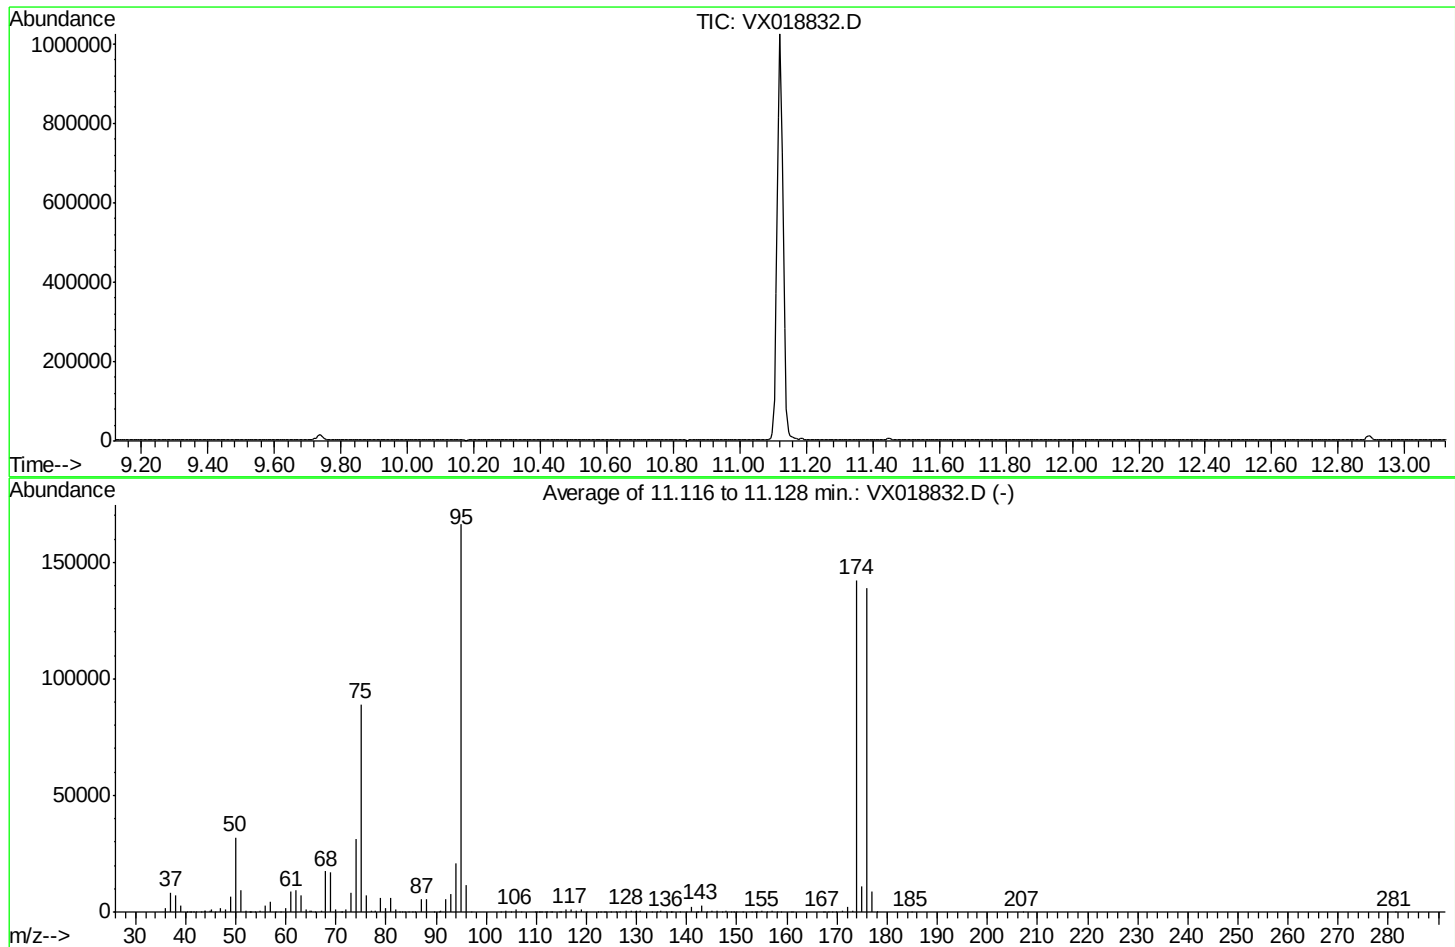

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	31880	PASS
75	95	30	80	53.6	89032	PASS
95	95	100	100	100.0	166229	PASS
96	95	5	9	7.0	11562	PASS
173	174	0.00	2	0.5	728	PASS
174	95	50	120	85.7	142445	PASS
175	174	5	9	7.8	11041	PASS
176	174	95	101	97.4	138717	PASS
177	176	5	9	6.4	8883	PASS

m/z	Abundance
36.10	1595.0
37.00	9476.0
38.00	8292.0
39.00	3520.0
40.20	283.0
40.80	141.0
43.00	159.0
43.90	1659.0
44.90	1759.0
46.00	290.0
47.10	1623.0
48.00	1217.0
49.10	7173.0
50.00	33656.0
51.00	10290.0
52.00	261.0
52.70	336.0
53.90	74.0
54.90	522.0
56.00	2685.0
57.00	4567.0
57.80	290.0
58.90	70.0
60.00	1795.0
61.00	9686.0
62.00	10191.0
63.00	7749.0
64.00	1353.0
64.90	1828.0
66.00	233.0
67.10	536.0
68.00	18032.0
69.00	17656.0
70.00	1368.0
71.20	81.0
72.10	920.0
73.00	8211.0
74.00	31496.0
75.00	89408.0
76.00	7977.0
77.00	1001.0
77.90	764.0
78.90	6523.0
80.00	1671.0
81.00	6388.0
82.00	1407.0
83.10	137.0
83.80	109.0
85.80	299.0
87.00	5894.0
88.00	5600.0
89.70	94.0
90.70	532.0
91.10	749.0
92.00	5819.0
93.00	7993.0
94.00	20904.0
95.00	159424.0
96.10	12137.0
97.10	269.0
102.80	133.0
103.90	729.0
105.10	302.0
106.00	933.0
107.00	174.0
109.80	195.0
111.10	226.0
111.80	188.0
113.00	243.0
114.70	314.0
115.80	875.0
116.90	1374.0
117.90	922.0
118.90	1101.0
120.10	57.0
123.80	97.0
124.90	124.0
125.90	104.0
127.90	600.0
129.00	355.0
129.80	514.0
130.70	285.0
133.00	98.0
134.00	91.0
134.80	328.0
135.80	87.0
136.80	282.0
137.10	285.0
138.70	95.0
140.00	241.0
140.90	2171.0
141.90	346.0

Instrument :
MSVOA_X
ClientSampleId :
BFB80

143.00	3083.0
144.10	182.0
145.00	984.0
146.10	344.0
147.10	71.0
147.90	600.0
148.70	144.0
149.30	80.0
149.90	154.0
151.10	73.0
153.20	85.0
153.90	238.0
155.10	451.0
156.00	67.0
156.90	242.0
158.10	62.0
158.90	134.0
160.80	218.0
167.20	94.0
168.30	104.0
169.10	53.0
171.00	395.0
172.00	2230.0
174.00	123656.0
175.00	10240.0
176.00	113176.0
177.00	8021.0
177.90	225.0
184.80	53.0
207.00	74.0

Instrument :
MSVOA_X
ClientSampleId :
BFB80

Scan 1646 (11.122 min): VX018832.D
BFB80

m/z	Abundance
36.00	1885.0
37.00	9893.0
38.00	8396.0
39.00	3505.0
39.90	424.0
40.90	177.0
41.70	119.0
42.30	69.0
42.80	130.0
43.20	181.0
44.10	1381.0
45.10	1496.0
45.80	167.0
46.20	147.0
46.90	1958.0
48.00	1440.0
49.00	8215.0
50.00	38024.0
51.00	11784.0
52.00	617.0
52.90	211.0
53.80	92.0
55.00	909.0
56.00	2947.0
57.00	5501.0
57.90	291.0
58.90	70.0
60.00	2055.0
61.00	10603.0
62.00	10488.0
63.00	7968.0
63.90	1002.0
65.10	1493.0
65.90	239.0
67.00	644.0
68.00	21168.0
69.00	20680.0
70.10	1712.0
70.90	53.0
72.00	1754.0
73.00	10024.0
74.00	39480.0
75.00	106736.0
76.00	8541.0
77.00	1027.0
77.90	814.0
78.90	7630.0
80.00	1853.0
80.90	6669.0
82.00	1391.0
82.80	171.0
83.80	91.0
85.80	219.0
87.10	6769.0
87.90	6510.0
90.90	893.0
92.00	6330.0
93.00	9500.0
94.00	25960.0
95.00	198912.0
96.00	13104.0
97.00	245.0
102.90	100.0
103.90	1053.0
105.10	269.0
105.90	1127.0
106.90	209.0
110.00	221.0
110.60	200.0
111.80	208.0
112.80	235.0
115.00	356.0
115.80	992.0
116.90	1708.0
117.90	945.0
119.00	1310.0
122.20	124.0
123.90	235.0
124.90	84.0
126.00	130.0
126.70	127.0
128.00	1029.0
128.80	383.0
130.00	702.0
130.80	438.0
133.00	69.0
134.10	83.0
134.80	511.0
135.90	96.0
137.00	444.0
138.60	149.0
140.00	179.0

Instrument :
MSVOA_X
ClientSampleId :
BFB80

141.00	2834.0
141.90	266.0
142.90	3509.0
144.00	167.0
144.90	678.0
146.10	447.0
147.00	170.0
147.90	569.0
148.80	242.0
150.00	350.0
153.00	150.0
153.70	189.0
154.90	588.0
156.10	124.0
157.00	458.0
158.00	119.0
159.00	285.0
160.70	271.0
161.20	346.0
167.60	52.0
168.30	124.0
169.10	103.0
169.80	132.0
171.10	472.0
172.10	2428.0
173.10	2184.0
174.00	169600.0
175.00	12559.0
176.00	167552.0
177.00	11062.0
178.10	264.0
207.30	80.0

Instrument :
MSVOA_X
ClientSampleId :
BFB80

m/z	Abundance
36.00	1250.0
37.00	6134.0
38.10	4685.0
39.00	2072.0
39.90	373.0
41.10	178.0
42.00	93.0
42.80	63.0
43.20	89.0
44.00	1040.0
45.10	1295.0
46.20	220.0
47.00	1300.0
48.00	763.0
49.00	4995.0
50.00	23960.0
51.00	6341.0
52.00	278.0
53.10	232.0
54.00	72.0
55.00	369.0
55.90	2262.0
57.00	3307.0
58.00	140.0
58.80	87.0
60.00	1430.0
61.00	6146.0
62.00	6619.0
63.00	5186.0
64.00	938.0
65.00	906.0
65.90	145.0
66.90	437.0
68.00	13042.0
69.00	13013.0
70.00	984.0
71.90	1089.0
73.00	5963.0
74.00	22400.0
75.00	70952.0
76.00	5753.0
77.10	411.0
77.80	498.0
78.90	4827.0
79.90	1255.0
80.90	4641.0
81.90	982.0
83.10	125.0
84.40	62.0
85.20	54.0
85.80	152.0
87.00	4635.0
87.90	4863.0
89.70	58.0
90.90	797.0
92.00	3768.0
93.00	6362.0
94.00	16344.0
95.00	140352.0
96.00	9445.0
97.10	130.0
102.90	137.0
103.90	729.0
104.90	313.0
106.00	684.0
106.80	257.0
109.70	143.0
110.80	167.0
112.10	118.0
112.70	116.0
113.10	103.0
114.90	181.0
115.90	787.0
117.00	914.0
118.00	589.0
118.90	1183.0
122.20	105.0
122.80	56.0
123.50	62.0
124.00	111.0
124.90	97.0
125.90	135.0
126.70	85.0
127.90	550.0
128.90	373.0
130.00	480.0
130.80	240.0
133.10	74.0
134.10	99.0
134.80	430.0
136.00	149.0
136.90	327.0

Instrument :
MSVOA_X
ClientSampleId :
BFB80

138.60	73.0
139.80	171.0
140.90	1692.0
142.10	321.0
142.90	2192.0
144.00	139.0
145.00	526.0
145.90	265.0
147.00	177.0
147.80	501.0
148.90	155.0
150.00	317.0
153.00	116.0
153.70	87.0
154.00	71.0
155.00	531.0
156.10	56.0
156.90	465.0
158.00	81.0
158.80	396.0
161.00	256.0
167.60	108.0
169.20	123.0
169.80	177.0
171.20	302.0
172.10	1497.0
174.00	134080.0
175.00	10324.0
176.00	135424.0
177.00	7566.0
178.10	152.0
207.30	110.0
281.40	133.0

Instrument :
MSVOA_X
ClientSampleId :
BFB80

m/z	Abundance
35.90	61.0
36.60	157.0
37.40	69.0
37.90	59.0
38.50	144.0
39.00	283.0
40.00	285.0
40.70	89.0
42.20	75.0
43.00	119.0
44.00	450.0
44.80	57.0
45.20	52.0
46.20	133.0
50.80	54.0
55.00	57.0
57.00	68.0
59.50	60.0
60.20	53.0
61.00	167.0
62.80	87.0
66.20	62.0
67.80	72.0
79.20	60.0
95.80	55.0
124.30	53.0
207.30	67.0
269.10	62.0

Instrument :
MSVOA_X
ClientSampleId :
BFB80