

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100821\
 Data File : VX024691.D
 Acq On : 09 Oct 2021 00:35
 Operator : JC/MD
 Sample : M4096-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MWHR2-9-100521

Quant Time: Oct 11 06:37:28 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
 Quant Title : SW846 8260
 QLast Update : Thu Sep 23 18:24:34 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	150206	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	259810	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	256217	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	115419	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	109643	51.792	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	103.580%
35) Dibromofluoromethane	5.397	113	86905	50.351	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	100.700%
50) Toluene-d8	8.653	98	318908	50.202	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	100.400%
62) 4-Bromofluorobenzene	11.085	95	120398	48.204	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	96.400%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100821\
Data File : VX024691.D
Acq On : 09 Oct 2021 00:35
Operator : JC/MD
Sample : M4096-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MWHR2-9-100521

Quant Time: Oct 11 06:37:28 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260
QLast Update : Thu Sep 23 18:24:34 2021
Response via : Initial Calibration

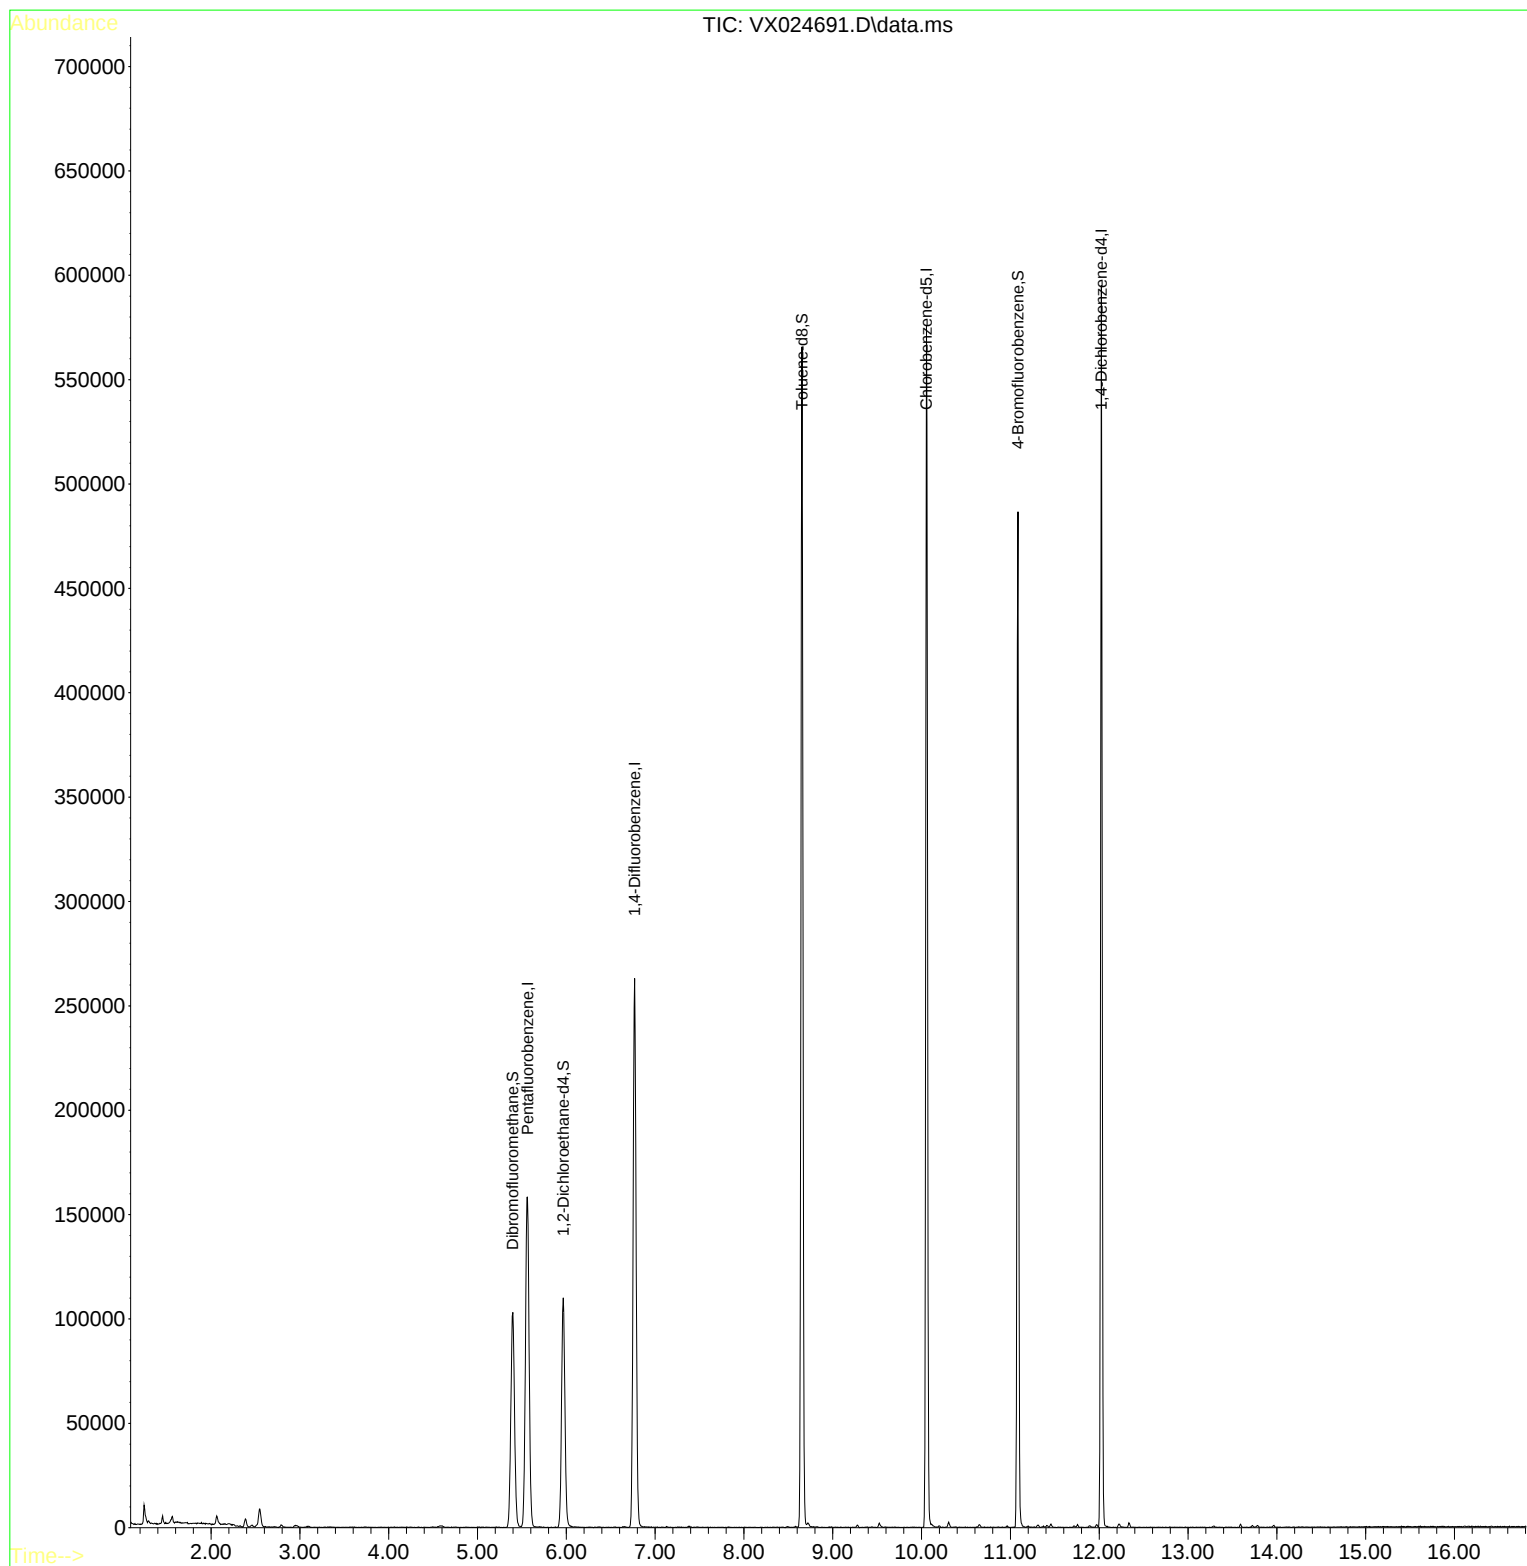

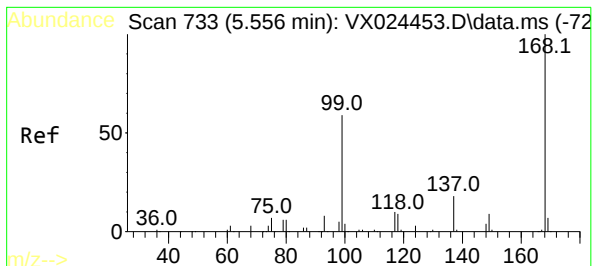

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.562 min Scan# 734

Delta R.T. 0.006 min

Lab File: VX024691.D





Acq: 09 Oct 2021 00:35

Tgt Ion:168 Resp: 150206

Ion Ratio Lower Upper

168 100

99 59.8 45.8 68.6

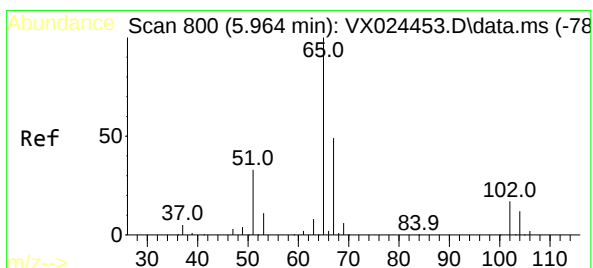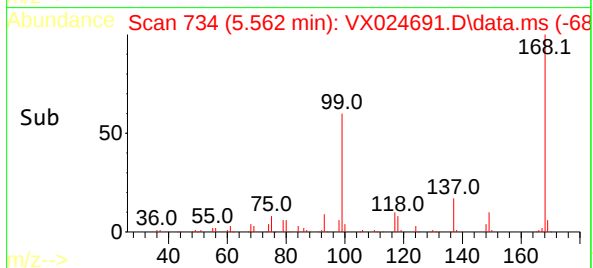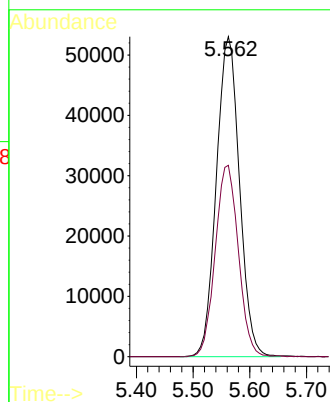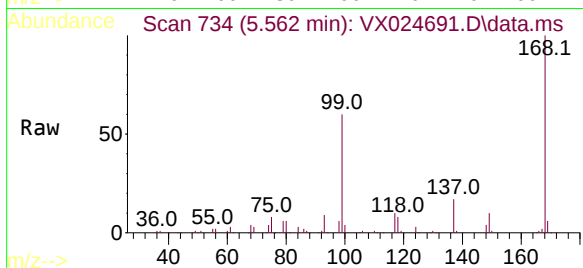

#33

1,2-Dichloroethane-d4

Concen: 51.792 ug/l

RT: 5.964 min Scan# 800

Delta R.T. 0.000 min

Lab File: VX024691.D




Acq: 09 Oct 2021 00:35


Tgt Ion: 65 Resp: 109643

Ion Ratio Lower Upper

65 100

67 50.2 0.0 105.4


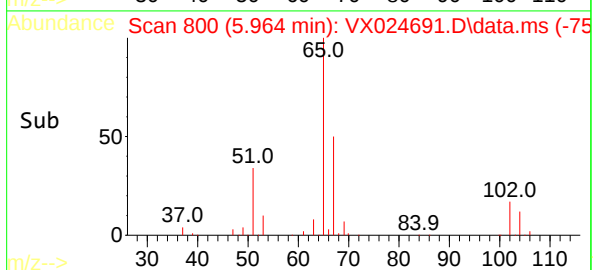
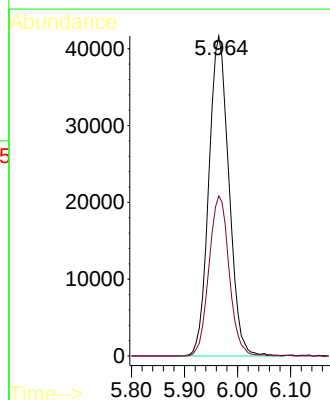
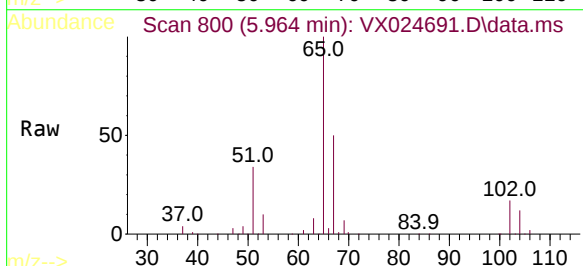


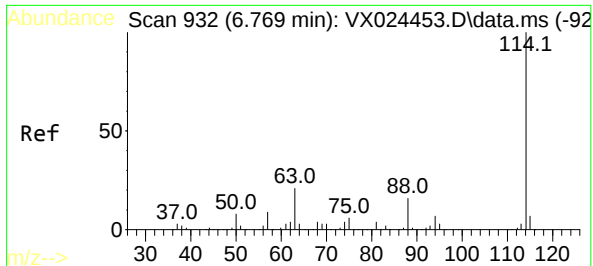

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. 0.000 min
Lab File: VX024691.D
Acq: 09 Oct 2021 00:35




Instrument :
MSVOA_X
ClientSampleId :
MWHHR2-9-100521


Tgt Ion:114 Resp: 259810
Ion Ratio Lower Upper
114 100
63 21.1 0.0 40.8
88 16.6 0.0 32.8

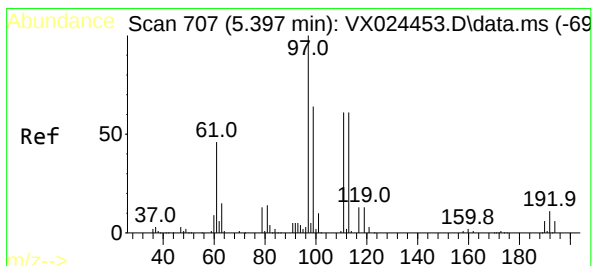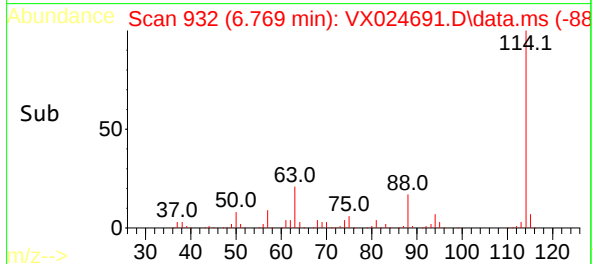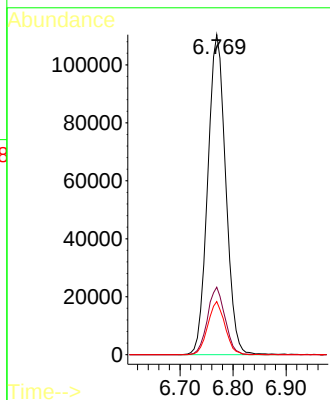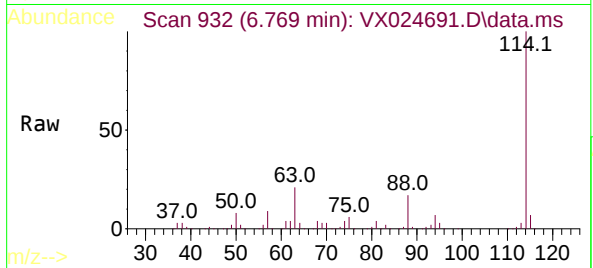

#35
Dibromofluoromethane
Concen: 50.351 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.000 min
Lab File: VX024691.D
Acq: 09 Oct 2021 00:35

Tgt Ion:113 Resp: 86905
Ion Ratio Lower Upper
113 100
111 102.0 81.9 122.9
192 20.2 16.7 25.1


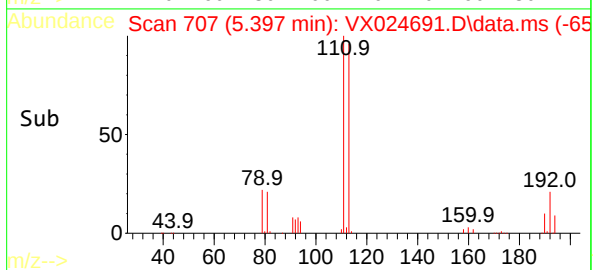
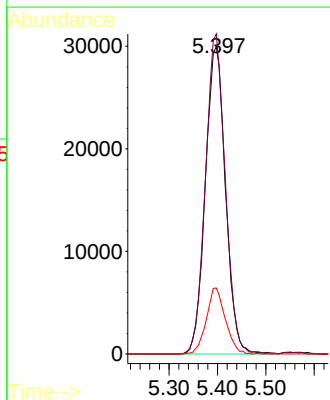
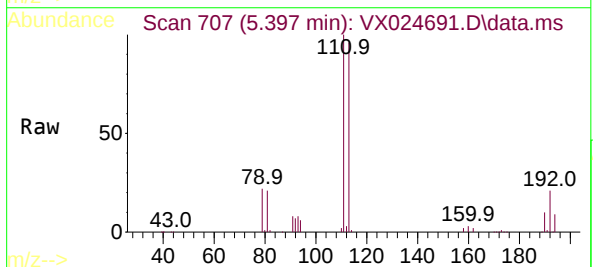


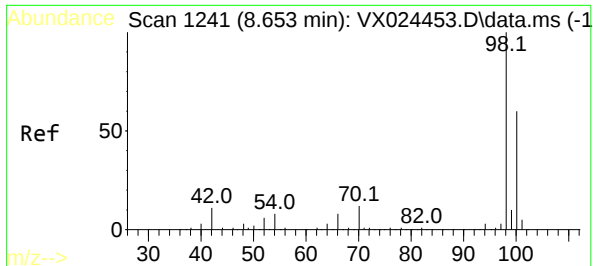

#50
Toluene-d8
Concen: 50.202 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX024691.D
Acq: 09 Oct 2021 00:35




Instrument :
MSVOA_X
ClientSampleId :
MWHR2-9-100521


Tgt Ion: 98 Resp: 318908
Ion Ratio Lower Upper
98 100
100 63.4 51.9 77.9

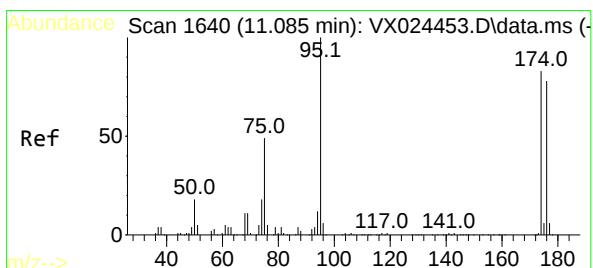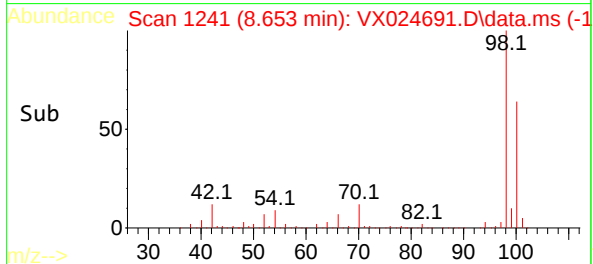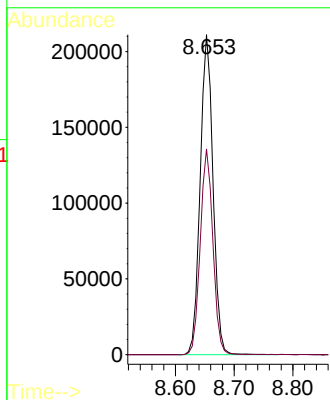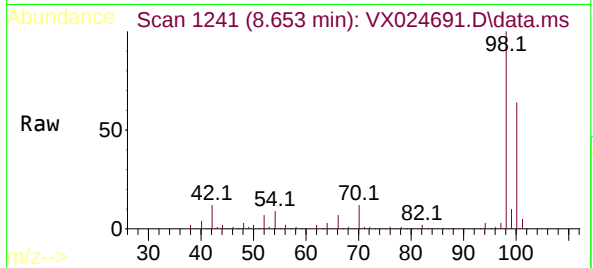

#62
4-Bromofluorobenzene
Concen: 48.204 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX024691.D
Acq: 09 Oct 2021 00:35

Tgt Ion: 95 Resp: 120398
Ion Ratio Lower Upper
95 100
174 83.6 0.0 154.6
176 79.5 0.0 155.8


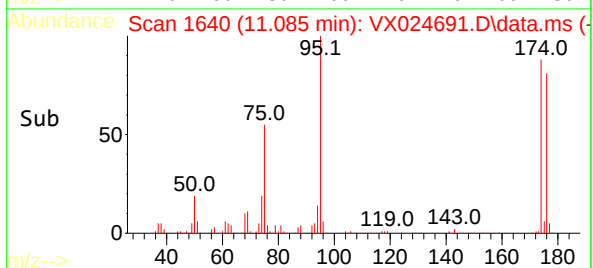
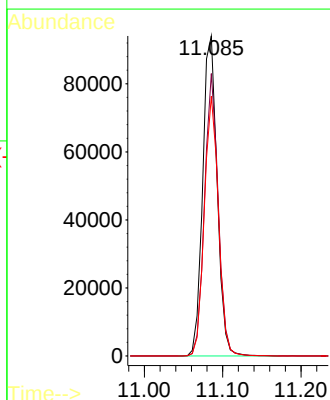
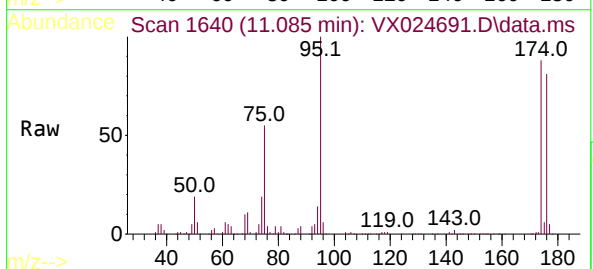


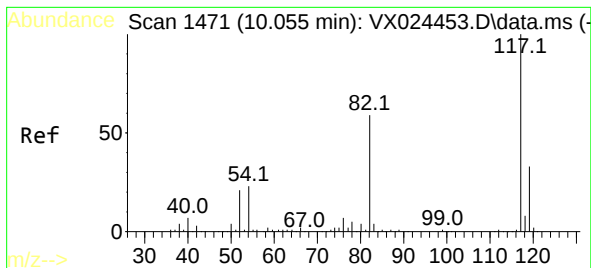

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX024691.D
Acq: 09 Oct 2021 00:35

Instrument :
MSVOA_X
ClientSampleId :
MWHR2-9-100521

Tgt Ion:117 Resp: 256217
Ion Ratio Lower Upper
117 100
82 56.2 47.4 71.2
119 31.5 26.6 39.8

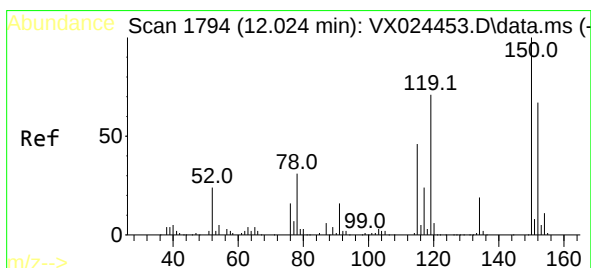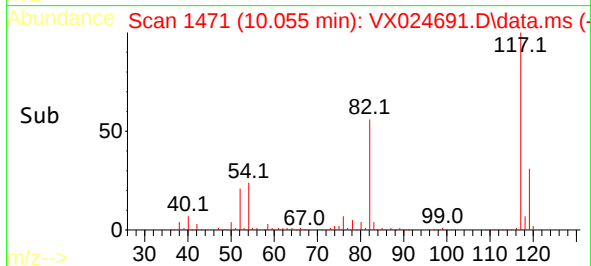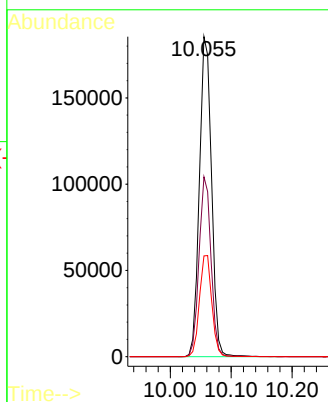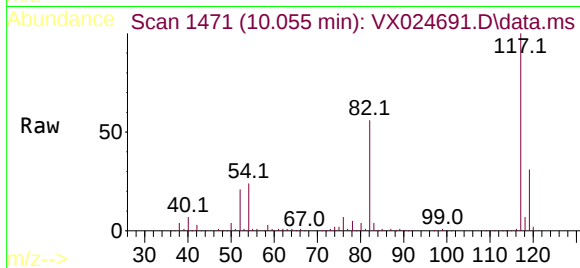

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX024691.D
Acq: 09 Oct 2021 00:35

Tgt Ion:152 Resp: 115419
Ion Ratio Lower Upper
152 100
115 59.6 41.1 123.3
150 157.2 0.0 349.0

