

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100821\
 Data File : VX024705.D
 Acq On : 09 Oct 2021 06:04
 Operator : JC/MD
 Sample : M4145-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IDW-SO-DRUM-5-100721


Quant Time: Oct 11 06:41:23 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
 Quant Title : SW846 8260
 QLast Update : Thu Sep 23 18:24:34 2021
 Response via : Initial Calibration


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100821\
Data File : VX024705.D
Acq On : 09 Oct 2021 06:04
Operator : JC/MD
Sample : M4145-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IDW-SO-DRUM-5-100721

Quant Time: Oct 11 06:41:23 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260
QLast Update : Thu Sep 23 18:24:34 2021
Response via : Initial Calibration

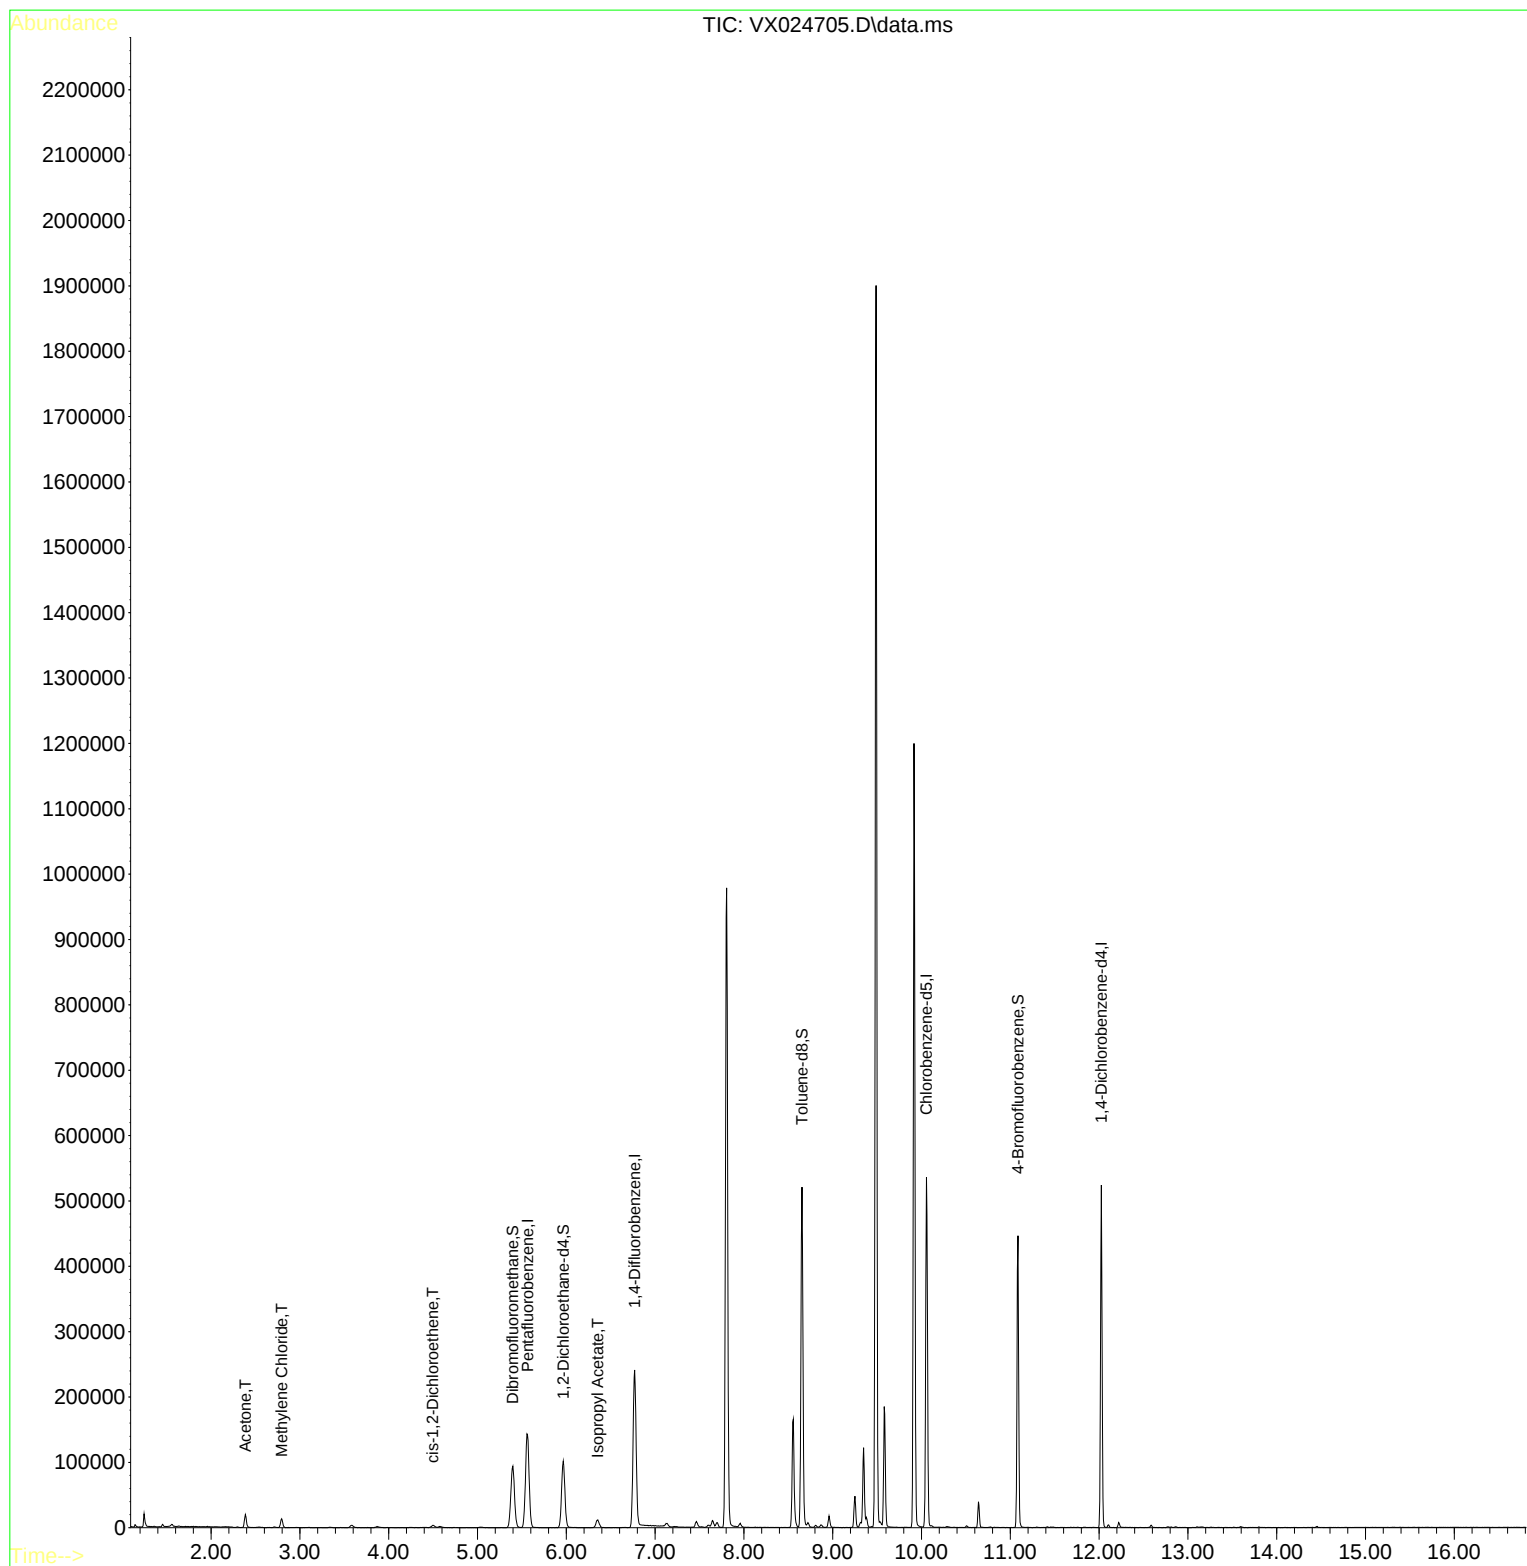

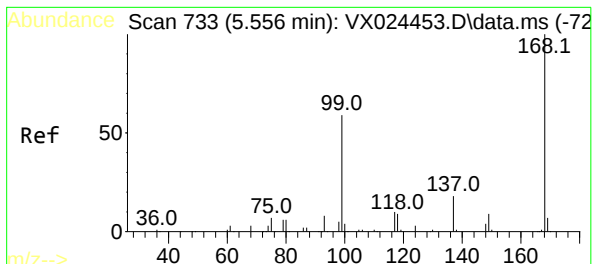

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.562 min Scan# 734

Delta R.T. 0.006 min

Lab File: VX024705.D





Acq: 09 Oct 2021 06:04

Tgt Ion:168 Resp: 135821

Ion Ratio Lower Upper

168 100

99 56.6 45.8 68.6

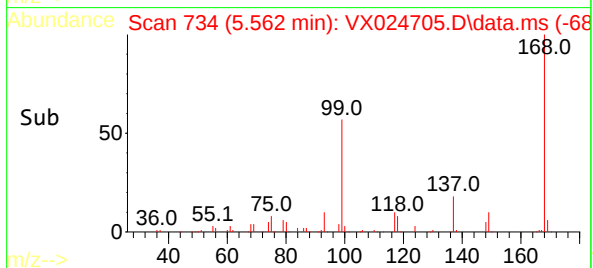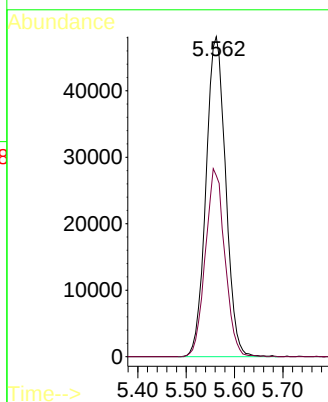

#16

Acetone

Concen: 15.689 ug/l

RT: 2.386 min Scan# 213

Delta R.T. -0.000 min

Lab File: VX024705.D




Acq: 09 Oct 2021 06:04


Tgt Ion: 43 Resp: 20348

Ion Ratio Lower Upper

43 100

58 28.1 27.8 41.8

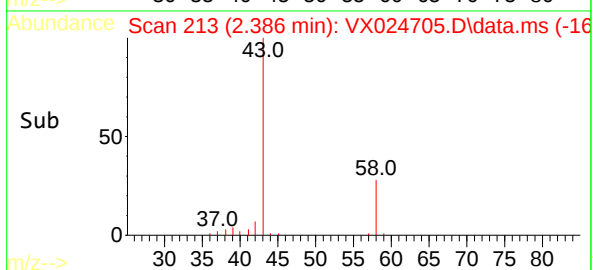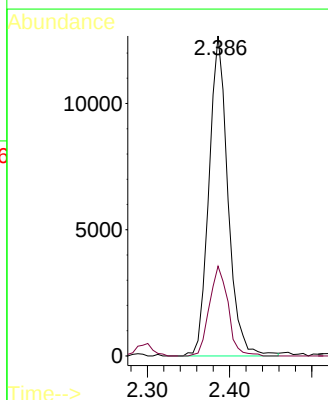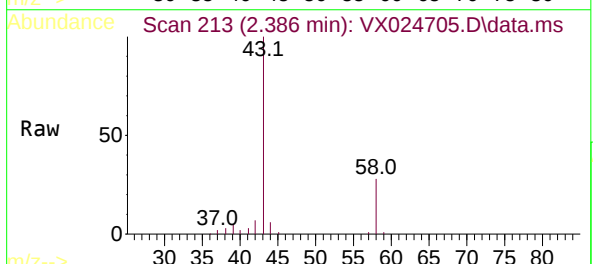



#20

Methylene Chloride

Concen: 3.118 ug/l

RT: 2.794 min Scan# 280

Delta R.T. 0.006 min

Lab File: VX024705.D

Acq: 09 Oct 2021 06:04

Tgt Ion: 84 Resp: 6003





Ion Ratio Lower Upper

84 100

49 111.9 88.6 132.8

51 37.6 27.0 40.6

86 58.5 50.3 75.5

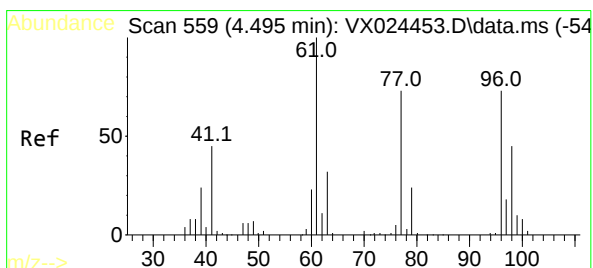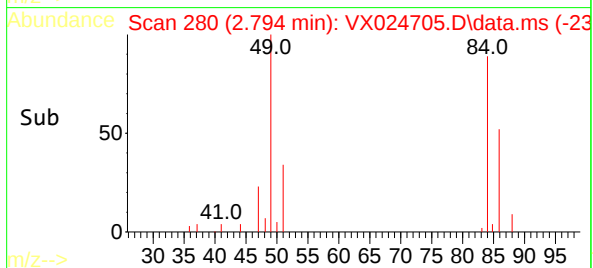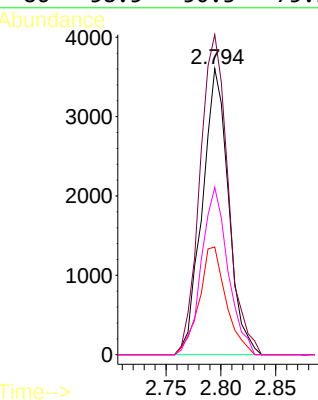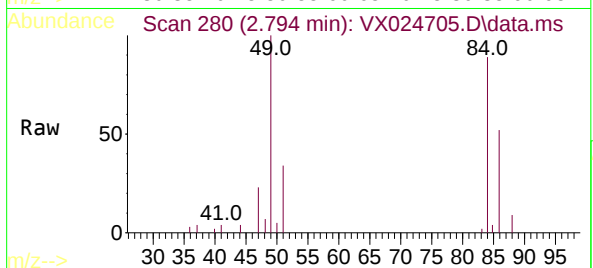

#27

cis-1,2-Dichloroethene

Concen: 1.438 ug/l

RT: 4.495 min Scan# 559

Delta R.T. 0.000 min

Lab File: VX024705.D

Acq: 09 Oct 2021 06:04




Tgt Ion: 96 Resp: 2376


Ion Ratio Lower Upper

96 100

61 136.7 0.0 285.6

98 61.1 0.0 129.6

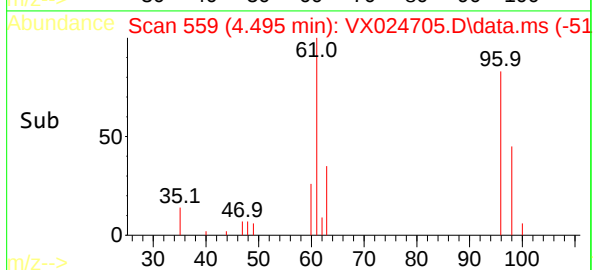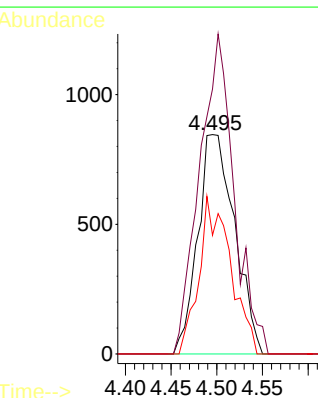







#33

1,2-Dichloroethane-d4
Concen: 53.382 ug/l
RT: 5.965 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX024705.D
Acq: 09 Oct 2021 06:04

Instrument :
MSVOA_X
ClientSampleId :
IDW-SO-DRUM-5-100721




Tgt Ion: 65 Resp: 102185
Ion Ratio Lower Upper
65 100
67 50.1 0.0 105.4

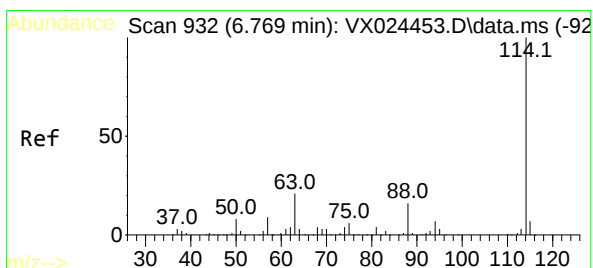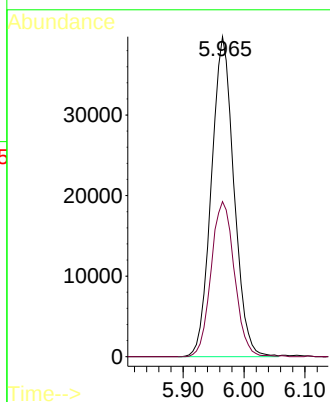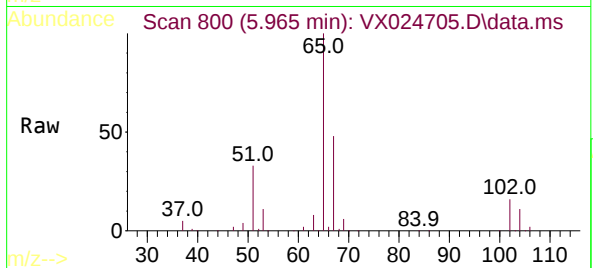


#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. 0.000 min
Lab File: VX024705.D
Acq: 09 Oct 2021 06:04

Tgt Ion: 114 Resp: 237105
Ion Ratio Lower Upper
114 100
63 21.0 0.0 40.8
88 15.7 0.0 32.8


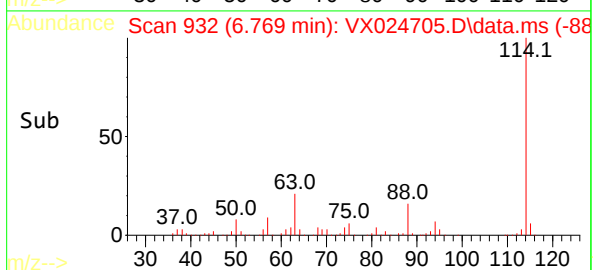
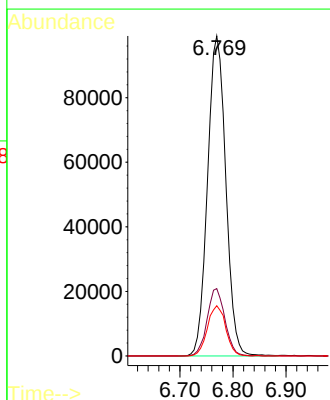



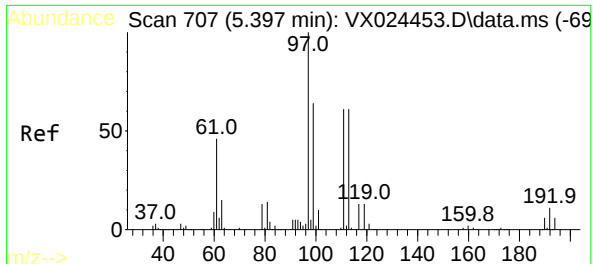

#35
Dibromofluoromethane
Concen: 50.531 ug/l
RT: 5.398 min Scan# 707
Delta R.T. 0.001 min
Lab File: VX024705.D
Acq: 09 Oct 2021 06:04




Instrument :
MSVOA_X
ClientSampleId :
IDW-SO-DRUM-5-100721


Tgt Ion:113 Resp: 79593
Ion Ratio Lower Upper
113 100
111 103.1 81.9 122.9
192 19.7 16.7 25.1

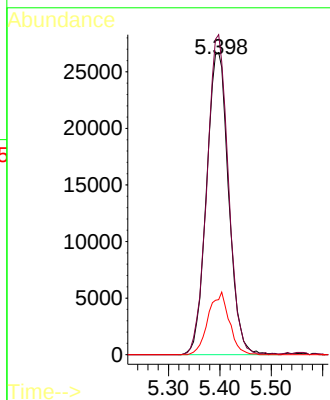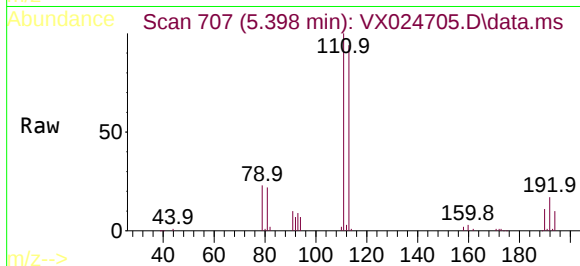

#43
Isopropyl Acetate
Concen: 3.755 ug/l
RT: 6.355 min Scan# 864
Delta R.T. 0.007 min
Lab File: VX024705.D
Acq: 09 Oct 2021 06:04

Tgt Ion: 43 Resp: 16202
Ion Ratio Lower Upper
43 100
61 18.2 18.2 27.4#
87 12.4 12.5 18.7#

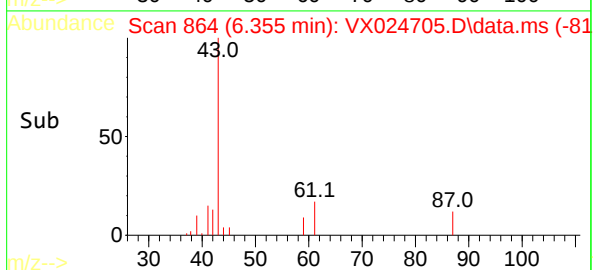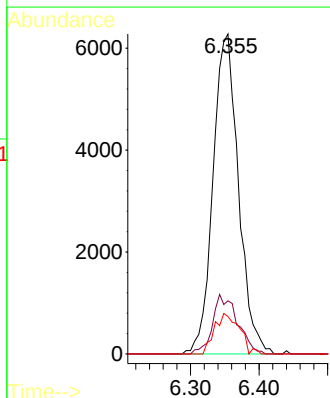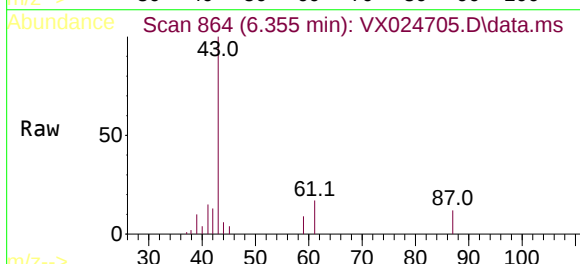

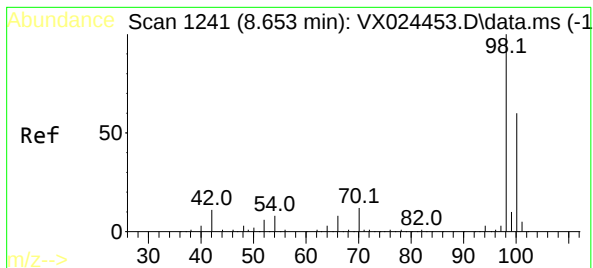

#50

Toluene-d8

Concen: 51.317 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. 0.000 min

Lab File: VX024705.D





Acq: 09 Oct 2021 06:04

Tgt Ion: 98 Resp: 297506

Ion Ratio Lower Upper

98 100

100 64.2 51.9 77.9

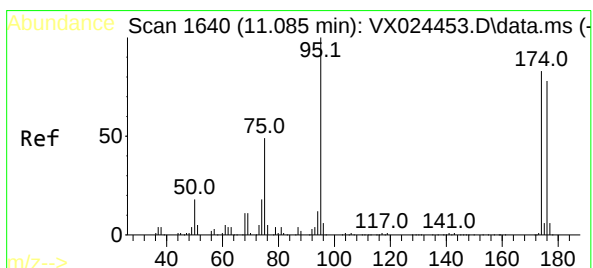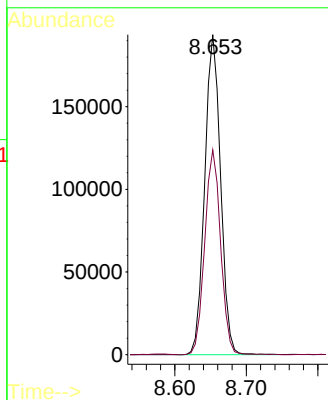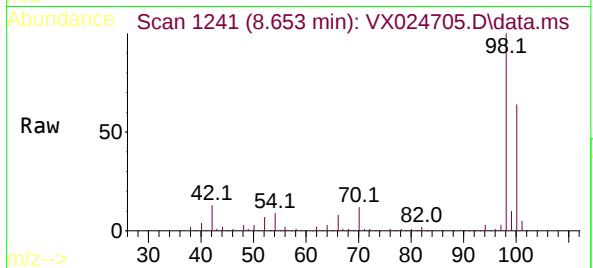

#62

4-Bromofluorobenzene

Concen: 49.265 ug/l

RT: 11.086 min Scan# 1640

Delta R.T. 0.001 min

Lab File: VX024705.D

Acq: 09 Oct 2021 06:04




Tgt Ion: 95 Resp: 112296


Ion Ratio Lower Upper

95 100

174 81.2 0.0 154.6

176 78.6 0.0 155.8


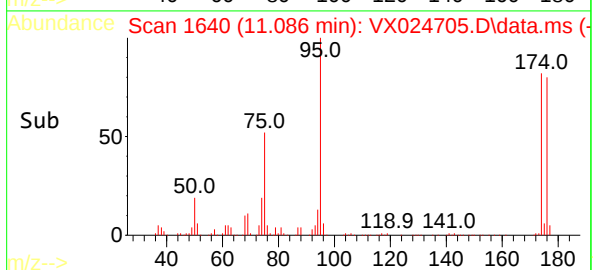
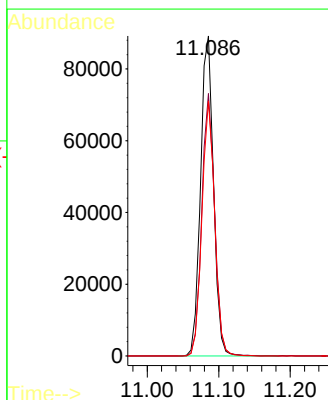



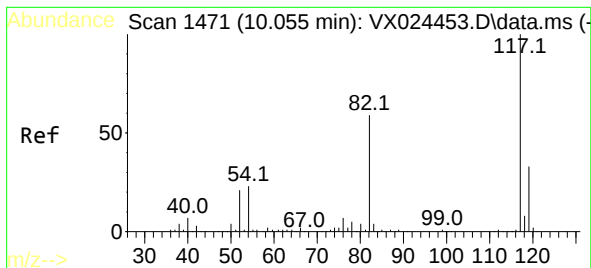

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX024705.D
Acq: 09 Oct 2021 06:04

Instrument :
MSVOA_X
ClientSampleId :
IDW-SO-DRUM-5-100721

Tgt Ion:117 Resp: 238648
Ion Ratio Lower Upper
117 100
82 57.9 47.4 71.2
119 32.9 26.6 39.8

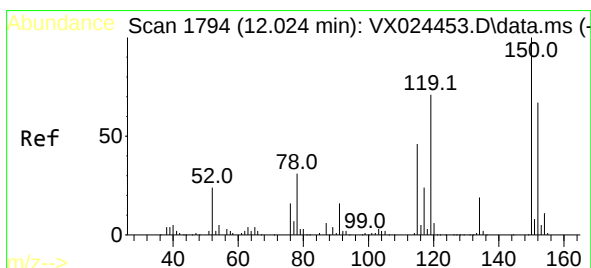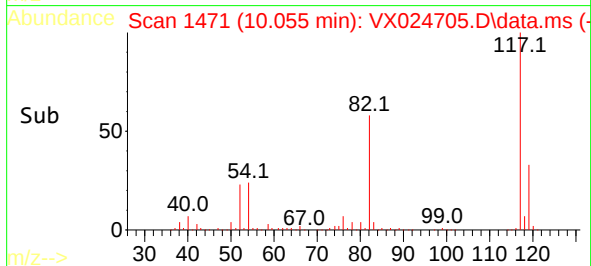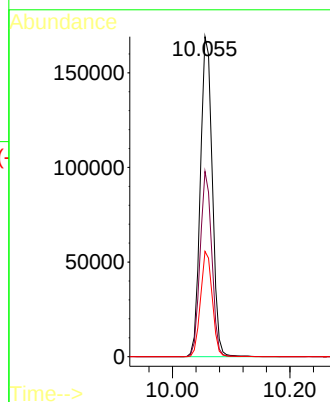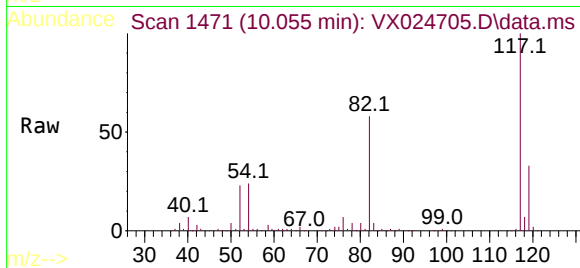

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX024705.D
Acq: 09 Oct 2021 06:04

Tgt Ion:152 Resp: 101562
Ion Ratio Lower Upper
152 100
115 61.2 41.1 123.3
150 159.1 0.0 349.0

