

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100821\
 Data File : VX024696.D
 Acq On : 09 Oct 2021 02:32
 Operator : JC/MD
 Sample : M4157-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FDR-20211008-WC

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M

Title : SW846 8260

Signal : TIC: VX024696.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	32	rBV	8308	12494	1.65%	0.304%
2	2.544	230	239	246	rBV	5358	11101	1.47%	0.270%
3	5.397	696	707	721	rBV3	89474	262982	34.76%	6.395%
4	5.562	723	734	751	rVB	141392	394362	52.12%	9.590%
5	5.964	788	800	813	rBV	100108	257773	34.07%	6.268%
6	6.769	918	932	945	rBV	230029	541962	71.63%	13.179%
7	8.653	1233	1241	1250	rBV	500260	756575	100.00%	18.398%
8	10.055	1465	1471	1482	rBV	514078	687652	90.89%	16.722%
9	11.085	1634	1640	1654	rVB	427176	536776	70.95%	13.053%
10	12.024	1789	1794	1802	rBV	508205	624093	82.49%	15.176%
11	13.780	2074	2082	2088	rBV	19953	26602	3.52%	0.647%




Sum of corrected areas: 4112372

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100821\
Data File : VX024696.D
Acq On : 09 Oct 2021 02:32
Operator : JC/MD
Sample : M4157-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FDR-20211008-WC

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

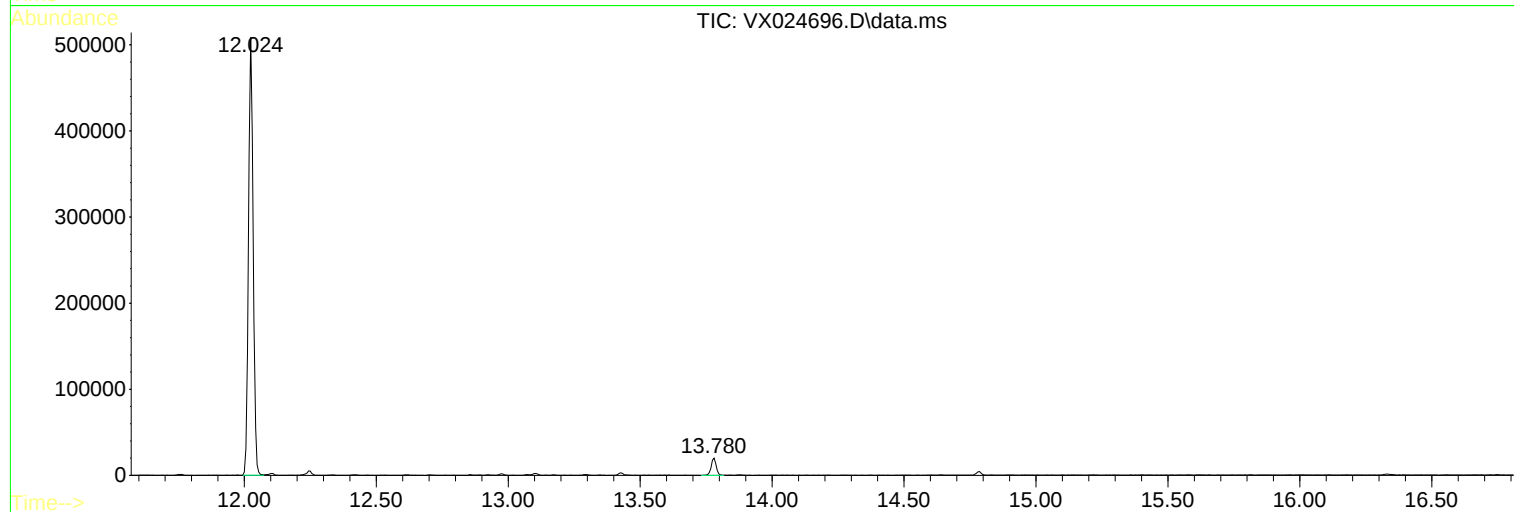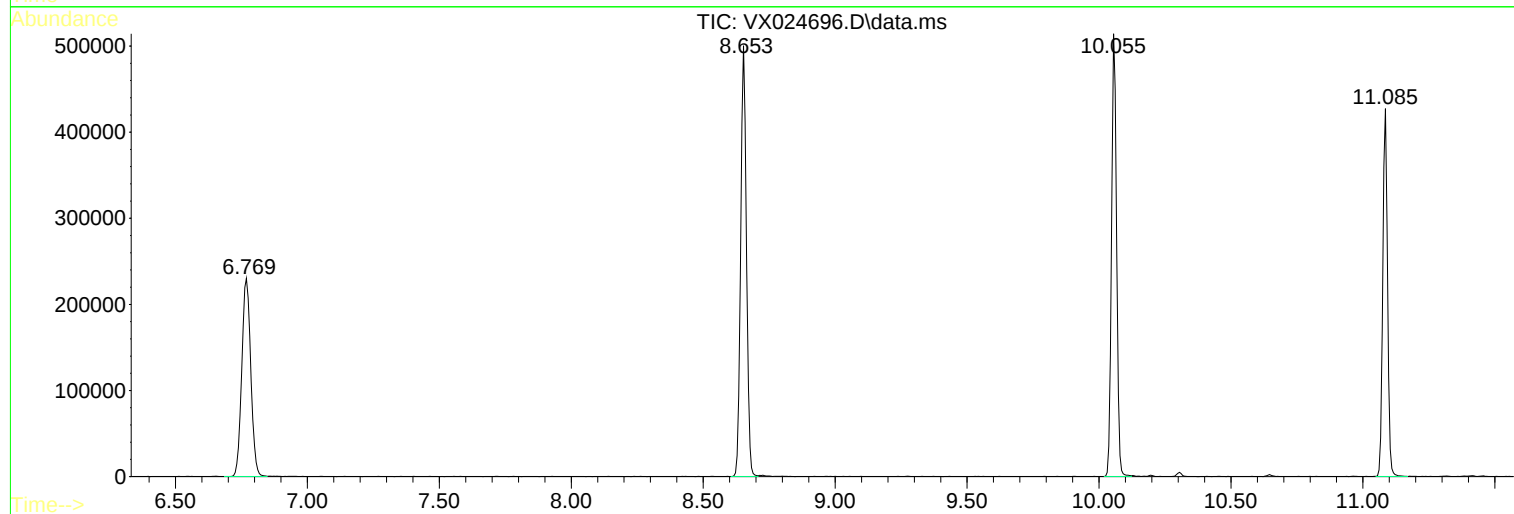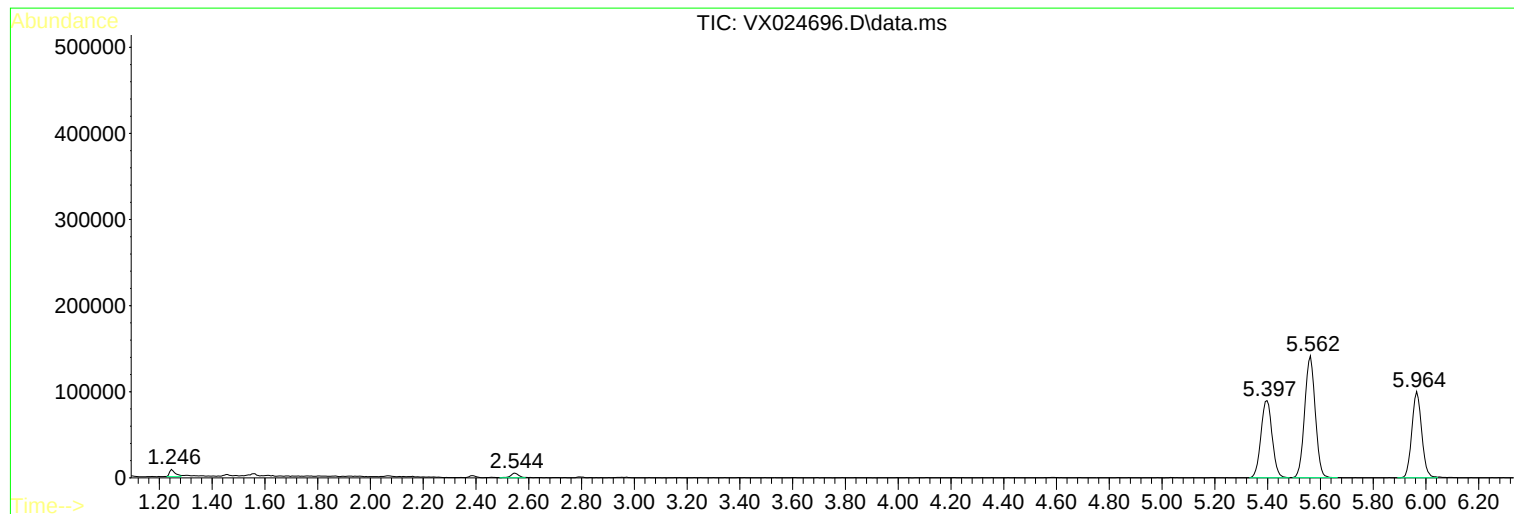

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100821\
Data File : VX024696.D
Acq On : 09 Oct 2021 02:32
Operator : JC/MD
Sample : M4157-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FDR-20211008-WC

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100821\
Data File : VX024696.D
Acq On : 09 Oct 2021 02:32
Operator : JC/MD
Sample : M4157-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FDR-20211008-WC

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
