
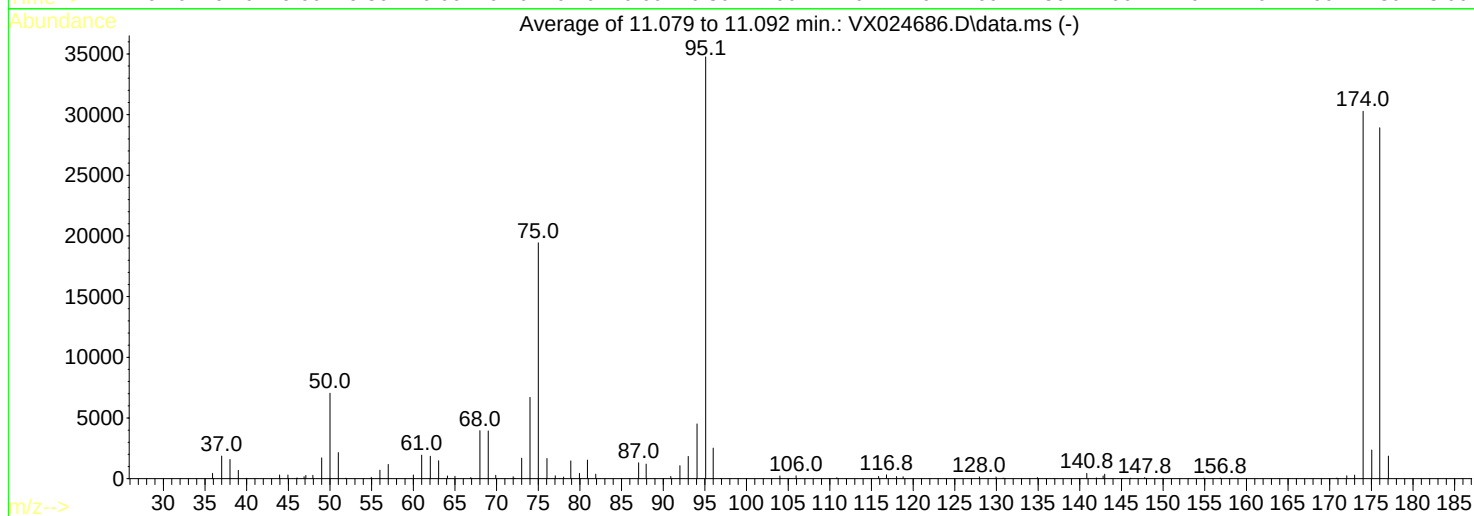


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100821\
Data File : VX024686.D
Acq On : 08 Oct 2021 21:28
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Title : SW846 8260
Last Update : Thu Sep 23 18:24:34 2021

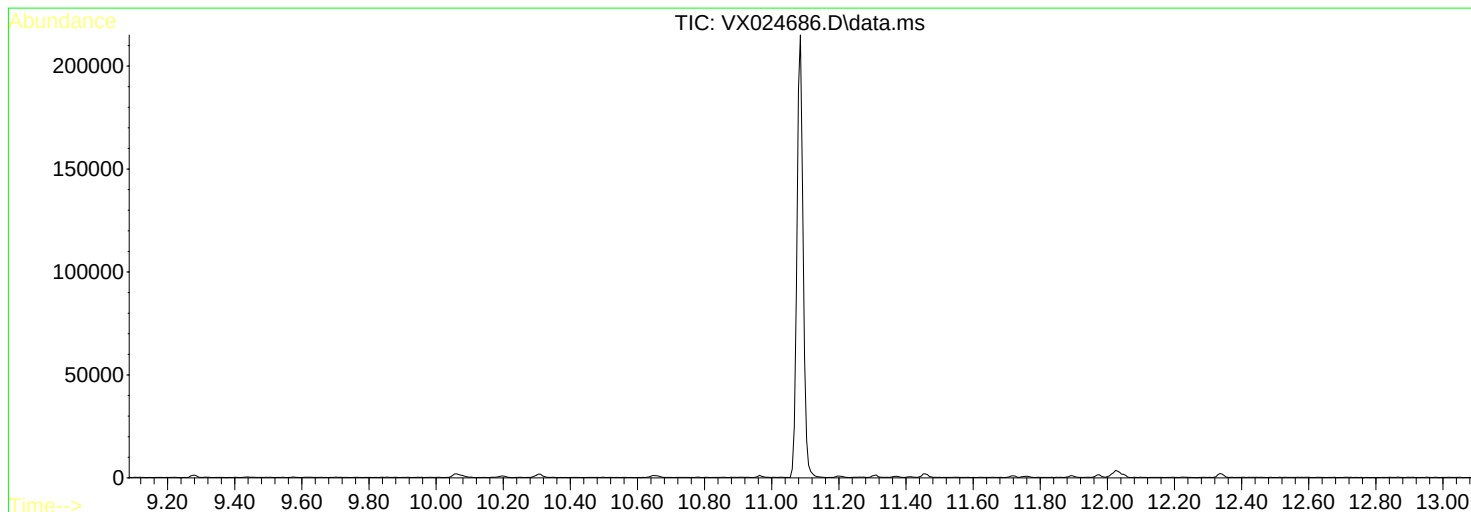

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	7048	PASS
75	95	30	60	55.9	19439	PASS
95	95	100	100	100.0	34760	PASS
96	95	5	9	7.3	2521	PASS
173	174	0.00	2	1.0	289	PASS
174	95	50	100	87.1	30275	PASS
175	174	5	9	7.8	2365	PASS
176	174	95	101	95.5	28915	PASS
177	176	5	9	6.4	1864	PASS