
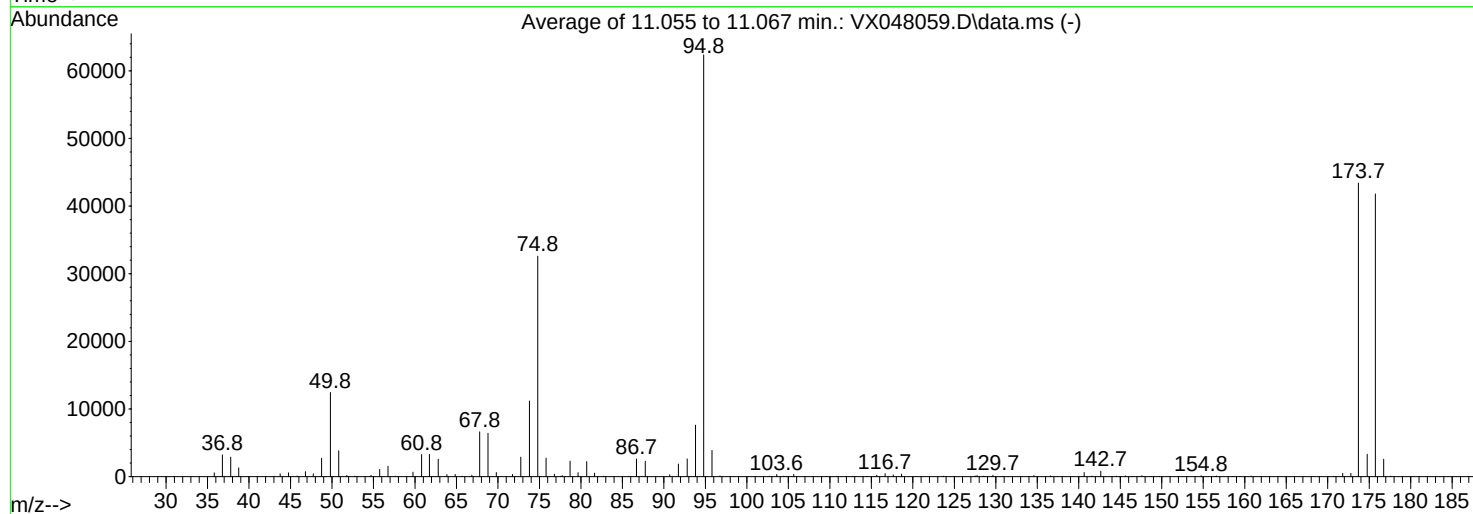


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100825\
Data File : VX048059.D
Acq On : 08 Oct 2025 08:44
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Title : SW846 8260
Last Update : Wed Sep 17 06:39:58 2025

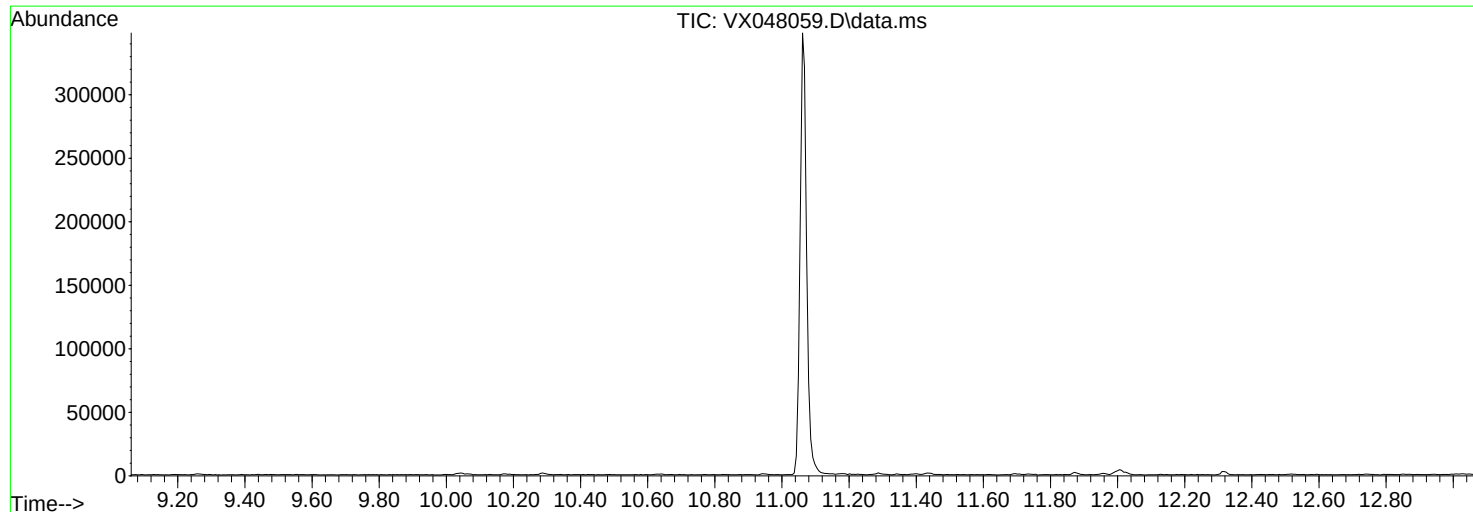

AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1629

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.9	12438	PASS
75	95	30	60	52.3	32592	PASS
95	95	100	100	100.0	62365	PASS
96	95	5	9	6.2	3875	PASS
173	174	0.00	2	1.1	499	PASS
174	95	50	100	69.6	43419	PASS
175	174	5	9	7.6	3314	PASS
176	174	95	101	96.3	41803	PASS
177	176	5	9	6.2	2579	PASS