

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100918\
 Data File : VX005167.D
 Acq On : 09 Oct 2018 18:56
 Operator : JC/MD
 Sample : J5284-06
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE-125D3-20181001

Quant Time: Oct 10 05:54:16 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 03 04:00:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	176796	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	278506	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	277121	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	155013	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	136117	53.90	ug/l	0.00
Spiked Amount	50.000		Recovery	=	107.80%	
35) Dibromofluoromethane	5.51	113	115239	48.82	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.64%	
50) Toluene-d8	8.72	98	408697	52.08	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.16%	
62) 4-Bromofluorobenzene	11.14	95	145033	51.30	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.60%	
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.20	85	849	0.352	ug/l	94
3) Chloromethane	1.32	50	847	0.290	ug/l #	68
5) Bromomethane	1.64	94	352	0.216	ug/l #	32
6) Chloroethane	1.70	64	93	Below Cal	#	45
9) 1,1,2-Trichlorotrifluoroet	2.39	101	53599	27.709	ug/l	100
11) Tert butyl alcohol	3.03	59	3290	4.659	ug/l #	76
12) 1,1-Dichloroethene	2.37	96	1771	0.924	ug/l	95
13) Acrolein	2.28	56	214	0.426	ug/l #	55
16) Acetone	2.45	43	6012	4.077	ug/l	92
20) Methylene Chloride	2.85	84	703	Below Cal	#	86
24) 1,1-Dichloroethane	3.69	63	1419	0.338	ug/l #	87
25) 2-Butanone	4.71	43	2279	1.049	ug/l #	86
27) cis-1,2-Dichloroethene	4.60	96	4591	1.960	ug/l	97
29) Tetrahydrofuran	5.16	42	399	0.295	ug/l #	72
30) Chloroform	5.22	83	1782	0.449	ug/l	99
31) Cyclohexane	5.66	56	3427	1.066	ug/l #	1
36) 1,1-Dichloropropene	5.66	75	12290	3.816	ug/l #	46
38) Carbon Tetrachloride	5.79	117	1186	0.350	ug/l #	81
39) Methylcyclohexane	7.21	83	3399	1.034	ug/l #	1
44) Trichloroethene	7.21	130	320267	129.218	ug/l	96
49) 1,4-Dioxane	7.76	88	654	9.400	ug/l #	75
60) Dibromochloromethane	9.34	129	1805	0.744	ug/l #	10
64) Tetrachloroethene	9.34	164	1859	0.682	ug/l	93
74) N-ethyl acetate	10.91	43	123	1.770	ug/l #	72
76) 1,2,3-Trichloropropane	11.14	75	72171	20.772	ug/l #	35
80) 1,3,5-Trimethylbenzene	11.51	105	121	Below Cal	#	59
81) trans-1,4-Dichloro-2-buten	11.14	75	72171	56.389	ug/l #	10
84) 1,2,4-Trimethylbenzene	11.81	105	286	Below Cal		70
95) Naphthalene	13.84	128	439	0.753	ug/l #	77

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.01 min

Lab File: VX005167.D

Acq: 09 Oct 2018 18:56

Instrument :

MSVOA_X

ClientSampleId :


RE-125D3-20181001

Tot Ion:168 Resp: 176796

Ion Ratio Lower Upper




168 100

99 50.2 39.3 58.9



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0



#2

Dichlorodifluoromethane

Concen: 0.352 ug/l

RT: 1.20 min Scan# 7

Delta R.T. -0.00 min

Lab File: VX005167.D


Acq: 09 Oct 2018 18:56

Tgt Ion: 85 Resp: 849

Ion Ratio Lower Upper



85 100


87 34.5 15.7 47.1



Abundance Ion 84.90 (84.60 to 85.60): VX0

Ion 86.90 (86.60 to 87.60): VX0





#3

Chloromethane

Concen: 0.290 ug/l

RT: 1.32 min Scan# 28

Delta R.T. -0.00 min

Lab File: VX005167.D

Acq: 09 Oct 2018 18:56

Instrument :

MSVOA_X

ClientSampleId :


RE-125D3-20181001

Tot Ion: 50 Resp: 847

Ion Ratio Lower Upper




50 100

52 50.2 25.8 38.6#



Abundance Ion 49.90 (49.60 to 50.60): VX0

Ion 51.90 (51.60 to 52.60): VX0



#5

Bromomethane

Concen: 0.216 ug/l

RT: 1.64 min Scan# 80

Delta R.T. 0.01 min

Lab File: VX005167.D


Acq: 09 Oct 2018 18:56

Tgt Ion: 94 Resp: 352

Ion Ratio Lower Upper



94 100


96 32.1 79.5 119.3#



Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0





#6

Chloroethane

Concen: Below Cal

RT: 1.70 min Scan# 90

Delta R.T. -0.01 min

Lab File: VX005167.D

Acq: 09 Oct 2018 18:56

Instrument :

MSVOA_X

ClientSampleId :





RE-125D3-20181001

Tot Ion: 64 Resp: 93

Ion Ratio Lower Upper

64 100

66 0.0 23.8 35.6#



#9

1,1,2-Trichlorotrifluoroethane

Concen: 27.709 ug/l

RT: 2.39 min Scan# 202

Delta R.T. 0.01 min

Lab File: VX005167.D

Acq: 09 Oct 2018 18:56




Tgt Ion:101 Resp: 53599


Ion Ratio Lower Upper

101 100

85 44.4 35.9 53.9

151 83.4 66.6 100.0









#11

Tert butyl alcohol
 Concen: 4.659 ug/l
 RT: 3.03 min Scan# 307
 Delta R.T. -0.06 min
 Lab File: VX005167.D
 Acq: 09 Oct 2018 18:56

Instrument :
 MSVOA_X
 ClientSampleId :
 RE-125D3-20181001




Tot Ion: 59 Resp: 3290
 Ion Ratio Lower Upper
 59 100
 57 1.8 8.6 12.8#




#12

1,1-Dichloroethene
 Concen: 0.924 ug/l
 RT: 2.37 min Scan# 200
 Delta R.T. 0.01 min
 Lab File: VX005167.D
 Acq: 09 Oct 2018 18:56

Tgt Ion: 96 Resp: 1771
 Ion Ratio Lower Upper
 96 100
 61 169.7 130.2 195.4
 98 62.1 53.4 80.0









#13
Acrolein
Concen: 0.426 ug/l
RT: 2.28 min Scan# 185
Delta R.T. -0.01 min
Lab File: VX005167.D
Acq: 09 Oct 2018 18:56




Instrument :
MSVOA_X
ClientSampleId :
RE-125D3-20181001


Tot Ion: 56 Resp: 214
Ion Ratio Lower Upper
56 100
55 119.2 63.4 95.2#



#16
Acetone
Concen: 4.077 ug/l
RT: 2.45 min Scan# 212
Delta R.T. -0.00 min
Lab File: VX005167.D
Acq: 09 Oct 2018 18:56

Tgt Ion: 43 Resp: 6012
Ion Ratio Lower Upper
43 100
58 31.4 21.8 32.6









#20
Methvlene Chloride
Concen: Below Cal
RT: 2.85 min Scan# 279
Delta R.T. -0.00 min
Lab File: VX005167.D
Acq: 09 Oct 2018 18:56




Instrument :
MSVOA_X
ClientSampleId :
RE-125D3-20181001


Tot Ion: 84 Resp: 703
Ion Ratio Lower Upper
84 100
49 97.3 92.3 138.5
51 38.4 31.8 47.6
86 46.9 48.5 72.7#



#24
1,1-Dichloroethane
Concen: 0.338 ug/l
RT: 3.69 min Scan# 416
Delta R.T. -0.01 min
Lab File: VX005167.D
Acq: 09 Oct 2018 18:56

Tgt Ion: 63 Resp: 1419
Ion Ratio Lower Upper
63 100
98 10.9 3.0 9.2#
100 0.0 2.0 5.8#





#25

2-Butanone

Concen: 1.049 ug/l

RT: 4.71 min Scan# 583

Delta R.T. -0.00 min

Lab File: VX005167.D

Acq: 09 Oct 2018 18:56

Instrument :

MSVOA_X

ClientSampleId :





RE-125D3-20181001

Tot Ion: 43 Resp: 2279

Ion Ratio Lower Upper

43 100

72 18.8 20.8 31.2#



#27

cis-1,2-Dichloroethene

Concen: 1.960 ug/l

RT: 4.60 min Scan# 566

Delta R.T. 0.01 min

Lab File: VX005167.D

Acq: 09 Oct 2018 18:56




Tgt Ion: 96 Resp: 4591


Ion Ratio Lower Upper

96 100

61 143.1 0.0 285.8

98 59.9 0.0 136.2





#29

Tetrahydrofuran

Concen: 0.295 ug/l

RT: 5.16 min Scan# 657

Delta R.T. -0.00 min

Lab File: VX005167.D

Acq: 09 Oct 2018 18:56

Instrument :

MSVOA_X

ClientSampleId :

RE-125D3-20181001





Tot Ion: 42 Resp: 399

Ion Ratio Lower Upper

42 100

72 16.5 33.7 50.5#

71 30.3 32.2 48.4#



#30

Chloroform

Concen: 0.449 ug/l

RT: 5.22 min Scan# 667

Delta R.T. 0.01 min

Lab File: VX005167.D




Acq: 09 Oct 2018 18:56


Tgt Ion: 83 Resp: 1782

Ion Ratio Lower Upper

83 100

85 64.9 52.4 78.6





#31

Cyclohexane

Concen: 1.066 ug/l

RT: 5.66 min Scan# 739

Delta R.T. 0.09 min

Lab File: VX005167.D

Acq: 09 Oct 2018 18:56

Instrument :

MSVOA_X

ClientSampleId :

RE-125D3-20181001


Tot Ion: 56 Resp: 3427

Ion Ratio Lower Upper

56 100

69 179.9 25.9 38.9#




84 143.7 71.9 107.9#



Abundance Ion 56.00 (55.70 to 56.70): VX0

Ion 69.00 (68.70 to 69.70): VX0

Ion 84.00 (83.70 to 84.70): VX0



#33

1,2-Dichloroethane-d4

Concen: 53.896 ug/l

RT: 6.07 min Scan# 806

Delta R.T. -0.00 min

Lab File: VX005167.D


Acq: 09 Oct 2018 18:56

Tgt Ion: 65 Resp: 136117

Ion Ratio Lower Upper



65 100


67 53.1 0.0 107.4



Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0









#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.87 min Scan# 937
 Delta R.T. 0.01 min
 Lab File: VX005167.D
 Acq: 09 Oct 2018 18:56




Instrument :
 MSVOA_X
 ClientSampleId :
 RE-125D3-20181001


Tot Ion:114 Resp: 278506
 Ion Ratio Lower Upper
 114 100
 63 20.8 0.0 39.8
 88 15.5 0.0 27.0



#35
 Dibromofluoromethane
 Concen: 48.822 ug/l
 RT: 5.51 min Scan# 714
 Delta R.T. 0.01 min
 Lab File: VX005167.D
 Acq: 09 Oct 2018 18:56

Tgt Ion:113 Resp: 115239
 Ion Ratio Lower Upper
 113 100
 111 101.8 77.0 115.4
 192 23.7 17.0 25.6









#36
 1,1-Dichloropropene
 Concen: 3.816 ug/l
 RT: 5.66 min Scan# 739
 Delta R.T. -0.14 min
 Lab File: VX005167.D
 Acq: 09 Oct 2018 18:56




Instrument :
 MSVOA_X
 ClientSampleId :
 RE-125D3-20181001


Tot Ion: 75 Resp: 12290
 Ion Ratio Lower Upper
 75 100
 110 9.3 20.0 59.9#
 77 0.0 27.1 40.7#



#38
 Carbon Tetrachloride
 Concen: 0.350 ug/l
 RT: 5.79 min Scan# 760
 Delta R.T. 0.01 min
 Lab File: VX005167.D
 Acq: 09 Oct 2018 18:56

Tgt Ion: 117 Resp: 1186
 Ion Ratio Lower Upper
 117 100
 119 117.0 75.2 112.8#
 121 30.6 22.5 33.7









#39
Methvlcvclohexane
Concen: 1.034 ug/l
RT: 7.21 min Scan# 994
Delta R.T. -0.25 min
Lab File: VX005167.D
Acq: 09 Oct 2018 18:56

Instrument :
MSVOA_X
ClientSampleId :
RE-125D3-20181001

Tot Ion: 83 Resp: 3399
Ion Ratio Lower Upper
83 100
55 0.0 81.1 121.7#
98 217.1 37.3 55.9#




Abundance Ion 83.00 (82.70 to 83.70): VX0
Ion 55.00 (54.70 to 55.70): VX0
Ion 98.00 (97.70 to 98.70): VX0






#44
Trichloroethene
Concen: 129.218 ug/l
RT: 7.21 min Scan# 994
Delta R.T. -0.00 min
Lab File: VX005167.D
Acq: 09 Oct 2018 18:56

Tgt Ion:130 Resp: 320267
Ion Ratio Lower Upper
130 100
95 96.9 0.0 186.8



Abundance Ion 129.80 (129.50 to 130.50): V
Ion 94.90 (94.60 to 95.60): VX0









#49
1,4-Dioxane
Concen: 9.400 ug/l
RT: 7.76 min Scan# 1083
Delta R.T. -0.00 min
Lab File: VX005167.D
Acq: 09 Oct 2018 18:56




Instrument :
MSVOA_X
ClientSampleId :
RE-125D3-20181001


Tot Ion: 88 Resp: 654
Ion Ratio Lower Upper
88 100
43 60.7 25.1 37.7#
58 80.1 56.2 84.2



#50
Toluene-d8
Concen: 52.083 ug/l
RT: 8.72 min Scan# 1241
Delta R.T. -0.00 min
Lab File: VX005167.D
Acq: 09 Oct 2018 18:56

Tgt Ion: 98 Resp: 408697
Ion Ratio Lower Upper
98 100
100 63.1 51.9 77.9









#60
Dibromochloromethane
Concen: 0.744 ug/l
RT: 9.34 min Scan# 1342
Delta R.T. -0.25 min
Lab File: VX005167.D
Acq: 09 Oct 2018 18:56

Instrument :
MSVOA_X
ClientSampleId :
RE-125D3-20181001

Tot Ion:129 Resp: 1805
Ion Ratio Lower Upper
129 100
127 0.0 39.1 117.2#




Abundance Ion 128.80 (128.50 to 129.50): V
Ion 126.80 (126.50 to 127.50): V






#62
4-Bromofluorobenzene
Concen: 51.304 ug/l
RT: 11.14 min Scan# 1638
Delta R.T. -0.00 min
Lab File: VX005167.D
Acq: 09 Oct 2018 18:56

Tgt Ion: 95 Resp: 145033
Ion Ratio Lower Upper
95 100
174 93.3 0.0 185.0
176 90.0 0.0 180.2



Abundance Ion 94.90 (94.60 to 95.60): VX0
Ion 173.80 (173.50 to 174.50): V
Ion 175.80 (175.50 to 176.50): V









#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.12 min Scan# 1470
Delta R.T. -0.00 min
Lab File: VX005167.D
Acq: 09 Oct 2018 18:56




Instrument :
MSVOA_X
ClientSampleId :
RE-125D3-20181001


Tot Ion:117 Resp: 277121
Ion Ratio Lower Upper
117 100
82 55.9 42.2 63.4
119 32.5 27.4 41.0



#64
Tetrachloroethene
Concen: 0.682 ug/l
RT: 9.34 min Scan# 1342
Delta R.T. -0.00 min
Lab File: VX005167.D
Acq: 09 Oct 2018 18:56

Tgt Ion:164 Resp: 1859
Ion Ratio Lower Upper
164 100
166 123.4 98.4 147.6
129 78.5 76.1 114.1
131 83.5 71.0 106.4





#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. -0.00 min

Lab File: VX005167.D

Acq: 09 Oct 2018 18:56

Instrument :

MSVOA_X

ClientSampleId :

RE-125D3-20181001


Tot Ion:152 Resp: 155013

Ion Ratio Lower Upper

152 100

115 55.3 40.2 120.6




150 154.4 0.0 351.0



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V



#74

N-ethyl acetate

Concen: 1.770 ug/l

RT: 10.91 min Scan# 1601

Delta R.T. 0.01 min

Lab File: VX005167.D

Acq: 09 Oct 2018 18:56

Tgt Ion: 43 Resp: 123


Ion Ratio Lower Upper

43 100

70 40.7 32.6 48.8

55 0.0 21.6 32.4#

61 0.0 19.1 28.7#






Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 70.00 (69.70 to 70.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

Ion 61.00 (60.70 to 61.70): VX0









#76
 1,2,3-Trichloropropane
 Concen: 20.772 ug/l
 RT: 11.14 min Scan# 1638
 Delta R.T. -0.16 min
 Lab File: VX005167.D
 Acq: 09 Oct 2018 18:56




Instrument :
 MSVOA_X
 ClientSampleId :
 RE-125D3-20181001


Tot Ion: 75 Resp: 72171
 Ion Ratio Lower Upper
 75 100
 77 1.4 21.4 64.3#



#81
 trans-1,4-Dichloro-2-butene
 Concen: 56.389 ug/l
 RT: 11.14 min Scan# 1638
 Delta R.T. 0.06 min
 Lab File: VX005167.D
 Acq: 09 Oct 2018 18:56

Tgt Ion: 75 Resp: 72171
 Ion Ratio Lower Upper
 75 100
 53 0.3 80.2 120.4#
 89 0.0 37.1 55.7#



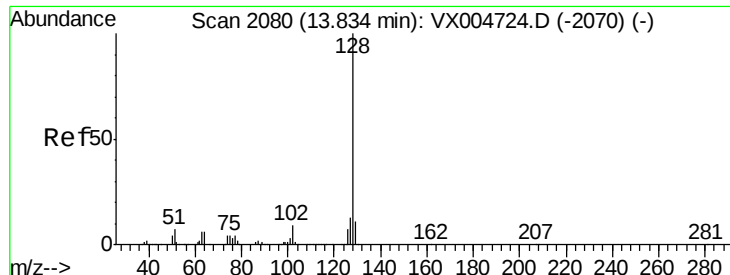

#95

Naphthalene

Concen: 0.753 ug/l

RT: 13.84 min Scan# 2081

Delta R.T. 0.01 min

Lab File: VX005167.D

Acq: 09 Oct 2018 18:56

Instrument :

MSVOA_X

ClientSampleId :

RE-125D3-20181001


Tot Ion:128 Resp: 439

Ion Ratio Lower Upper

128 100

127 6.2 10.4 15.6#



129 0.0 8.7 13.1#



Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V



Time-->