


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX100918\
Data File : VX005155.D
Acq On : 09 Oct 2018 12:56
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D100118S.M
Title : SW846 8260
Last Update : Tue Oct 02 06:56:35 2018

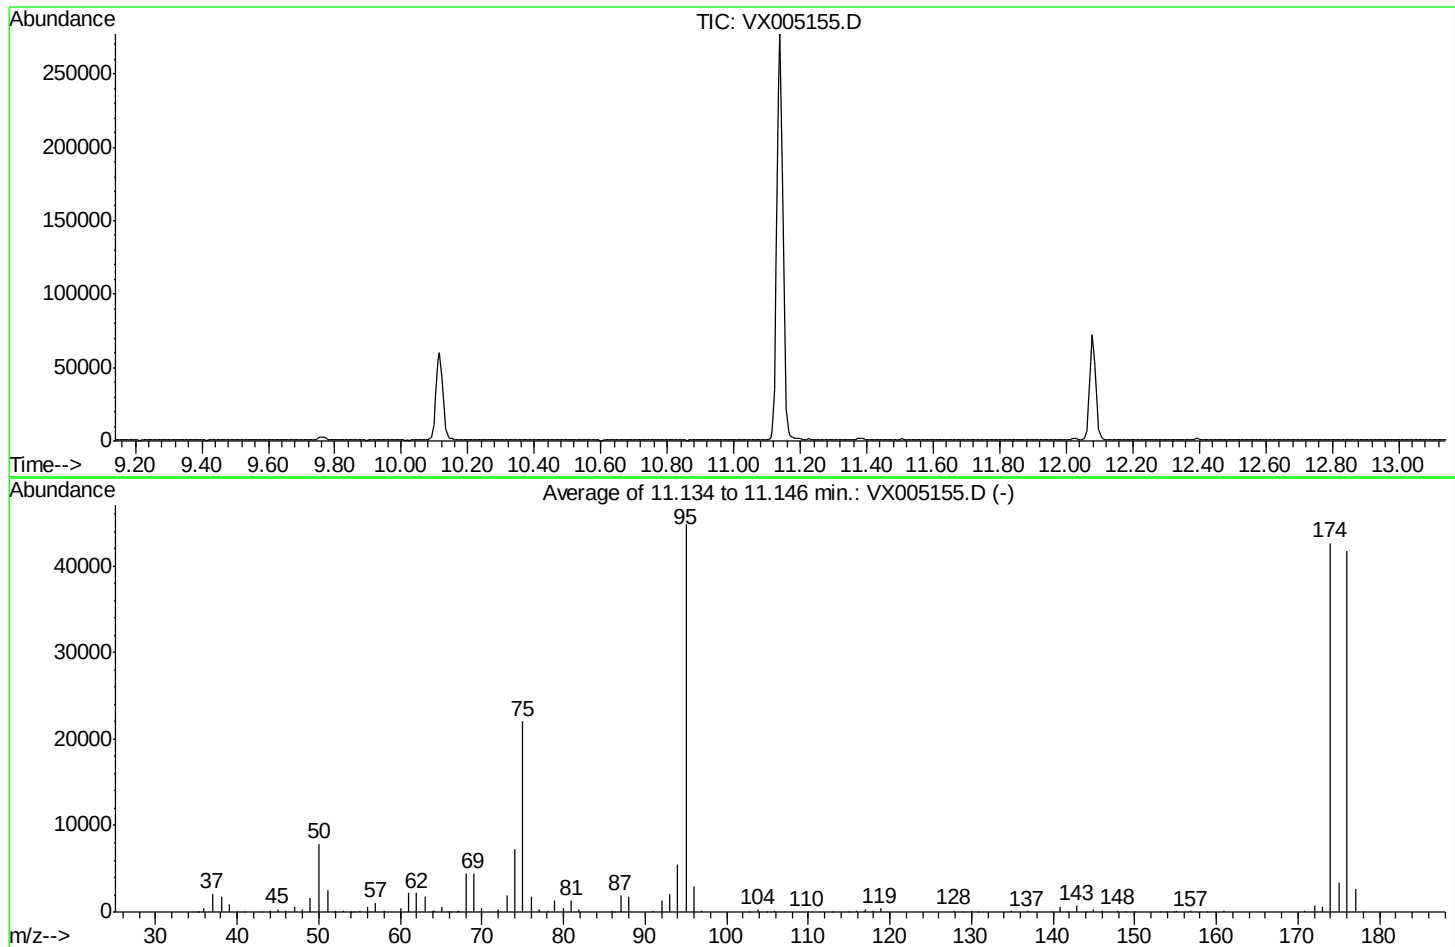

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	7924	PASS
75	95	30	60	49.2	22050	PASS
95	95	100	100	100.0	44834	PASS
96	95	5	9	6.6	2977	PASS
173	174	0.00	2	1.4	581	PASS
174	95	50	100	95.3	42709	PASS
175	174	5	9	7.9	3390	PASS
176	174	95	101	97.6	41688	PASS
177	176	5	9	6.2	2601	PASS