


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX100918\
Data File : VX005181.D
Acq On : 10 Oct 2018 01:38
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D100118S.M
Title : SW846 8260
Last Update : Tue Oct 02 06:56:35 2018

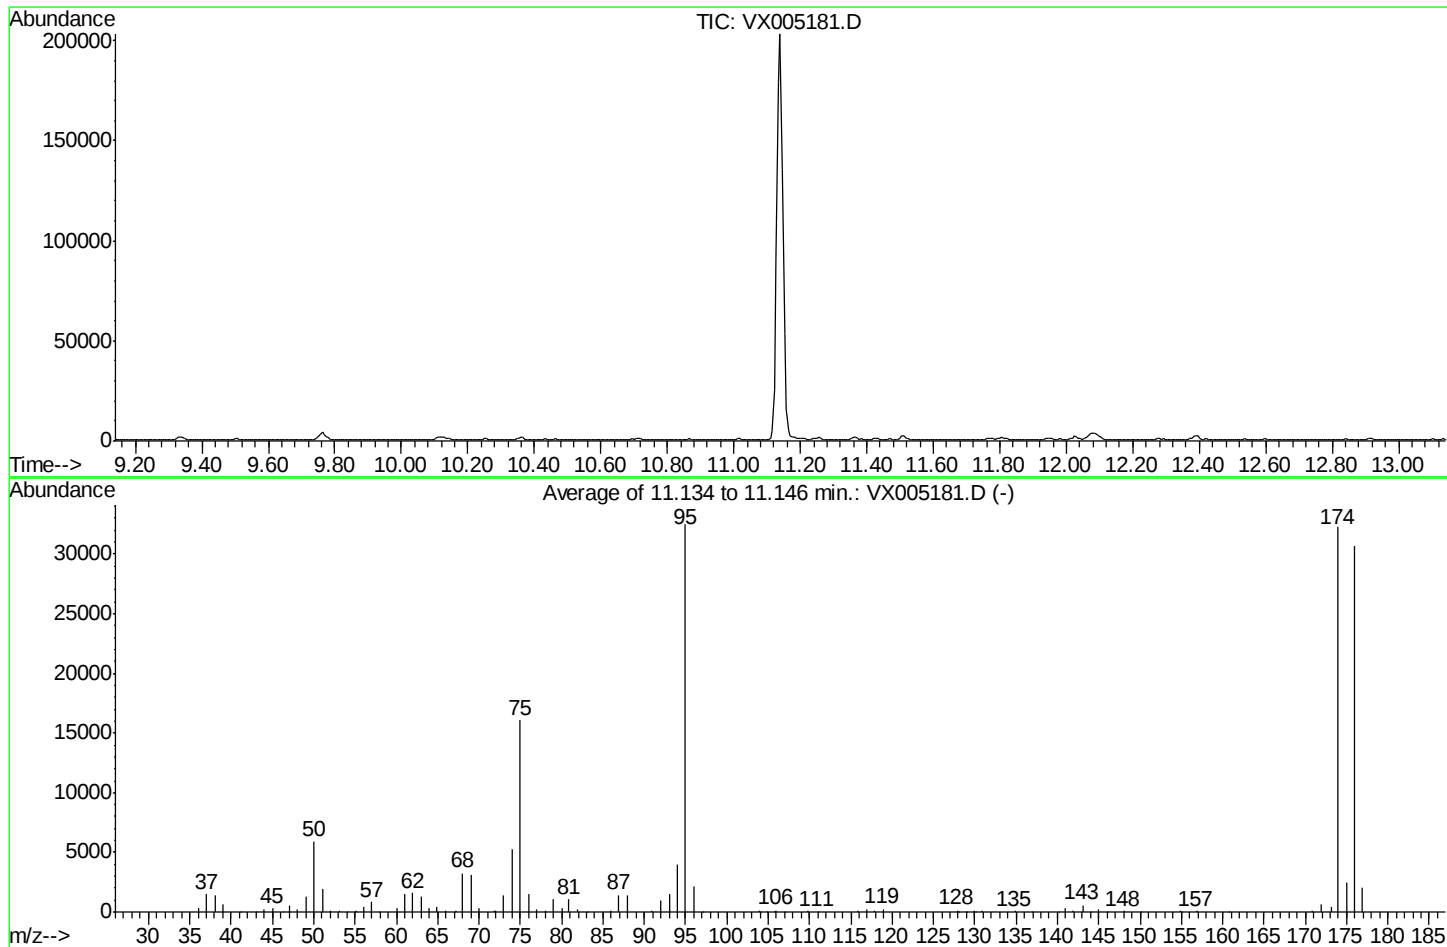

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	5888	PASS
75	95	30	60	49.4	16048	PASS
95	95	100	100	100.0	32498	PASS
96	95	5	9	6.5	2115	PASS
173	174	0.00	2	1.4	457	PASS
174	95	50	100	99.3	32280	PASS
175	174	5	9	7.8	2502	PASS
176	174	95	101	95.0	30677	PASS
177	176	5	9	6.6	2028	PASS