


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX100919\
Data File : VX012928.D
Acq On : 09 Oct 2019 09:00
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X100819W.M
Title : SW846 8260
Last Update : Wed Oct 09 01:51:23 2019

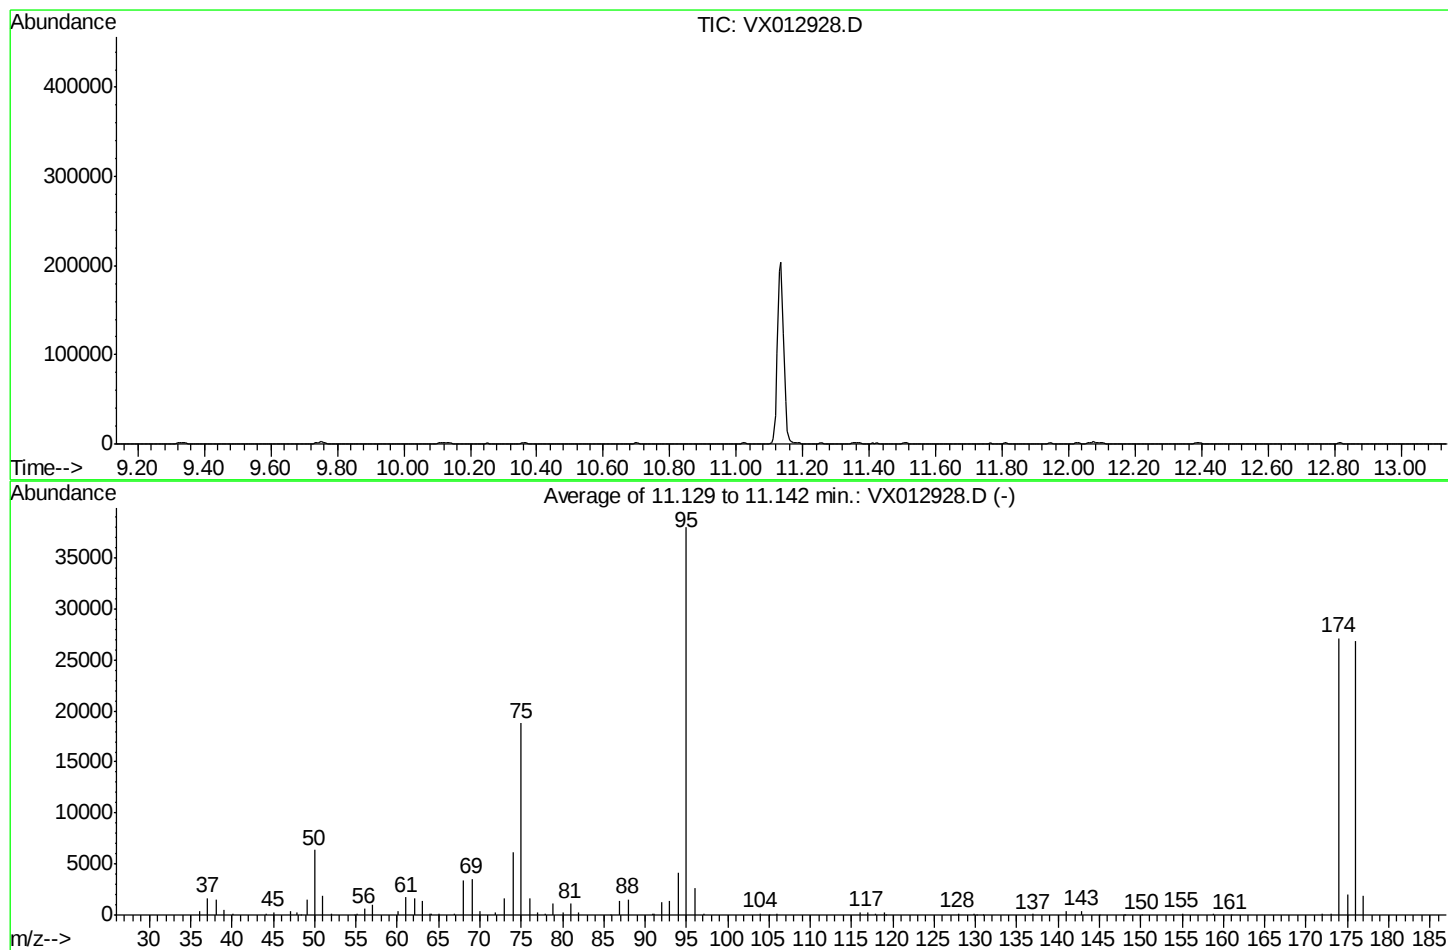

AutoFind: Scans 1680, 1681, 1682; Background Corrected with Scan 1673

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	6385	PASS
75	95	30	60	49.4	18775	PASS
95	95	100	100	100.0	38002	PASS
96	95	5	9	7.1	2693	PASS
173	174	0.00	2	0.4	102	PASS
174	95	50	100	71.5	27160	PASS
175	174	5	9	7.5	2039	PASS
176	174	95	101	99.1	26914	PASS
177	176	5	9	6.8	1840	PASS