



1,1-Dichloroethene

Response Ratio

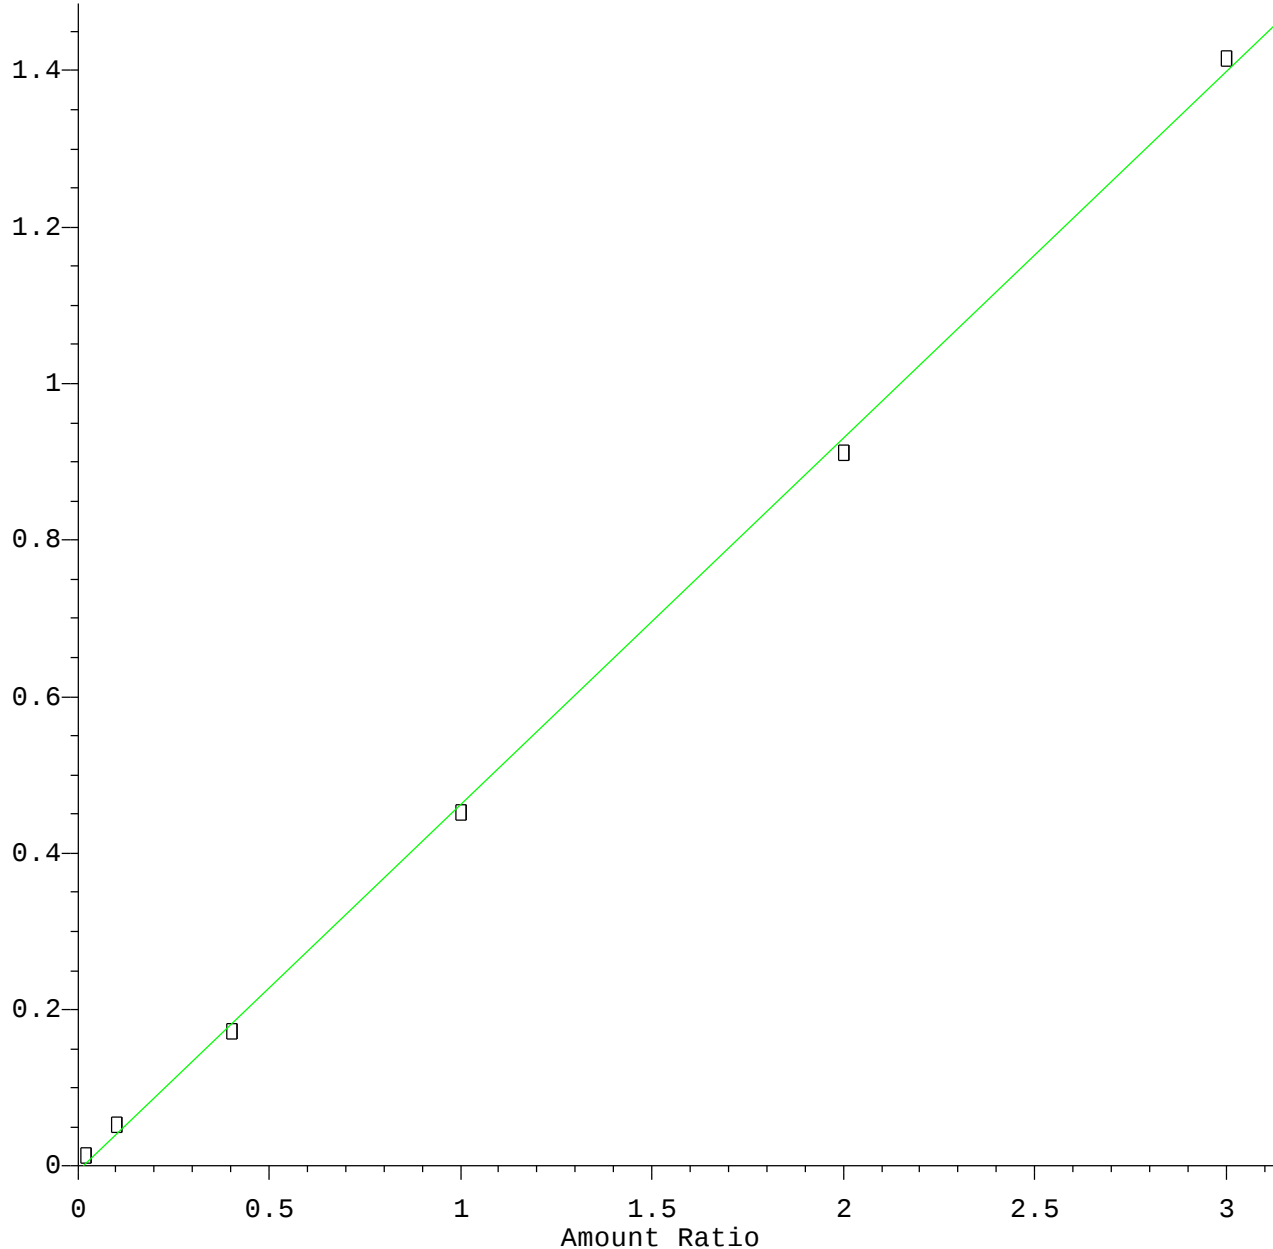

Resp Ratio = 4.68e-001 * Amt - 6.60e-003
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X100920W.M
Calibration Table Last Updated: Sat Oct 10 06:09:09 2020

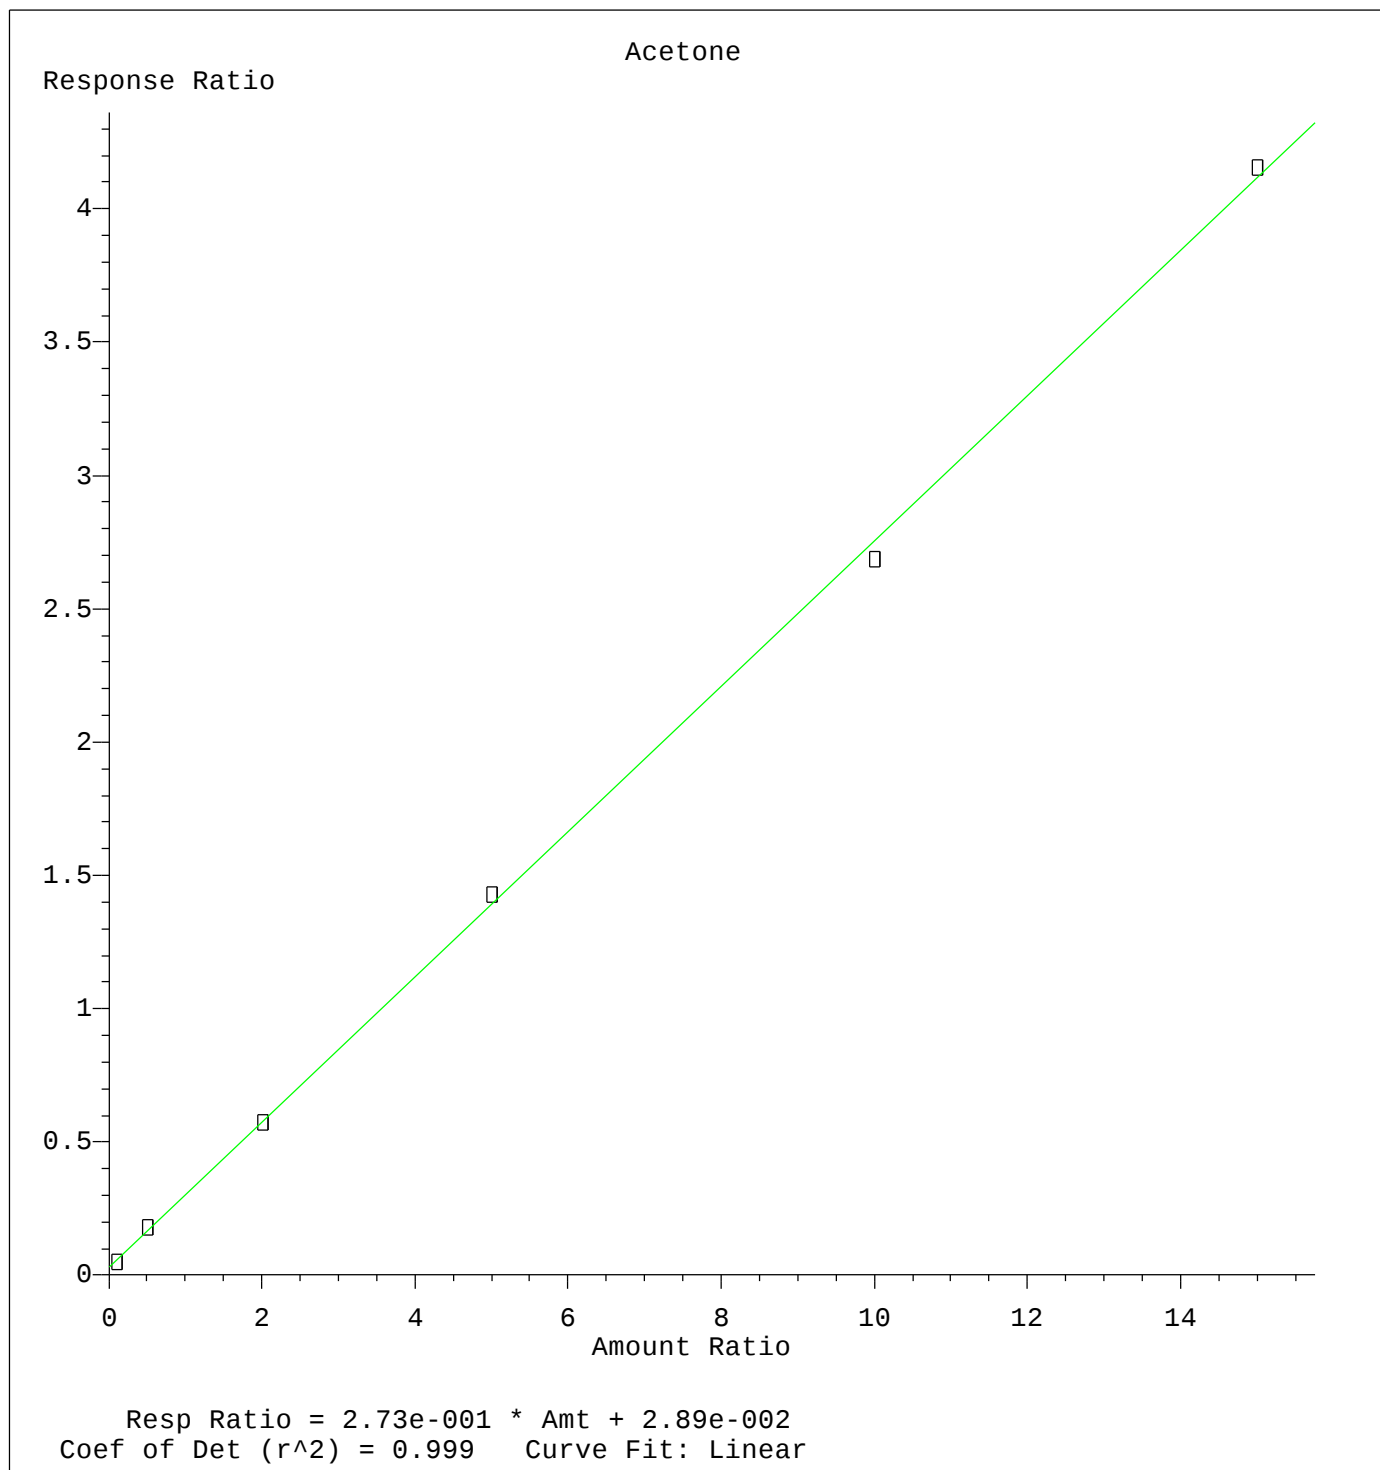

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X100920W.M
Calibration Table Last Updated: Sat Oct 10 06:09:09 2020

Methylene Chloride

Response Ratio

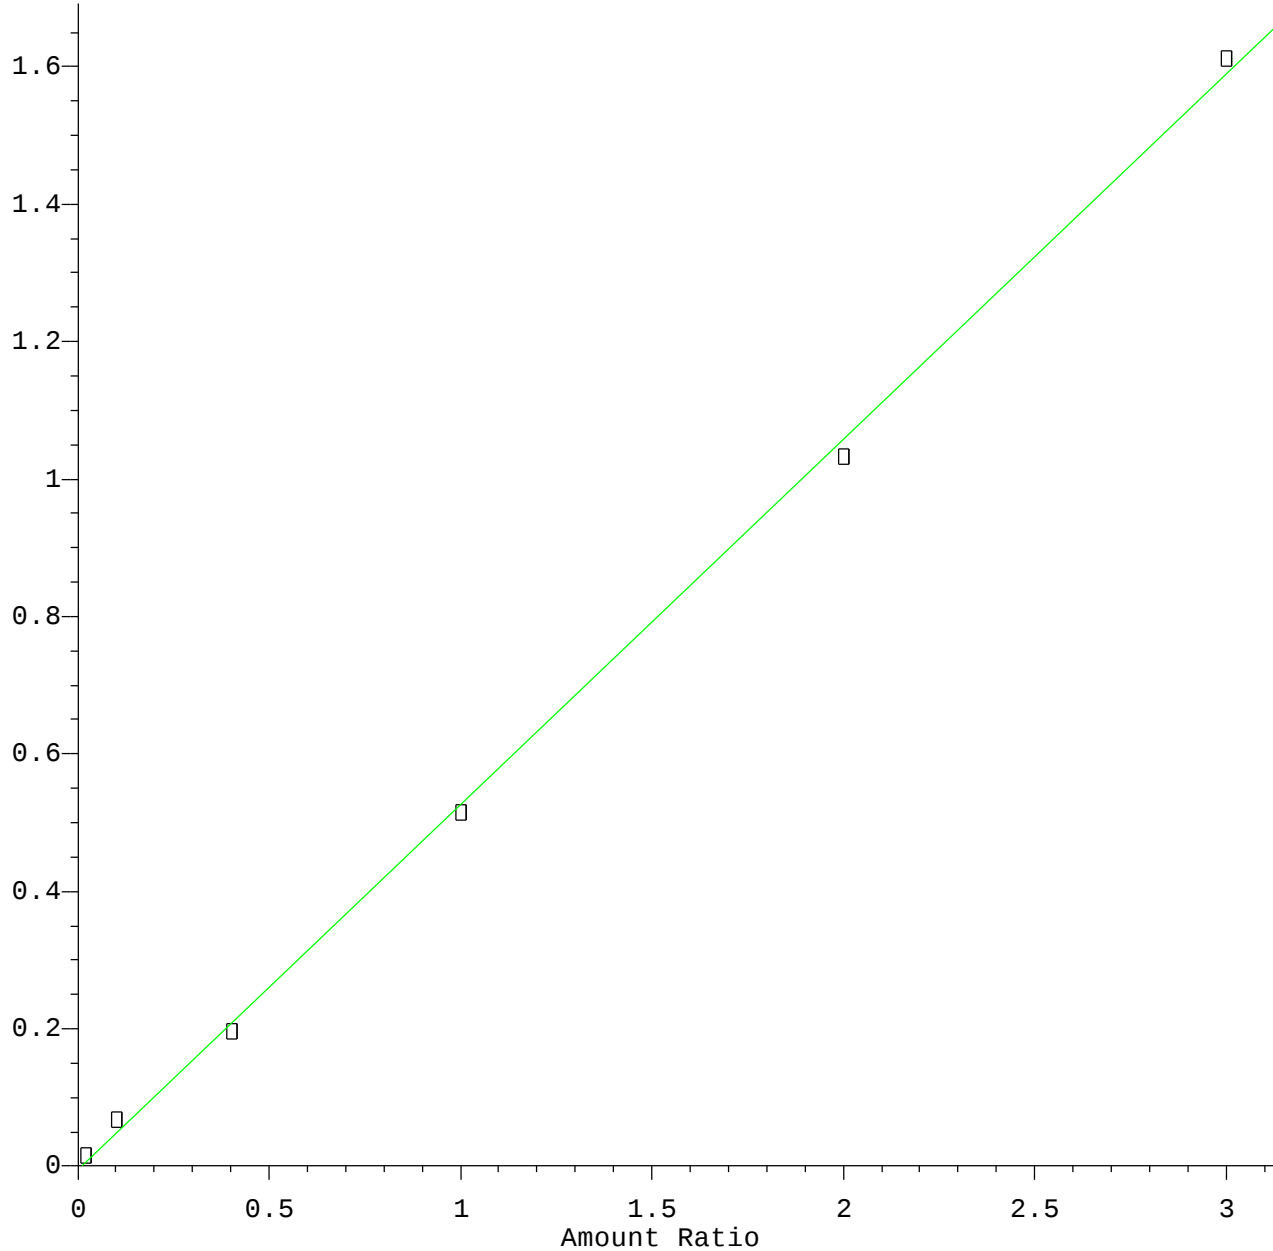


Resp Ratio = $5.31 \times 10^{-1} \times \text{Amt} - 5.35 \times 10^{-3}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X100920W.M
Calibration Table Last Updated: Sat Oct 10 06:09:09 2020


Bromochloromethane

Response Ratio

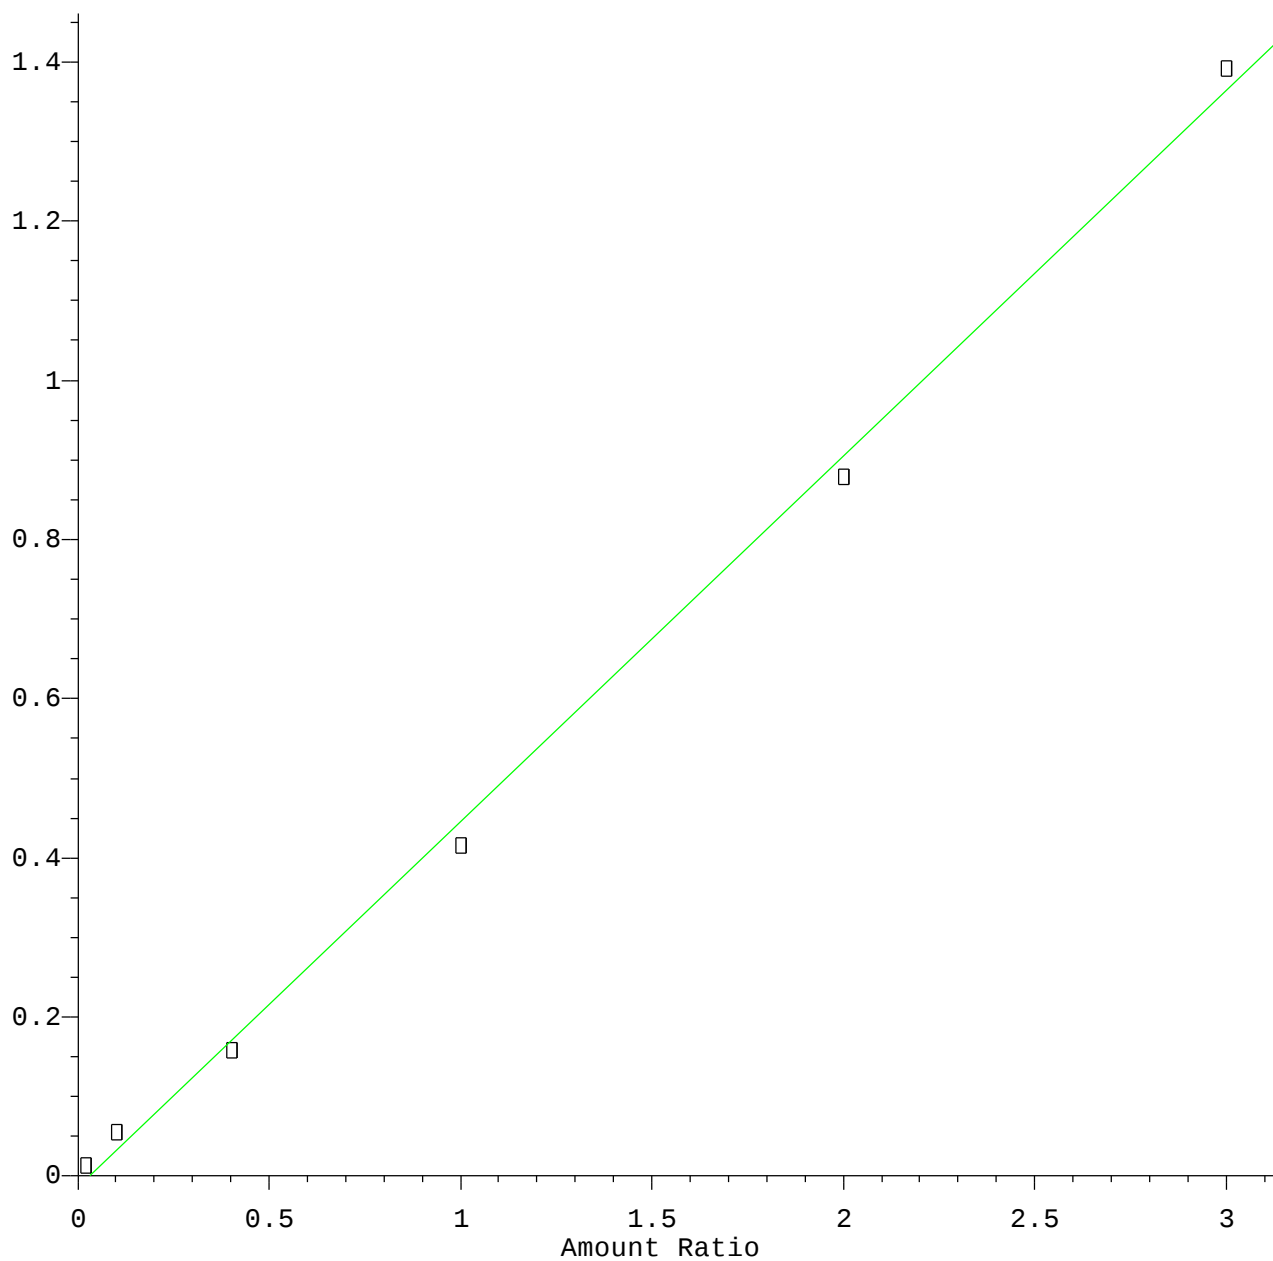

Resp Ratio = $4.59 \times 10^{-1} \times \text{Amt} - 1.40 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X100920W.M
Calibration Table Last Updated: Sat Oct 10 06:09:09 2020

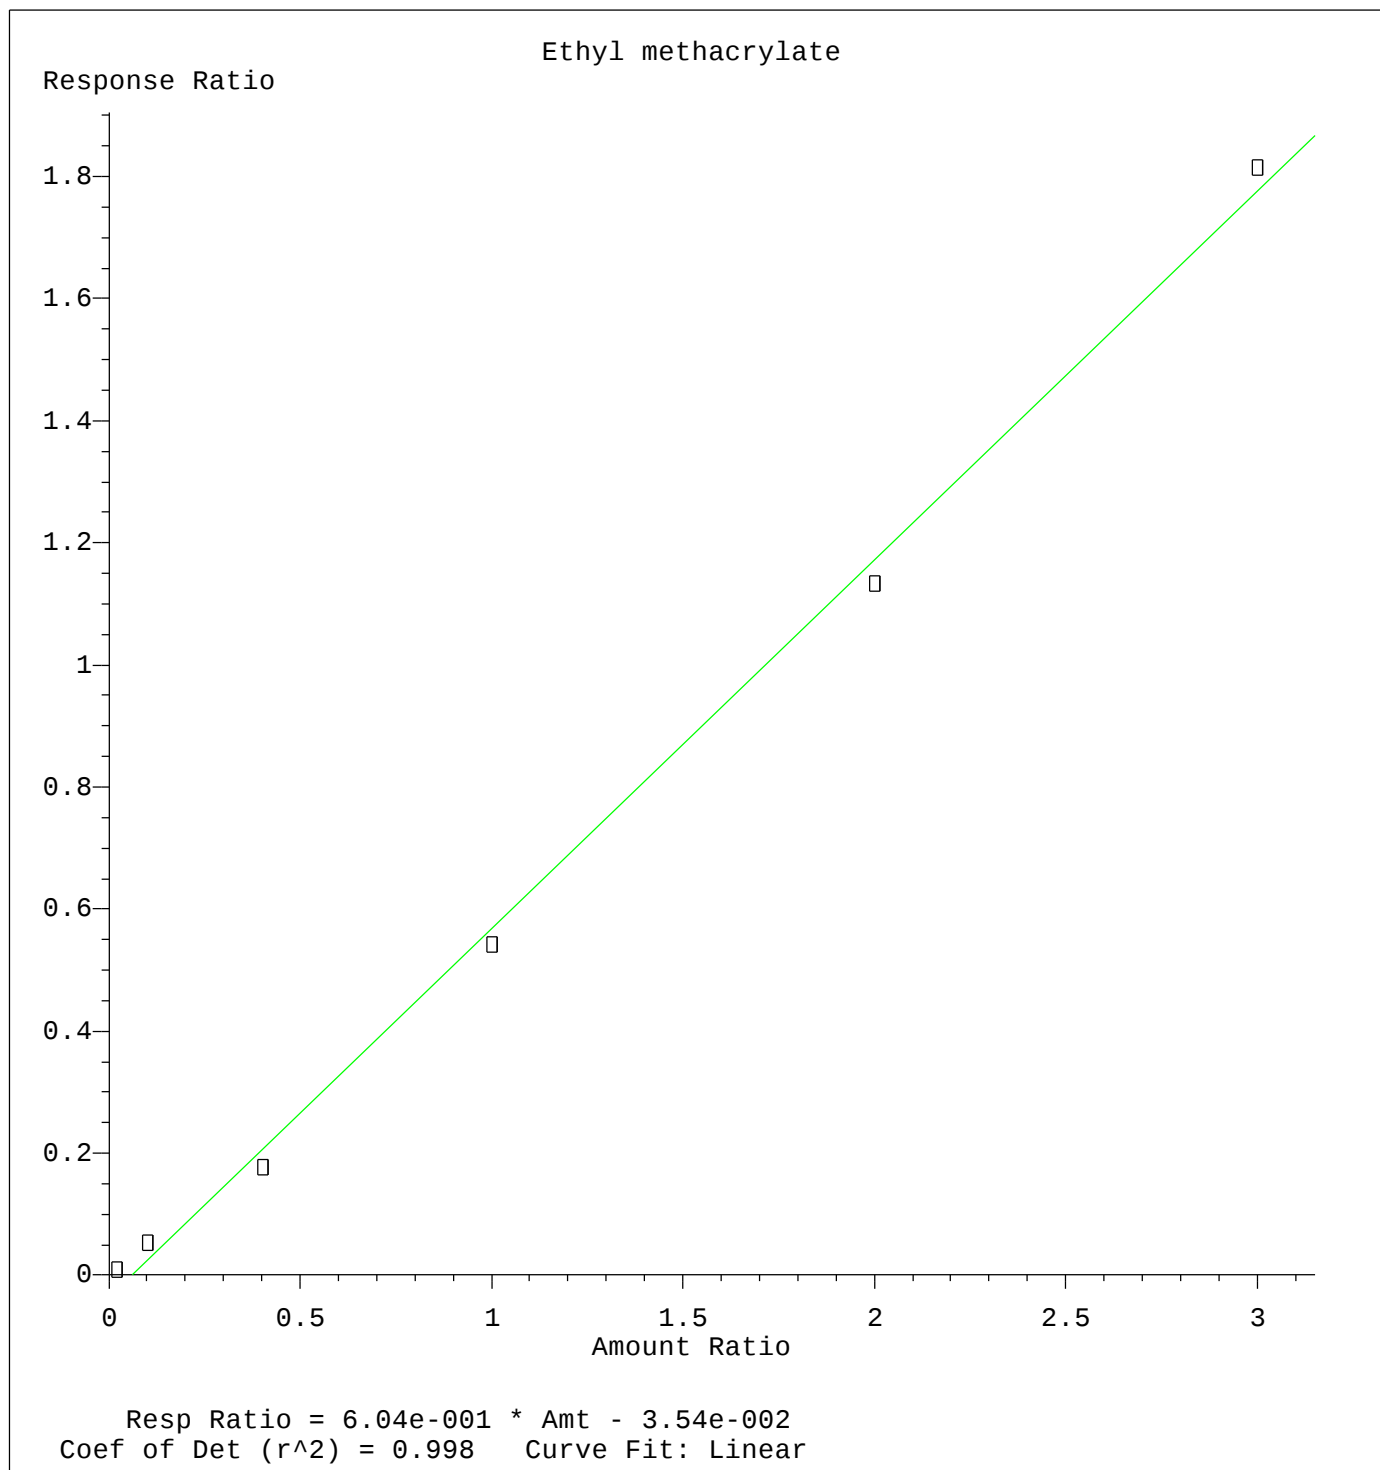

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X100920W.M
Calibration Table Last Updated: Sat Oct 10 06:09:09 2020

Tetrachloroethene

Response Ratio

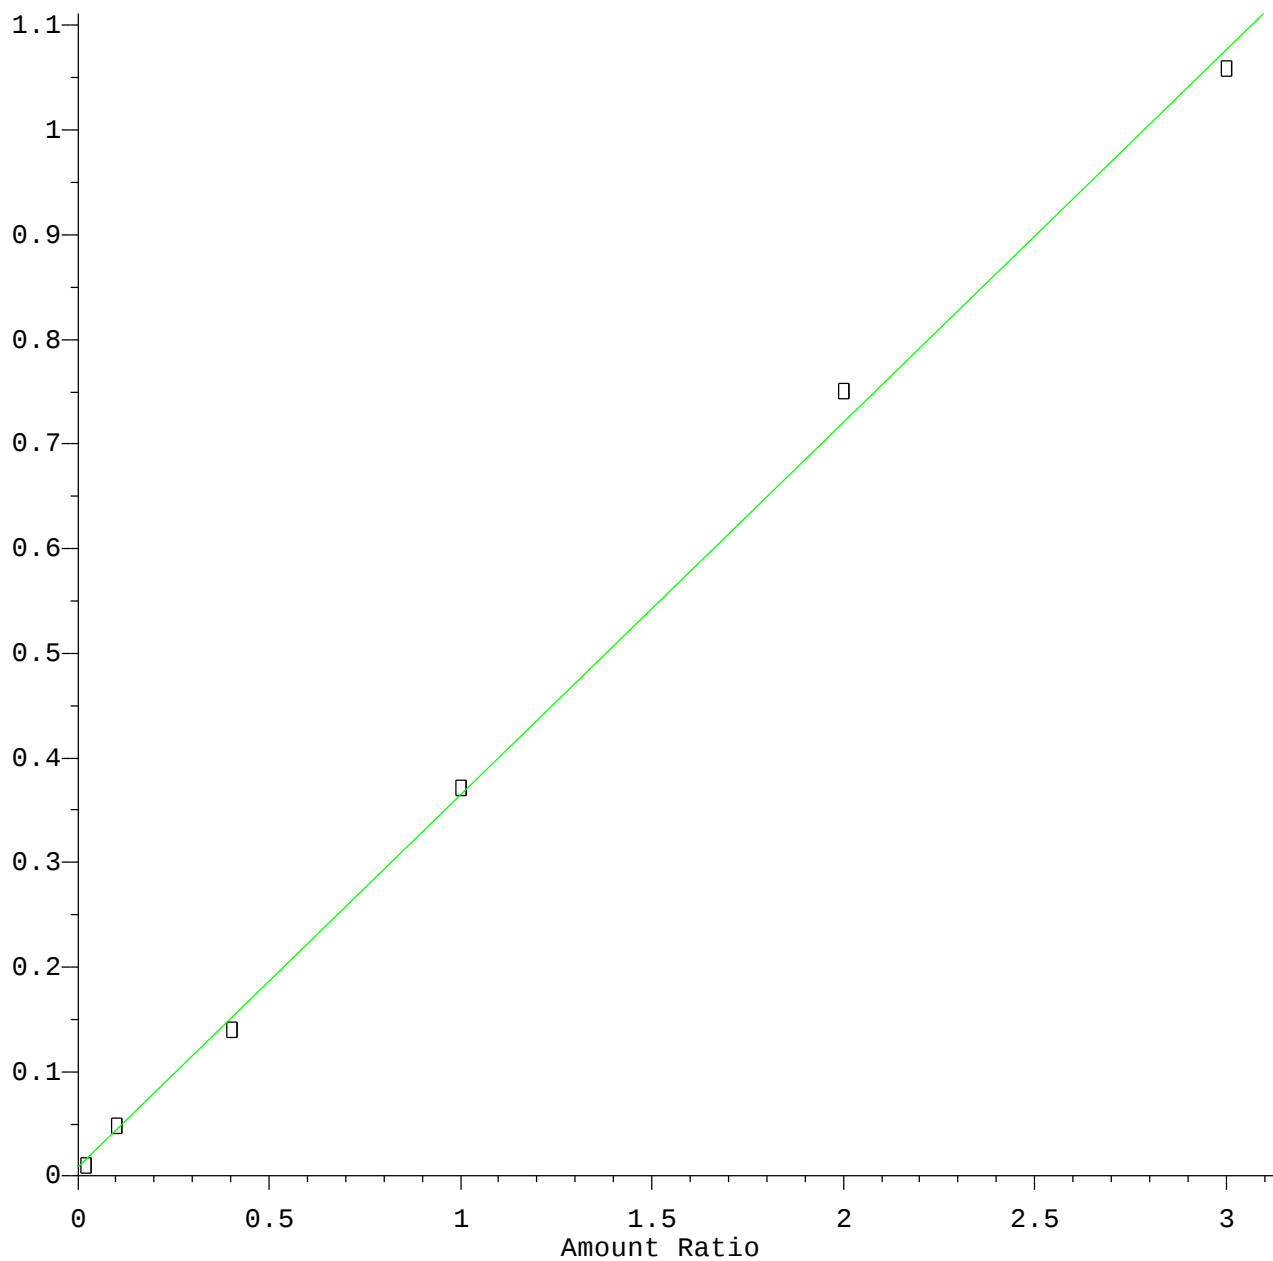


Resp Ratio = $3.56 \times 10^{-1} \times \text{Amt} + 8.66 \times 10^{-3}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X100920W.M
Calibration Table Last Updated: Sat Oct 10 06:09:09 2020

Naphthalene

Response Ratio

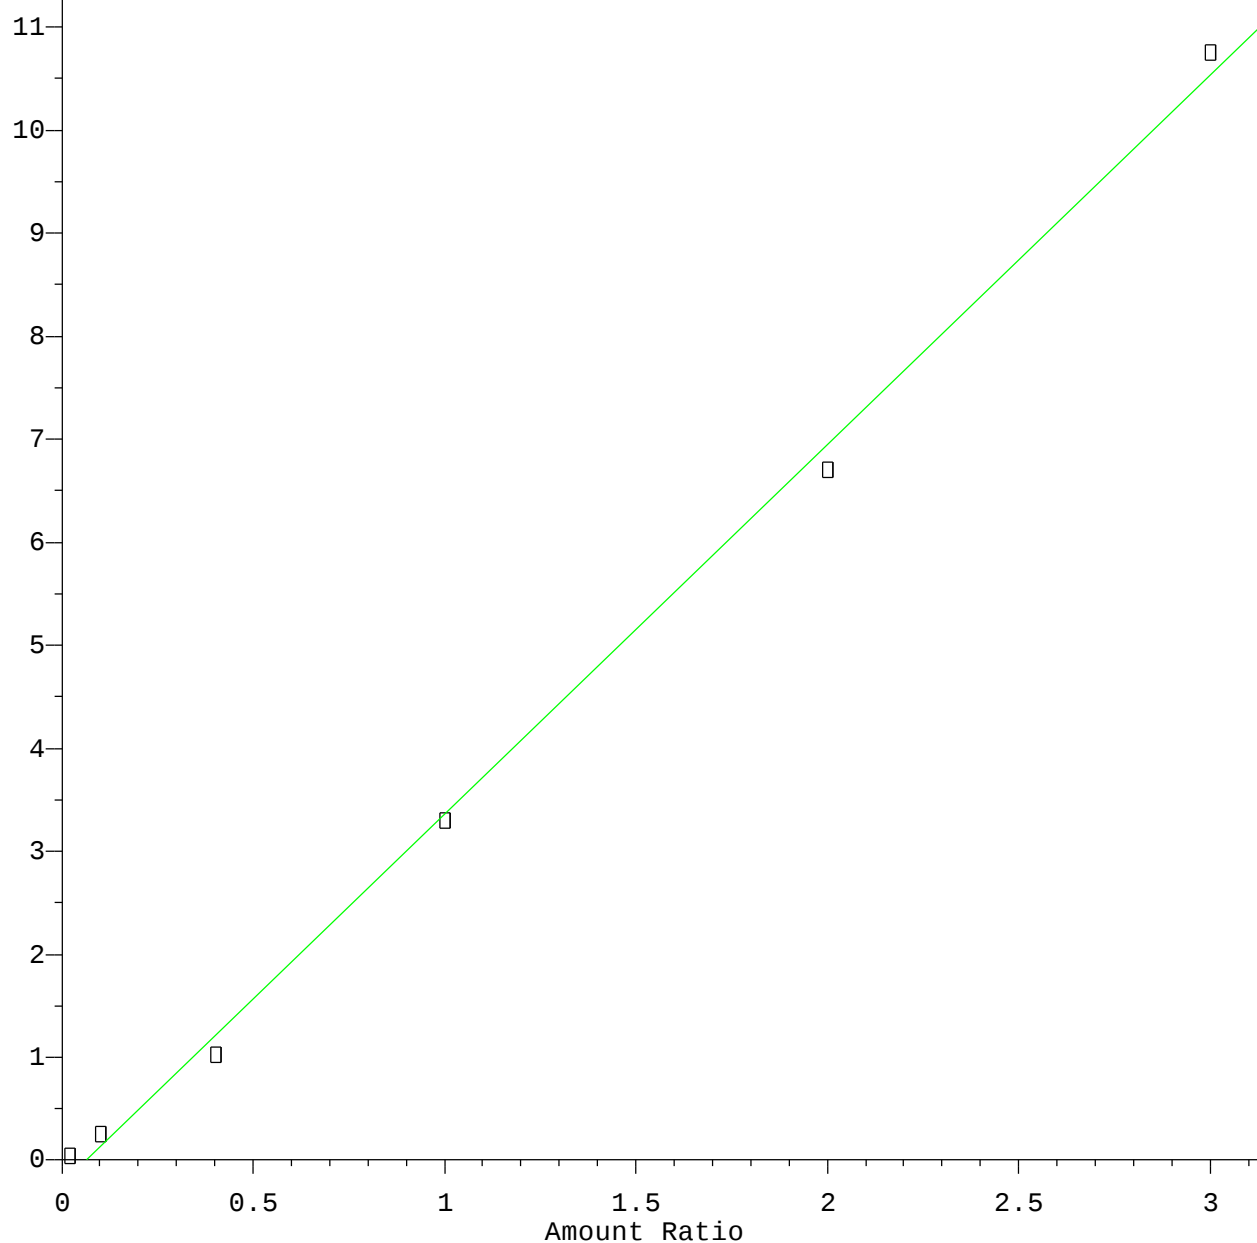


Resp Ratio = 3.58×10^0 * Amt - 2.21×10^{-1}
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X100920W.M
Calibration Table Last Updated: Sat Oct 10 06:09:09 2020


Dichlorodifluoromethane

Response Ratio

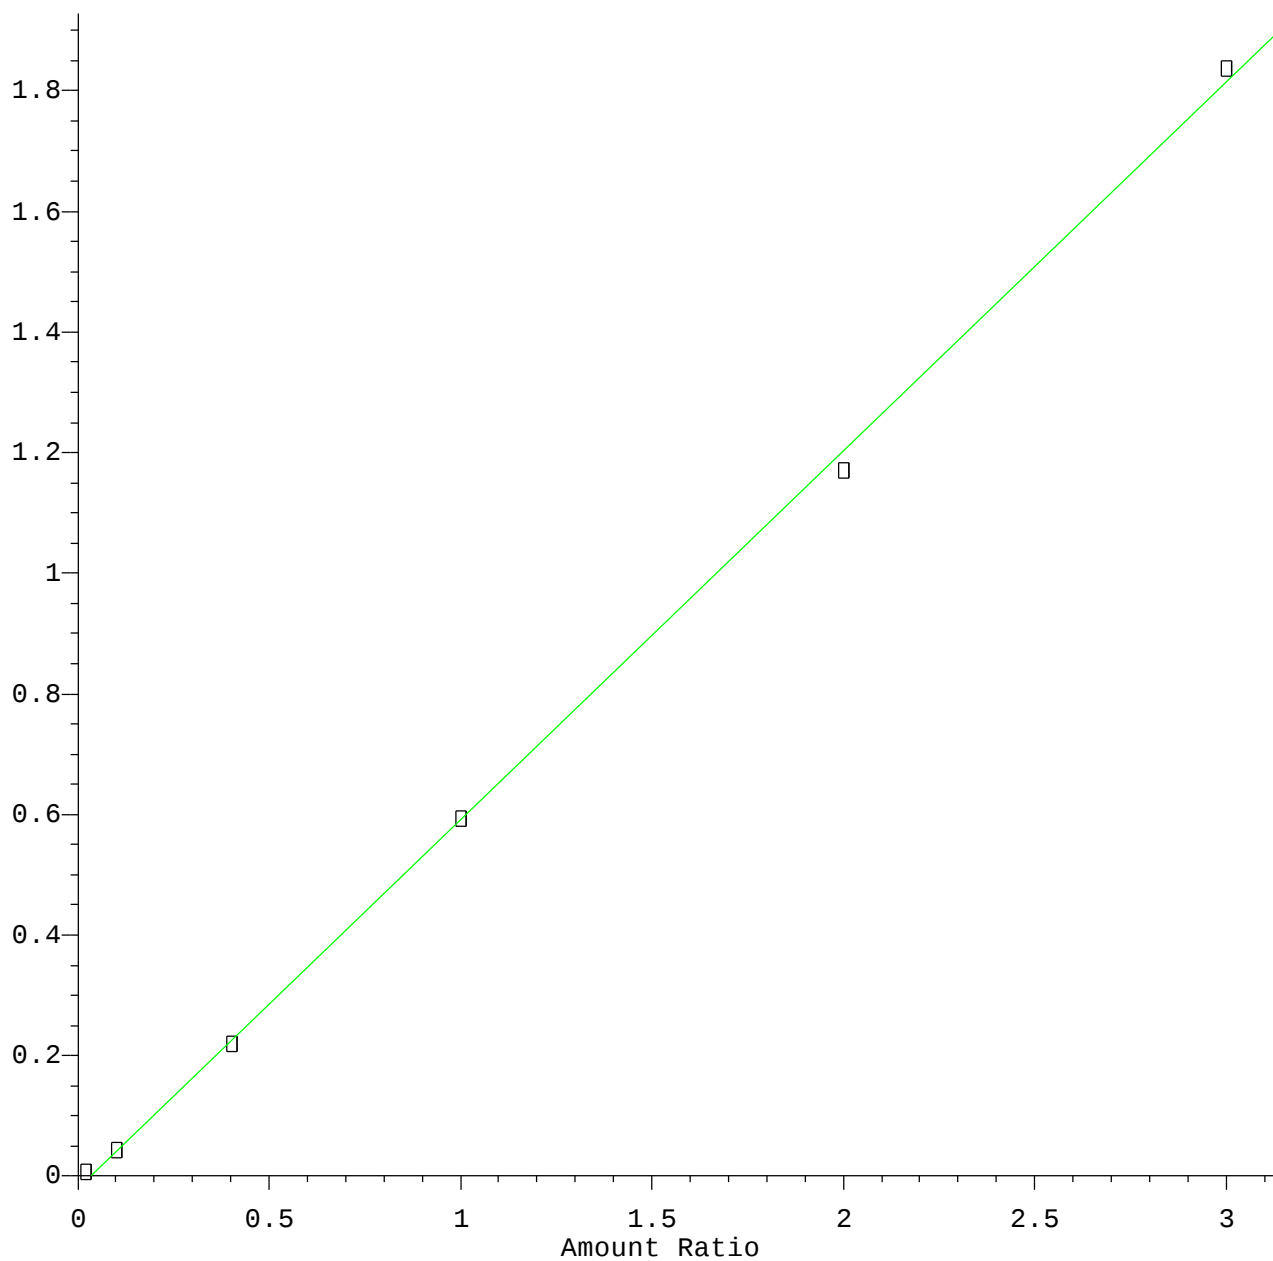


Resp Ratio = $6.11 \times 10^{-1} \times \text{Amt} - 1.98 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X100920W.M
Calibration Table Last Updated: Sat Oct 10 06:09:09 2020

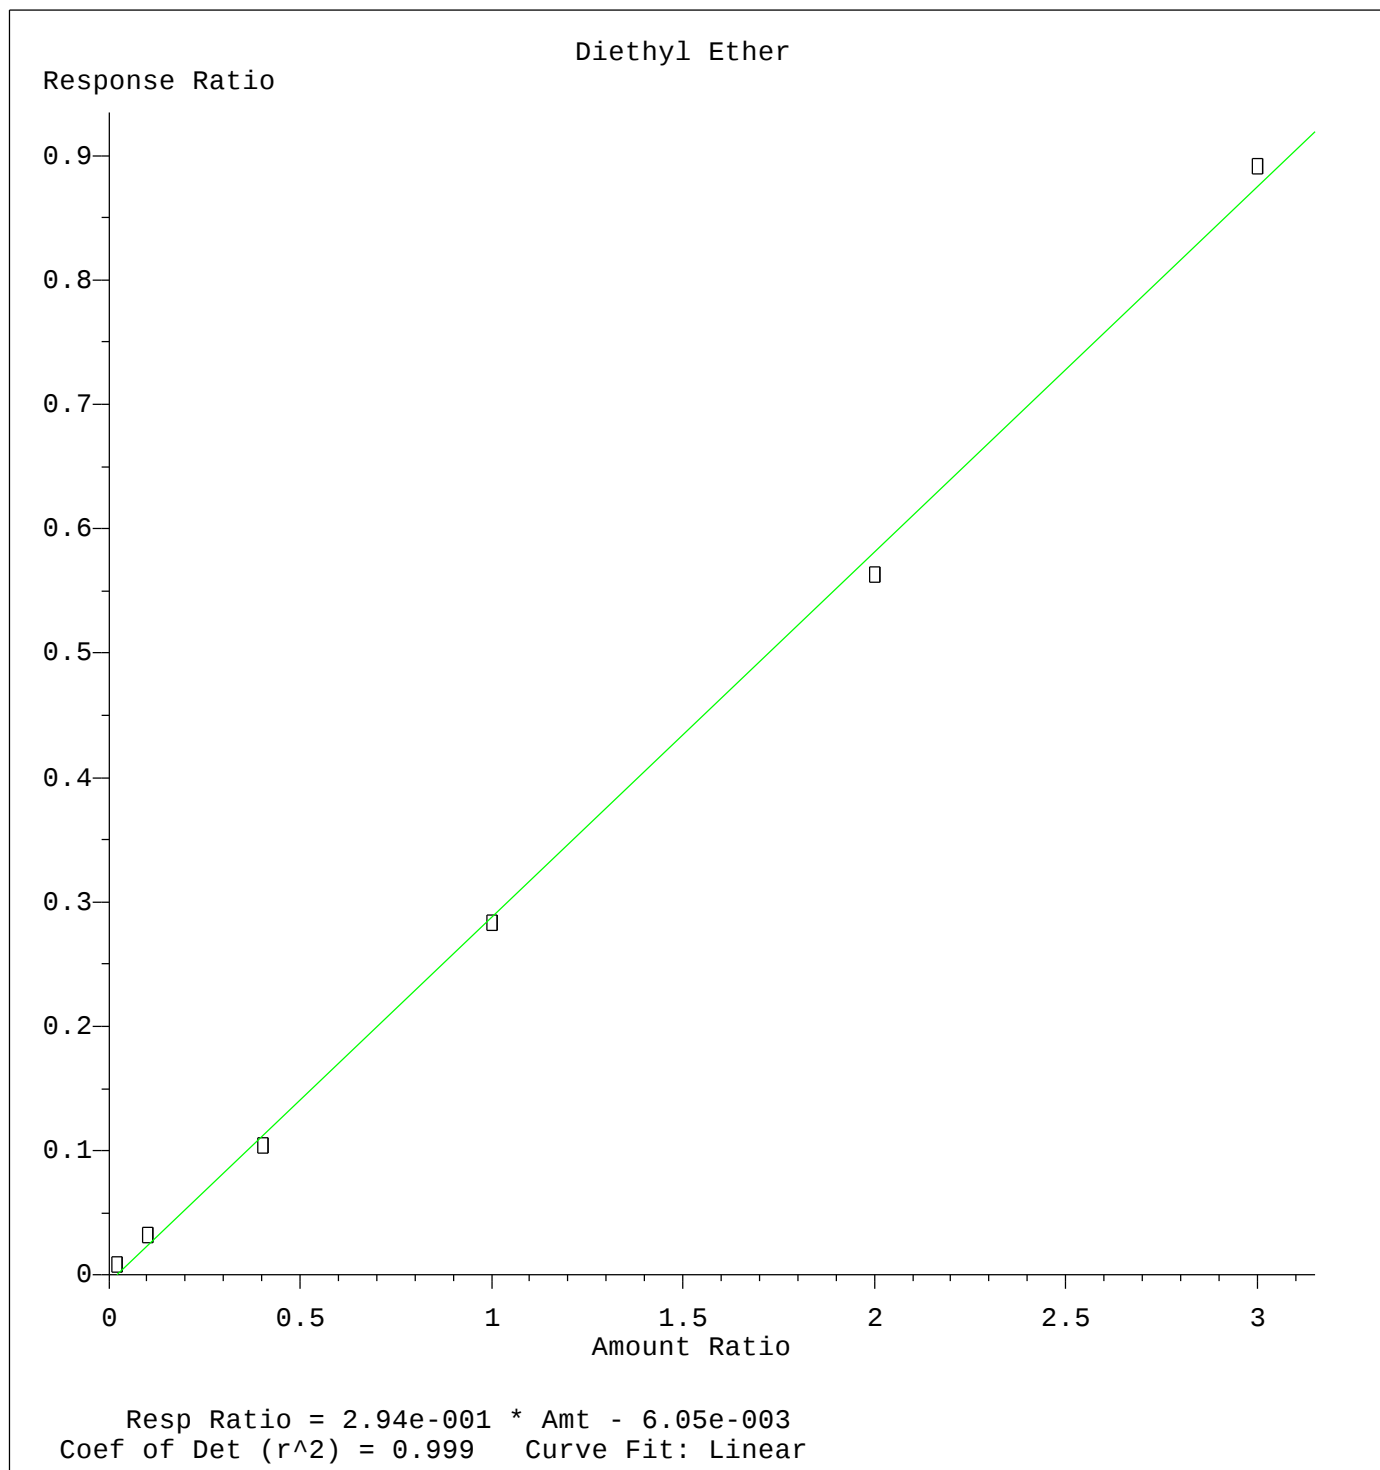

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X100920W.M
Calibration Table Last Updated: Sat Oct 10 06:09:09 2020

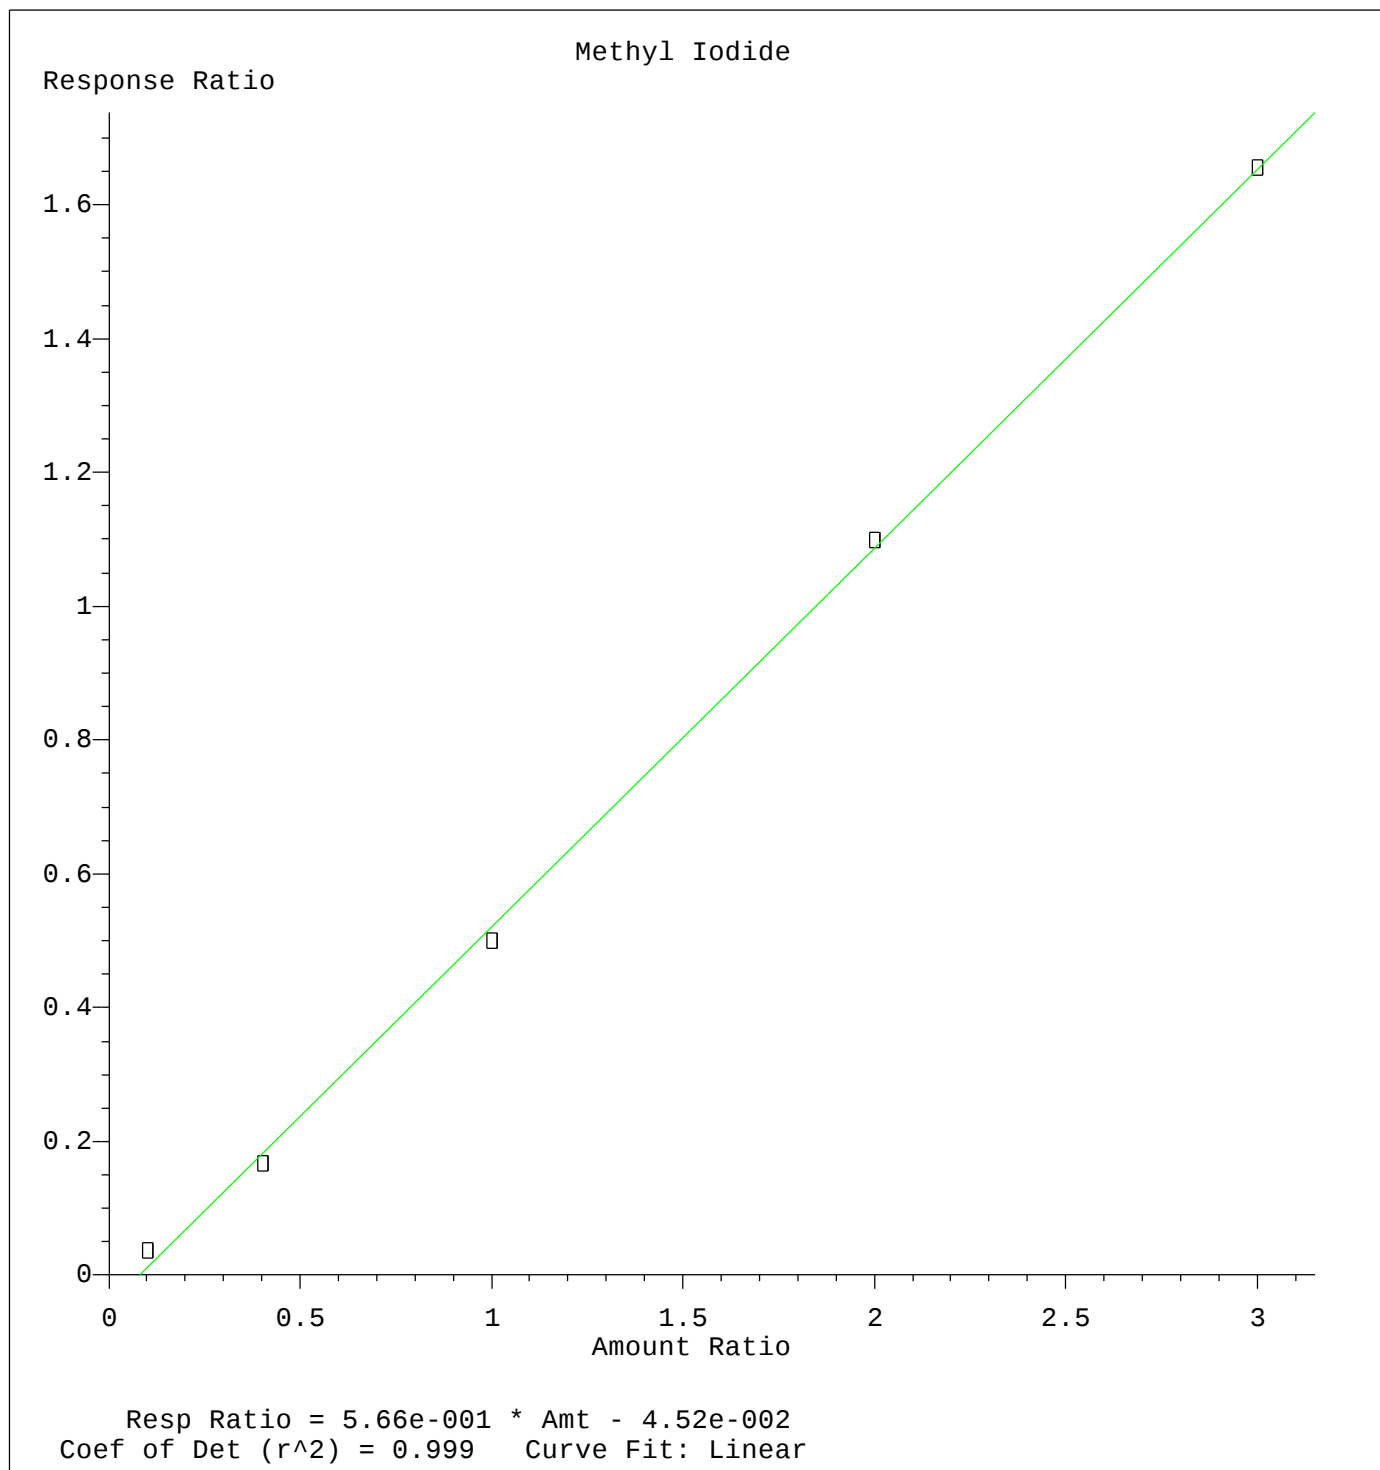

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X100920W.M
Calibration Table Last Updated: Sat Oct 10 06:09:09 2020