

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100920\
 Data File : VX018881.D
 Acq On : 10 Oct 2020 02:27
 Operator : JC/SP
 Sample : L4303-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FT-MW06S-20201002

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X100920W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.233	183	188	197	rVB10	5765	16181	1.55%	0.271%
2	2.575	237	244	250	rBV	18280	34700	3.32%	0.581%
3	2.837	279	287	293	rBV8	4652	10477	1.00%	0.175%
4	5.470	709	719	734	rVB	131762	383742	36.73%	6.423%
5	5.629	734	745	758	rBV	227099	625514	59.87%	10.469%
6	6.031	799	811	824	rBV	148571	392926	37.61%	6.577%
7	6.830	933	942	954	rBV	330278	773042	74.00%	12.939%
8	8.695	1241	1248	1259	rBV	665335	1044716	100.00%	17.486%
9	10.098	1471	1478	1485	rBV	714621	953153	91.24%	15.953%
10	11.122	1639	1646	1655	rBV	614301	769360	73.64%	12.877%
11	12.061	1795	1800	1808	rVB	799328	958616	91.76%	16.045%
12	13.890	2095	2100	2106	rBV6	6571	12233	1.17%	0.205%


Sum of corrected areas: 5974660

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100920\
Data File : VX018881.D
Acq On : 10 Oct 2020 02:27
Operator : JC/SP
Sample : L4303-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FT-MW06S-20201002

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X100920W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

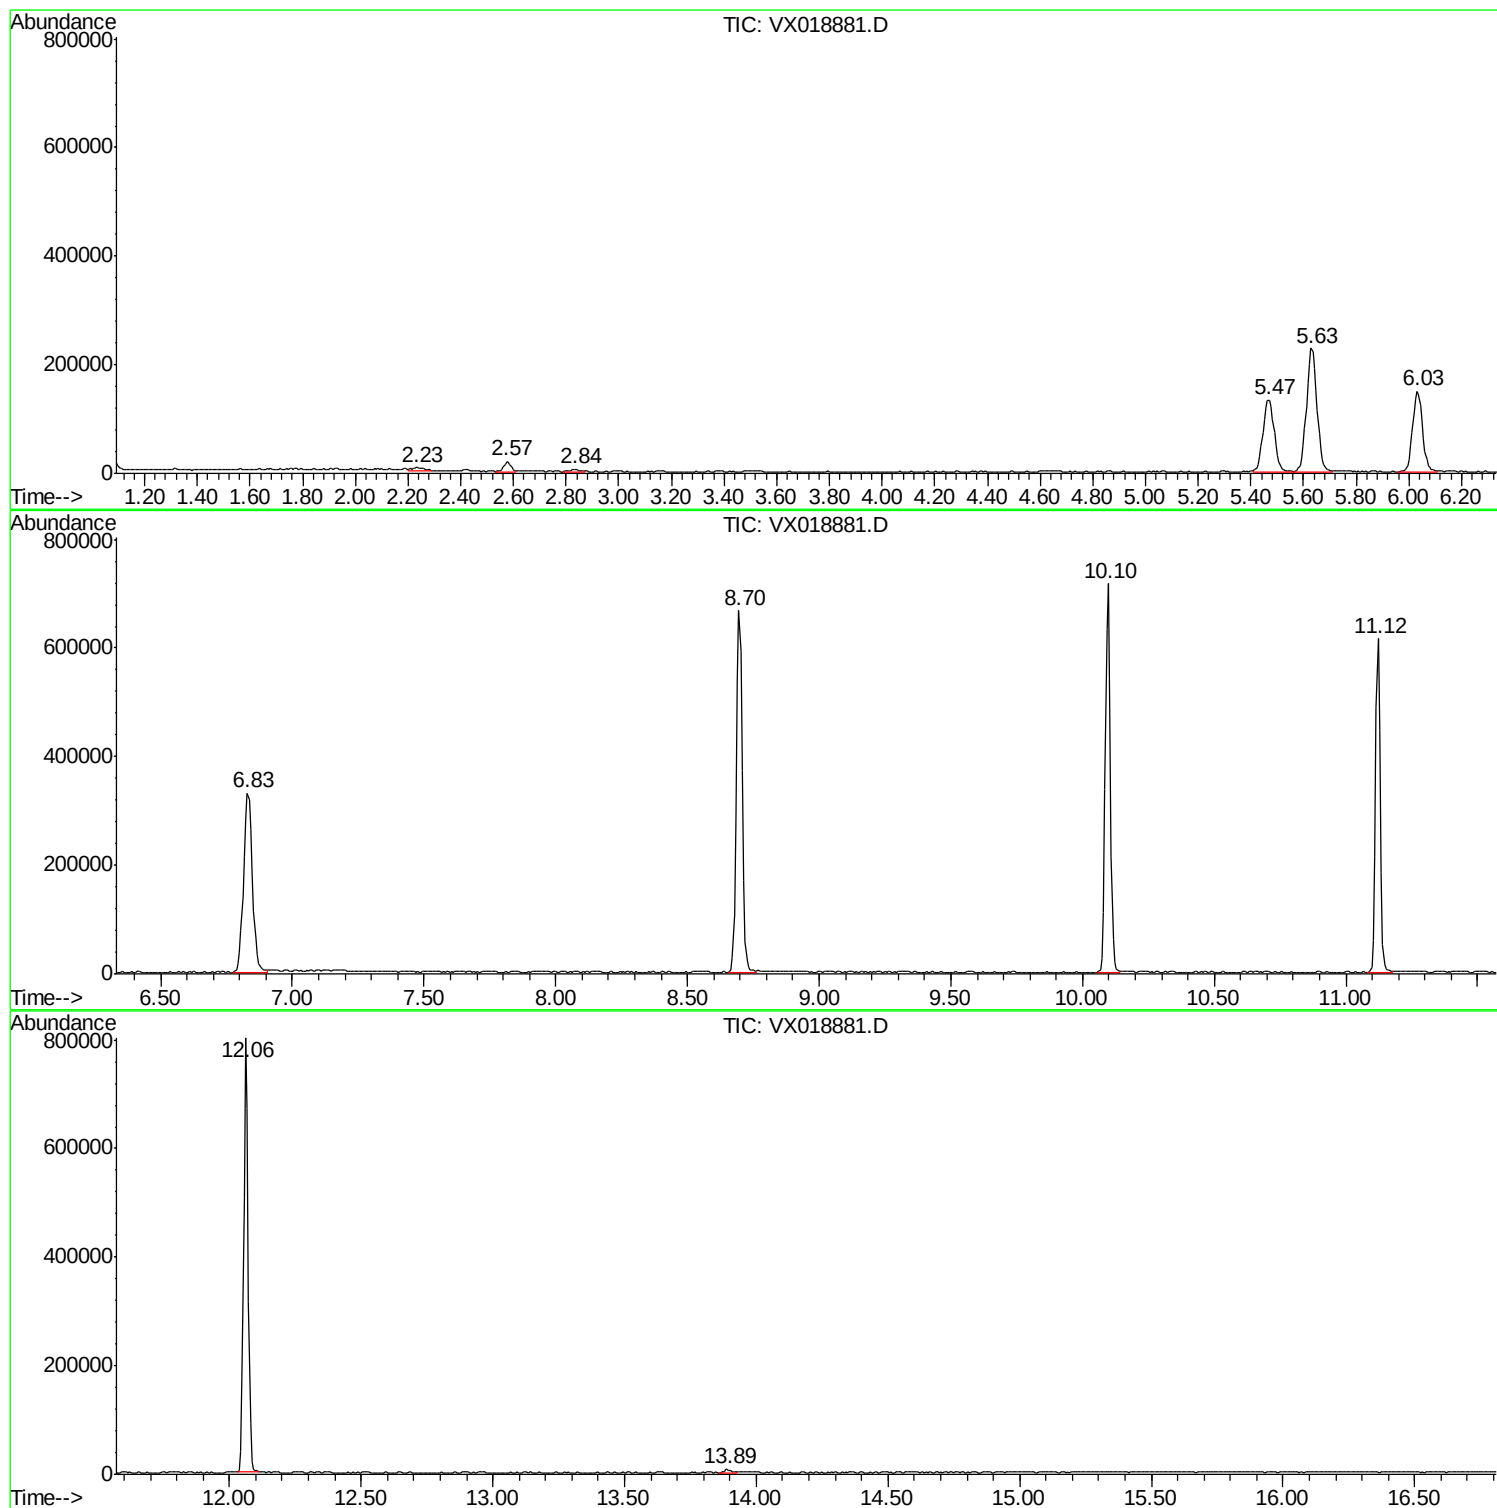

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX100920\
Data File : VX018881.D
Acq On : 10 Oct 2020 02:27
Operator : JC/SP
Sample : L4303-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FT-MW06S-20201002

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X100920W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX100920\
Data File : VX018881.D
Acq On : 10 Oct 2020 02:27
Operator : JC/SP
Sample : L4303-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FT-MW06S-20201002

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X100920W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc