

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100920\
 Data File : VX018885.D
 Acq On : 10 Oct 2020 03:58
 Operator : JC/SP
 Sample : L4303-05
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FC-MW10S-20201002

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X100920W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.294	28	34	36	rBV3	13095	23443	2.14%	0.375%
2	2.574	236	244	252	rBV	17268	35476	3.23%	0.568%
3	5.470	702	719	732	rBV	138465	403521	36.77%	6.459%
4	5.635	732	746	758	rBV	227869	650389	59.27%	10.411%
5	6.031	798	811	825	rBV2	153953	403132	36.74%	6.453%
6	6.830	932	942	955	rBV	345892	826218	75.30%	13.225%
7	8.537	1216	1222	1226	rBV	8542	15860	1.45%	0.254%
8	8.695	1241	1248	1258	rBV	711781	1097303	100.00%	17.564%
9	10.097	1472	1478	1487	rBV	746617	988718	90.10%	15.826%
10	11.122	1640	1646	1654	rBV	637125	777900	70.89%	12.452%
11	12.060	1794	1800	1808	rBV	833883	1005964	91.68%	16.102%
12	13.889	2096	2100	2108	rBV2	11521	19390	1.77%	0.310%


Sum of corrected areas: 6247314

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100920\
Data File : VX018885.D
Acq On : 10 Oct 2020 03:58
Operator : JC/SP
Sample : L4303-05
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FC-MW10S-20201002

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X100920W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

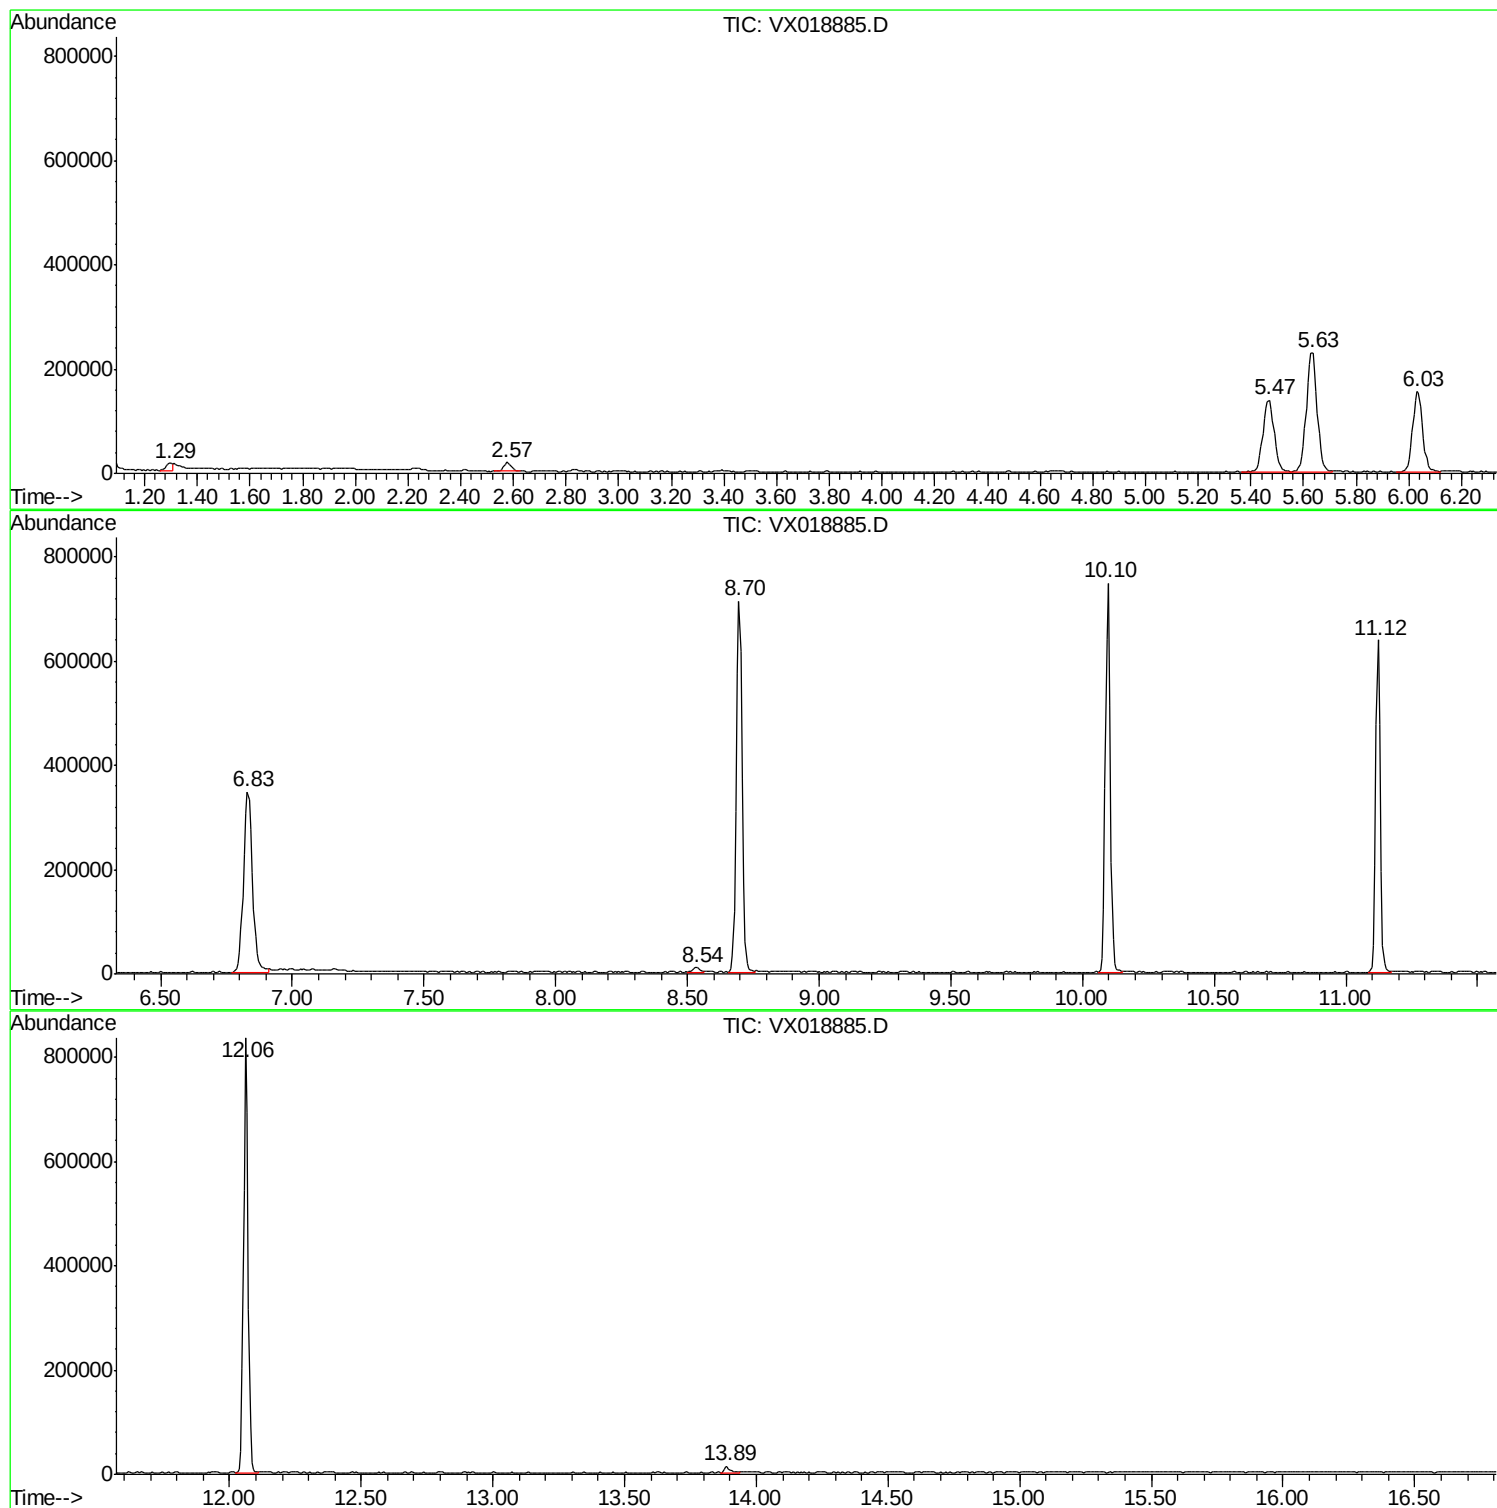

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX100920\
Data File : VX018885.D
Acq On : 10 Oct 2020 03:58
Operator : JC/SP
Sample : L4303-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FC-MW10S-20201002

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X100920W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX100920\
Data File : VX018885.D
Acq On : 10 Oct 2020 03:58
Operator : JC/SP
Sample : L4303-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FC-MW10S-20201002

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X100920W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc