

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100920\
 Data File : VX018887.D
 Acq On : 10 Oct 2020 04:43
 Operator : JC/SP
 Sample : L4255-13
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FT-PZ-458I-20200928

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X100920W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.331	33	40	41	rBV2	6005	11412	1.08%	0.185%
2	5.464	707	718	730	rBV2	135712	394918	37.25%	6.417%
3	5.629	733	745	757	rBV	220712	619447	58.43%	10.065%
4	6.031	800	811	825	rBV	151844	397794	37.52%	6.464%
5	6.830	932	942	953	rBV	332148	810526	76.46%	13.170%
6	7.190	993	1001	1010	rVB2	38687	96356	9.09%	1.566%
7	8.695	1241	1248	1259	rBV	692542	1060120	100.00%	17.226%
8	10.098	1472	1478	1489	rBV	723927	972274	91.71%	15.798%
9	11.122	1640	1646	1654	rBV	619684	772188	72.84%	12.547%
10	12.061	1795	1800	1810	rBV	806519	981452	92.58%	15.947%
11	12.256	1826	1832	1836	rBV4	7370	12951	1.22%	0.210%
12	13.884	2095	2099	2105	rBV2	16536	24889	2.35%	0.404%


Sum of corrected areas: 6154327

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100920\
Data File : VX018887.D
Acq On : 10 Oct 2020 04:43
Operator : JC/SP
Sample : L4255-13
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FT-PZ-458I-20200928

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X100920W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

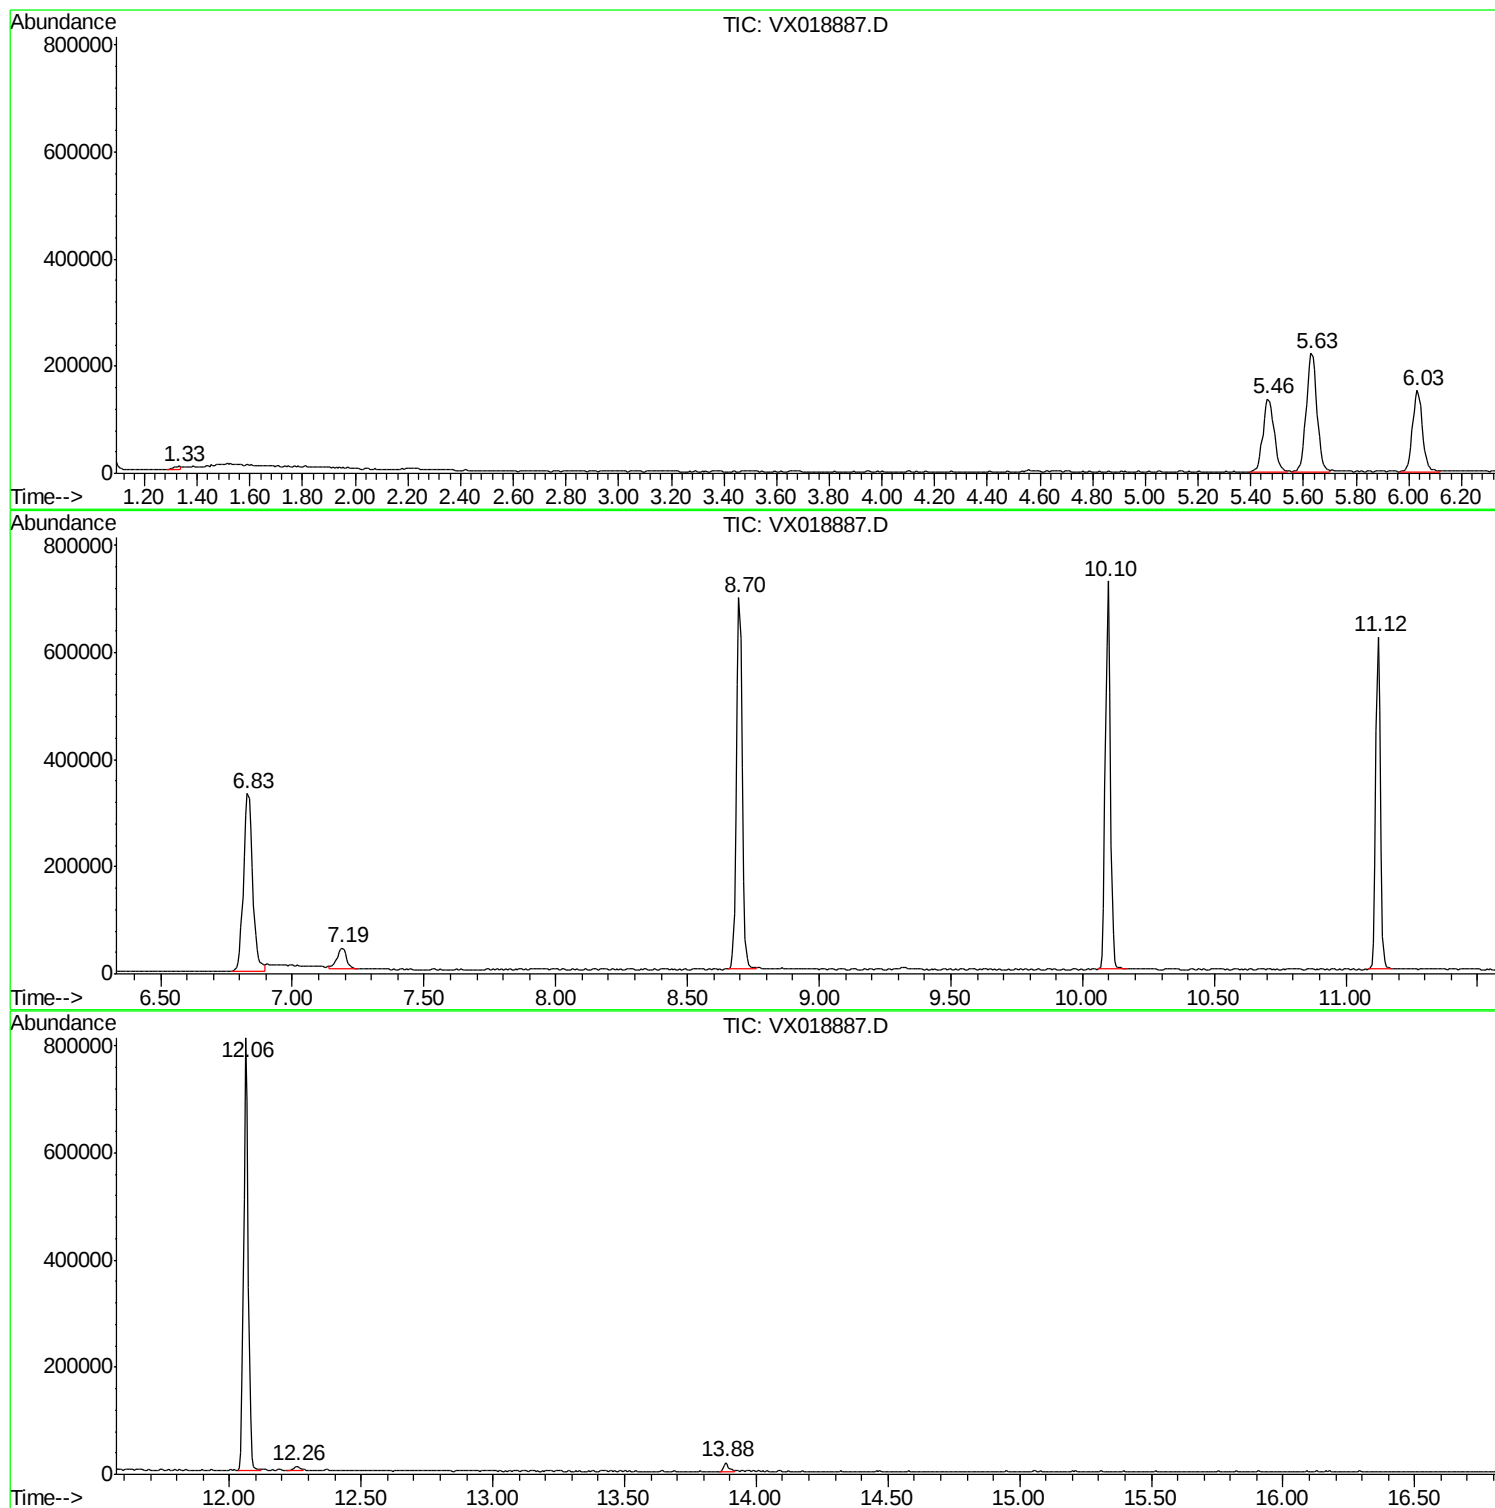

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX100920\
Data File : VX018887.D
Acq On : 10 Oct 2020 04:43
Operator : JC/SP
Sample : L4255-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FT-PZ-458I-20200928

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X100920W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX100920\
Data File : VX018887.D
Acq On : 10 Oct 2020 04:43
Operator : JC/SP
Sample : L4255-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FT-PZ-458I-20200928

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X100920W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc