

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100923\
 Data File : VX038166.D
 Acq On : 09 Oct 2023 13:04
 Operator : JC/MD
 Sample : 04724-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TRIP-BLANK

Quant Time: Oct 10 00:54:57 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 05 15:27:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	116134	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	210352	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	203478	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	101508	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	85919	45.997	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	92.000%
35) Dibromofluoromethane	5.391	113	68955	45.493	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	90.980%
50) Toluene-d8	8.647	98	261297	45.114	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	90.220%#
62) 4-Bromofluorobenzene	11.079	95	94526	43.049	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	86.100%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100923\
Data File : VX038166.D
Acq On : 09 Oct 2023 13:04
Operator : JC/MD
Sample : 04724-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRIP-BLANK

Quant Time: Oct 10 00:54:57 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 05 15:27:13 2023
Response via : Initial Calibration




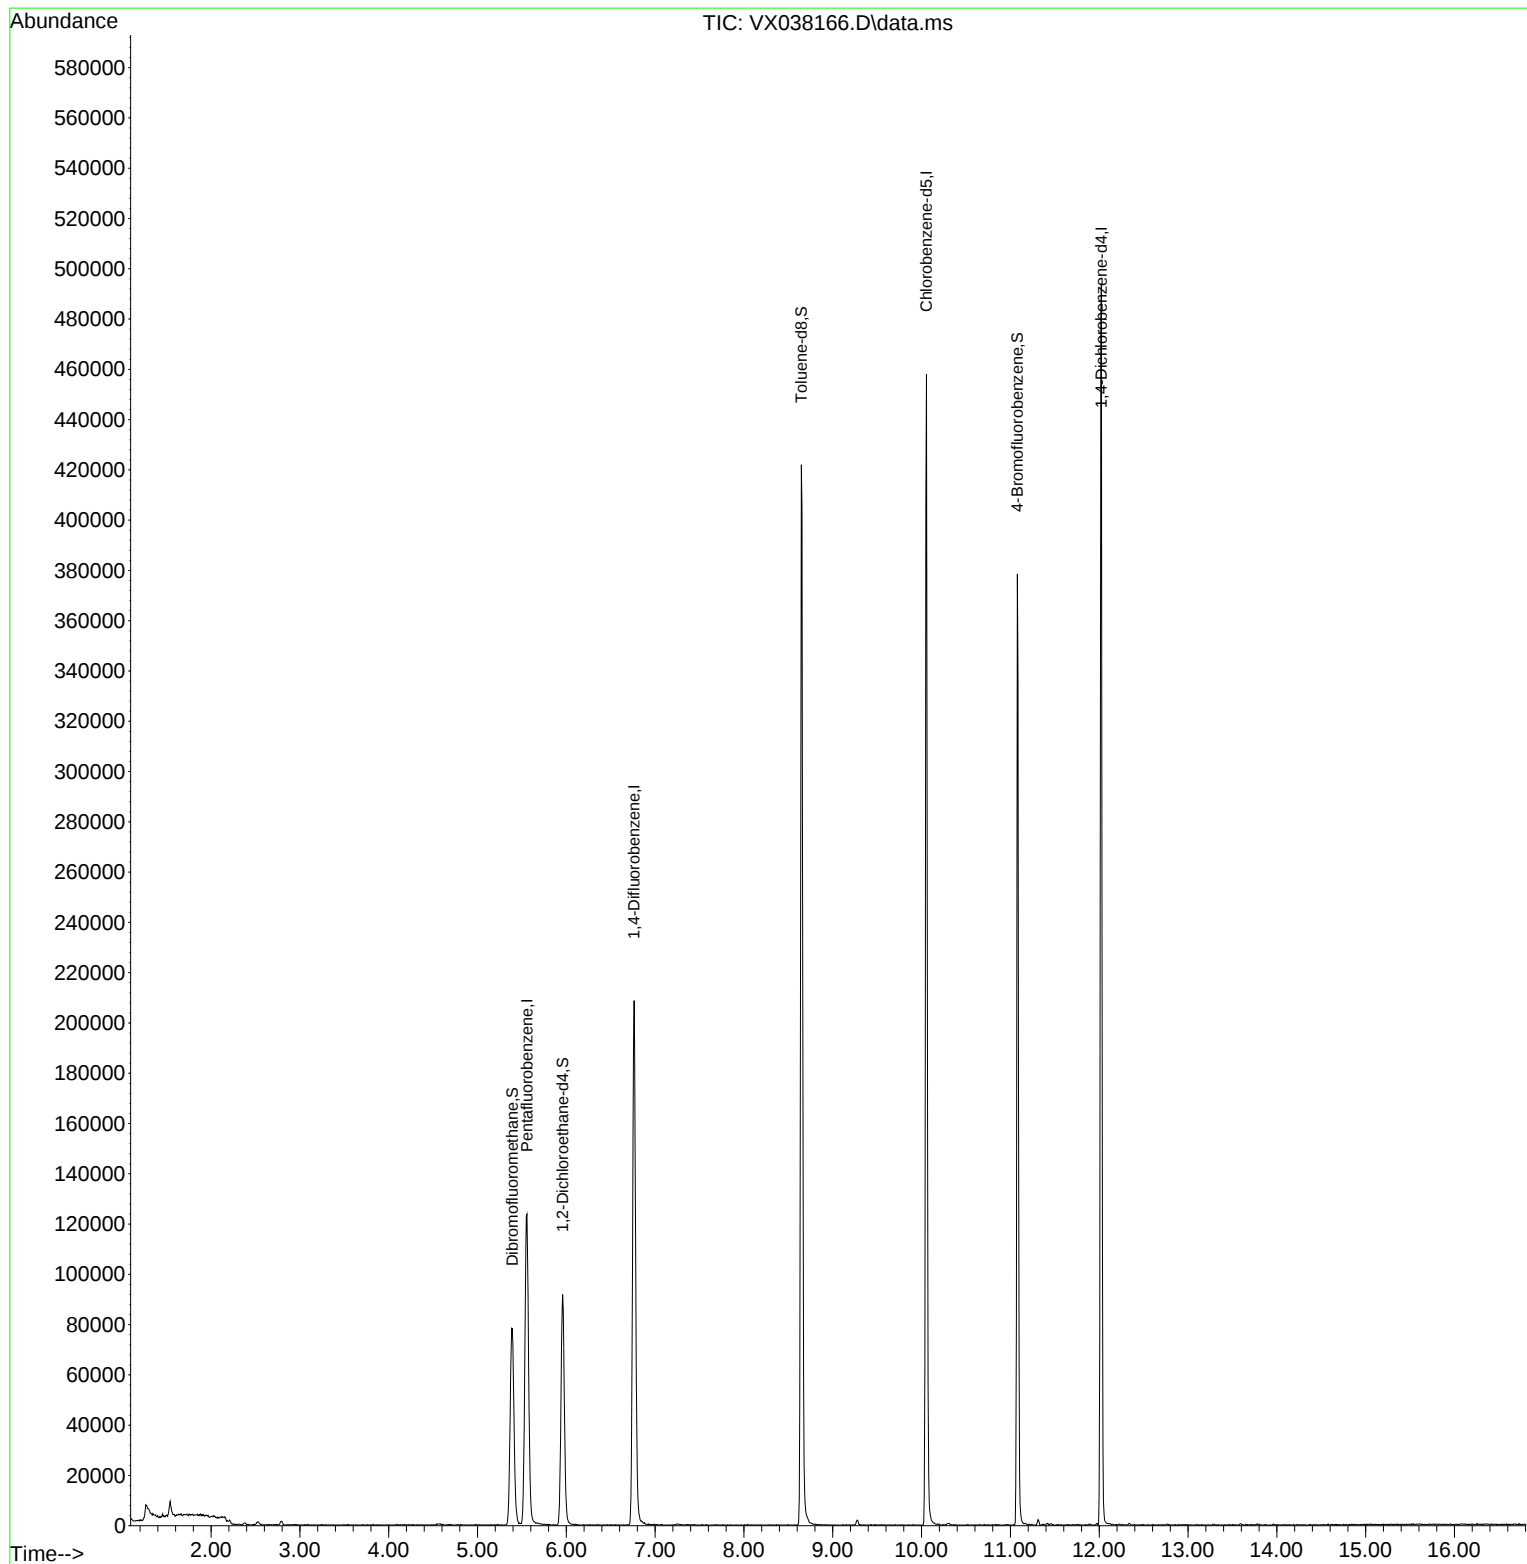


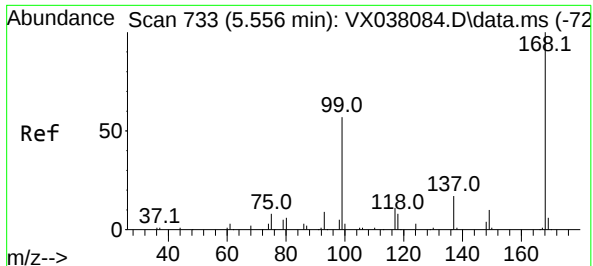

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 711
Delta R.T. -0.000 min
Lab File: VX038166.D
Acq: 09 Oct 2023 13:04




Instrument :
MSVOA_X
ClientSampleId :
TRIP-BLANK


Tgt Ion:168 Resp: 116134
Ion Ratio Lower Upper
168 100
99 59.6 56.6 85.0

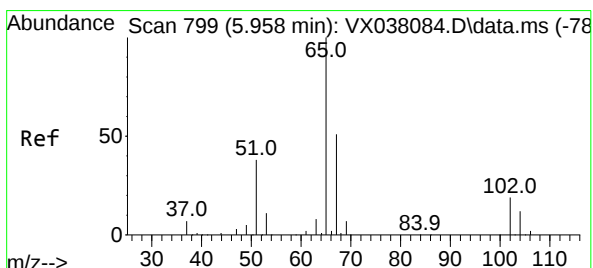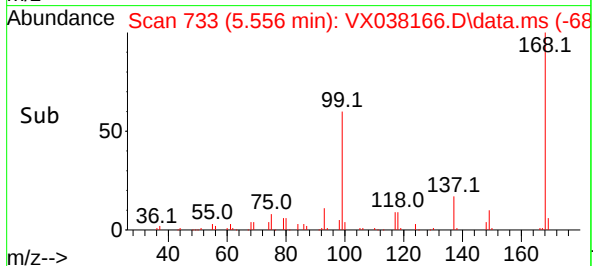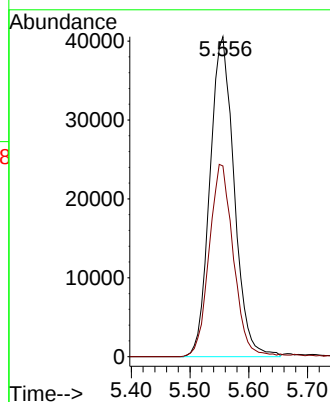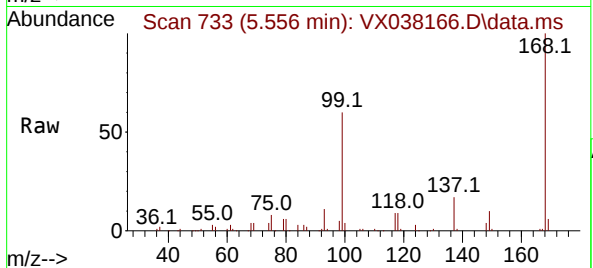

#33
1,2-Dichloroethane-d4
Concen: 45.997 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX038166.D
Acq: 09 Oct 2023 13:04

Tgt Ion: 65 Resp: 85919
Ion Ratio Lower Upper
65 100
67 52.0 0.0 100.2


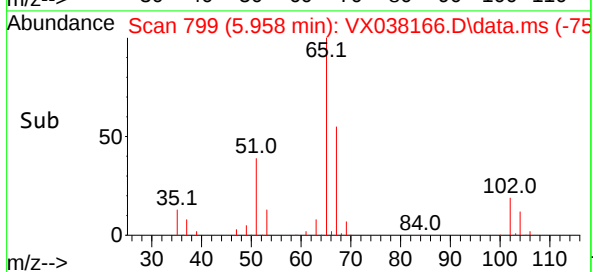
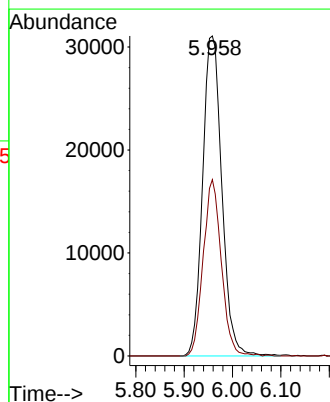
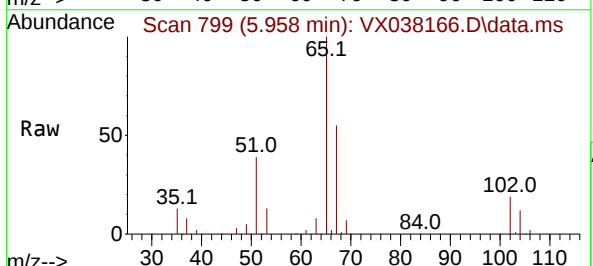


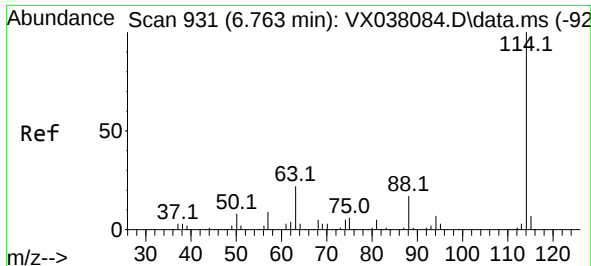

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX038166.D
Acq: 09 Oct 2023 13:04




Instrument :
MSVOA_X
ClientSampleId :
TRIP-BLANK


Tgt Ion:114 Resp: 210352
Ion Ratio Lower Upper
114 100
63 20.5 0.0 45.0
88 15.3 0.0 36.6

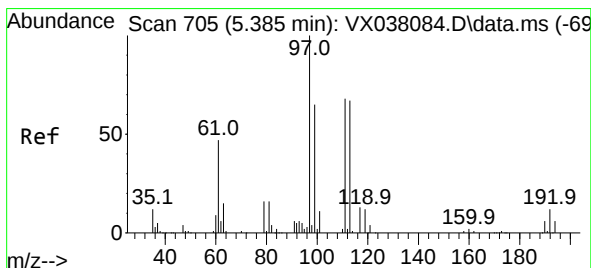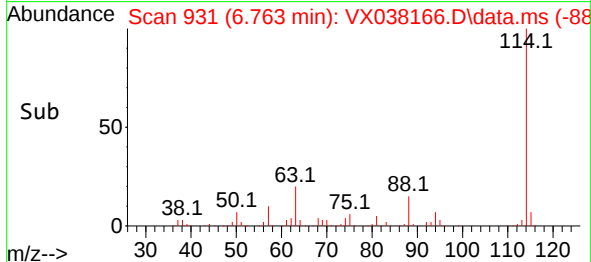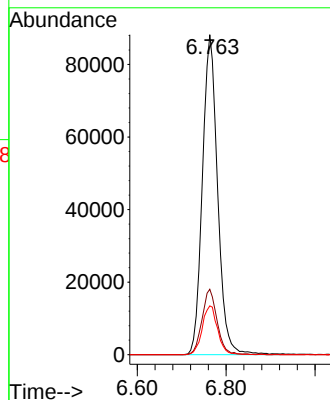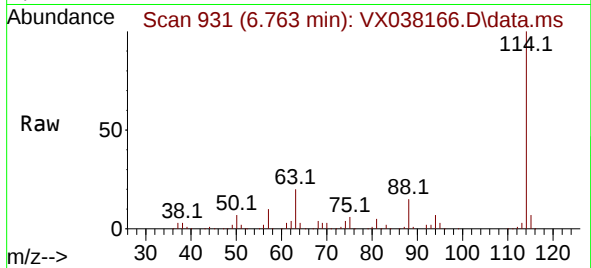

#35
Dibromofluoromethane
Concen: 45.493 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.006 min
Lab File: VX038166.D
Acq: 09 Oct 2023 13:04

Tgt Ion:113 Resp: 68955
Ion Ratio Lower Upper
113 100
111 102.0 82.9 124.3
192 18.7 13.3 19.9


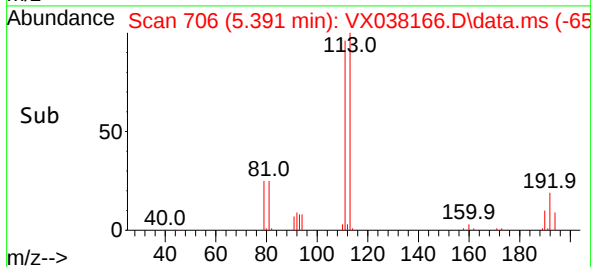
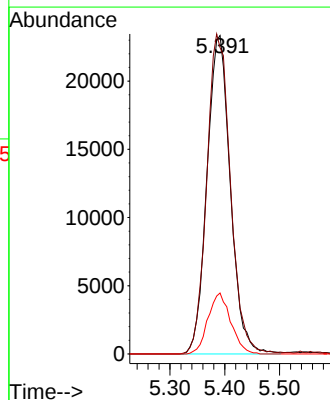
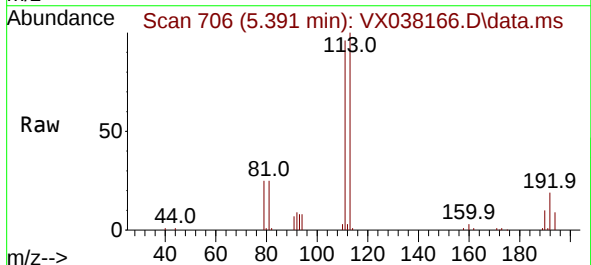


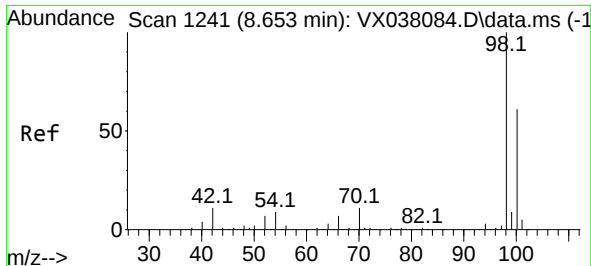

#50
Toluene-d8
Concen: 45.114 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX038166.D
Acq: 09 Oct 2023 13:04




Instrument :
MSVOA_X
ClientSampleId :
TRIP-BLANK


Tgt Ion: 98 Resp: 261297
Ion Ratio Lower Upper
98 100
100 62.5 53.1 79.7

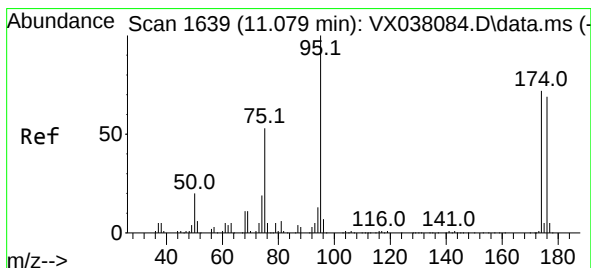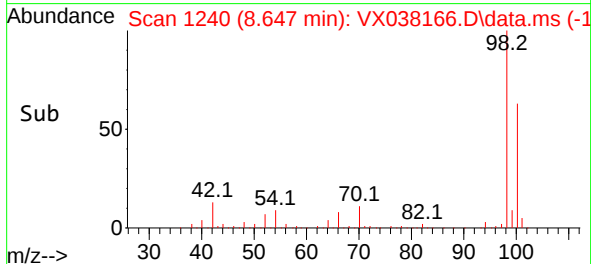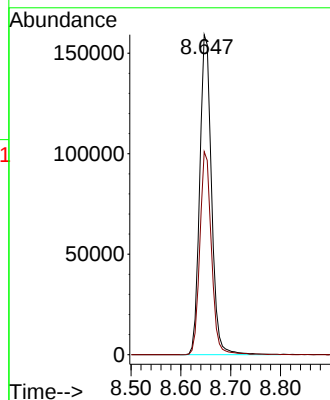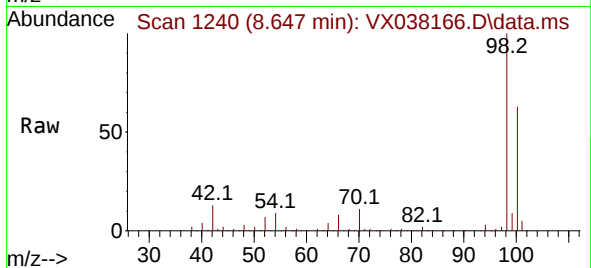

#62
4-Bromofluorobenzene
Concen: 43.049 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX038166.D
Acq: 09 Oct 2023 13:04

Tgt Ion: 95 Resp: 94526
Ion Ratio Lower Upper
95 100
174 80.3 0.0 135.6
176 77.4 0.0 131.0

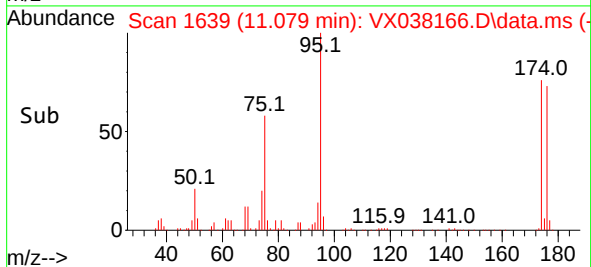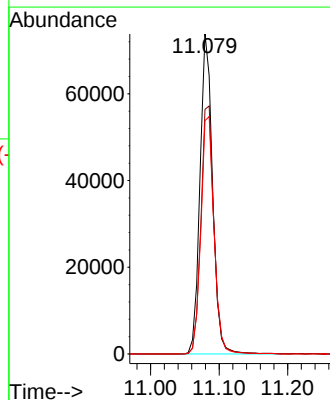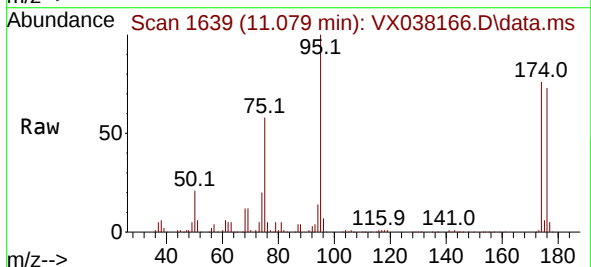

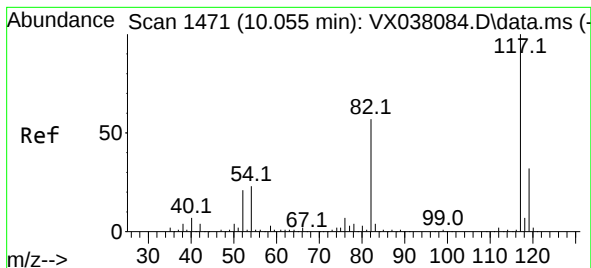

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX038166.D

Acq: 09 Oct 2023 13:04

Instrument :

MSVOA_X

ClientSampleId :

TRIP-BLANK





Tgt Ion:117 Resp: 203478

Ion Ratio Lower Upper

117 100

82 55.3 46.2 69.4

119 31.1 25.5 38.3

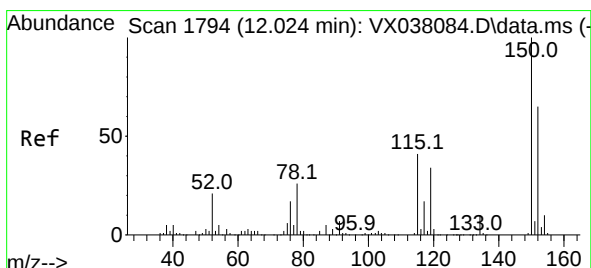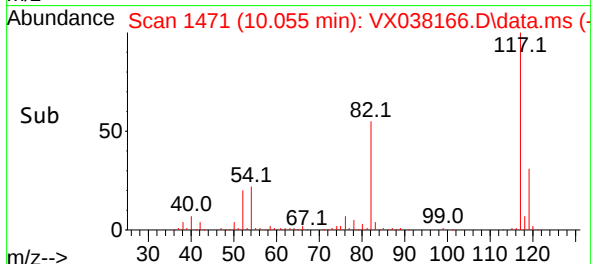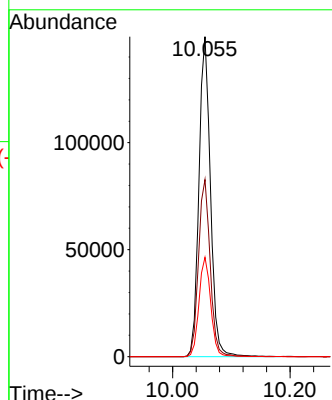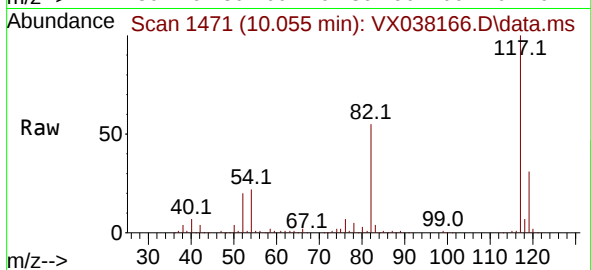

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. 0.000 min

Lab File: VX038166.D

Acq: 09 Oct 2023 13:04

Tgt Ion:152 Resp: 101508

Ion Ratio Lower Upper

152 100

115 60.1 43.3 129.9

150 155.5 0.0 345.0

