

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100924\
 Data File : VX043327.D
 Acq On : 09 Oct 2024 10:28
 Operator : JC/MD
 Sample : VX1009MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1009MBL01

Quant Time: Oct 10 01:26:10 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100124W.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 02 16:50:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	78108	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	145096	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	129860	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	59168	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	64966	50.929	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 101.860%			
35) Dibromofluoromethane	5.379	113	48131	48.100	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 96.200%			
50) Toluene-d8	8.647	98	176544	50.911	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 101.820%			
62) 4-Bromofluorobenzene	11.079	95	65439	51.945	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery = 103.880%			
Target Compounds						Qvalue
5) Bromomethane	1.599	94	332	0.867	ug/l	82
6) Chloroethane	1.660	64	73	0.209	ug/l #	33
11) Tert butyl alcohol	2.940	59	766	3.156	ug/l #	71
13) Acrolein	2.239	56	320	1.396	ug/l #	62
15) Acrylonitrile	3.068	53	345	0.696	ug/l #	79
16) Acetone	2.386	43	785	1.474	ug/l	95
17) Carbon Disulfide	2.501	76	1199	0.568	ug/l #	77
18) Methyl Acetate	2.709	43	451	0.337	ug/l #	51
21) trans-1,2-Dichloroethene	3.093	96	259	0.300	ug/l #	52
23) Vinyl Acetate	3.751	43	552	6.511	ug/l #	71
25) 2-Butanone	4.623	43	184	0.252	ug/l #	49
36) 1,1-Dichloropropene	5.544	75	6765	5.352	ug/l #	50
38) Carbon Tetrachloride	5.550	117	8938	5.973	ug/l #	14
44) Trichloroethene	7.123	130	222	0.218	ug/l	58
51) 4-Methyl-2-Pentanone	8.586	43	439	0.288	ug/l #	71
58) 2-Chloroethyl Vinyl ether	8.269	63	156	0.222	ug/l #	45
59) 2-Hexanone	9.464	43	535	0.465	ug/l	73
68) m/p-Xylenes	10.305	106	513	0.281	ug/l	99
76) 1,2,3-Trichloropropane	11.079	75	35892	27.348	ug/l #	33
77) Bromobenzene	11.201	156	250	0.223	ug/l	85
79) 2-Chlorotoluene	11.463	91	829	0.255	ug/l	90
81) trans-1,4-Dichloro-2-b...	11.079	75	35892	70.877	ug/l #	8
82) 4-Chlorotoluene	11.463	91	829	0.224	ug/l	99
87) 1,3-Dichlorobenzene	11.975	146	534	0.271	ug/l	88
88) 1,4-Dichlorobenzene	11.975	146	534	0.263	ug/l	87
89) n-Butylbenzene	12.335	91	1104	0.341	ug/l	85
91) 1,2-Dichlorobenzene	12.347	146	474	0.235	ug/l	96
93) 1,2,4-Trichlorobenzene	13.591	180	839	0.722	ug/l	87
94) Hexachlorobutadiene	13.725	225	127	0.276	ug/l #	59
95) Naphthalene	13.780	128	5659	1.324	ug/l	99
96) 1,2,3-Trichlorobenzene	13.963	180	1087	0.906	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100924\
Data File : VX043327.D
Acq On : 09 Oct 2024 10:28
Operator : JC/MD
Sample : VX1009MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1009MBL01

Quant Time: Oct 10 01:26:10 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100124W.M
Quant Title : SW846 8260
QLast Update : Wed Oct 02 16:50:57 2024
Response via : Initial Calibration




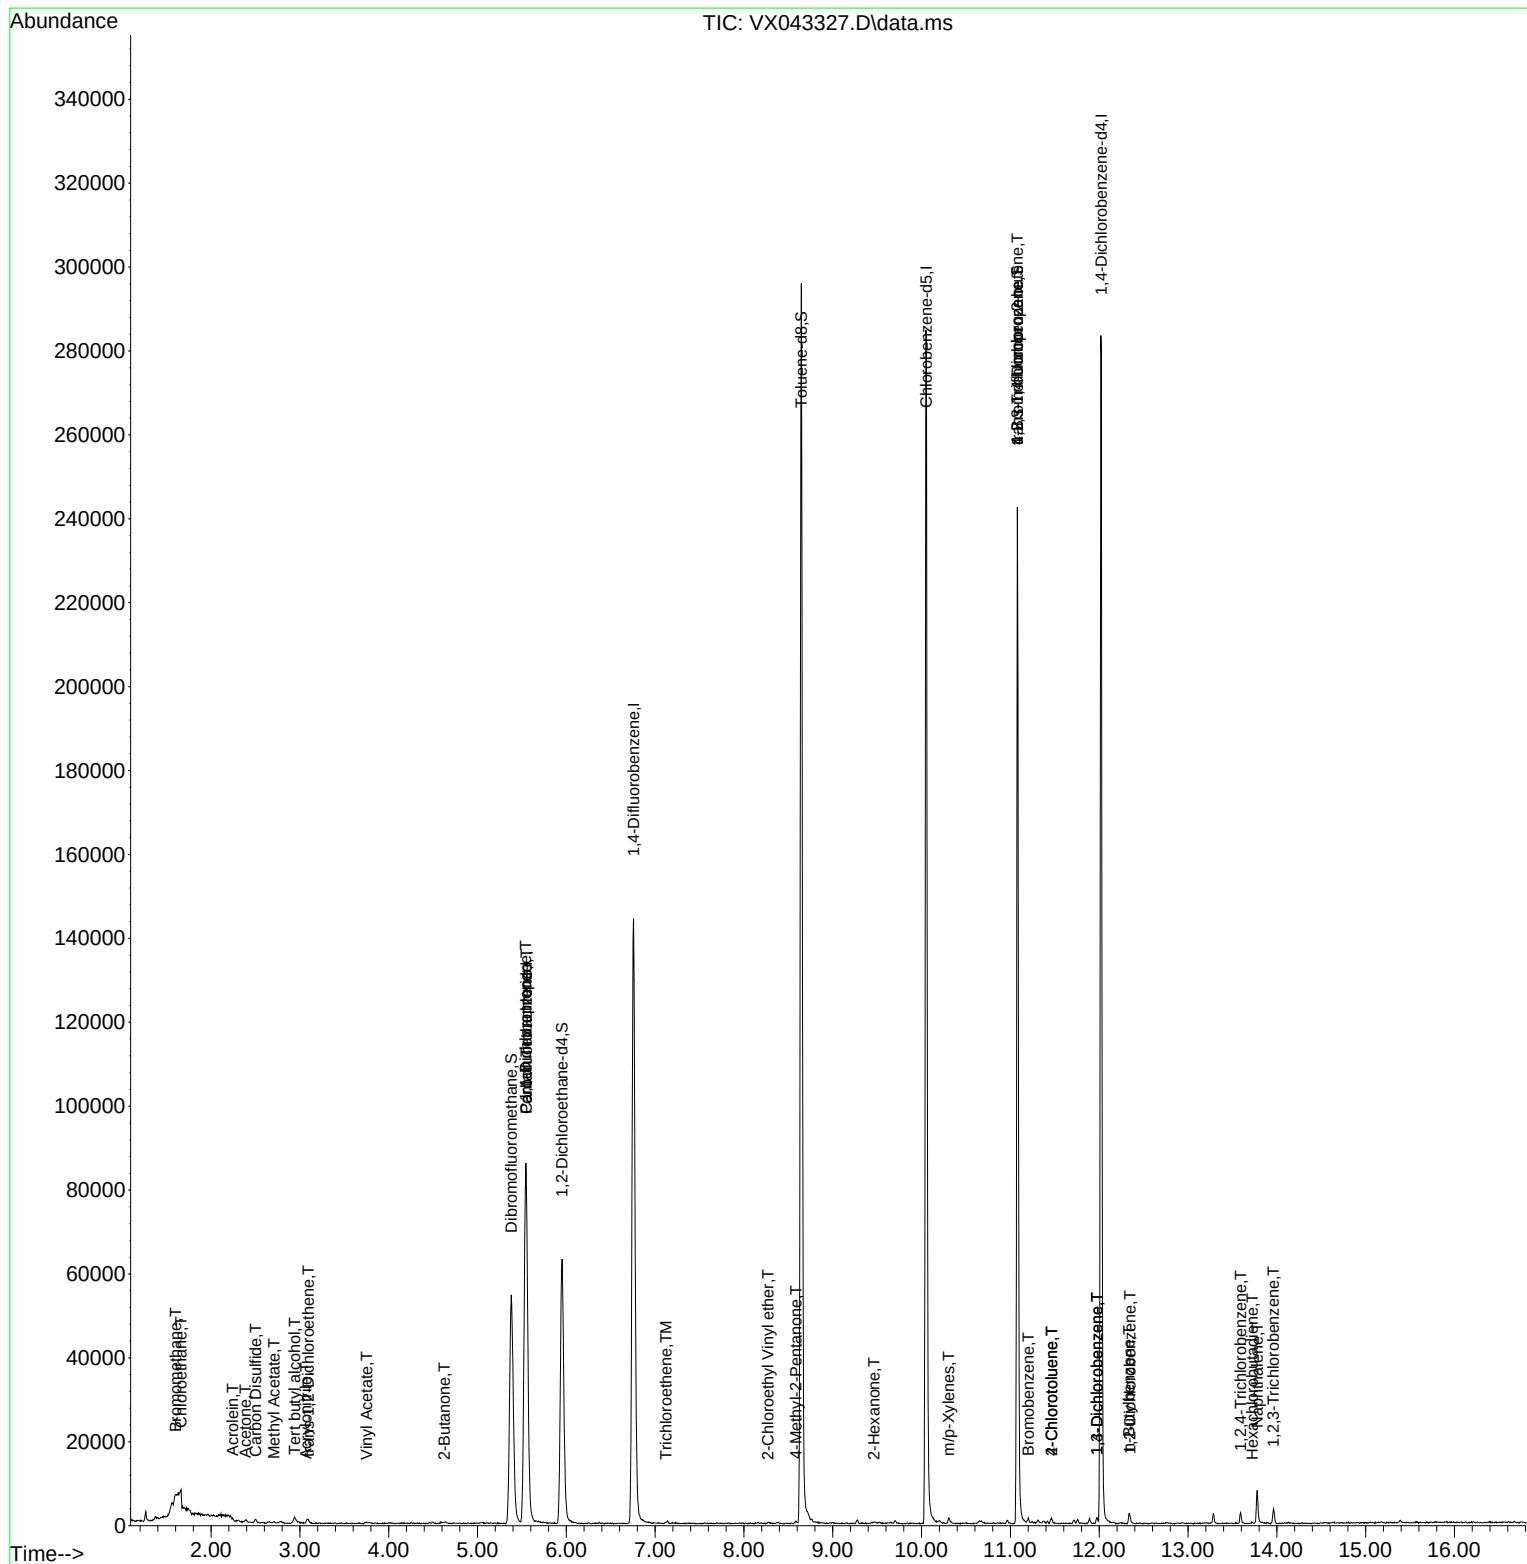




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX043327.D
Acq: 09 Oct 2024 10:28




Instrument :
MSVOA_X
ClientSampleId :
VX1009MBL01


Tgt Ion:168 Resp: 78108
Ion Ratio Lower Upper
168 100
99 63.2 49.7 74.5

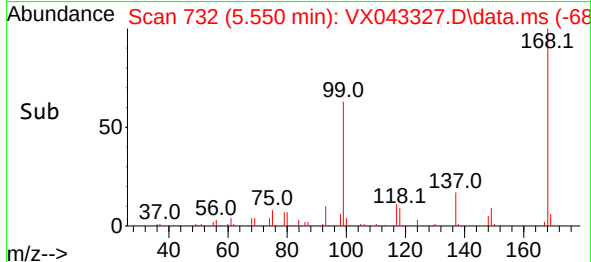

#5
Bromomethane
Concen: 0.867 ug/l
RT: 1.599 min Scan# 84
Delta R.T. 0.000 min
Lab File: VX043327.D
Acq: 09 Oct 2024 10:28

Tgt Ion: 94 Resp: 332
Ion Ratio Lower Upper
94 100
96 78.2 76.6 115.0


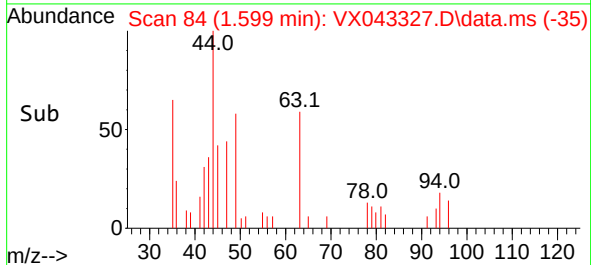




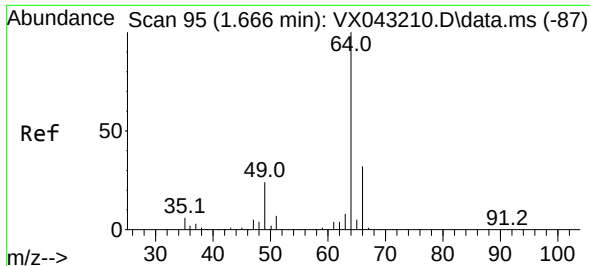

#6
Chloroethane
Concen: 0.209 ug/l
RT: 1.660 min Scan# 94
Delta R.T. -0.006 min
Lab File: VX043327.D
Acq: 09 Oct 2024 10:28




Instrument :
MSVOA_X
ClientSampleId :
VX1009MBL01


Tgt Ion: 64 Resp: 73
Ion Ratio Lower Upper
64 100
66 69.6 25.8 38.8#

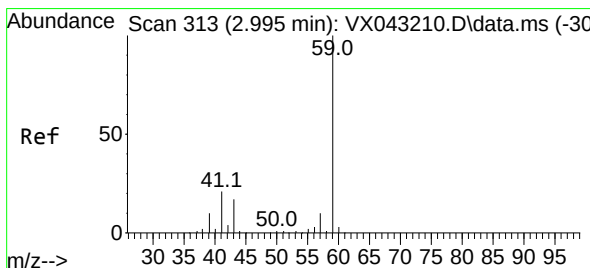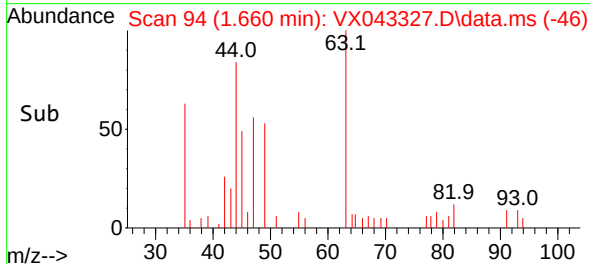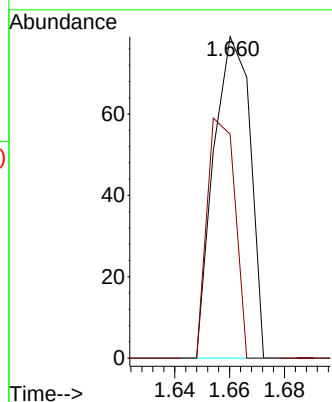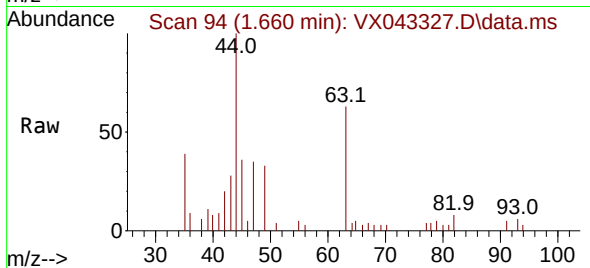

#11
Tert butyl alcohol
Concen: 3.156 ug/l
RT: 2.940 min Scan# 304
Delta R.T. -0.055 min
Lab File: VX043327.D
Acq: 09 Oct 2024 10:28

Tgt Ion: 59 Resp: 766
Ion Ratio Lower Upper
59 100
57 0.0 8.6 13.0#


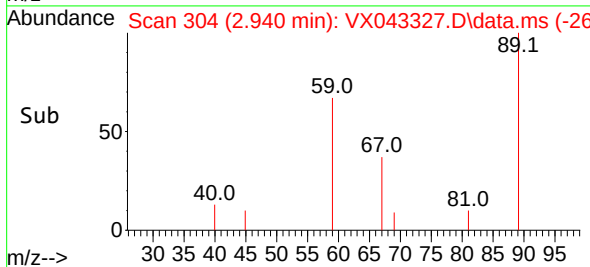
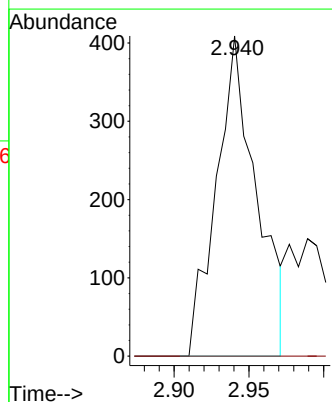
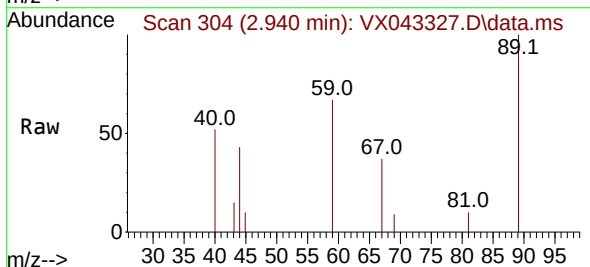


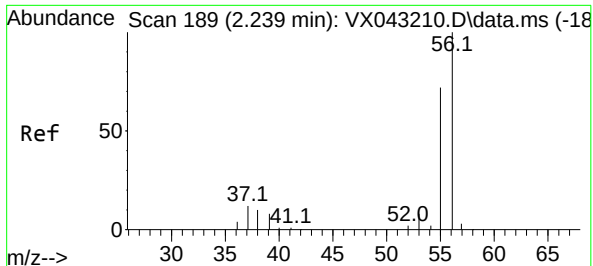

#13
Acrolein
Concen: 1.396 ug/l
RT: 2.239 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX043327.D
Acq: 09 Oct 2024 10:28




Instrument :
MSVOA_X
ClientSampleId :
VX1009MBL01


Tgt Ion: 56 Resp: 320
Ion Ratio Lower Upper
56 100
55 103.1 57.4 86.0#

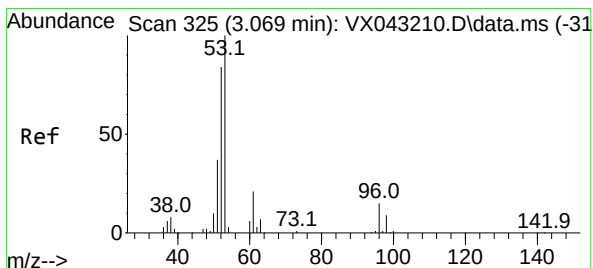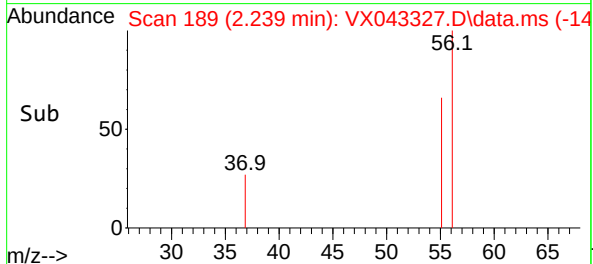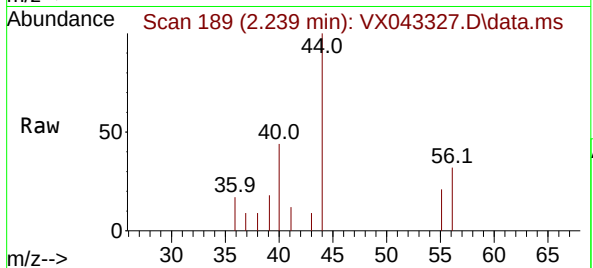

#15
Acrylonitrile
Concen: 0.696 ug/l
RT: 3.068 min Scan# 325
Delta R.T. -0.000 min
Lab File: VX043327.D
Acq: 09 Oct 2024 10:28

Tgt Ion: 53 Resp: 345
Ion Ratio Lower Upper
53 100
52 92.8 67.6 101.4
51 8.4 30.3 45.5#


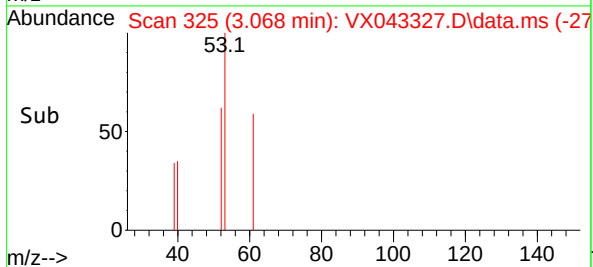

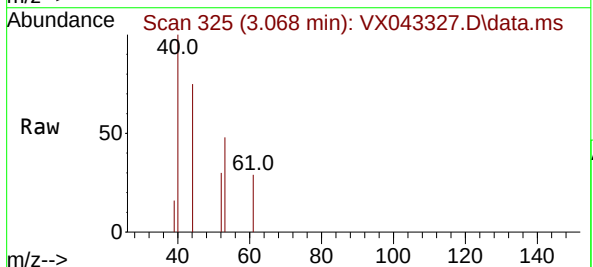




#16
Acetone
Concen: 1.474 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.000 min
Lab File: VX043327.D
Acq: 09 Oct 2024 10:28




Instrument :
MSVOA_X
ClientSampleId :
VX1009MBL01


Tgt Ion: 43 Resp: 785
Ion Ratio Lower Upper
43 100
58 25.6 22.6 33.8



#17
Carbon Disulfide
Concen: 0.568 ug/l
RT: 2.501 min Scan# 232
Delta R.T. -0.000 min
Lab File: VX043327.D
Acq: 09 Oct 2024 10:28

Tgt Ion: 76 Resp: 1199
Ion Ratio Lower Upper
76 100
78 16.4 6.7 10.1#


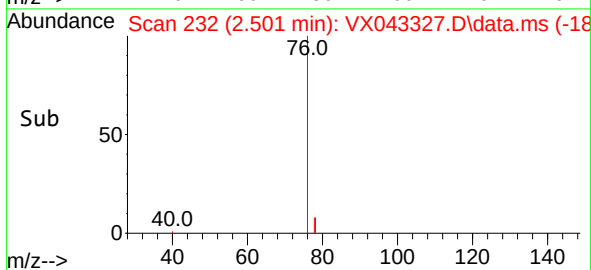






#18
Methyl Acetate
Concen: 0.337 ug/l
RT: 2.709 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX043327.D
Acq: 09 Oct 2024 10:28




Instrument :
MSVOA_X
ClientSampleId :
VX1009MBL01


Tgt Ion: 43 Resp: 451
Ion Ratio Lower Upper
43 100
74 0.0 19.1 28.7#

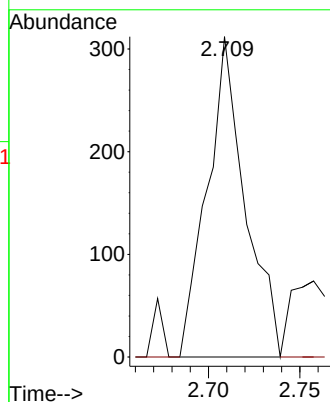

#21
trans-1,2-Dichloroethene
Concen: 0.300 ug/l
RT: 3.093 min Scan# 329
Delta R.T. 0.006 min
Lab File: VX043327.D
Acq: 09 Oct 2024 10:28

Tgt Ion: 96 Resp: 259
Ion Ratio Lower Upper
96 100
61 68.6 112.3 168.5#
98 46.6 54.6 82.0#



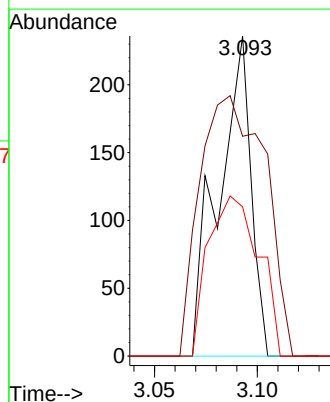





#23
 Vinyl Acetate
 Concen: 6.511 ug/l
 RT: 3.751 min Scan# 41
 Delta R.T. 0.030 min
 Lab File: VX043327.D
 Acq: 09 Oct 2024 10:28




Instrument :
 MSVOA_X
 ClientSampleId :
 VX1009MBL01


Tgt Ion: 43 Resp: 552
 Ion Ratio Lower Upper
 43 100
 86 0.0 8.8 13.2#



#25
 2-Butanone
 Concen: 0.252 ug/l
 RT: 4.623 min Scan# 580
 Delta R.T. 0.061 min
 Lab File: VX043327.D
 Acq: 09 Oct 2024 10:28

Tgt Ion: 43 Resp: 184
 Ion Ratio Lower Upper
 43 100
 72 0.0 20.6 31.0#


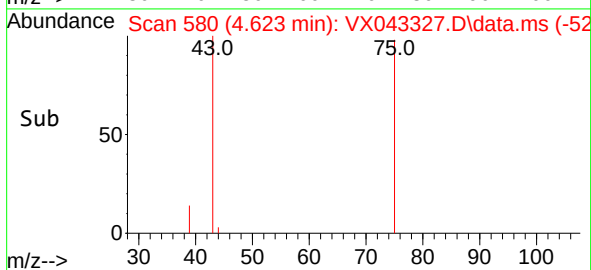






#33
 1,2-Dichloroethane-d4
 Concen: 50.929 ug/l
 RT: 5.952 min Scan# 798
 Delta R.T. -0.000 min
 Lab File: VX043327.D
 Acq: 09 Oct 2024 10:28




Instrument :
 MSVOA_X
 ClientSampleId :
 VX1009MBL01


Tgt Ion: 65 Resp: 64966
 Ion Ratio Lower Upper
 65 100
 67 49.1 0.0 99.0

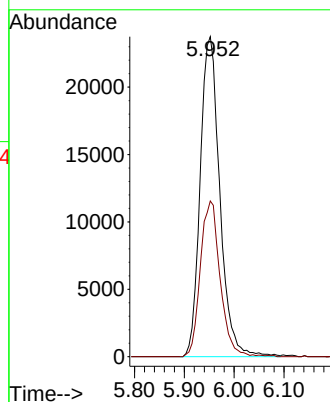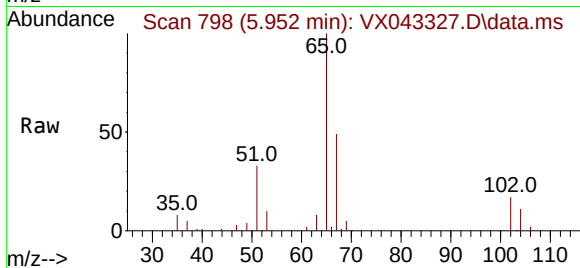

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.757 min Scan# 930
 Delta R.T. -0.000 min
 Lab File: VX043327.D
 Acq: 09 Oct 2024 10:28

Tgt Ion: 114 Resp: 145096
 Ion Ratio Lower Upper
 114 100
 63 21.0 0.0 43.0
 88 16.6 0.0 33.0


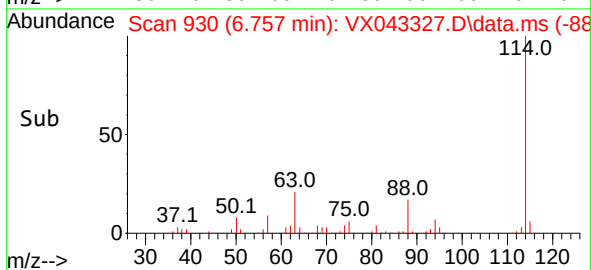
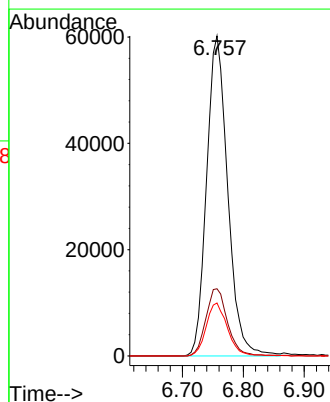
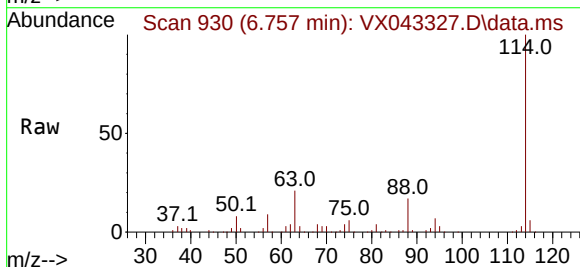


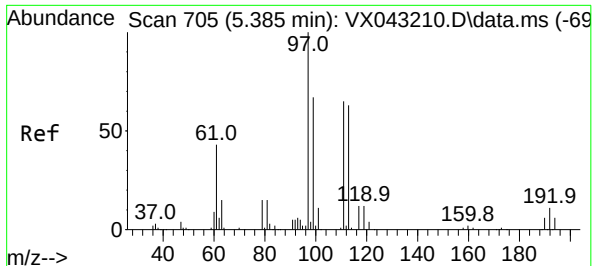

#35
Dibromofluoromethane
Concen: 48.100 ug/l
RT: 5.379 min Scan# 705
Delta R.T. -0.006 min
Lab File: VX043327.D
Acq: 09 Oct 2024 10:28




Instrument :
MSVOA_X
ClientSampleId :
VX1009MBL01


Tgt Ion:113 Resp: 48131
Ion Ratio Lower Upper
113 100
111 101.4 83.4 125.0
192 17.5 14.1 21.1

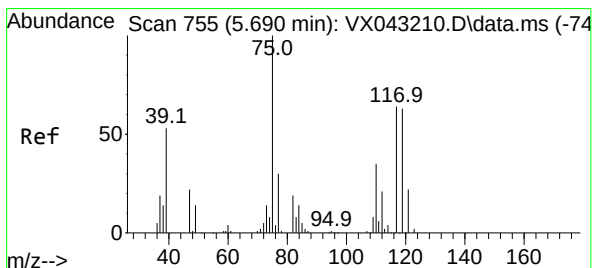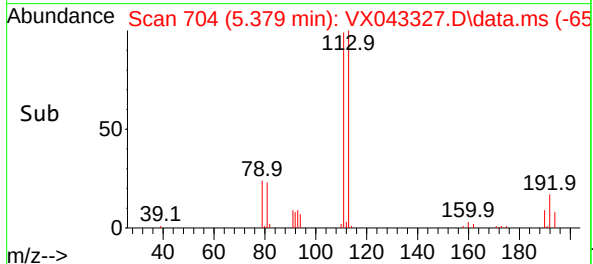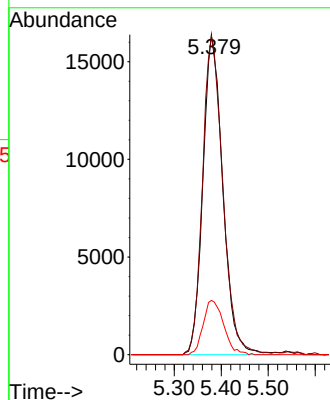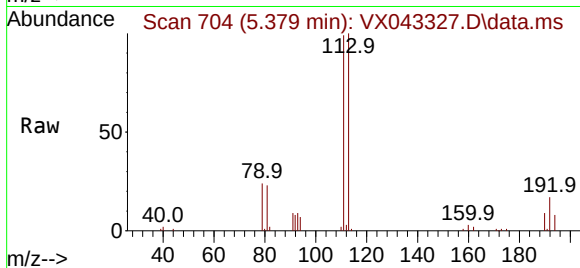

#36
1,1-Dichloropropene
Concen: 5.352 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.146 min
Lab File: VX043327.D
Acq: 09 Oct 2024 10:28


Tgt Ion: 75 Resp: 6765
Ion Ratio Lower Upper
75 100
110 9.1 17.8 53.3#
77 0.0 24.9 37.3#

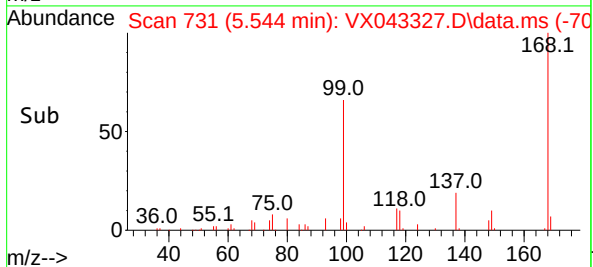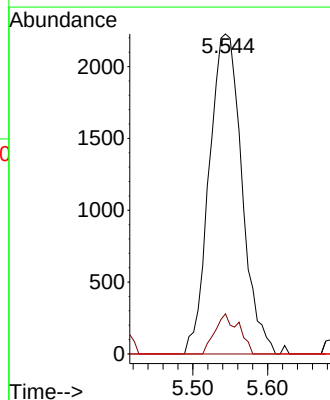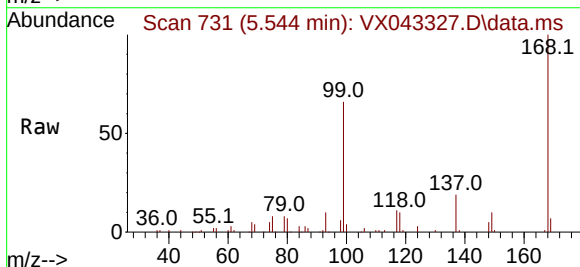






#38
Carbon Tetrachloride
Concen: 5.973 ug/l
RT: 5.550 min Scan# 711
Delta R.T. -0.122 min
Lab File: VX043327.D
Acq: 09 Oct 2024 10:28

Instrument :
MSVOA_X
ClientSampleId :
VX1009MBL01







Tgt Ion:117 Resp: 8938
Ion Ratio Lower Upper
117 100
119 2.9 77.7 116.5#
121 0.0 24.3 36.5#

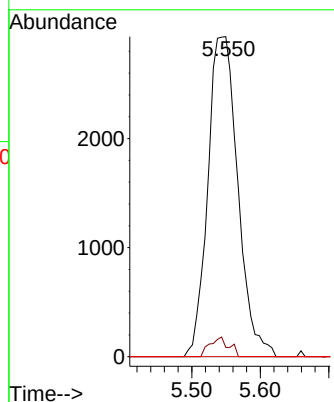

#44
Trichloroethene
Concen: 0.218 ug/l
RT: 7.123 min Scan# 990
Delta R.T. -0.000 min
Lab File: VX043327.D
Acq: 09 Oct 2024 10:28

Tgt Ion:130 Resp: 222
Ion Ratio Lower Upper
130 100
95 55.0 0.0 192.2



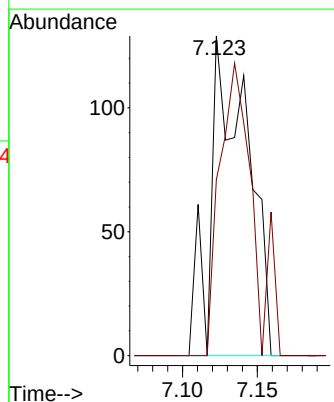





#50
Toluene-d8
Concen: 50.911 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX043327.D
Acq: 09 Oct 2024 10:28




Instrument :
MSVOA_X
ClientSampleId :
VX1009MBL01


Tgt Ion: 98 Resp: 176544
Ion Ratio Lower Upper
98 100
100 65.1 52.4 78.6

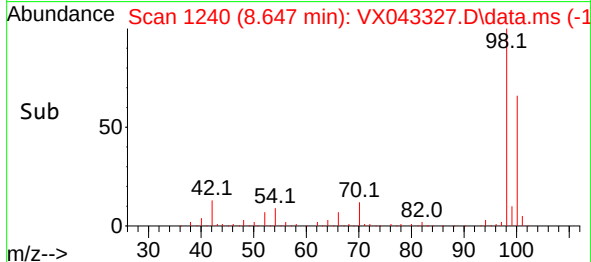

#51
4-Methyl-2-Pentanone
Concen: 0.288 ug/l
RT: 8.586 min Scan# 1230
Delta R.T. 0.012 min
Lab File: VX043327.D
Acq: 09 Oct 2024 10:28

Tgt Ion: 43 Resp: 439
Ion Ratio Lower Upper
43 100
58 20.0 30.0 45.0#




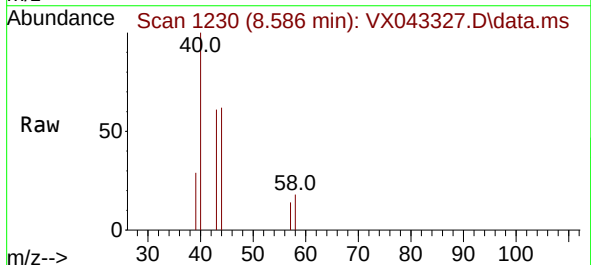


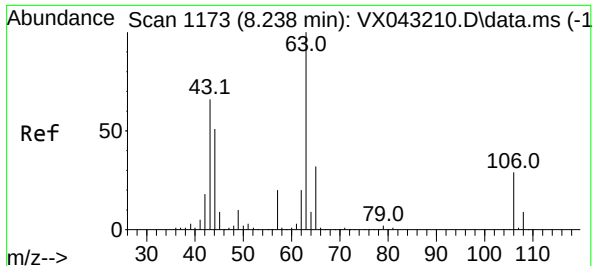

#58
 2-Chloroethyl Vinyl ether
 Concen: 0.222 ug/l
 RT: 8.269 min Scan# 1178
 Delta R.T. 0.030 min
 Lab File: VX043327.D
 Acq: 09 Oct 2024 10:28




Instrument :
 MSVOA_X
 ClientSampleId :
 VX1009MBL01


Tgt Ion: 63 Resp: 156
 Ion Ratio Lower Upper
 63 100
 106 0.0 23.7 35.5#

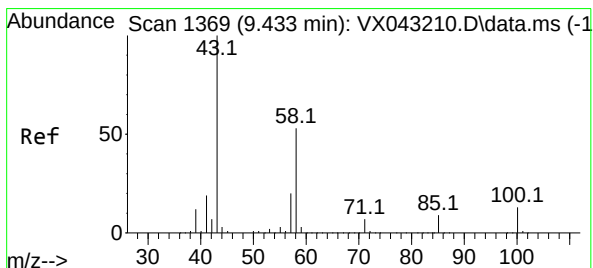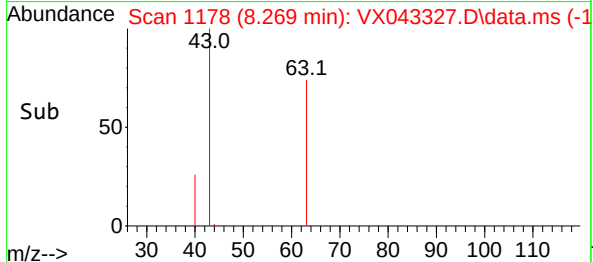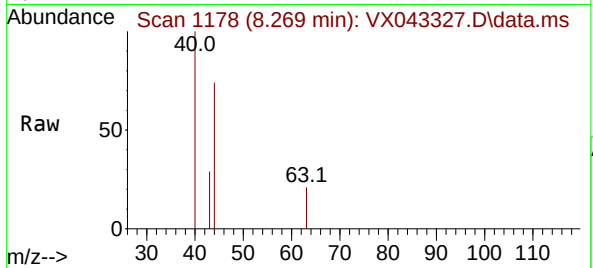

#59
 2-Hexanone
 Concen: 0.465 ug/l
 RT: 9.464 min Scan# 1374
 Delta R.T. 0.030 min
 Lab File: VX043327.D
 Acq: 09 Oct 2024 10:28

Tgt Ion: 43 Resp: 535
 Ion Ratio Lower Upper
 43 100
 58 33.1 26.1 78.3


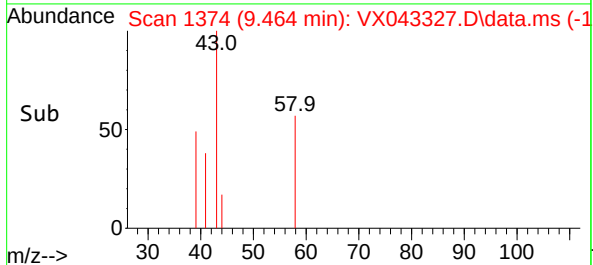

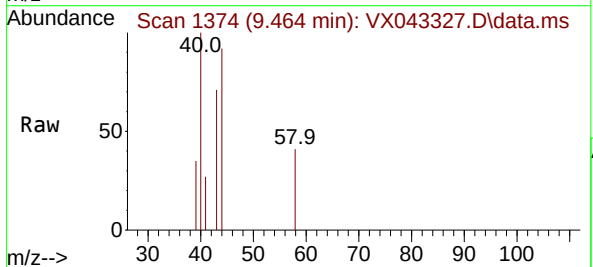




#62
4-Bromofluorobenzene
Concen: 51.945 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX043327.D
Acq: 09 Oct 2024 10:28




Instrument :
MSVOA_X
ClientSampleId :
VX1009MBL01


Tgt Ion: 95 Resp: 65439
Ion Ratio Lower Upper
95 100
174 71.7 0.0 145.0
176 68.9 0.0 143.0

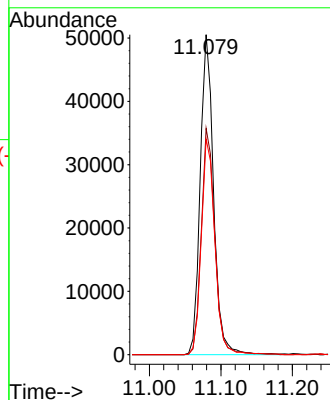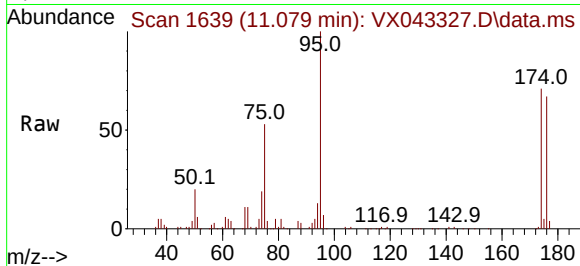

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX043327.D
Acq: 09 Oct 2024 10:28

Tgt Ion: 117 Resp: 129860
Ion Ratio Lower Upper
117 100
82 55.1 45.0 67.6
119 31.7 25.3 37.9



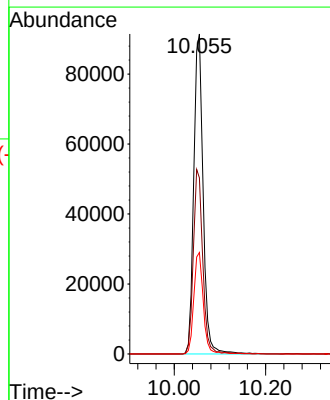
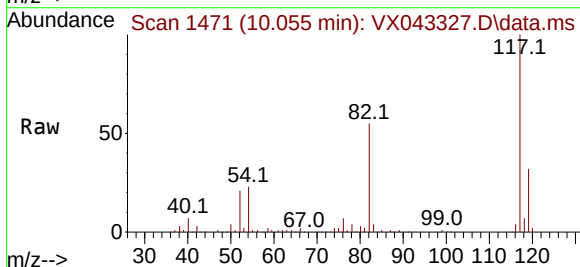




#68
m/p-Xylenes
Concen: 0.281 ug/l
RT: 10.305 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX043327.D
Acq: 09 Oct 2024 10:28




Instrument :
MSVOA_X
ClientSampleId :
VX1009MBL01


Tgt Ion:106 Resp: 513
Ion Ratio Lower Upper
106 100
91 207.2 167.0 250.6

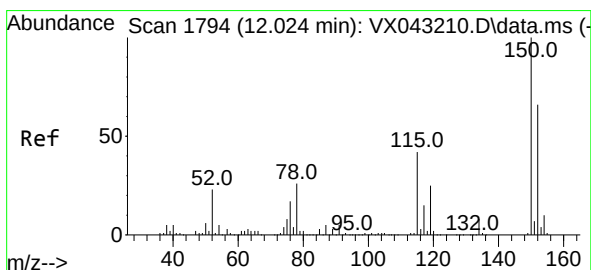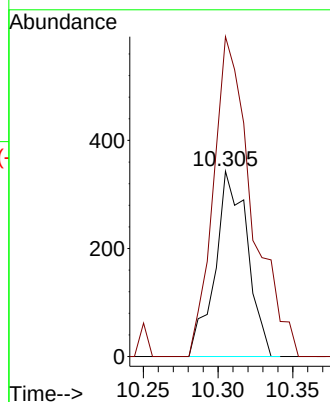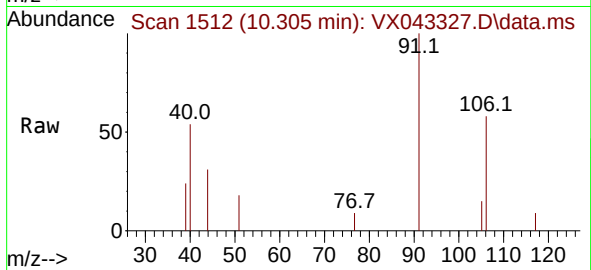

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX043327.D
Acq: 09 Oct 2024 10:28

Tgt Ion:152 Resp: 59168
Ion Ratio Lower Upper
152 100
115 61.9 44.1 132.3
150 154.1 0.0 347.4



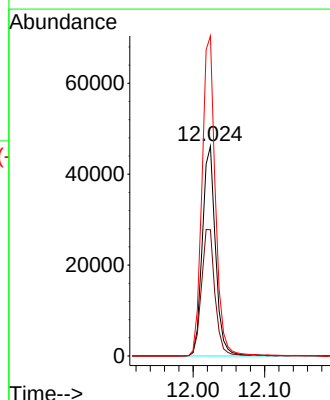





#76
1,2,3-Trichloropropane
Concen: 27.348 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX043327.D
Acq: 09 Oct 2024 10:28




Instrument :
MSVOA_X
ClientSampleId :
VX1009MBL01


Tgt Ion: 75 Resp: 35892
Ion Ratio Lower Upper
75 100
77 0.8 22.0 66.0#

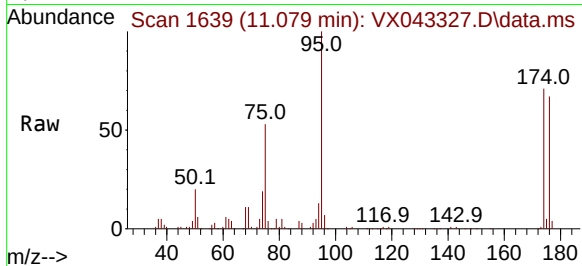

#77
Bromobenzene
Concen: 0.223 ug/l
RT: 11.201 min Scan# 1659
Delta R.T. 0.006 min
Lab File: VX043327.D
Acq: 09 Oct 2024 10:28

Tgt Ion:156 Resp: 250
Ion Ratio Lower Upper
156 100
77 182.8 82.0 245.8
158 79.6 48.1 144.3




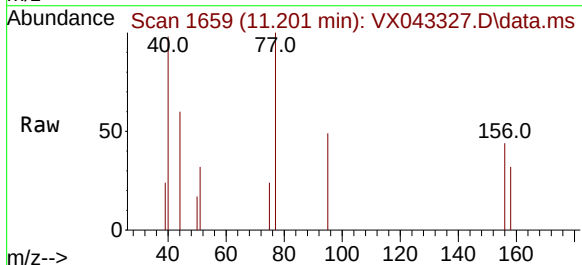




#79
2-Chlorotoluene
Concen: 0.255 ug/l
RT: 11.463 min Scan# 11
Delta R.T. 0.097 min
Lab File: VX043327.D
Acq: 09 Oct 2024 10:28




Instrument :
MSVOA_X
ClientSampleId :
VX1009MBL01


Tgt Ion: 91 Resp: 829
Ion Ratio Lower Upper
91 100
126 27.5 16.6 49.7

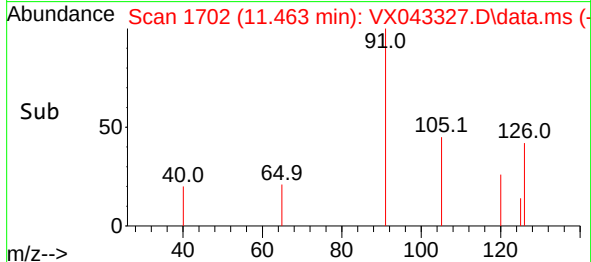

#81
trans-1,4-Dichloro-2-butene
Concen: 70.877 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX043327.D
Acq: 09 Oct 2024 10:28

Tgt Ion: 75 Resp: 35892
Ion Ratio Lower Upper
75 100
53 0.0 83.9 125.9#
89 0.0 38.6 58.0#

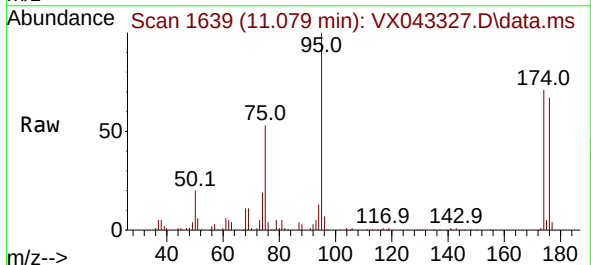



#82

4-Chlorotoluene

Concen: 0.224 ug/l

RT: 11.463 min Scan# 1702

Delta R.T. 0.012 min

Lab File: VX043327.D

Acq: 09 Oct 2024 10:28

Instrument :

MSVOA_X

ClientSampleId :





VX1009MBL01

Tgt Ion: 91 Resp: 829

Ion Ratio Lower Upper

91 100

126 27.5 14.1 42.3

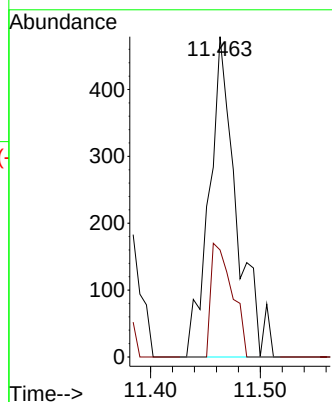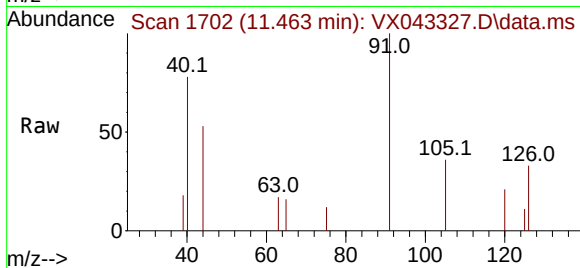

#87

1,3-Dichlorobenzene

Concen: 0.271 ug/l

RT: 11.975 min Scan# 1786

Delta R.T. 0.006 min

Lab File: VX043327.D

Acq: 09 Oct 2024 10:28




Tgt Ion: 146 Resp: 534


Ion Ratio Lower Upper

146 100

111 47.9 21.8 65.3

148 76.8 32.4 97.2


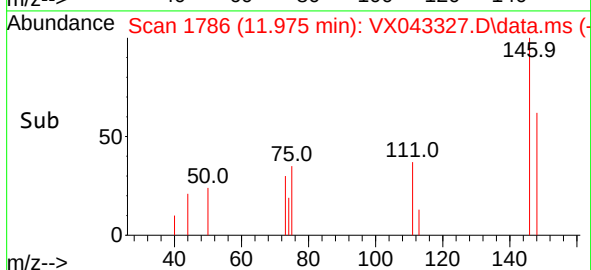

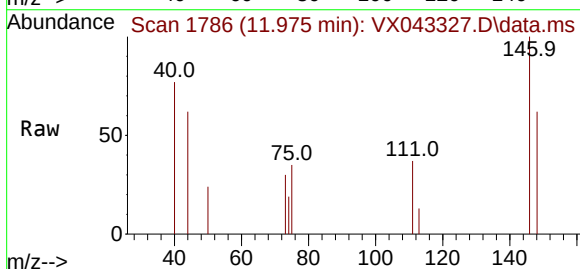




#88
1,4-Dichlorobenzene
Concen: 0.263 ug/l
RT: 11.975 min Scan# 11
Delta R.T. -0.067 min
Lab File: VX043327.D
Acq: 09 Oct 2024 10:28




Instrument :
MSVOA_X
ClientSampleId :
VX1009MBL01


Tgt Ion:146 Resp: 534
Ion Ratio Lower Upper
146 100
111 47.9 20.8 62.5
148 76.8 32.4 97.0

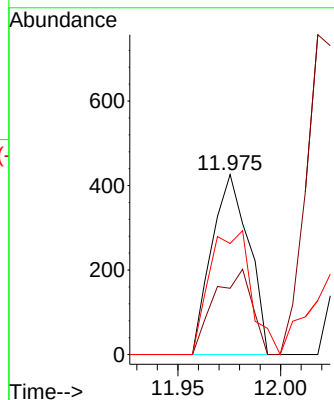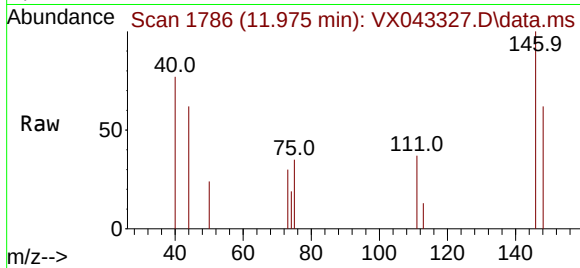

#89
n-Butylbenzene
Concen: 0.341 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. 0.006 min
Lab File: VX043327.D
Acq: 09 Oct 2024 10:28

Tgt Ion: 91 Resp: 1104
Ion Ratio Lower Upper
91 100
92 44.0 27.0 81.0
134 17.6 12.9 38.6

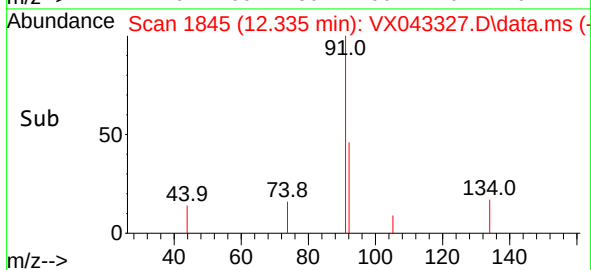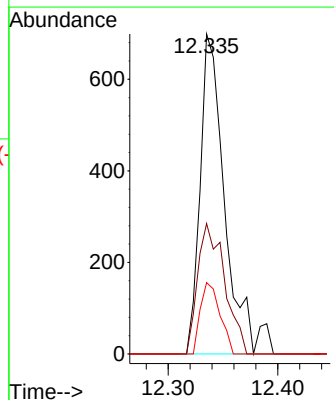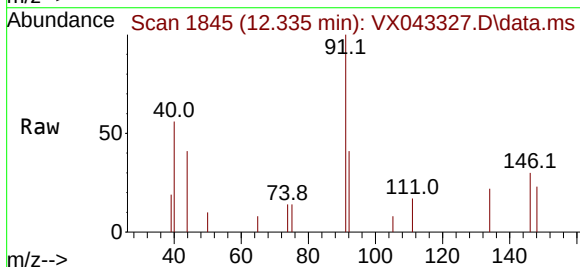

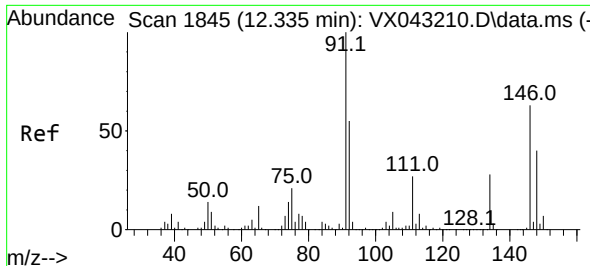

#91

1,2-Dichlorobenzene

Concen: 0.235 ug/l

RT: 12.347 min Scan# 11

Delta R.T. 0.012 min

Lab File: VX043327.D

Acq: 09 Oct 2024 10:28

Instrument :

MSVOA_X

ClientSampleId :

VX1009MBL01





Tgt Ion:146 Resp: 474

Ion Ratio Lower Upper

146 100

111 44.9 21.9 65.5

148 67.5 31.9 95.5

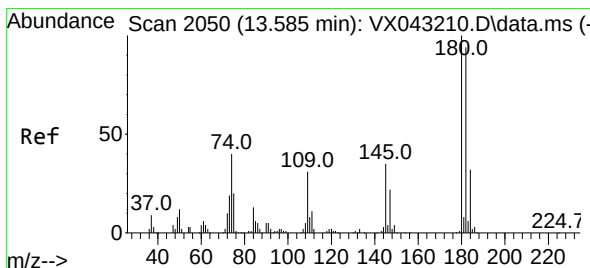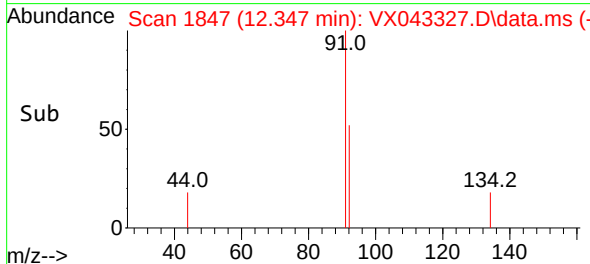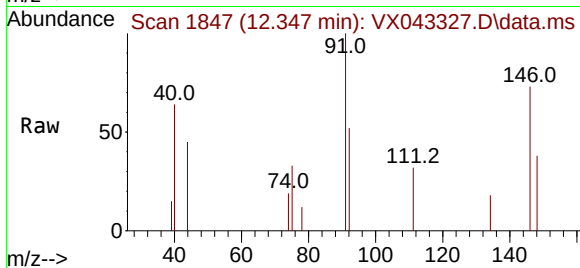

#93

1,2,4-Trichlorobenzene

Concen: 0.722 ug/l

RT: 13.591 min Scan# 2051

Delta R.T. 0.006 min

Lab File: VX043327.D

Acq: 09 Oct 2024 10:28




Tgt Ion:180 Resp: 839


Ion Ratio Lower Upper

180 100

182 111.2 47.1 141.3

145 32.5 16.6 49.8

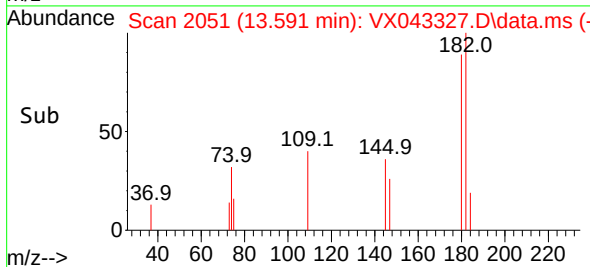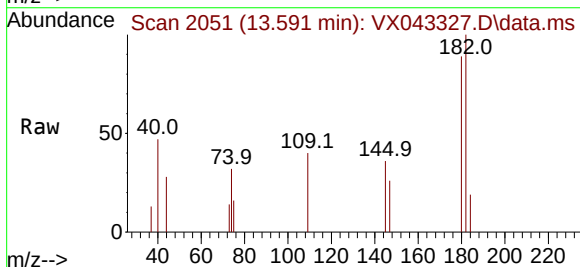



#94

Hexachlorobutadiene

Concen: 0.276 ug/l

RT: 13.725 min Scan# 2073

Delta R.T. -0.000 min

Lab File: VX043327.D

Acq: 09 Oct 2024 10:28

Instrument :

MSVOA_X

ClientSampleId :

VX1009MBL01





Tgt Ion:225 Resp: 127

Ion Ratio Lower Upper

225 100

223 20.5 30.8 92.4#

227 40.9 32.2 96.6

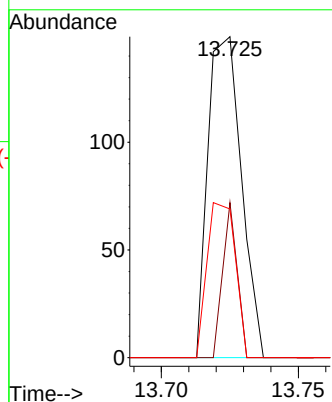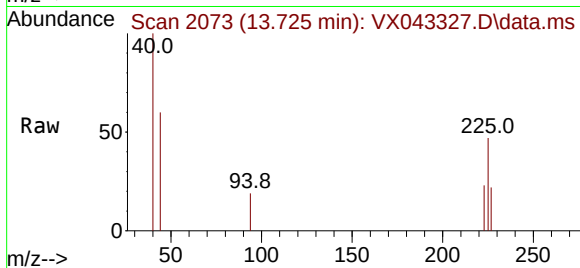

#95

Naphthalene

Concen: 1.324 ug/l

RT: 13.780 min Scan# 2082

Delta R.T. 0.006 min

Lab File: VX043327.D

Acq: 09 Oct 2024 10:28




Tgt Ion:128 Resp: 5659


Ion Ratio Lower Upper

128 100

127 11.9 10.2 15.2

129 11.0 8.6 13.0

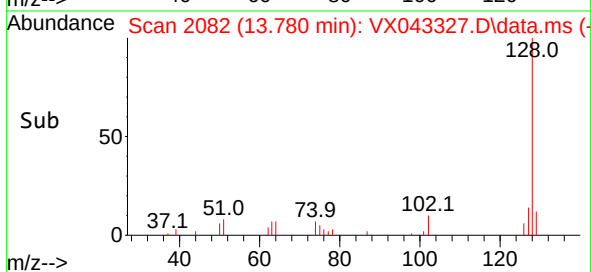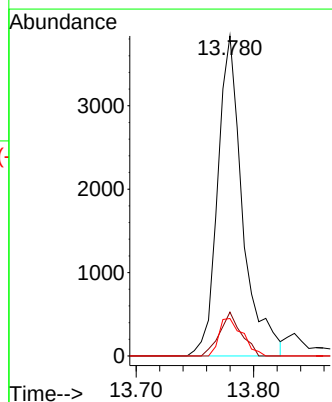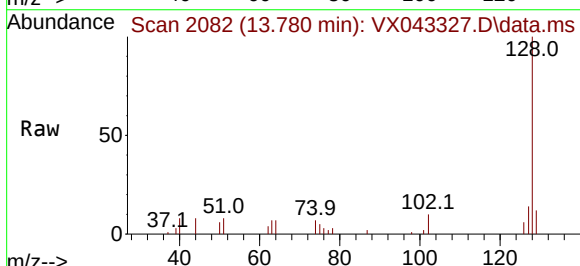



#96

1,2,3-Trichlorobenzene

Concen: 0.906 ug/l

RT: 13.963 min Scan# 21

Delta R.T. -0.000 min

Lab File: VX043327.D


Acq: 09 Oct 2024 10:28

Instrument :

MSVOA_X

ClientSampleId :

VX1009MBL01

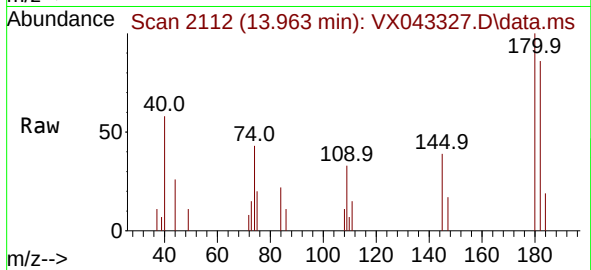

Tgt Ion:180 Resp: 1087

Ion Ratio Lower Upper

180 100

182 93.8 46.5 139.3

145 31.2 17.2 51.6

