


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100925\
Data File : VX048071.D
Acq On : 09 Oct 2025 08:35
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Title : SW846 8260
Last Update : Wed Sep 17 06:39:58 2025

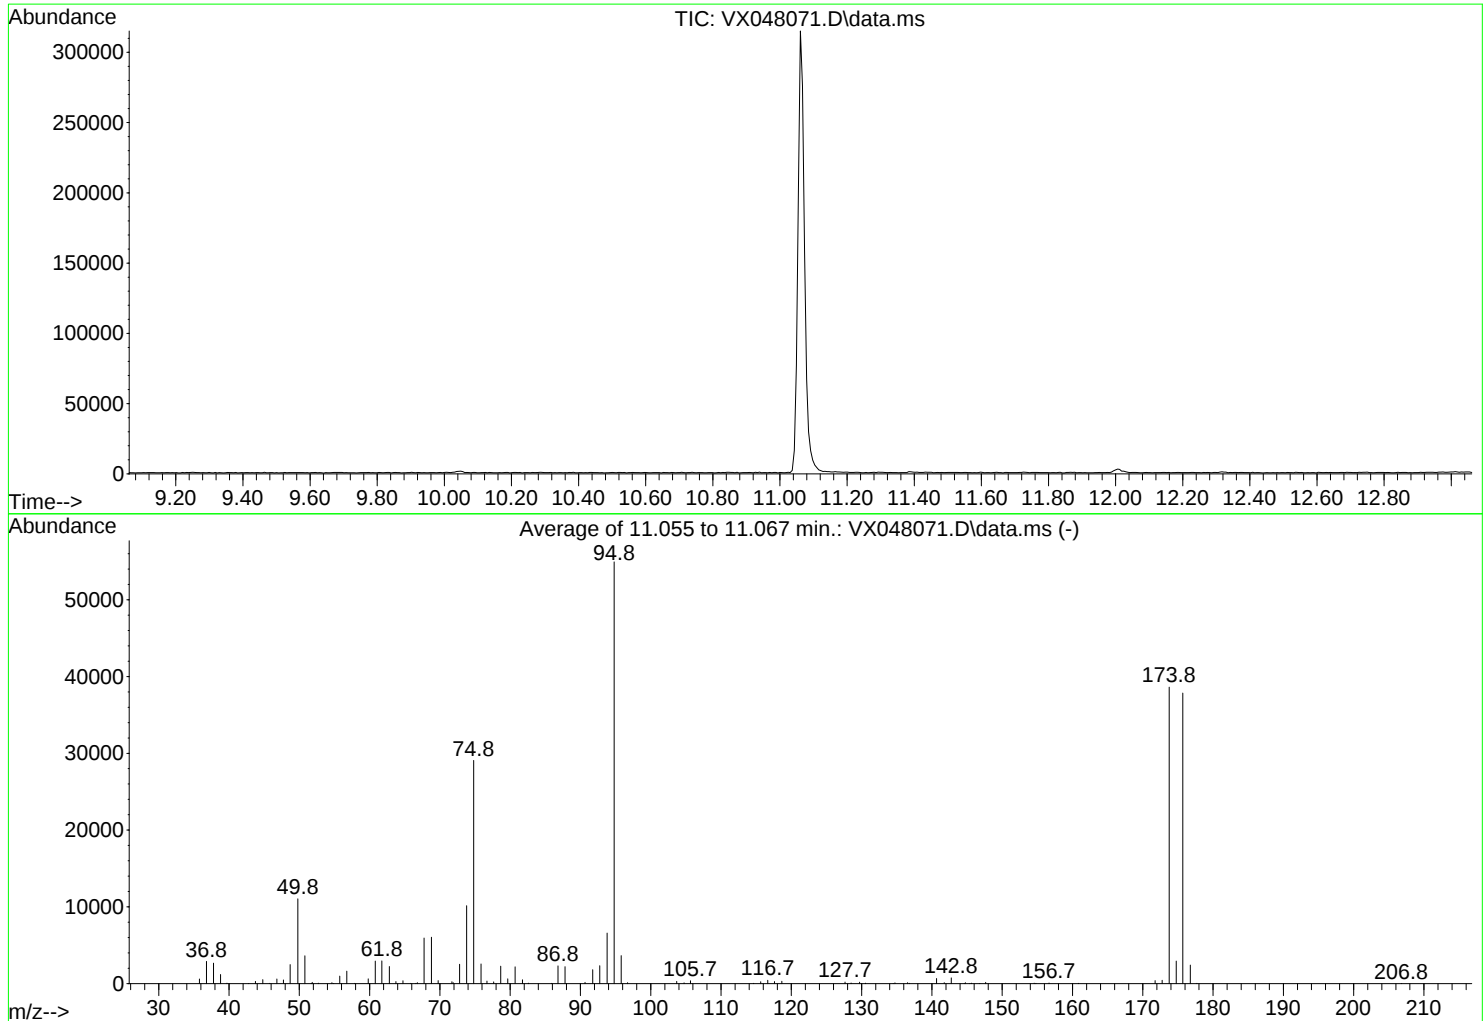

AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1629

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.1	11054	PASS
75	95	30	60	52.9	29067	PASS
95	95	100	100	100.0	54939	PASS
96	95	5	9	6.6	3653	PASS
173	174	0.00	2	1.1	442	PASS
174	95	50	100	70.3	38624	PASS
175	174	5	9	7.6	2932	PASS
176	174	95	101	98.0	37843	PASS
177	176	5	9	6.4	2426	PASS