

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX101018\
 Data File : VX005232.D
 Acq On : 11 Oct 2018 04:31
 Operator : JC/MD
 Sample : J5390-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FA18-GMZ5-TB1

Quant Time: Oct 12 09:52:26 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 03 04:00:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.66	168	164573	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	260078	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	253149	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	137798	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	130509	55.51	ug/l	0.00
Spiked Amount	50.000		Recovery	=	111.02%	
35) Dibromofluoromethane	5.51	113	107962	48.98	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.96%	
50) Toluene-d8	8.72	98	376131	51.33	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.66%	
62) 4-Bromofluorobenzene	11.14	95	128879	48.82	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.64%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX101018\
Data File : VX005232.D
Acq On : 11 Oct 2018 04:31
Operator : JC/MD
Sample : J5390-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FA18-GMZ5-TB1

Quant Time: Oct 12 09:52:26 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
Quant Title : SW846 8260
QLast Update : Wed Oct 03 04:00:03 2018
Response via : Initial Calibration

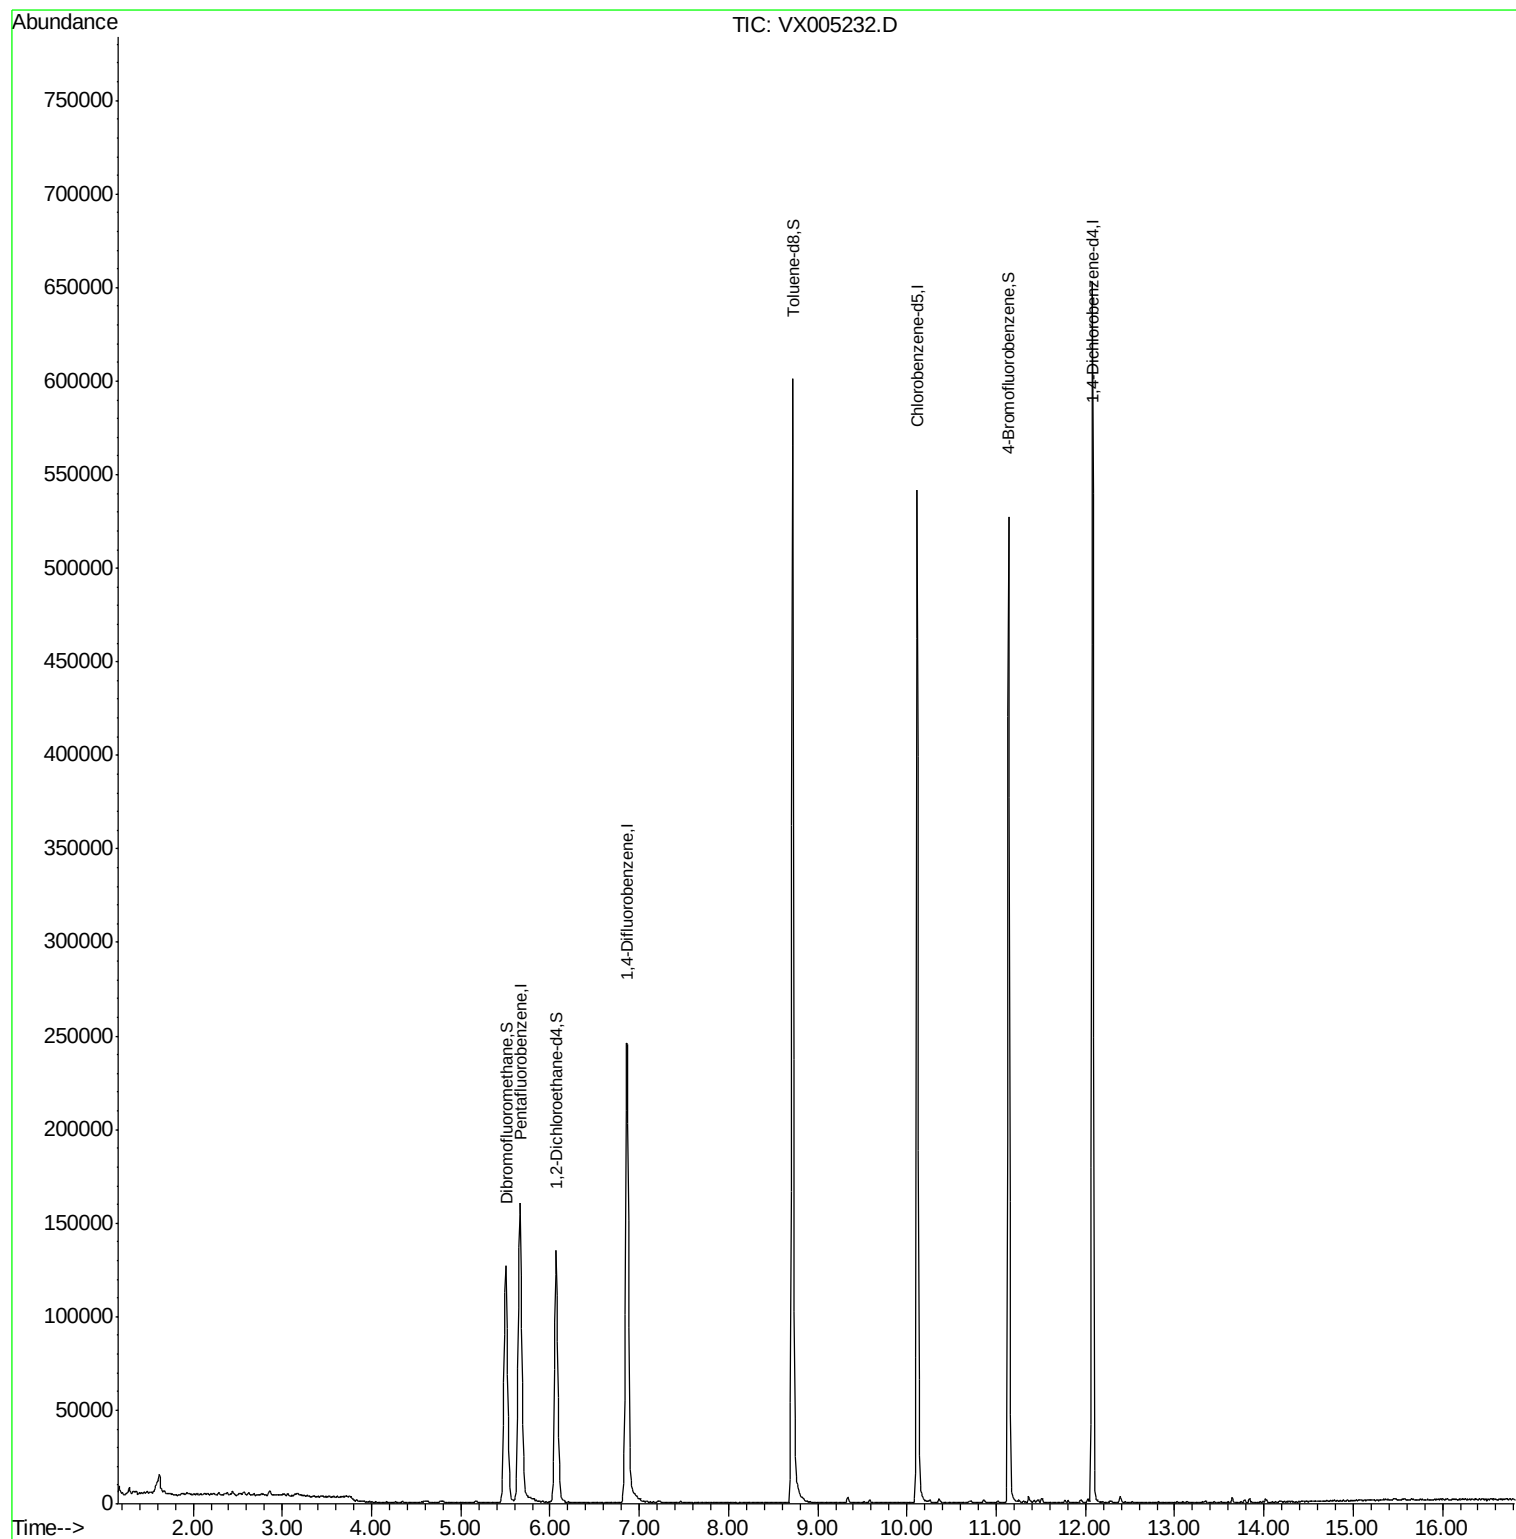

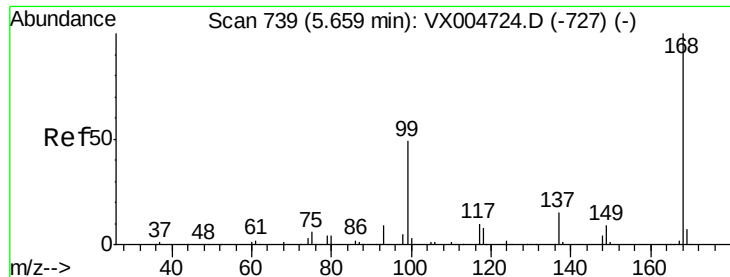

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.66 min Scan# 740

Delta R.T. 0.01 min

Lab File: VX005232.D

Acq: 11 Oct 2018 04:31

Instrument :

MSVOA_X

ClientSampleId :


FA18-GMZ5-TB1

Tgt Ion:168 Resp: 164573

Ion Ratio Lower Upper

168 100

99 49.0 39.3 58.9

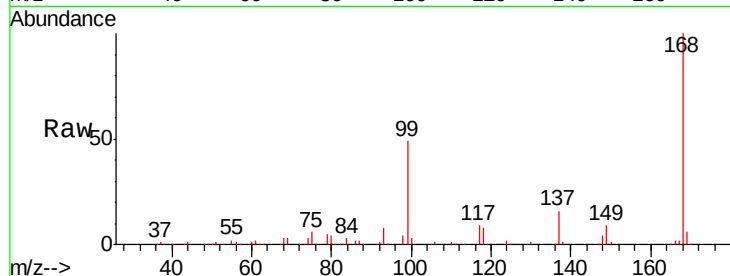

Abundance Ion 167.90 (167.60 to 168.60): VX004724.D (-727) (-)

Ion 98.90 (98.60 to 99.60): VX004724.D (-727) (-)

5.66



60000

40000

20000

0

Time--> 5.50 5.60 5.70 5.80

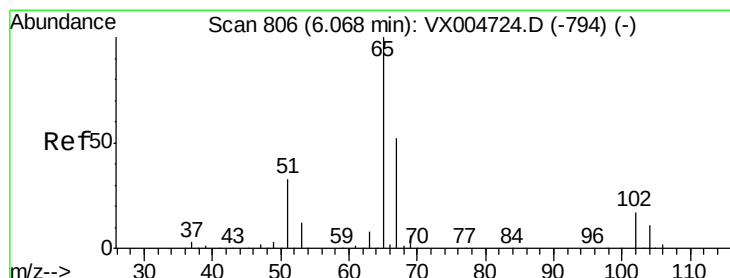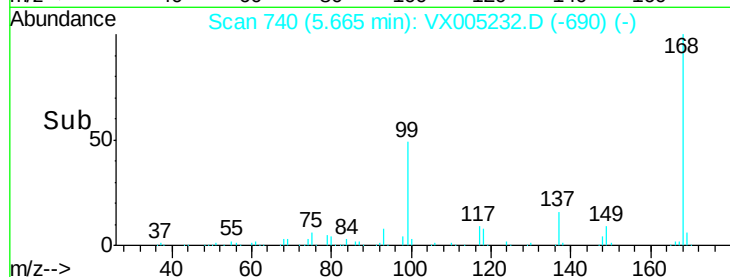

#33

1,2-Dichloroethane-d4

Concen: 55.51 ug/l

RT: 6.07 min Scan# 806

Delta R.T. -0.00 min

Lab File: VX005232.D


Acq: 11 Oct 2018 04:31

Tgt Ion: 65 Resp: 130509

Ion Ratio Lower Upper

65 100

67 52.3 0.0 107.4

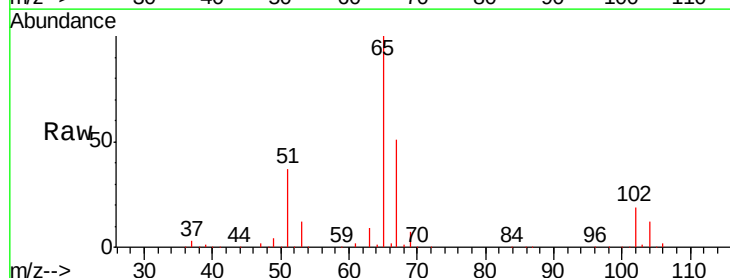

Abundance Ion 64.90 (64.60 to 65.60): VX004724.D (-794) (-)

Ion 66.90 (66.60 to 67.60): VX004724.D (-794) (-)

6.07

50000

40000


30000


20000

10000

0

Time--> 5.90 6.00 6.10 6.20

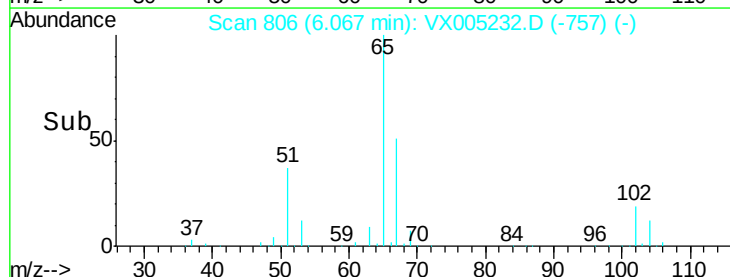


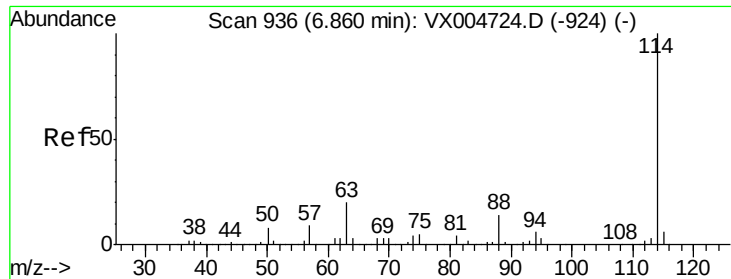




#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 6.87 min Scan# 937
 Delta R.T. 0.01 min
 Lab File: VX005232.D
 Acq: 11 Oct 2018 04:31

Instrument :
 MSVOA_X
 ClientSampleId :
 FA18-GMZ5-TB1

Tgt Ion:114 Resp: 260078
 Ion Ratio Lower Upper
 114 100
 63 19.9 0.0 39.8
 88 15.0 0.0 27.0

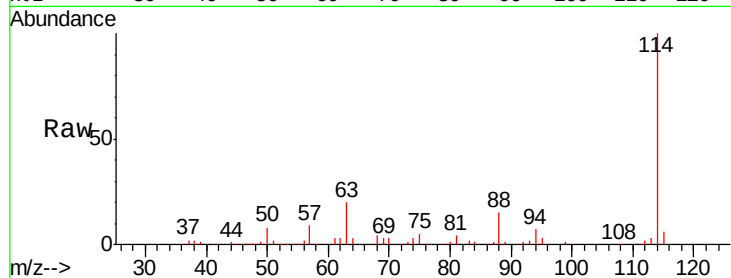


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VX
 Ion 87.90 (87.60 to 88.60): VX

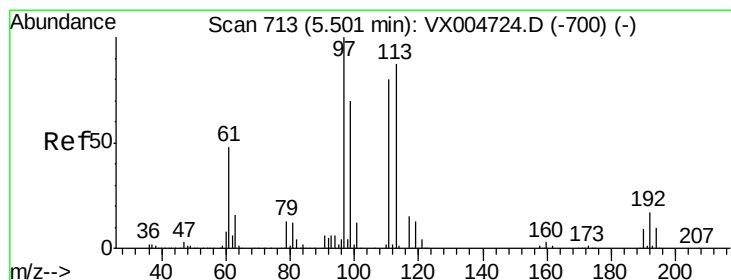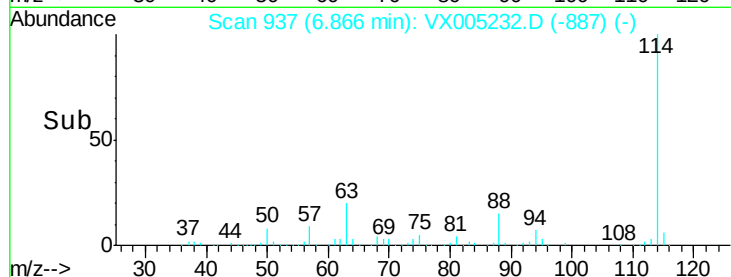
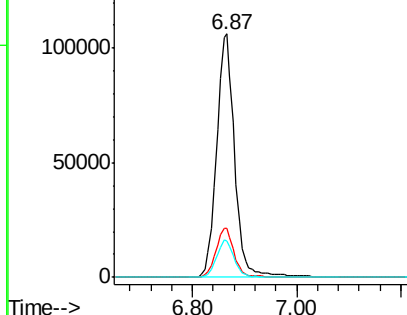



#35
 Dibromofluoromethane
 Concen: 48.98 ug/l
 RT: 5.51 min Scan# 714
 Delta R.T. 0.01 min
 Lab File: VX005232.D
 Acq: 11 Oct 2018 04:31

Tgt Ion:113 Resp: 107962
 Ion Ratio Lower Upper
 113 100
 111 102.8 77.0 115.4
 192 24.2 17.0 25.6

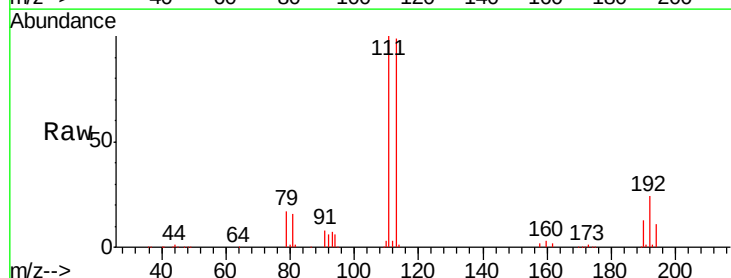

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V



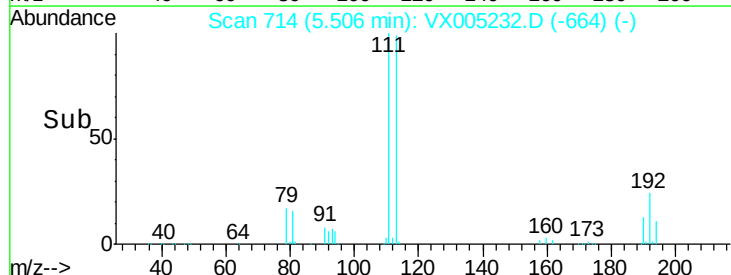
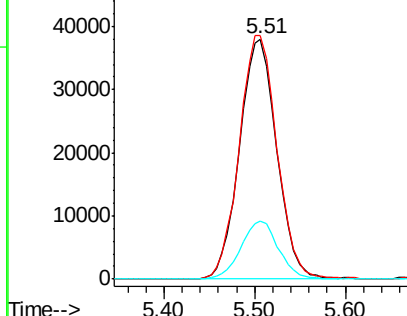


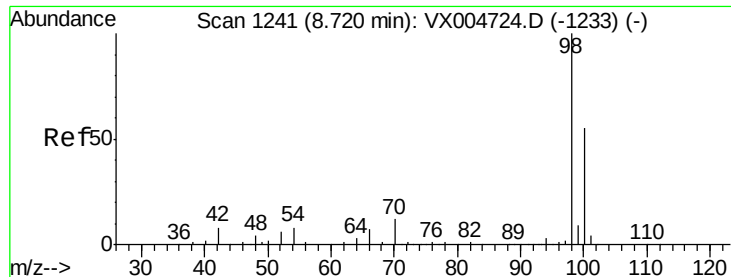

#50
Toluene-d8
Concen: 51.33 ug/l
RT: 8.72 min Scan# 1241
Delta R.T. -0.00 min
Lab File: VX005232.D
Acq: 11 Oct 2018 04:31




Instrument :
MSVOA_X
ClientSampled :
FA18-GMZ5-TB1


Tgt Ion: 98 Resp: 376131
Ion Ratio Lower Upper
98 100
100 63.2 51.9 77.9

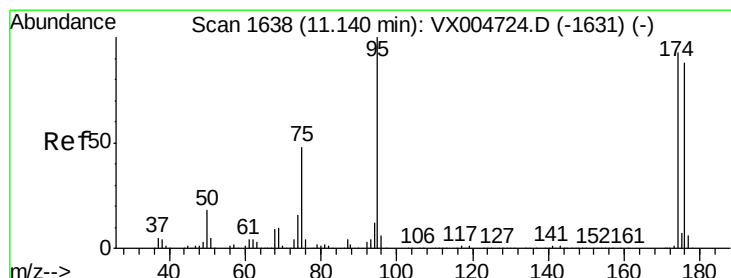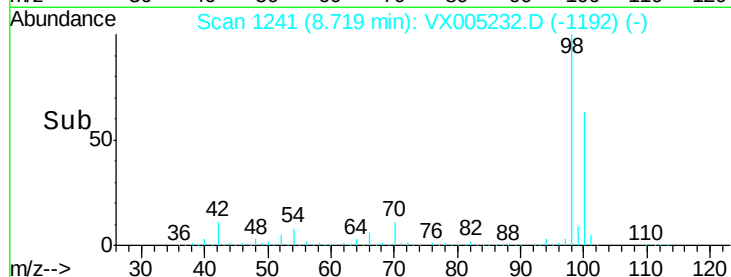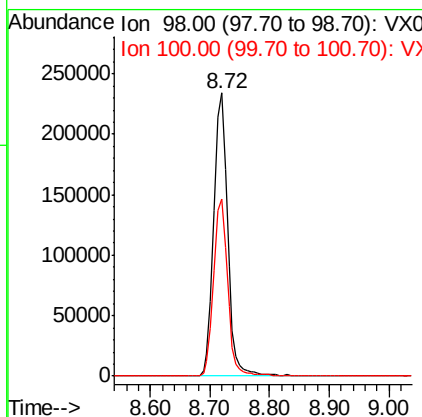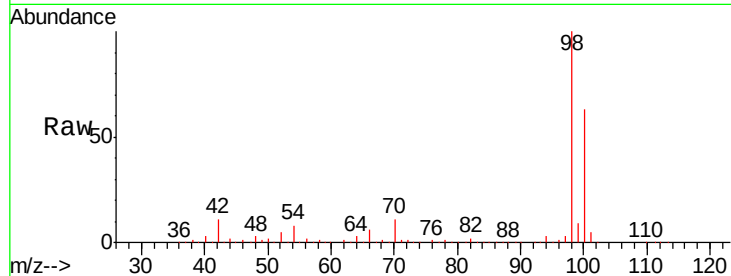

#62
4-Bromofluorobenzene
Concen: 48.82 ug/l
RT: 11.14 min Scan# 1638
Delta R.T. -0.00 min
Lab File: VX005232.D
Acq: 11 Oct 2018 04:31

Tgt Ion: 95 Resp: 128879
Ion Ratio Lower Upper
95 100
174 95.3 0.0 185.0
176 90.1 0.0 180.2

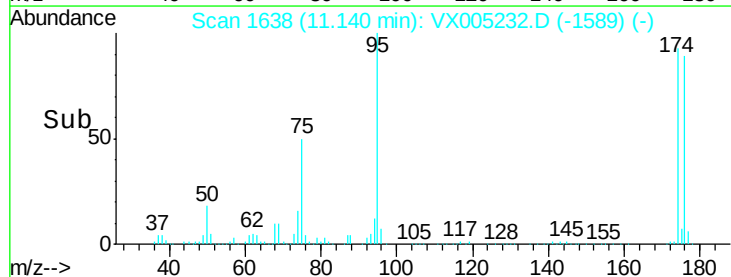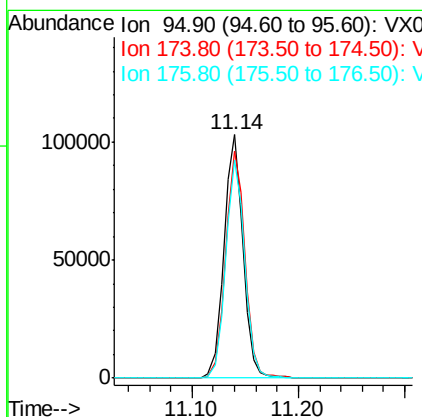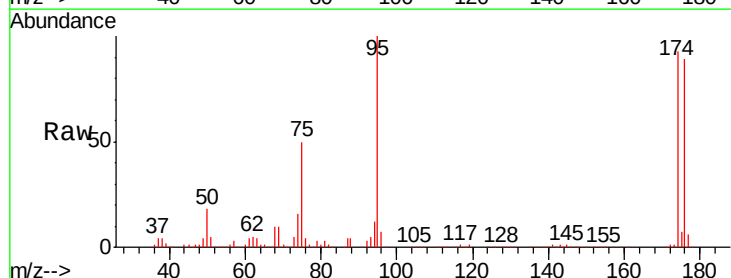


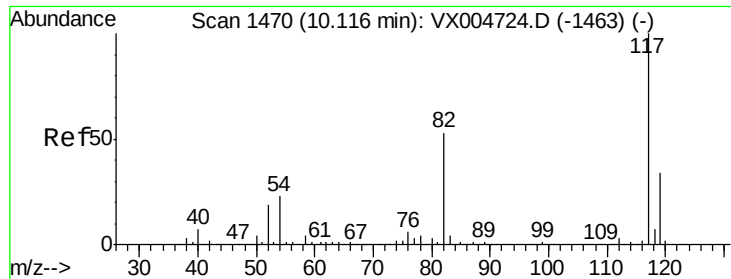




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.12 min Scan# 1470
Delta R.T. -0.00 min
Lab File: VX005232.D
Acq: 11 Oct 2018 04:31

Instrument :
MSVOA_X
ClientSampleId :
FA18-GMZ5-TB1

Tgt Ion:117 Resp: 253149
Ion Ratio Lower Upper
117 100
82 54.3 42.2 63.4
119 32.2 27.4 41.0

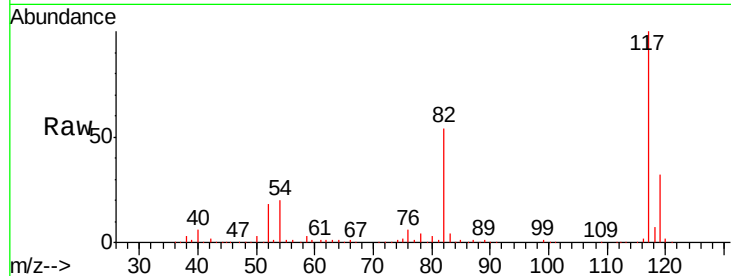


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VXO
Ion 118.90 (118.60 to 119.60): V

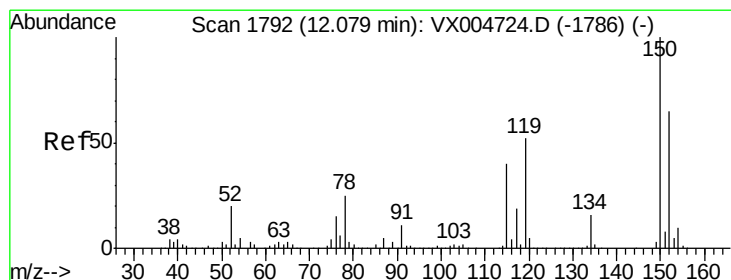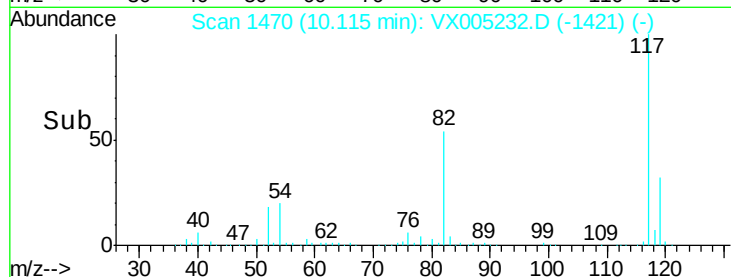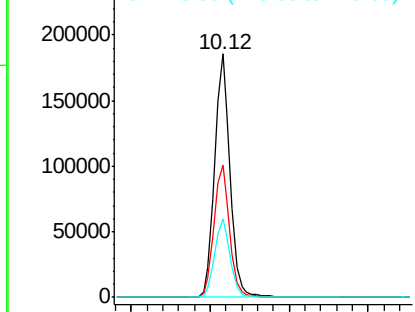

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. -0.00 min
Lab File: VX005232.D
Acq: 11 Oct 2018 04:31

Tgt Ion:152 Resp: 137798
Ion Ratio Lower Upper
152 100
115 55.0 40.2 120.6
150 156.8 0.0 351.0

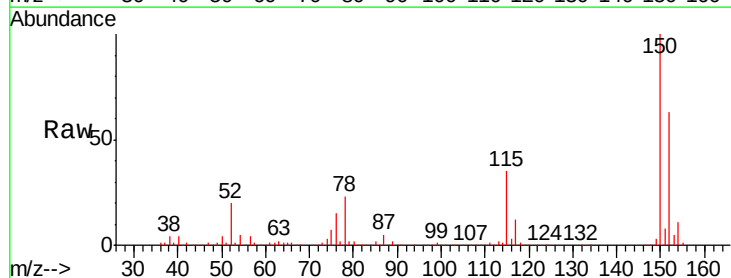

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

