


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101018\
Data File : VX005206.D
Acq On : 10 Oct 2018 13:14
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampled :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
Title : SW846 8260
Last Update : Wed Oct 03 04:00:03 2018

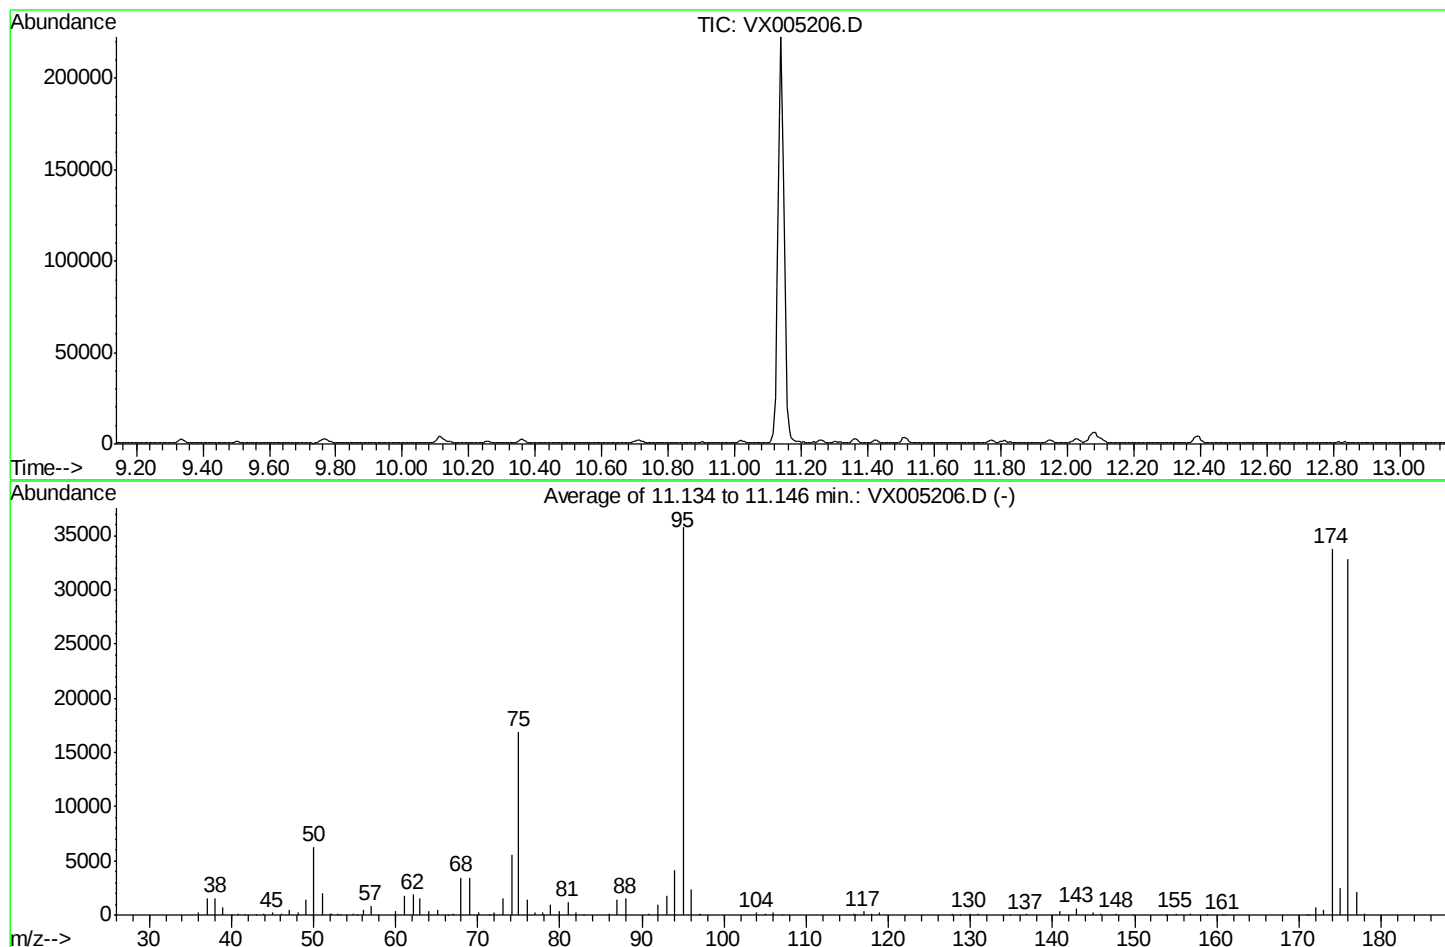

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	6295	PASS
75	95	30	60	47.3	16924	PASS
95	95	100	100	100.0	35749	PASS
96	95	5	9	6.8	2423	PASS
173	174	0.00	2	1.5	501	PASS
174	95	50	100	94.5	33797	PASS
175	174	5	9	7.4	2494	PASS
176	174	95	101	97.0	32781	PASS
177	176	5	9	6.6	2169	PASS