


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX101019\
Data File : VX012981.D
Acq On : 10 Oct 2019 08:57
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X100819W.M
Title : SW846 8260
Last Update : Fri Oct 11 09:48:22 2019

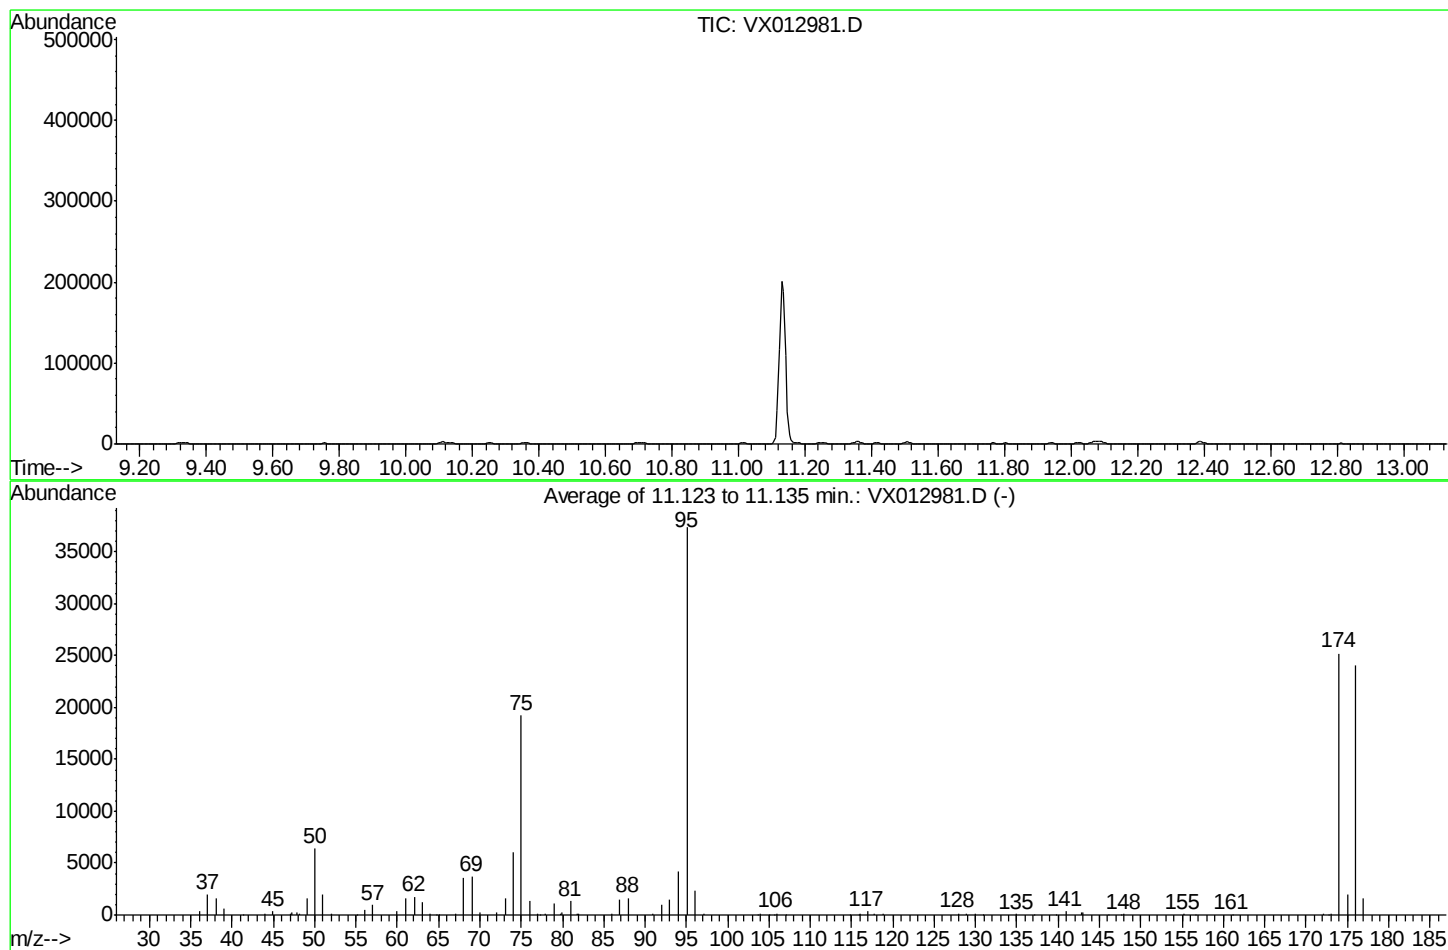

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1673

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	6390	PASS
75	95	30	60	51.4	19213	PASS
95	95	100	100	100.0	37357	PASS
96	95	5	9	6.3	2338	PASS
173	174	0.00	2	0.5	126	PASS
174	95	50	100	67.5	25214	PASS
175	174	5	9	8.0	2022	PASS
176	174	95	101	95.6	24100	PASS
177	176	5	9	6.7	1623	PASS