
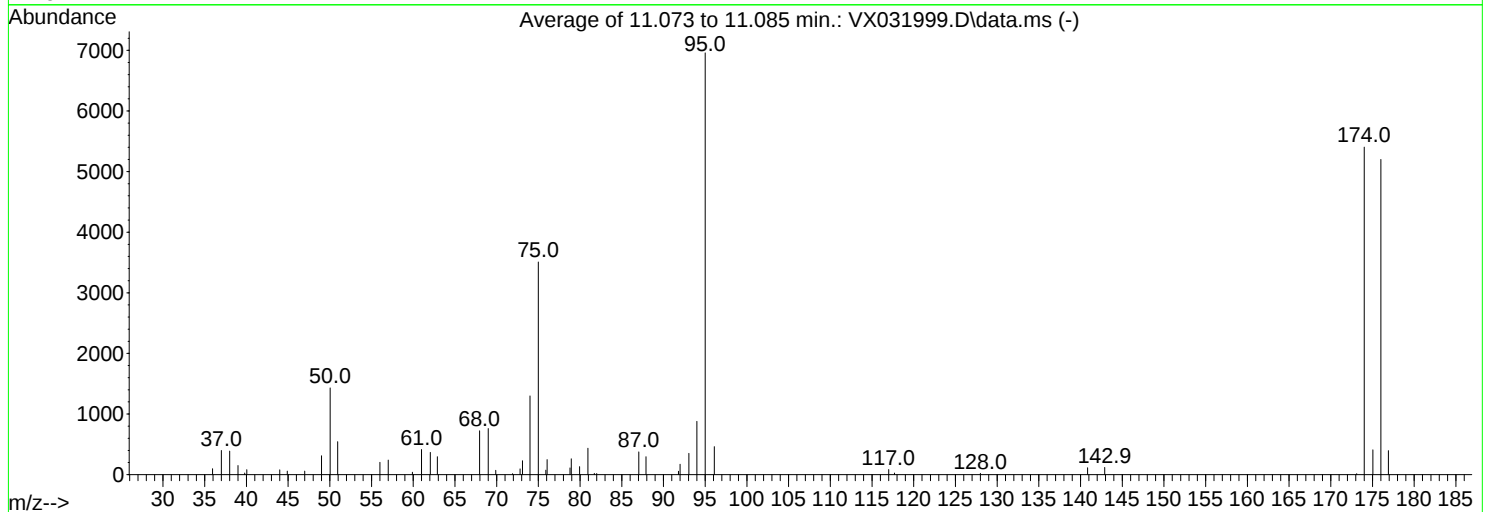


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101022\
 Data File : VX031999.D
 Acq On : 10 Oct 2022 08:41
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
 Title : SW846 8260
 Last Update : Thu Oct 06 14:28:46 2022

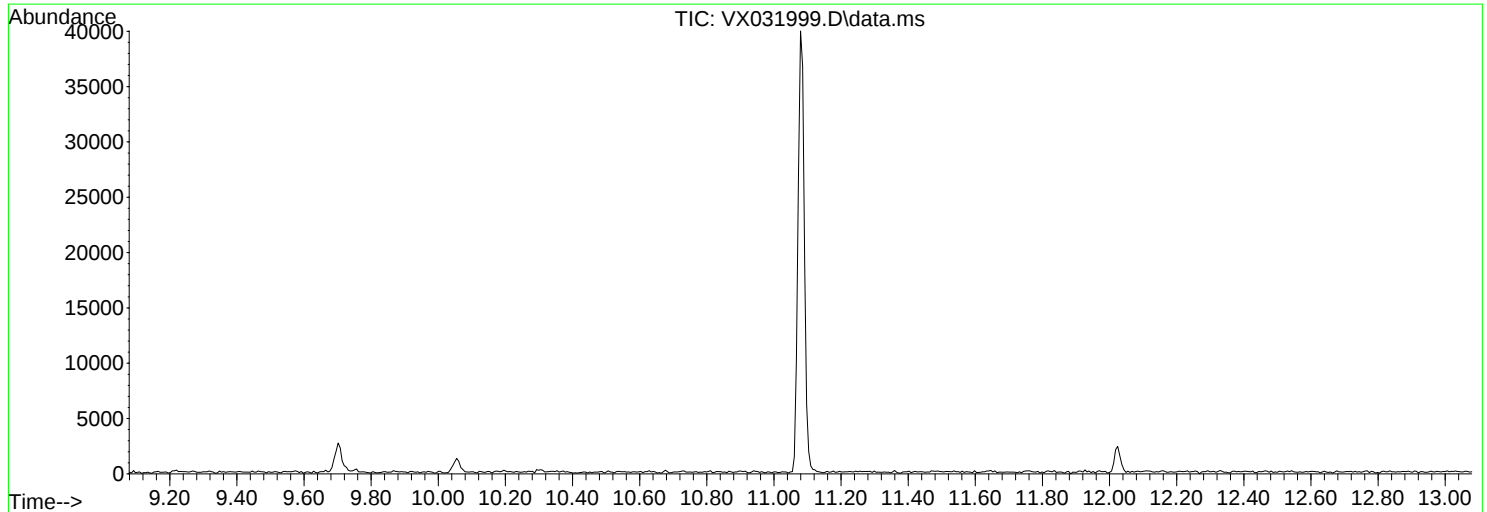

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	1430	PASS
75	95	30	60	50.4	3508	PASS
95	95	100	100	100.0	6959	PASS
96	95	5	9	6.7	463	PASS
173	174	0.00	2	0.3	17	PASS
174	95	50	100	77.7	5405	PASS
175	174	5	9	7.5	408	PASS
176	174	95	101	96.2	5200	PASS
177	176	5	9	7.6	395	PASS