

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101023\
 Data File : VX038200.D
 Acq On : 10 Oct 2023 14:46
 Operator : JC/MD
 Sample : 04782-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FB-100323

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M

Title : SW846 8260

Signal : TIC: VX038200.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.568	560	571	585	rBV	23115	80315	12.33%	2.139%
2	5.385	694	705	722	rBV	75695	220455	33.85%	5.872%
3	5.549	722	732	746	rBV	113501	330508	50.75%	8.804%
4	5.958	787	799	814	rBV	86540	228759	35.13%	6.094%
5	6.763	921	931	949	rBV	189940	462650	71.05%	12.324%
6	8.646	1234	1240	1259	rBV	398719	651185	100.00%	17.346%
7	10.055	1465	1471	1487	rBV	451335	611839	93.96%	16.298%
8	10.201	1490	1495	1501	rBV2	5994	8852	1.36%	0.236%
9	10.299	1506	1511	1524	rVB	22600	34257	5.26%	0.913%
10	11.079	1634	1639	1651	rBV	369760	479646	73.66%	12.777%
11	12.024	1788	1794	1802	rBV	498159	645608	99.14%	17.198%




Sum of corrected areas: 3754074

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101023\
Data File : VX038200.D
Acq On : 10 Oct 2023 14:46
Operator : JC/MD
Sample : 04782-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB-100323

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

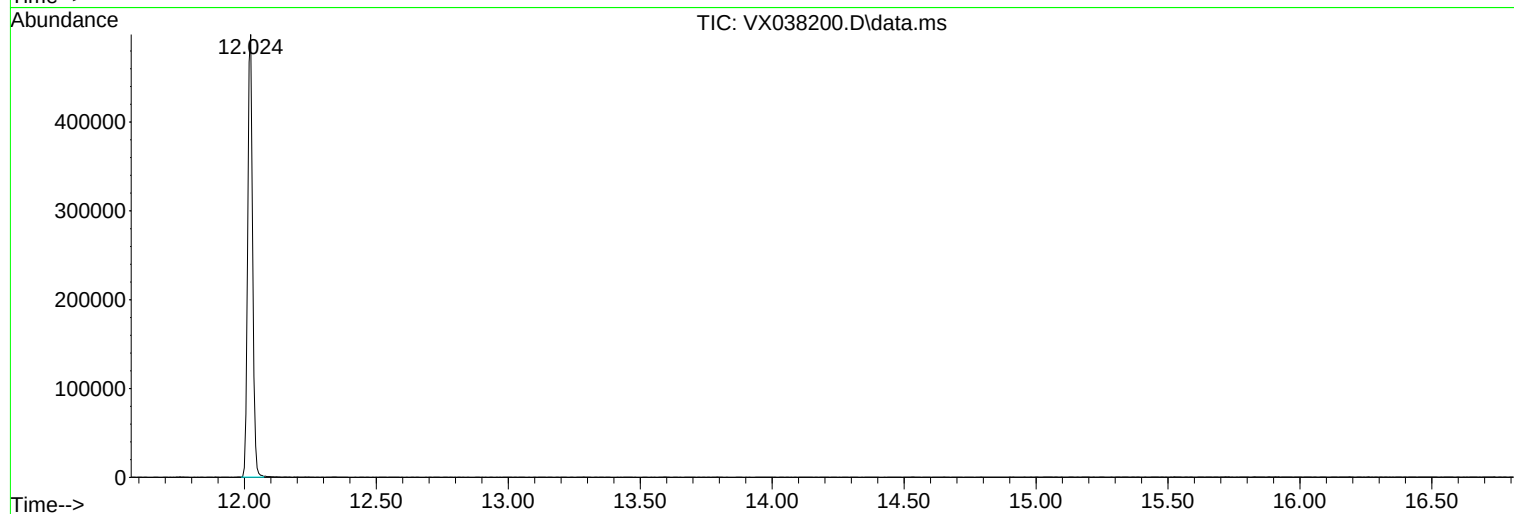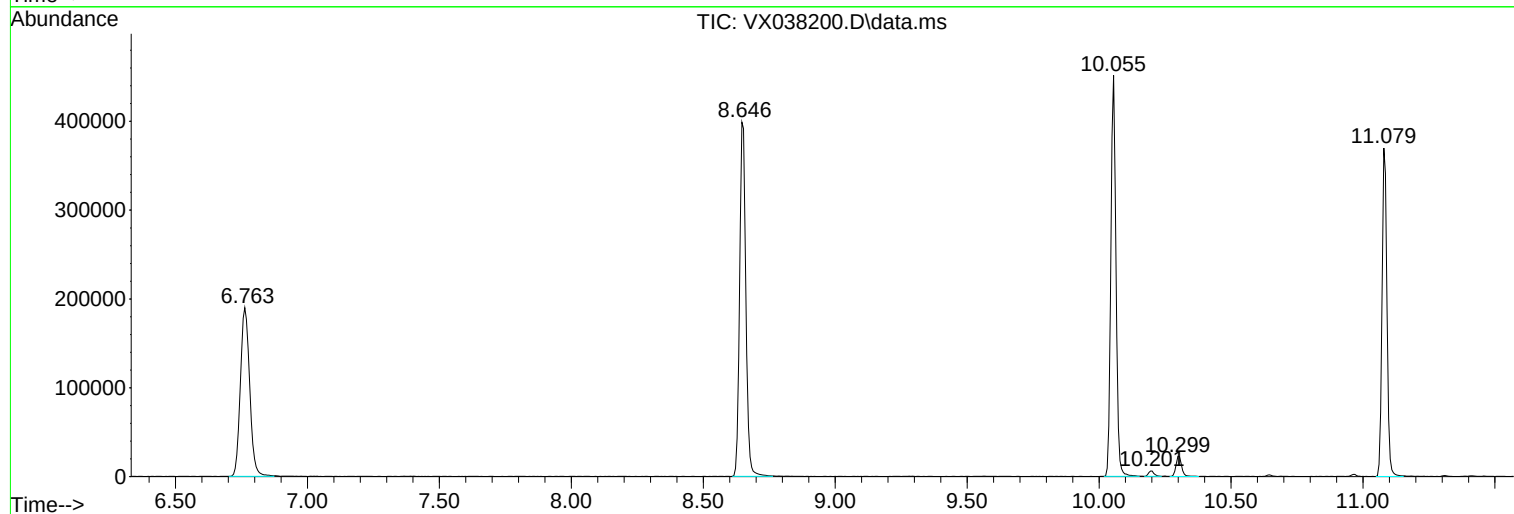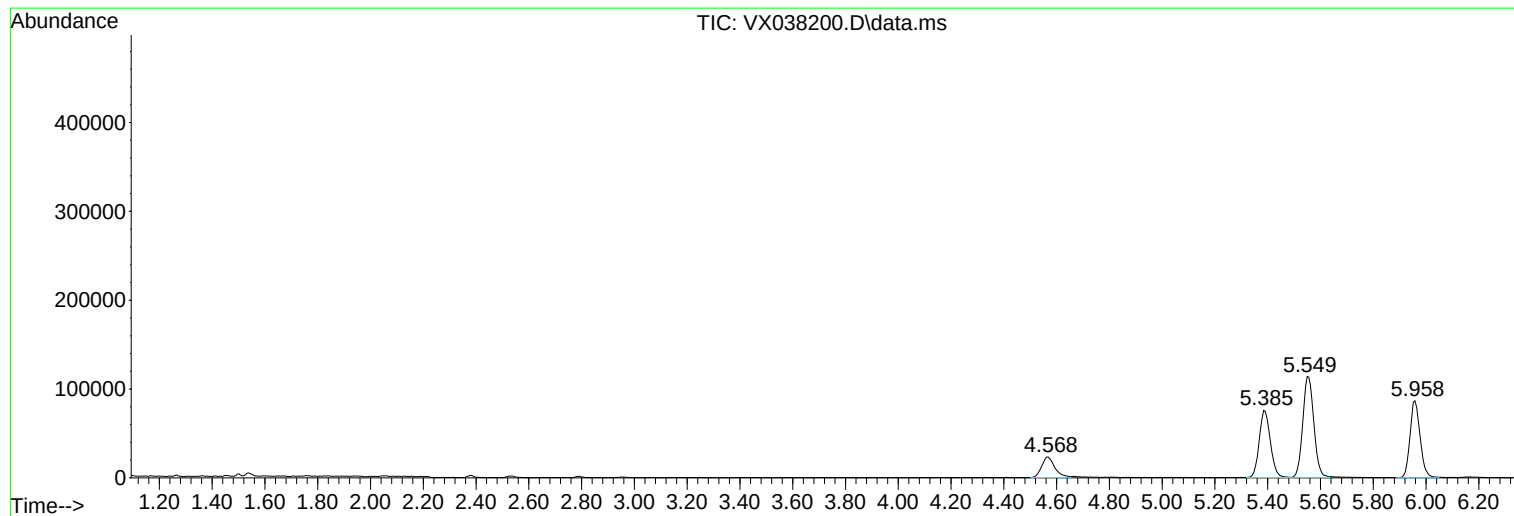

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101023\
Data File : VX038200.D
Acq On : 10 Oct 2023 14:46
Operator : JC/MD
Sample : 04782-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB-100323

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101023\
Data File : VX038200.D
Acq On : 10 Oct 2023 14:46
Operator : JC/MD
Sample : 04782-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB-100323

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------