

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101023\
 Data File : VX038206.D
 Acq On : 10 Oct 2023 17:05
 Operator : JC/MD
 Sample : 04782-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GW-5-23-26

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M

Title : SW846 8260

Signal : TIC: VX038206.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.099	648	658	673	rVB3	8165	23659	3.82%	0.678%
2	5.385	693	705	721	rBV2	73149	213298	34.42%	6.114%
3	5.550	721	732	750	rVV	109797	317063	51.16%	9.088%
4	5.958	789	799	812	rBV	85921	219650	35.44%	6.296%
5	6.763	922	931	950	rBV2	182649	444387	71.70%	12.738%
6	8.647	1234	1240	1250	rBV	382171	619744	100.00%	17.765%
7	8.720	1250	1252	1261	rVB	3769	6258	1.01%	0.179%
8	9.275	1335	1343	1349	rBV3	6312	9433	1.52%	0.270%
9	10.055	1465	1471	1490	rBV	427869	582786	94.04%	16.705%
10	10.305	1505	1512	1519	rVB2	5621	8389	1.35%	0.240%
11	11.079	1634	1639	1654	rBV	339225	445301	71.85%	12.764%
12	12.024	1788	1794	1807	rBV	461012	598685	96.60%	17.161%




Sum of corrected areas: 3488653

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101023\
Data File : VX038206.D
Acq On : 10 Oct 2023 17:05
Operator : JC/MD
Sample : 04782-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GW-5-23-26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

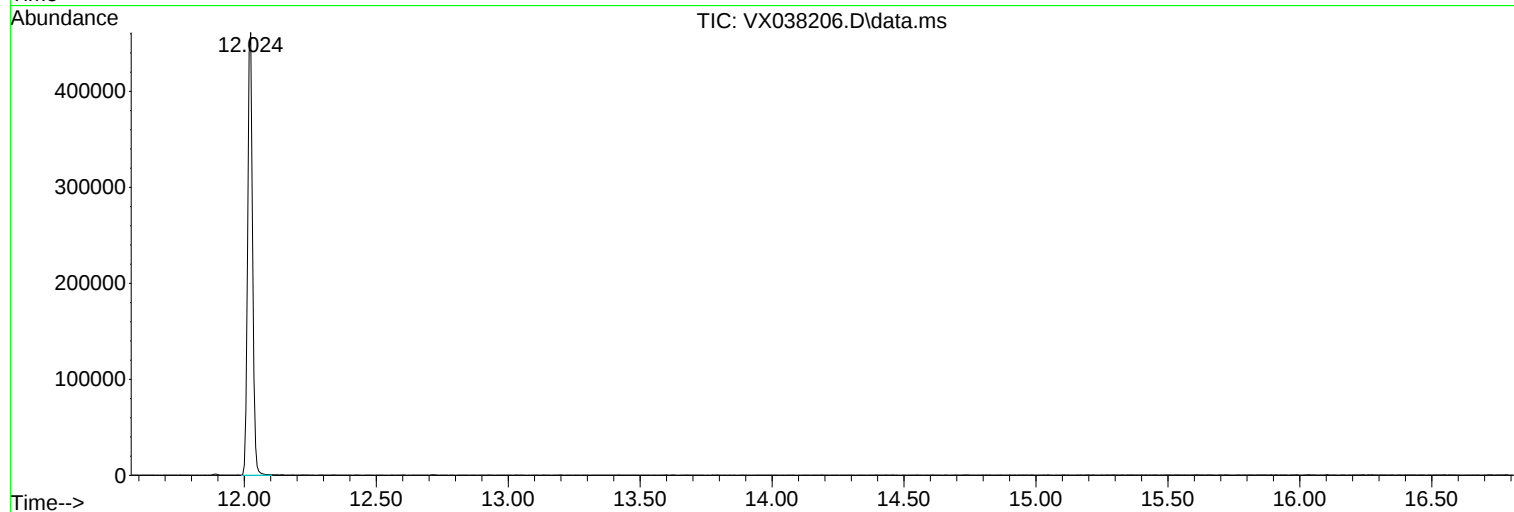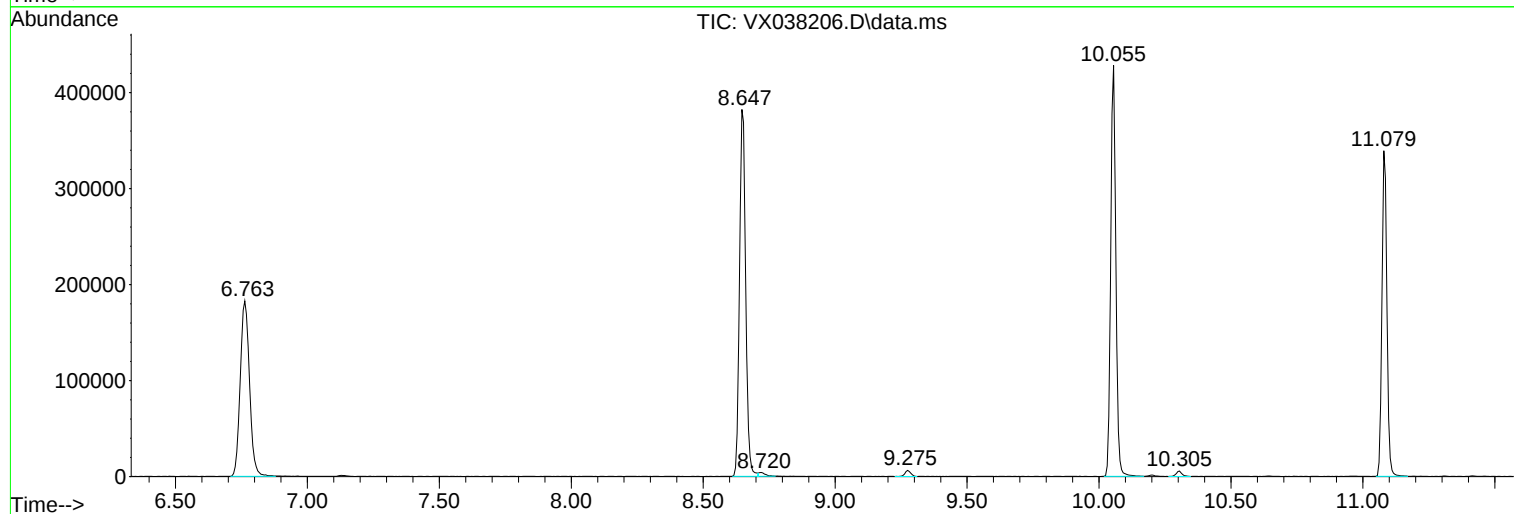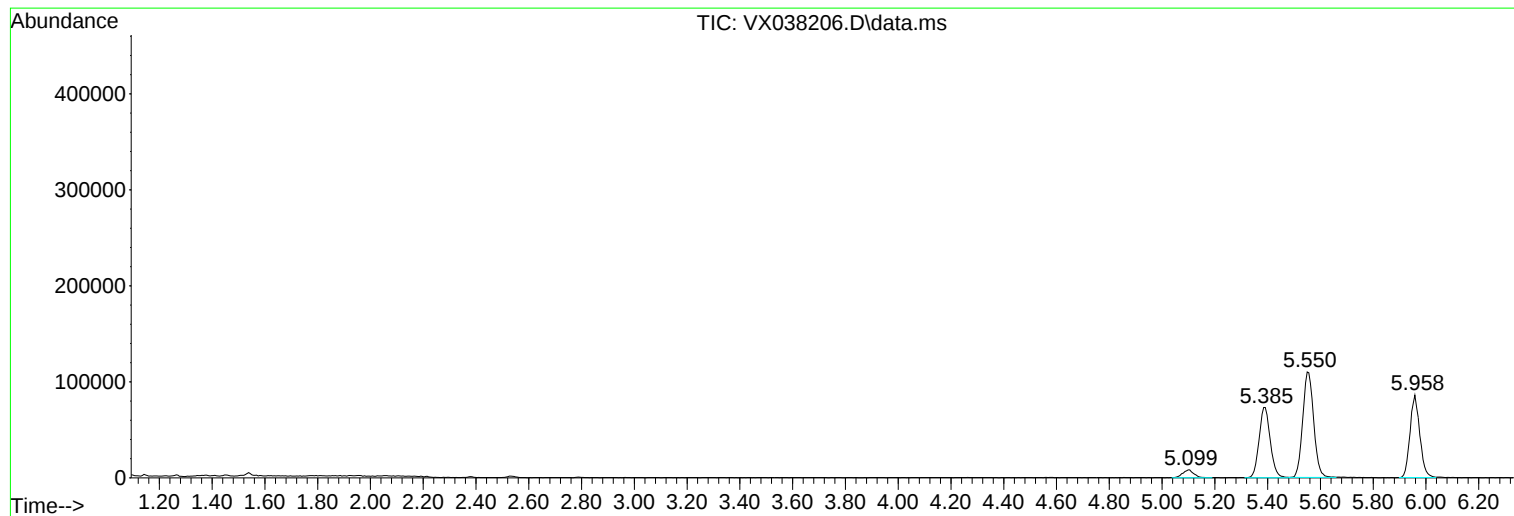

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101023\
Data File : VX038206.D
Acq On : 10 Oct 2023 17:05
Operator : JC/MD
Sample : 04782-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GW-5-23-26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101023\
Data File : VX038206.D
Acq On : 10 Oct 2023 17:05
Operator : JC/MD
Sample : 04782-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GW-5-23-26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc