

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101023\
 Data File : VX038208.D
 Acq On : 10 Oct 2023 17:52
 Operator : JC/MD
 Sample : 04782-17 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP-1

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M

Title : SW846 8260

Signal : TIC: VX038208.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.550	69	76	80	rBV	8995	15813	2.54%	0.454%
2	4.562	560	570	582	rBV2	4100	14054	2.26%	0.403%
3	5.385	693	705	722	rBV3	71900	211882	34.08%	6.078%
4	5.556	722	733	749	rVV	107085	316007	50.82%	9.064%
5	5.958	789	799	816	rBV	83018	218623	35.16%	6.271%
6	6.763	921	931	944	rBV	179676	438963	70.60%	12.591%
7	8.647	1234	1240	1255	rBV	376216	610255	98.15%	17.504%
8	10.055	1465	1471	1487	rBV	424895	578151	92.99%	16.583%
9	10.299	1502	1511	1519	rBV2	4370	6754	1.09%	0.194%
10	11.079	1634	1639	1652	rBV	345245	454036	73.02%	13.023%
11	12.024	1788	1794	1805	rBV	482242	621768	100.00%	17.835%




Sum of corrected areas: 3486306

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101023\
Data File : VX038208.D
Acq On : 10 Oct 2023 17:52
Operator : JC/MD
Sample : 04782-17 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

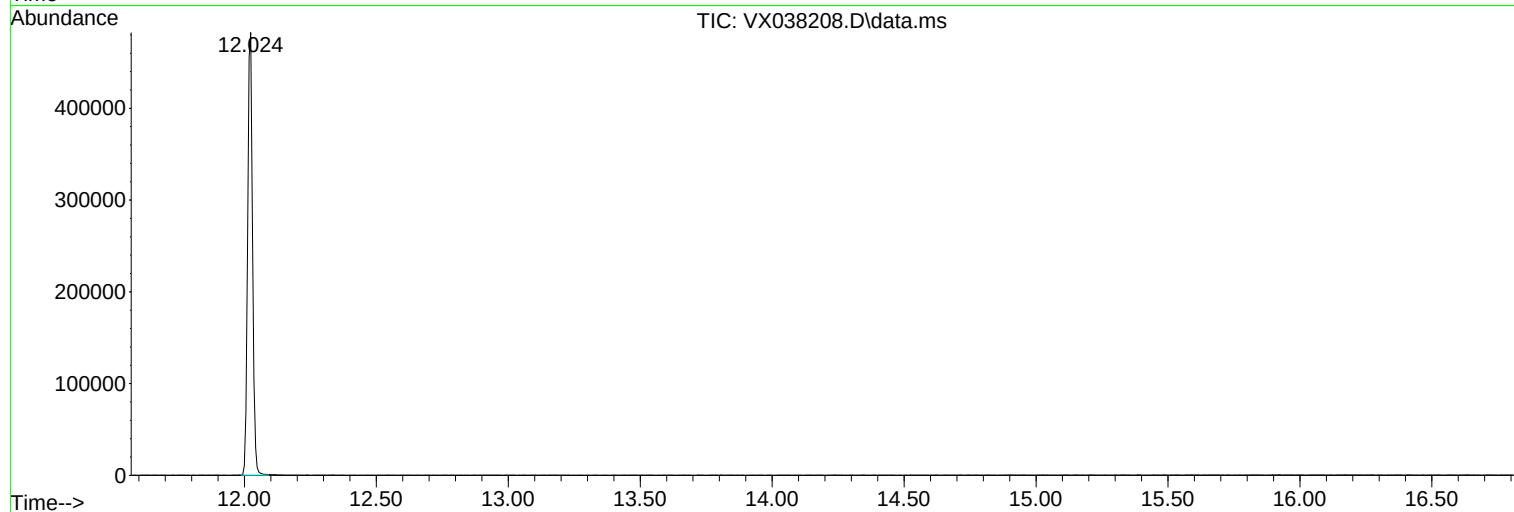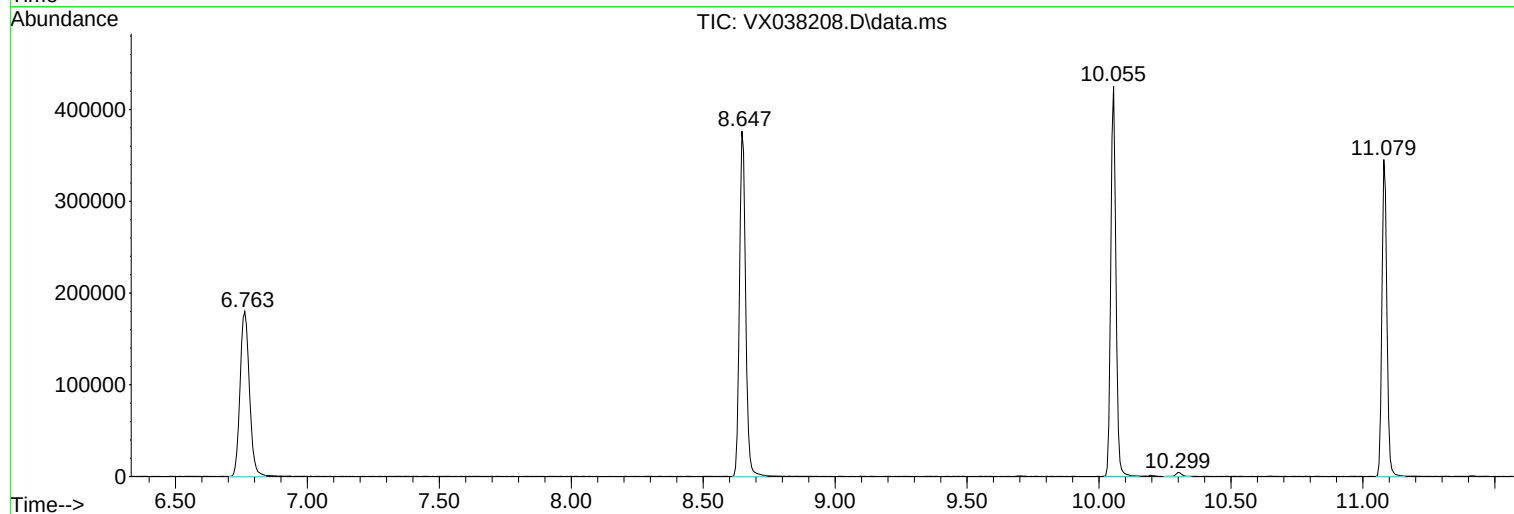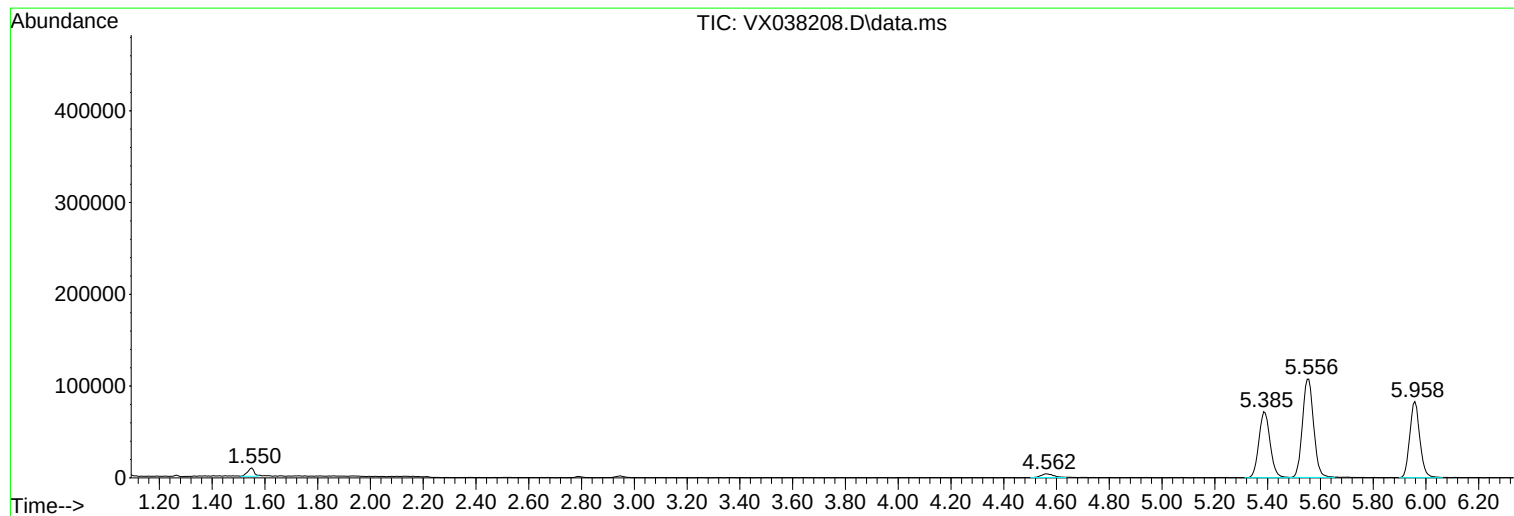

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101023\
Data File : VX038208.D
Acq On : 10 Oct 2023 17:52
Operator : JC/MD
Sample : 04782-17 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101023\
Data File : VX038208.D
Acq On : 10 Oct 2023 17:52
Operator : JC/MD
Sample : 04782-17 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------