


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101118\
Data File : VX005254.D
Acq On : 11 Oct 2018 15:16
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
Title : SW846 8260
Last Update : Wed Oct 03 04:00:03 2018

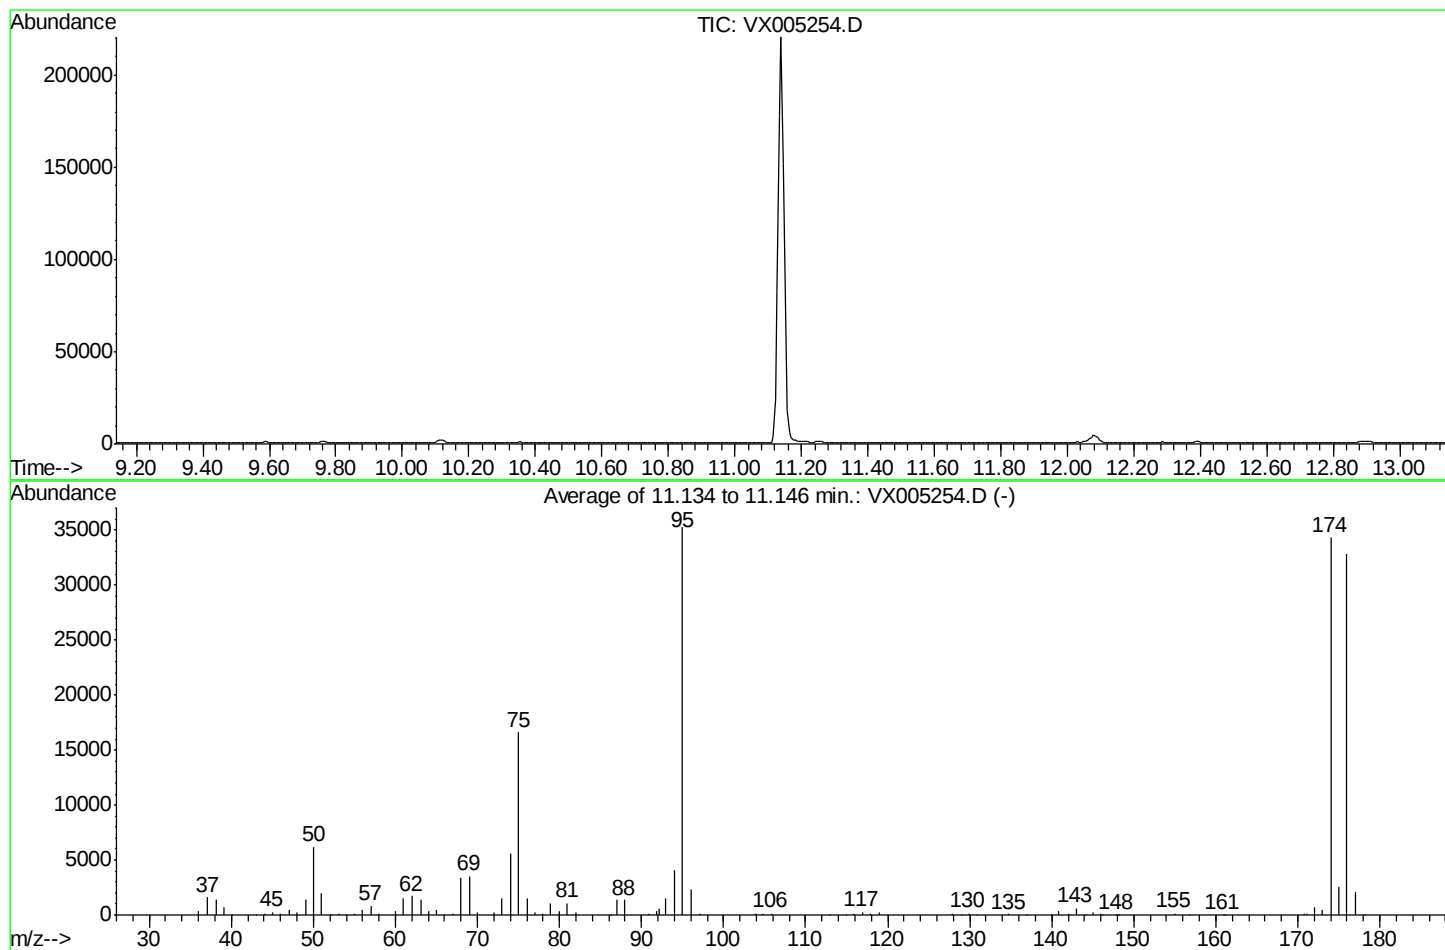

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	6230	PASS
75	95	30	60	47.2	16640	PASS
95	95	100	100	100.0	35248	PASS
96	95	5	9	6.7	2375	PASS
173	174	0.00	2	1.3	442	PASS
174	95	50	100	97.3	34280	PASS
175	174	5	9	7.6	2604	PASS
176	174	95	101	95.6	32773	PASS
177	176	5	9	6.3	2066	PASS