


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX101119\
Data File : VX013009.D
Acq On : 11 Oct 2019 11:31
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X100819W.M
Title : SW846 8260
Last Update : Fri Oct 11 09:48:22 2019

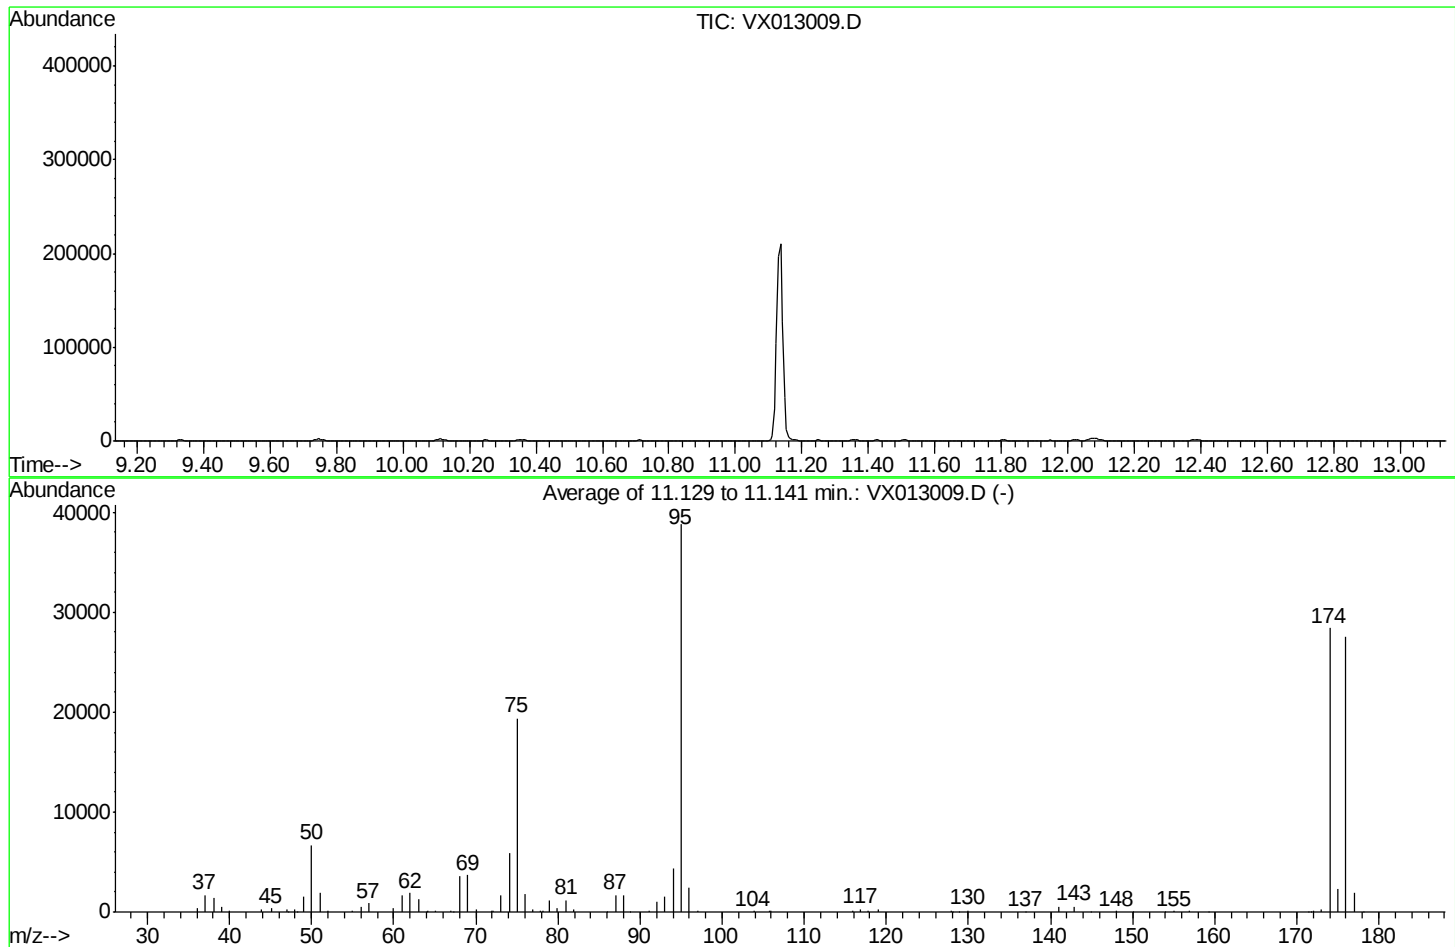

AutoFind: Scans 1680, 1681, 1682; Background Corrected with Scan 1673

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	6666	PASS
75	95	30	60	50.0	19386	PASS
95	95	100	100	100.0	38805	PASS
96	95	5	9	6.3	2435	PASS
173	174	0.00	2	0.9	262	PASS
174	95	50	100	73.2	28416	PASS
175	174	5	9	7.9	2251	PASS
176	174	95	101	96.9	27528	PASS
177	176	5	9	7.1	1941	PASS