

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101122\
 Data File : VX032049.D
 Acq On : 11 Oct 2022 20:01
 Operator : JC/MD
 Sample : N5067-16MEDL 20X
 Misc : 9.68g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMP-B-3-VERTME

Quant Time: Oct 12 05:19:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 06 14:28:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	75635	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	112411	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	114975	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	70511	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	78418	50.203	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 100.400%			
35) Dibromofluoromethane	5.385	113	59103	46.449	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 92.900%			
50) Toluene-d8	8.647	98	228874	49.987	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 99.980%			
62) 4-Bromofluorobenzene	11.079	95	75554	46.676	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 93.360%			
Target Compounds						Qvalue
5) Bromomethane	1.611	94	433	Below Cal		96
11) Tert butyl alcohol	2.946	59	1093	5.624 ug/l #		73
16) Acetone	2.386	43	193	0.364 ug/l #		45
18) Methyl Acetate	2.703	43	780	0.445 ug/l #		88
20) Methylene Chloride	2.794	84	479	0.343 ug/l #		84
31) Cyclohexane	5.556	56	1921	1.029 ug/l #		30
36) 1,1-Dichloropropene	5.550	75	6431	3.811 ug/l #		50
38) Carbon Tetrachloride	5.556	117	7851	4.551 ug/l #		16
39) Methylcyclohexane	7.379	83	871	0.433 ug/l #		73
40) Benzene	6.037	78	17567	3.555 ug/l		95
43) Isopropyl Acetate	6.610	43	853	0.354 ug/l #		61
51) 4-Methyl-2-Pentanone	8.647	43	1193	0.747 ug/l #		1
52) Toluene	8.720	92	2961	0.917 ug/l		92
55) 1,1,2-Trichloroethane	9.104	97	274	0.201 ug/l #		15
59) 2-Hexanone	9.384	43	450	0.382 ug/l #		25
67) Ethyl Benzene	10.195	91	169262	28.720 ug/l		100
68) m/p-Xylenes	10.299	106	67283	28.728 ug/l		97
69) o-Xylene	10.640	106	24951	10.961 ug/l		99
70) Styrene	10.640	104	1665	0.458 ug/l #		1
73) Isopropylbenzene	10.963	105	17616	3.312 ug/l		96
75) 1,1,2,2-Tetrachloroethane	11.219	83	359	0.212 ug/l #		25
76) 1,2,3-Trichloropropane	11.079	75	41558	28.757 ug/l #		37
78) n-propylbenzene	11.305	91	11638	1.924 ug/l		99
79) 2-Chlorotoluene	11.378	91	8726	2.397 ug/l #		40
80) 1,3,5-Trimethylbenzene	11.451	105	27011	6.124 ug/l		98
81) trans-1,4-Dichloro-2-b...	11.079	75	41558	98.305 ug/l #		11
82) 4-Chlorotoluene	11.451	91	3033	0.728 ug/l #		44
83) tert-Butylbenzene	11.969	119	7031	1.611 ug/l		69
84) 1,2,4-Trimethylbenzene	11.756	105	81129	18.106 ug/l		100
85) sec-Butylbenzene	11.756	105	81129	15.011 ug/l #		56
86) p-Isopropyltoluene	11.969	119	7224	1.588 ug/l		92
89) n-Butylbenzene	12.329	91	3898	1.023 ug/l #		34
90) Hexachloroethane	12.414	117	4154	6.899 ug/l #		15
92) 1,2-Dibromo-3-Chloropr...	12.963	75	86	0.278 ug/l #		3
95) Naphthalene	13.774	128	490117	95.029 ug/l		100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101122\
Data File : VX032049.D
Acq On : 11 Oct 2022 20:01
Operator : JC/MD
Sample : N5067-16MEDL 20X
Misc : 9.68g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP-B-3-VERTME

Quant Time: Oct 12 05:19:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 06 14:28:46 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101122\
Data File : VX032049.D
Acq On : 11 Oct 2022 20:01
Operator : JC/MD
Sample : N5067-16MEDL 20X
Misc : 9.68g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP-B-3-VERTME


Quant Time: Oct 12 05:19:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 06 14:28:46 2022
Response via : Initial Calibration

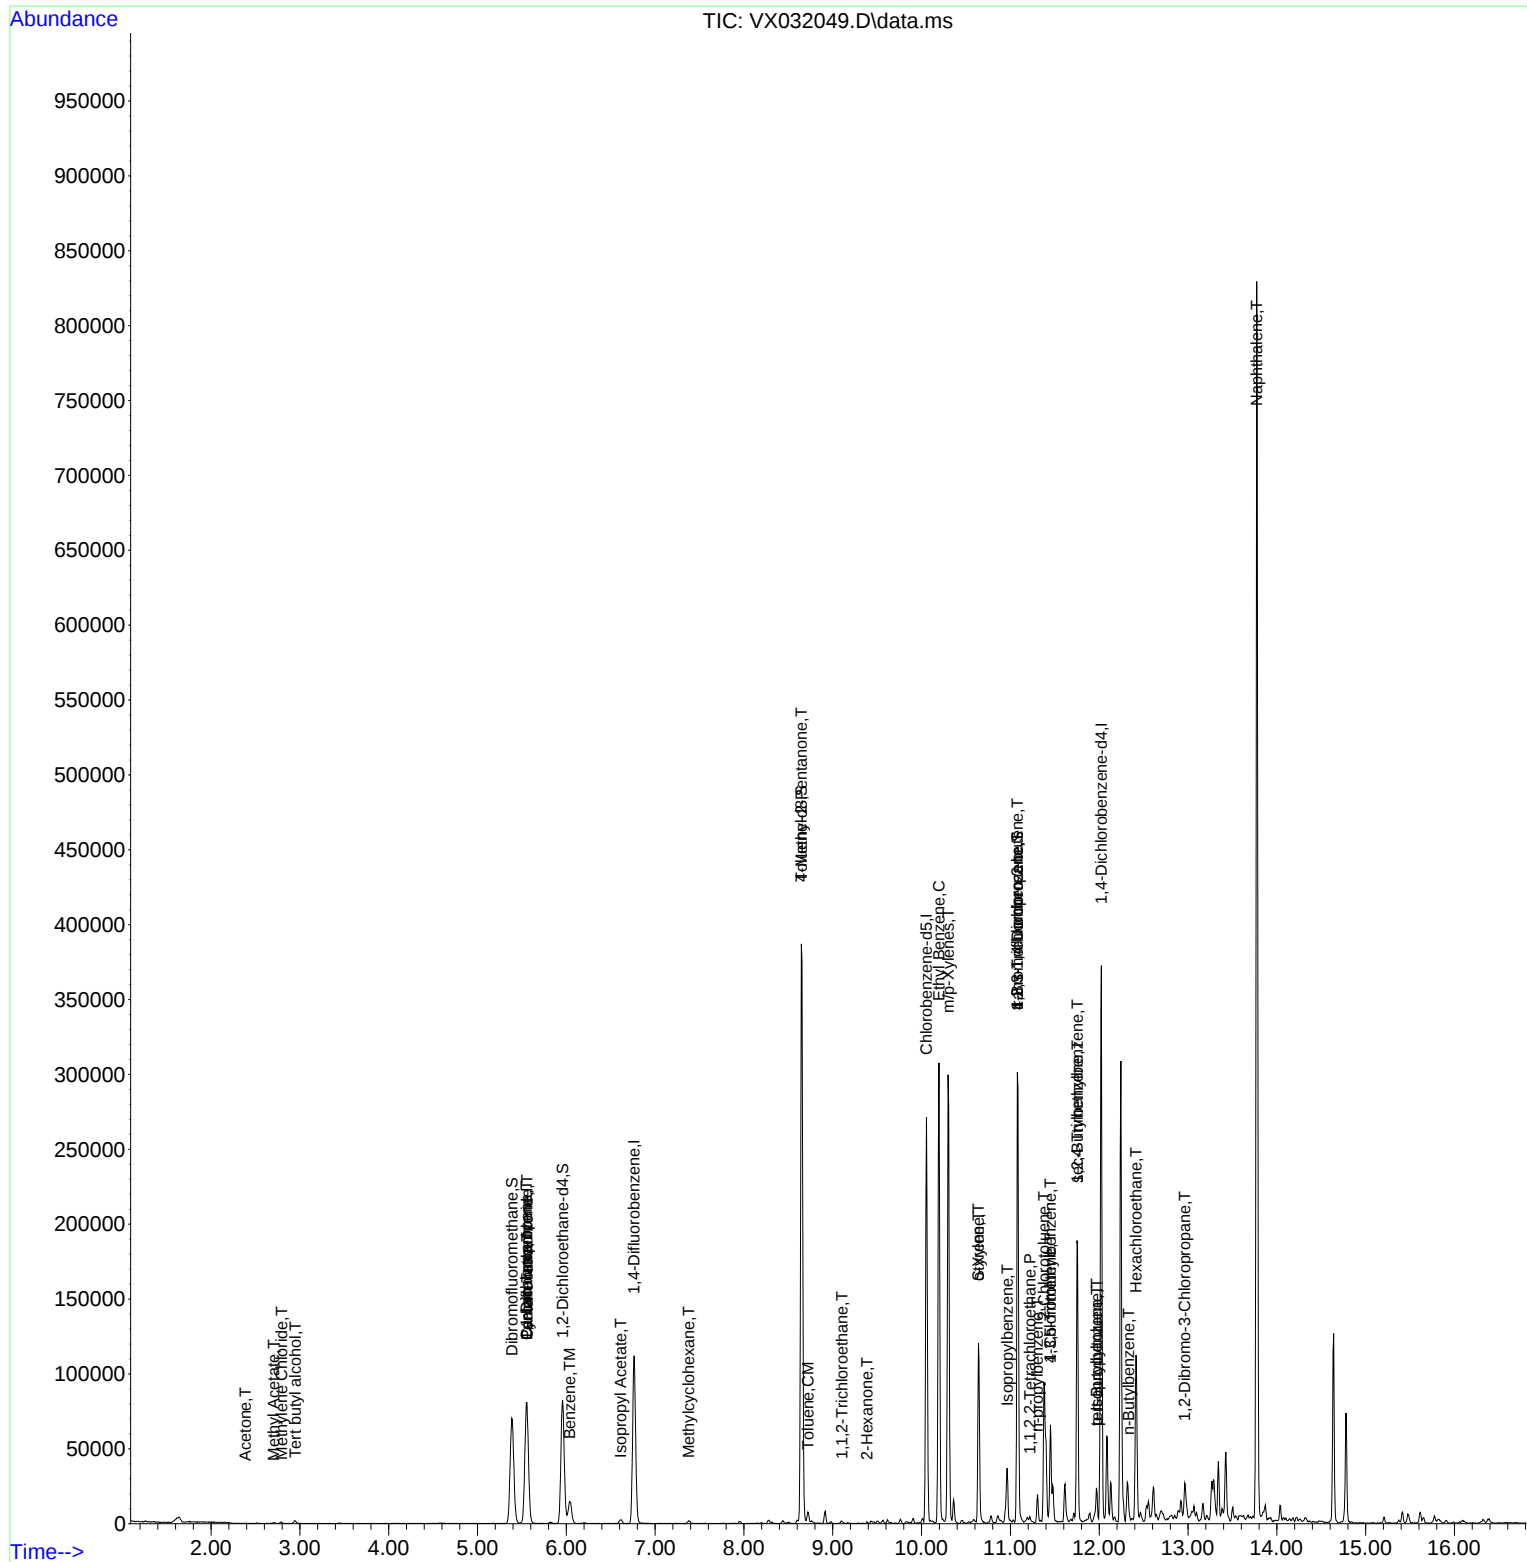



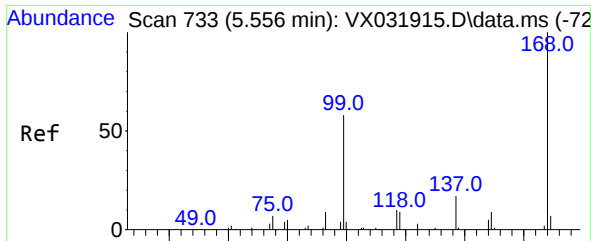


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01

Instrument :
MSVOA_X
ClientSampleId :
COMP-B-3-VERTEME



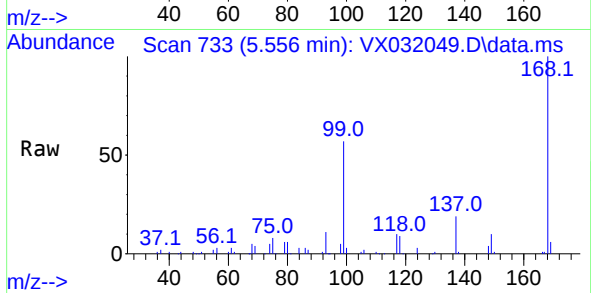



Tgt Ion:168 Resp: 75635
Ion Ratio Lower Upper
168 100
99 56.5 48.8 73.2

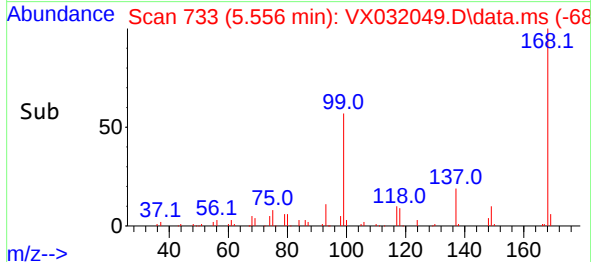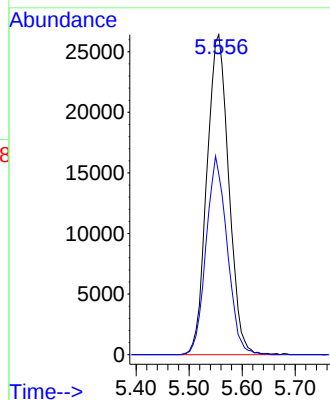

#5
Bromomethane
Concen: Below Cal
RT: 1.611 min Scan# 86
Delta R.T. 0.000 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01

Tgt Ion: 94 Resp: 433
Ion Ratio Lower Upper
94 100
96 97.1 74.4 111.6

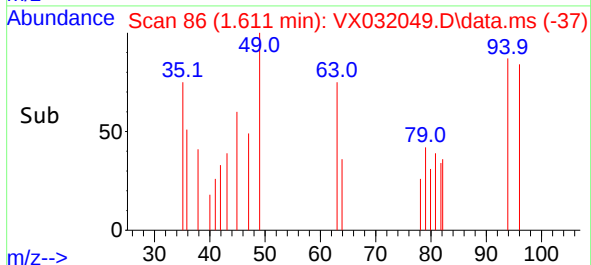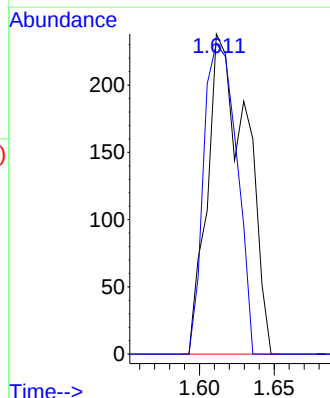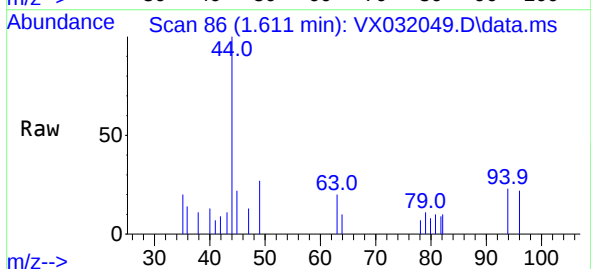



#11

Tert butyl alcohol

Concen: 5.624 ug/l

RT: 2.946 min Scan# 305

Delta R.T. -0.061 min

Lab File: VX032049.D

Acq: 11 Oct 2022 20:01

Instrument :

MSVOA_X

ClientSampleId :





COMP-B-3-VERTME

Tgt Ion: 59 Resp: 1093

Ion Ratio Lower Upper

59 100

57 0.0 8.2 12.2#

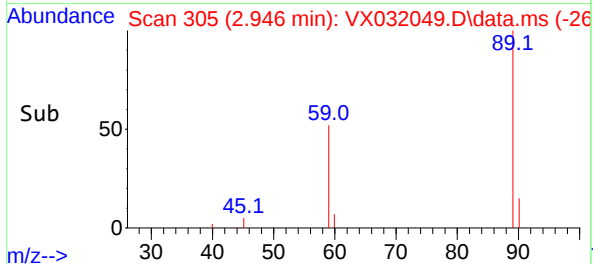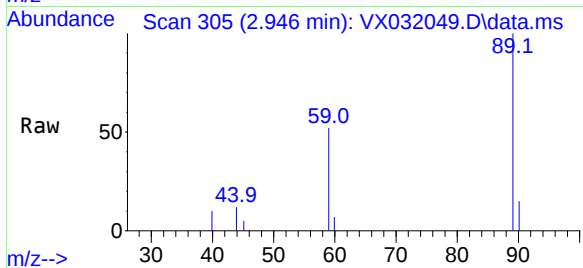

#16

Acetone

Concen: 0.364 ug/l

RT: 2.386 min Scan# 213

Delta R.T. -0.006 min

Lab File: VX032049.D




Acq: 11 Oct 2022 20:01


Tgt Ion: 43 Resp: 193

Ion Ratio Lower Upper

43 100

58 0.0 23.8 35.8#


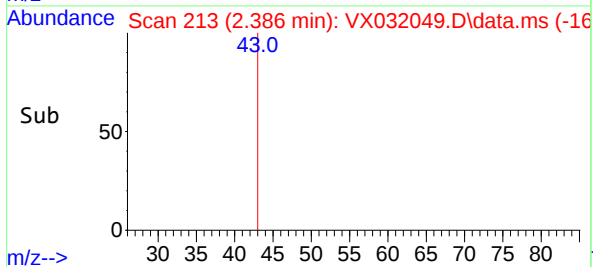

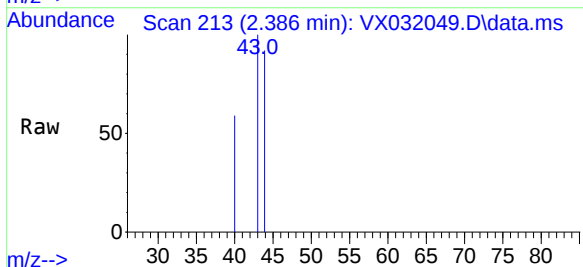




#18
Methyl Acetate
Concen: 0.445 ug/l
RT: 2.703 min Scan# 20
Delta R.T. -0.006 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01




Instrument :
MSVOA_X
ClientSampleId :
COMP-B-3-VERTEME


Tgt Ion: 43 Resp: 780
Ion Ratio Lower Upper
43 100
74 17.2 18.6 27.8#

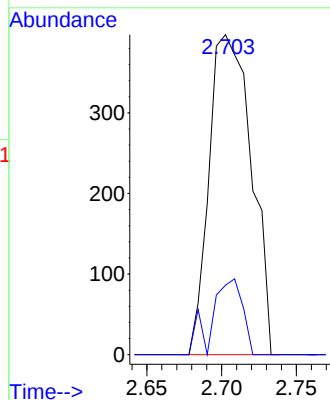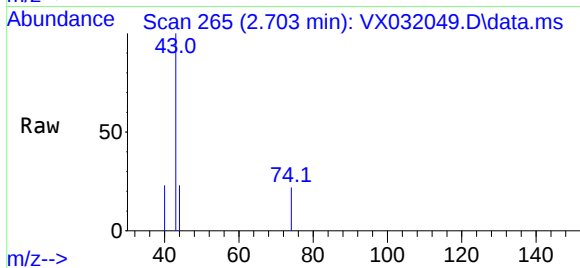

#20
Methylene Chloride
Concen: 0.343 ug/l
RT: 2.794 min Scan# 280
Delta R.T. 0.006 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01


Tgt Ion: 84 Resp: 479
Ion Ratio Lower Upper
84 100
49 136.7 105.9 158.9
51 65.7 32.2 48.2#
86 43.3 50.8 76.2#

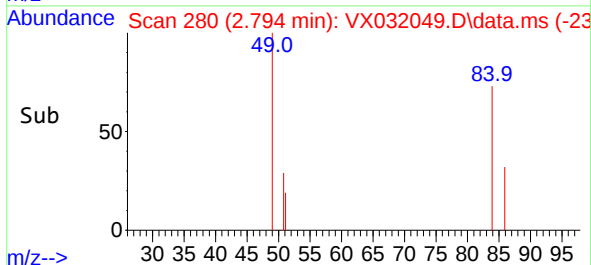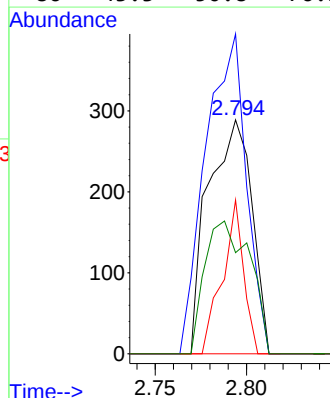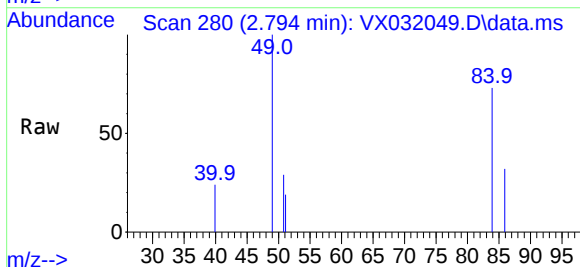



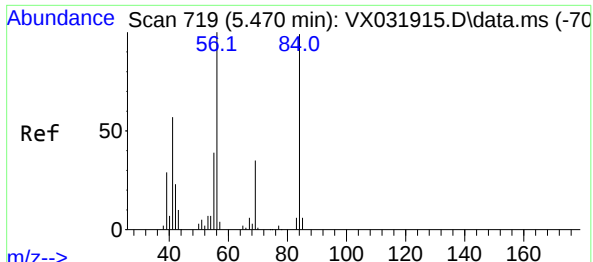


#31
Cyclohexane
Concen: 1.029 ug/l
RT: 5.556 min Scan# 719
Delta R.T. 0.086 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01

Instrument :
MSVOA_X
ClientSampleId :
COMP-B-3-VERTME



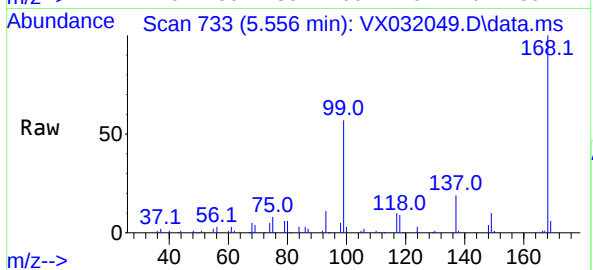



Tgt Ion: 56 Resp: 1921
Ion Ratio Lower Upper
56 100
69 140.2 25.1 37.7#
84 111.0 70.2 105.4#

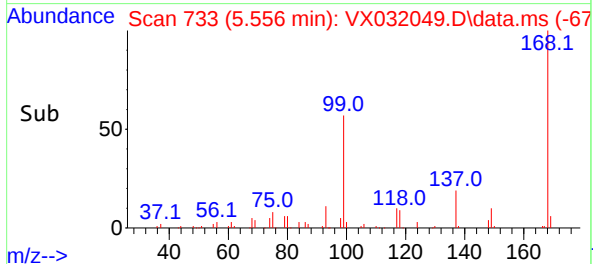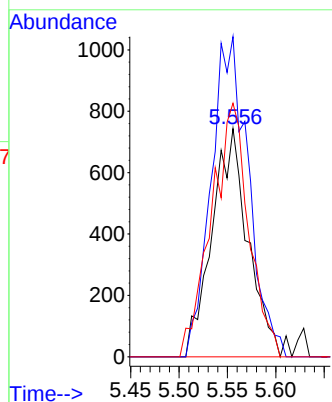

#33
1,2-Dichloroethane-d4
Concen: 50.203 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01

Tgt Ion: 65 Resp: 78418
Ion Ratio Lower Upper
65 100
67 50.1 0.0 102.4


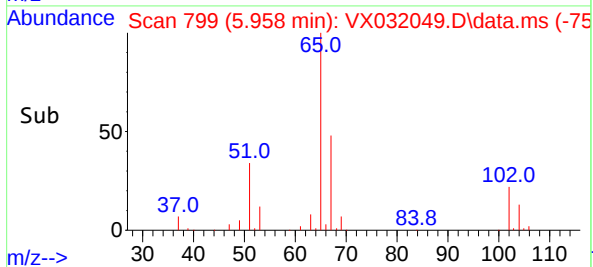
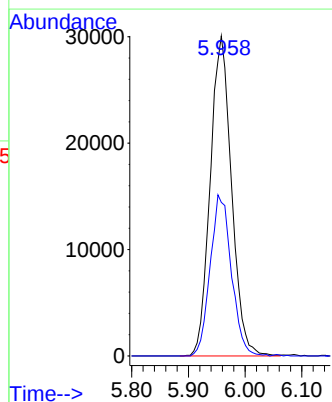
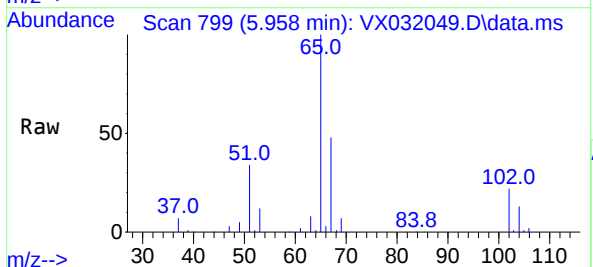




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. -0.000 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01




Instrument :
MSVOA_X
ClientSampleId :
COMP-B-3-VERTME


Tgt Ion:114 Resp: 112411
Ion Ratio Lower Upper
114 100
63 20.1 0.0 42.6
88 16.1 0.0 33.0



#35
Dibromofluoromethane
Concen: 46.449 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01


Tgt Ion:113 Resp: 59103
Ion Ratio Lower Upper
113 100
111 104.6 82.4 123.6
192 19.3 14.1 21.1

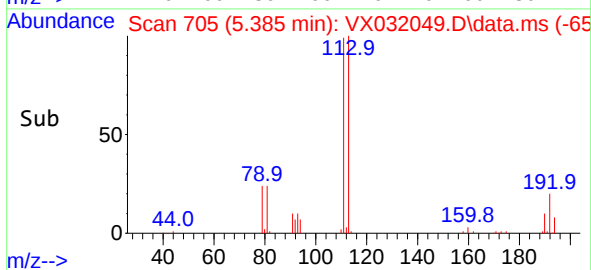



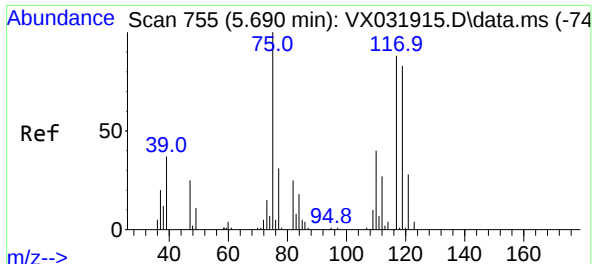


#36
1,1-Dichloropropene
Concen: 3.811 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.140 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01


Instrument :
MSVOA_X
ClientSampleId :
COMP-B-3-VERTME

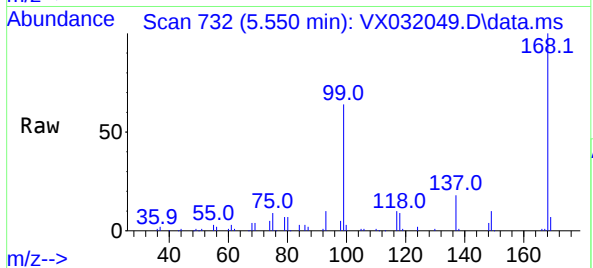



Tgt Ion: 75 Resp: 6431
Ion Ratio Lower Upper
75 100
110 9.5 17.5 52.5#
77 0.0 24.9 37.3#

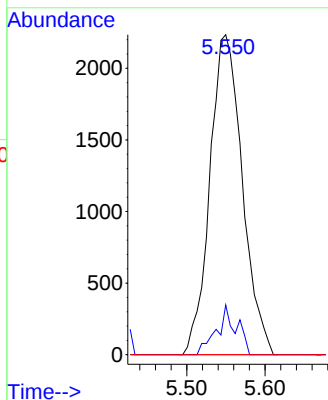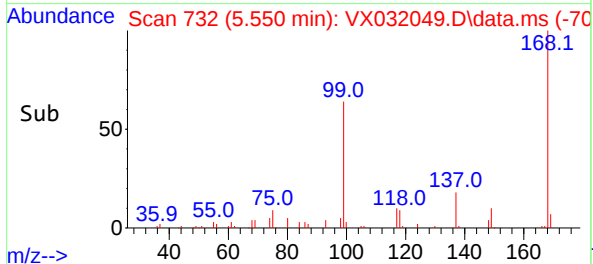


#38
Carbon Tetrachloride
Concen: 4.551 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.121 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01

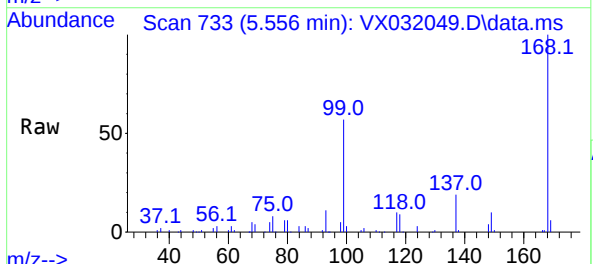

Tgt Ion: 117 Resp: 7851
Ion Ratio Lower Upper
117 100
119 3.3 74.6 112.0#
121 0.0 25.3 37.9#

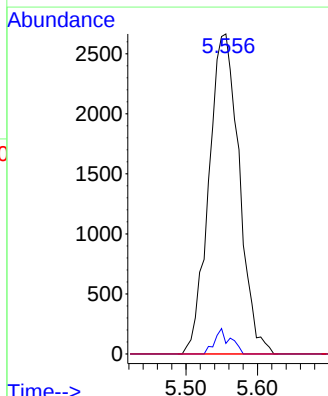



#39

Methylcyclohexane

Concen: 0.433 ug/l

RT: 7.379 min Scan# 1032

Delta R.T. -0.006 min

Lab File: VX032049.D

Acq: 11 Oct 2022 20:01

Instrument :

MSVOA_X

ClientSampleId :

COMP-B-3-VERTME





Tgt Ion: 83 Resp: 871

Ion Ratio Lower Upper

83 100

55 56.0 61.0 91.4#

98 68.7 37.7 56.5#

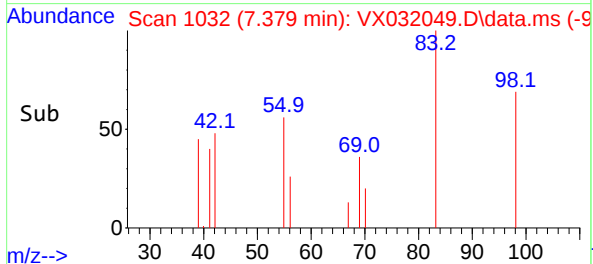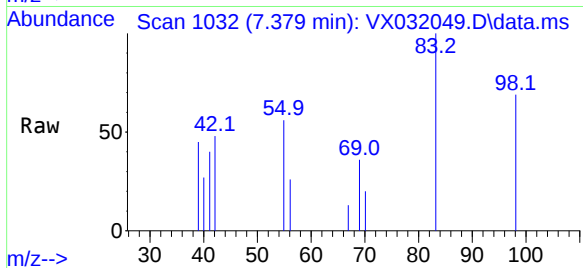

#40

Benzene

Concen: 3.555 ug/l

RT: 6.037 min Scan# 812

Delta R.T. 0.000 min

Lab File: VX032049.D




Acq: 11 Oct 2022 20:01


Tgt Ion: 78 Resp: 17567

Ion Ratio Lower Upper

78 100

77 21.0 18.7 28.1


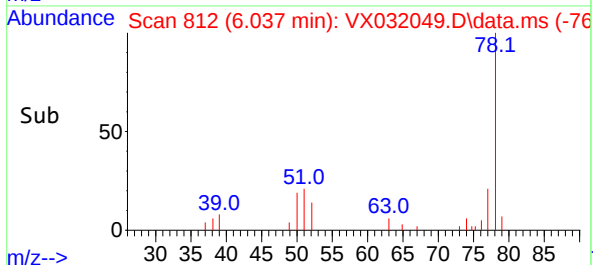
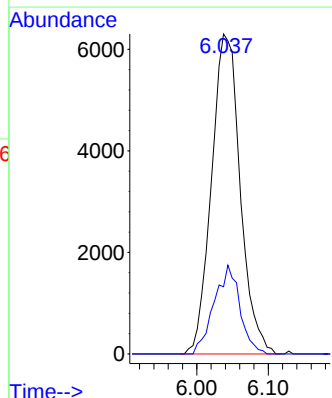
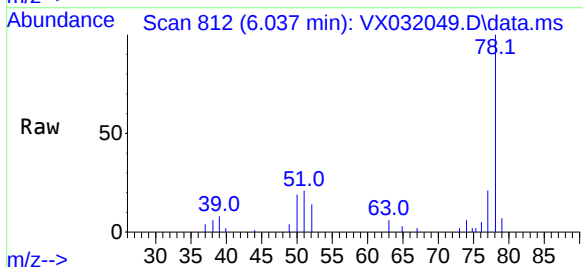




#43
Isopropyl Acetate
Concen: 0.354 ug/l
RT: 6.610 min Scan# 90
Delta R.T. 0.268 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01




Instrument :
MSVOA_X
ClientSampleId :
COMP-B-3-VERTME


Tgt Ion: 43 Resp: 853
Ion Ratio Lower Upper
43 100
61 0.0 15.3 22.9#
87 0.0 10.6 15.8#

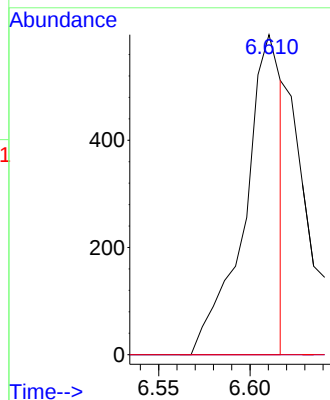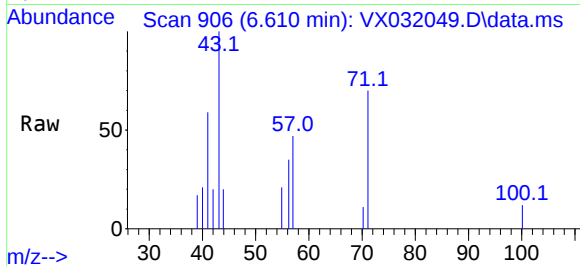

#50
Toluene-d8
Concen: 49.987 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.006 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01

Tgt Ion: 98 Resp: 228874
Ion Ratio Lower Upper
98 100
100 65.6 52.5 78.7

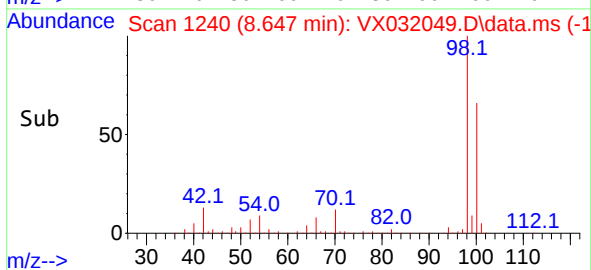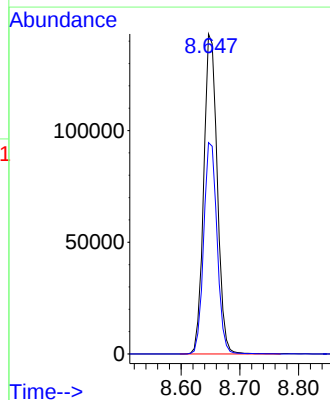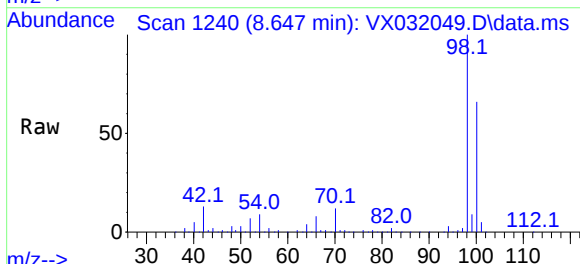



#51

4-Methyl-2-Pentanone

Concen: 0.747 ug/l

RT: 8.647 min Scan# 1193

Delta R.T. 0.074 min

Lab File: VX032049.D

Acq: 11 Oct 2022 20:01

Instrument :

MSVOA_X

ClientSampleId :





COMP-B-3-VERTME

Tgt Ion: 43 Resp: 1193

Ion Ratio Lower Upper

43 100

58 157.7 30.6 46.0#

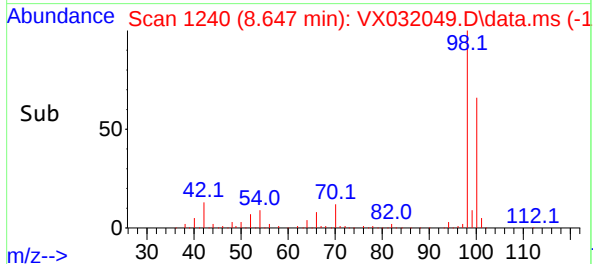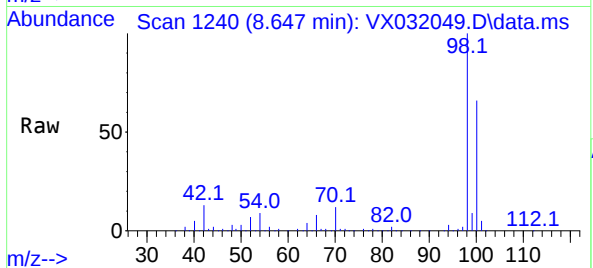

#52

Toluene

Concen: 0.917 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. -0.000 min

Lab File: VX032049.D




Acq: 11 Oct 2022 20:01


Tgt Ion: 92 Resp: 2961

Ion Ratio Lower Upper

92 100

91 160.2 137.1 205.7

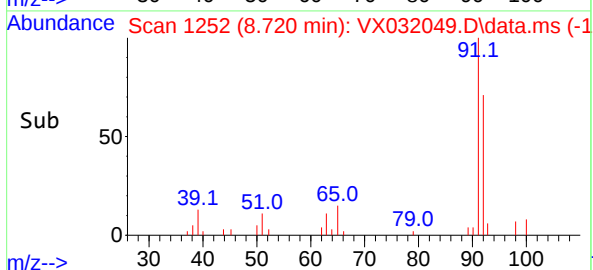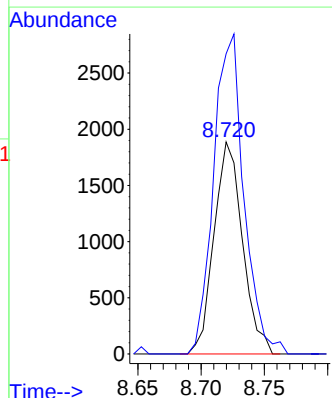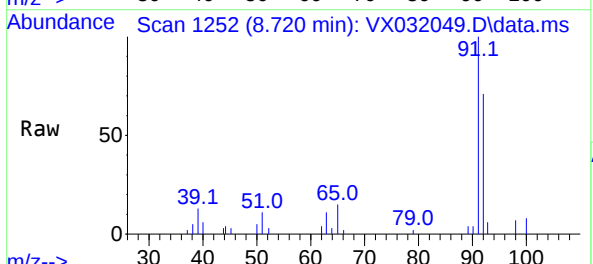







#55
1,1,2-Trichloroethane
Concen: 0.201 ug/l
RT: 9.104 min Scan# 11
Delta R.T. -0.048 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01

Instrument :
MSVOA_X
ClientSampleId :
COMP-B-3-VERTEME

Tgt Ion: 97 Resp: 274




Ion	Ratio	Lower	Upper
97	100		
83	0.0	69.0	103.6#
85	0.0	44.1	66.1#
99	0.0	51.3	76.9#

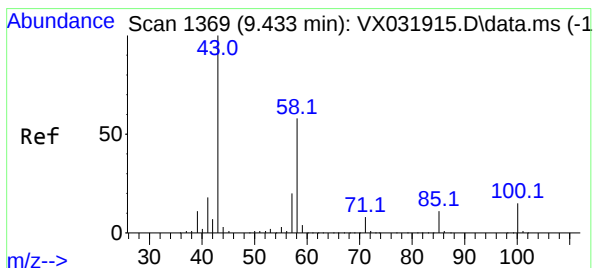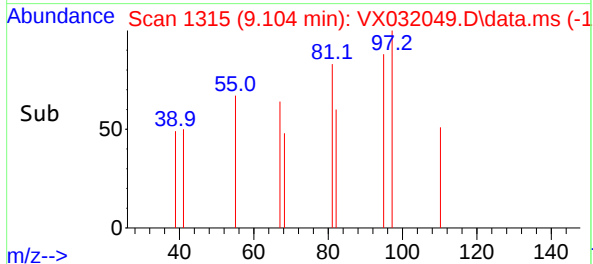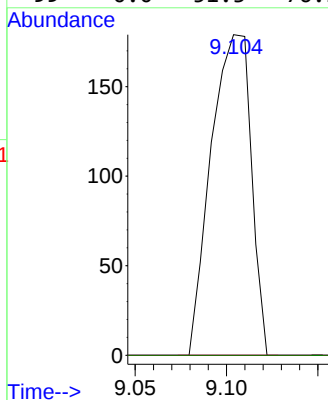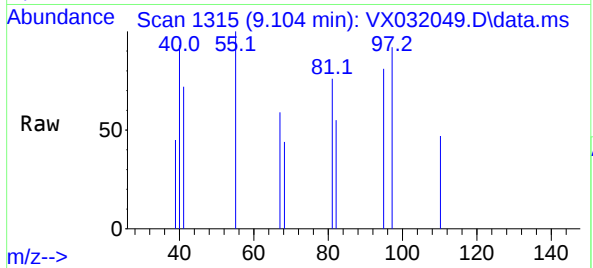


#59
2-Hexanone
Concen: 0.382 ug/l
RT: 9.384 min Scan# 1361
Delta R.T. -0.049 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01

Tgt Ion: 43 Resp: 450

Ion	Ratio	Lower	Upper
43	100		
58	0.0	26.7	80.0#


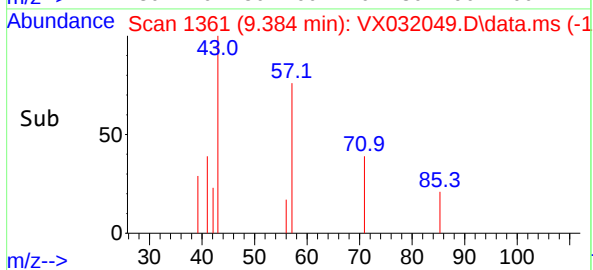
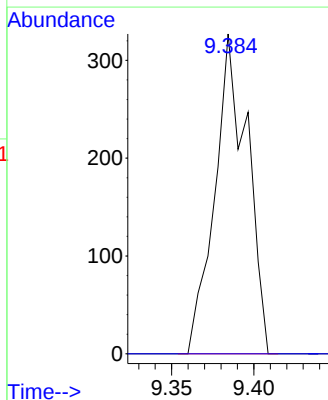
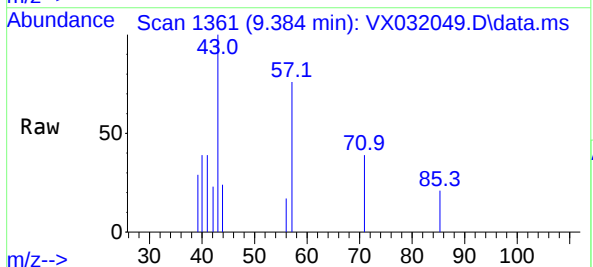




#62
4-Bromofluorobenzene
Concen: 46.676 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01




Instrument :
MSVOA_X
ClientSampleId :
COMP-B-3-VERTME


Tgt Ion: 95 Resp: 75554
Ion Ratio Lower Upper
95 100
174 78.4 0.0 153.2
176 75.5 0.0 144.0

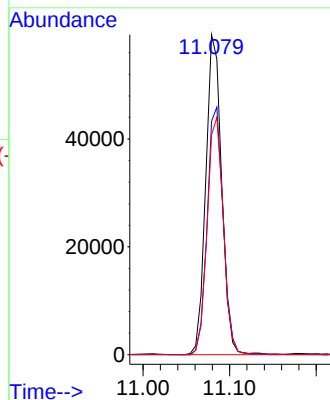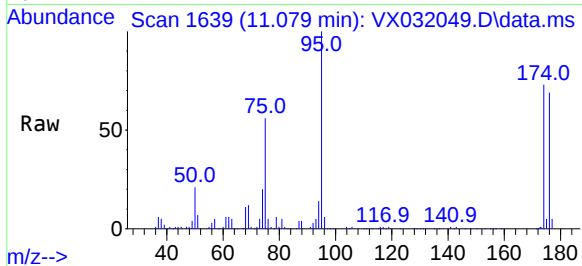

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01

Tgt Ion: 117 Resp: 114975
Ion Ratio Lower Upper
117 100
82 56.7 46.8 70.2
119 32.5 26.4 39.6


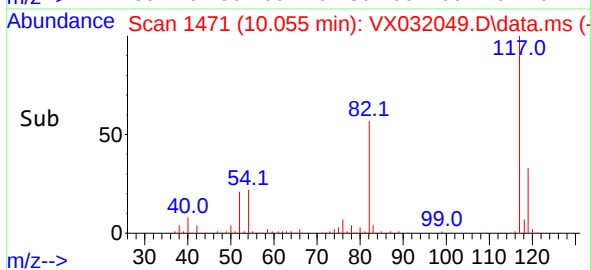
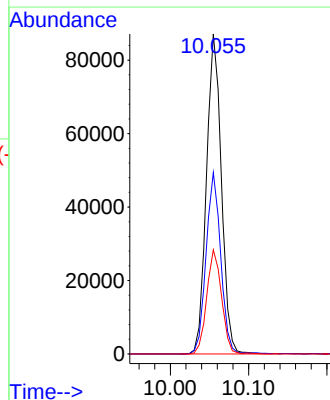
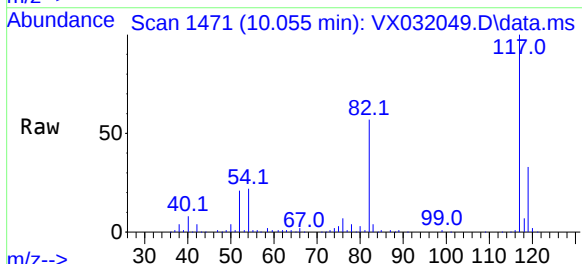




#67
Ethyl Benzene
Concen: 28.720 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01




Instrument :
MSVOA_X
ClientSampleId :
COMP-B-3-VERTEME


Tgt Ion: 91 Resp: 169262
Ion Ratio Lower Upper
91 100
106 31.7 25.2 37.8

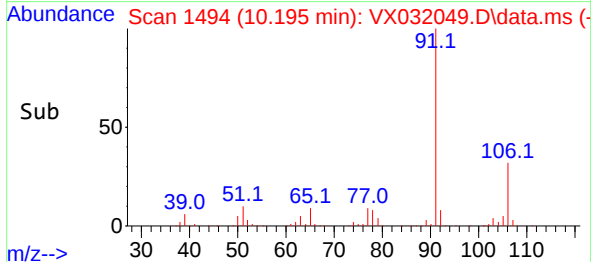

#68
m/p-Xylenes
Concen: 28.728 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.006 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01

Tgt Ion: 106 Resp: 67283
Ion Ratio Lower Upper
106 100
91 205.1 161.0 241.4


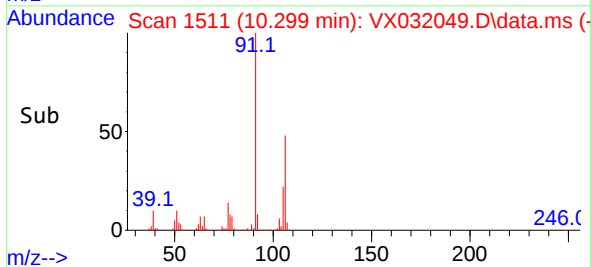

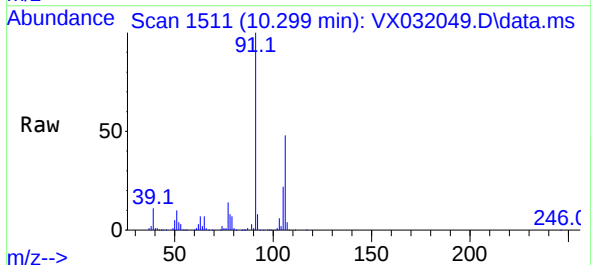




#69
o-Xylene
Concen: 10.961 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. 0.000 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01




Instrument :
MSVOA_X
ClientSampleId :
COMP-B-3-VERTEME


Tgt Ion:106 Resp: 24951
Ion Ratio Lower Upper
106 100
91 216.4 107.2 321.6

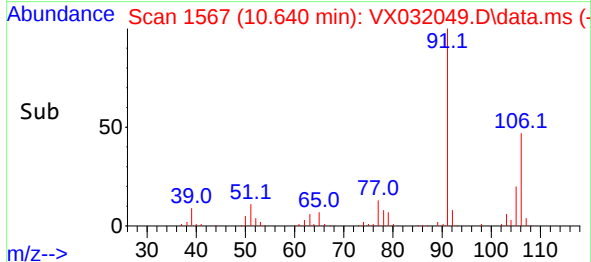

#70
Styrene
Concen: 0.458 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.018 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01


Tgt Ion:104 Resp: 1665
Ion Ratio Lower Upper
104 100
78 241.9 41.4 62.2#
103 209.5 43.8 65.8#

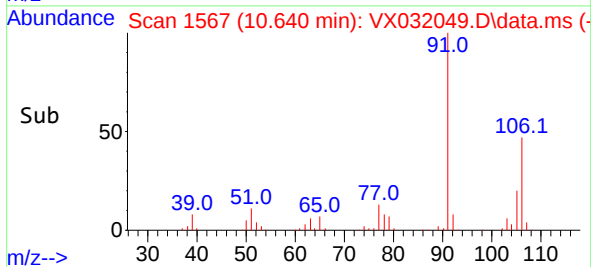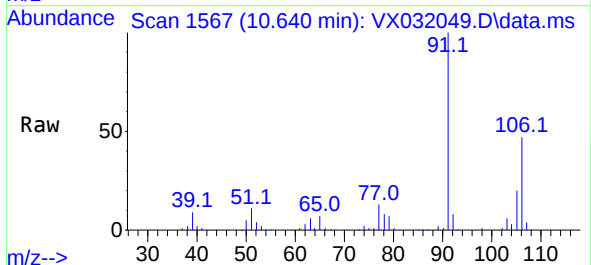






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01


Instrument :
MSVOA_X
ClientSampleId :
COMP-B-3-VERTME

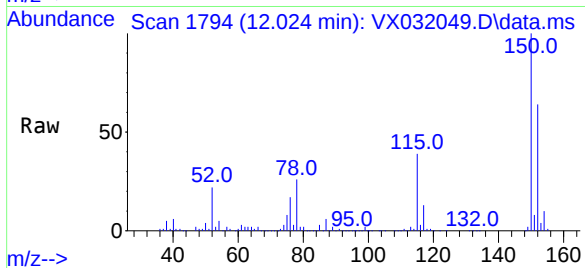



Tgt Ion:152 Resp: 70511
Ion Ratio Lower Upper
152 100
115 60.5 43.4 130.1
150 156.0 0.0 346.8

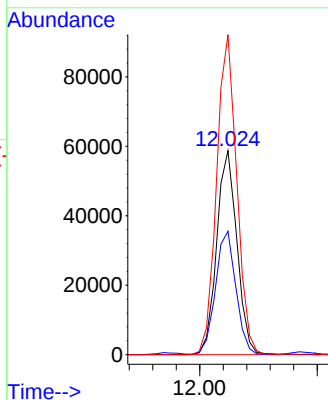


#73
Isopropylbenzene
Concen: 3.312 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01

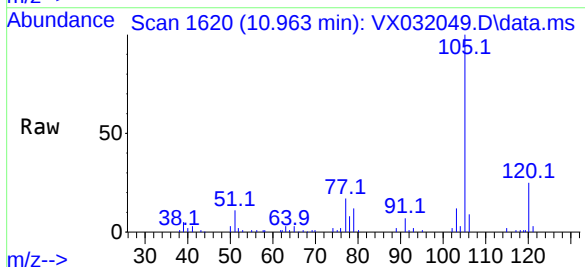

Tgt Ion:105 Resp: 17616
Ion Ratio Lower Upper
105 100
120 25.4 13.7 41.0



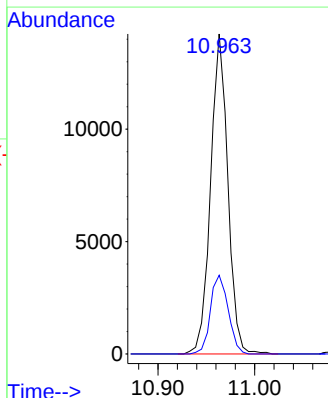





#75
1,1,2,2-Tetrachloroethane
Concen: 0.212 ug/l
RT: 11.219 min Scan# 1662
Delta R.T. 0.006 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01




Instrument :
MSVOA_X
ClientSampleId :
COMP-B-3-VERTME


Tgt Ion: 83 Resp: 359
Ion Ratio Lower Upper
83 100
131 0.0 5.1 15.4#
85 0.0 32.6 97.8#

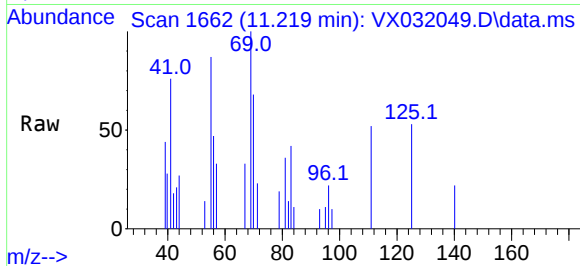

#76
1,2,3-Trichloropropane
Concen: 28.757 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.158 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01

Tgt Ion: 75 Resp: 41558
Ion Ratio Lower Upper
75 100
77 1.3 20.3 60.9#


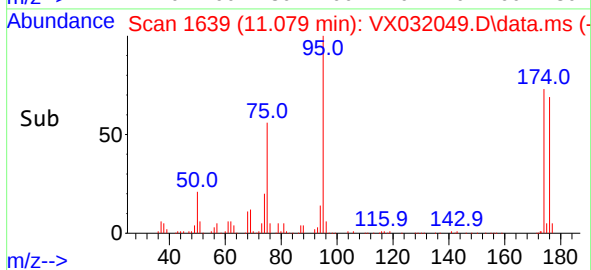

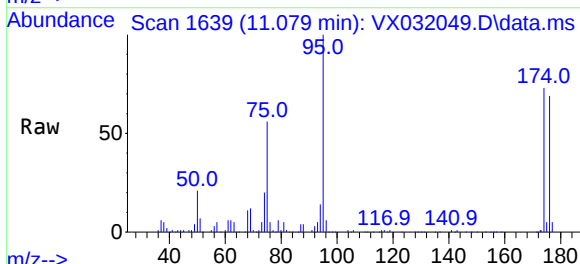




#78
n-propylbenzene
Concen: 1.924 ug/l
RT: 11.305 min Scan# 11638
Delta R.T. -0.000 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01




Instrument :
MSVOA_X
ClientSampleId :
COMP-B-3-VERTME


Tgt Ion: 91 Resp: 11638
Ion Ratio Lower Upper
91 100
120 23.1 11.8 35.4

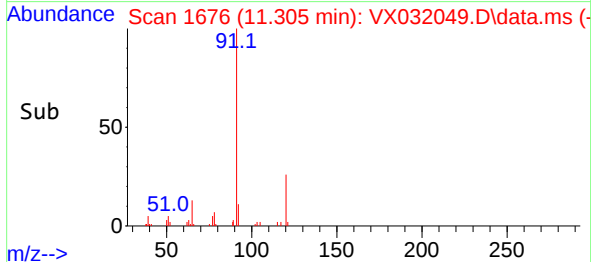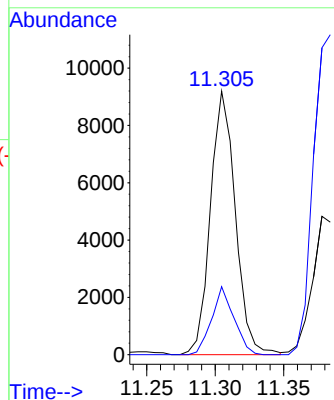

#79
2-Chlorotoluene
Concen: 2.397 ug/l
RT: 11.378 min Scan# 1688
Delta R.T. 0.012 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01

Tgt Ion: 91 Resp: 8726
Ion Ratio Lower Upper
91 100
126 0.2 17.4 52.3#


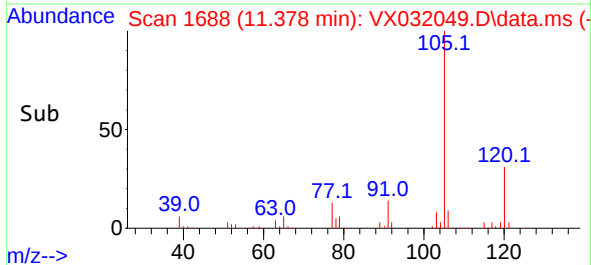
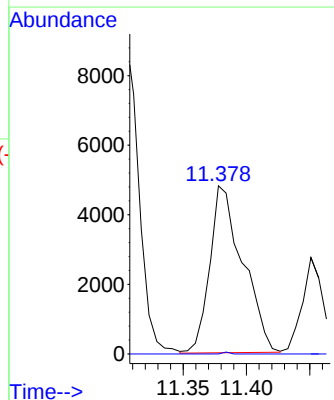
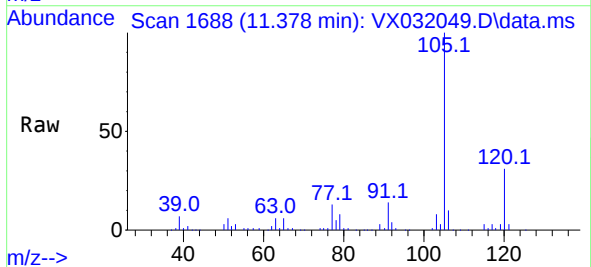




#80
1,3,5-Trimethylbenzene
Concen: 6.124 ug/l
RT: 11.451 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01




Instrument :
MSVOA_X
ClientSampleId :
COMP-B-3-VERTME


Tgt Ion:105 Resp: 27011
Ion Ratio Lower Upper
105 100
120 47.6 24.5 73.5

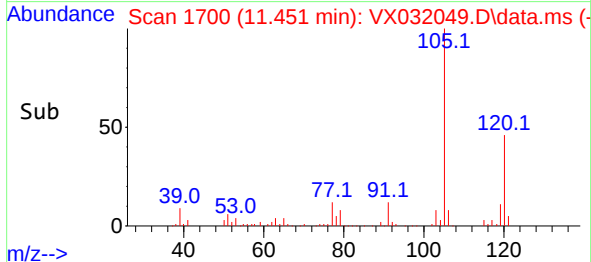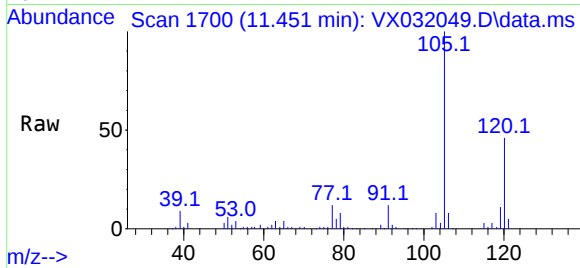

#81
trans-1,4-Dichloro-2-butene
Concen: 98.305 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01

Tgt Ion: 75 Resp: 41558
Ion Ratio Lower Upper
75 100
53 0.1 77.6 116.4#
89 0.1 37.4 56.0#


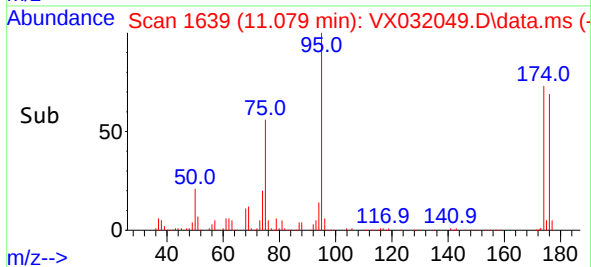

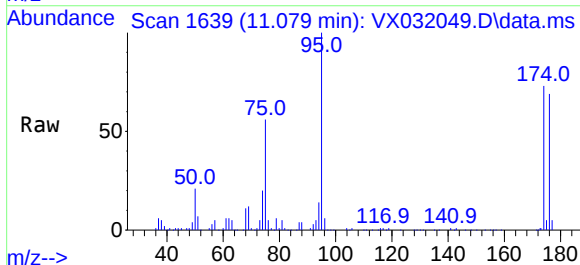




#82
4-Chlorotoluene
Concen: 0.728 ug/l
RT: 11.451 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01




Instrument :
MSVOA_X
ClientSampleId :
COMP-B-3-VERTEME


Tgt Ion: 91 Resp: 3033
Ion Ratio Lower Upper
91 100
126 0.0 15.1 45.3#

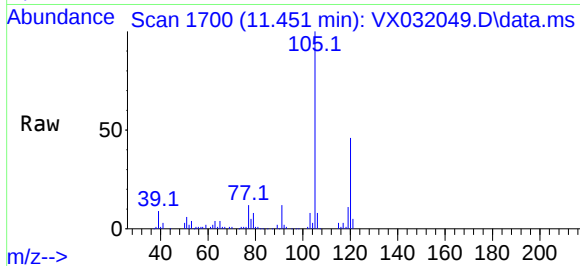

#83
tert-Butylbenzene
Concen: 1.611 ug/l
RT: 11.969 min Scan# 1785
Delta R.T. 0.256 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01

Tgt Ion: 119 Resp: 7031
Ion Ratio Lower Upper
119 100
91 30.3 29.2 87.6
134 29.8 11.6 34.8


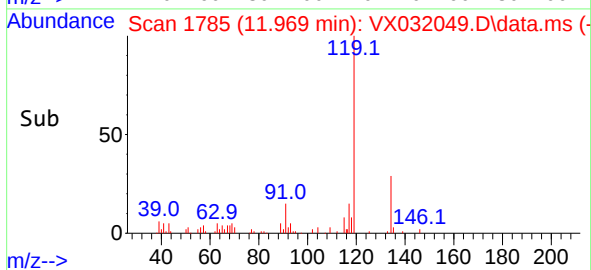

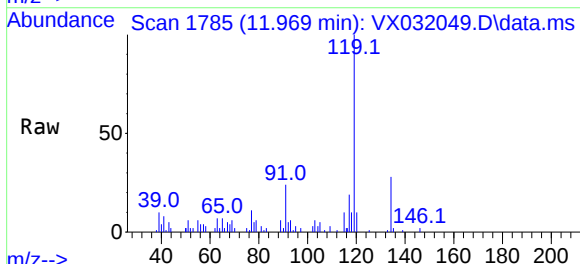




#84
1,2,4-Trimethylbenzene
Concen: 18.106 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01




Instrument :
MSVOA_X
ClientSampleId :
COMP-B-3-VERTEME


Tgt Ion:105 Resp: 81129
Ion Ratio Lower Upper
105 100
120 45.4 22.6 67.8

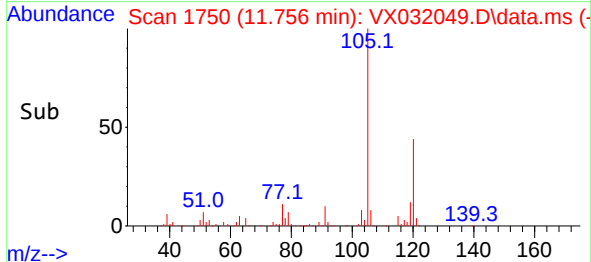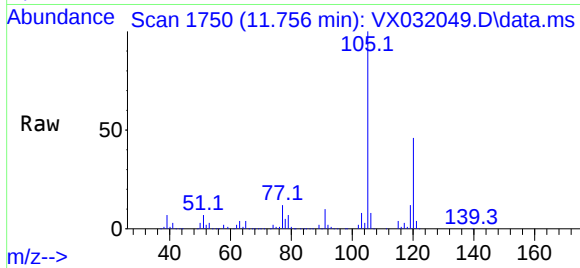

#85
sec-Butylbenzene
Concen: 15.011 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.134 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01

Tgt Ion:105 Resp: 81129
Ion Ratio Lower Upper
105 100
134 0.0 10.4 31.1#


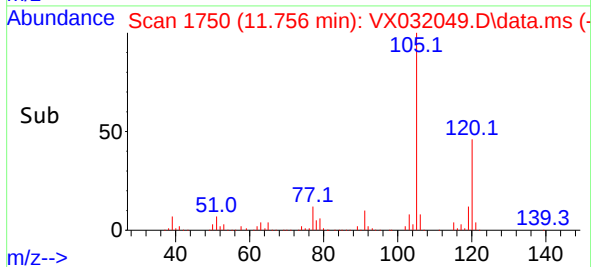

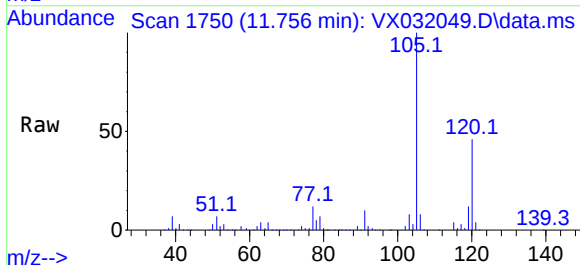




#86
p-Isopropyltoluene
Concen: 1.588 ug/l
RT: 11.969 min Scan# 11
Delta R.T. -0.043 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01




Instrument :
MSVOA_X
ClientSampleId :
COMP-B-3-VERTME


Tgt Ion:119 Resp: 7224
Ion Ratio Lower Upper
119 100
134 29.3 13.4 40.2
91 30.8 12.4 37.2

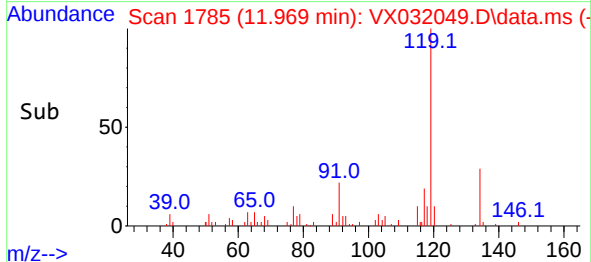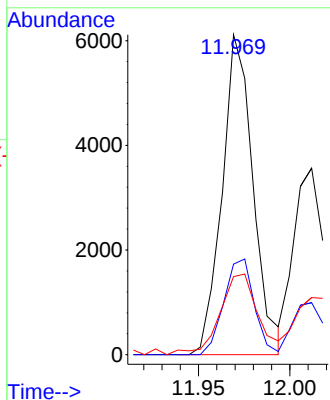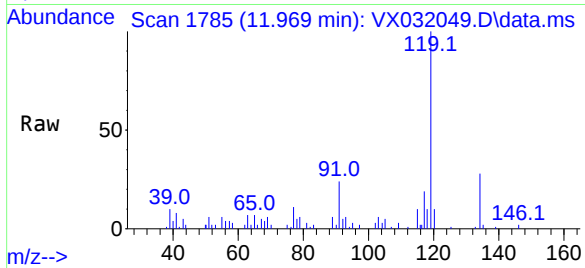

#89
n-Butylbenzene
Concen: 1.023 ug/l
RT: 12.329 min Scan# 1844
Delta R.T. -0.006 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01

Tgt Ion: 91 Resp: 3898
Ion Ratio Lower Upper
91 100
92 33.7 27.0 81.0
134 100.1 13.3 39.9#


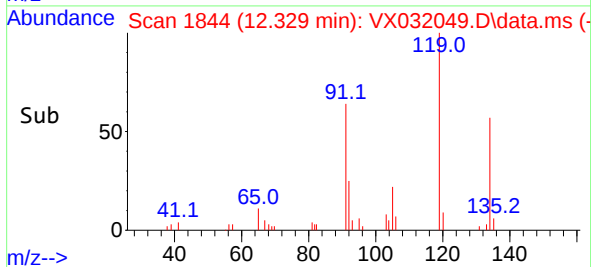
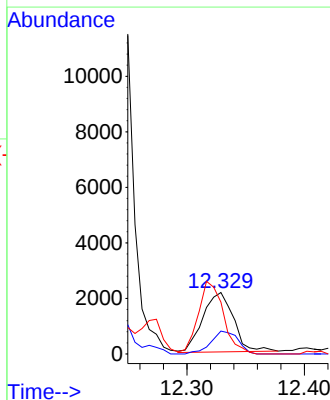
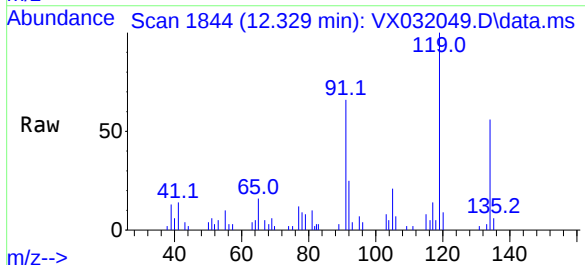




#90
 Hexachloroethane
 Concen: 6.899 ug/l
 RT: 12.414 min Scan# 117
 Delta R.T. -0.128 min
 Lab File: VX032049.D
 Acq: 11 Oct 2022 20:01




Instrument :
 MSVOA_X
 ClientSampleId :
 COMP-B-3-VERTME


Tgt Ion:117 Resp: 4154
 Ion Ratio Lower Upper
 117 100
 201 0.0 34.8 104.4#

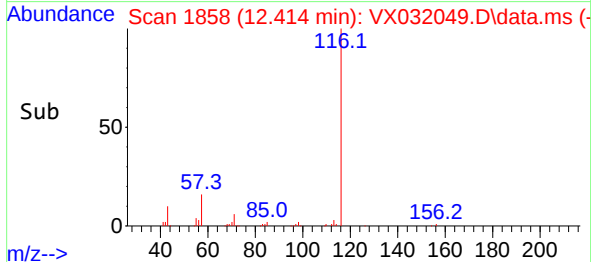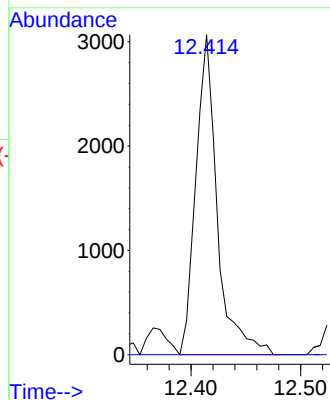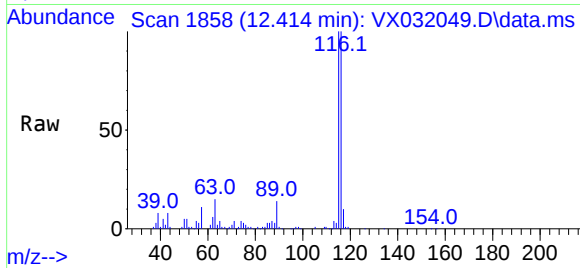

#92
 1,2-Dibromo-3-Chloropropane
 Concen: 0.278 ug/l
 RT: 12.963 min Scan# 1948
 Delta R.T. 0.019 min
 Lab File: VX032049.D
 Acq: 11 Oct 2022 20:01


Tgt Ion: 75 Resp: 86
 Ion Ratio Lower Upper
 75 100
 155 0.0 40.3 120.8#
 157 0.0 51.5 154.5#

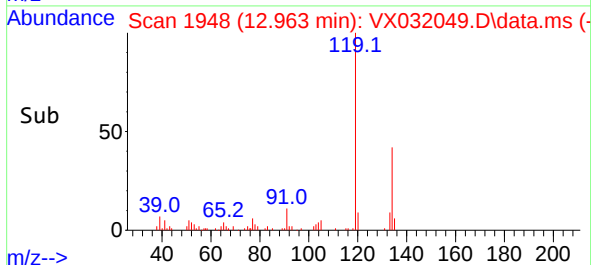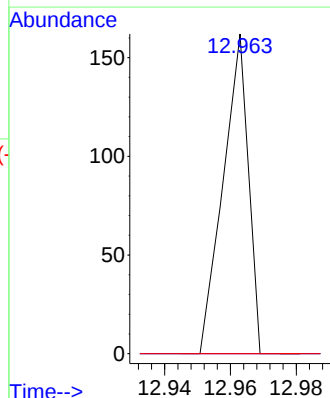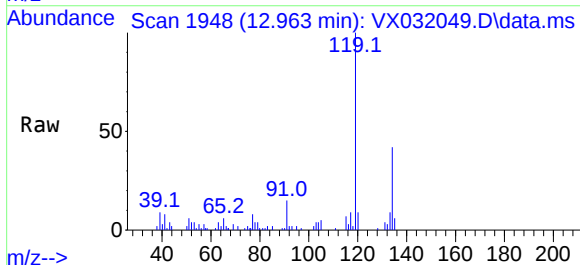



#95
Naphthalene
Concen: 95.029 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.006 min
Lab File: VX032049.D
Acq: 11 Oct 2022 20:01

Instrument :
MSVOA_X
ClientSampleId :
COMP-B-3-VERTME

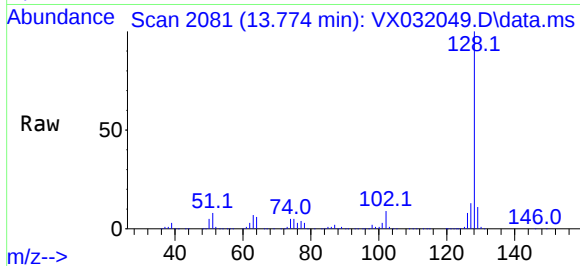

Tgt Ion:128 Resp: 490117
Ion Ratio Lower Upper
128 100
127 12.8 10.4 15.6
129 11.1 8.8 13.2

