

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101122\
 Data File : VX032050.D
 Acq On : 11 Oct 2022 20:24
 Operator : JC/MD
 Sample : N5067-18MEDL 20X
 Misc : 5.05g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMP-B-2-VERTME

Quant Time: Oct 12 05:19:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 06 14:28:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	74541	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	109983	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	117830	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	72771	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	76783	49.878	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	99.760%		
35) Dibromofluoromethane	5.385	113	59136	47.501	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	95.000%		
50) Toluene-d8	8.647	98	224842	50.191	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	100.380%		
62) 4-Bromofluorobenzene	11.079	95	78621	49.643	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	99.280%		
Target Compounds						Qvalue
5) Bromomethane	1.611	94	574	Below Cal	#	64
11) Tert butyl alcohol	2.947	59	3237	16.901	ug/l #	73
16) Acetone	2.392	43	318	0.608	ug/l #	45
20) Methylene Chloride	2.788	84	642	0.467	ug/l #	87
31) Cyclohexane	5.556	56	1924	1.046	ug/l #	7
36) 1,1-Dichloropropene	5.556	75	6220	3.768	ug/l #	49
38) Carbon Tetrachloride	5.556	117	8193	4.854	ug/l #	18
39) Methylcyclohexane	7.379	83	1454	0.738	ug/l	91
40) Benzene	6.044	78	32088	6.638	ug/l	100
43) Isopropyl Acetate	6.610	43	1316	0.558	ug/l #	61
52) Toluene	8.720	92	19036	6.023	ug/l	100
53) t-1,3-Dichloropropene	8.726	75	275	1.364	ug/l #	1
55) 1,1,2-Trichloroethane	9.098	97	450	0.337	ug/l #	15
59) 2-Hexanone	9.384	43	534	0.463	ug/l #	25
67) Ethyl Benzene	10.195	91	171184	28.342	ug/l	98
68) m/p-Xylenes	10.299	106	99689	41.534	ug/l	97
69) o-Xylene	10.640	106	40064	17.173	ug/l	97
70) Styrene	10.646	104	2585	0.693	ug/l #	1
73) Isopropylbenzene	10.963	105	16633	3.030	ug/l	96
76) 1,2,3-Trichloropropane	11.079	75	42340	28.389	ug/l #	37
78) n-propylbenzene	11.305	91	15667	2.510	ug/l	95
79) 2-Chlorotoluene	11.378	91	9689	2.579	ug/l #	40
80) 1,3,5-Trimethylbenzene	11.451	105	37870	8.319	ug/l	97
81) trans-1,4-Dichloro-2-b...	11.079	75	42340	97.090	ug/l #	11
82) 4-Chlorotoluene	11.616	91	2140	0.497	ug/l	75
83) tert-Butylbenzene	11.756	119	13887	3.082	ug/l #	54
84) 1,2,4-Trimethylbenzene	11.750	105	111368	24.083	ug/l	100
85) sec-Butylbenzene	11.750	105	111368	19.966	ug/l #	56
86) p-Isopropyltoluene	11.969	119	7260	1.546	ug/l	96
89) n-Butylbenzene	12.329	91	5264	1.339	ug/l #	30
90) Hexachloroethane	12.701	117	4278	6.887	ug/l #	15
92) 1,2-Dibromo-3-Chloropr...	12.969	75	144	0.451	ug/l #	3
95) Naphthalene	13.774	128	780521	146.635	ug/l	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :

MSVOA_X


ClientSampleId :


COMP-B-2-VERTME

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101122\
Data File : VX032050.D
Acq On : 11 Oct 2022 20:24
Operator : JC/MD
Sample : N5067-18MEDL 20X
Misc : 5.05g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP-B-2-VERTME


Quant Time: Oct 12 05:19:33 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 06 14:28:46 2022
Response via : Initial Calibration

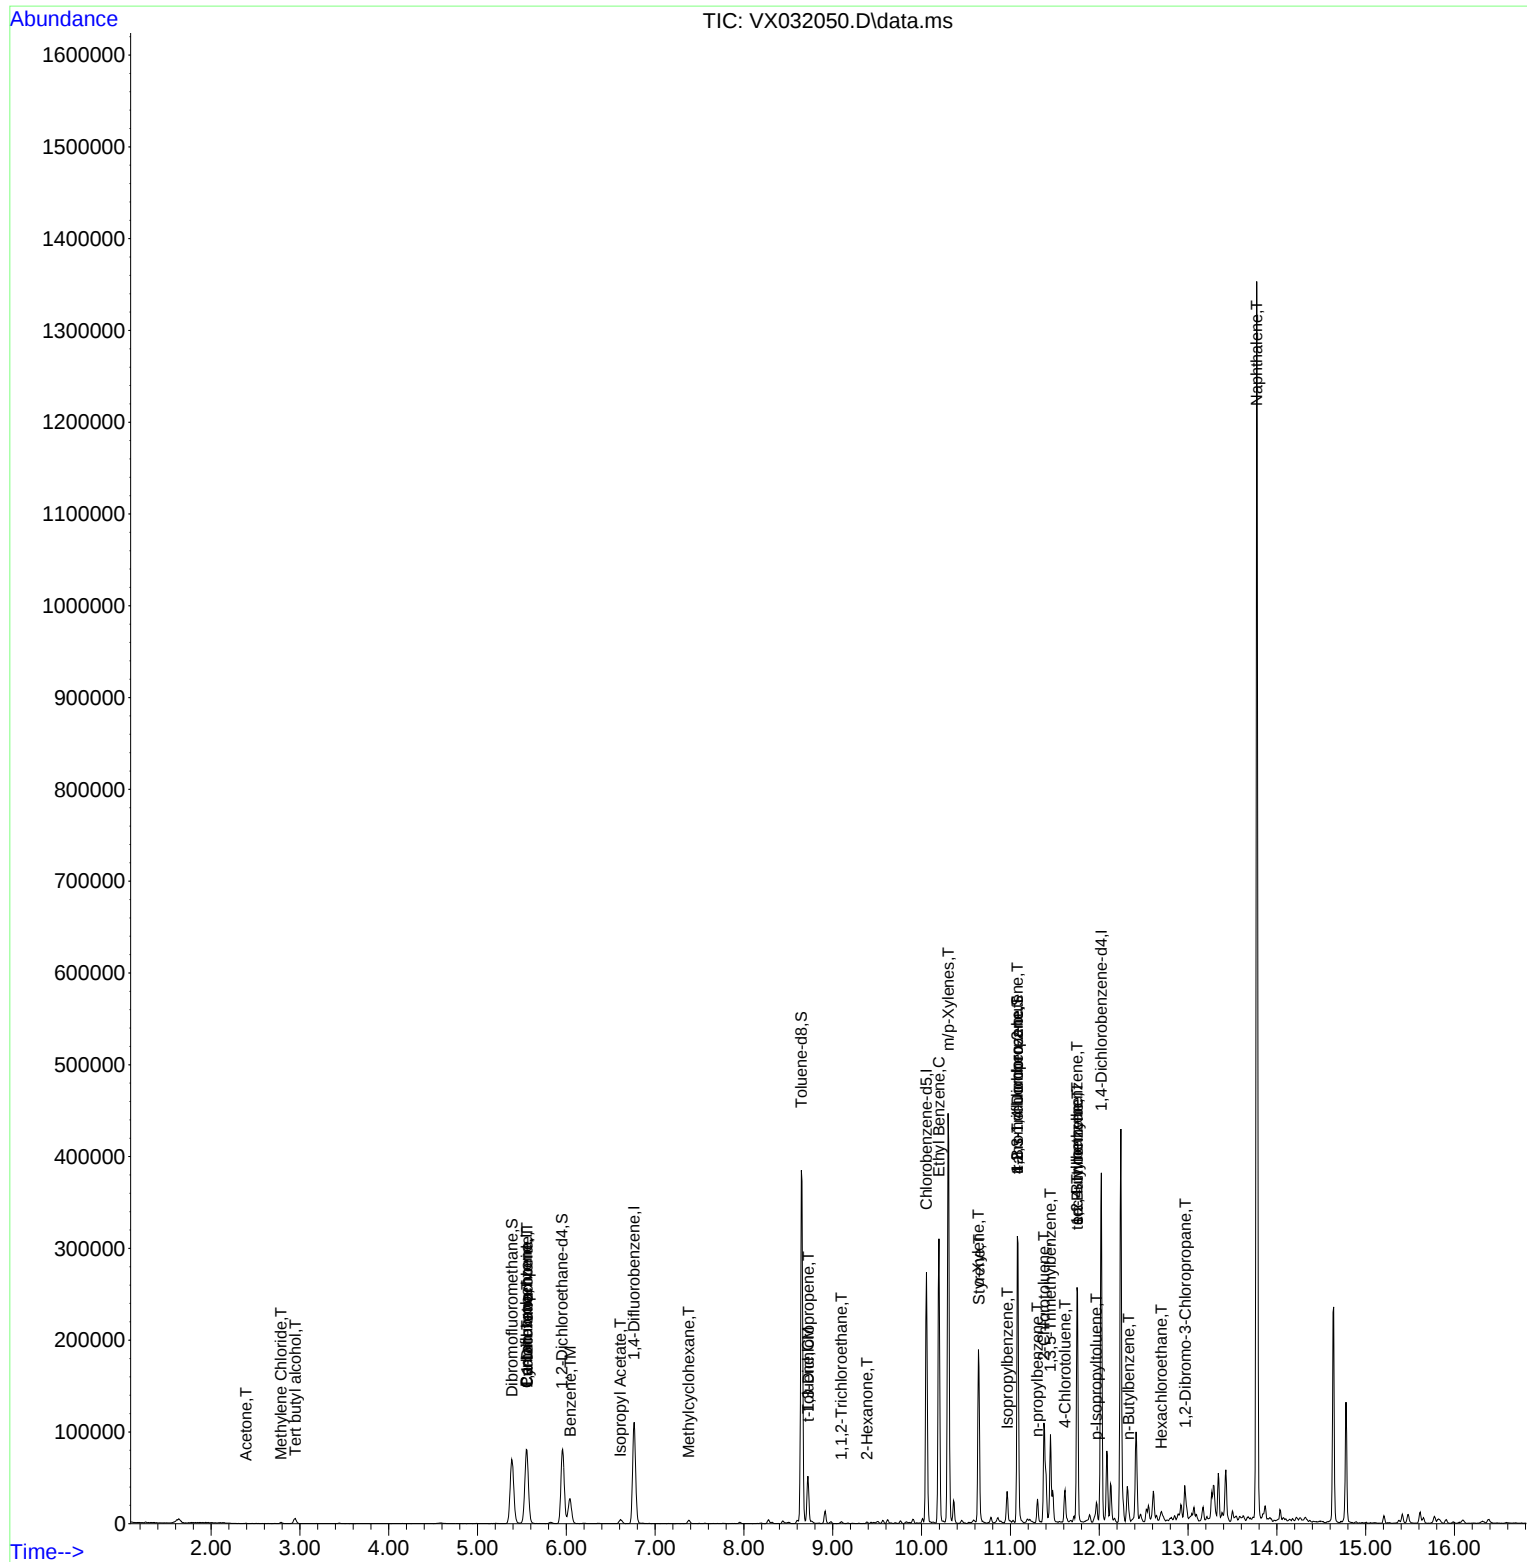



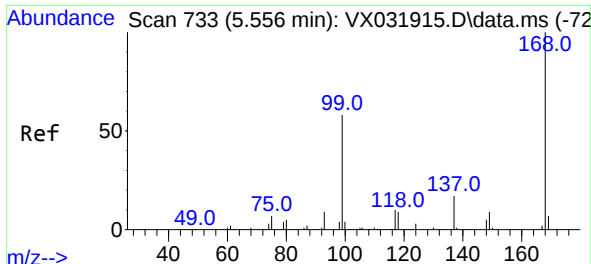


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX032050.D
Acq: 11 Oct 2022 20:24

Instrument :
MSVOA_X
ClientSampleId :
COMP-B-2-VERTEME







Tgt Ion:168 Resp: 74541
Ion Ratio Lower Upper
168 100
99 61.2 48.8 73.2

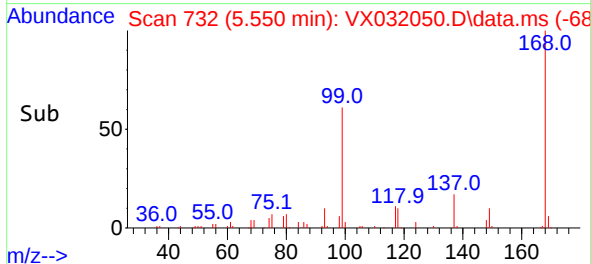

#5
Bromomethane
Concen: Below Cal
RT: 1.611 min Scan# 86
Delta R.T. 0.000 min
Lab File: VX032050.D
Acq: 11 Oct 2022 20:24

Tgt Ion: 94 Resp: 574
Ion Ratio Lower Upper
94 100
96 58.1 74.4 111.6#

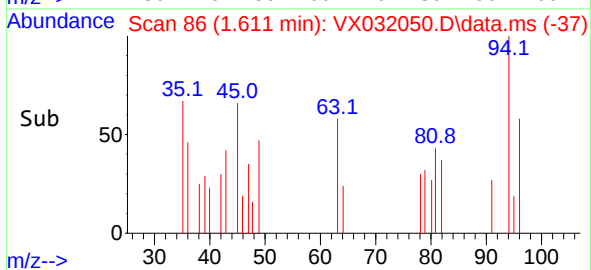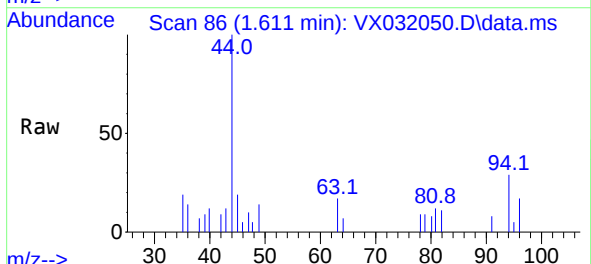



#11

Tert butyl alcohol

Concen: 16.901 ug/l

RT: 2.947 min Scan# 305

Delta R.T. -0.060 min

Lab File: VX032050.D

Acq: 11 Oct 2022 20:24

Instrument :

MSVOA_X

ClientSampleId :





COMP-B-2-VERTME

Tgt Ion: 59 Resp: 3237

Ion Ratio Lower Upper

59 100

57 0.0 8.2 12.2#

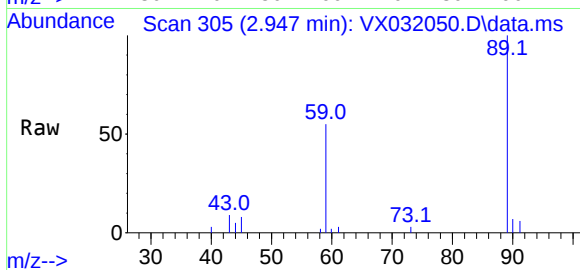

#16

Acetone

Concen: 0.608 ug/l

RT: 2.392 min Scan# 214

Delta R.T. -0.000 min

Lab File: VX032050.D




Acq: 11 Oct 2022 20:24


Tgt Ion: 43 Resp: 318

Ion Ratio Lower Upper

43 100

58 0.0 23.8 35.8#

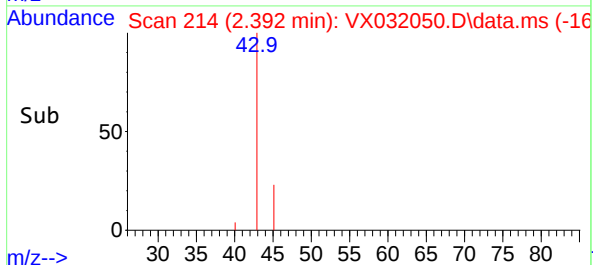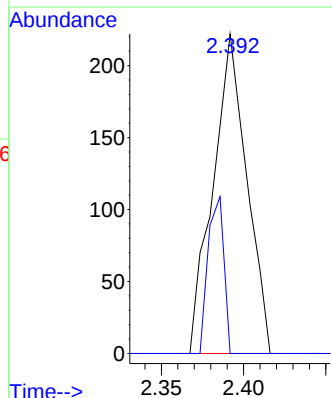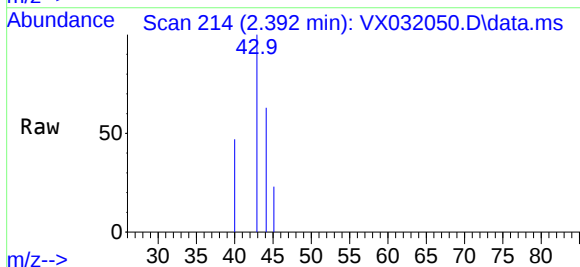



#20

Methylene Chloride

Concen: 0.467 ug/l

RT: 2.788 min Scan# 21

Delta R.T. 0.000 min

Lab File: VX032050.D

Acq: 11 Oct 2022 20:24

Instrument :

MSVOA_X

ClientSampleId :

COMP-B-2-VERTEME

Tgt Ion: 84 Resp: 642


Ion Ratio Lower Upper

84 100




49 119.4 105.9 158.9

51 16.7 32.2 48.2#

86 61.4 50.8 76.2

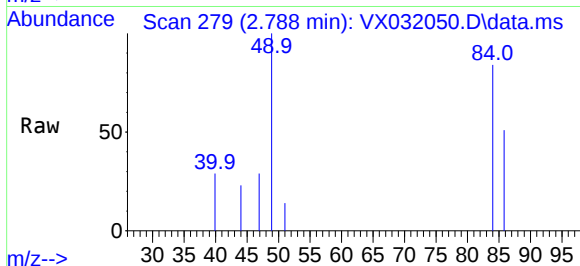

Abundance

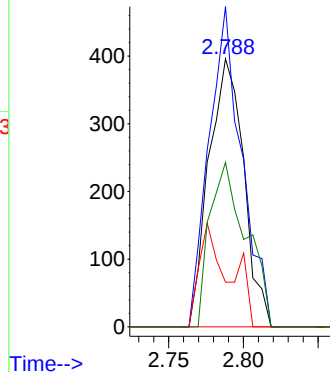

#31

Cyclohexane

Concen: 1.046 ug/l

RT: 5.556 min Scan# 733

Delta R.T. 0.086 min

Lab File: VX032050.D

Acq: 11 Oct 2022 20:24


Tgt Ion: 56 Resp: 1924

Ion Ratio Lower Upper



56 100


69 165.6 25.1 37.7#

84 124.4 70.2 105.4#

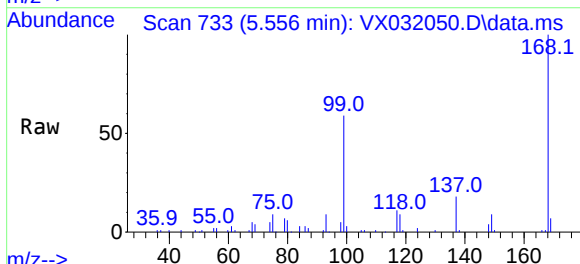

Abundance

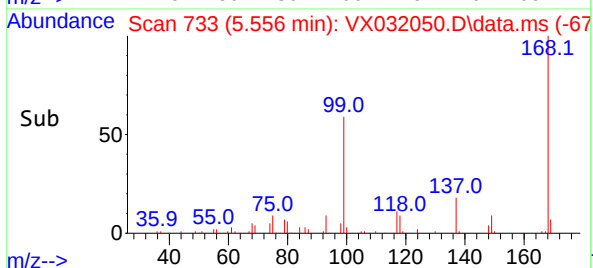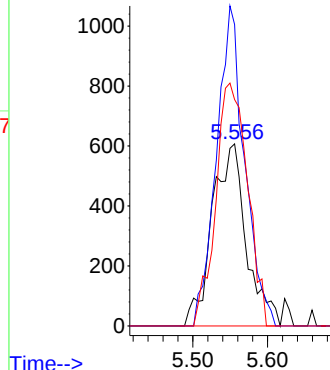



#33

1,2-Dichloroethane-d4

Concen: 49.878 ug/l

RT: 5.952 min Scan# 799

Delta R.T. -0.006 min

Lab File: VX032050.D

Acq: 11 Oct 2022 20:24

Instrument :

MSVOA_X

ClientSampleId :





COMP-B-2-VERTME

Tgt Ion: 65 Resp: 76783

Ion Ratio Lower Upper

65 100

67 51.3 0.0 102.4

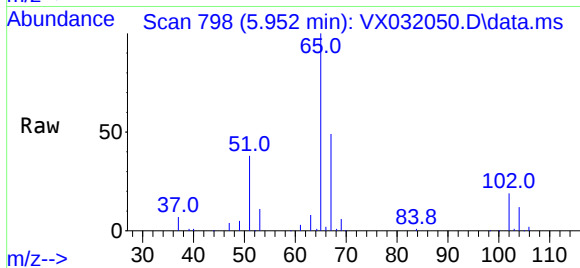

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.000 min

Lab File: VX032050.D

Acq: 11 Oct 2022 20:24




Tgt Ion: 114 Resp: 109983


Ion Ratio Lower Upper

114 100

63 21.0 0.0 42.6


88 16.8 0.0 33.0

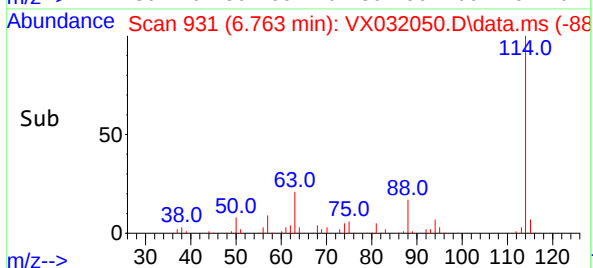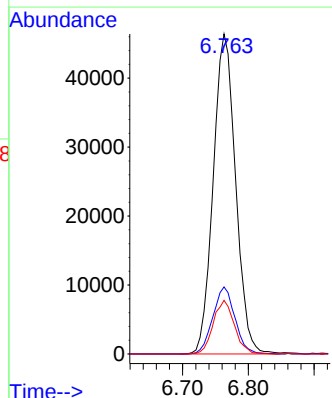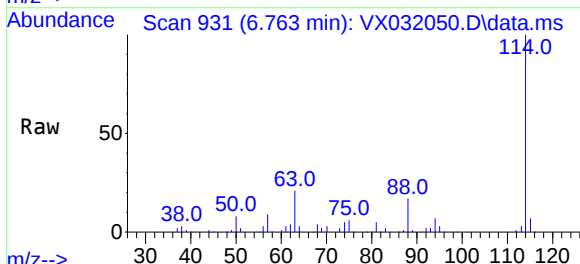



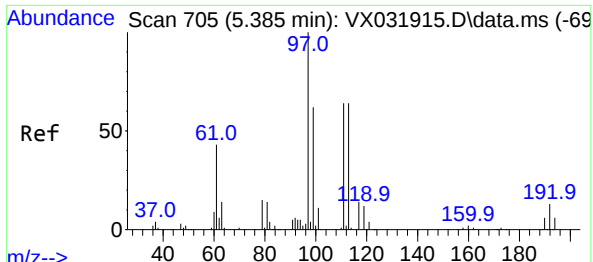


#35
Dibromofluoromethane
Concen: 47.501 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX032050.D
Acq: 11 Oct 2022 20:24


Instrument :
MSVOA_X
ClientSampleId :
COMP-B-2-VERTEME

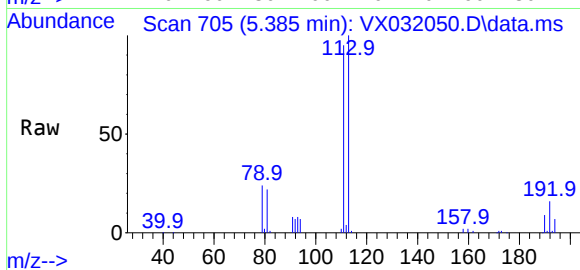



Tgt Ion:113 Resp: 59136
Ion Ratio Lower Upper
113 100
111 104.2 82.4 123.6
192 17.9 14.1 21.1




#36
1,1-Dichloropropene
Concen: 3.768 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.134 min
Lab File: VX032050.D
Acq: 11 Oct 2022 20:24

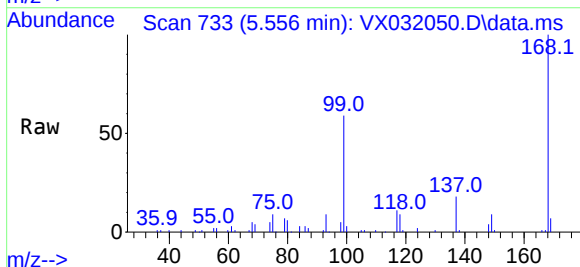


Tgt Ion: 75 Resp: 6220
Ion Ratio Lower Upper
75 100
110 8.4 17.5 52.5#
77 0.0 24.9 37.3#

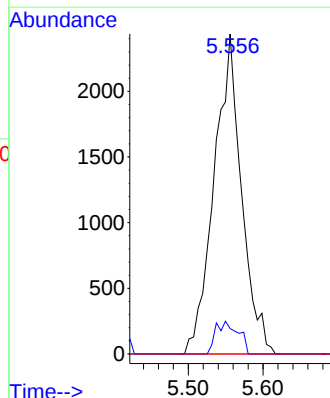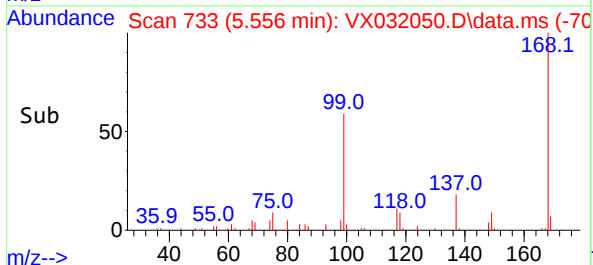






#38
Carbon Tetrachloride
Concen: 4.854 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.121 min
Lab File: VX032050.D
Acq: 11 Oct 2022 20:24

Instrument :
MSVOA_X
ClientSampleId :
COMP-B-2-VERTME



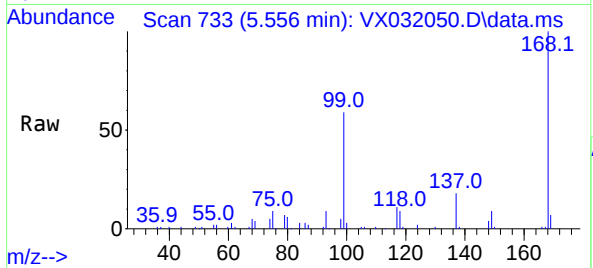



Tgt Ion:117 Resp: 8193
Ion Ratio Lower Upper
117 100
119 5.7 74.6 112.0#
121 0.0 25.3 37.9#

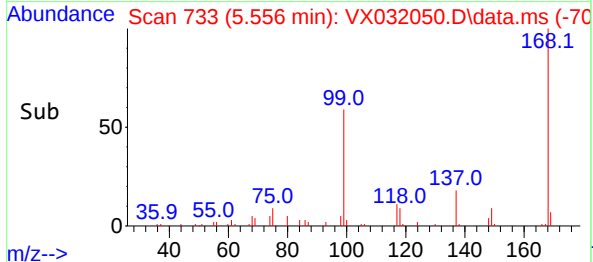

#39
Methylcyclohexane
Concen: 0.738 ug/l
RT: 7.379 min Scan# 1032
Delta R.T. -0.006 min
Lab File: VX032050.D
Acq: 11 Oct 2022 20:24

Tgt Ion: 83 Resp: 1454
Ion Ratio Lower Upper
83 100
55 83.2 61.0 91.4
98 53.7 37.7 56.5


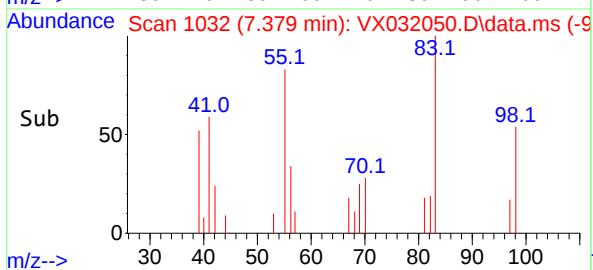






#40
Benzene
Concen: 6.638 ug/l
RT: 6.044 min Scan# 812
Delta R.T. 0.007 min
Lab File: VX032050.D
Acq: 11 Oct 2022 20:24




Instrument :
MSVOA_X
ClientSampleId :
COMP-B-2-VERTME


Tgt Ion: 78 Resp: 32088
Ion Ratio Lower Upper
78 100
77 23.3 18.7 28.1

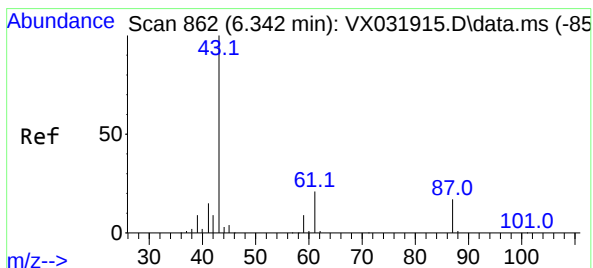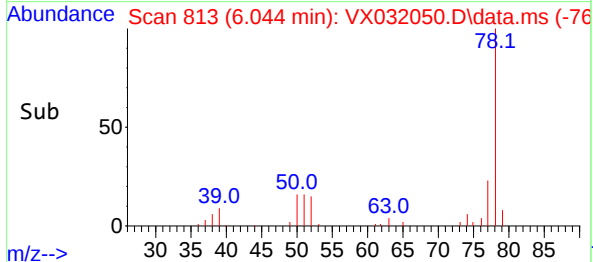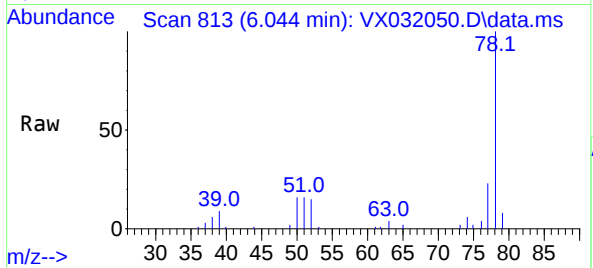

#43
Isopropyl Acetate
Concen: 0.558 ug/l
RT: 6.610 min Scan# 906
Delta R.T. 0.268 min
Lab File: VX032050.D
Acq: 11 Oct 2022 20:24

Tgt Ion: 43 Resp: 1316
Ion Ratio Lower Upper
43 100
61 0.0 15.3 22.9#
87 0.0 10.6 15.8#

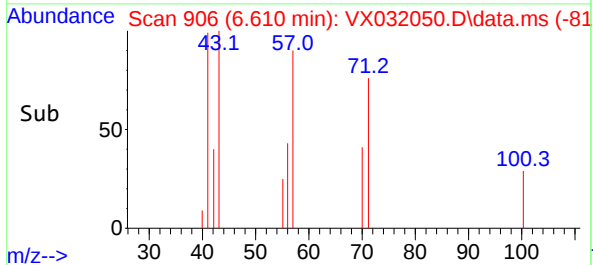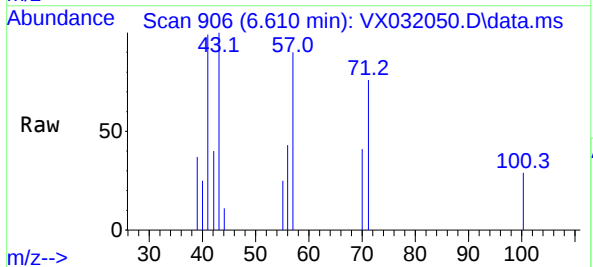



#50

Toluene-d8

Concen: 50.191 ug/l

RT: 8.647 min Scan# 11

Delta R.T. -0.006 min

Lab File: VX032050.D

Acq: 11 Oct 2022 20:24

Instrument :

MSVOA_X

ClientSampleId :





COMP-B-2-VERTME

Tgt Ion: 98 Resp: 224842

Ion Ratio Lower Upper

98 100

100 65.4 52.5 78.7

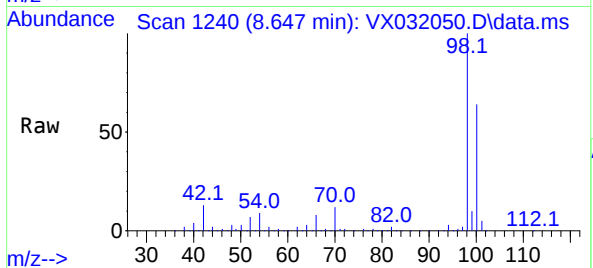

#52

Toluene

Concen: 6.023 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. -0.000 min

Lab File: VX032050.D




Acq: 11 Oct 2022 20:24


Tgt Ion: 92 Resp: 19036

Ion Ratio Lower Upper

92 100

91 171.7 137.1 205.7

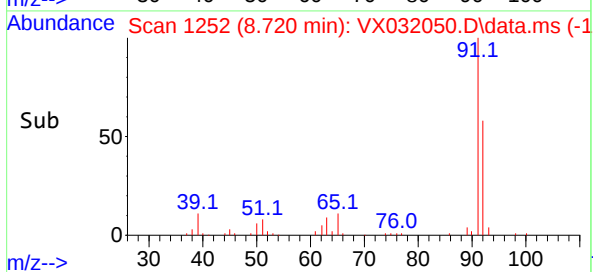



#53

t-1,3-Dichloropropene

Concen: 1.364 ug/l

RT: 8.726 min Scan# 11

Delta R.T. -0.256 min

Lab File: VX032050.D

Acq: 11 Oct 2022 20:24

Instrument :

MSVOA_X

ClientSampleId :





COMP-B-2-VERTME

Tgt Ion: 75 Resp: 275

Ion Ratio Lower Upper

75 100

77 88.5 24.8 37.2#

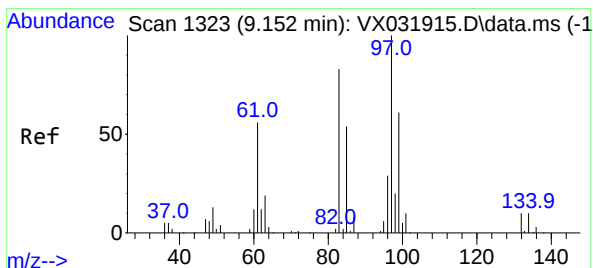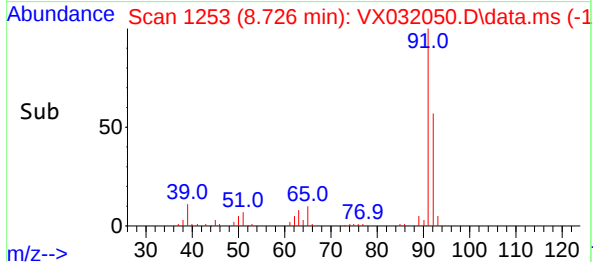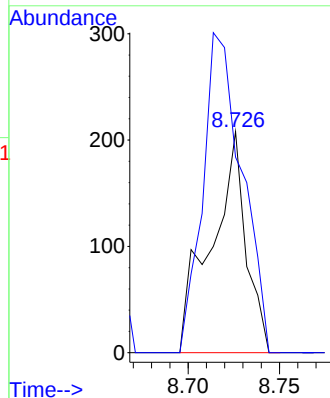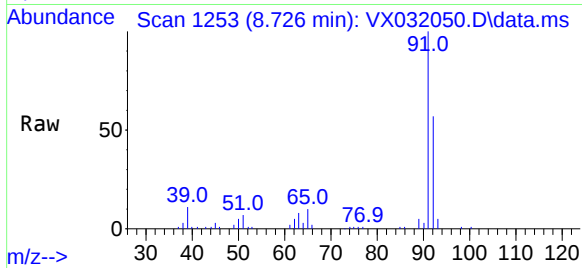

#55

1,1,2-Trichloroethane

Concen: 0.337 ug/l

RT: 9.098 min Scan# 1314

Delta R.T. -0.054 min

Lab File: VX032050.D

Acq: 11 Oct 2022 20:24

Tgt Ion: 97 Resp: 450




Ion Ratio Lower Upper


97 100

83 0.0 69.0 103.6#

85 0.0 44.1 66.1#

99 0.0 51.3 76.9#


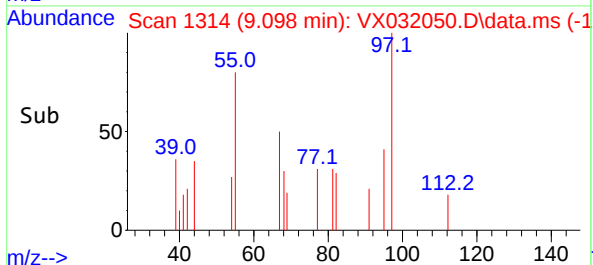
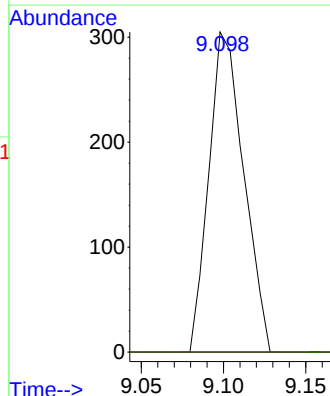
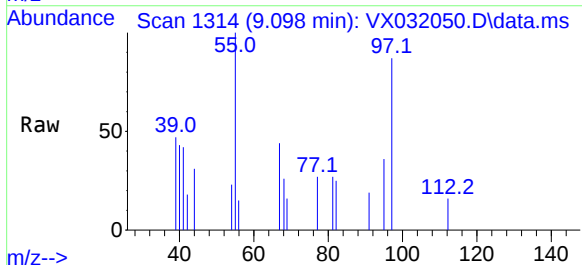




#59
2-Hexanone
Concen: 0.463 ug/l
RT: 9.384 min Scan# 1361
Delta R.T. -0.049 min
Lab File: VX032050.D
Acq: 11 Oct 2022 20:24




Instrument :
MSVOA_X
ClientSampleId :
COMP-B-2-VERTEME


Tgt Ion: 43 Resp: 534
Ion Ratio Lower Upper
43 100
58 0.0 26.7 80.0#

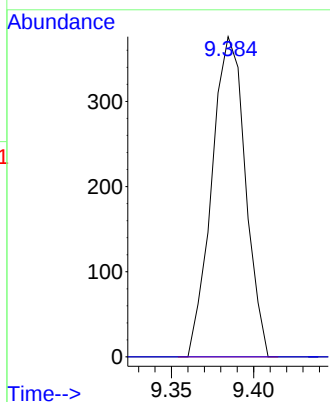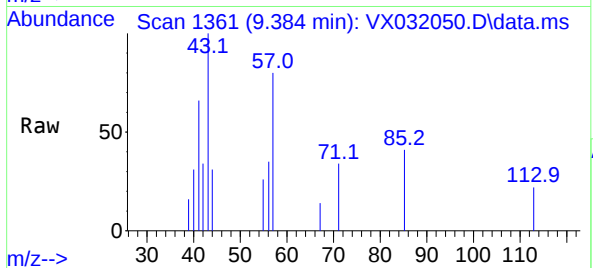

#62
4-Bromofluorobenzene
Concen: 49.643 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX032050.D
Acq: 11 Oct 2022 20:24

Tgt Ion: 95 Resp: 78621
Ion Ratio Lower Upper
95 100
174 77.4 0.0 153.2
176 75.4 0.0 144.0


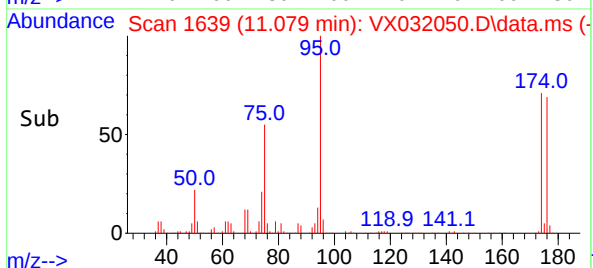






#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX032050.D
Acq: 11 Oct 2022 20:24




Instrument :
MSVOA_X
ClientSampleId :
COMP-B-2-VERTME


Tgt Ion:117 Resp: 117830
Ion Ratio Lower Upper
117 100
82 55.2 46.8 70.2
119 32.1 26.4 39.6

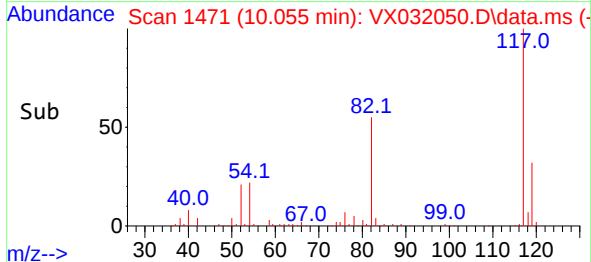

#67
Ethyl Benzene
Concen: 28.342 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX032050.D
Acq: 11 Oct 2022 20:24

Tgt Ion: 91 Resp: 171184
Ion Ratio Lower Upper
91 100
106 30.6 25.2 37.8


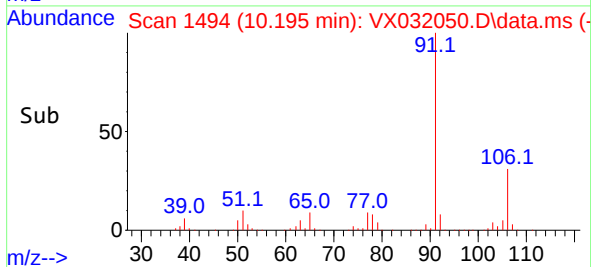

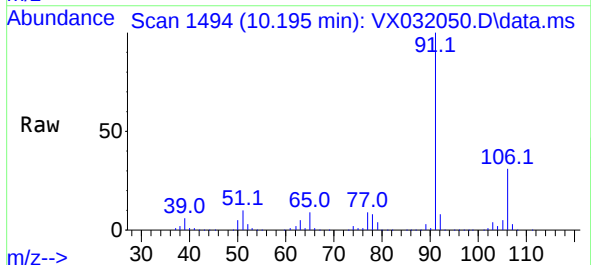




#68
m/p-Xylenes
Concen: 41.534 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.006 min
Lab File: VX032050.D
Acq: 11 Oct 2022 20:24




Instrument :
MSVOA_X
ClientSampleId :
COMP-B-2-VERTEME


Tgt Ion:106 Resp: 99689
Ion Ratio Lower Upper
106 100
91 206.1 161.0 241.4

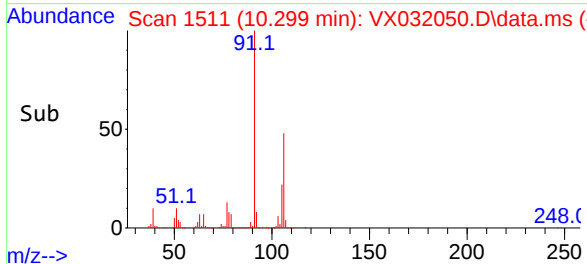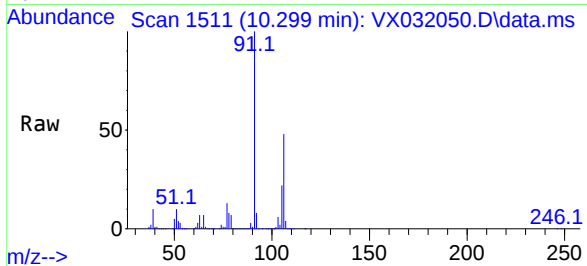

#69
o-Xylene
Concen: 17.173 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. 0.000 min
Lab File: VX032050.D
Acq: 11 Oct 2022 20:24

Tgt Ion:106 Resp: 40064
Ion Ratio Lower Upper
106 100
91 218.7 107.2 321.6


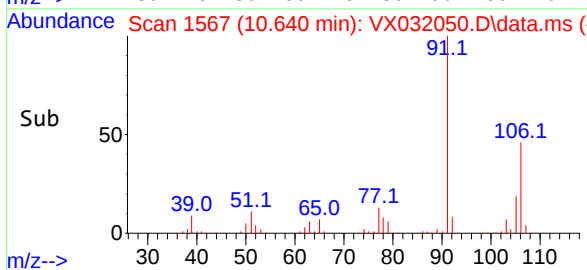

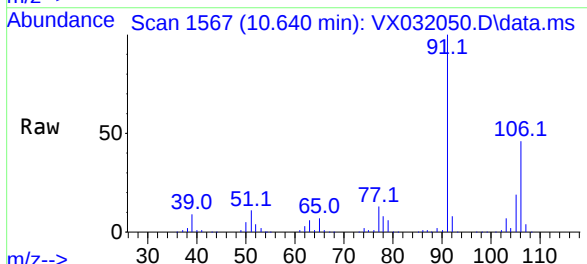




#70
Styrene
Concen: 0.693 ug/l
RT: 10.646 min Scan# 11
Delta R.T. -0.012 min
Lab File: VX032050.D
Acq: 11 Oct 2022 20:24




Instrument :
MSVOA_X
ClientSampleId :
COMP-B-2-VERTME


Tgt Ion:104 Resp: 2585
Ion Ratio Lower Upper
104 100
78 267.9 41.4 62.2#
103 236.4 43.8 65.8#

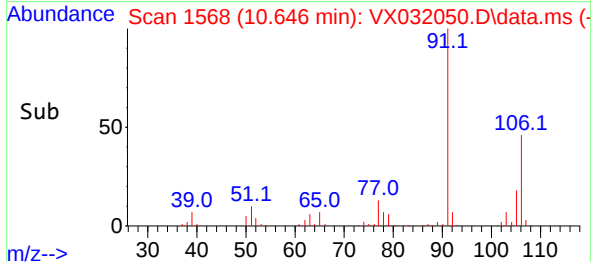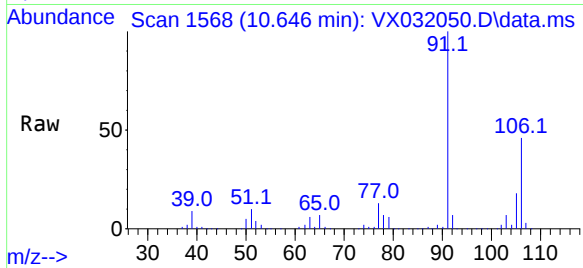

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX032050.D
Acq: 11 Oct 2022 20:24

Tgt Ion:152 Resp: 72771
Ion Ratio Lower Upper
152 100
115 61.8 43.4 130.1
150 156.3 0.0 346.8


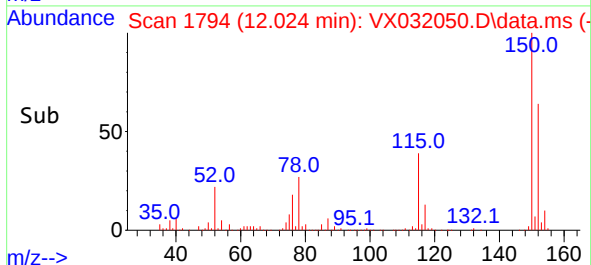
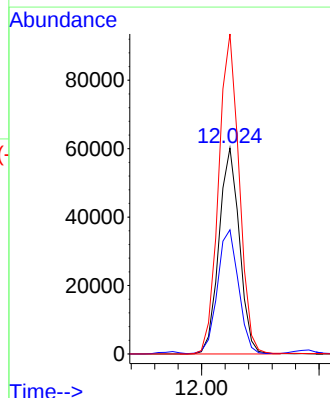
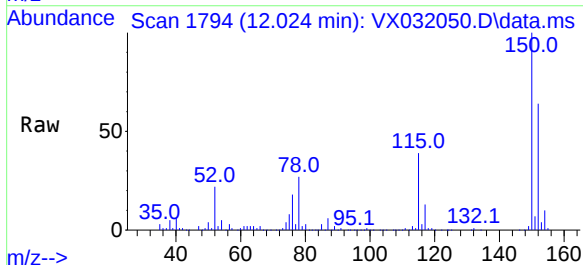




#73
Isopropylbenzene
Concen: 3.030 ug/l
RT: 10.963 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX032050.D
Acq: 11 Oct 2022 20:24




Instrument :
MSVOA_X
ClientSampleId :
COMP-B-2-VERTME


Tgt Ion:105 Resp: 16633
Ion Ratio Lower Upper
105 100
120 25.1 13.7 41.0

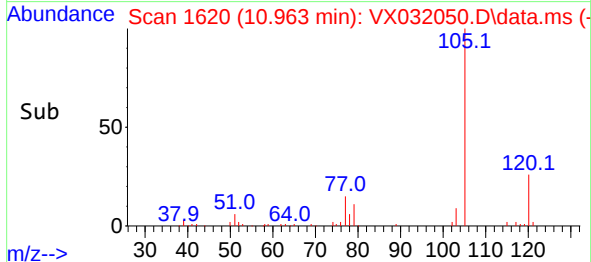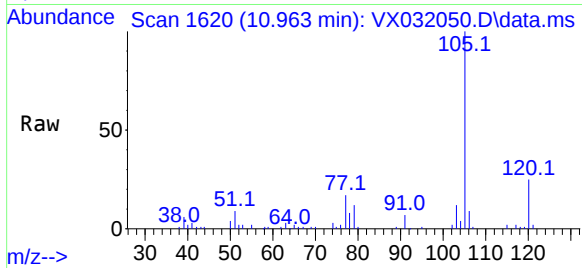

#76
1,2,3-Trichloropropane
Concen: 28.389 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.158 min
Lab File: VX032050.D
Acq: 11 Oct 2022 20:24

Tgt Ion: 75 Resp: 42340
Ion Ratio Lower Upper
75 100
77 1.5 20.3 60.9#


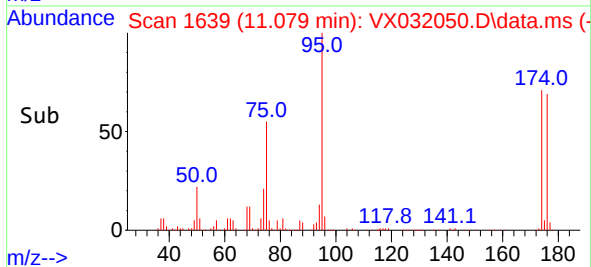

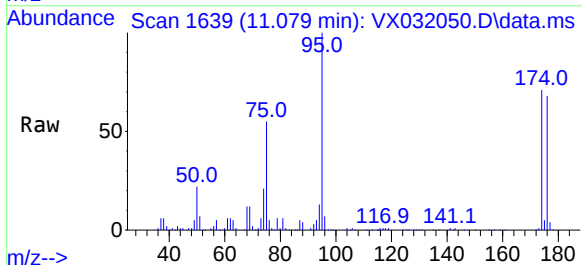




#78
n-propylbenzene
Concen: 2.510 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX032050.D
Acq: 11 Oct 2022 20:24




Instrument :
MSVOA_X
ClientSampleId :
COMP-B-2-VERTME


Tgt Ion: 91 Resp: 15667
Ion Ratio Lower Upper
91 100
120 21.3 11.8 35.4

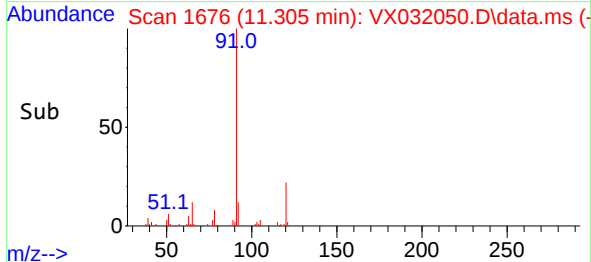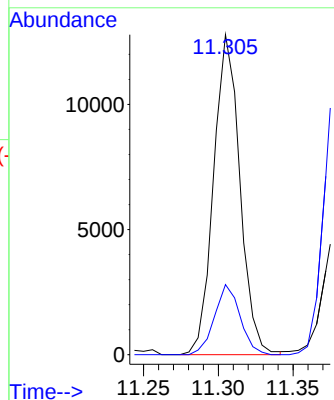

#79
2-Chlorotoluene
Concen: 2.579 ug/l
RT: 11.378 min Scan# 1688
Delta R.T. 0.012 min
Lab File: VX032050.D
Acq: 11 Oct 2022 20:24

Tgt Ion: 91 Resp: 9689
Ion Ratio Lower Upper
91 100
126 0.0 17.4 52.3#


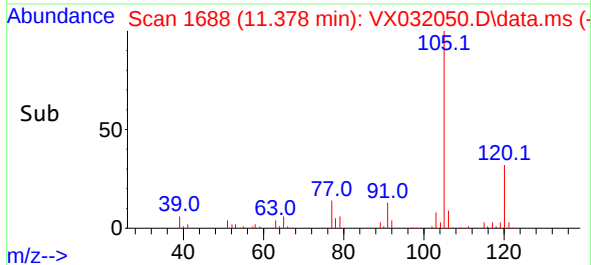
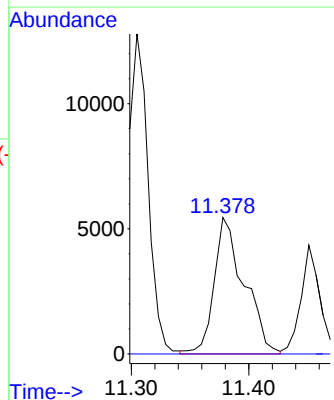
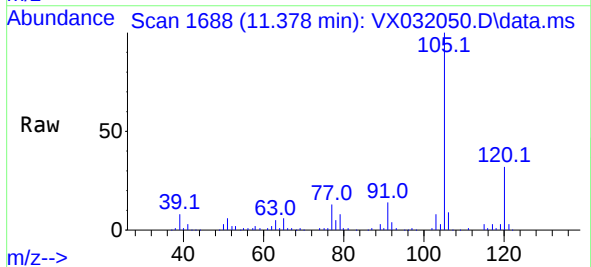


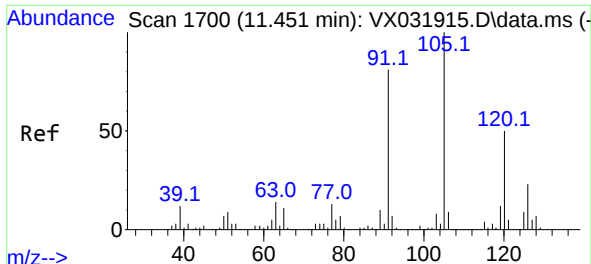

#80
1,3,5-Trimethylbenzene
Concen: 8.319 ug/l
RT: 11.451 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX032050.D
Acq: 11 Oct 2022 20:24




Instrument :
MSVOA_X
ClientSampleId :
COMP-B-2-VERTME


Tgt Ion:105 Resp: 37870
Ion Ratio Lower Upper
105 100
120 46.8 24.5 73.5

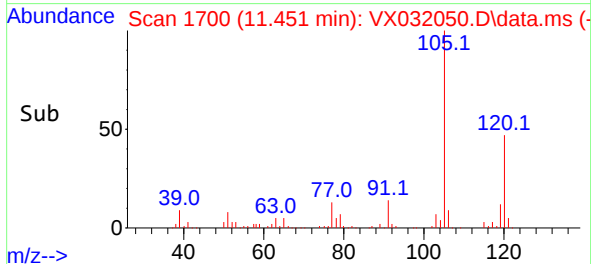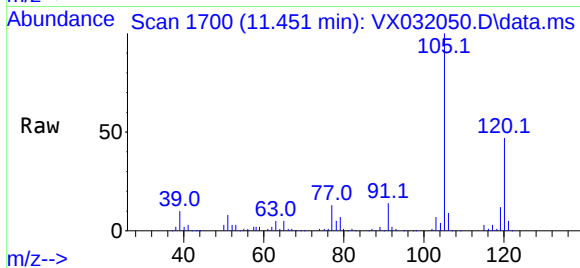

#81
trans-1,4-Dichloro-2-butene
Concen: 97.090 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX032050.D
Acq: 11 Oct 2022 20:24

Tgt Ion: 75 Resp: 42340
Ion Ratio Lower Upper
75 100
53 0.2 77.6 116.4#
89 0.0 37.4 56.0#


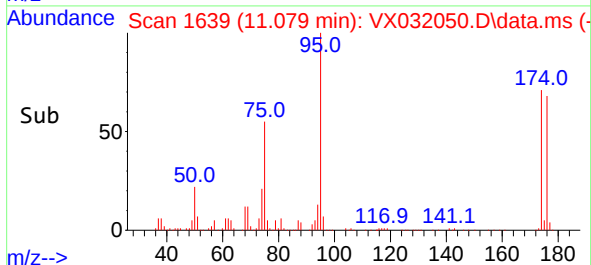
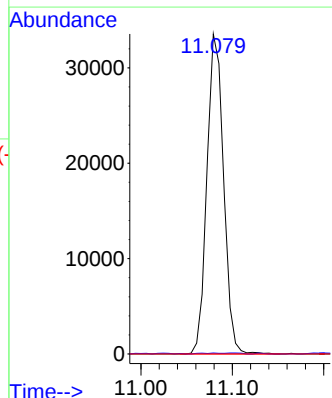
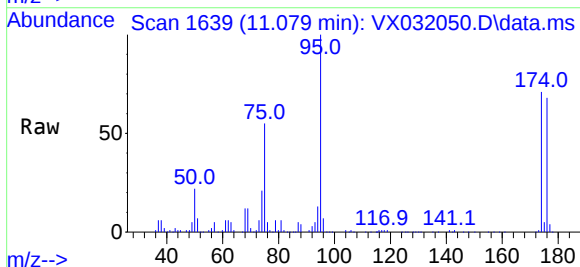




#82
4-Chlorotoluene
Concen: 0.497 ug/l
RT: 11.616 min Scan# 11
Delta R.T. 0.159 min
Lab File: VX032050.D
Acq: 11 Oct 2022 20:24




Instrument :
MSVOA_X
ClientSampleId :
COMP-B-2-VERTEME


Tgt Ion: 91 Resp: 2140
Ion Ratio Lower Upper
91 100
126 16.7 15.1 45.3

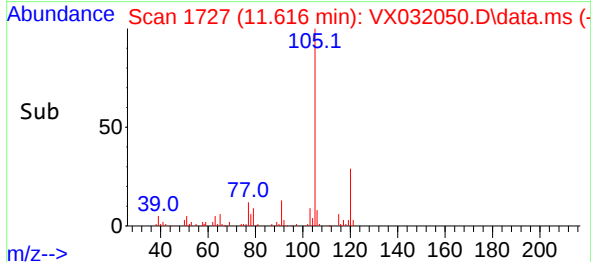

#83
tert-Butylbenzene
Concen: 3.082 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.043 min
Lab File: VX032050.D
Acq: 11 Oct 2022 20:24

Tgt Ion: 119 Resp: 13887
Ion Ratio Lower Upper
119 100
91 91.9 29.2 87.6#
134 0.0 11.6 34.8#


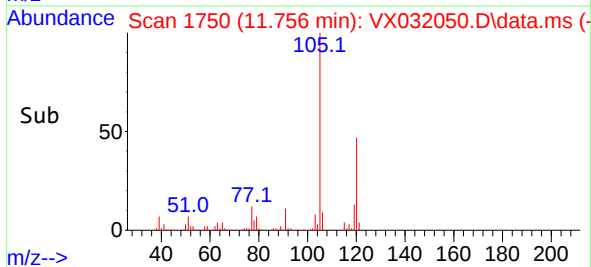

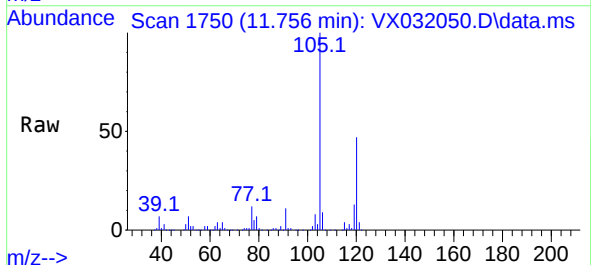




#84
1,2,4-Trimethylbenzene
Concen: 24.083 ug/l
RT: 11.750 min Scan# 1750
Delta R.T. -0.006 min
Lab File: VX032050.D
Acq: 11 Oct 2022 20:24




Instrument :
MSVOA_X
ClientSampleId :
COMP-B-2-VERTEME


Tgt Ion:105 Resp: 111368
Ion Ratio Lower Upper
105 100
120 45.2 22.6 67.8

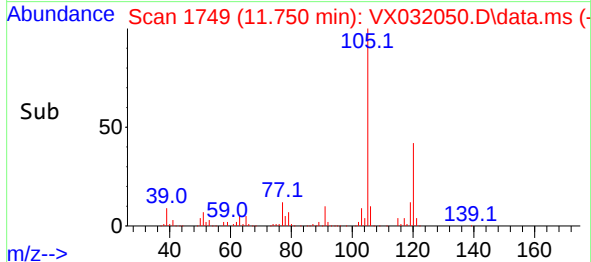

#85
sec-Butylbenzene
Concen: 19.966 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. -0.140 min
Lab File: VX032050.D
Acq: 11 Oct 2022 20:24

Tgt Ion:105 Resp: 111368
Ion Ratio Lower Upper
105 100
134 0.0 10.4 31.1#


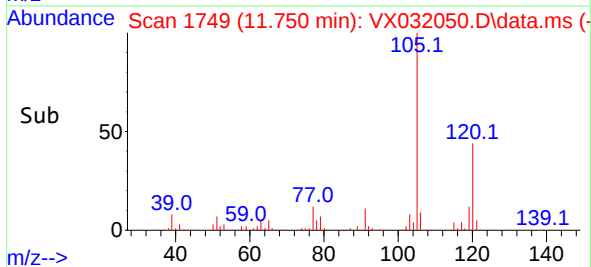

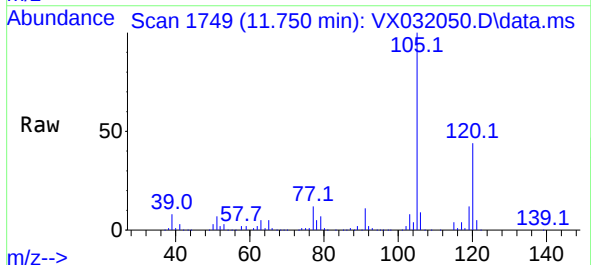




#86
p-Isopropyltoluene
Concen: 1.546 ug/l
RT: 11.969 min Scan# 1199
Delta R.T. -0.043 min
Lab File: VX032050.D
Acq: 11 Oct 2022 20:24




Instrument :
MSVOA_X
ClientSampleId :
COMP-B-2-VERTEME


Tgt Ion:119 Resp: 7260
Ion Ratio Lower Upper
119 100
134 25.4 13.4 40.2
91 27.6 12.4 37.2

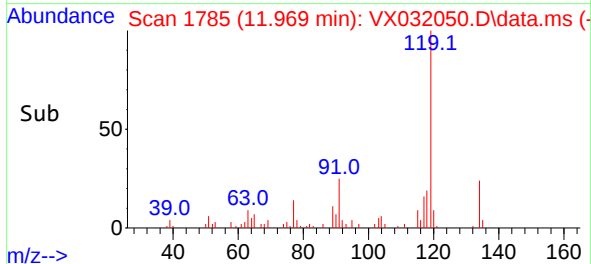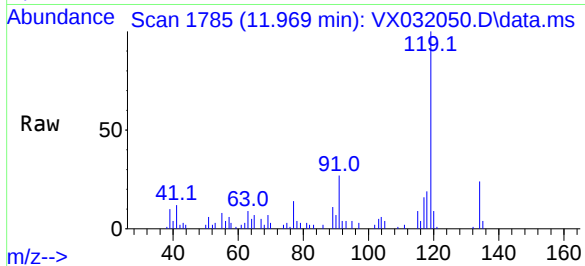

#89
n-Butylbenzene
Concen: 1.339 ug/l
RT: 12.329 min Scan# 1844
Delta R.T. -0.006 min
Lab File: VX032050.D
Acq: 11 Oct 2022 20:24

Tgt Ion: 91 Resp: 5264
Ion Ratio Lower Upper
91 100
92 31.8 27.0 81.0
134 103.8 13.3 39.9#


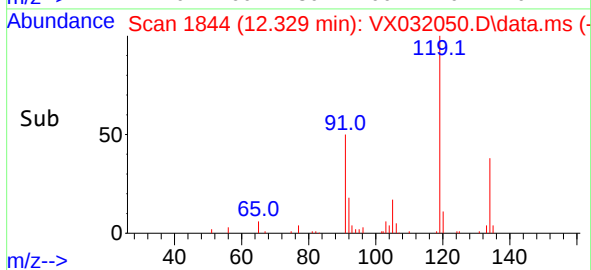

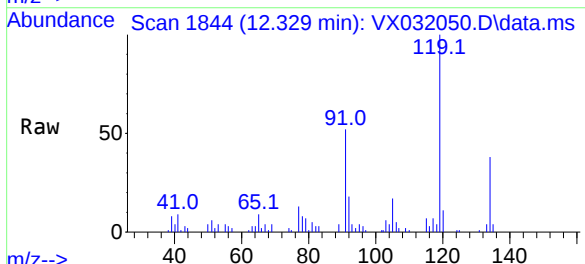




#90
Hexachloroethane
Concen: 6.887 ug/l
RT: 12.701 min Scan# 1905
Delta R.T. 0.159 min
Lab File: VX032050.D
Acq: 11 Oct 2022 20:24




Instrument :
MSVOA_X
ClientSampleId :
COMP-B-2-VERTME


Tgt Ion:117 Resp: 4278
Ion Ratio Lower Upper
117 100
201 0.0 34.8 104.4#

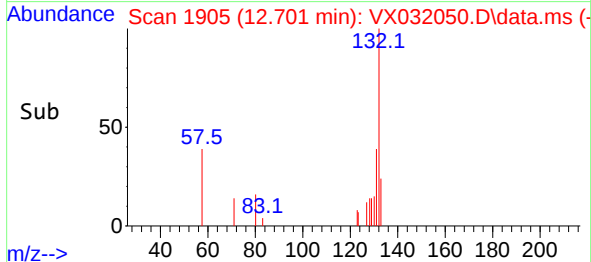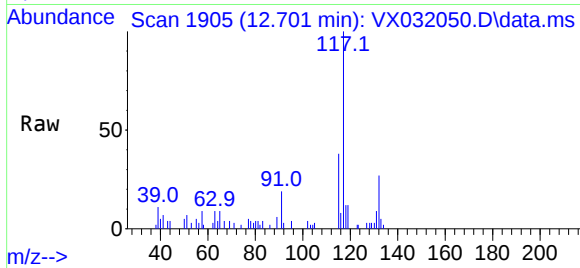

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.451 ug/l
RT: 12.969 min Scan# 1949
Delta R.T. 0.025 min
Lab File: VX032050.D
Acq: 11 Oct 2022 20:24

Tgt Ion: 75 Resp: 144
Ion Ratio Lower Upper
75 100
155 0.0 40.3 120.8#
157 0.0 51.5 154.5#

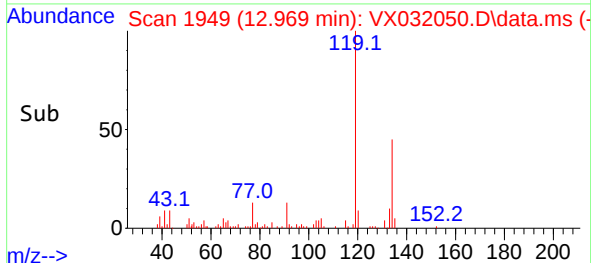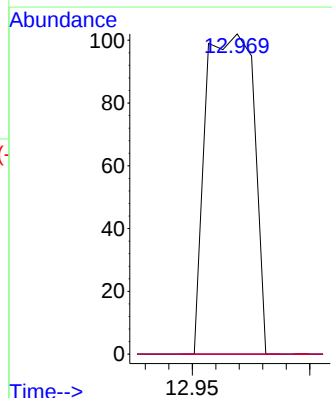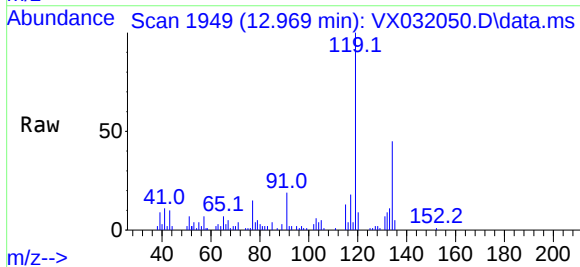



#95

Naphthalene

Concen: 146.635 ug/l

RT: 13.774 min Scan# 2081

Delta R.T. -0.006 min

Lab File: VX032050.D


Acq: 11 Oct 2022 20:24

Instrument :

MSVOA_X

ClientSampleId :

COMP-B-2-VERTME

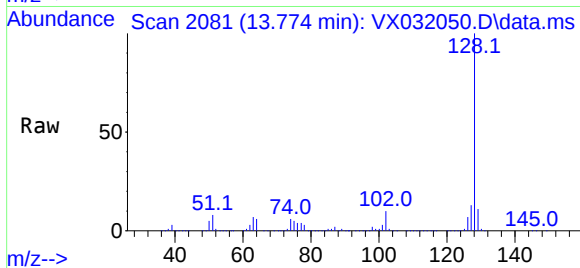

Tgt Ion:128 Resp: 780521

Ion Ratio Lower Upper

128 100

127 12.9 10.4 15.6

129 11.1 8.8 13.2

