

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101122\
 Data File : VX032059.D
 Acq On : 12 Oct 2022 04:18
 Operator : JC/MD
 Sample : N5067-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 B6(18-19)

Quant Time: Oct 12 06:22:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 06 14:28:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	76461	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	115965	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	129783	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	76236	50.000	ug/l	0.00


System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	80864	51.210	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 102.420%	
35) Dibromofluoromethane	5.385	113	63837	48.632	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 97.260%	
50) Toluene-d8	8.647	98	242530	51.347	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 102.700%	
62) 4-Bromofluorobenzene	11.079	95	84087	50.356	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 100.720%	

Target Compounds				Qvalue		
5) Bromomethane	1.617	94	333	Below Cal	#	74
10) Methyl Iodide	2.459	142	188	2.893	ug/l #	50
11) Tert butyl alcohol	2.934	59	719	3.660	ug/l #	73
13) Acrolein	2.239	56	279	Below Cal		86
16) Acetone	2.386	43	23422	43.643	ug/l	100
17) Carbon Disulfide	2.514	76	1073	0.429	ug/l #	75
18) Methyl Acetate	2.715	43	805	0.455	ug/l #	77
20) Methylene Chloride	2.794	84	7759	5.502	ug/l	87
25) 2-Butanone	4.580	43	3078	3.669	ug/l #	82
29) Tetrahydrofuran	5.038	42	524	0.968	ug/l #	54
31) Cyclohexane	5.550	56	1844	0.978	ug/l #	8
36) 1,1-Dichloropropene	5.550	75	6455	3.708	ug/l #	50
37) Ethyl Acetate	4.721	43	13868	8.463	ug/l	100
38) Carbon Tetrachloride	5.556	117	8220	4.619	ug/l #	17
40) Benzene	6.043	78	2272	0.446	ug/l	95
41) Methacrylonitrile	5.025	41	229	0.269	ug/l #	39
43) Isopropyl Acetate	6.342	43	60107	24.175	ug/l	98
48) Methyl methacrylate	7.799	41	58644	49.360	ug/l #	46
49) 1,4-Dioxane	7.793	88	85	Below Cal	#	1
51) 4-Methyl-2-Pentanone	8.549	43	50399	30.588	ug/l #	50
53) t-1,3-Dichloropropene	8.951	75	399	1.423	ug/l #	44
54) cis-1,3-Dichloropropene	8.549	75	21649	11.920	ug/l #	68
56) Ethyl methacrylate	9.250	69	608	0.337	ug/l #	1
57) 1,3-Dichloropropane	9.482	76	2895	1.281	ug/l #	43
59) 2-Hexanone	9.482	43	41309	34.002	ug/l #	52
68) m/p-Xylenes	10.305	106	545	0.206	ug/l	82
74) N-amyl acetate	10.640	43	12904	7.349	ug/l #	52
76) 1,2,3-Trichloropropane	11.079	75	46610	29.831	ug/l #	37
81) trans-1,4-Dichloro-2-b...	11.079	75	46610	101.841	ug/l #	11
84) 1,2,4-Trimethylbenzene	11.750	105	1178	0.243	ug/l	89
90) Hexachloroethane	12.414	117	597	2.051	ug/l #	15
95) Naphthalene	13.774	128	842277	151.045	ug/l	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Quant Time: Oct 12 06:22:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 06 14:28:46 2022
Response via : Initial Calibration





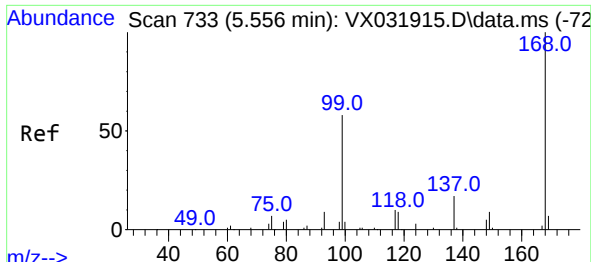


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX032059.D
Acq: 12 Oct 2022 04:18

Instrument :
MSVOA_X
ClientSampleId :
B6(18-19)



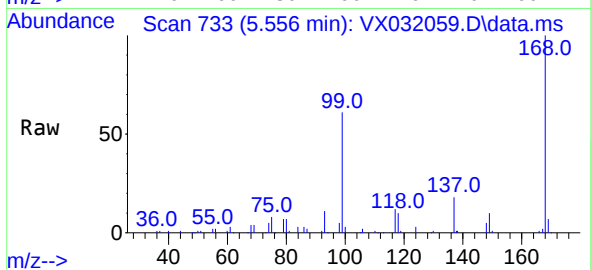



Tgt Ion:168 Resp: 76461
Ion Ratio Lower Upper
168 100
99 60.9 48.8 73.2

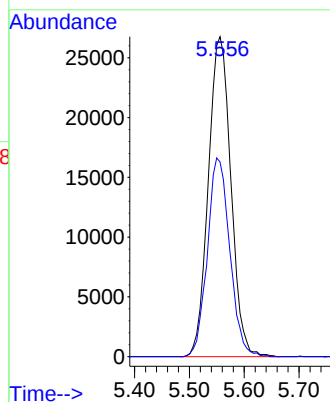

#5
Bromomethane
Concen: Below Cal
RT: 1.617 min Scan# 87
Delta R.T. 0.006 min
Lab File: VX032059.D
Acq: 12 Oct 2022 04:18

Tgt Ion: 94 Resp: 333
Ion Ratio Lower Upper
94 100
96 68.4 74.4 111.6#


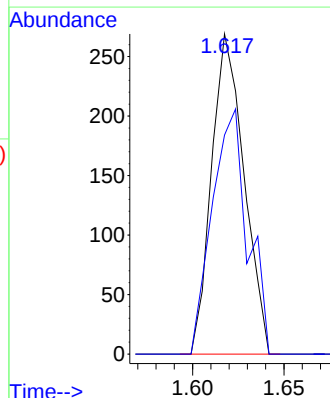
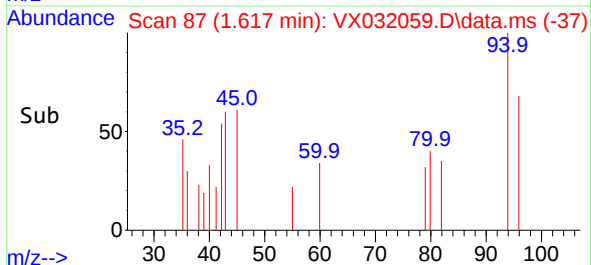
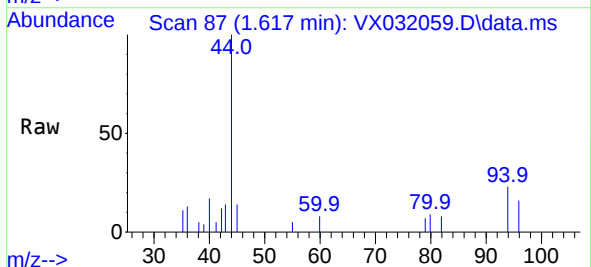


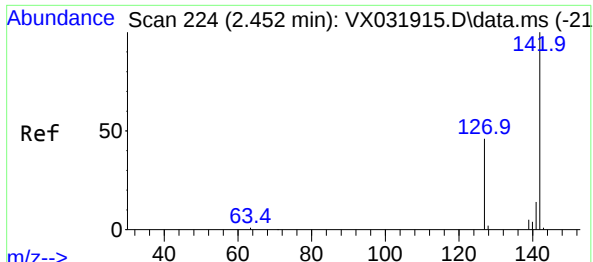

#10
Methyl Iodide
Concen: 2.893 ug/l
RT: 2.459 min Scan# 21
Delta R.T. 0.007 min
Lab File: VX032059.D
Acq: 12 Oct 2022 04:18




Instrument :
MSVOA_X
ClientSampleId :
B6(18-19)

Tgt Ion:142 Resp: 188
Ion Ratio Lower Upper
142 100
127 10.6 37.4 56.0#
141 0.0 11.6 17.4#

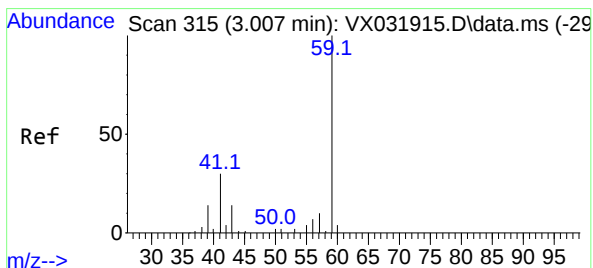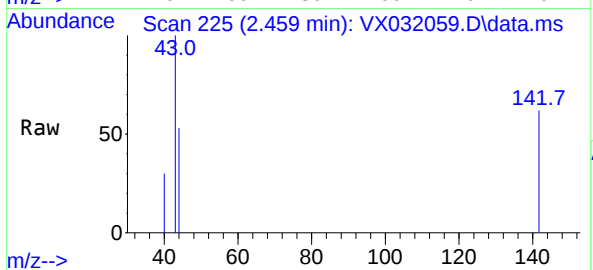


#11
Tert butyl alcohol
Concen: 3.660 ug/l
RT: 2.934 min Scan# 303
Delta R.T. -0.073 min
Lab File: VX032059.D
Acq: 12 Oct 2022 04:18


Tgt Ion: 59 Resp: 719
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.2#

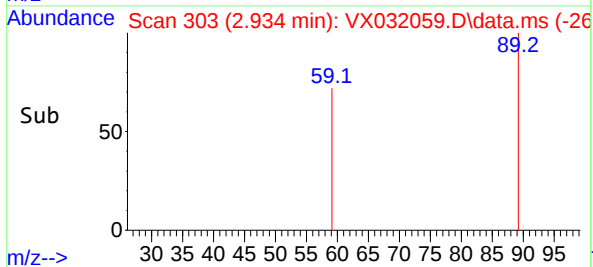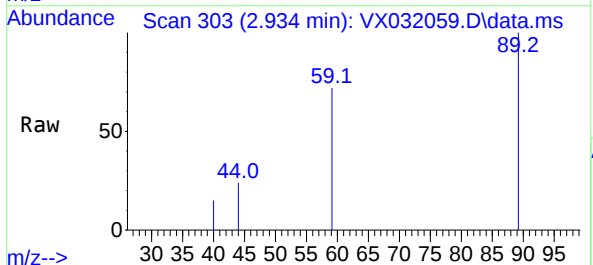


Abundance Scan 189 (2.239 min): VX031915.D\data.ms (-18)

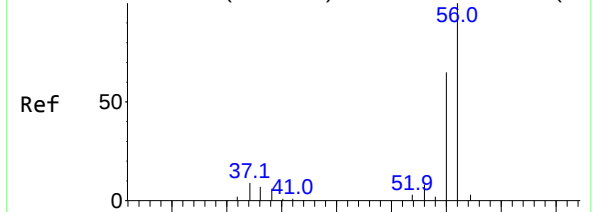

Abundance Scan 189 (2.239 min): VX032059.D\data.ms

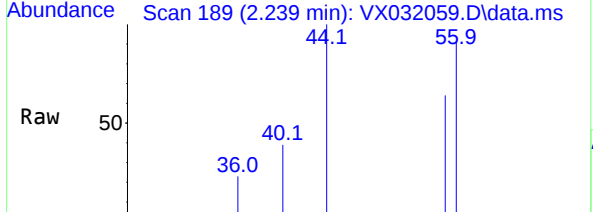

Abundance Scan 189 (2.239 min): VX032059.D\data.ms (-14)

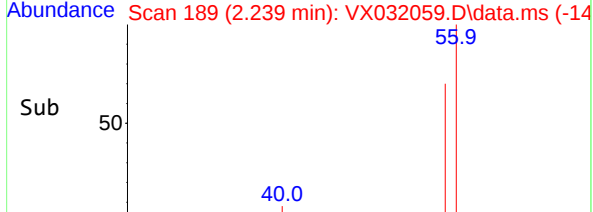

#13

Acrolein

Concen: Below Cal

RT: 2.239 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX032059.D

Acq: 12 Oct 2022 04:18

Instrument :

MSVOA_X

ClientSampleId :

B6(18-19)


Tgt Ion: 56 Resp: 279

Ion Ratio Lower Upper


56 100

55 58.8 56.0 84.0


Abundance

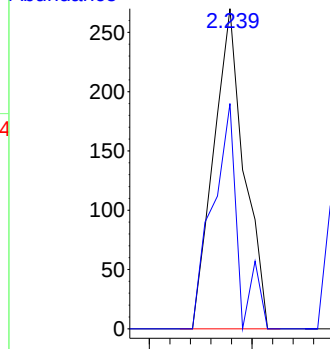


Abundance Scan 214 (2.392 min): VX031915.D\data.ms (-20)

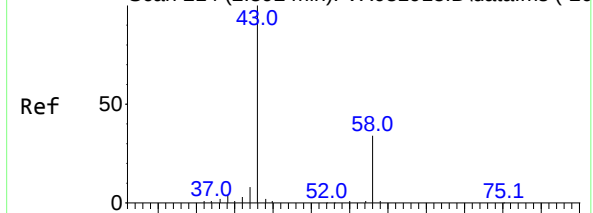

Abundance Scan 213 (2.386 min): VX032059.D\data.ms

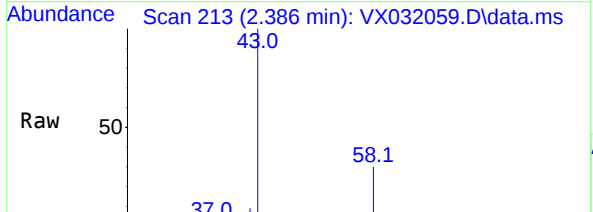

Abundance Scan 213 (2.386 min): VX032059.D\data.ms (-16)

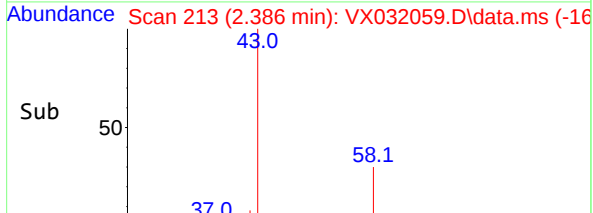

#16

Acetone

Concen: 43.643 ug/l

RT: 2.386 min Scan# 213

Delta R.T. -0.006 min

Lab File: VX032059.D

Acq: 12 Oct 2022 04:18


Tgt Ion: 43 Resp: 23422


Ion Ratio Lower Upper

43 100

58 29.6 23.8 35.8

Abundance




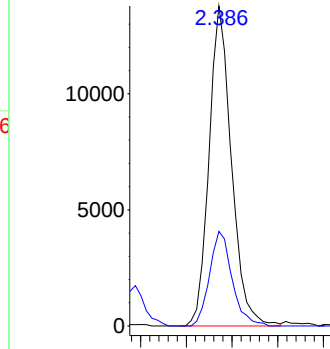




#17
Carbon Disulfide
Concen: 0.429 ug/l
RT: 2.514 min Scan# 21
Delta R.T. 0.001 min
Lab File: VX032059.D
Acq: 12 Oct 2022 04:18




Instrument :
MSVOA_X
ClientSampleId :
B6(18-19)


Tgt Ion: 76 Resp: 1073
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#

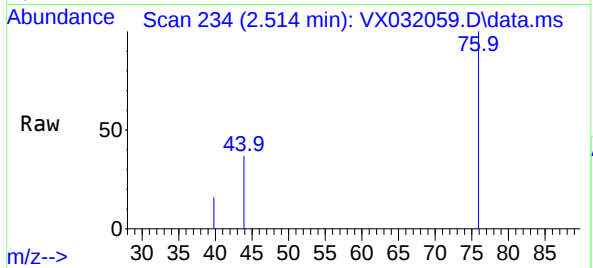

#18
Methyl Acetate
Concen: 0.455 ug/l
RT: 2.715 min Scan# 267
Delta R.T. 0.006 min
Lab File: VX032059.D
Acq: 12 Oct 2022 04:18

Tgt Ion: 43 Resp: 805
Ion Ratio Lower Upper
43 100
74 11.8 18.6 27.8#

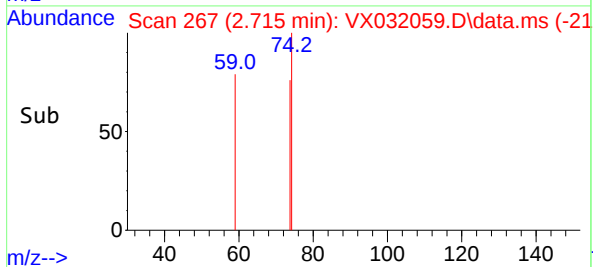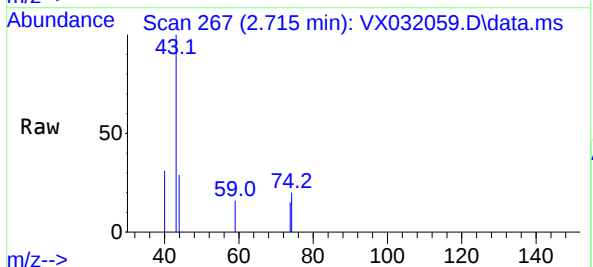



#20

Methylene Chloride

Concen: 5.502 ug/l

RT: 2.794 min Scan# 21

Delta R.T. 0.006 min

Lab File: VX032059.D

Acq: 12 Oct 2022 04:18

Instrument :

MSVOA_X

ClientSampleId :

B6(18-19)

Tgt Ion: 84 Resp: 7759





Ion Ratio Lower Upper

84 100

49 111.0 105.9 158.9

51 35.4 32.2 48.2

86 58.6 50.8 76.2

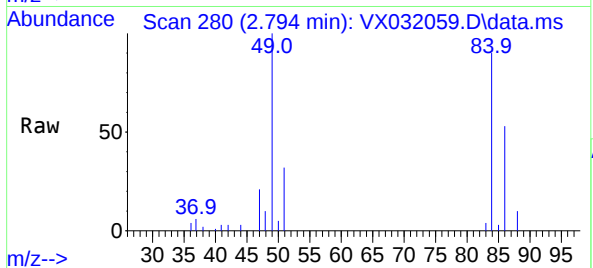

#25

2-Butanone

Concen: 3.669 ug/l

RT: 4.580 min Scan# 573

Delta R.T. 0.018 min

Lab File: VX032059.D




Acq: 12 Oct 2022 04:18


Tgt Ion: 43 Resp: 3078

Ion Ratio Lower Upper

43 100

72 17.4 21.1 31.7#

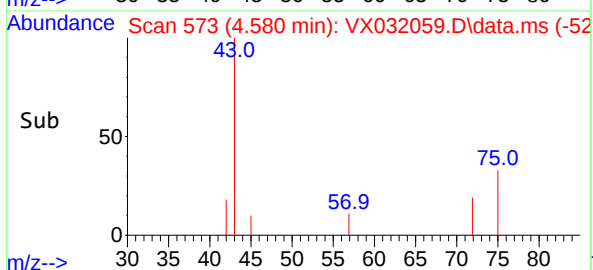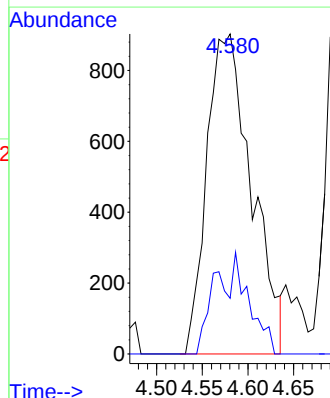



#29

Tetrahydrofuran

Concen: 0.968 ug/l

RT: 5.038 min Scan# 64

Delta R.T. 0.025 min

Lab File: VX032059.D

Acq: 12 Oct 2022 04:18

Instrument :

MSVOA_X

ClientSampleId :

B6(18-19)





Tgt Ion: 42 Resp: 524

Ion Ratio Lower Upper

42 100

72 23.1 36.4 54.6#

71 4.4 33.5 50.3#

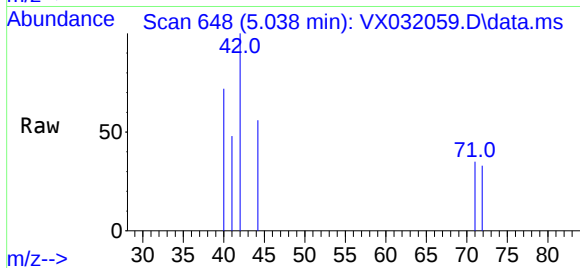

#31

Cyclohexane

Concen: 0.978 ug/l

RT: 5.550 min Scan# 732

Delta R.T. 0.080 min

Lab File: VX032059.D

Acq: 12 Oct 2022 04:18




Tgt Ion: 56 Resp: 1844


Ion Ratio Lower Upper

56 100

69 168.9 25.1 37.7#

84 121.7 70.2 105.4#

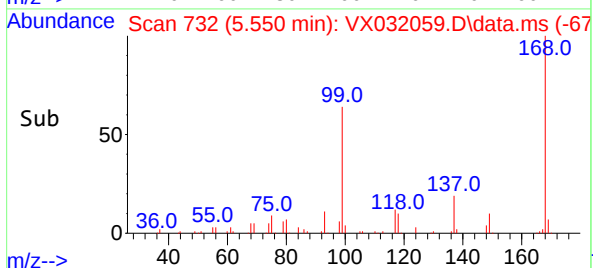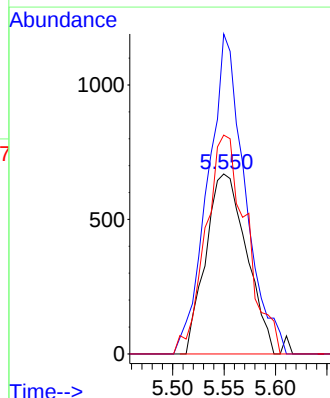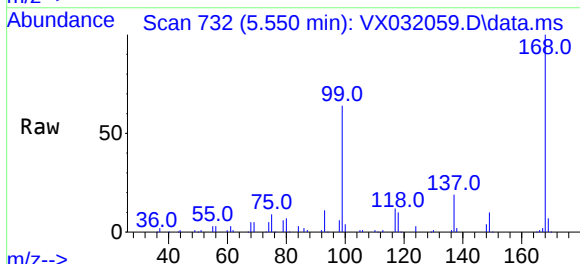



#33

1,2-Dichloroethane-d4

Concen: 51.210 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX032059.D

Acq: 12 Oct 2022 04:18

Instrument :

MSVOA_X

ClientSampleId :





B6(18-19)

Tgt Ion: 65 Resp: 80864

Ion Ratio Lower Upper

65 100

67 51.5 0.0 102.4

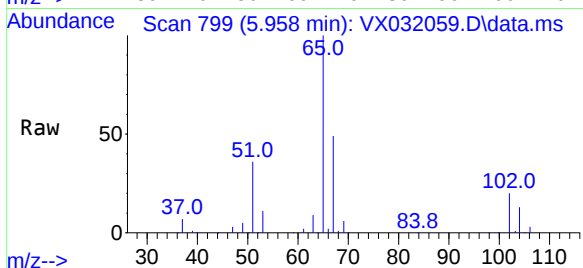

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.000 min

Lab File: VX032059.D

Acq: 12 Oct 2022 04:18




Tgt Ion: 114 Resp: 115965


Ion Ratio Lower Upper

114 100

63 20.5 0.0 42.6

88 16.6 0.0 33.0


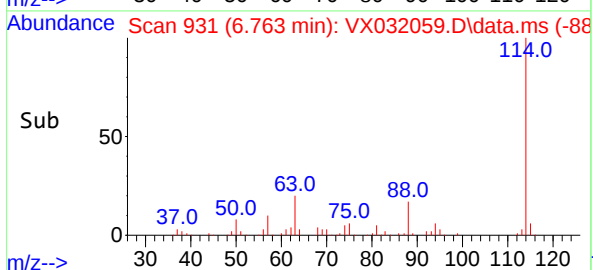

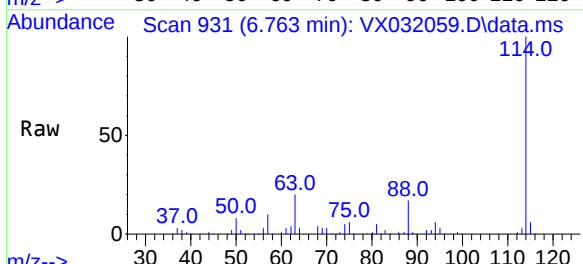


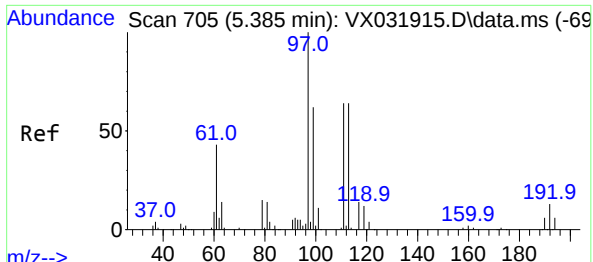

#35
Dibromofluoromethane
Concen: 48.632 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX032059.D
Acq: 12 Oct 2022 04:18




Instrument :
MSVOA_X
ClientSampleId :
B6(18-19)


Tgt Ion:113 Resp: 63837
Ion Ratio Lower Upper
113 100
111 102.0 82.4 123.6
192 18.8 14.1 21.1

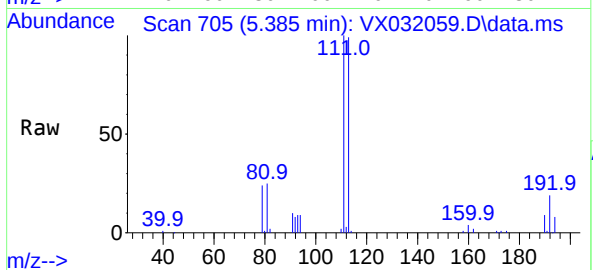

#36
1,1-Dichloropropene
Concen: 3.708 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.140 min
Lab File: VX032059.D
Acq: 12 Oct 2022 04:18

Tgt Ion: 75 Resp: 6455
Ion Ratio Lower Upper
75 100
110 8.9 17.5 52.5#
77 0.0 24.9 37.3#


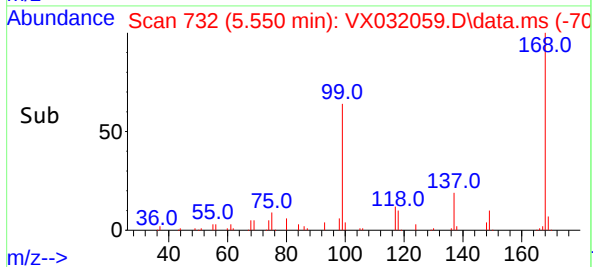

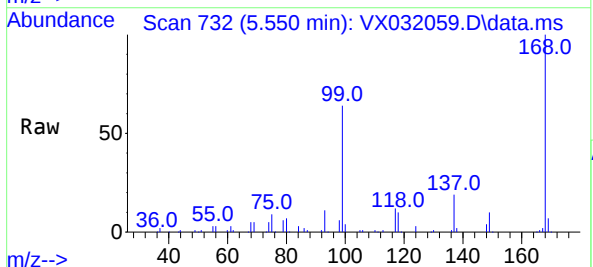




#37
Ethyl Acetate
Concen: 8.463 ug/l
RT: 4.721 min Scan# 51
Delta R.T. 0.007 min
Lab File: VX032059.D
Acq: 12 Oct 2022 04:18




Instrument :
MSVOA_X
ClientSampleId :
B6(18-19)


Tgt Ion:	43	Resp:	13868
Ion	Ratio	Lower	Upper
43	100		
61	13.7	11.1	16.7
70	11.0	8.6	13.0



#38
Carbon Tetrachloride
Concen: 4.619 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.121 min
Lab File: VX032059.D
Acq: 12 Oct 2022 04:18

Tgt Ion:	117	Resp:	8220
Ion	Ratio	Lower	Upper
117	100		
119	5.5	74.6	112.0#
121	0.0	25.3	37.9#


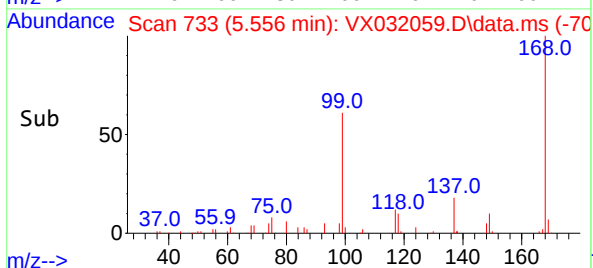
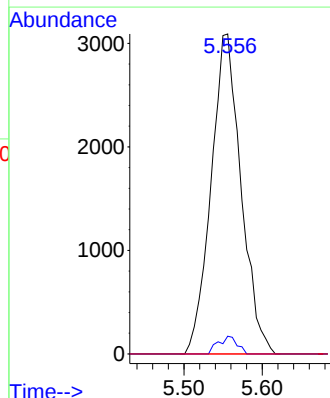





#40
Benzene
Concen: 0.446 ug/l
RT: 6.043 min Scan# 812
Delta R.T. 0.006 min
Lab File: VX032059.D
Acq: 12 Oct 2022 04:18




Instrument :
MSVOA_X
ClientSampleId :
B6(18-19)


Tgt Ion: 78 Resp: 2272
Ion Ratio Lower Upper
78 100
77 21.0 18.7 28.1

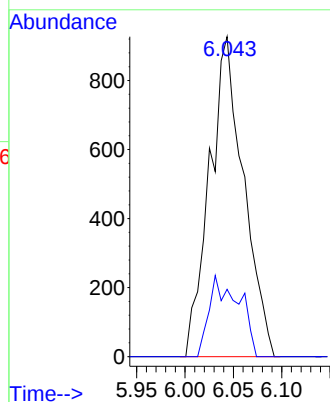

#41
Methacrylonitrile
Concen: 0.269 ug/l
RT: 5.025 min Scan# 646
Delta R.T. 0.103 min
Lab File: VX032059.D
Acq: 12 Oct 2022 04:18

Tgt Ion: 41 Resp: 229
Ion Ratio Lower Upper
41 100
39 35.4 45.0 67.6#
67 0.0 58.2 87.4#
52 0.0 25.0 37.6#


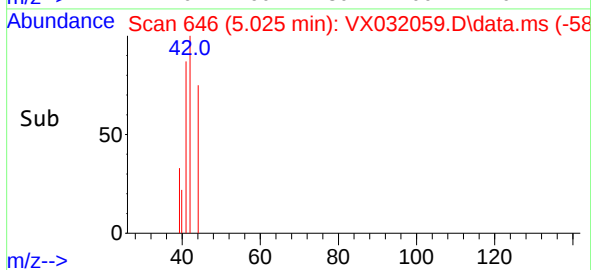






#43
Isopropyl Acetate
Concen: 24.175 ug/l
RT: 6.342 min Scan# 80
Delta R.T. 0.000 min
Lab File: VX032059.D
Acq: 12 Oct 2022 04:18




Instrument :
MSVOA_X
ClientSampleId :
B6(18-19)


Tgt Ion: 43 Resp: 60107
Ion Ratio Lower Upper
43 100
61 18.4 15.3 22.9
87 14.0 10.6 15.8

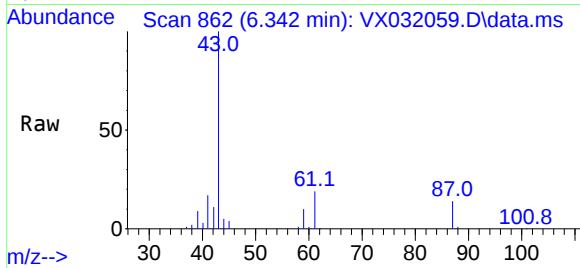

#48
Methyl methacrylate
Concen: 49.360 ug/l
RT: 7.799 min Scan# 1101
Delta R.T. 0.104 min
Lab File: VX032059.D
Acq: 12 Oct 2022 04:18

Tgt Ion: 41 Resp: 58644
Ion Ratio Lower Upper
41 100
69 0.0 64.6 96.8#
39 58.9 51.4 77.0

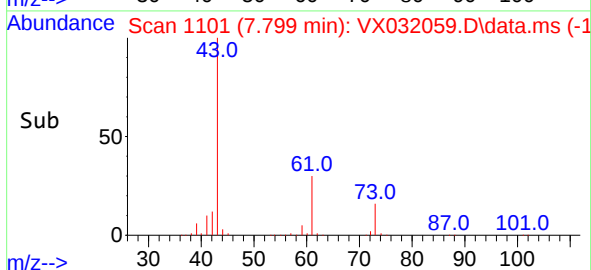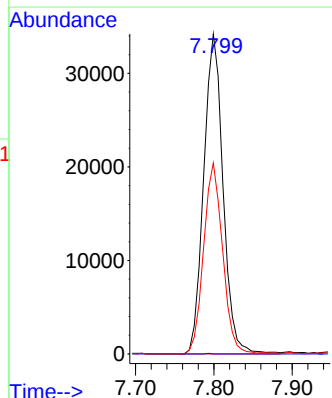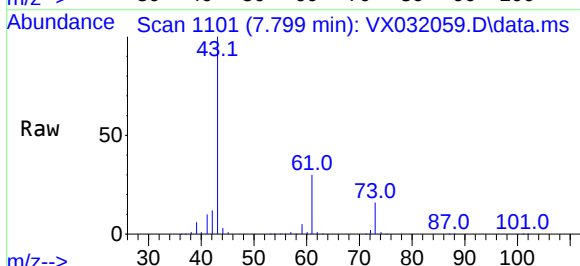



#49

1,4-Dioxane

Concen: Below Cal

RT: 7.793 min Scan# 1100

Delta R.T. 0.098 min

Lab File: VX032059.D

Acq: 12 Oct 2022 04:18

Instrument :

MSVOA_X

ClientSampleId :

B6(18-19)


Tgt Ion: 88 Resp: 85

Ion Ratio Lower Upper




88 100

43 680832.9 27.1 40.7#

58 3103.5 53.9 80.9#

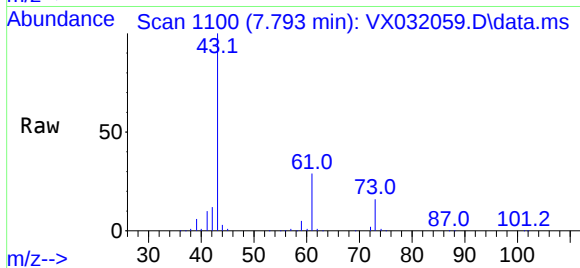

Abundance

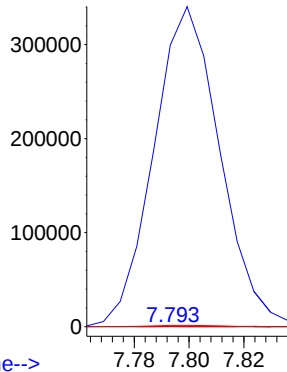

#50

Toluene-d8

Concen: 51.347 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. -0.006 min

Lab File: VX032059.D


Acq: 12 Oct 2022 04:18

Tgt Ion: 98 Resp: 242530



Ion Ratio Lower Upper


98 100

100 65.7 52.5 78.7

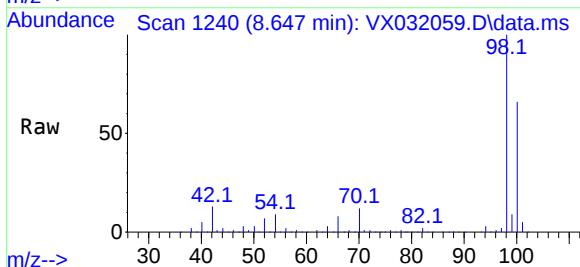

Abundance



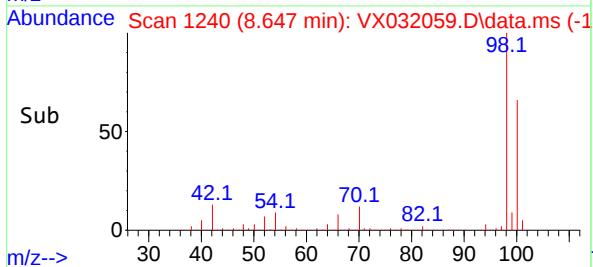
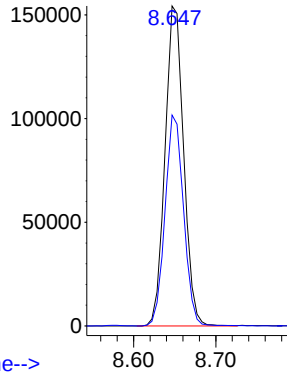




#51
4-Methyl-2-Pentanone
Concen: 30.588 ug/l
RT: 8.549 min Scan# 11
Delta R.T. -0.024 min
Lab File: VX032059.D
Acq: 12 Oct 2022 04:18




Instrument :
MSVOA_X
ClientSampleId :
B6(18-19)


Tgt Ion: 43 Resp: 50399
Ion Ratio Lower Upper
43 100
58 7.8 30.6 46.0#

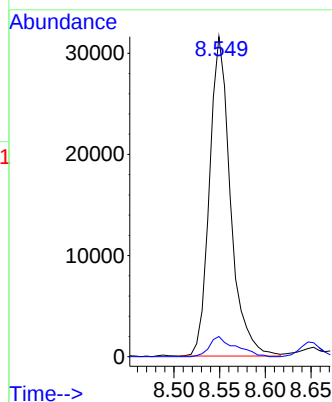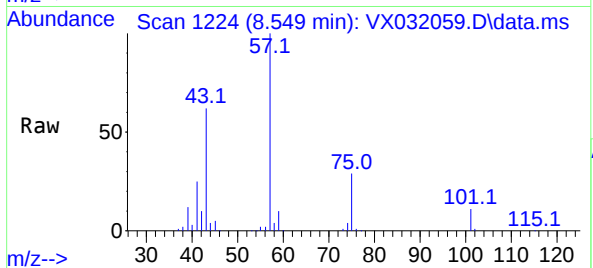

#53
t-1,3-Dichloropropene
Concen: 1.423 ug/l
RT: 8.951 min Scan# 1290
Delta R.T. -0.031 min
Lab File: VX032059.D
Acq: 12 Oct 2022 04:18

Tgt Ion: 75 Resp: 399
Ion Ratio Lower Upper
75 100
77 0.0 24.8 37.2#


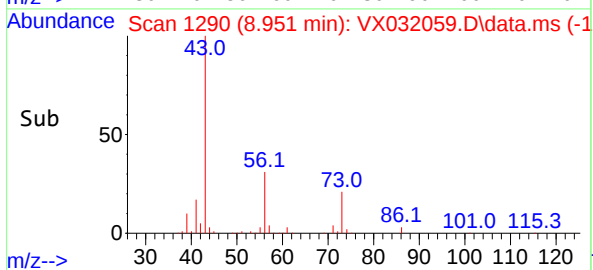
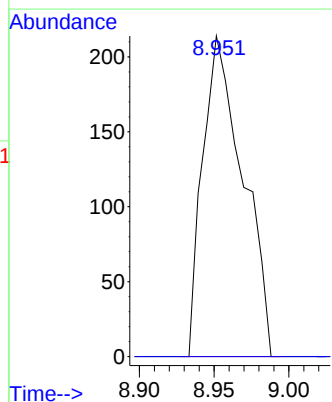





#54
cis-1,3-Dichloropropene
Concen: 11.920 ug/l
RT: 8.549 min Scan# 1194
Delta R.T. 0.183 min
Lab File: VX032059.D
Acq: 12 Oct 2022 04:18




Instrument :
MSVOA_X
ClientSampleId :
B6(18-19)


Tgt Ion: 75 Resp: 21649
Ion Ratio Lower Upper
75 100
77 0.7 24.4 36.6#
39 40.9 43.7 65.5#

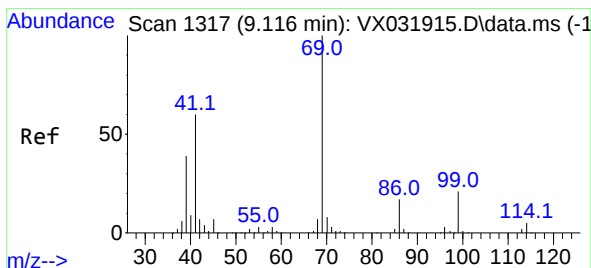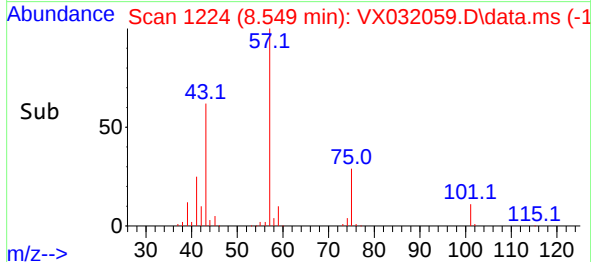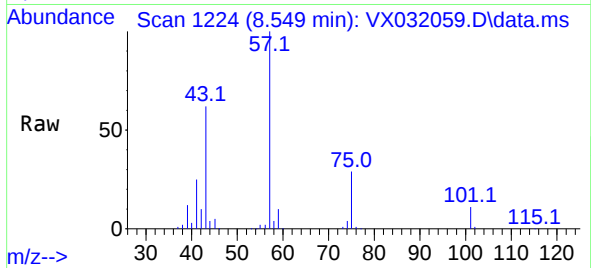

#56
Ethyl methacrylate
Concen: 0.337 ug/l
RT: 9.250 min Scan# 1339
Delta R.T. 0.134 min
Lab File: VX032059.D
Acq: 12 Oct 2022 04:18

Tgt Ion: 69 Resp: 608
Ion Ratio Lower Upper
69 100
41 5986.3 54.2 81.4#
39 2935.4 34.2 51.2#


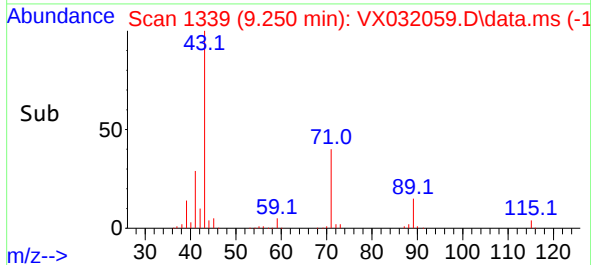

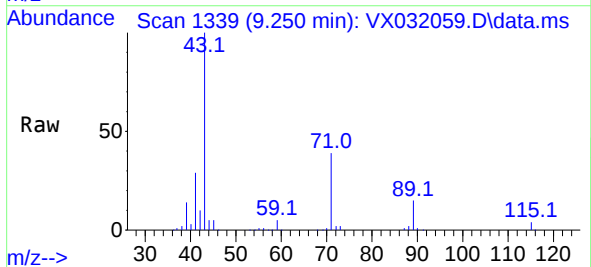




#57
1,3-Dichloropropane
Concen: 1.281 ug/l
RT: 9.482 min Scan# 1377
Delta R.T. 0.171 min
Lab File: VX032059.D
Acq: 12 Oct 2022 04:18




Instrument :
MSVOA_X
ClientSampleId :
B6(18-19)


Tgt Ion: 76 Resp: 2895
Ion Ratio Lower Upper
76 100
78 0.0 25.5 38.3#



#59
2-Hexanone
Concen: 34.002 ug/l
RT: 9.482 min Scan# 1377
Delta R.T. 0.049 min
Lab File: VX032059.D
Acq: 12 Oct 2022 04:18

Tgt Ion: 43 Resp: 41309
Ion Ratio Lower Upper
43 100
58 19.3 26.7 80.0#


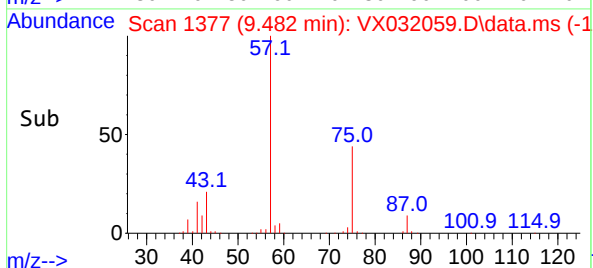






#62
4-Bromofluorobenzene
Concen: 50.356 ug/l
RT: 11.079 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX032059.D
Acq: 12 Oct 2022 04:18




Instrument :
MSVOA_X
ClientSampleId :
B6(18-19)


Tgt Ion: 95 Resp: 84087
Ion Ratio Lower Upper
95 100
174 76.7 0.0 153.2
176 74.1 0.0 144.0

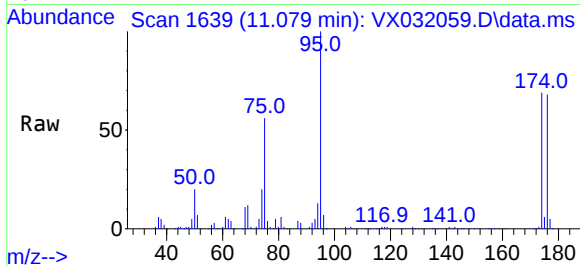

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX032059.D
Acq: 12 Oct 2022 04:18

Tgt Ion: 117 Resp: 129783
Ion Ratio Lower Upper
117 100
82 56.4 46.8 70.2
119 31.7 26.4 39.6


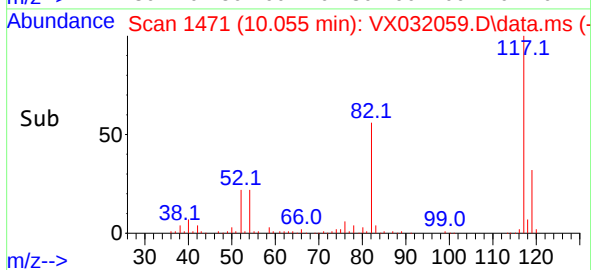

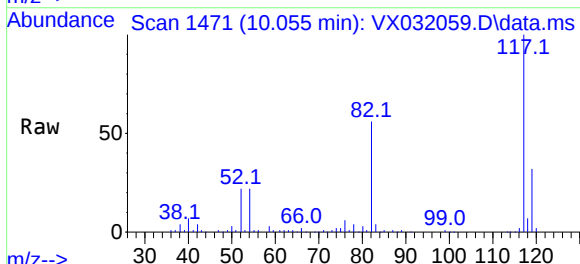




#68
m/p-Xylenes
Concen: 0.206 ug/l
RT: 10.305 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX032059.D
Acq: 12 Oct 2022 04:18




Instrument :
MSVOA_X
ClientSampleId :
B6(18-19)


Tgt Ion:106 Resp: 545
Ion Ratio Lower Upper
106 100
91 228.6 161.0 241.4



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX032059.D
Acq: 12 Oct 2022 04:18

Tgt Ion:152 Resp: 76236
Ion Ratio Lower Upper
152 100
115 62.4 43.4 130.1
150 157.2 0.0 346.8


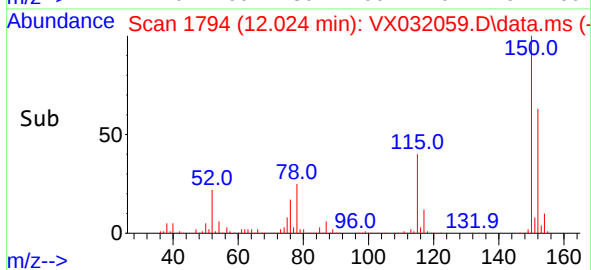






#74
N-amy1 acetate
Concen: 7.349 ug/l
RT: 10.640 min Scan# 11
Delta R.T. -0.207 min
Lab File: VX032059.D
Acq: 12 Oct 2022 04:18




Instrument :
MSVOA_X
ClientSampleId :
B6(18-19)


Tgt Ion: 43	Resp:	12904
Ion	Ratio	Lower Upper
43	100	
70	2.2	33.4 50.2#
55	4.9	18.2 27.2#
61	8.7	19.3 28.9#

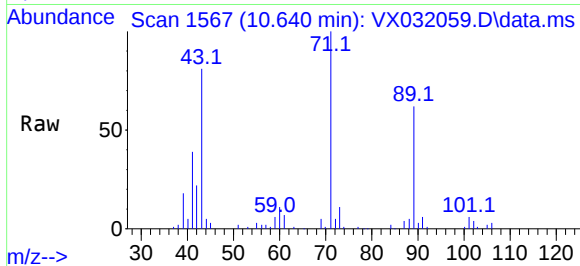

#76
1,2,3-Trichloropropane
Concen: 29.831 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.158 min
Lab File: VX032059.D
Acq: 12 Oct 2022 04:18

Tgt Ion: 75	Resp:	46610
Ion	Ratio	Lower Upper
75	100	
77	1.1	20.3 60.9#


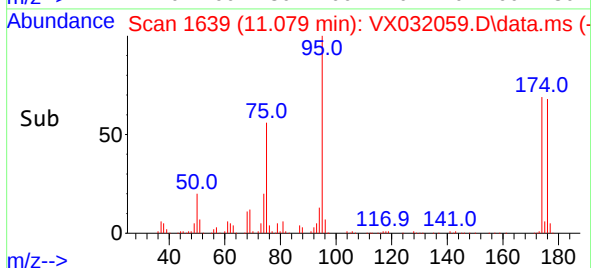

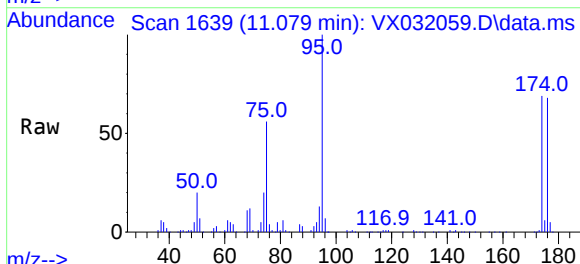




#81
trans-1,4-Dichloro-2-butene
Concen: 101.841 ug/l
RT: 11.079 min Scan# 1629
Delta R.T. 0.061 min
Lab File: VX032059.D
Acq: 12 Oct 2022 04:18




Instrument :
MSVOA_X
ClientSampleId :
B6(18-19)


Tgt Ion: 75 Resp: 46610
Ion Ratio Lower Upper
75 100
53 0.0 77.6 116.4#
89 0.0 37.4 56.0#

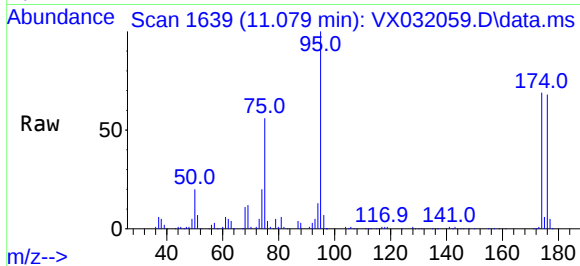

#84
1,2,4-Trimethylbenzene
Concen: 0.243 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. -0.006 min
Lab File: VX032059.D
Acq: 12 Oct 2022 04:18

Tgt Ion:105 Resp: 1178
Ion Ratio Lower Upper
105 100
120 37.9 22.6 67.8


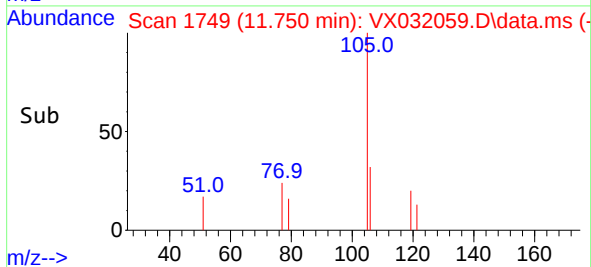

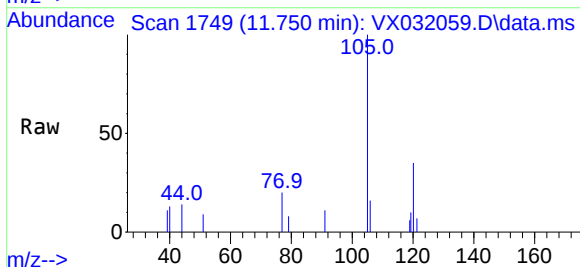




#90
Hexachloroethane
Concen: 2.051 ug/l
RT: 12.414 min Scan# 1879
Delta R.T. -0.128 min
Lab File: VX032059.D
Acq: 12 Oct 2022 04:18

Instrument :
MSVOA_X
ClientSampleId :
B6(18-19)

Tgt Ion:117 Resp: 597
Ion Ratio Lower Upper
117 100
201 0.0 34.8 104.4#

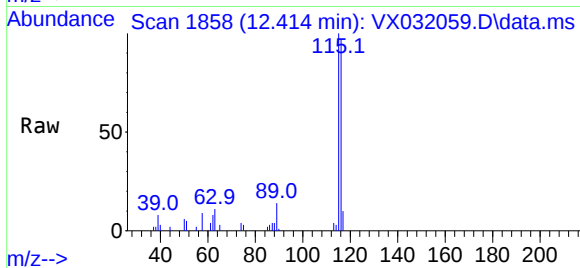

#95
Naphthalene
Concen: 151.045 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.006 min
Lab File: VX032059.D
Acq: 12 Oct 2022 04:18

Tgt Ion:128 Resp: 842277
Ion Ratio Lower Upper
128 100
127 12.8 10.4 15.6
129 11.0 8.8 13.2

