

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101122\
 Data File : VX032066.D
 Acq On : 12 Oct 2022 07:01
 Operator : JC/MD
 Sample : N5067-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 B5(20-21)

Quant Time: Oct 12 13:26:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 06 14:28:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	73671	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	111934	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	121106	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	72434	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	79589	52.311	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 104.620%	
35) Dibromofluoromethane	5.391	113	60197	47.510	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 95.020%	
50) Toluene-d8	8.647	98	232806	51.063	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 102.120%	
62) 4-Bromofluorobenzene	11.079	95	78999	49.013	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 98.020%	


Target Compounds				Qvalue		
5) Bromomethane	1.611	94	213	Below Cal	#	80
11) Tert butyl alcohol	2.995	59	131	0.692	ug/l #	73
13) Acrolein	2.239	56	168	Below Cal		93
16) Acetone	2.386	43	24690	47.748	ug/l	97
17) Carbon Disulfide	2.520	76	943	0.391	ug/l #	75
18) Methyl Acetate	2.703	43	813	0.477	ug/l #	67
20) Methylene Chloride	2.788	84	8148	5.996	ug/l	94
25) 2-Butanone	4.580	43	3650	4.516	ug/l	92
29) Tetrahydrofuran	5.025	42	360	0.690	ug/l #	43
31) Cyclohexane	5.556	56	1717	0.945	ug/l #	55
36) 1,1-Dichloropropene	5.556	75	6046	3.599	ug/l #	50
37) Ethyl Acetate	4.714	43	13948	8.818	ug/l #	84
38) Carbon Tetrachloride	5.550	117	7983	4.647	ug/l #	18
40) Benzene	6.037	78	7276	1.479	ug/l	98
43) Isopropyl Acetate	6.342	43	59108	24.629	ug/l	100
48) Methyl methacrylate	7.799	41	58721	51.204	ug/l #	46
49) 1,4-Dioxane	7.799	88	46	Below Cal	#	1
51) 4-Methyl-2-Pentanone	8.549	43	50132	31.522	ug/l #	50
52) Toluene	8.720	92	1388	0.431	ug/l	91
53) t-1,3-Dichloropropene	8.958	75	356	1.407	ug/l #	44
54) cis-1,3-Dichloropropene	8.549	75	22279	12.709	ug/l #	69
56) Ethyl methacrylate	9.244	69	548	0.315	ug/l #	1
57) 1,3-Dichloropropane	9.482	76	2945	1.350	ug/l #	43
59) 2-Hexanone	9.482	43	41411	35.314	ug/l #	51
67) Ethyl Benzene	10.195	91	2662	0.429	ug/l	97
68) m/p-Xylenes	10.305	106	945	0.383	ug/l	97
69) o-Xylene	10.640	106	635	0.265	ug/l	84
74) N-amyl acetate	10.640	43	12744	7.639	ug/l #	52
76) 1,2,3-Trichloropropane	11.079	75	44909	30.251	ug/l #	37
81) trans-1,4-Dichloro-2-b...	11.079	75	44909	103.225	ug/l #	11
90) Hexachloroethane	12.695	117	187	1.553	ug/l #	15
95) Naphthalene	13.774	128	27350	5.162	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101122\
Data File : VX032066.D
Acq On : 12 Oct 2022 07:01
Operator : JC/MD
Sample : N5067-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
B5(20-21)

Quant Time: Oct 12 13:26:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 06 14:28:46 2022
Response via : Initial Calibration




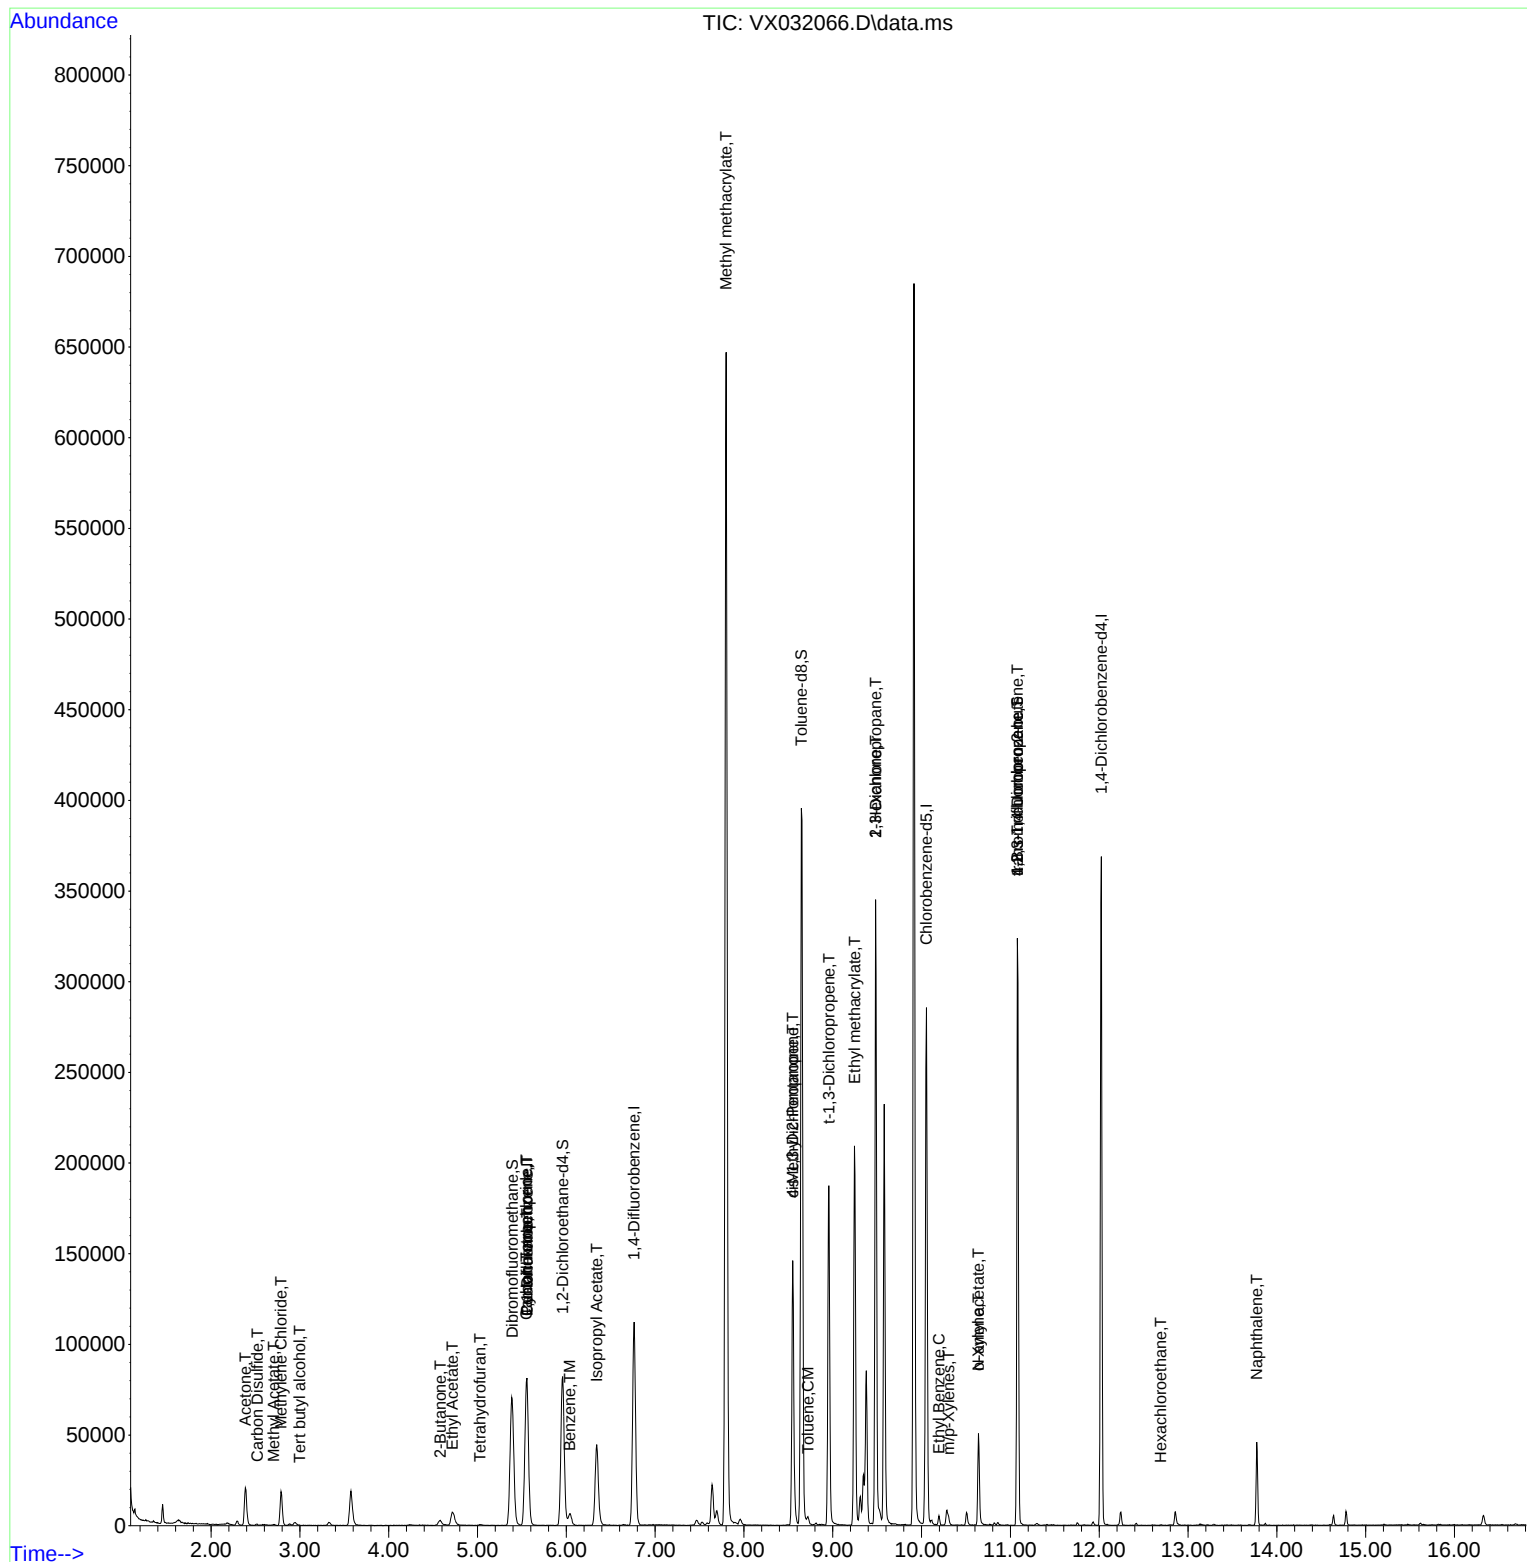


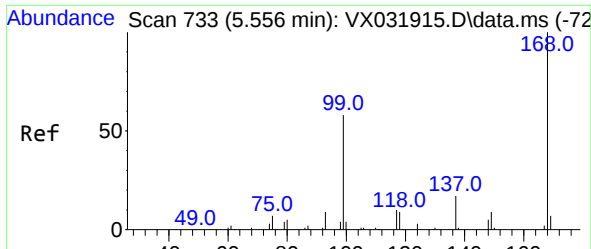

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX032066.D
Acq: 12 Oct 2022 07:01




Instrument :
MSVOA_X
ClientSampleId :
B5(20-21)


Tgt Ion:168 Resp: 73671
Ion Ratio Lower Upper
168 100
99 62.4 48.8 73.2

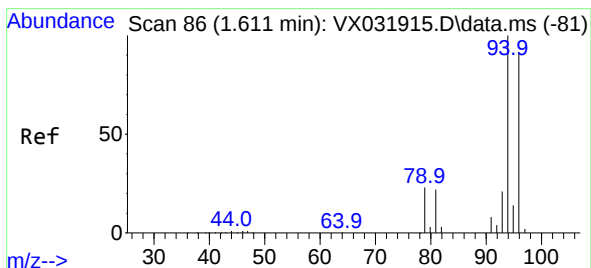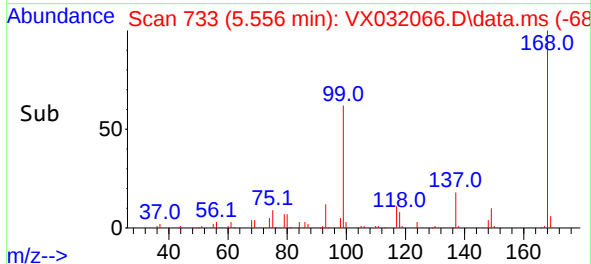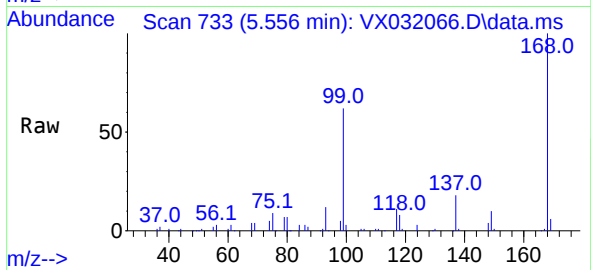

#5
Bromomethane
Concen: Below Cal
RT: 1.611 min Scan# 86
Delta R.T. 0.000 min
Lab File: VX032066.D
Acq: 12 Oct 2022 07:01

Tgt Ion: 94 Resp: 213
Ion Ratio Lower Upper
94 100
96 74.3 74.4 111.6#

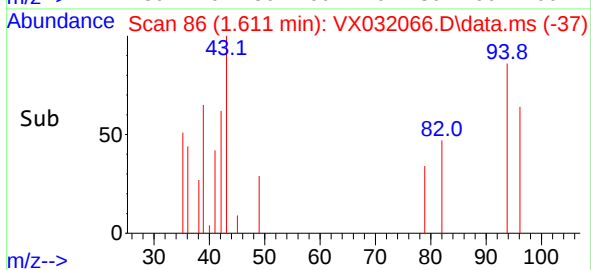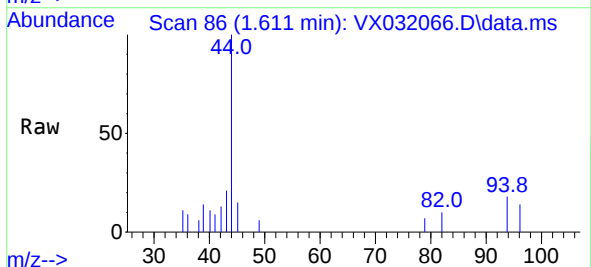



#11

Tert butyl alcohol

Concen: 0.692 ug/l

RT: 2.995 min Scan# 31

Delta R.T. -0.012 min

Lab File: VX032066.D

Acq: 12 Oct 2022 07:01

Instrument :

MSVOA_X

ClientSampleId :





B5(20-21)

Tgt Ion: 59 Resp: 131

Ion Ratio Lower Upper

59 100

57 0.0 8.2 12.2#

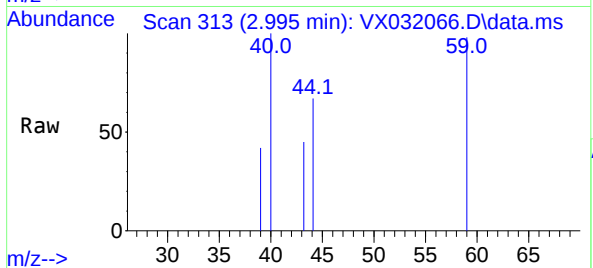

#13

Acrolein

Concen: Below Cal

RT: 2.239 min Scan# 189

Delta R.T. 0.000 min

Lab File: VX032066.D




Acq: 12 Oct 2022 07:01


Tgt Ion: 56 Resp: 168

Ion Ratio Lower Upper

56 100

55 64.3 56.0 84.0


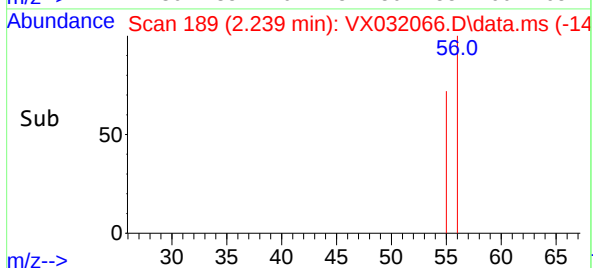
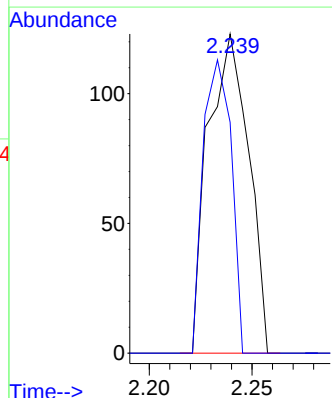





#16
Acetone
Concen: 47.748 ug/l
RT: 2.386 min Scan# 214
Delta R.T. -0.006 min
Lab File: VX032066.D
Acq: 12 Oct 2022 07:01




Instrument :
MSVOA_X
ClientSampleId :
B5(20-21)


Tgt Ion: 43 Resp: 24690
Ion Ratio Lower Upper
43 100
58 28.0 23.8 35.8

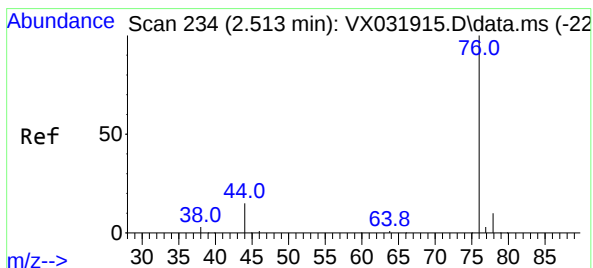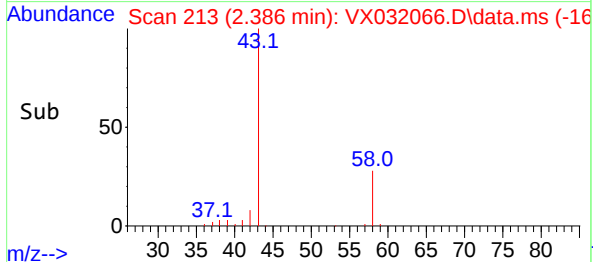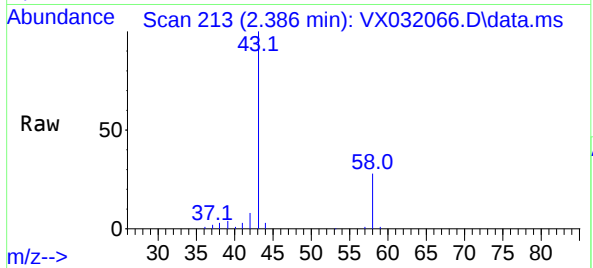

#17
Carbon Disulfide
Concen: 0.391 ug/l
RT: 2.520 min Scan# 235
Delta R.T. 0.007 min
Lab File: VX032066.D
Acq: 12 Oct 2022 07:01

Tgt Ion: 76 Resp: 943
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#


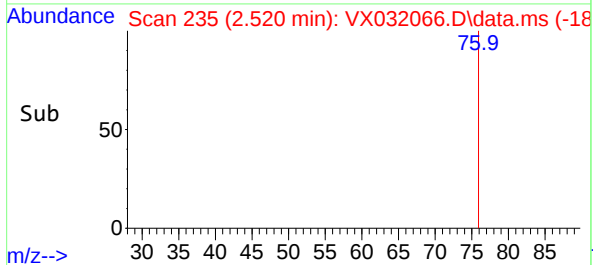

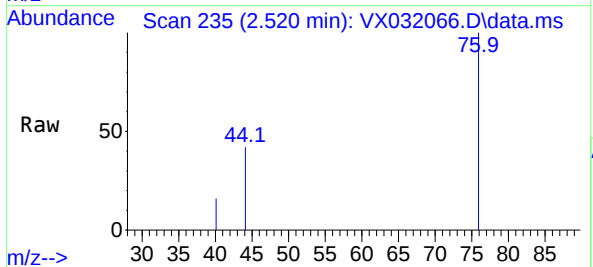




#18
Methyl Acetate
Concen: 0.477 ug/l
RT: 2.703 min Scan# 206
Delta R.T. -0.006 min
Lab File: VX032066.D
Acq: 12 Oct 2022 07:01




Instrument :
MSVOA_X
ClientSampleId :
B5(20-21)


Tgt Ion: 43 Resp: 813
Ion Ratio Lower Upper
43 100
74 7.3 18.6 27.8#

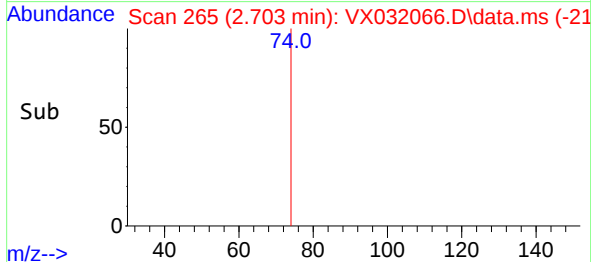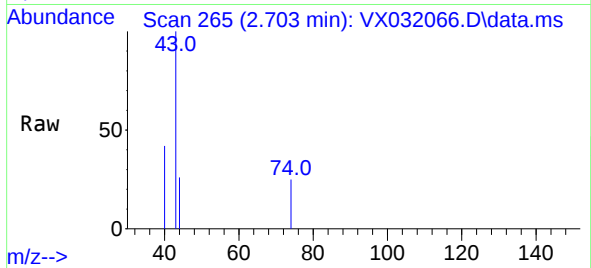

#20
Methylene Chloride
Concen: 5.996 ug/l
RT: 2.788 min Scan# 279
Delta R.T. -0.000 min
Lab File: VX032066.D
Acq: 12 Oct 2022 07:01

Tgt Ion: 84 Resp: 8148
Ion Ratio Lower Upper
84 100
49 120.1 105.9 158.9
51 38.4 32.2 48.2
86 63.6 50.8 76.2


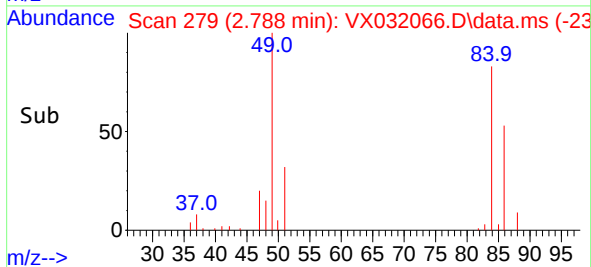

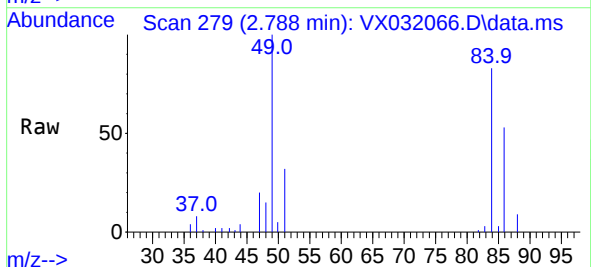




#25
2-Butanone
Concen: 4.516 ug/l
RT: 4.580 min Scan# 51
Delta R.T. 0.018 min
Lab File: VX032066.D
Acq: 12 Oct 2022 07:01




Instrument :
MSVOA_X
ClientSampleId :
B5(20-21)


Tgt Ion: 43 Resp: 3650
Ion Ratio Lower Upper
43 100
72 30.7 21.1 31.7

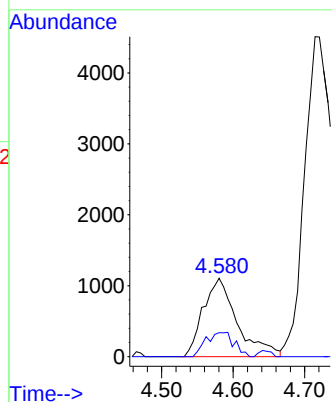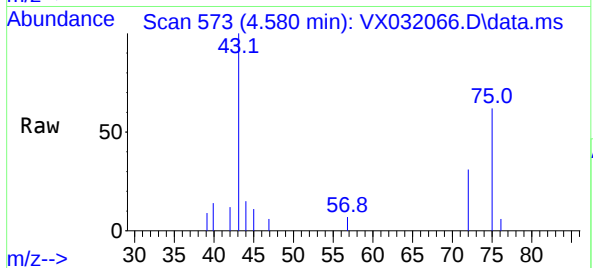

#29
Tetrahydrofuran
Concen: 0.690 ug/l
RT: 5.025 min Scan# 646
Delta R.T. 0.012 min
Lab File: VX032066.D
Acq: 12 Oct 2022 07:01


Tgt Ion: 42 Resp: 360
Ion Ratio Lower Upper
42 100
72 0.0 36.4 54.6#
71 14.2 33.5 50.3#

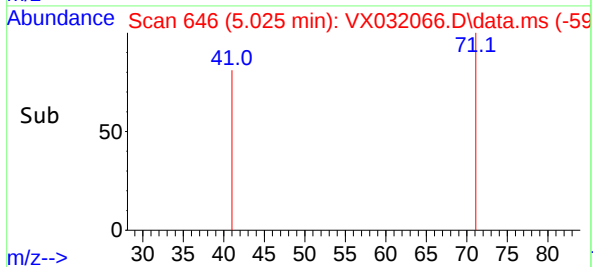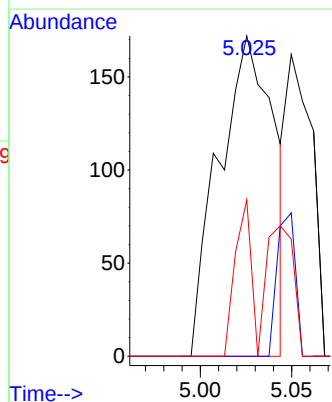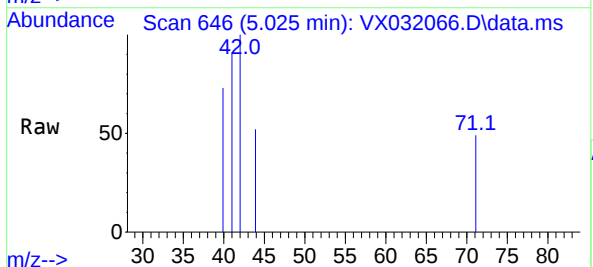






#31
Cyclohexane
Concen: 0.945 ug/l
RT: 5.556 min Scan# 719
Delta R.T. 0.086 min
Lab File: VX032066.D
Acq: 12 Oct 2022 07:01

Instrument :
MSVOA_X
ClientSampleId :
B5(20-21)



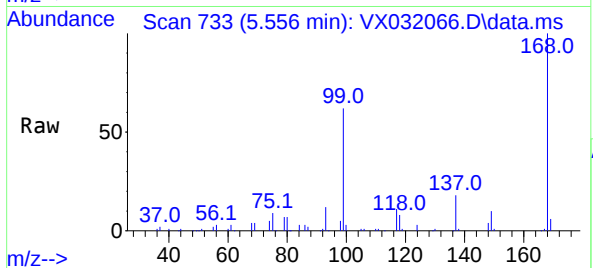



Tgt Ion: 56 Resp: 1717
Ion Ratio Lower Upper
56 100
69 124.8 25.1 37.7#
84 88.9 70.2 105.4



#33
1,2-Dichloroethane-d4
Concen: 52.311 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX032066.D
Acq: 12 Oct 2022 07:01

Tgt Ion: 65 Resp: 79589
Ion Ratio Lower Upper
65 100
67 50.2 0.0 102.4


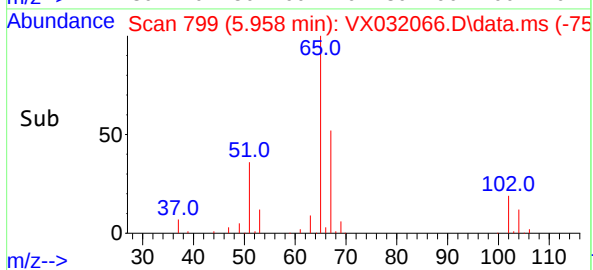






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX032066.D
Acq: 12 Oct 2022 07:01




Instrument :
MSVOA_X
ClientSampleId :
B5(20-21)


Tgt Ion:114 Resp: 111934
Ion Ratio Lower Upper
114 100
63 20.1 0.0 42.6
88 16.3 0.0 33.0

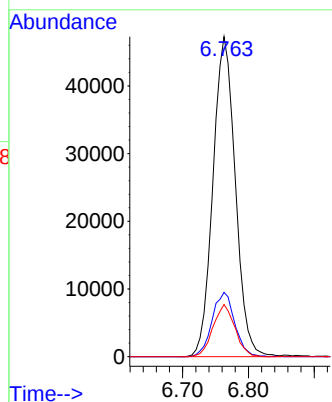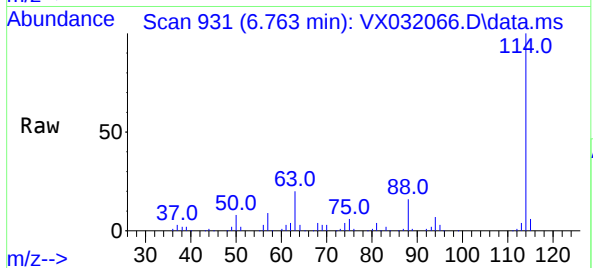

#35
Dibromofluoromethane
Concen: 47.510 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.006 min
Lab File: VX032066.D
Acq: 12 Oct 2022 07:01

Tgt Ion:113 Resp: 60197
Ion Ratio Lower Upper
113 100
111 103.4 82.4 123.6
192 18.7 14.1 21.1

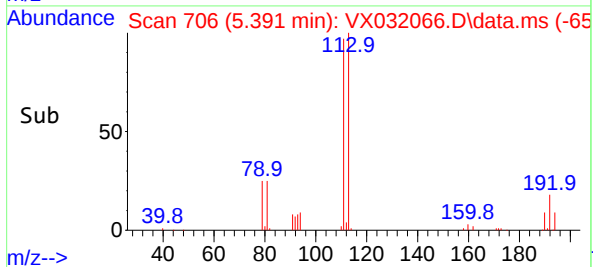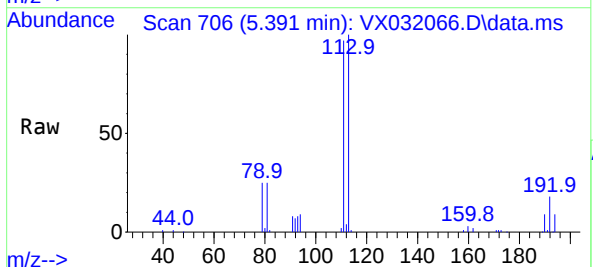



#36

1,1-Dichloropropene

Concen: 3.599 ug/l

RT: 5.556 min Scan# 71

Delta R.T. -0.134 min

Lab File: VX032066.D

Acq: 12 Oct 2022 07:01

Instrument :

MSVOA_X

ClientSampleId :

B5(20-21)





Tgt Ion: 75 Resp: 6046

Ion Ratio Lower Upper

75 100

110 9.6 17.5 52.5#

77 0.0 24.9 37.3#

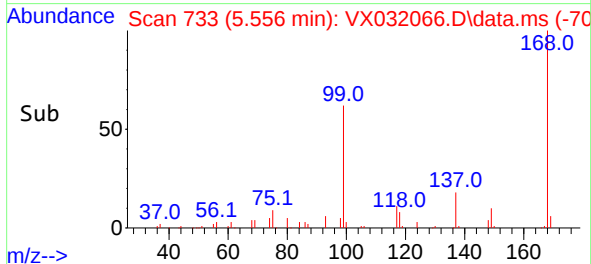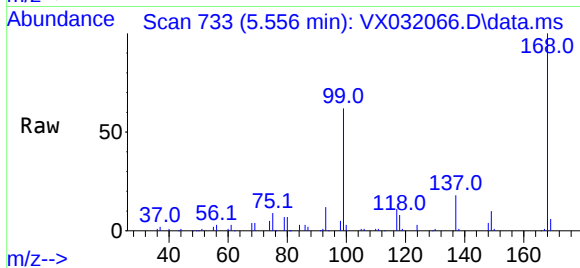

#37

Ethyl Acetate

Concen: 8.818 ug/l

RT: 4.714 min Scan# 595

Delta R.T. 0.000 min

Lab File: VX032066.D

Acq: 12 Oct 2022 07:01




Tgt Ion: 43 Resp: 13948


Ion Ratio Lower Upper

43 100

61 6.4 11.1 16.7#


70 5.6 8.6 13.0#

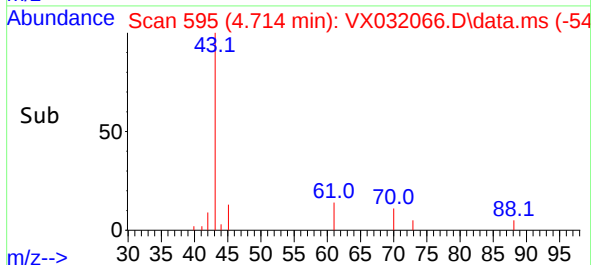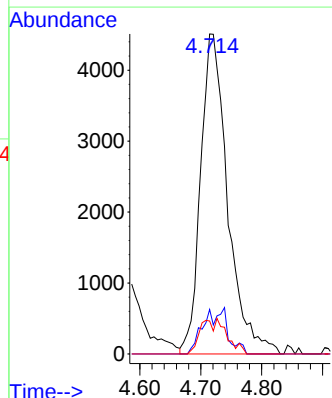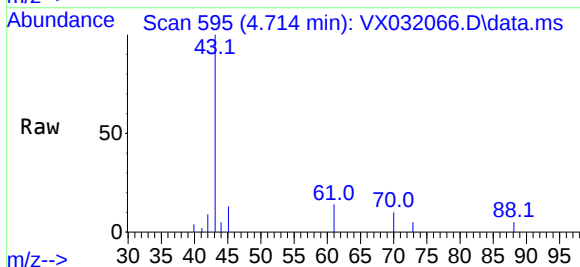






#38
Carbon Tetrachloride
Concen: 4.647 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.127 min
Lab File: VX032066.D
Acq: 12 Oct 2022 07:01

Instrument :
MSVOA_X
ClientSampleId :
B5(20-21)



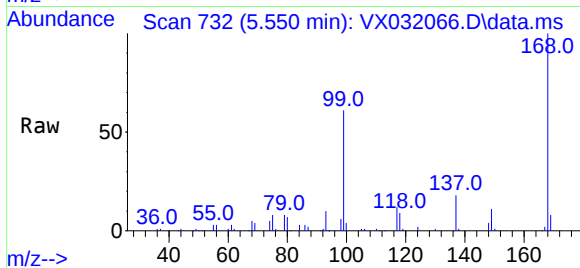



Tgt Ion:117 Resp: 7983
Ion Ratio Lower Upper
117 100
119 6.4 74.6 112.0#
121 0.0 25.3 37.9#

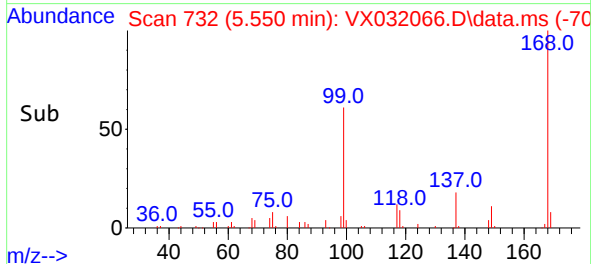

#40
Benzene
Concen: 1.479 ug/l
RT: 6.037 min Scan# 812
Delta R.T. 0.000 min
Lab File: VX032066.D
Acq: 12 Oct 2022 07:01

Tgt Ion: 78 Resp: 7276
Ion Ratio Lower Upper
78 100
77 24.5 18.7 28.1


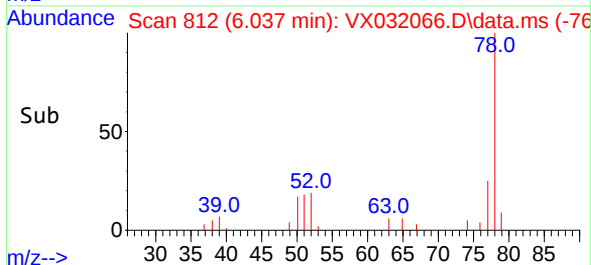
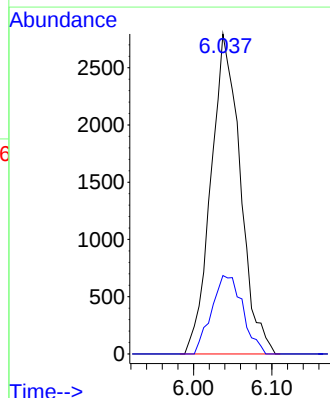
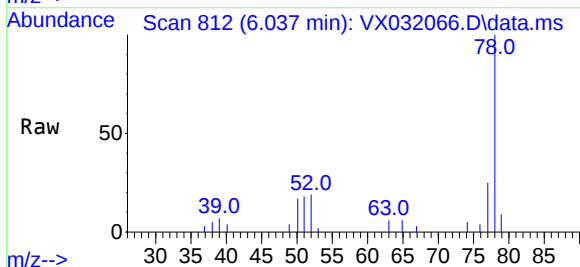




#43
Isopropyl Acetate
Concen: 24.629 ug/l
RT: 6.342 min Scan# 81
Delta R.T. 0.000 min
Lab File: VX032066.D
Acq: 12 Oct 2022 07:01




Instrument :
MSVOA_X
ClientSampleId :
B5(20-21)


Tgt Ion: 43 Resp: 59108
Ion Ratio Lower Upper
43 100
61 18.9 15.3 22.9
87 13.2 10.6 15.8

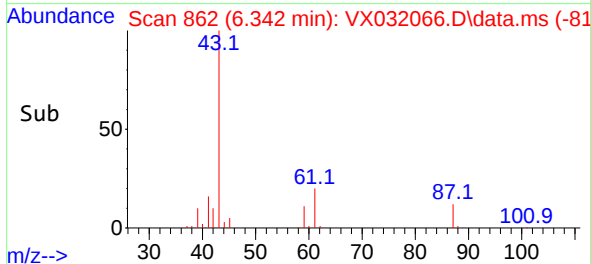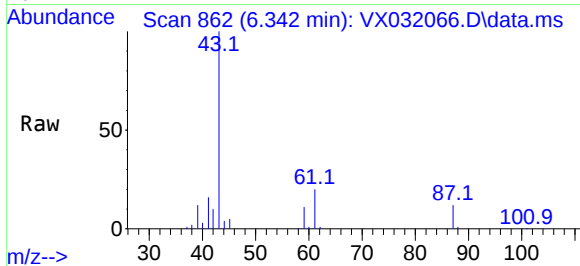

#48
Methyl methacrylate
Concen: 51.204 ug/l
RT: 7.799 min Scan# 1101
Delta R.T. 0.104 min
Lab File: VX032066.D
Acq: 12 Oct 2022 07:01

Tgt Ion: 41 Resp: 58721
Ion Ratio Lower Upper
41 100
69 0.0 64.6 96.8#
39 58.7 51.4 77.0

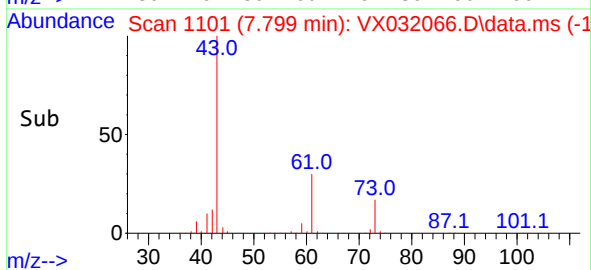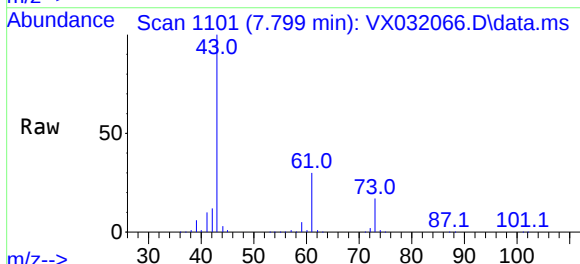



#49

1,4-Dioxane

Concen: Below Cal

RT: 7.799 min Scan# 1101

Delta R.T. 0.104 min

Lab File: VX032066.D

Acq: 12 Oct 2022 07:01

Instrument :

MSVOA_X

ClientSampleId :

B5(20-21)





Tgt Ion: 88 Resp: 46

Ion Ratio Lower Upper

88 100

43 1251358.7 27.1 40.7#

58 5850.0 53.9 80.9#

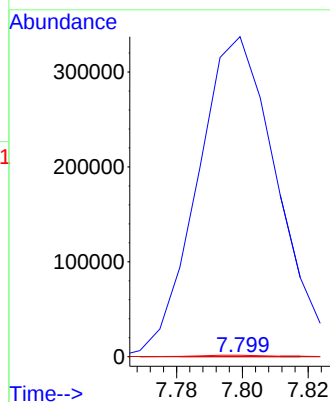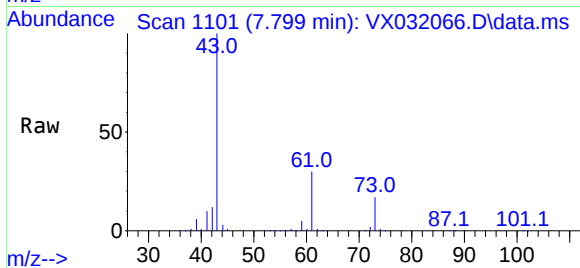

#50

Toluene-d8

Concen: 51.063 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. -0.006 min

Lab File: VX032066.D




Acq: 12 Oct 2022 07:01


Tgt Ion: 98 Resp: 232806

Ion Ratio Lower Upper

98 100

100 66.3 52.5 78.7

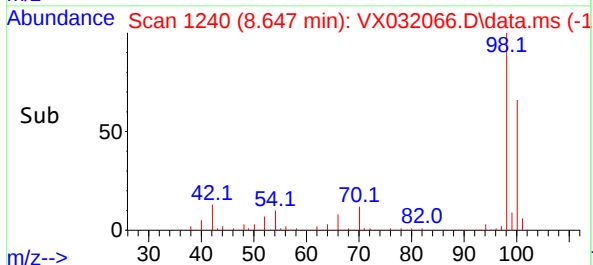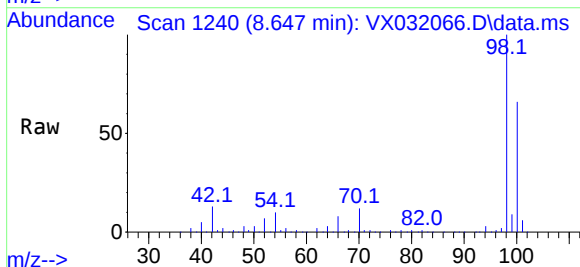



#51

4-Methyl-2-Pentanone

Concen: 31.522 ug/l

RT: 8.549 min Scan# 11

Delta R.T. -0.024 min

Lab File: VX032066.D

Acq: 12 Oct 2022 07:01

Instrument :

MSVOA_X

ClientSampleId :





B5(20-21)

Tgt Ion: 43 Resp: 50132

Ion Ratio Lower Upper

43 100

58 8.2 30.6 46.0#

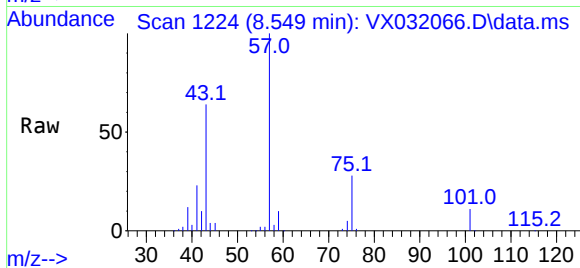

#52

Toluene

Concen: 0.431 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. -0.000 min

Lab File: VX032066.D




Acq: 12 Oct 2022 07:01


Tgt Ion: 92 Resp: 1388

Ion Ratio Lower Upper

92 100

91 183.3 137.1 205.7

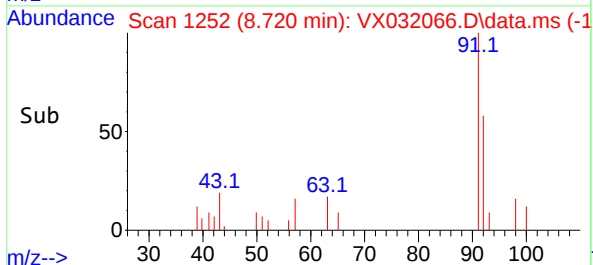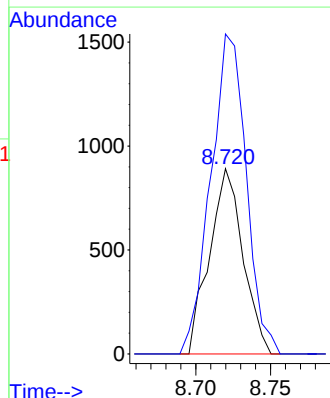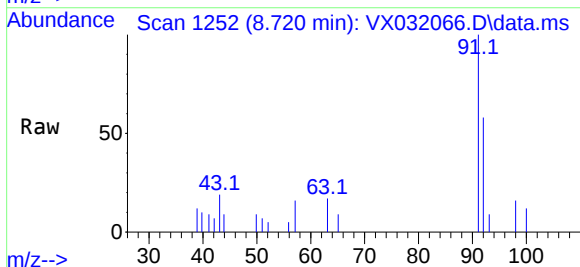



#53

t-1,3-Dichloropropene

Concen: 1.407 ug/l

RT: 8.958 min Scan# 11

Delta R.T. -0.024 min

Lab File: VX032066.D

Acq: 12 Oct 2022 07:01

Instrument :

MSVOA_X

ClientSampleId :





B5(20-21)

Tgt Ion: 75 Resp: 356

Ion Ratio Lower Upper

75 100

77 0.0 24.8 37.2#

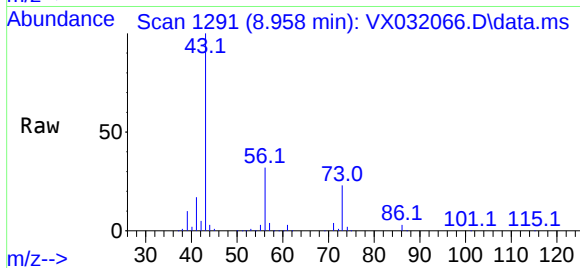

#54

cis-1,3-Dichloropropene

Concen: 12.709 ug/l

RT: 8.549 min Scan# 1224

Delta R.T. 0.183 min

Lab File: VX032066.D

Acq: 12 Oct 2022 07:01




Tgt Ion: 75 Resp: 22279


Ion Ratio Lower Upper

75 100

77 0.0 24.4 36.6#

39 41.8 43.7 65.5#

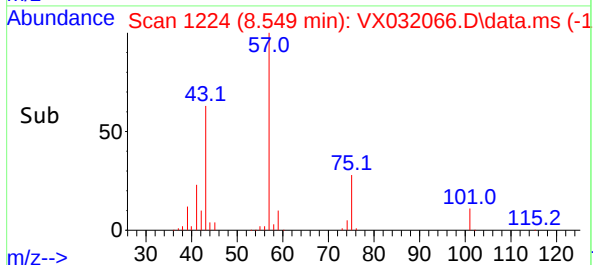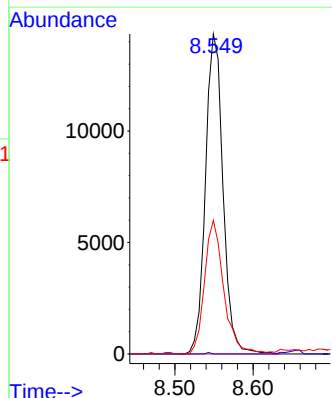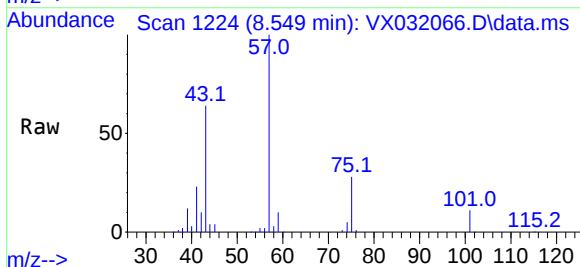



#56

Ethyl methacrylate

Concen: 0.315 ug/l

RT: 9.244 min Scan# 1

Delta R.T. 0.128 min

Lab File: VX032066.D

Acq: 12 Oct 2022 07:01





Instrument :

MSVOA_X

ClientSampleId :

B5(20-21)

Tgt Ion:	69	Resp:	548
Ion	Ratio	Lower	Upper
69	100		
41	6612.2	54.2	81.4#
39	3239.8	34.2	51.2#

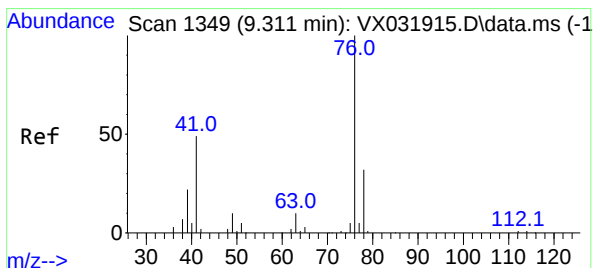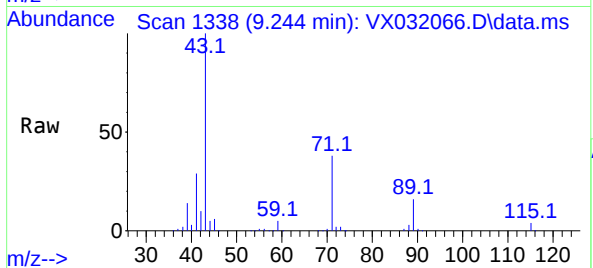

#57

1,3-Dichloropropane

Concen: 1.350 ug/l




RT: 9.482 min Scan# 1377


Delta R.T. 0.171 min

Lab File: VX032066.D

Acq: 12 Oct 2022 07:01

Tgt Ion:	76	Resp:	2945
Ion	Ratio	Lower	Upper
76	100		
78	0.0	25.5	38.3#

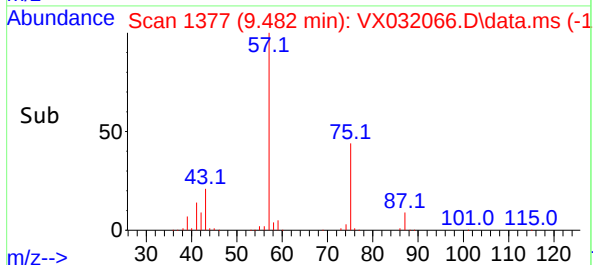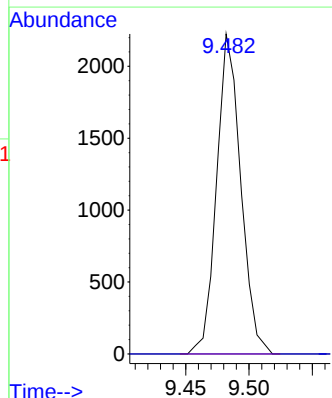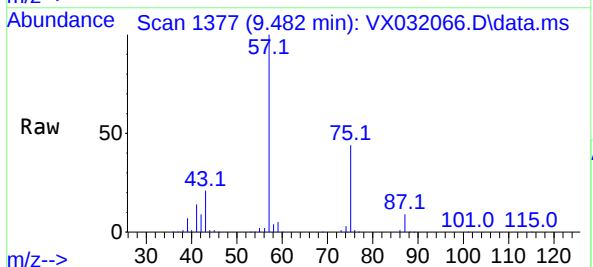



#59

2-Hexanone

Concen: 35.314 ug/l

RT: 9.482 min Scan# 11

Delta R.T. 0.049 min

Lab File: VX032066.D

Acq: 12 Oct 2022 07:01

Instrument :

MSVOA_X

ClientSampleId :





B5(20-21)

Tgt Ion: 43 Resp: 41411

Ion Ratio Lower Upper

43 100

58 18.4 26.7 80.0#

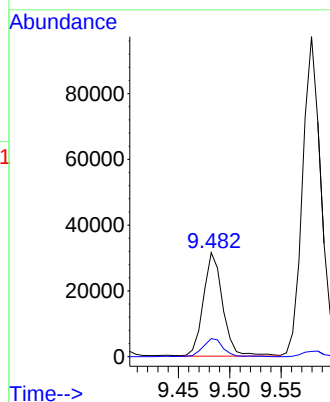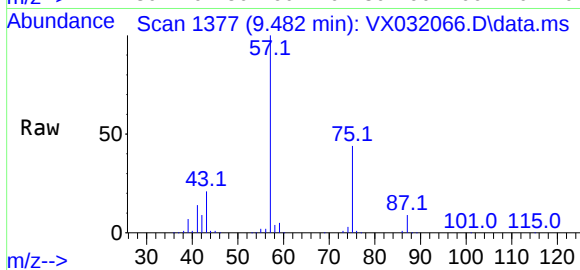

#62

4-Bromofluorobenzene

Concen: 49.013 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX032066.D

Acq: 12 Oct 2022 07:01




Tgt Ion: 95 Resp: 78999


Ion Ratio Lower Upper

95 100

174 78.0 0.0 153.2

176 73.9 0.0 144.0


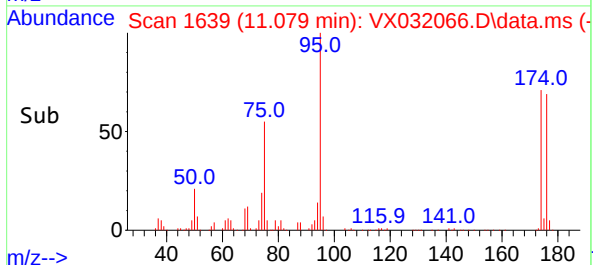

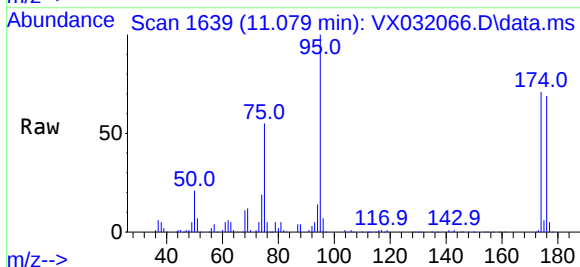




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX032066.D
Acq: 12 Oct 2022 07:01




Instrument :
MSVOA_X
ClientSampleId :
B5(20-21)


Tgt Ion:117 Resp: 121106
Ion Ratio Lower Upper
117 100
82 55.7 46.8 70.2
119 32.8 26.4 39.6

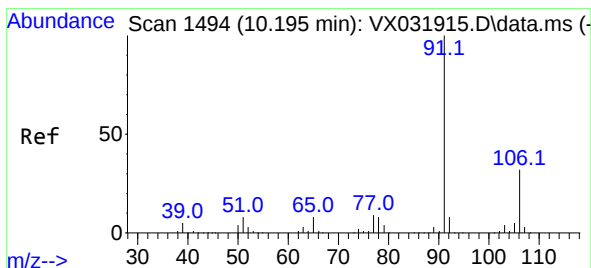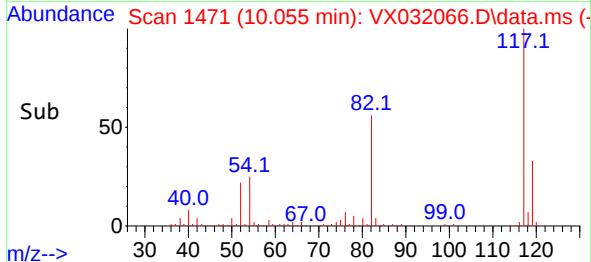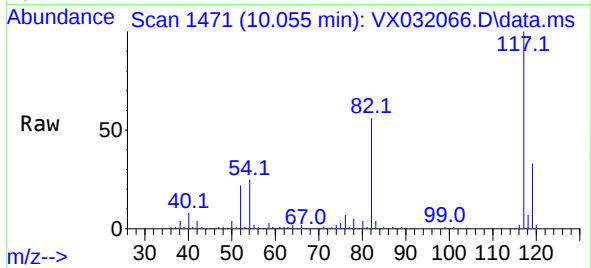

#67
Ethyl Benzene
Concen: 0.429 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX032066.D
Acq: 12 Oct 2022 07:01

Tgt Ion: 91 Resp: 2662
Ion Ratio Lower Upper
91 100
106 29.8 25.2 37.8


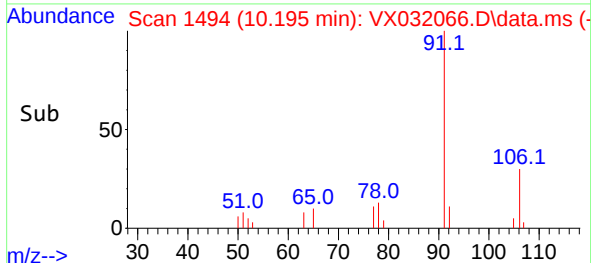
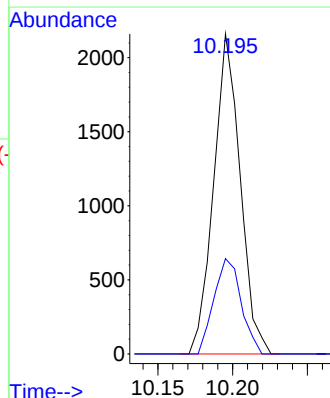
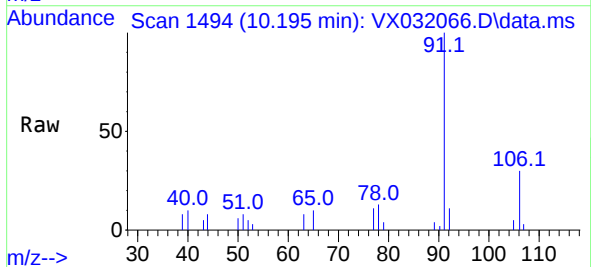




#68
m/p-Xylenes
Concen: 0.383 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX032066.D
Acq: 12 Oct 2022 07:01




Instrument :
MSVOA_X
ClientSampleId :
B5(20-21)


Tgt Ion:106 Resp: 945
Ion Ratio Lower Upper
106 100
91 205.7 161.0 241.4

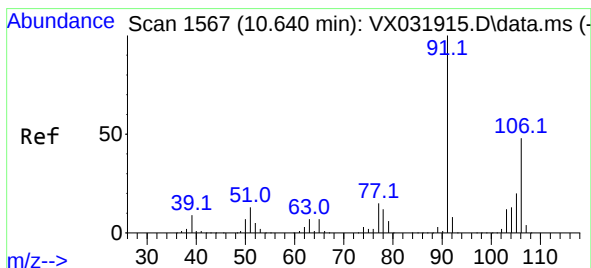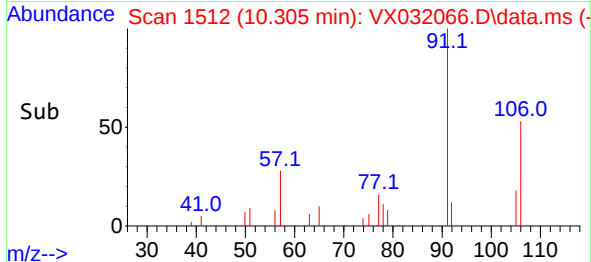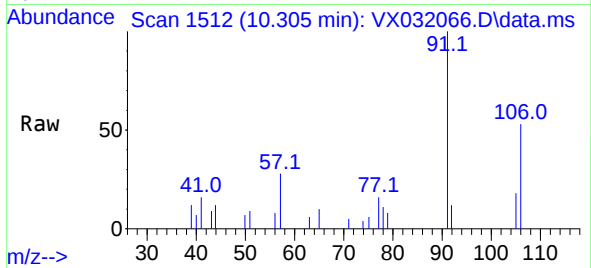

#69
o-Xylene
Concen: 0.265 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. 0.000 min
Lab File: VX032066.D
Acq: 12 Oct 2022 07:01


Tgt Ion:106 Resp: 635
Ion Ratio Lower Upper
106 100
91 240.5 107.2 321.6

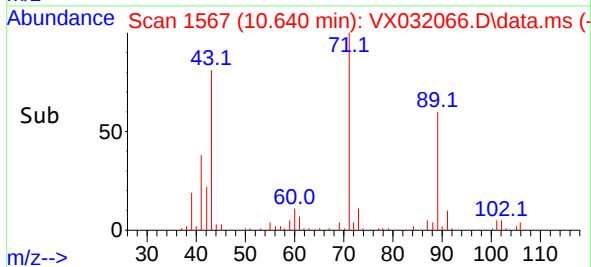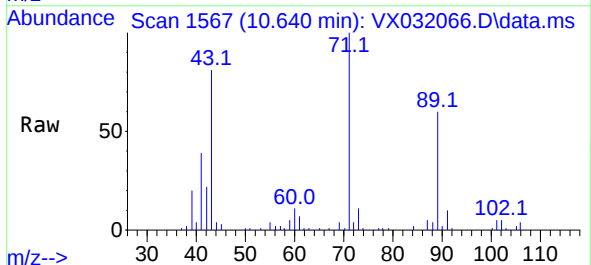






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX032066.D
Acq: 12 Oct 2022 07:01


Instrument :
MSVOA_X
ClientSampleId :
B5(20-21)

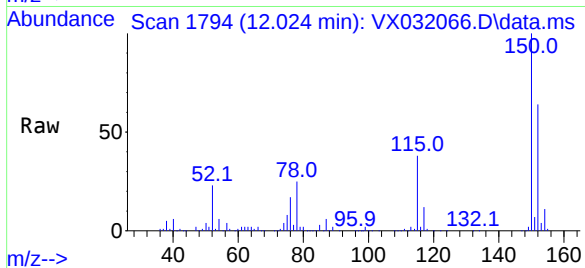



Tgt Ion:152 Resp: 72434
Ion Ratio Lower Upper
152 100
115 61.1 43.4 130.1
150 155.6 0.0 346.8

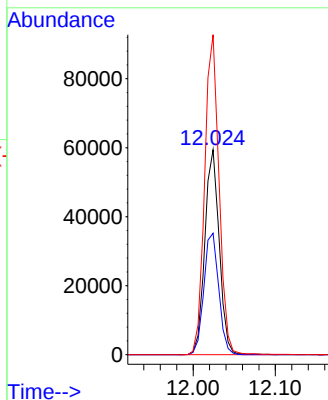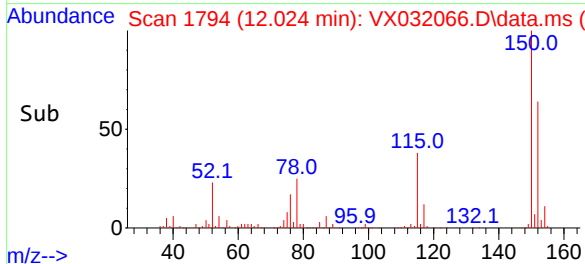


#74
N-ethyl acetate
Concen: 7.639 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.207 min
Lab File: VX032066.D
Acq: 12 Oct 2022 07:01

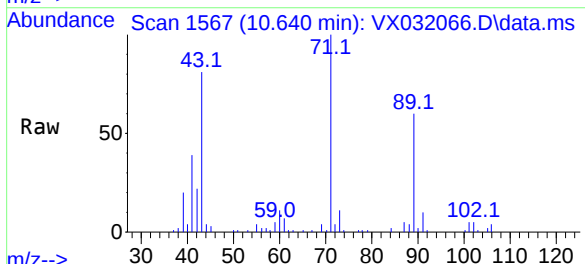

Tgt Ion: 43 Resp: 12744
Ion Ratio Lower Upper
43 100
70 1.8 33.4 50.2#
55 5.1 18.2 27.2#
61 8.8 19.3 28.9#



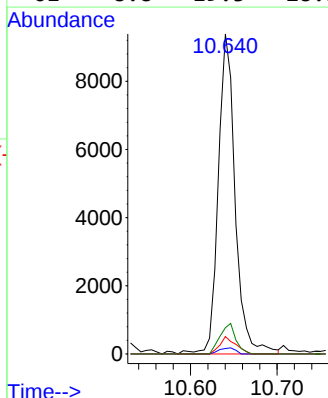
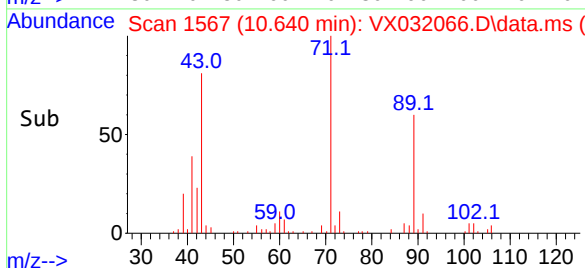




#76
1,2,3-Trichloropropane
Concen: 30.251 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.158 min
Lab File: VX032066.D
Acq: 12 Oct 2022 07:01




Instrument :
MSVOA_X
ClientSampleId :
B5(20-21)


Tgt Ion: 75 Resp: 44909
Ion Ratio Lower Upper
75 100
77 1.1 20.3 60.9#

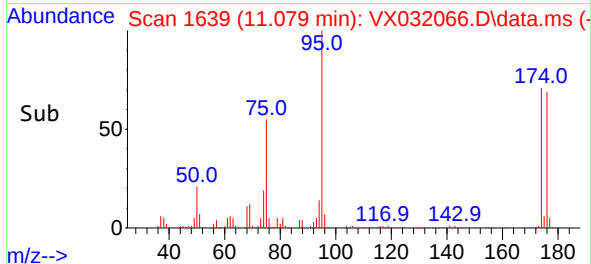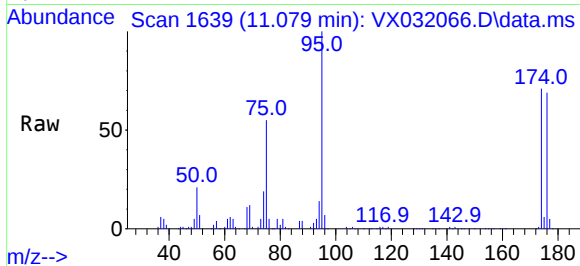

#81
trans-1,4-Dichloro-2-butene
Concen: 103.225 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX032066.D
Acq: 12 Oct 2022 07:01

Tgt Ion: 75 Resp: 44909
Ion Ratio Lower Upper
75 100
53 0.0 77.6 116.4#
89 0.1 37.4 56.0#


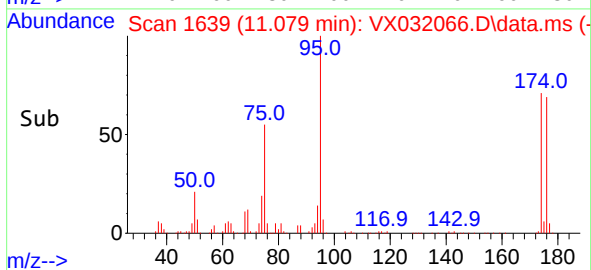

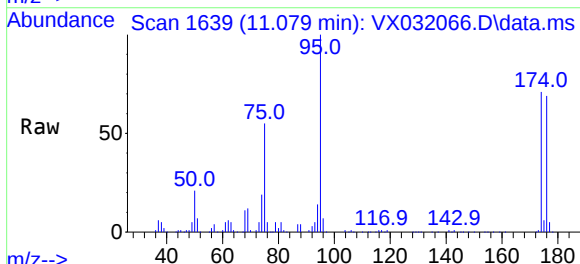




#90
Hexachloroethane
Concen: 1.553 ug/l
RT: 12.695 min Scan# 1904
Delta R.T. 0.153 min
Lab File: VX032066.D
Acq: 12 Oct 2022 07:01

Instrument :
MSVOA_X
ClientSampleId :
B5(20-21)

Tgt Ion:117 Resp: 187
Ion Ratio Lower Upper
117 100
201 0.0 34.8 104.4#

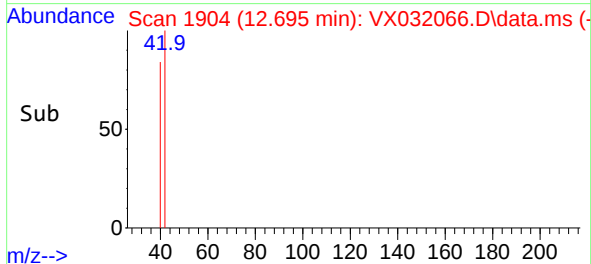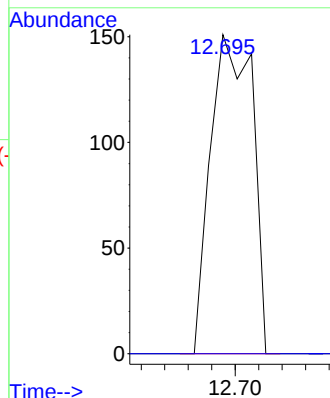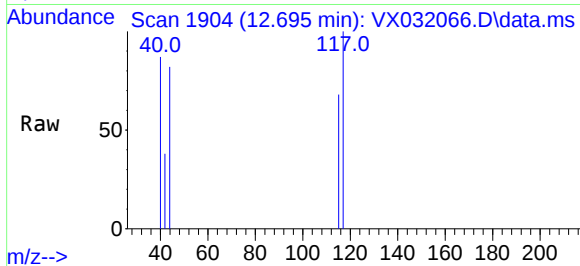

#95
Naphthalene
Concen: 5.162 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.006 min
Lab File: VX032066.D
Acq: 12 Oct 2022 07:01

Tgt Ion:128 Resp: 27350
Ion Ratio Lower Upper
128 100
127 12.7 10.4 15.6
129 11.9 8.8 13.2

