

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX101122\  
 Data File : VX032068.D  
 Acq On : 12 Oct 2022 07:47  
 Operator : JC/MD  
 Sample : N5066-10  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 45 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 B-4(12-13)


Quant Time: Oct 12 13:26:45 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X100622W.M  
 Quant Title : SW846 8260  
 QLast Update : Thu Oct 06 14:28:46 2022  
 Response via : Initial Calibration

| Compound                      | R.T.           | QIon | Response            | Conc      | Units  | Dev(Min) |
|-------------------------------|----------------|------|---------------------|-----------|--------|----------|
| -----                         |                |      |                     |           |        |          |
| Internal Standards            |                |      |                     |           |        |          |
| 1) Pentafluorobenzene         | 5.550          | 168  | 76696               | 50.000    | ug/l   | 0.00     |
| 34) 1,4-Difluorobenzene       | 6.763          | 114  | 116650              | 50.000    | ug/l   | 0.00     |
| 63) Chlorobenzene-d5          | 10.055         | 117  | 128250              | 50.000    | ug/l   | 0.00     |
| 72) 1,4-Dichlorobenzene-d4    | 12.024         | 152  | 74642               | 50.000    | ug/l   | 0.00     |
|                               |                |      |                     |           |        |          |
| System Monitoring Compounds   |                |      |                     |           |        |          |
| 33) 1,2-Dichloroethane-d4     | 5.958          | 65   | 83479               | 52.704    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 74 - 125 |      | Recovery = 105.400% |           |        |          |
| 35) Dibromofluoromethane      | 5.385          | 113  | 62471               | 47.312    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 75 - 124 |      | Recovery = 94.620%  |           |        |          |
| 50) Toluene-d8                | 8.647          | 98   | 245852              | 51.744    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 86 - 113 |      | Recovery = 103.480% |           |        |          |
| 62) 4-Bromofluorobenzene      | 11.079         | 95   | 83629               | 49.788    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 83 - 123 |      | Recovery = 99.580%  |           |        |          |
|                               |                |      |                     |           |        |          |
| Target Compounds              |                |      |                     |           | Qvalue |          |
| 5) Bromomethane               | 1.618          | 94   | 272                 | Below Cal | #      | 79       |
| 16) Acetone                   | 2.386          | 43   | 22026               | 40.916    | ug/l   | 99       |
| 17) Carbon Disulfide          | 2.514          | 76   | 2878                | 1.147     | ug/l   | 100      |
| 18) Methyl Acetate            | 2.697          | 43   | 728                 | 0.410     | ug/l   | # 77     |
| 20) Methylene Chloride        | 2.788          | 84   | 7420                | 5.245     | ug/l   | # 85     |
| 25) 2-Butanone                | 4.587          | 43   | 3229                | 3.837     | ug/l   | 93       |
| 29) Tetrahydrofuran           | 5.032          | 42   | 403                 | 0.742     | ug/l   | # 61     |
| 31) Cyclohexane               | 5.550          | 56   | 1839                | 0.972     | ug/l   | # 36     |
| 36) 1,1-Dichloropropene       | 5.550          | 75   | 6734                | 3.846     | ug/l   | # 49     |
| 37) Ethyl Acetate             | 4.721          | 43   | 12545               | 7.610     | ug/l   | 98       |
| 38) Carbon Tetrachloride      | 5.556          | 117  | 8392                | 4.687     | ug/l   | # 17     |
| 40) Benzene                   | 6.038          | 78   | 1402                | 0.273     | ug/l   | # 90     |
| 43) Isopropyl Acetate         | 6.342          | 43   | 59064               | 23.616    | ug/l   | 98       |
| 48) Methyl methacrylate       | 7.799          | 41   | 57571               | 48.172    | ug/l   | # 46     |
| 49) 1,4-Dioxane               | 7.806          | 88   | 100                 | Below Cal | #      | 1        |
| 51) 4-Methyl-2-Pentanone      | 8.549          | 43   | 49243               | 29.711    | ug/l   | # 50     |
| 53) t-1,3-Dichloropropene     | 8.952          | 75   | 424                 | 1.435     | ug/l   | # 44     |
| 54) cis-1,3-Dichloropropene   | 8.549          | 75   | 21859               | 11.965    | ug/l   | # 67     |
| 56) Ethyl methacrylate        | 9.250          | 69   | 508                 | 0.280     | ug/l   | # 1      |
| 57) 1,3-Dichloropropane       | 9.482          | 76   | 2761                | 1.214     | ug/l   | # 43     |
| 59) 2-Hexanone                | 9.482          | 43   | 39349               | 32.199    | ug/l   | # 52     |
| 74) N-amyl acetate            | 10.823         | 43   | 740                 | 0.430     | ug/l   | # 45     |
| 76) 1,2,3-Trichloropropane    | 11.079         | 75   | 46946               | 30.688    | ug/l   | # 37     |
| 81) trans-1,4-Dichloro-2-b... | 11.079         | 75   | 46946               | 104.663   | ug/l   | # 11     |
| 95) Naphthalene               | 13.780         | 128  | 1165                | 0.213     | ug/l   | 97       |
| -----                         |                |      |                     |           |        |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Oct 12 13:26:45 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X100622W.M  
Quant Title : SW846 8260  
QLast Update : Thu Oct 06 14:28:46 2022  
Response via : Initial Calibration







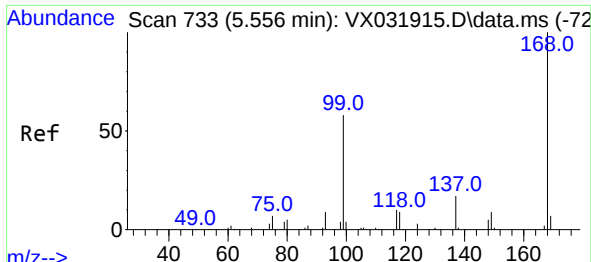

#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.550 min Scan# 71  
Delta R.T. -0.006 min  
Lab File: VX032068.D  
Acq: 12 Oct 2022 07:47




Instrument :  
MSVOA\_X  
ClientSampleId :  
B-4(12-13)


Tgt Ion:168 Resp: 76696  
Ion Ratio Lower Upper  
168 100  
99 62.2 48.8 73.2

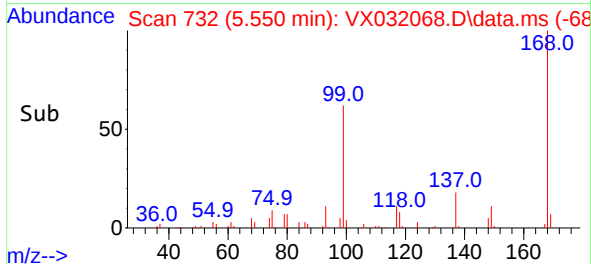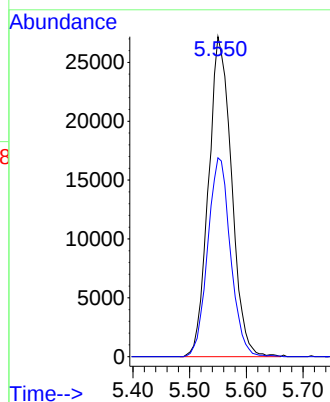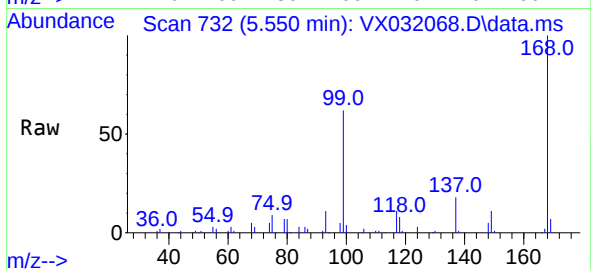

#5  
Bromomethane  
Concen: Below Cal  
RT: 1.618 min Scan# 87  
Delta R.T. 0.007 min  
Lab File: VX032068.D  
Acq: 12 Oct 2022 07:47

Tgt Ion: 94 Resp: 272  
Ion Ratio Lower Upper  
94 100  
96 113.1 74.4 111.6#

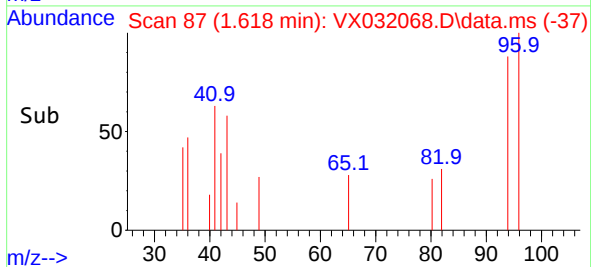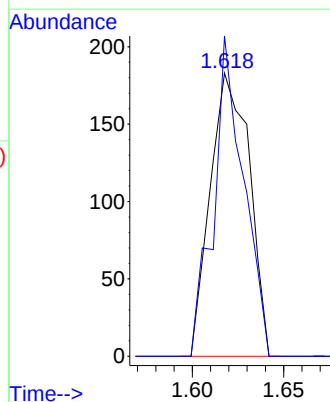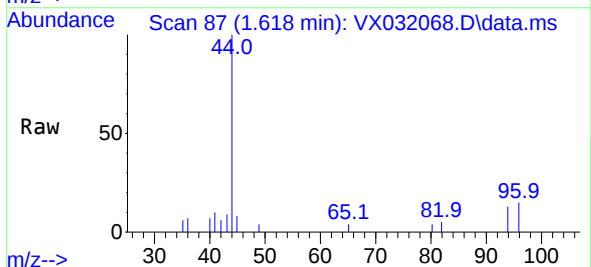



#16

Acetone

Concen: 40.916 ug/l

RT: 2.386 min Scan# 214

Delta R.T. -0.006 min

Lab File: VX032068.D

Acq: 12 Oct 2022 07:47

Instrument :

MSVOA\_X

ClientSampleId :





B-4(12-13)

Tgt Ion: 43 Resp: 22026

Ion Ratio Lower Upper

43 100

58 30.4 23.8 35.8

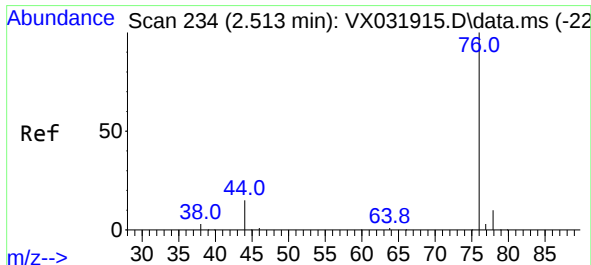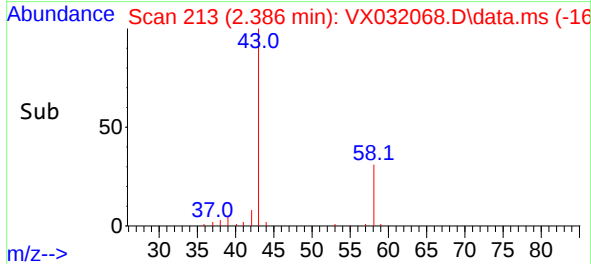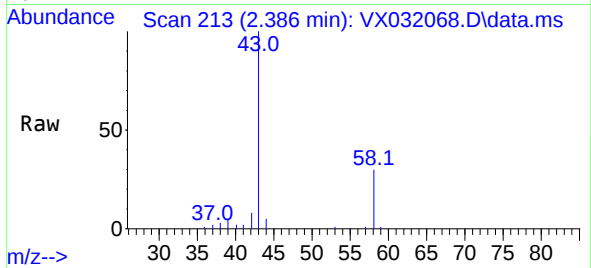

#17

Carbon Disulfide

Concen: 1.147 ug/l

RT: 2.514 min Scan# 234

Delta R.T. 0.001 min

Lab File: VX032068.D




Acq: 12 Oct 2022 07:47


Tgt Ion: 76 Resp: 2878

Ion Ratio Lower Upper

76 100

78 8.9 7.2 10.8

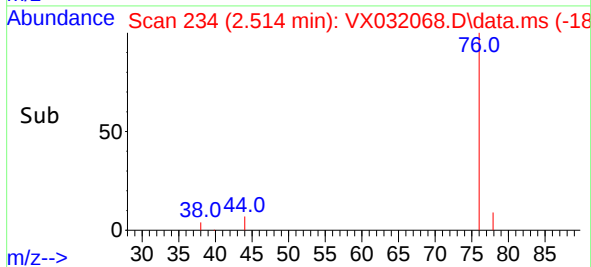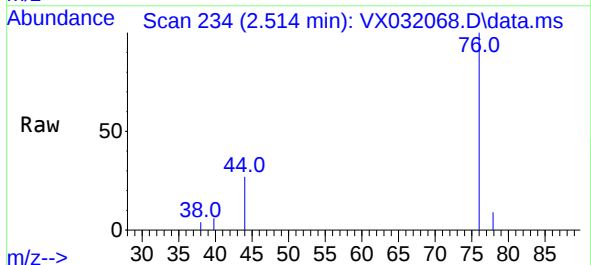



#18

Methyl Acetate

Concen: 0.410 ug/l

RT: 2.697 min Scan# 2

Delta R.T. -0.012 min

Lab File: VX032068.D

Acq: 12 Oct 2022 07:47

Instrument :

MSVOA\_X

ClientSampleId :





B-4(12-13)

Tgt Ion: 43 Resp: 728

Ion Ratio Lower Upper

43 100

74 12.1 18.6 27.8#

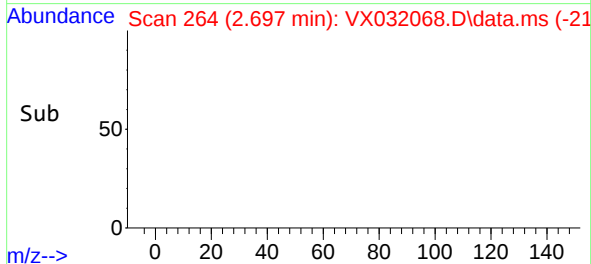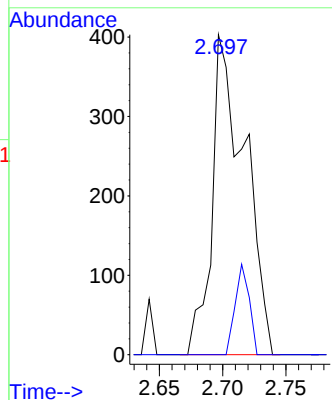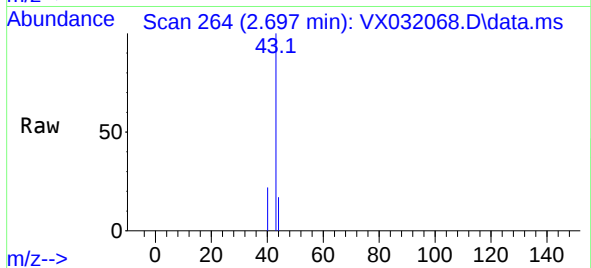

#20

Methylene Chloride

Concen: 5.245 ug/l

RT: 2.788 min Scan# 279

Delta R.T. 0.000 min

Lab File: VX032068.D

Acq: 12 Oct 2022 07:47

Tgt Ion: 84 Resp: 7420




Ion Ratio Lower Upper


84 100

49 105.4 105.9 158.9#

51 35.0 32.2 48.2

86 62.2 50.8 76.2


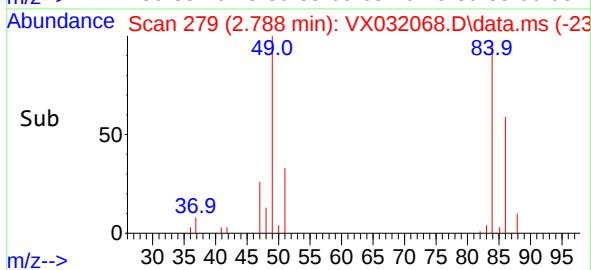
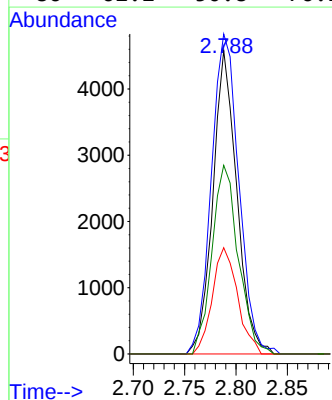
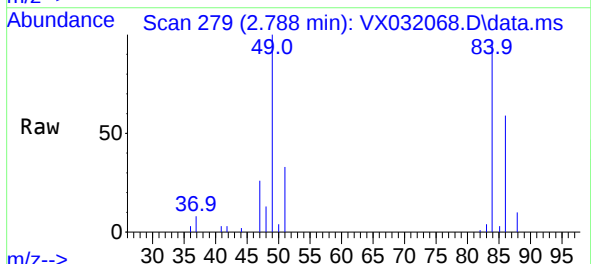




#25  
2-Butanone  
Concen: 3.837 ug/l  
RT: 4.587 min Scan# 51  
Delta R.T. 0.025 min  
Lab File: VX032068.D  
Acq: 12 Oct 2022 07:47




Instrument :  
MSVOA\_X  
ClientSampleId :  
B-4(12-13)


Tgt Ion: 43 Resp: 3229  
Ion Ratio Lower Upper  
43 100  
72 22.6 21.1 31.7

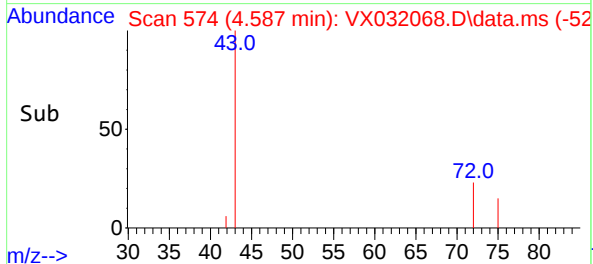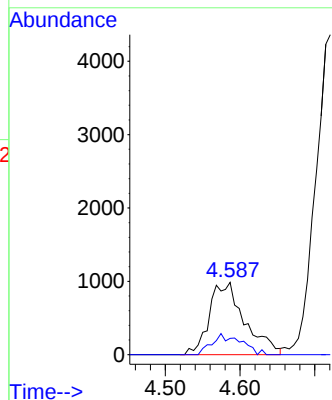

#29  
Tetrahydrofuran  
Concen: 0.742 ug/l  
RT: 5.032 min Scan# 647  
Delta R.T. 0.019 min  
Lab File: VX032068.D  
Acq: 12 Oct 2022 07:47


Tgt Ion: 42 Resp: 403  
Ion Ratio Lower Upper  
42 100  
72 17.1 36.4 54.6#  
71 19.9 33.5 50.3#

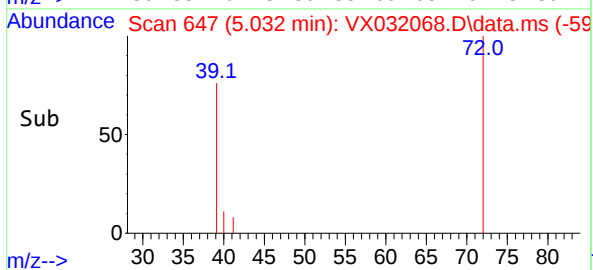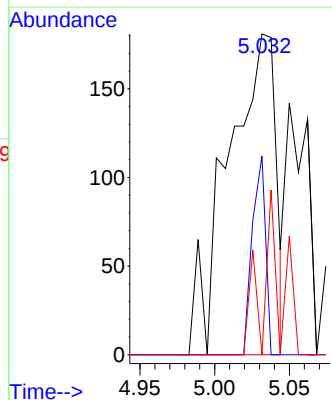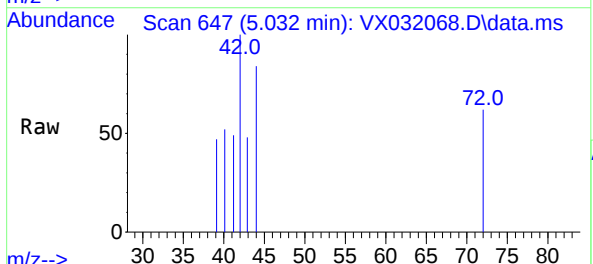



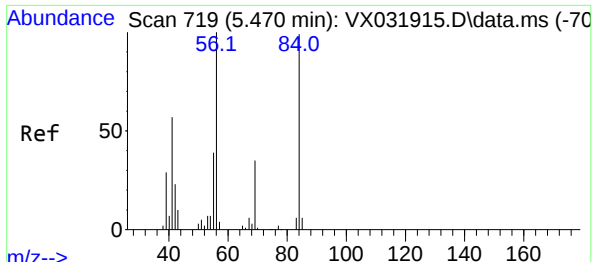


#31  
Cyclohexane  
Concen: 0.972 ug/l  
RT: 5.550 min Scan# 719  
Delta R.T. 0.080 min  
Lab File: VX032068.D  
Acq: 12 Oct 2022 07:47

Instrument :  
MSVOA\_X  
ClientSampleId :  
B-4(12-13)



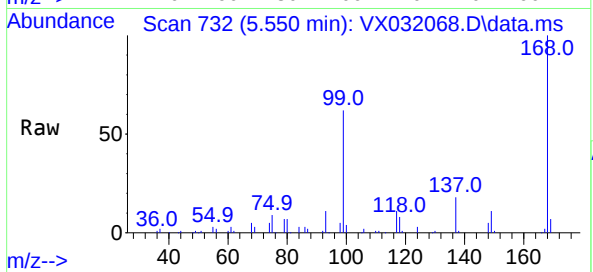



Tgt Ion: 56 Resp: 1839  
Ion Ratio Lower Upper  
56 100  
69 128.0 25.1 37.7#  
84 110.2 70.2 105.4#

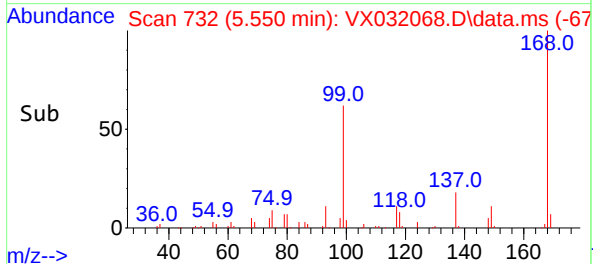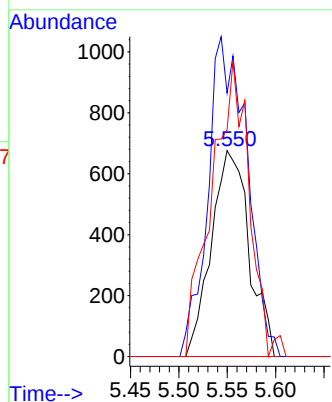

#33  
1,2-Dichloroethane-d4  
Concen: 52.704 ug/l  
RT: 5.958 min Scan# 799  
Delta R.T. 0.000 min  
Lab File: VX032068.D  
Acq: 12 Oct 2022 07:47

Tgt Ion: 65 Resp: 83479  
Ion Ratio Lower Upper  
65 100  
67 51.2 0.0 102.4

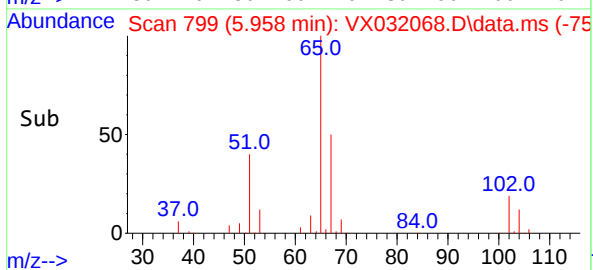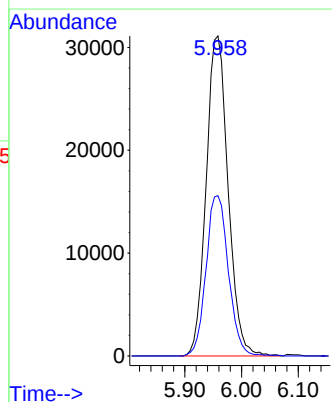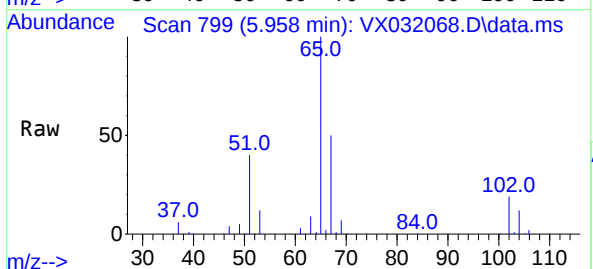




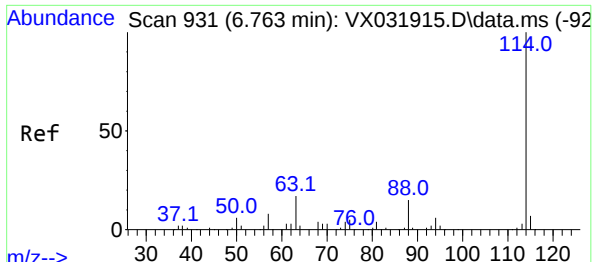


#34  
1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 6.763 min Scan# 91  
Delta R.T. 0.000 min  
Lab File: VX032068.D  
Acq: 12 Oct 2022 07:47

Instrument :  
MSVOA\_X  
ClientSampleId :  
B-4(12-13)

Tgt Ion:114 Resp: 116650




| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 114 | 100   |       |       |
| 63  | 19.8  | 0.0   | 42.6  |
| 88  | 17.4  | 0.0   | 33.0  |

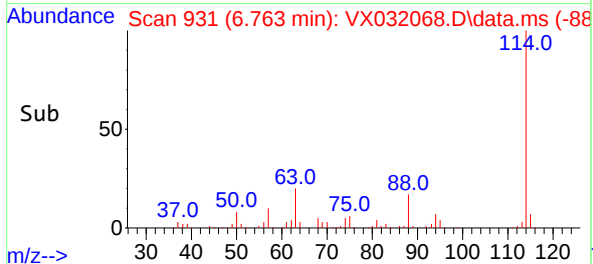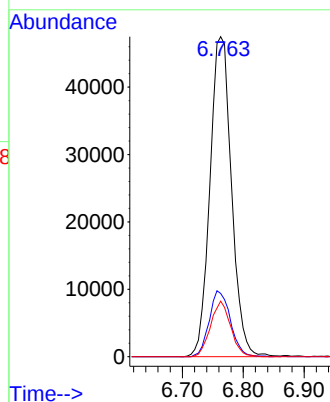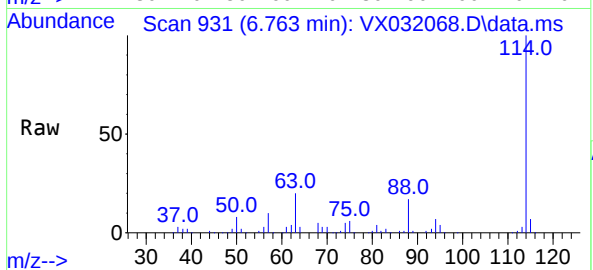


#35  
Dibromofluoromethane  
Concen: 47.312 ug/l  
RT: 5.385 min Scan# 705  
Delta R.T. 0.000 min  
Lab File: VX032068.D  
Acq: 12 Oct 2022 07:47

Tgt Ion:113 Resp: 62471

| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 113 | 100   |       |       |
| 111 | 103.7 | 82.4  | 123.6 |
| 192 | 18.2  | 14.1  | 21.1  |

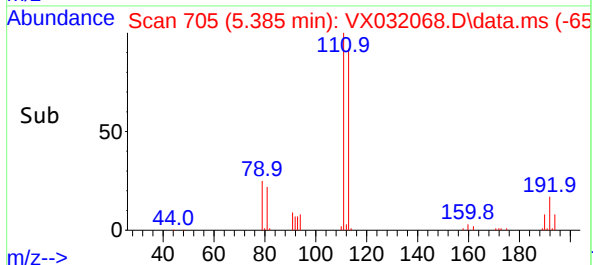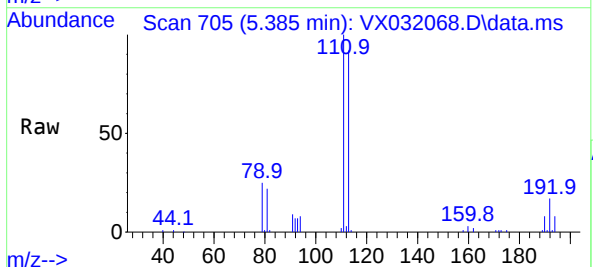



#36

1,1-Dichloropropene

Concen: 3.846 ug/l

RT: 5.550 min Scan# 71

Delta R.T. -0.140 min

Lab File: VX032068.D


Acq: 12 Oct 2022 07:47

Instrument :

MSVOA\_X

ClientSampleId :

B-4(12-13)

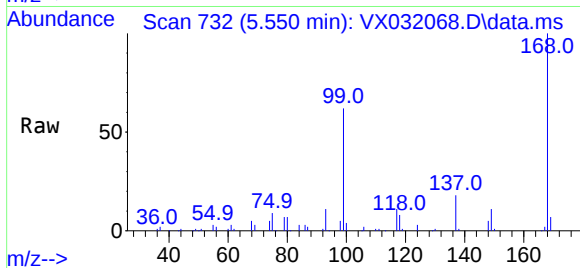




Tgt Ion: 75 Resp: 6734

Ion Ratio Lower Upper

75 100

110 8.2 17.5 52.5#

77 0.0 24.9 37.3#

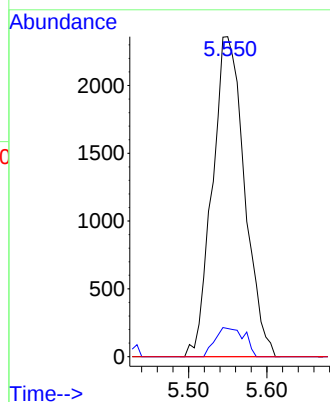

#37

Ethyl Acetate

Concen: 7.610 ug/l

RT: 4.721 min Scan# 596

Delta R.T. 0.007 min

Lab File: VX032068.D

Acq: 12 Oct 2022 07:47




Tgt Ion: 43 Resp: 12545


Ion Ratio Lower Upper

43 100

61 13.3 11.1 16.7


70 11.7 8.6 13.0

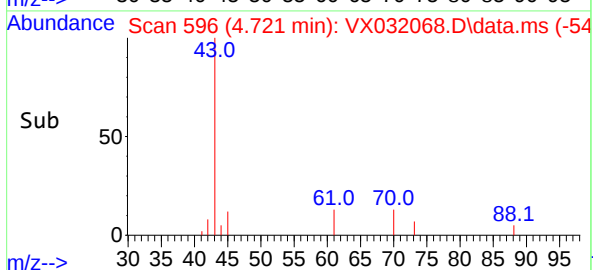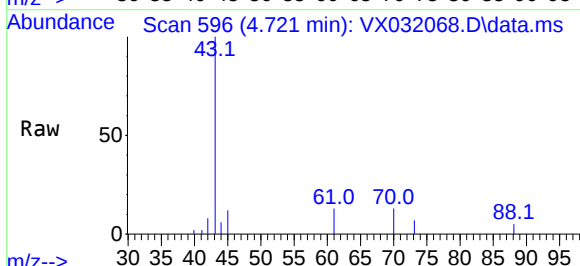






#38  
Carbon Tetrachloride  
Concen: 4.687 ug/l  
RT: 5.556 min Scan# 71  
Delta R.T. -0.121 min  
Lab File: VX032068.D  
Acq: 12 Oct 2022 07:47

Instrument :  
MSVOA\_X  
ClientSampleId :  
B-4(12-13)



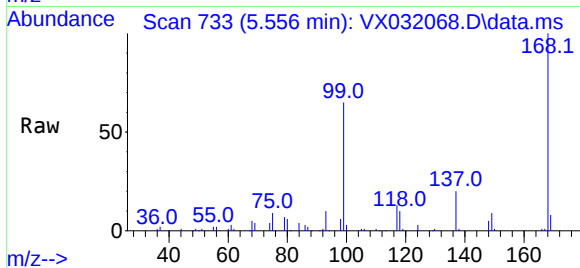



Tgt Ion:117 Resp: 8392  
Ion Ratio Lower Upper  
117 100  
119 4.5 74.6 112.0#  
121 0.0 25.3 37.9#

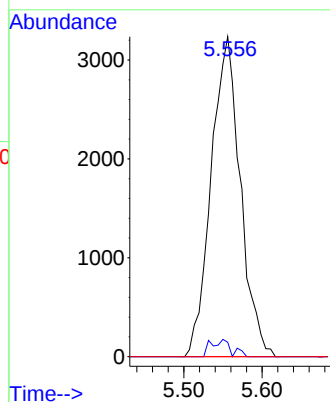

#40  
Benzene  
Concen: 0.273 ug/l  
RT: 6.038 min Scan# 812  
Delta R.T. 0.001 min  
Lab File: VX032068.D  
Acq: 12 Oct 2022 07:47

Tgt Ion: 78 Resp: 1402  
Ion Ratio Lower Upper  
78 100  
77 18.6 18.7 28.1#


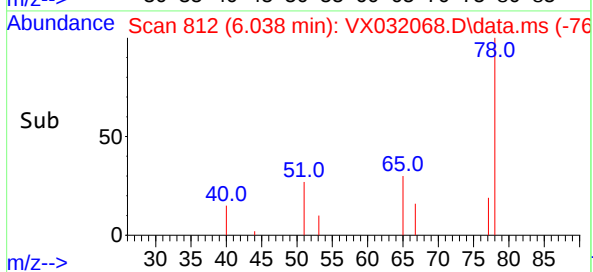
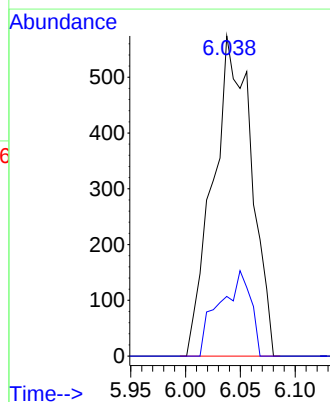
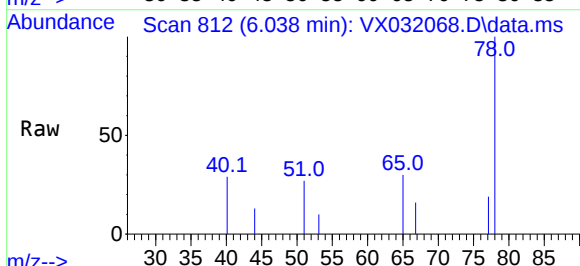




#43  
Isopropyl Acetate  
Concen: 23.616 ug/l  
RT: 6.342 min Scan# 862  
Delta R.T. 0.000 min  
Lab File: VX032068.D  
Acq: 12 Oct 2022 07:47




Instrument :  
MSVOA\_X  
ClientSampleId :  
B-4(12-13)


|             |                |
|-------------|----------------|
| Tgt Ion: 43 | Resp: 59064    |
| Ion Ratio   | Lower Upper    |
| 43          | 100            |
| 61          | 18.6 15.3 22.9 |
| 87          | 14.2 10.6 15.8 |

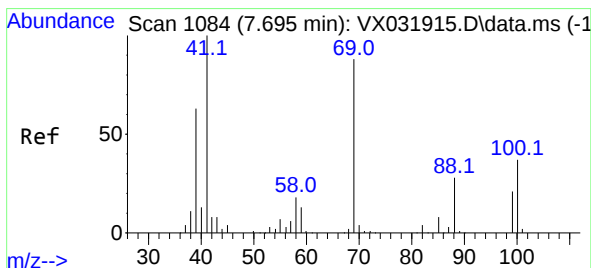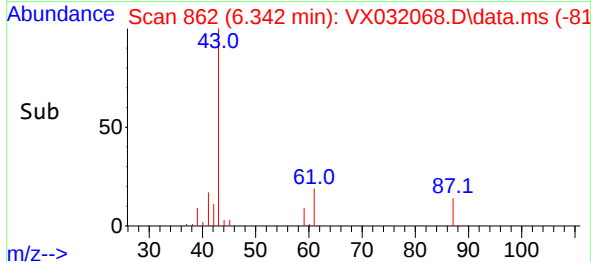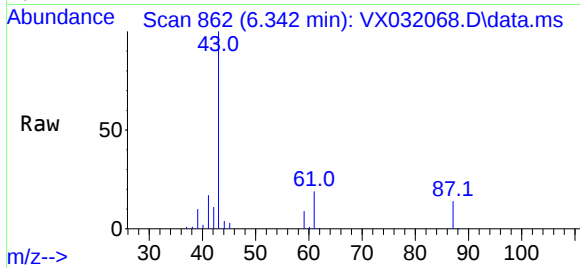

#48  
Methyl methacrylate  
Concen: 48.172 ug/l  
RT: 7.799 min Scan# 1101  
Delta R.T. 0.104 min  
Lab File: VX032068.D  
Acq: 12 Oct 2022 07:47

|             |                |
|-------------|----------------|
| Tgt Ion: 41 | Resp: 57571    |
| Ion Ratio   | Lower Upper    |
| 41          | 100            |
| 69          | 0.1 64.6 96.8  |
| 39          | 59.1 51.4 77.0 |


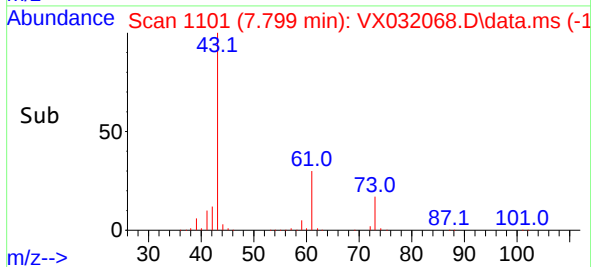

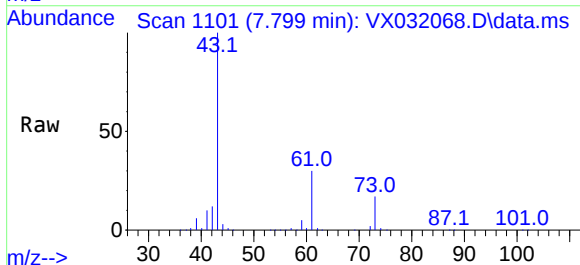




#49  
1,4-Dioxane  
Concen: Below Cal  
RT: 7.806 min Scan# 1102  
Delta R.T. 0.111 min  
Lab File: VX032068.D  
Acq: 12 Oct 2022 07:47




Instrument :  
MSVOA\_X  
ClientSampleId :  
B-4(12-13)


Tgt Ion: 88 Resp: 100  
Ion Ratio Lower Upper  
88 100  
43 560893.0 27.1 40.7#  
58 2601.0 53.9 80.9#

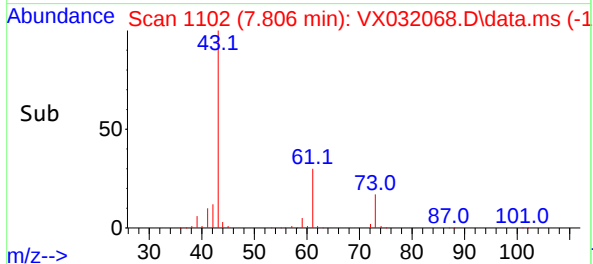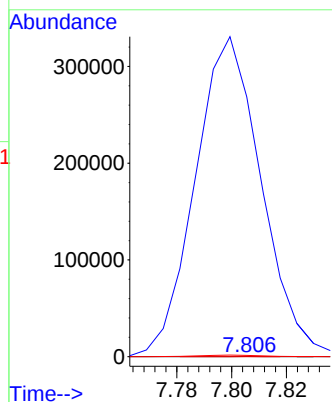

#50  
Toluene-d8  
Concen: 51.744 ug/l  
RT: 8.647 min Scan# 1240  
Delta R.T. -0.006 min  
Lab File: VX032068.D  
Acq: 12 Oct 2022 07:47

Tgt Ion: 98 Resp: 245852  
Ion Ratio Lower Upper  
98 100  
100 65.8 52.5 78.7



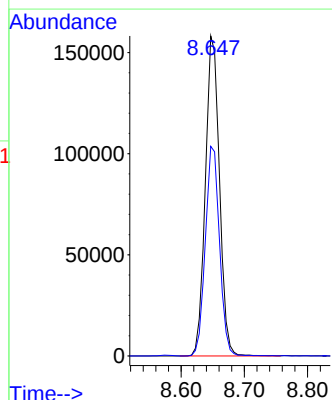
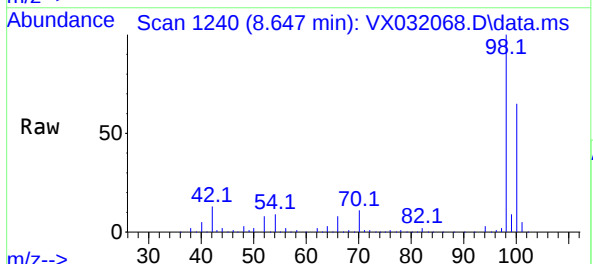




#51  
4-Methyl-2-Pentanone  
Concen: 29.711 ug/l  
RT: 8.549 min Scan# 11  
Delta R.T. -0.024 min  
Lab File: VX032068.D  
Acq: 12 Oct 2022 07:47




Instrument :  
MSVOA\_X  
ClientSampleId :  
B-4(12-13)


Tgt Ion: 43 Resp: 49243  
Ion Ratio Lower Upper  
43 100  
58 8.3 30.6 46.0#

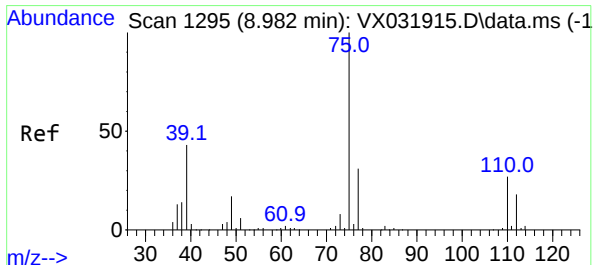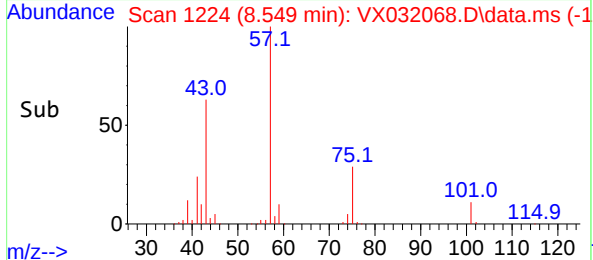

#53  
t-1,3-Dichloropropene  
Concen: 1.435 ug/l  
RT: 8.952 min Scan# 1290  
Delta R.T. -0.030 min  
Lab File: VX032068.D  
Acq: 12 Oct 2022 07:47

Tgt Ion: 75 Resp: 424  
Ion Ratio Lower Upper  
75 100  
77 0.0 24.8 37.2#


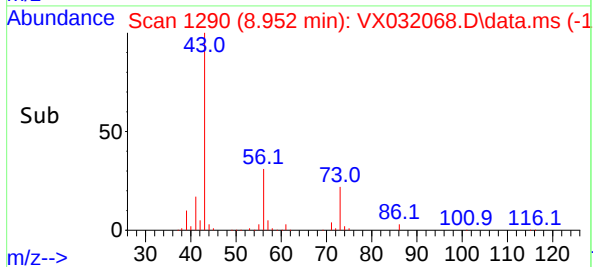

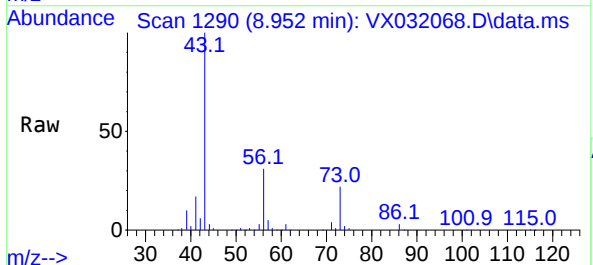




#54  
cis-1,3-Dichloropropene  
Concen: 11.965 ug/l  
RT: 8.549 min Scan# 1194  
Delta R.T. 0.183 min  
Lab File: VX032068.D  
Acq: 12 Oct 2022 07:47




Instrument :  
MSVOA\_X  
ClientSampleId :  
B-4(12-13)


Tgt Ion: 75 Resp: 21859  
Ion Ratio Lower Upper  
75 100  
77 0.4 24.4 36.6#  
39 39.9 43.7 65.5#

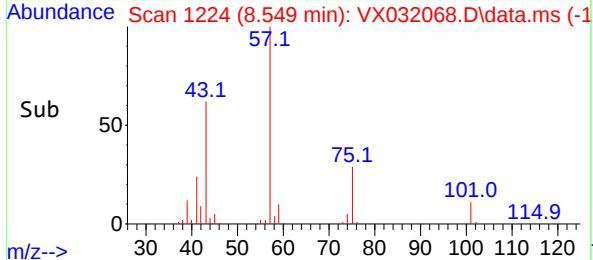

#56  
Ethyl methacrylate  
Concen: 0.280 ug/l  
RT: 9.250 min Scan# 1339  
Delta R.T. 0.134 min  
Lab File: VX032068.D  
Acq: 12 Oct 2022 07:47

Tgt Ion: 69 Resp: 508  
Ion Ratio Lower Upper  
69 100  
41 7025.2 54.2 81.4#  
39 3507.5 34.2 51.2#


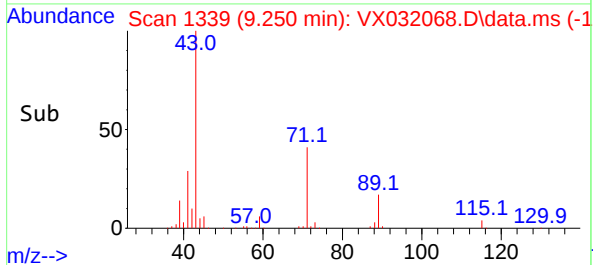

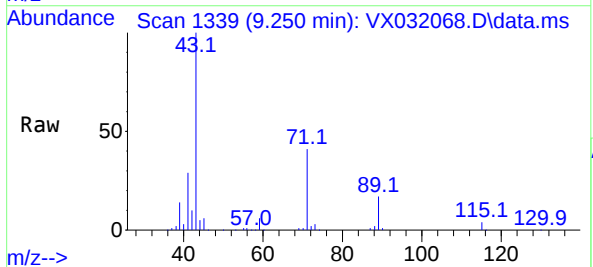




#57  
1,3-Dichloropropane  
Concen: 1.214 ug/l  
RT: 9.482 min Scan# 1377  
Delta R.T. 0.171 min  
Lab File: VX032068.D  
Acq: 12 Oct 2022 07:47




Instrument :  
MSVOA\_X  
ClientSampleId :  
B-4(12-13)


Tgt Ion: 76 Resp: 2761  
Ion Ratio Lower Upper  
76 100  
78 0.0 25.5 38.3#

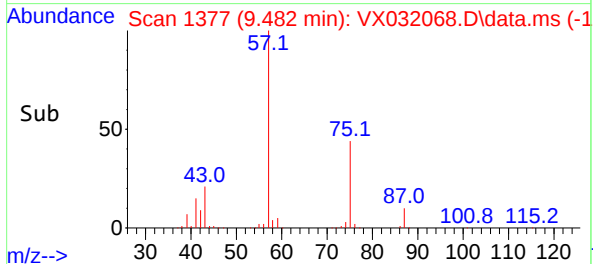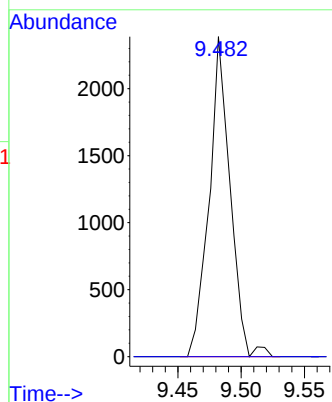

#59  
2-Hexanone  
Concen: 32.199 ug/l  
RT: 9.482 min Scan# 1377  
Delta R.T. 0.049 min  
Lab File: VX032068.D  
Acq: 12 Oct 2022 07:47

Tgt Ion: 43 Resp: 39349  
Ion Ratio Lower Upper  
43 100  
58 19.4 26.7 80.0#



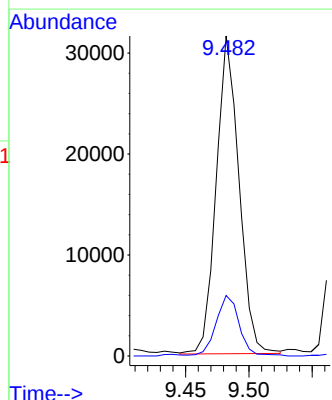
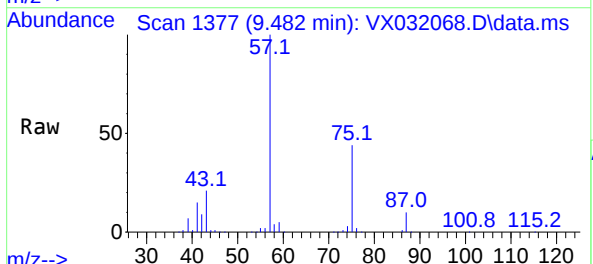


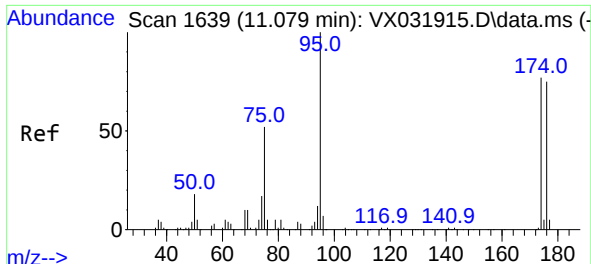

#62  
4-Bromofluorobenzene  
Concen: 49.788 ug/l  
RT: 11.079 min Scan# 1639  
Delta R.T. 0.000 min  
Lab File: VX032068.D  
Acq: 12 Oct 2022 07:47




Instrument :  
MSVOA\_X  
ClientSampleId :  
B-4(12-13)


Tgt Ion: 95 Resp: 83629  
Ion Ratio Lower Upper  
95 100  
174 76.9 0.0 153.2  
176 73.9 0.0 144.0

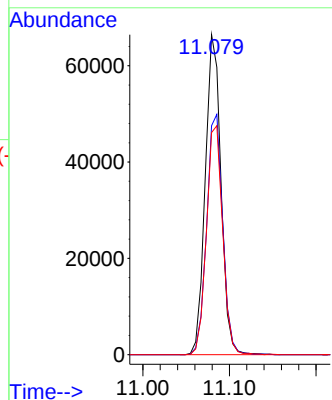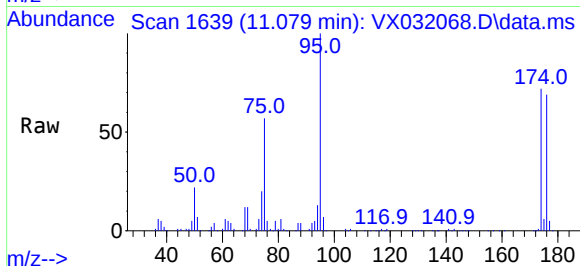

#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.055 min Scan# 1471  
Delta R.T. 0.000 min  
Lab File: VX032068.D  
Acq: 12 Oct 2022 07:47

Tgt Ion: 117 Resp: 128250  
Ion Ratio Lower Upper  
117 100  
82 54.6 46.8 70.2  
119 30.8 26.4 39.6


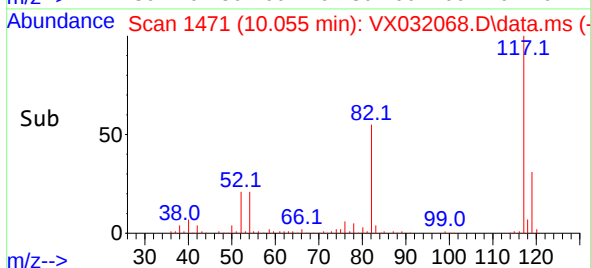
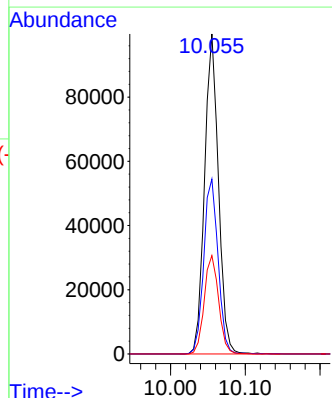
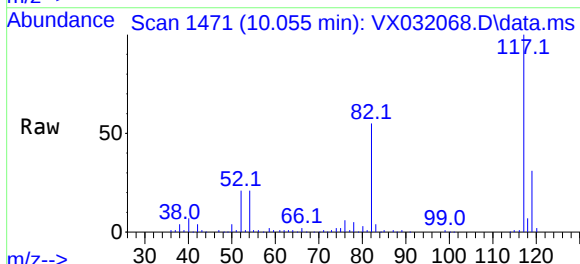




#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 12.024 min Scan# 11  
Delta R.T. 0.000 min  
Lab File: VX032068.D  
Acq: 12 Oct 2022 07:47




Instrument :  
MSVOA\_X  
ClientSampleId :  
B-4(12-13)


Tgt Ion:152 Resp: 74642  
Ion Ratio Lower Upper  
152 100  
115 63.7 43.4 130.1  
150 156.9 0.0 346.8

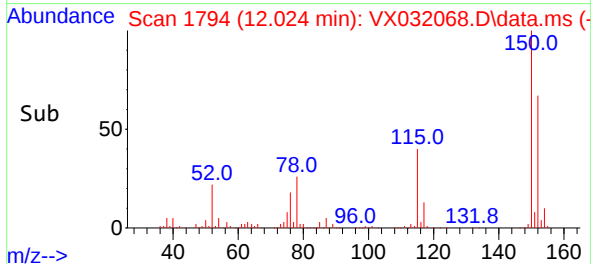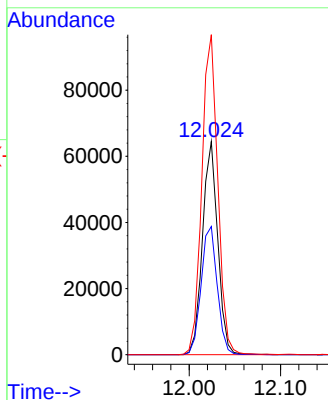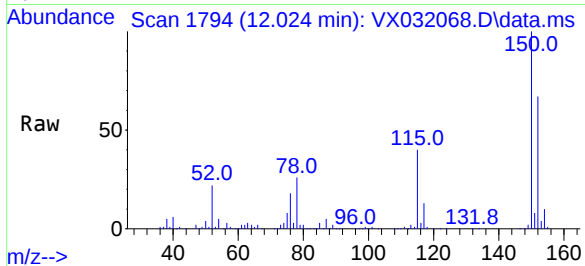

#74  
N-ethyl acetate  
Concen: 0.430 ug/l  
RT: 10.823 min Scan# 1597  
Delta R.T. -0.024 min  
Lab File: VX032068.D  
Acq: 12 Oct 2022 07:47

Tgt Ion: 43 Resp: 740  
Ion Ratio Lower Upper  
43 100  
70 0.0 33.4 50.2#  
55 2.7 18.2 27.2#  
61 0.0 19.3 28.9#


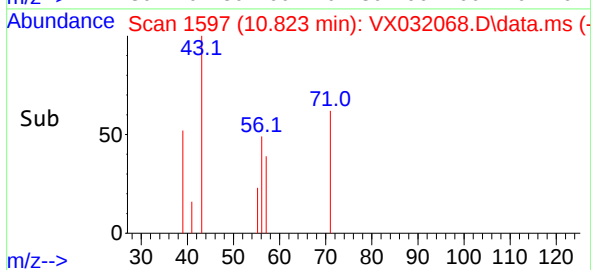
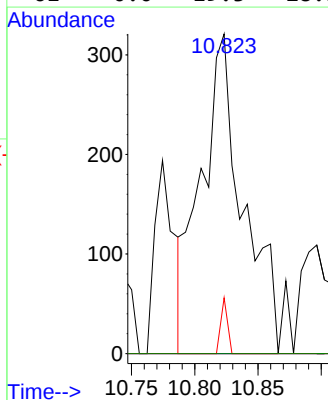
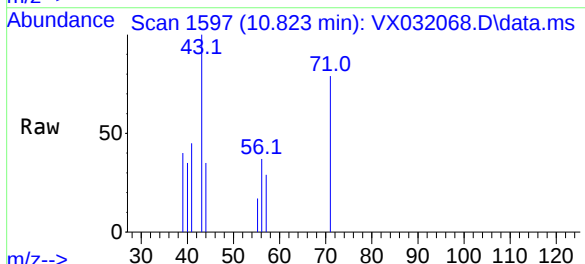


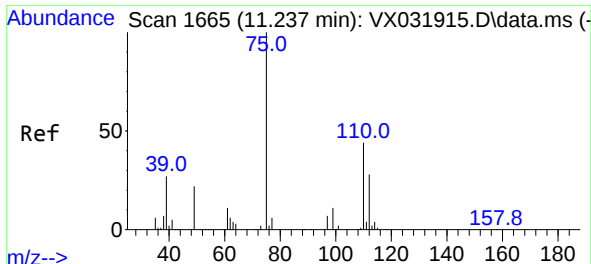

#76  
1,2,3-Trichloropropane  
Concen: 30.688 ug/l  
RT: 11.079 min Scan# 1639  
Delta R.T. -0.158 min  
Lab File: VX032068.D  
Acq: 12 Oct 2022 07:47




Instrument :  
MSVOA\_X  
ClientSampleId :  
B-4(12-13)


Tgt Ion: 75 Resp: 46946  
Ion Ratio Lower Upper  
75 100  
77 1.1 20.3 60.9#

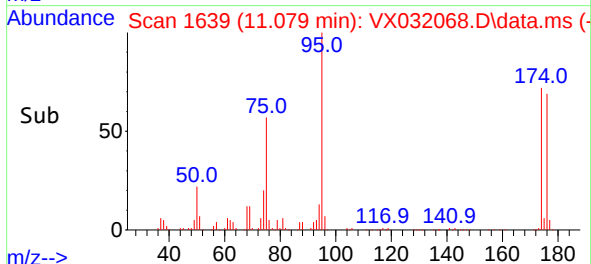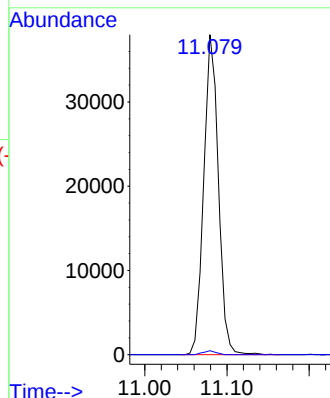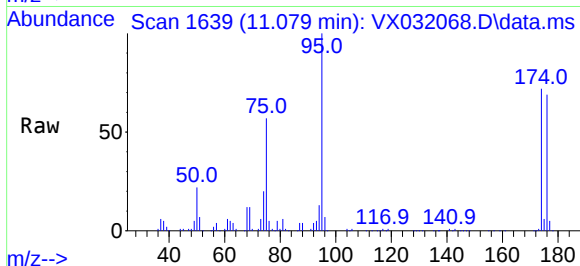

#81  
trans-1,4-Dichloro-2-butene  
Concen: 104.663 ug/l  
RT: 11.079 min Scan# 1639  
Delta R.T. 0.061 min  
Lab File: VX032068.D  
Acq: 12 Oct 2022 07:47


Tgt Ion: 75 Resp: 46946  
Ion Ratio Lower Upper  
75 100  
53 0.0 77.6 116.4#  
89 0.0 37.4 56.0#

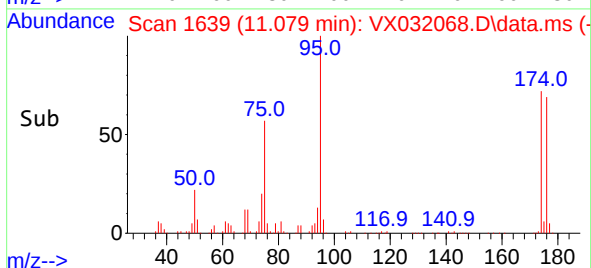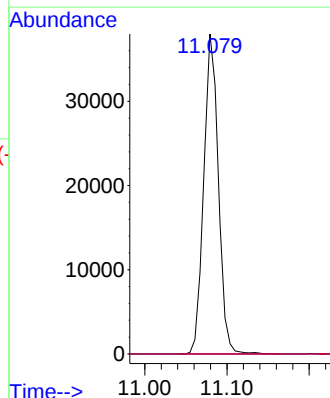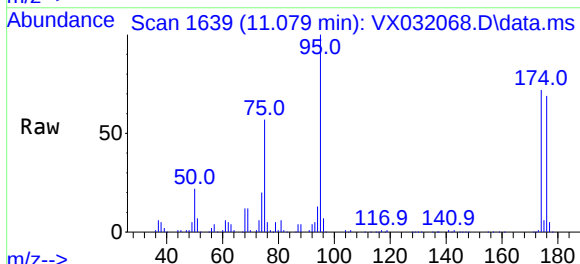

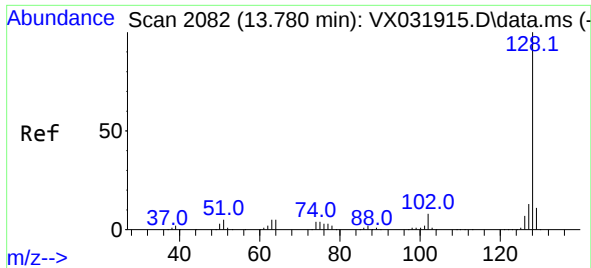

#95  
Naphthalene  
Concen: 0.213 ug/l  
RT: 13.780 min Scan# 20  
Delta R.T. 0.000 min  
Lab File: VX032068.D  
Acq: 12 Oct 2022 07:47

Instrument :  
MSVOA\_X  
ClientSampleId :  
B-4(12-13)

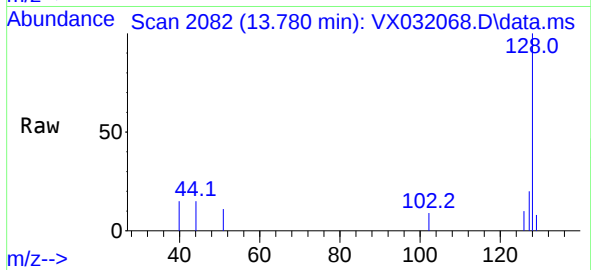

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 128   | Resp: | 1165  |
| Ion      | Ratio | Lower | Upper |
| 128      | 100   |       |       |
| 127      | 13.6  | 10.4  | 15.6  |
| 129      | 9.4   | 8.8   | 13.2  |

