

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101122\
 Data File : VX032035.D
 Acq On : 11 Oct 2022 14:36
 Operator : JC/MD
 Sample : N5091-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB-01-101022

Quant Time: Oct 11 16:25:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 06 14:28:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	74321	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	112057	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	115868	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	68994	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	76054	49.550	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	99.100%
35) Dibromofluoromethane	5.385	113	59640	47.019	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	94.040%
50) Toluene-d8	8.653	98	225929	49.500	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	99.000%
62) 4-Bromofluorobenzene	11.079	95	73754	45.708	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	91.420%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101122\
Data File : VX032035.D
Acq On : 11 Oct 2022 14:36
Operator : JC/MD
Sample : N5091-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-01-101022

Quant Time: Oct 11 16:25:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 06 14:28:46 2022
Response via : Initial Calibration




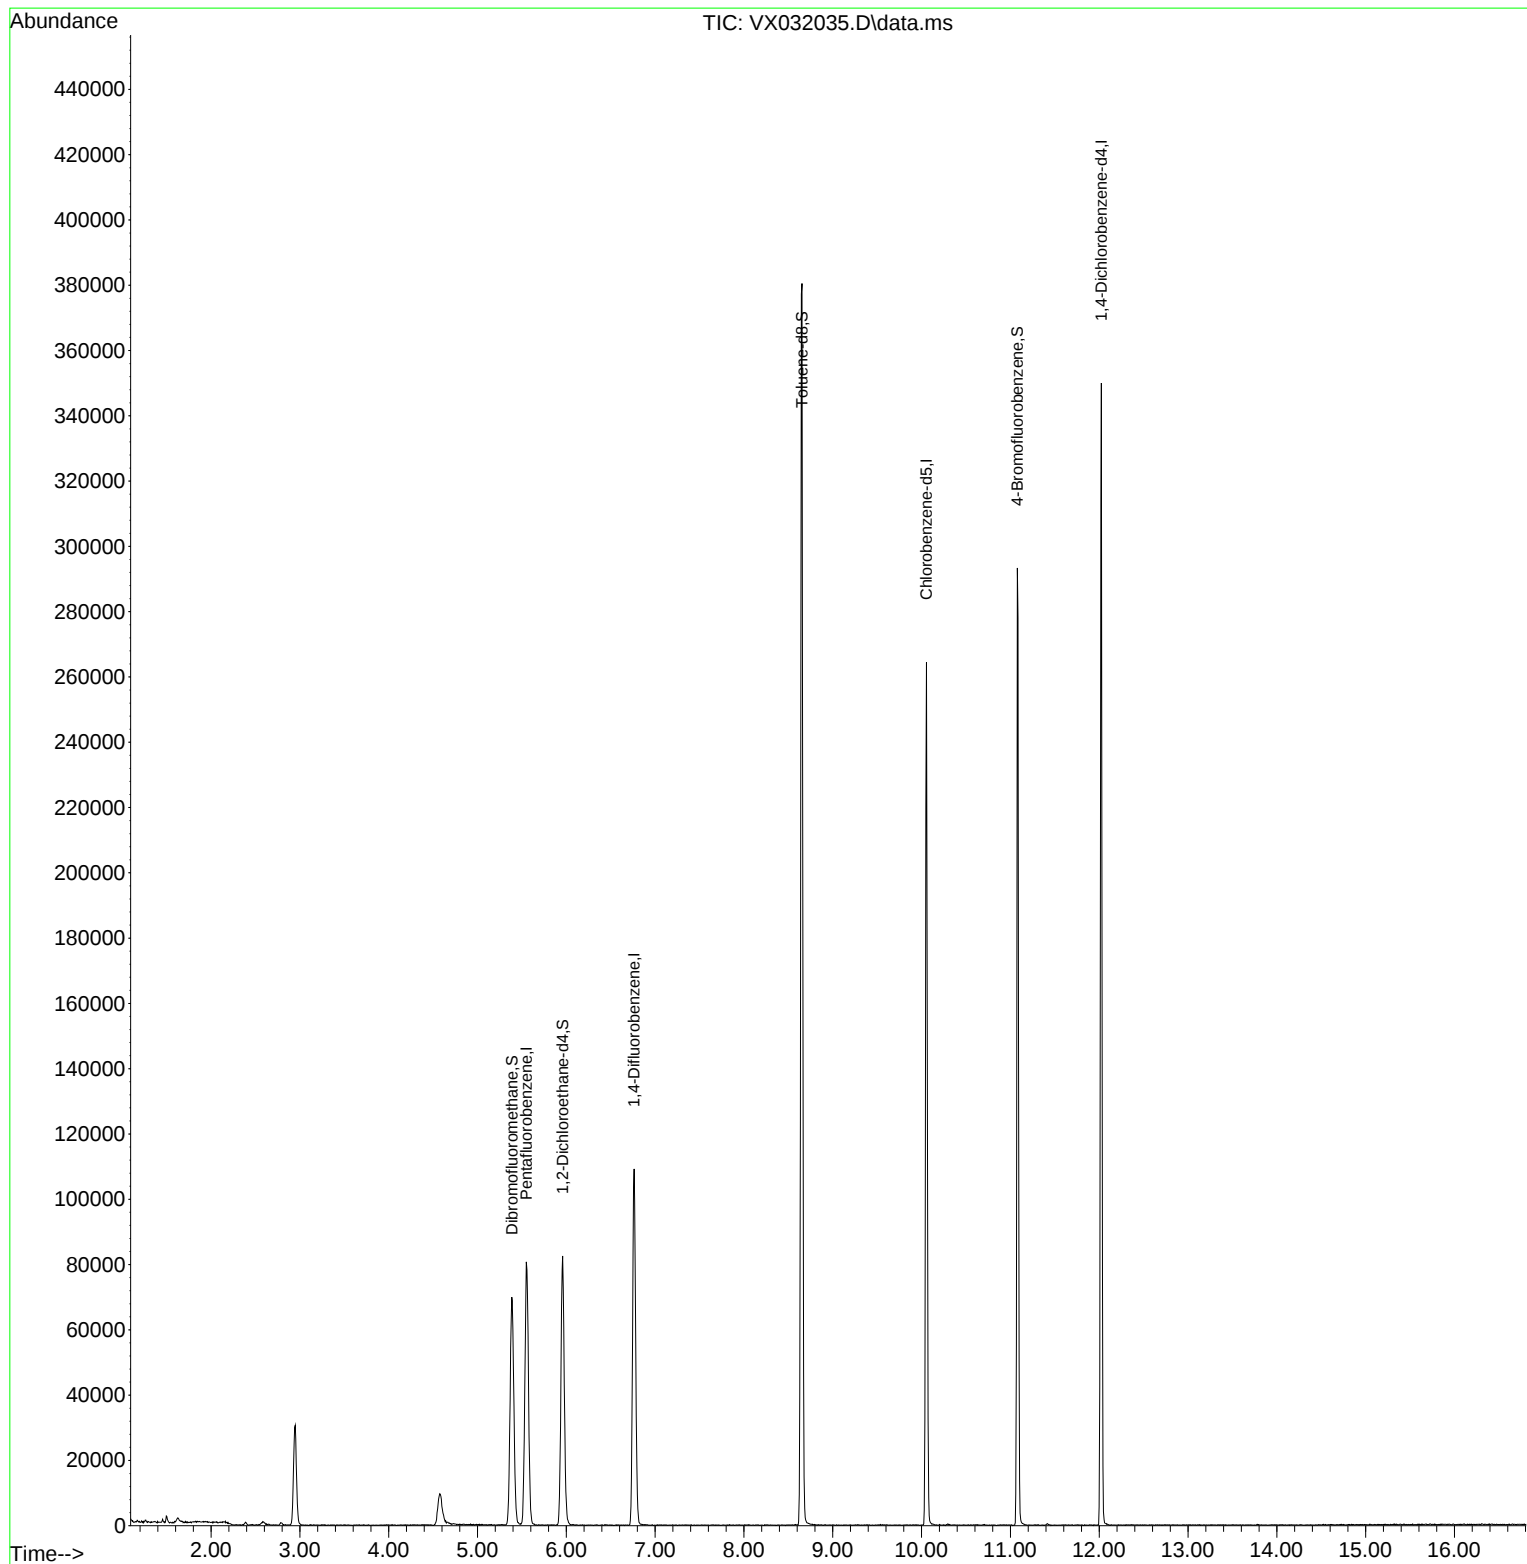




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 713
Delta R.T. -0.006 min
Lab File: VX032035.D
Acq: 11 Oct 2022 14:36




Instrument :
MSVOA_X
ClientSampleId :
TB-01-101022


Tgt Ion:168 Resp: 74321
Ion Ratio Lower Upper
168 100
99 60.4 48.8 73.2

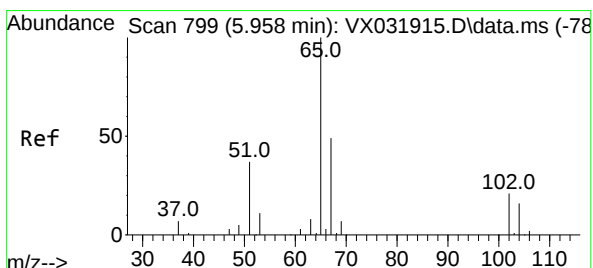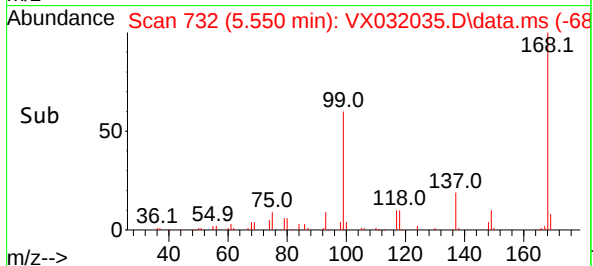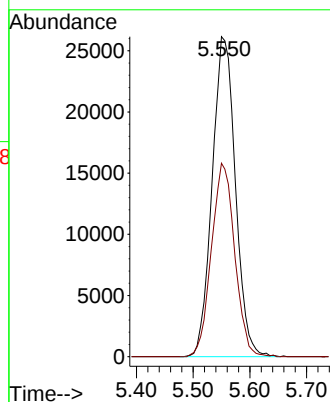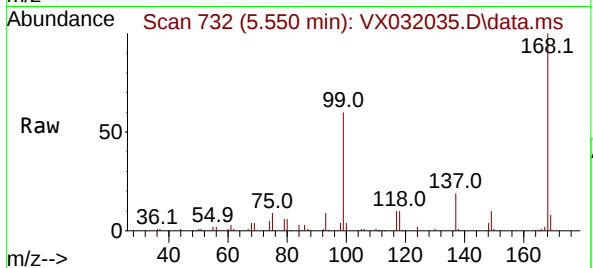

#33
1,2-Dichloroethane-d4
Concen: 49.550 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX032035.D
Acq: 11 Oct 2022 14:36

Tgt Ion: 65 Resp: 76054
Ion Ratio Lower Upper
65 100
67 51.4 0.0 102.4


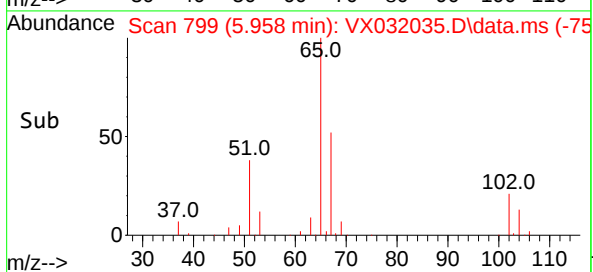
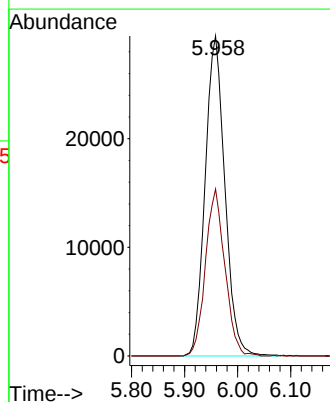
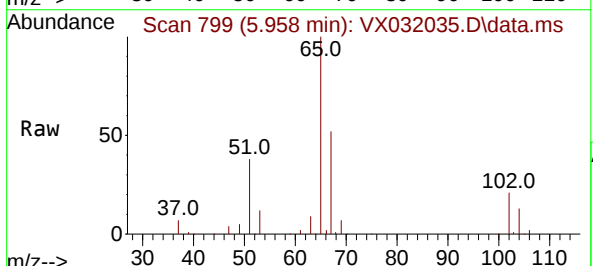


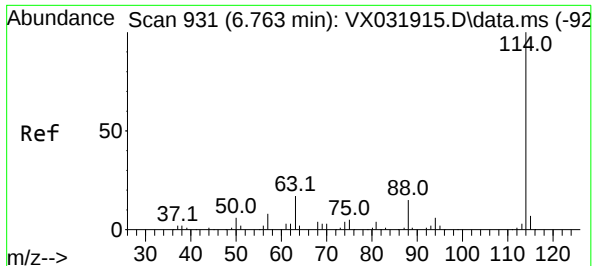

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. -0.000 min
Lab File: VX032035.D
Acq: 11 Oct 2022 14:36




Instrument :
MSVOA_X
ClientSampleId :
TB-01-101022


Tgt Ion:114 Resp: 112057
Ion Ratio Lower Upper
114 100
63 19.9 0.0 42.6
88 15.2 0.0 33.0

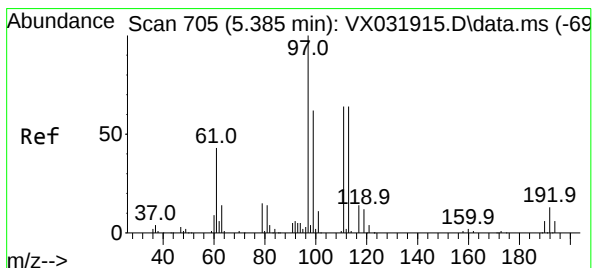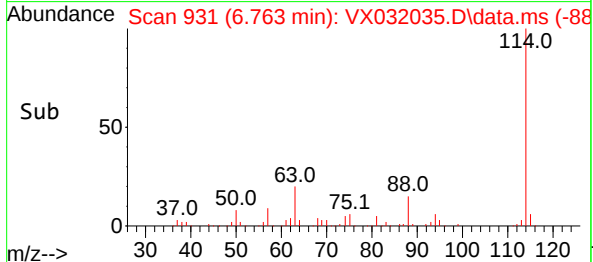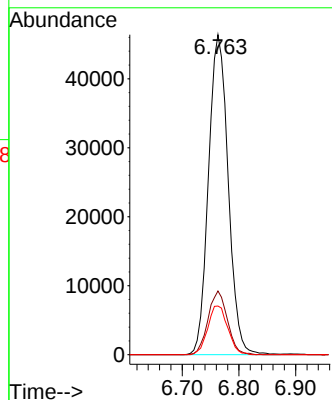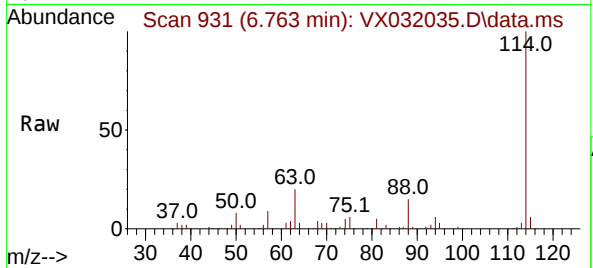

#35
Dibromofluoromethane
Concen: 47.019 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX032035.D
Acq: 11 Oct 2022 14:36

Tgt Ion:113 Resp: 59640
Ion Ratio Lower Upper
113 100
111 102.4 82.4 123.6
192 19.4 14.1 21.1


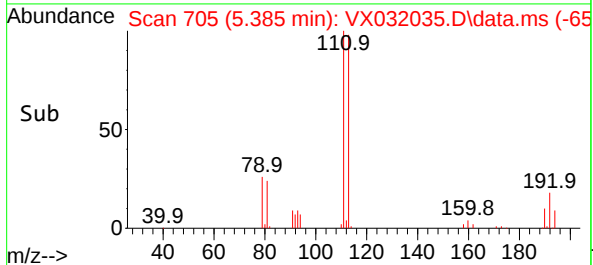
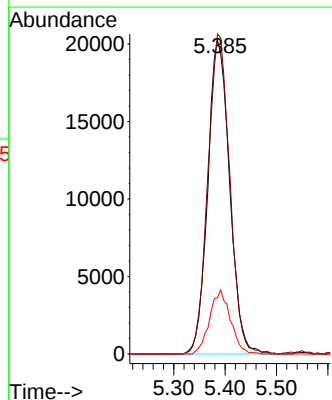
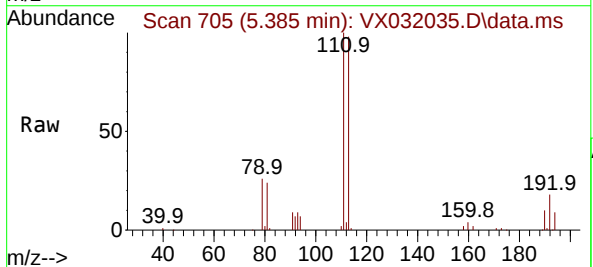


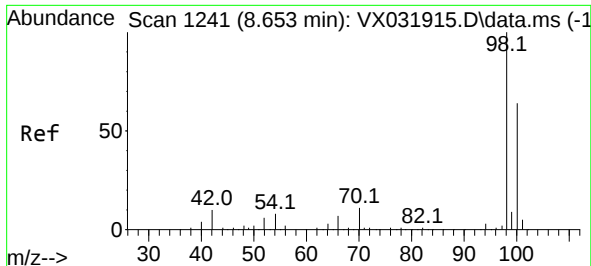

#50
Toluene-d8
Concen: 49.500 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX032035.D
Acq: 11 Oct 2022 14:36




Instrument :
MSVOA_X
ClientSampleId :
TB-01-101022


Tgt Ion: 98 Resp: 225929
Ion Ratio Lower Upper
98 100
100 66.1 52.5 78.7

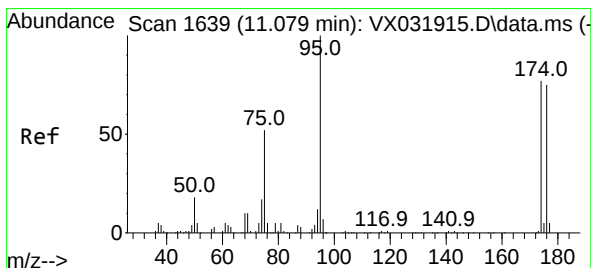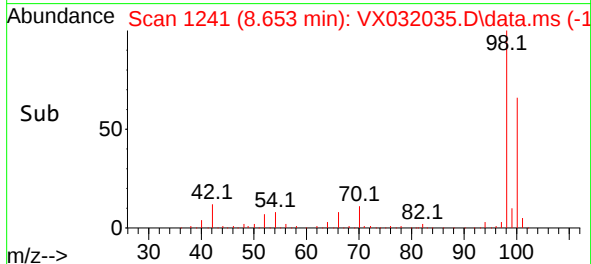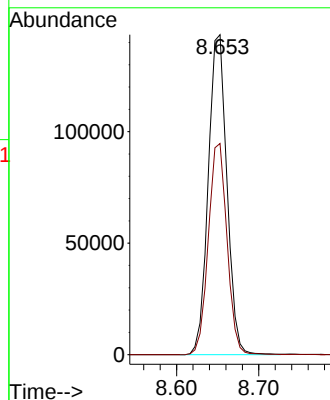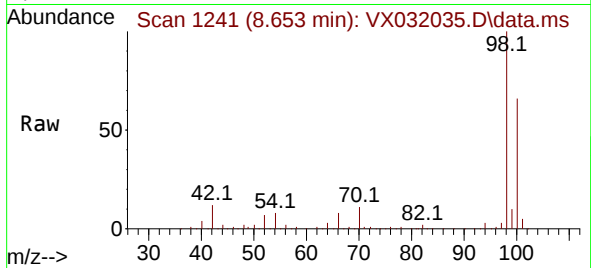

#62
4-Bromofluorobenzene
Concen: 45.708 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX032035.D
Acq: 11 Oct 2022 14:36

Tgt Ion: 95 Resp: 73754
Ion Ratio Lower Upper
95 100
174 78.7 0.0 153.2
176 78.6 0.0 144.0


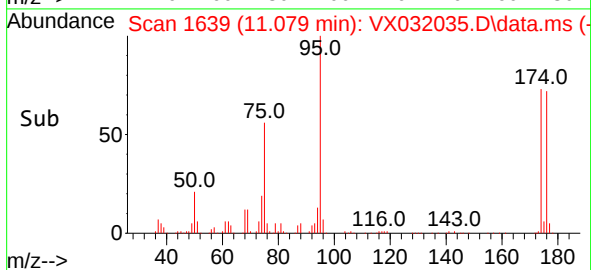
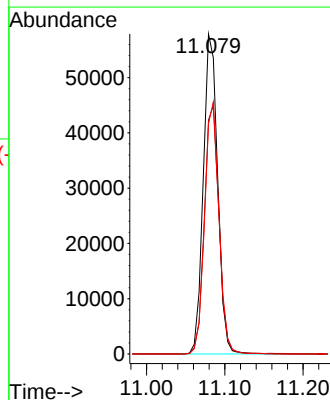
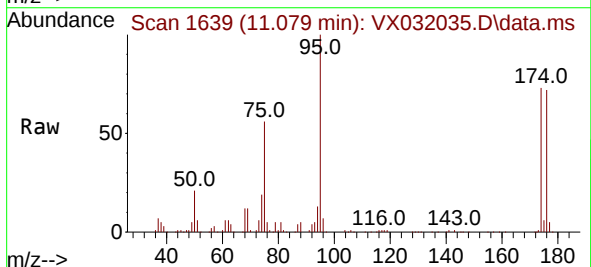


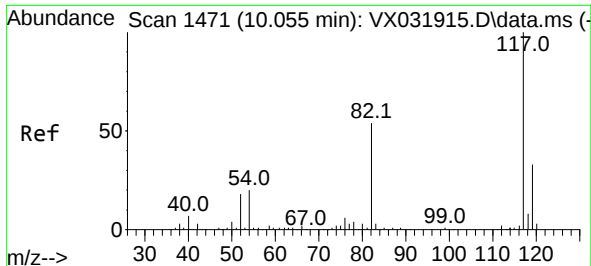

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX032035.D
Acq: 11 Oct 2022 14:36

Instrument :
MSVOA_X
ClientSampleId :
TB-01-101022

Tgt Ion:117 Resp: 115868
Ion Ratio Lower Upper
117 100
82 53.5 46.8 70.2
119 31.5 26.4 39.6

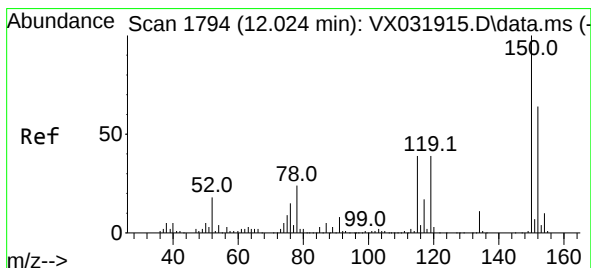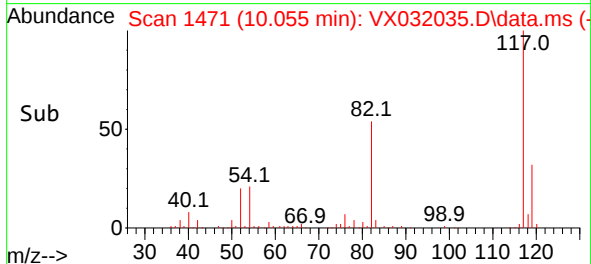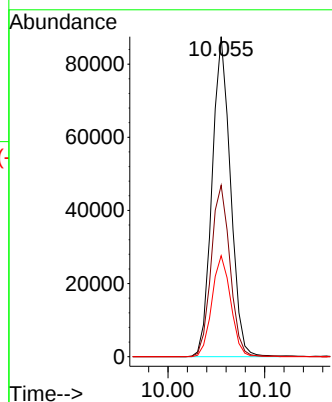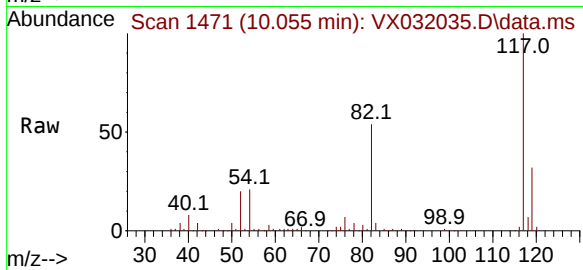

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX032035.D
Acq: 11 Oct 2022 14:36

Tgt Ion:152 Resp: 68994
Ion Ratio Lower Upper
152 100
115 61.2 43.4 130.1
150 157.1 0.0 346.8

