

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101122\
 Data File : VX032038.D
 Acq On : 11 Oct 2022 15:45
 Operator : JC/MD
 Sample : N4937-05 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-112

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
 Title : SW846 8260

Signal : TIC: VX032038.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	52	rVB	18678	18542	1.79%	0.214%
2	1.746	102	108	116	rBV	44484	59698	5.78%	0.688%
3	1.953	138	142	150	rVB2	7907	10781	1.04%	0.124%
4	2.069	156	161	167	rVB	9702	13550	1.31%	0.156%
5	2.867	287	292	298	rVB2	8174	15084	1.46%	0.174%
6	2.947	298	305	319	rVB	7845	22030	2.13%	0.254%
7	3.111	324	332	344	rVB3	15555	38557	3.73%	0.445%
8	4.300	517	527	539	rBB3	13422	37050	3.59%	0.427%
9	4.580	561	573	583	rBV2	4061	13204	1.28%	0.152%
10	5.385	693	705	715	rBV2	69316	202068	19.56%	2.330%
11	5.556	723	733	750	rVB2	78768	227088	21.98%	2.618%
12	5.958	789	799	805	rBV	78154	212648	20.58%	2.452%
13	6.037	805	812	828	rVB	359422	958795	92.79%	11.054%
14	6.245	830	846	857	rBV3	76456	232891	22.54%	2.685%
15	6.763	921	931	942	rBV	107293	259345	25.10%	2.990%
16	7.373	1024	1031	1039	rBV6	3970	10392	1.01%	0.120%
17	8.427	1197	1204	1211	rBV	42516	75694	7.33%	0.873%
18	8.507	1211	1217	1225	rVV	122093	200485	19.40%	2.312%
19	8.647	1234	1240	1246	rBV	374393	598493	57.92%	6.900%
20	8.720	1246	1252	1262	rVB	582706	881886	85.35%	10.168%
21	8.842	1262	1272	1285	rBV	128106	206762	20.01%	2.384%
22	9.445	1364	1371	1378	rBV3	16435	27543	2.67%	0.318%
23	9.567	1385	1391	1398	rBV2	17351	27066	2.62%	0.312%
24	10.055	1459	1471	1476	rBV	261212	408080	39.49%	4.705%
25	10.104	1476	1479	1482	rVV2	12429	18029	1.74%	0.208%
26	10.146	1482	1486	1490	rVV	47299	67497	6.53%	0.778%
27	10.195	1490	1494	1499	rVV	186325	238256	23.06%	2.747%
28	10.244	1499	1502	1506	rVV	10599	18825	1.82%	0.217%
29	10.299	1506	1511	1517	rVV	790901	1033254	100.00%	11.913%
30	10.354	1517	1520	1528	rVB5	5872	11657	1.13%	0.134%
31	10.640	1562	1567	1578	rBV	373224	483176	46.76%	5.571%
32	10.793	1586	1592	1598	rBV5	4760	10528	1.02%	0.121%
33	10.963	1614	1620	1625	rVB	14723	21427	2.07%	0.247%
34	11.079	1634	1639	1649	rBV	293451	387796	37.53%	4.471%
35	11.171	1649	1654	1660	rVB5	6305	12825	1.24%	0.148%
36	11.274	1666	1671	1673	rBV2	8277	10808	1.05%	0.125%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101122\
 Data File : VX032038.D
 Acq On : 11 Oct 2022 15:45
 Operator : JC/MD
 Sample : N4937-05 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-112

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
 Title : SW846 8260

37	11.305	1673	1676	1680	rVV	30176	37162	3.60%	0.428%
38	11.378	1683	1688	1696	rVV	162191	267321	25.87%	3.082%
39	11.451	1696	1700	1713	rVB	80322	102912	9.96%	1.187%
40	11.610	1721	1726	1733	rBV	69013	90084	8.72%	1.039%
41	11.750	1744	1749	1755	rBV	253207	320256	30.99%	3.692%
42	12.024	1788	1794	1800	rBV	357310	442443	42.82%	5.101%
43	12.085	1800	1804	1812	rVB	75210	95174	9.21%	1.097%
44	12.244	1825	1830	1833	rBV	53553	68950	6.67%	0.795%
45	12.317	1838	1842	1849	rVB2	19300	26836	2.60%	0.309%
46	12.530	1872	1877	1879	rBV2	10128	12626	1.22%	0.146%
47	12.555	1879	1881	1886	rVB	9733	10570	1.02%	0.122%
48	12.616	1886	1891	1894	rBV	17317	21394	2.07%	0.247%
49	12.701	1900	1905	1912	rBV2	8609	13200	1.28%	0.152%
50	12.920	1934	1941	1944	rBV	10252	12487	1.21%	0.144%
51	12.963	1944	1948	1953	rVB	15679	18966	1.84%	0.219%
52	13.170	1974	1982	1986	rBV2	8959	12878	1.25%	0.148%
53	13.292	1998	2002	2009	rVB2	17353	23501	2.27%	0.271%
54	13.774	2077	2081	2086	rBV	20399	24783	2.40%	0.286%




Sum of corrected areas: 8673353

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101122\
Data File : VX032038.D
Acq On : 11 Oct 2022 15:45
Operator : JC/MD
Sample : N4937-05 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-112

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

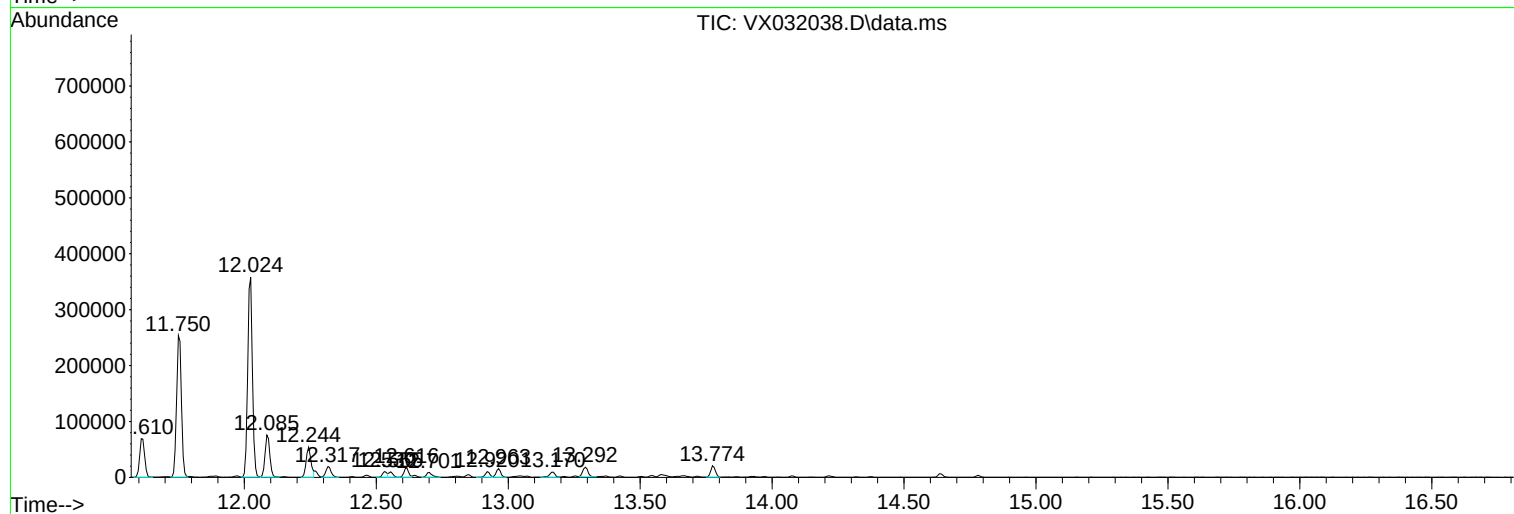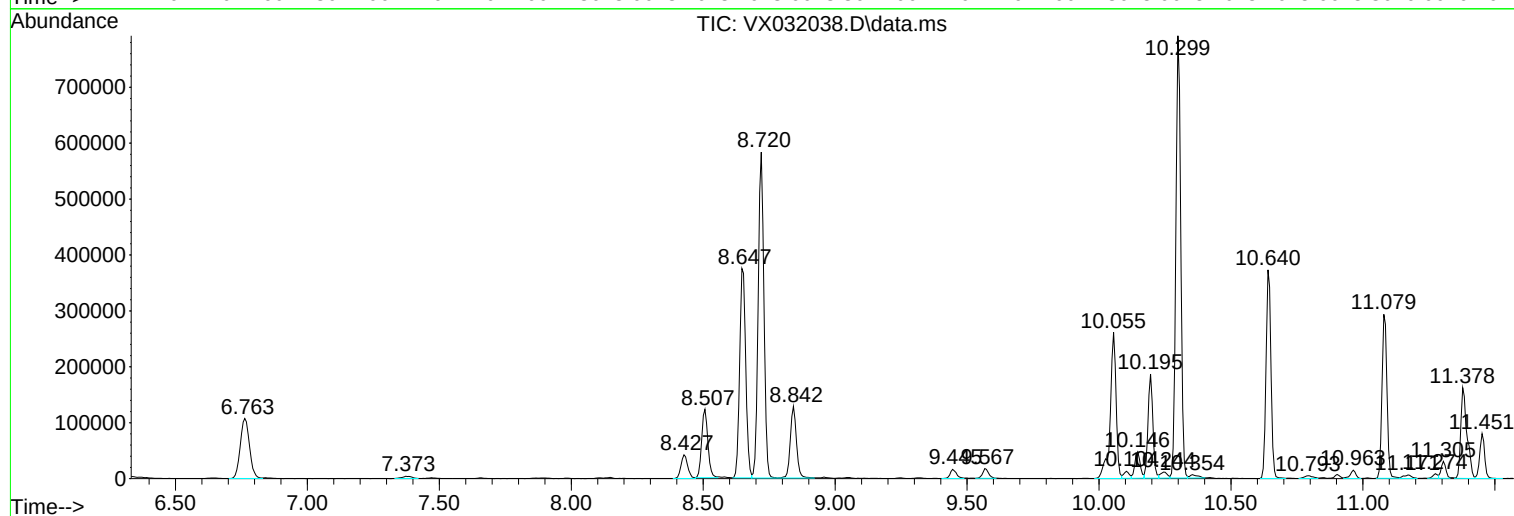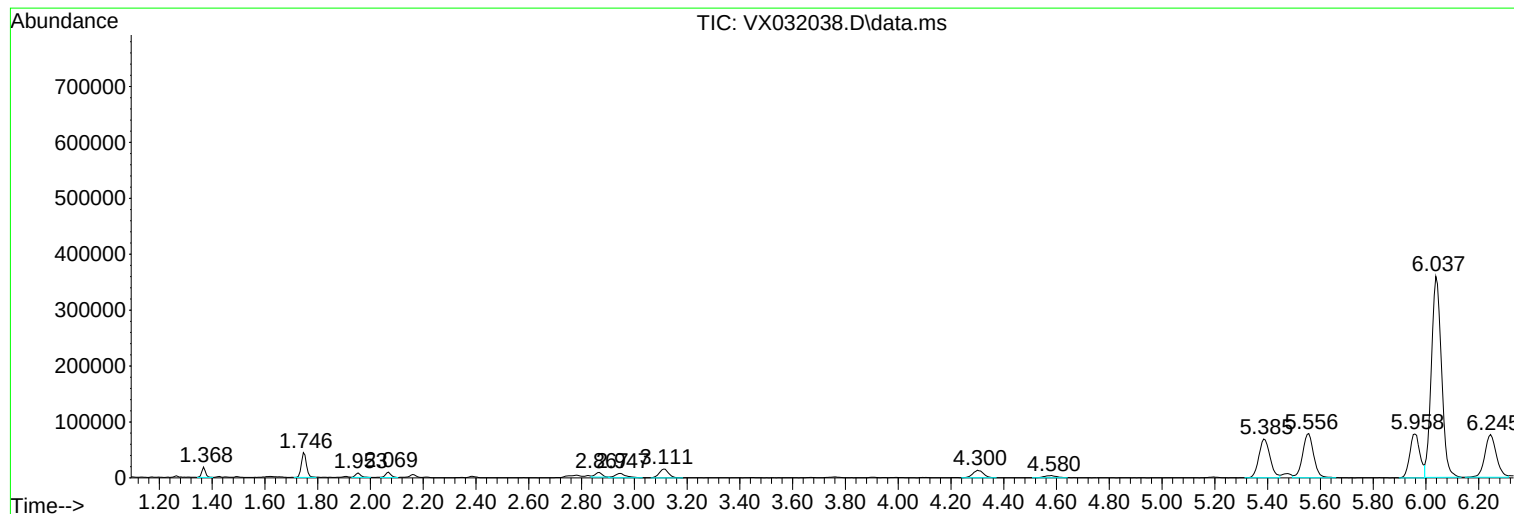

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101122\
Data File : VX032038.D
Acq On : 11 Oct 2022 15:45
Operator : JC/MD
Sample : N4937-05 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-112

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101122\
Data File : VX032038.D
Acq On : 11 Oct 2022 15:45
Operator : JC/MD
Sample : N4937-05 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-112

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------