

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101122\
 Data File : VX032039.D
 Acq On : 11 Oct 2022 16:09
 Operator : JC/MD
 Sample : N4937-06 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-114

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M

Title : SW846 8260

Signal : TIC: VX032039.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.940	298	304	322	rBV2	4625	14763	2.52%	0.462%
2	3.111	322	332	347	rBV	189498	434820	74.14%	13.607%
3	3.757	431	438	452	rVB4	2805	6908	1.18%	0.216%
4	4.580	564	573	583	rBV3	1940	6312	1.08%	0.198%
5	5.385	695	705	720	rBV	68330	200181	34.13%	6.264%
6	5.550	720	732	746	rVB	77901	217457	37.08%	6.805%
7	5.958	789	799	808	rBV2	78000	206306	35.18%	6.456%
8	6.043	808	813	820	rVB3	6074	15489	2.64%	0.485%
9	6.251	837	847	851	rBV4	7545	20216	3.45%	0.633%
10	6.324	852	859	871	rVB2	34582	97755	16.67%	3.059%
11	6.763	921	931	943	rBV	106885	254330	43.37%	7.959%
12	8.653	1234	1241	1250	rBV	367603	586486	100.00%	18.353%
13	8.842	1268	1272	1279	rVB2	4572	6752	1.15%	0.211%
14	10.055	1465	1471	1483	rBV	259390	346466	59.07%	10.842%
15	11.079	1634	1639	1653	rBV	283871	366087	62.42%	11.456%
16	12.024	1789	1794	1804	rVB	341412	415181	70.79%	12.993%




Sum of corrected areas: 3195509

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101122\
Data File : VX032039.D
Acq On : 11 Oct 2022 16:09
Operator : JC/MD
Sample : N4937-06 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-114

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

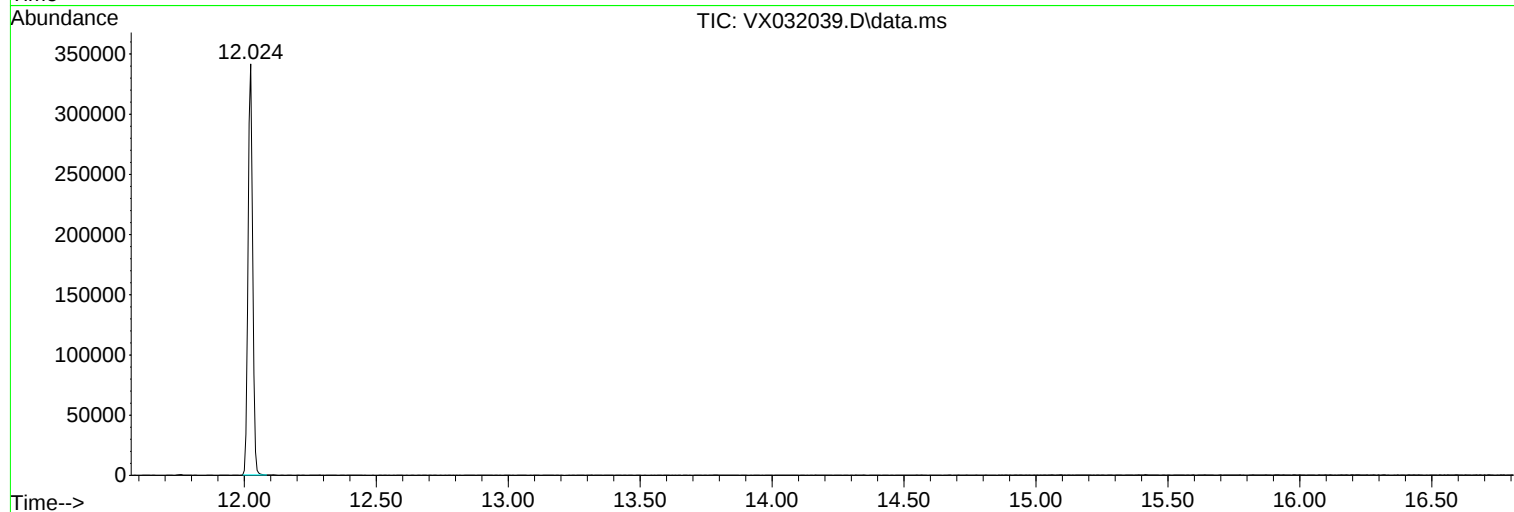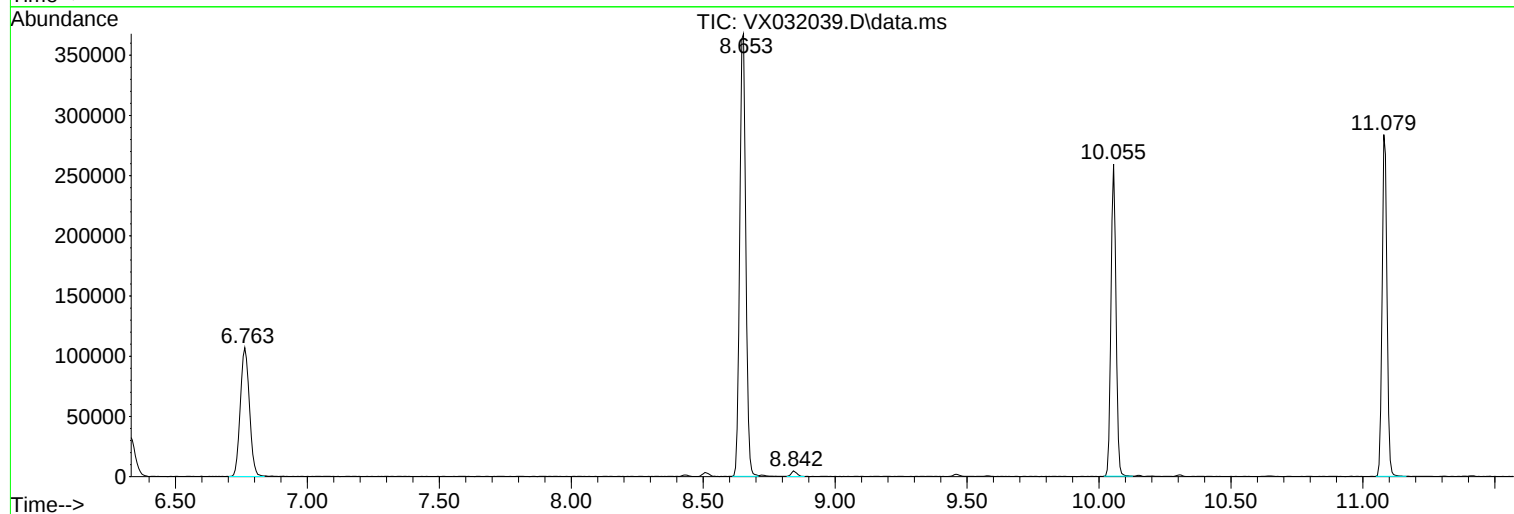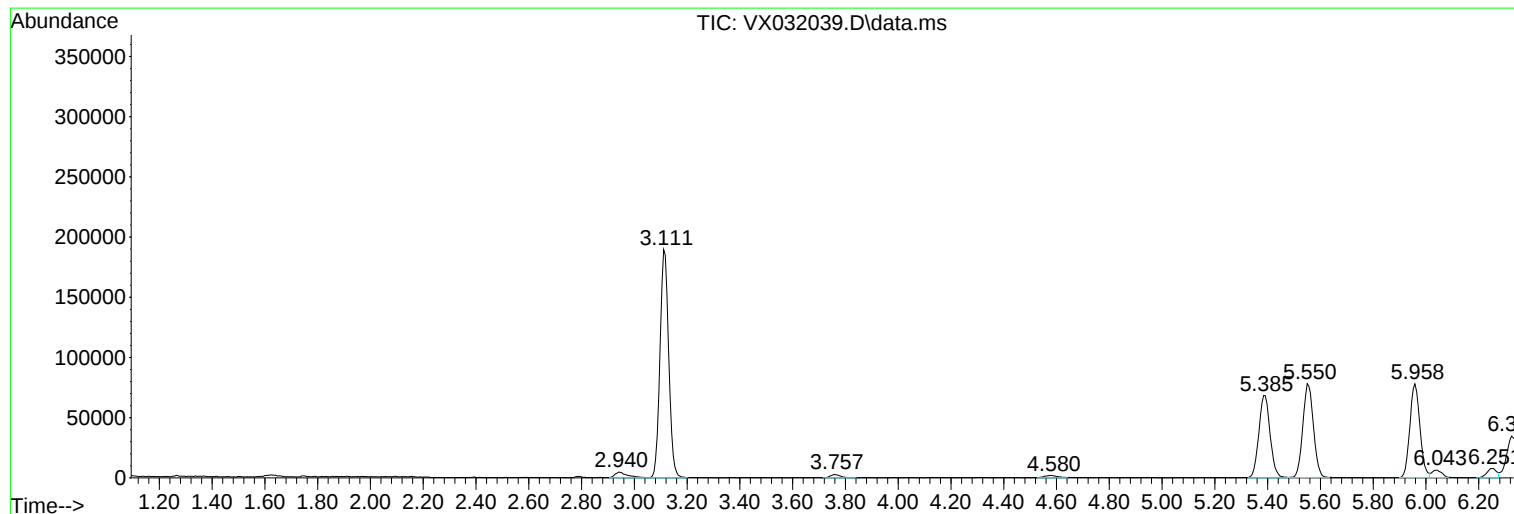

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101122\
Data File : VX032039.D
Acq On : 11 Oct 2022 16:09
Operator : JC/MD
Sample : N4937-06 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-114










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.324	19.22 ug/l	97755	1,4-Difluorobenzene	6.763

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			3-Pentanol, 3-methyl-	102	C6H14O	000077-74-7	23
3			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	9
4			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9
5			Methane, isothiocyanato-	73	C2H3NS	000556-61-6	9

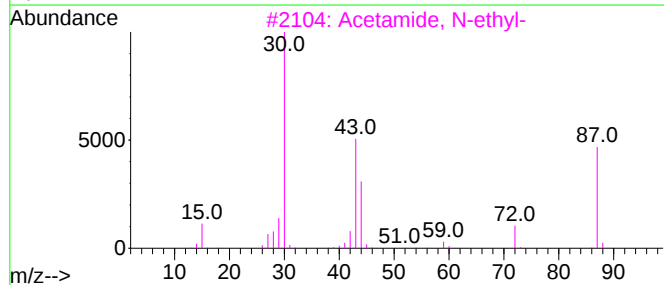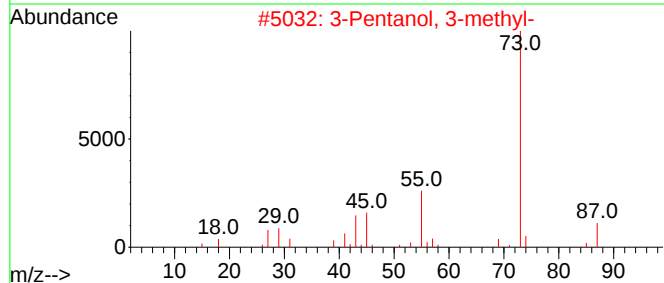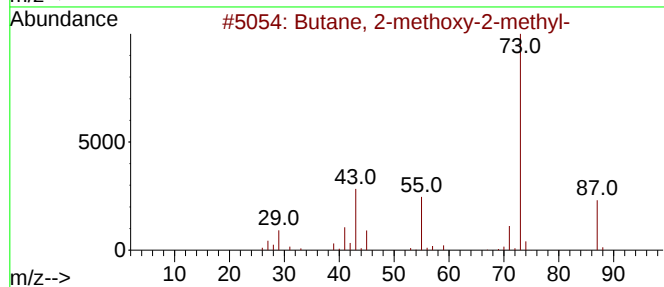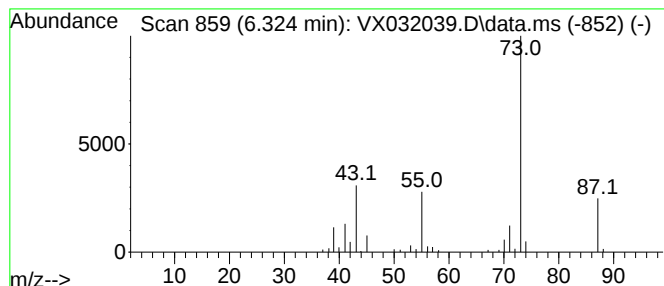

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101122\
Data File : VX032039.D
Acq On : 11 Oct 2022 16:09
Operator : JC/MD
Sample : N4937-06 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-114

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	6.324	19.2	ug/l	97755	2	6.763	254330	50.0