
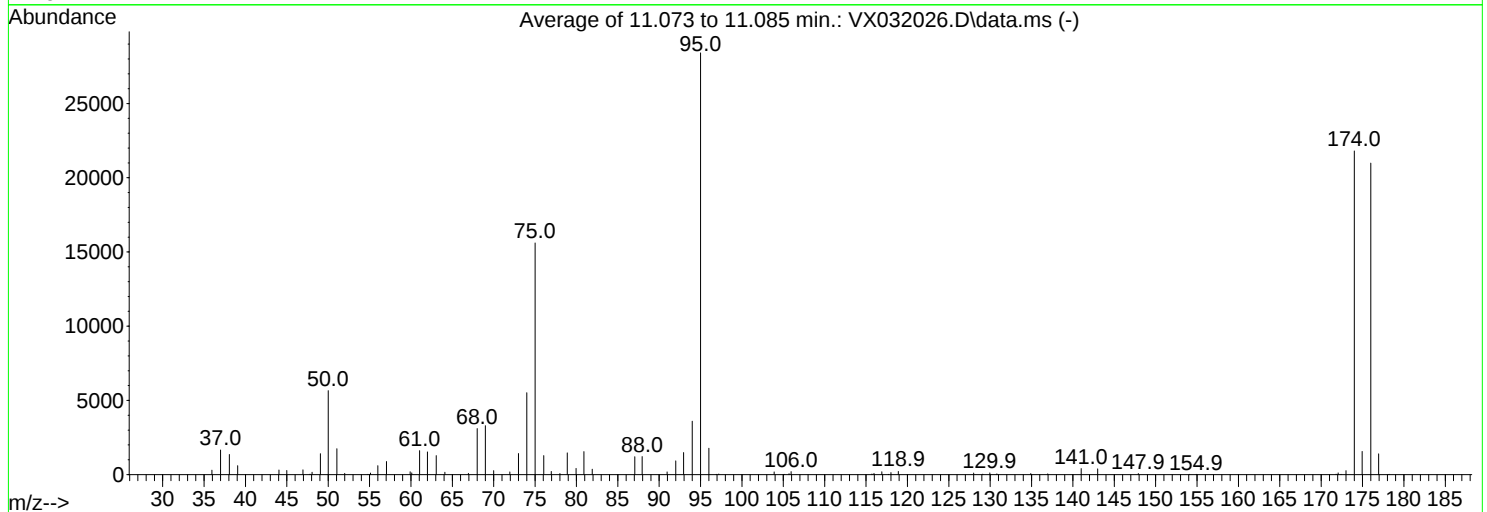


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101122\
 Data File : VX032026.D
 Acq On : 11 Oct 2022 09:43
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
 Title : SW846 8260
 Last Update : Thu Oct 06 14:28:46 2022

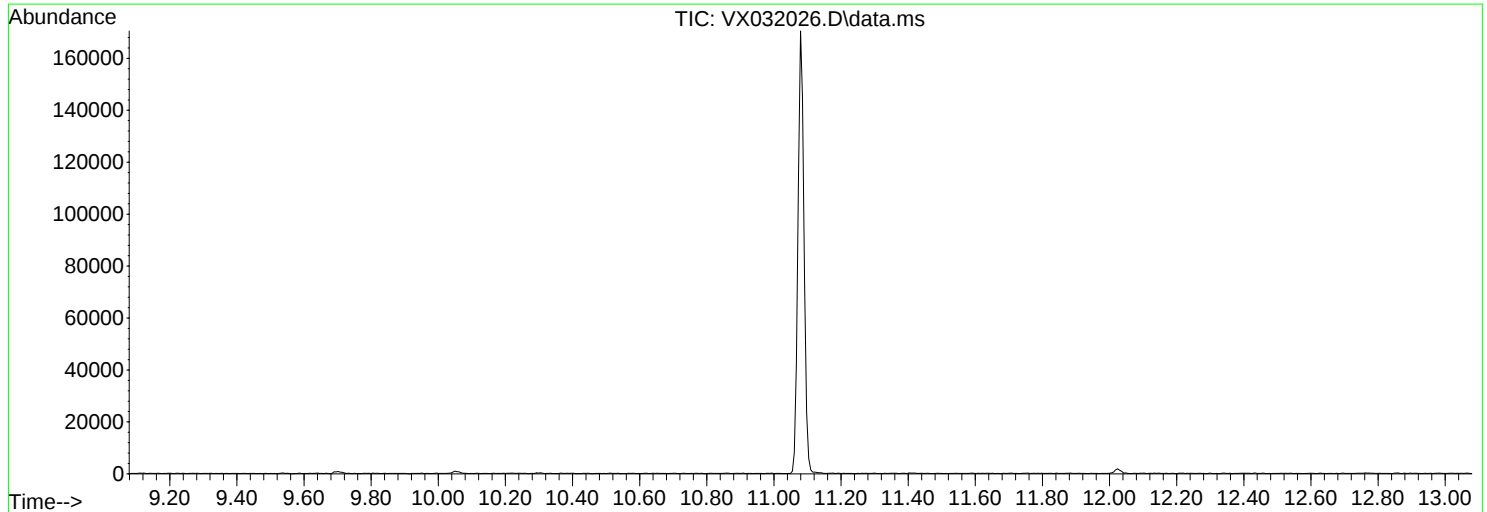

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	5661	PASS
75	95	30	60	54.9	15610	PASS
95	95	100	100	100.0	28413	PASS
96	95	5	9	6.3	1781	PASS
173	174	0.00	2	1.2	268	PASS
174	95	50	100	76.8	21809	PASS
175	174	5	9	7.2	1563	PASS
176	174	95	101	96.2	20985	PASS
177	176	5	9	6.7	1398	PASS