

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101123\
 Data File : VX038239.D
 Acq On : 11 Oct 2023 19:01
 Operator : JC/MD
 Sample : 04803-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GW-9-37-40

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M

Title : SW846 8260

Signal : TIC: VX038239.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	18	rVB	14874	15940	2.62%	0.447%
2	1.361	40	45	52	rBV3	7608	13823	2.28%	0.388%
3	5.385	694	705	721	rBV2	69735	208609	34.34%	5.849%
4	5.550	721	732	745	rBV	109841	308695	50.82%	8.655%
5	5.952	789	798	814	rBV	78309	212362	34.96%	5.954%
6	6.763	922	931	947	rBV2	173596	423896	69.79%	11.886%
7	7.129	984	991	1005	rBV3	23472	49981	8.23%	1.401%
8	8.647	1233	1240	1250	rBV	381185	606754	99.89%	17.013%
9	9.275	1337	1343	1352	rVB	61178	90246	14.86%	2.530%
10	10.055	1465	1471	1487	rBV	427054	579301	95.37%	16.243%
11	11.079	1634	1639	1651	rBV	347340	449484	74.00%	12.603%
12	12.024	1788	1794	1811	rBV	464661	607402	100.00%	17.031%




Sum of corrected areas: 3566493

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101123\
Data File : VX038239.D
Acq On : 11 Oct 2023 19:01
Operator : JC/MD
Sample : 04803-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GW-9-37-40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

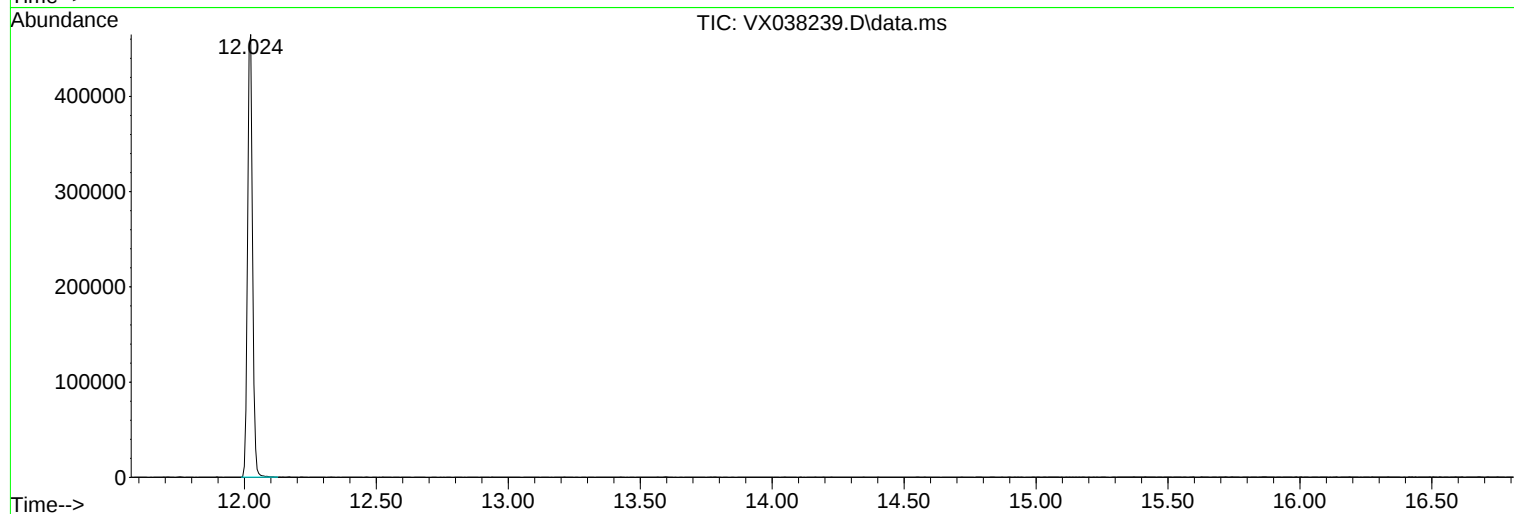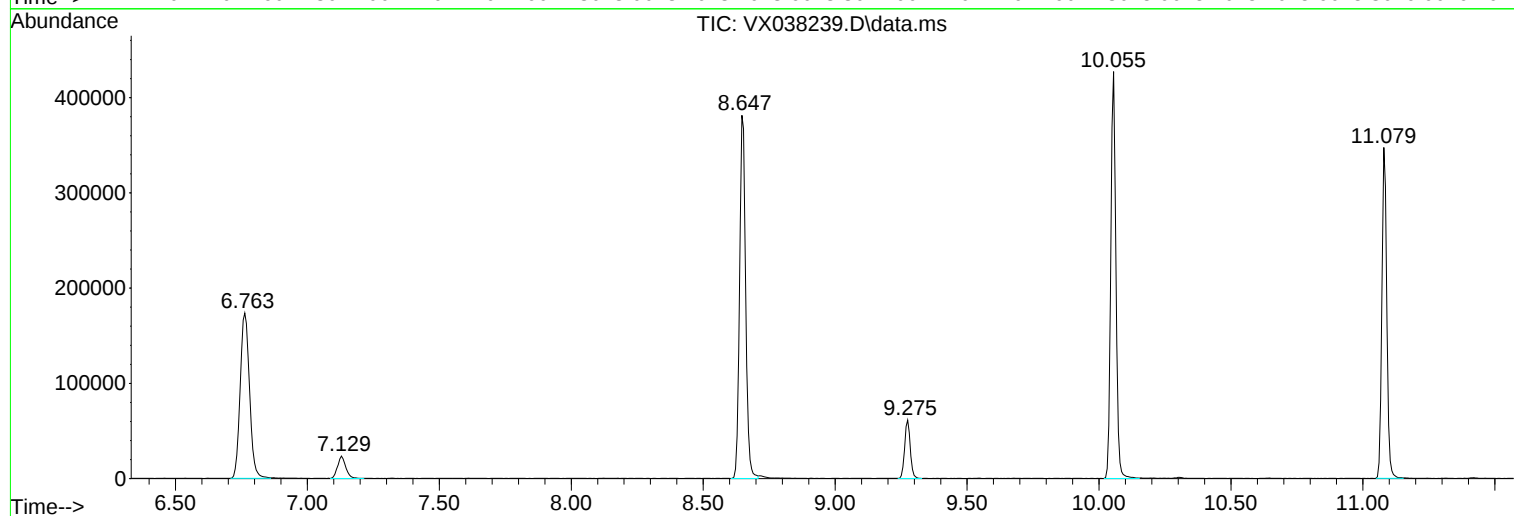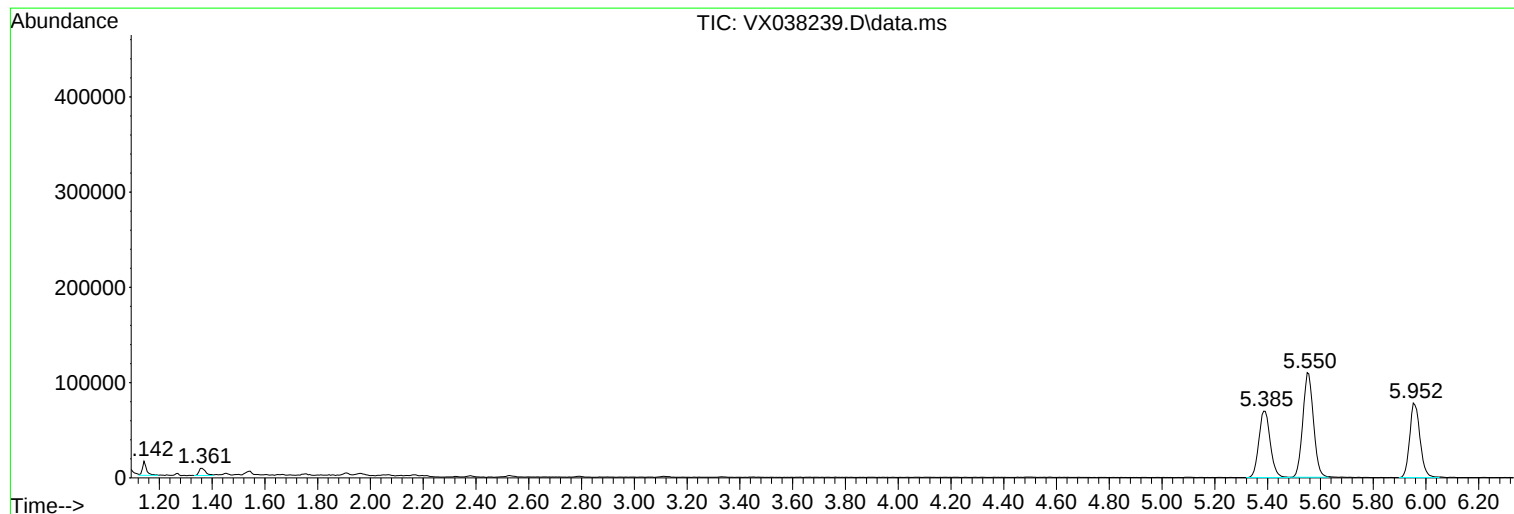

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101123\
Data File : VX038239.D
Acq On : 11 Oct 2023 19:01
Operator : JC/MD
Sample : 04803-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GW-9-37-40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101123\
Data File : VX038239.D
Acq On : 11 Oct 2023 19:01
Operator : JC/MD
Sample : 04803-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GW-9-37-40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc