

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101124\
 Data File : VX043366.D
 Acq On : 11 Oct 2024 15:37
 Operator : JC/MD
 Sample : P4396-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WASTE-WATER-FRAC-TANK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100124W.M
 Title : SW846 8260

Signal : TIC: VX043366.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	24	27	32	rBV3	3822	5096	1.28%	0.213%
2	1.587	71	82	83	rBV4	4052	11342	2.86%	0.474%
3	2.386	209	213	221	rVB2	3900	6568	1.66%	0.275%
4	5.087	644	656	668	rBV2	20947	63962	16.13%	2.675%
5	5.379	692	704	720	rBV	47369	141873	35.77%	5.932%
6	5.544	720	731	745	rVV2	72668	209125	52.73%	8.745%
7	5.946	788	797	812	rBV	58484	156660	39.50%	6.551%
8	6.751	920	929	942	rBV	122957	296600	74.78%	12.402%
9	7.226	1000	1007	1027	rBV2	16837	67398	16.99%	2.818%
10	7.818	1095	1104	1112	rBV3	9779	19271	4.86%	0.806%
11	8.580	1224	1229	1234	rBV2	4331	7781	1.96%	0.325%
12	8.647	1234	1240	1248	rVV	239812	396630	100.00%	16.585%
13	8.720	1248	1252	1262	rVB2	7561	15073	3.80%	0.630%
14	9.519	1379	1383	1394	rBV2	3771	6287	1.59%	0.263%
15	10.049	1465	1470	1484	rBV	246693	356237	89.82%	14.896%
16	10.153	1484	1487	1492	rVB4	3263	4573	1.15%	0.191%
17	10.293	1506	1510	1519	rBV4	2443	4414	1.11%	0.185%
18	10.640	1563	1567	1577	rBV	7020	10635	2.68%	0.445%
19	11.079	1634	1639	1653	rBV	212758	273530	68.96%	11.438%
20	12.018	1788	1793	1801	rBV	254478	330072	83.22%	13.802%
21	12.183	1815	1820	1824	rBV	6201	8337	2.10%	0.349%




Sum of corrected areas: 2391464

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101124\
Data File : VX043366.D
Acq On : 11 Oct 2024 15:37
Operator : JC/MD
Sample : P4396-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WASTE-WATER-FRAC-TANK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

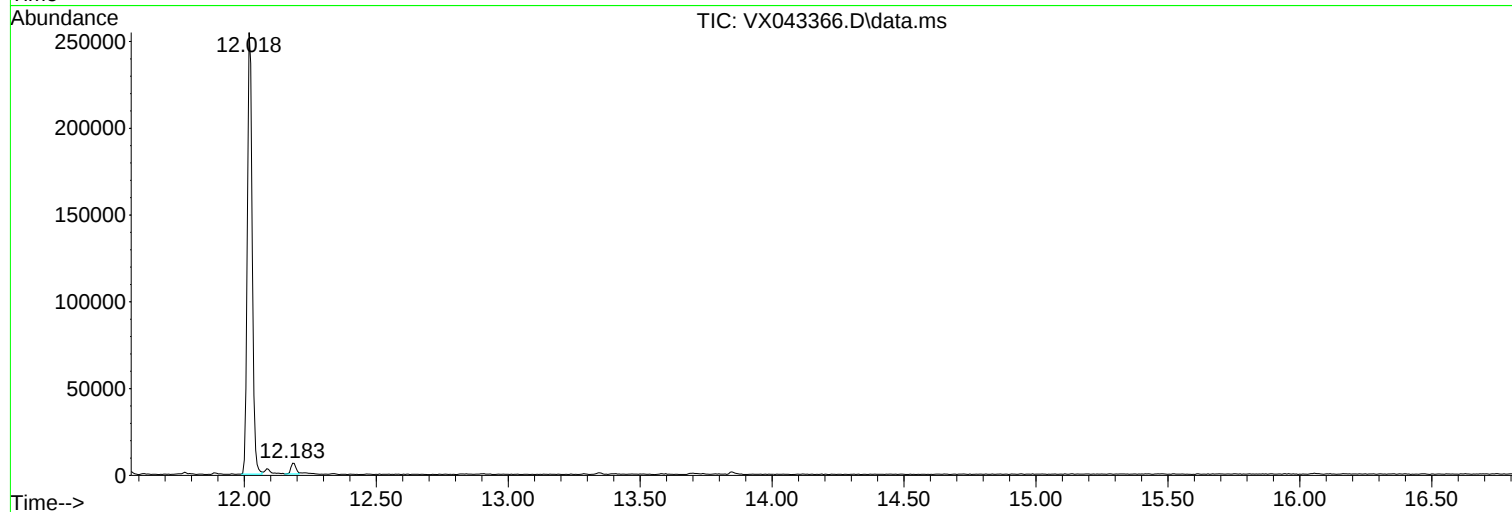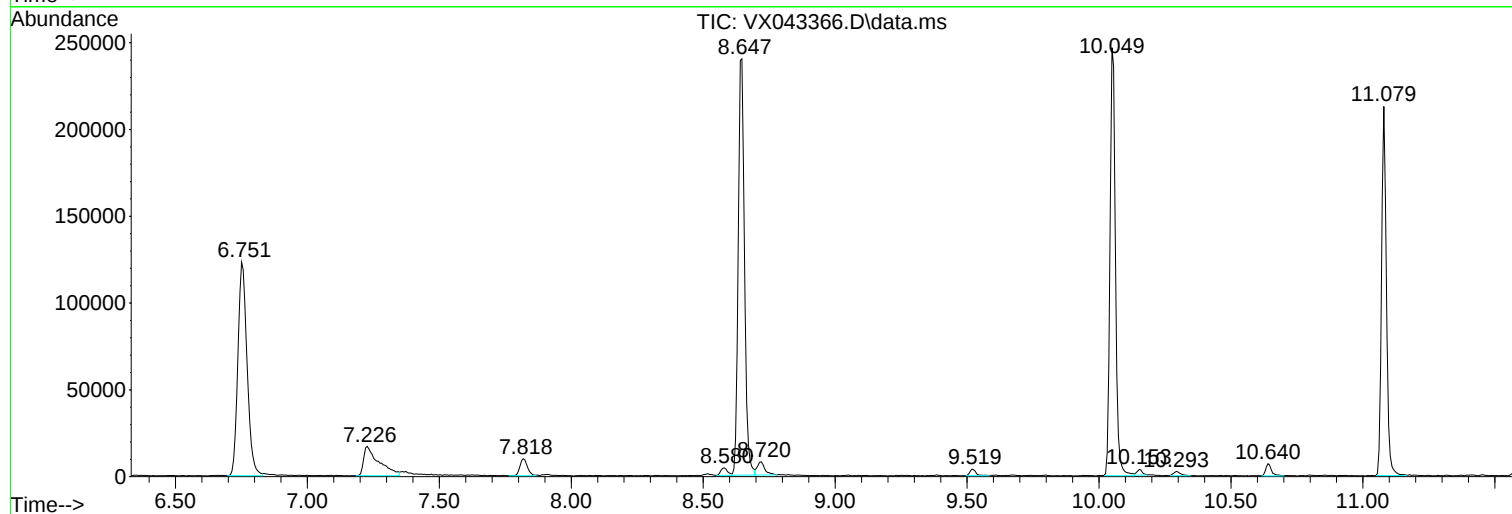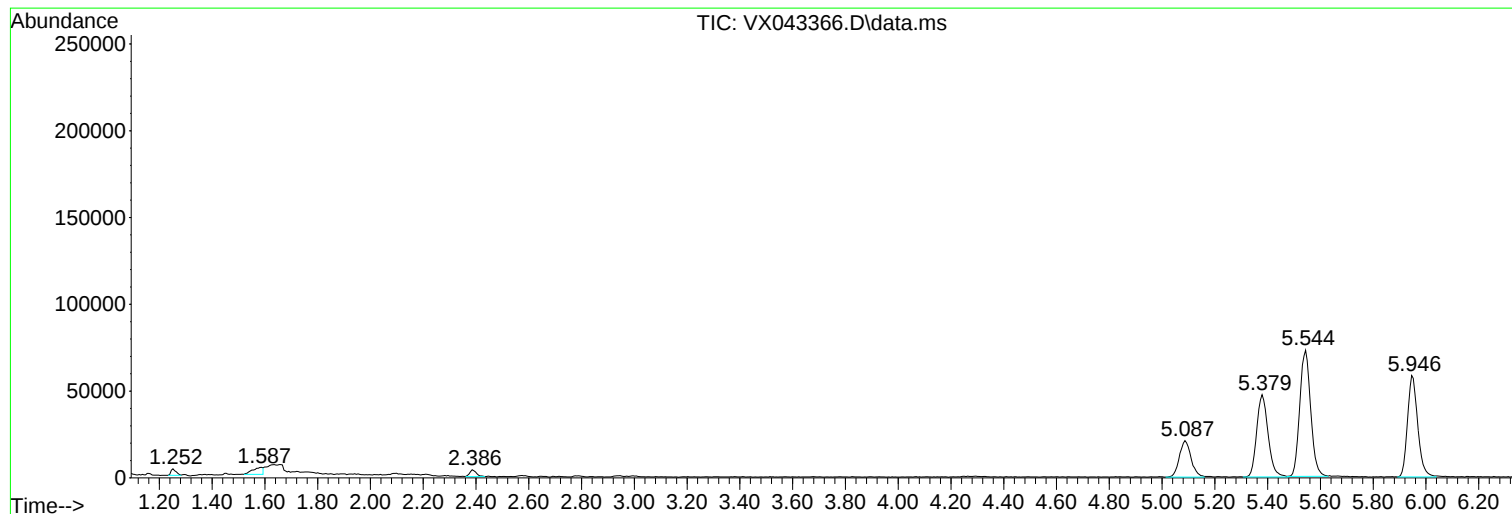

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101124\
Data File : VX043366.D
Acq On : 11 Oct 2024 15:37
Operator : JC/MD
Sample : P4396-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WASTE-WATER-FRAC-TANK










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1-Butanol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.226	11.36 ug/l	67398	1,4-Difluorobenzene	6.751

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Butanol			74	C4H10O	000071-36-3	78
2	Oxetane, 3,3-dimethyl-			86	C5H10O	006921-35-3	36
3	Oxirane, 2-methyl-3-(1-methyleth...			100	C6H12O	001192-31-0	36
4	Butane, 1-chloro-			92	C4H9Cl	000109-69-3	36
5	1-Pentanol, 4-methyl-			102	C6H14O	000626-89-1	9

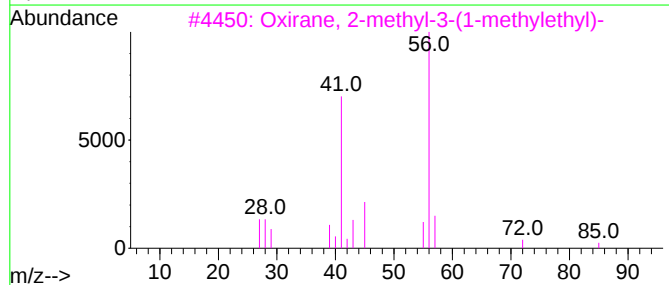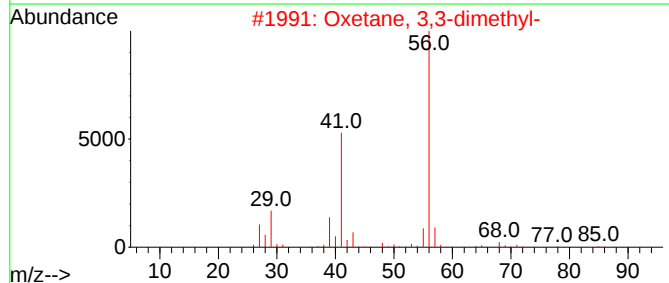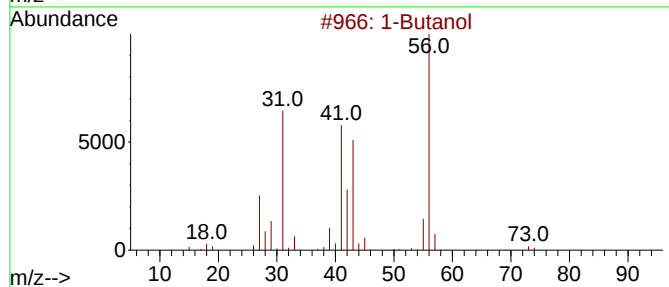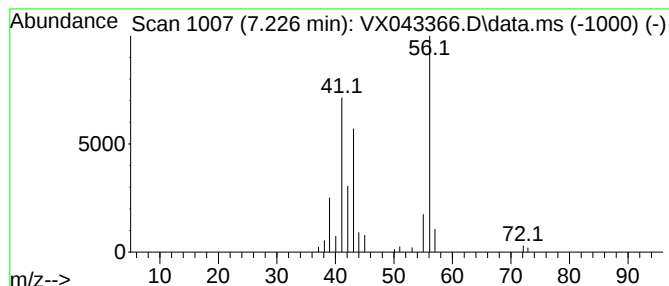

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101124\
Data File : VX043366.D
Acq On : 11 Oct 2024 15:37
Operator : JC/MD
Sample : P4396-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WASTE-WATER-FRAC-TANK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Butanol	7.226	11.4	ug/l	67398	2	6.751	296600	50.0