




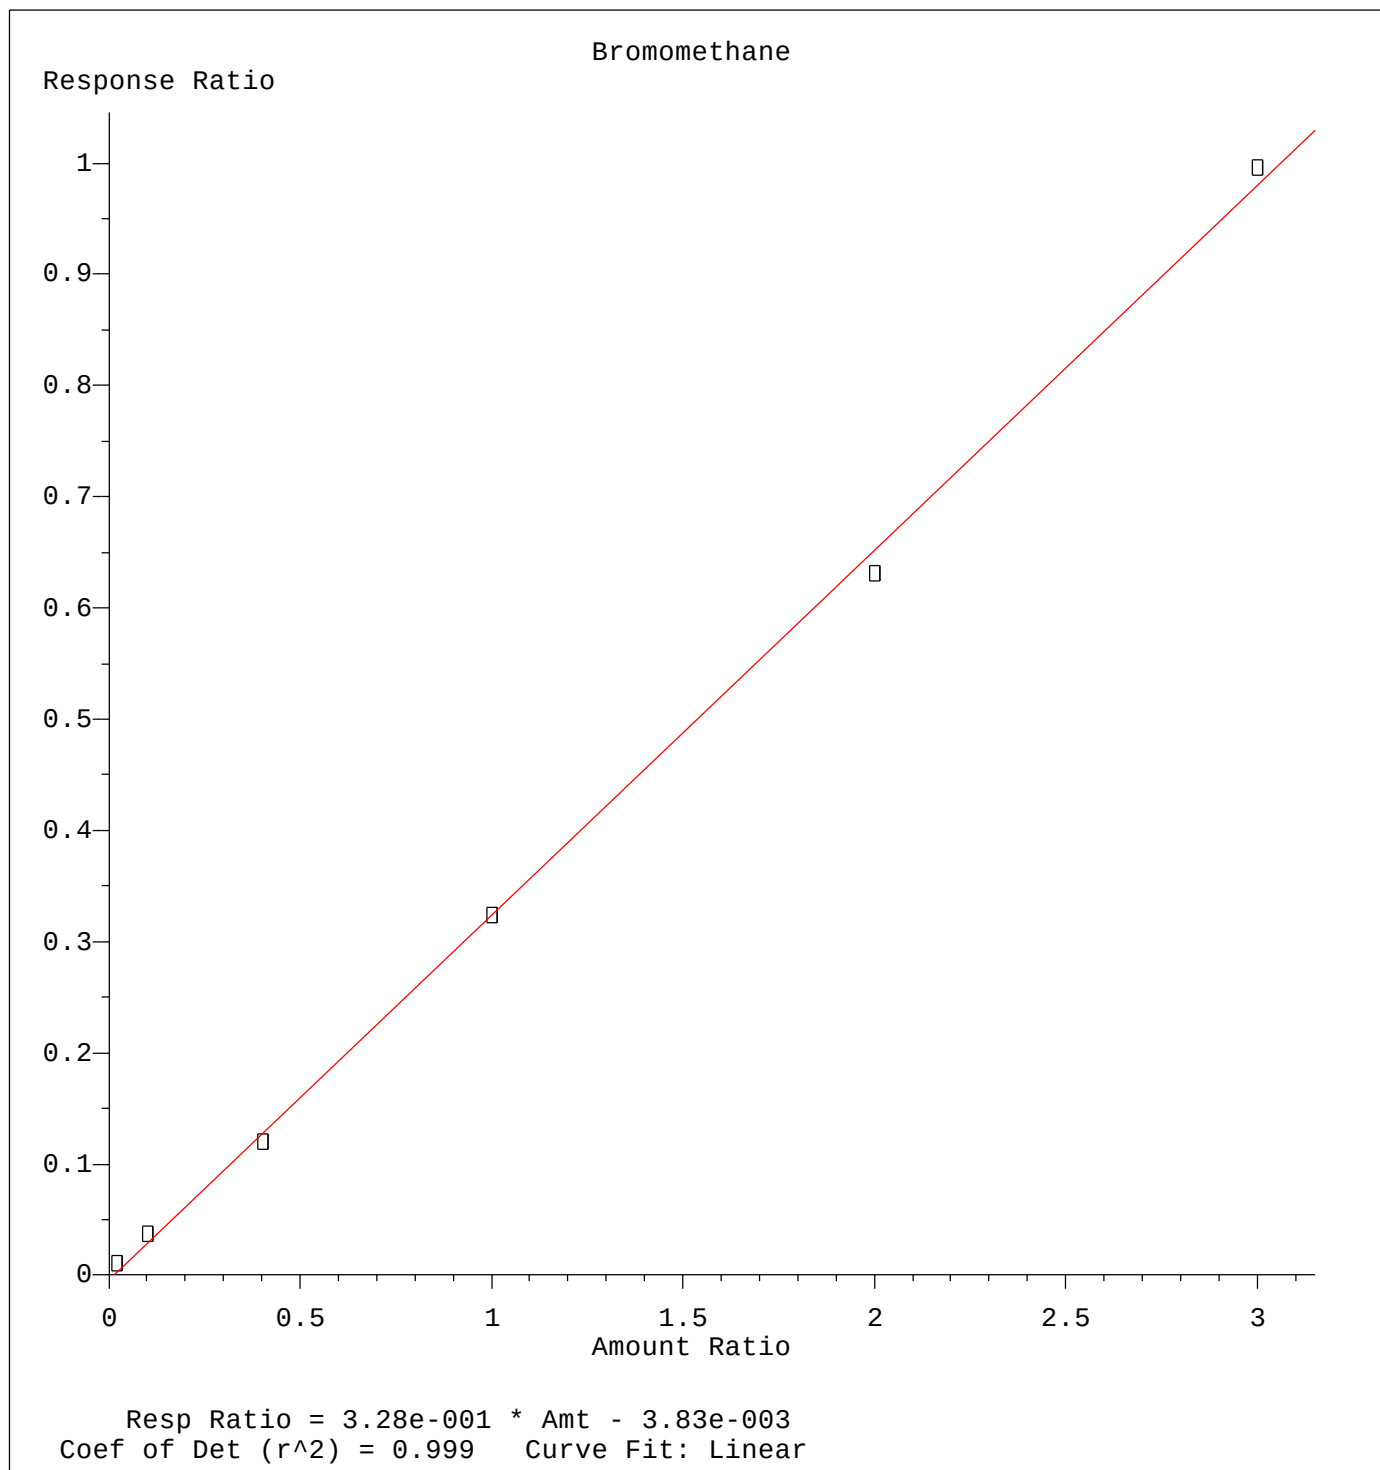


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X101218W.M
Calibration Table Last Updated: Fri Oct 12 11:28:43 2018

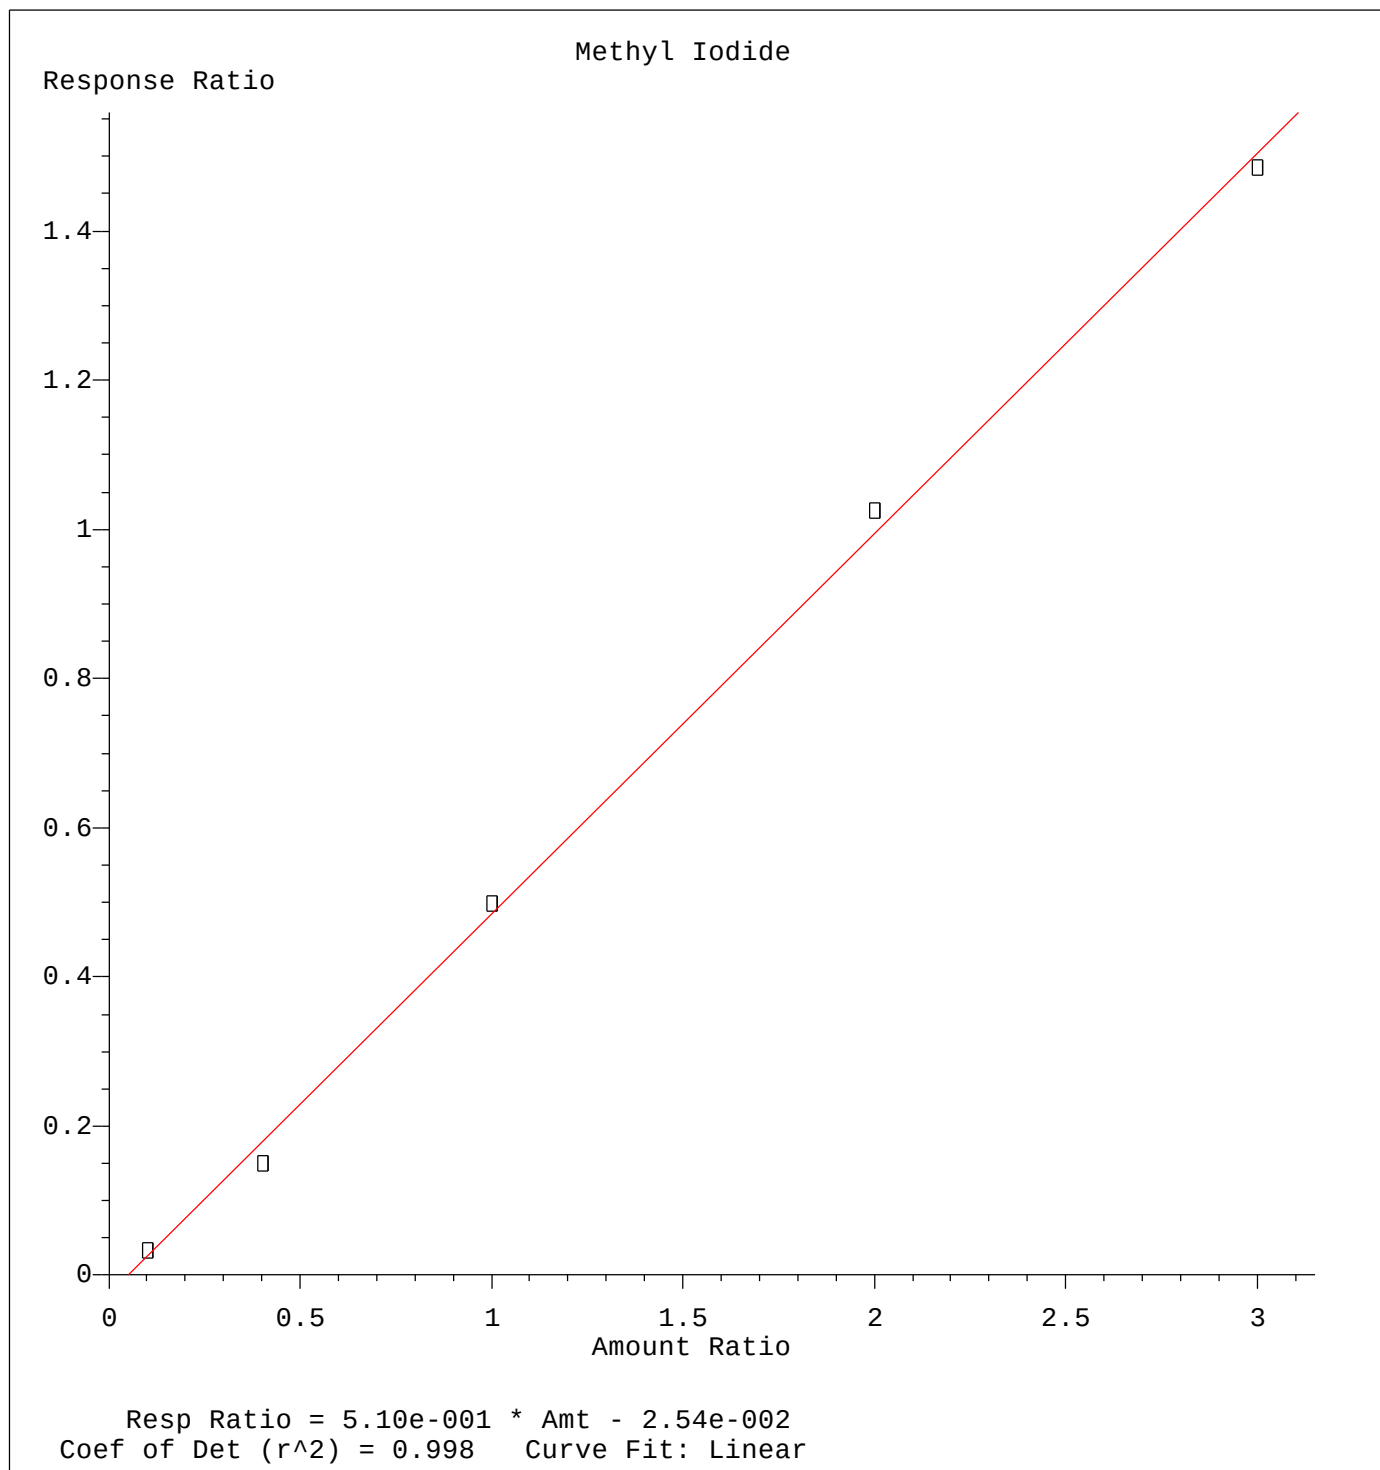

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X101218W.M
Calibration Table Last Updated: Fri Oct 12 11:28:43 2018

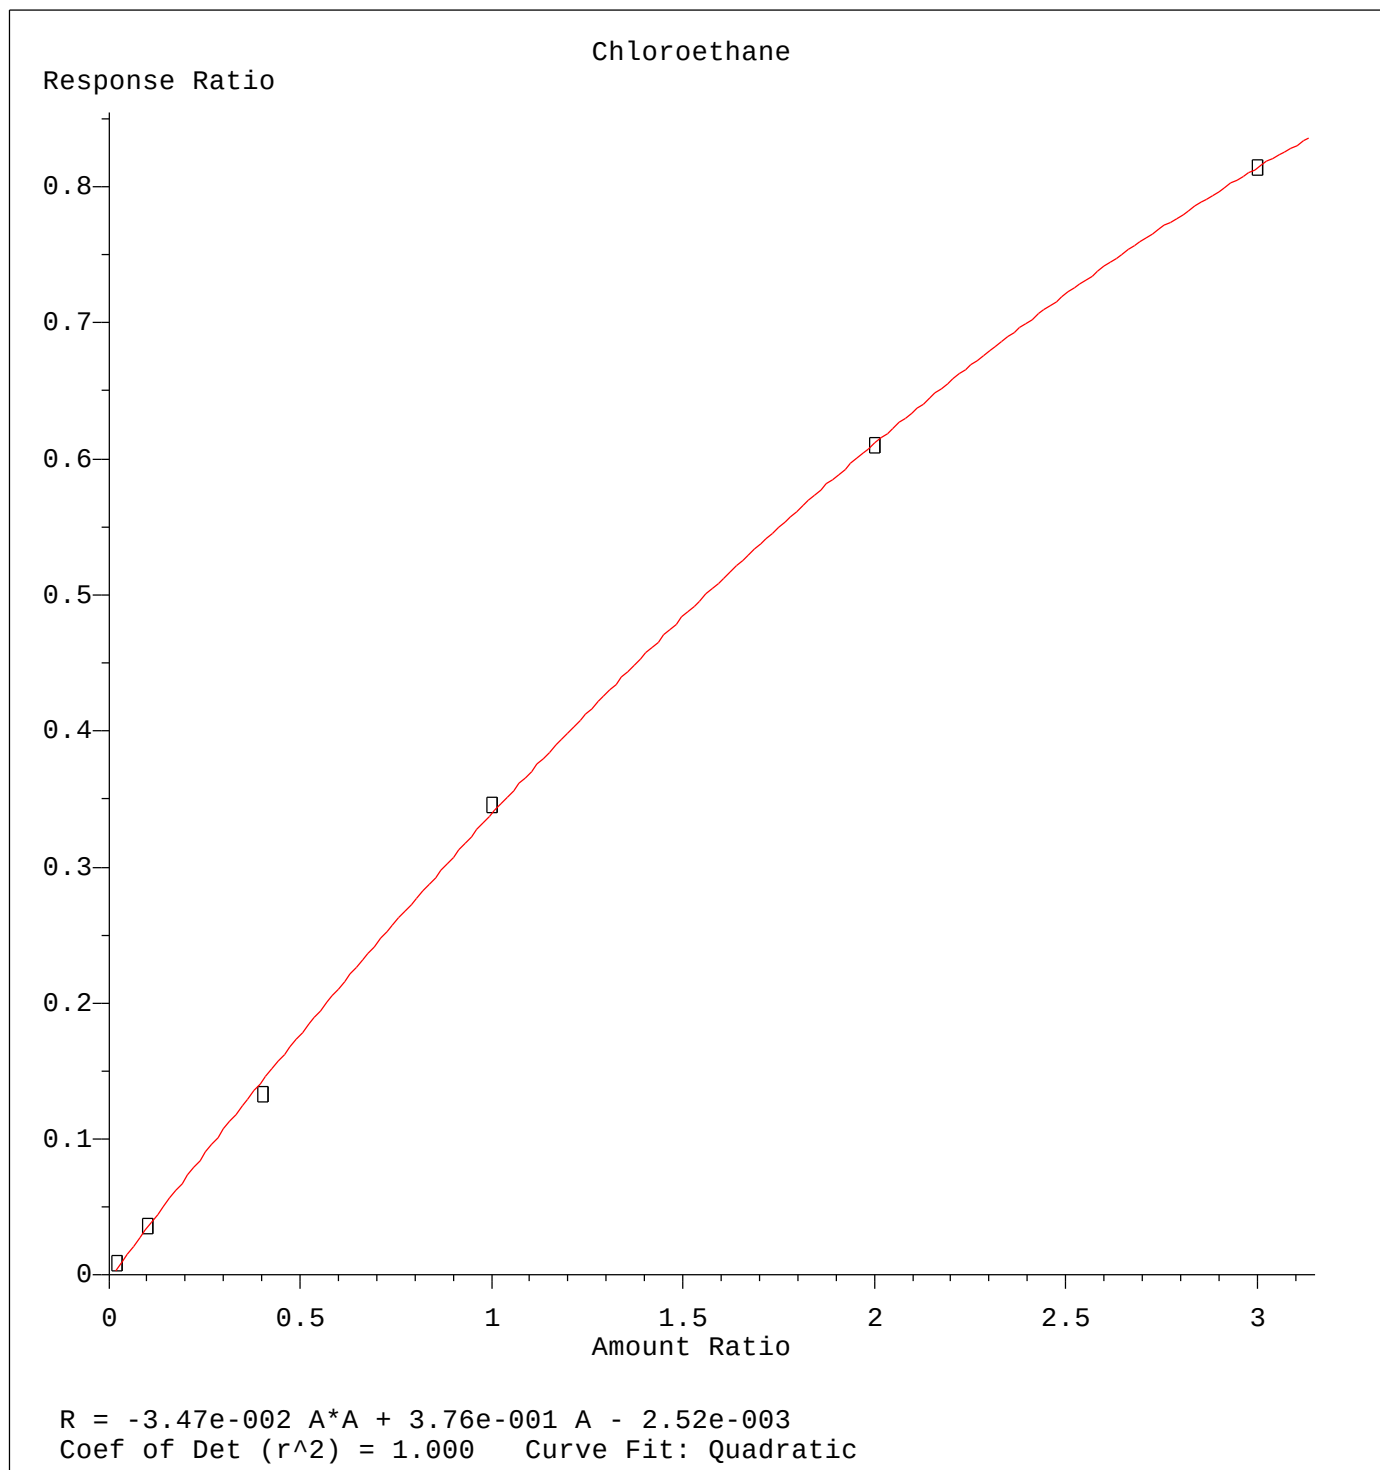


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X101218W.M
Calibration Table Last Updated: Fri Oct 12 11:28:43 2018

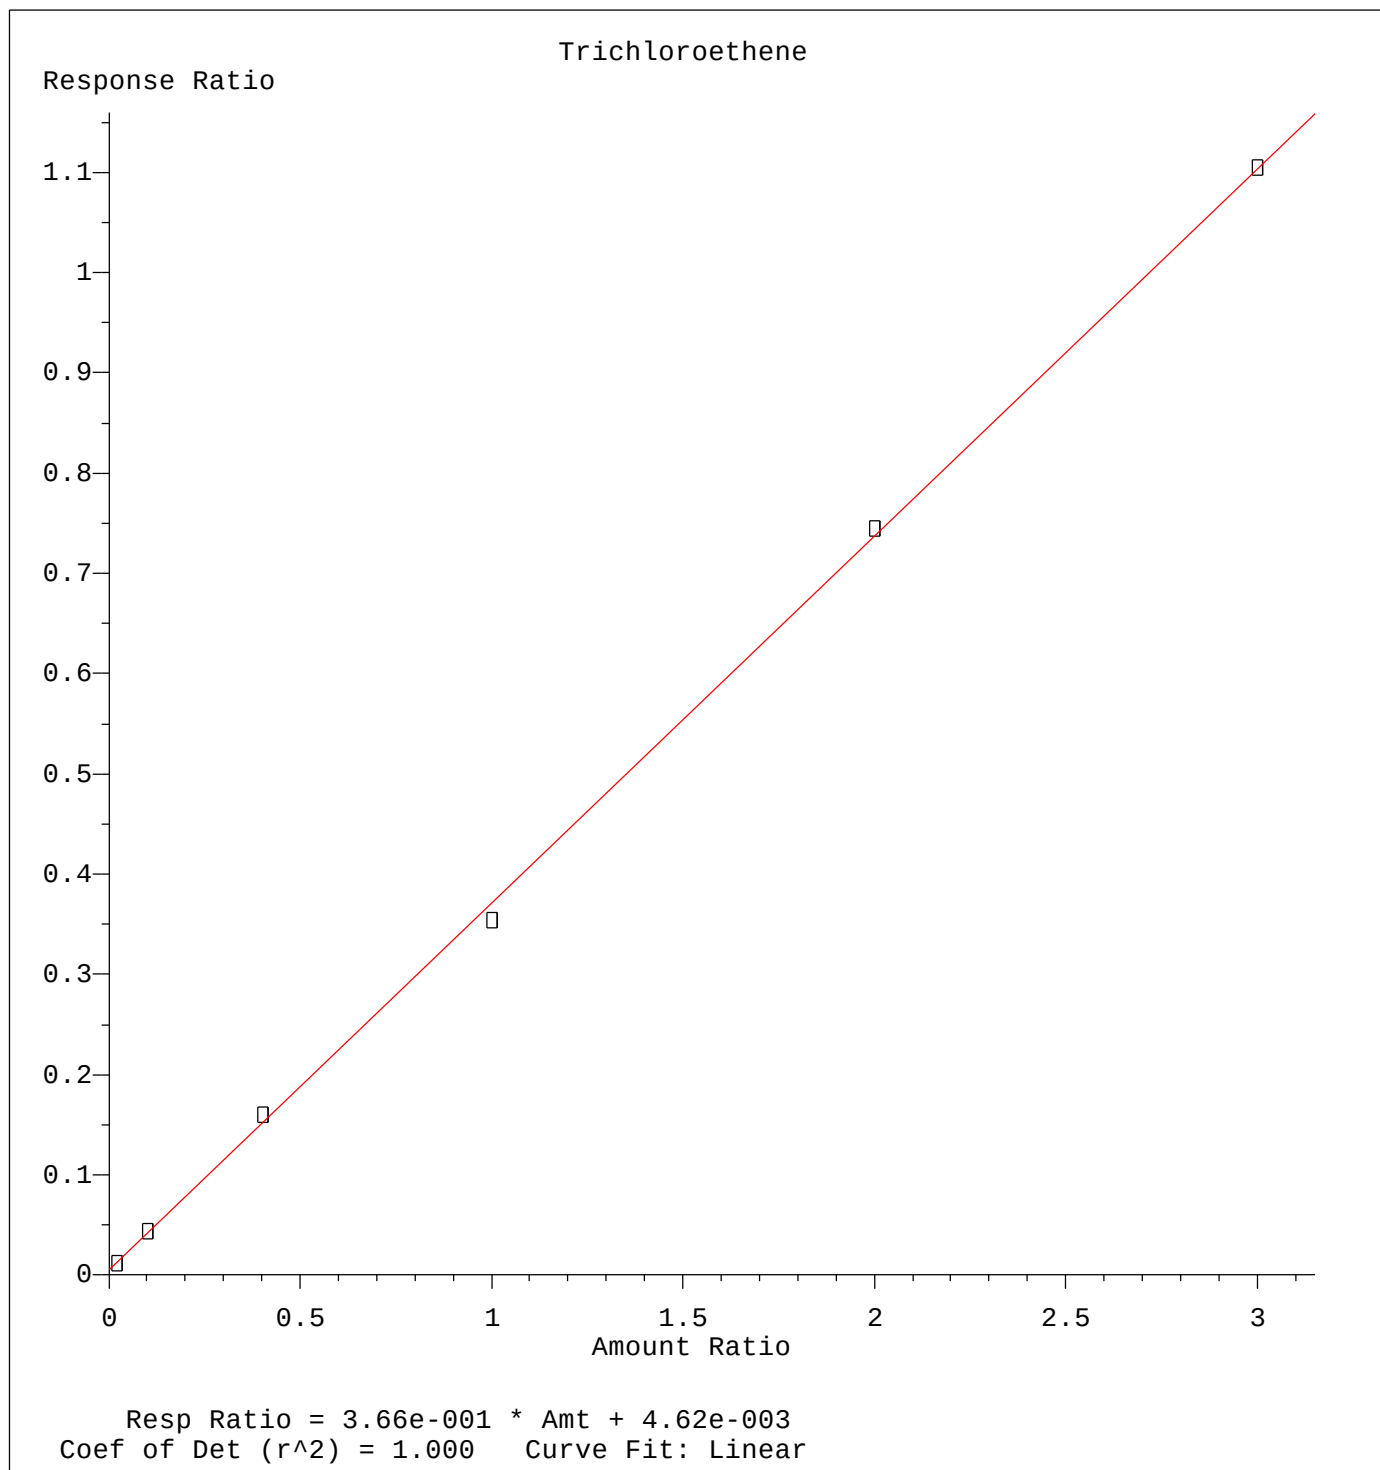

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X101218W.M
Calibration Table Last Updated: Fri Oct 12 11:28:43 2018


Methylene Chloride

Response Ratio

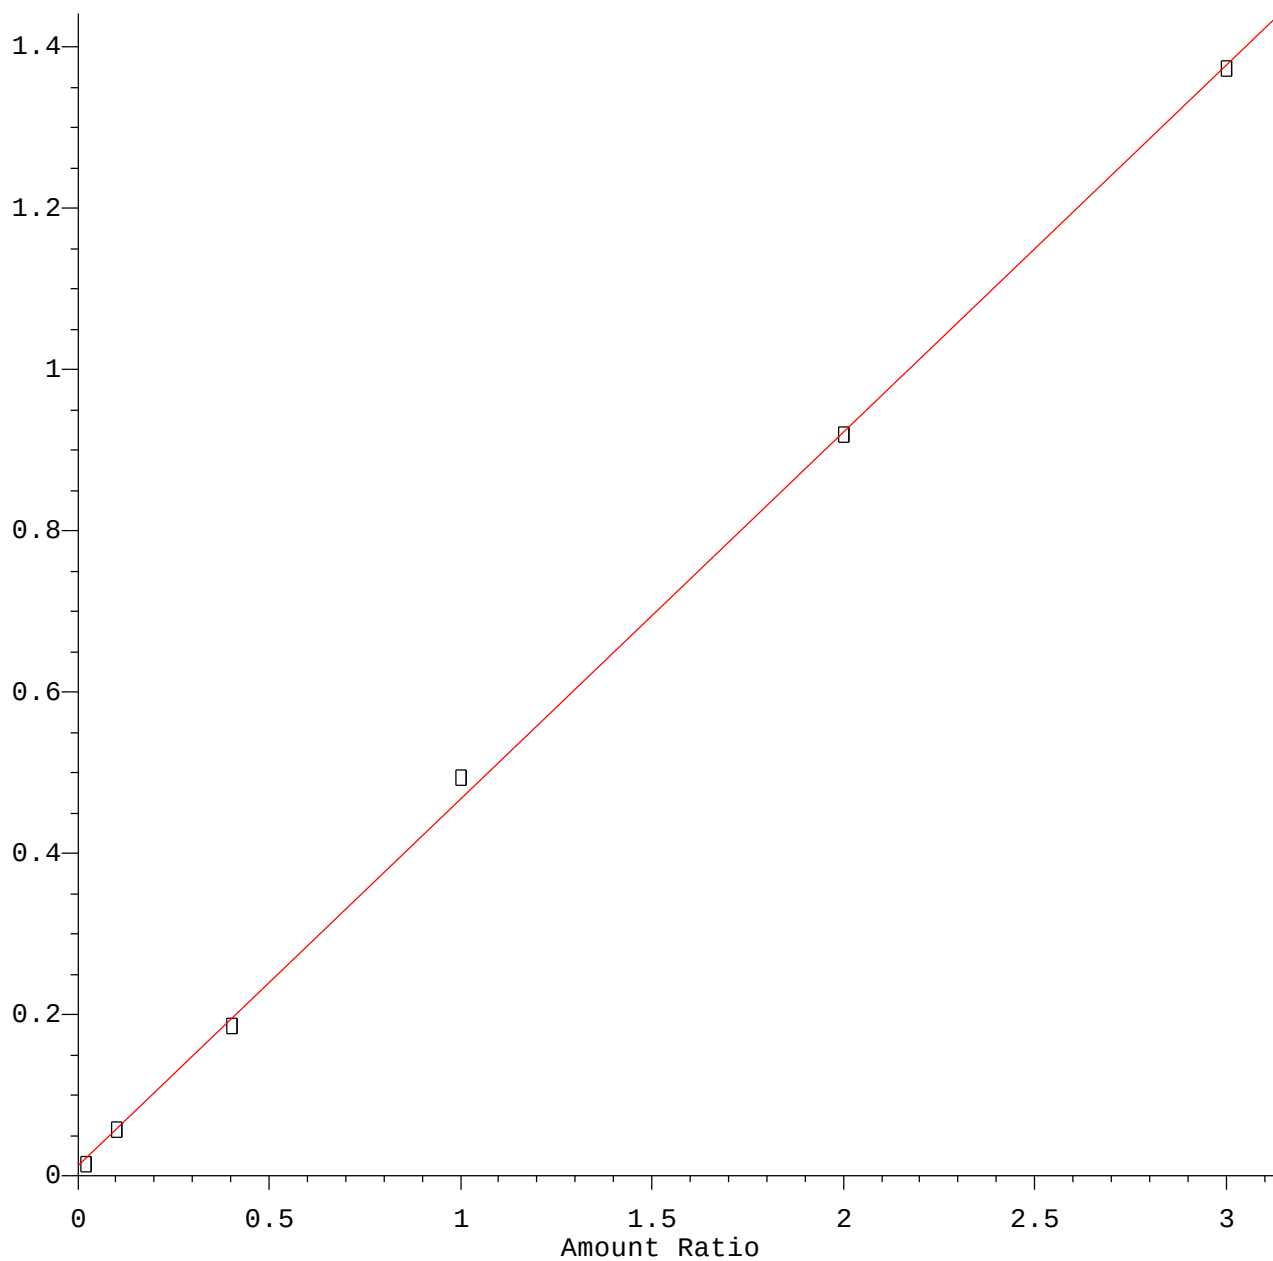

Resp Ratio = $4.55 \times 10^{-1} \times \text{Amt} + 1.22 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X101218W.M
Calibration Table Last Updated: Fri Oct 12 11:28:43 2018

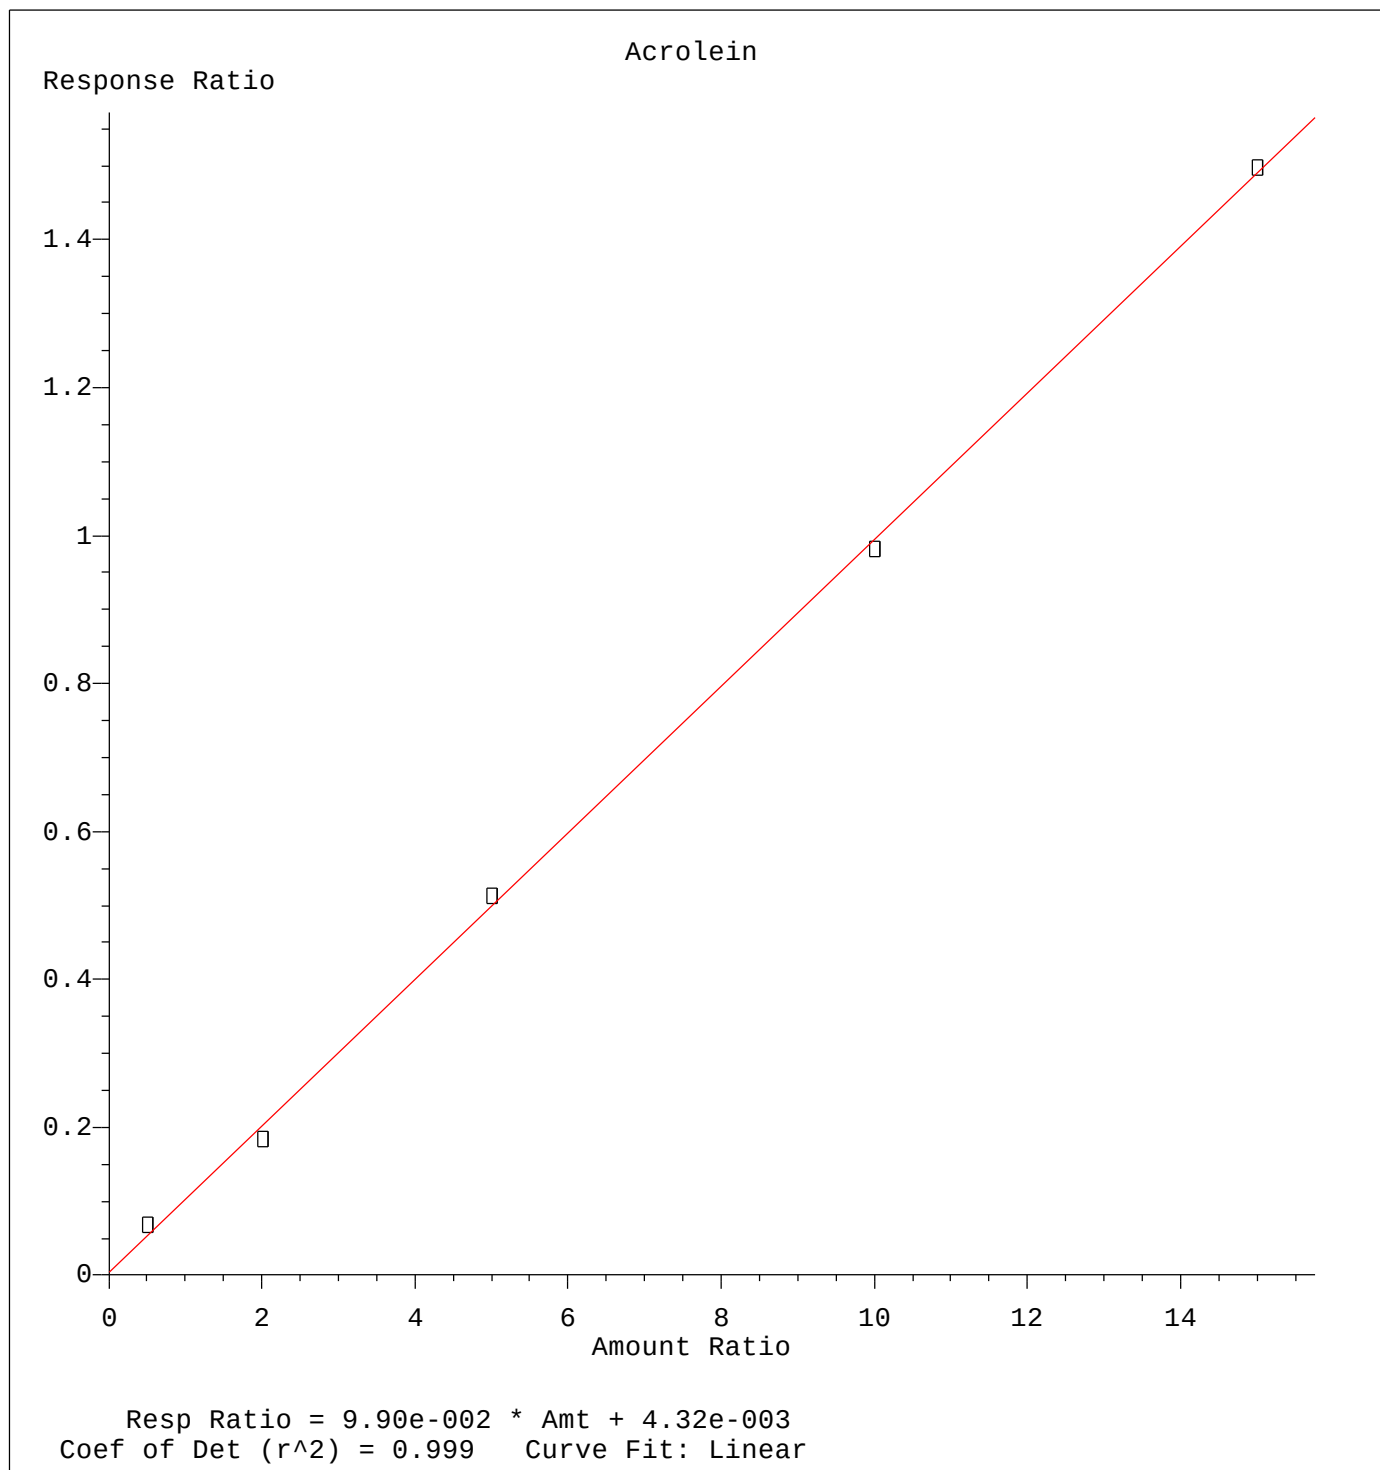

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X101218W.M
Calibration Table Last Updated: Fri Oct 12 11:28:43 2018