


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101218\
Data File : VX005280.D
Acq On : 12 Oct 2018 08:13
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X101218W.M
Title : SW846 8260
Last Update : Fri Oct 12 11:28:43 2018

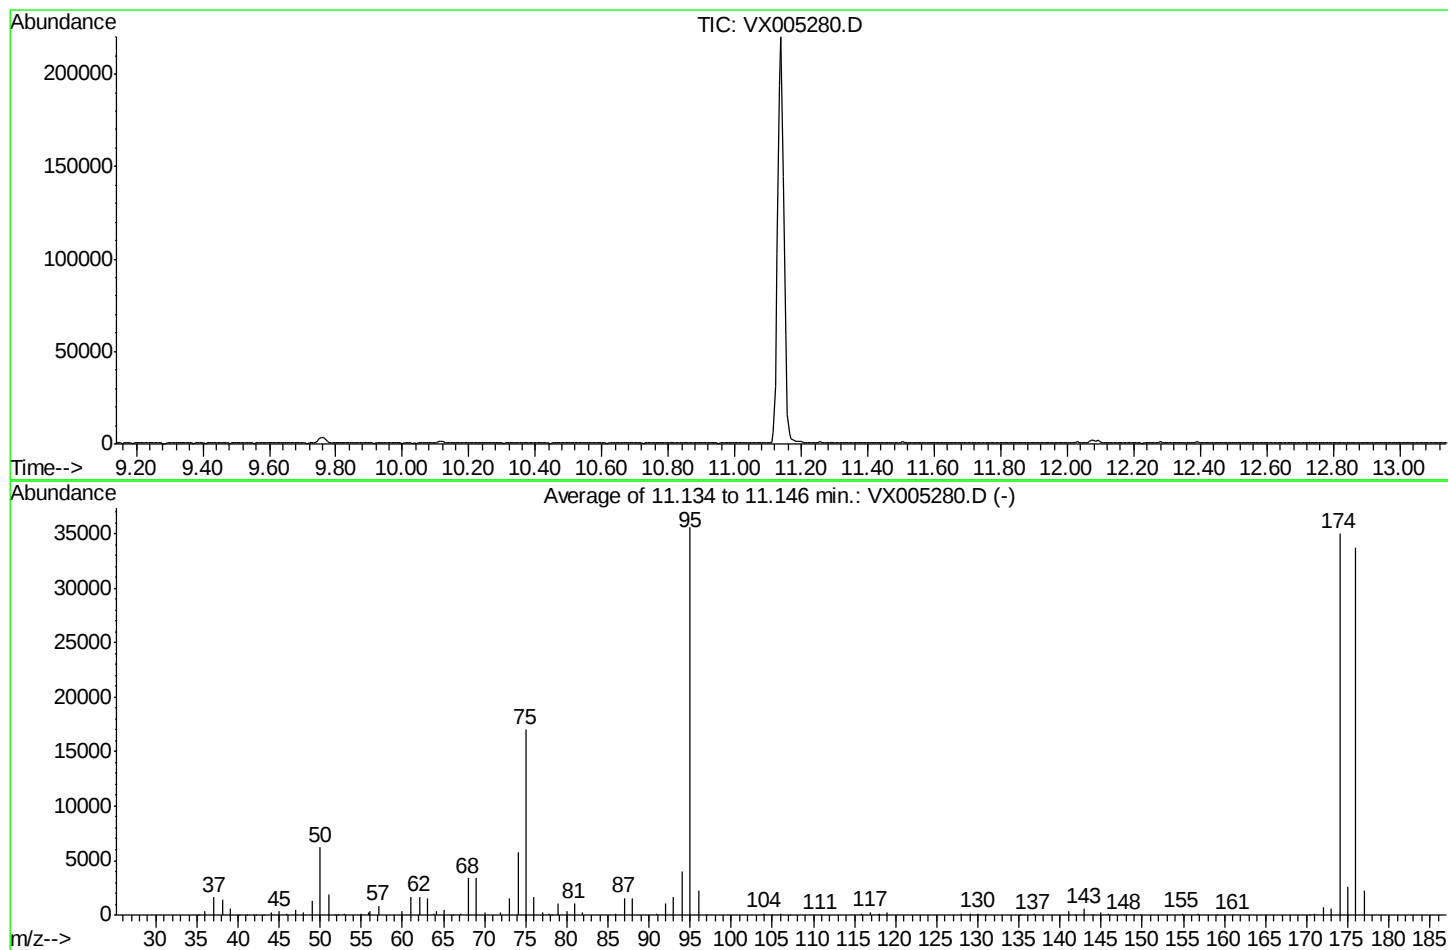

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	6188	PASS
75	95	30	60	47.7	16994	PASS
95	95	100	100	100.0	35610	PASS
96	95	5	9	6.4	2291	PASS
173	174	0.00	2	1.5	541	PASS
174	95	50	100	98.3	35000	PASS
175	174	5	9	7.4	2594	PASS
176	174	95	101	96.5	33786	PASS
177	176	5	9	6.7	2252	PASS