

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX101220\
 Data File : VX018901.D
 Acq On : 12 Oct 2020 14:28
 Operator : JC/SP
 Sample : L4344-02DL 100X
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WASTE-ROOM-SAMPLEDL

Quant Time: Oct 13 04:07:32 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X100920W.M
 Quant Title : SW846 8260
 QLast Update : Sat Oct 10 06:09:09 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	269290	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	428074	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	395432	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	211370	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.03	65	203554	51.25	ug/l	0.00
Spiked Amount			Recovery	=	102.50%	
35) Dibromofluoromethane	5.46	113	148596	48.71	ug/l	0.00
Spiked Amount			Recovery	=	97.42%	
50) Toluene-d8	8.70	98	495730	46.85	ug/l	0.00
Spiked Amount			Recovery	=	93.70%	
62) 4-Bromofluorobenzene	11.12	95	186780	44.29	ug/l	0.00
Spiked Amount			Recovery	=	88.58%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Dichlorodifluoromethane	1.18	85	112	1.653	ug/l	89
3) Chloromethane	1.32	50	713	0.282	ug/l #	65
5) Bromomethane	1.63	94	936	0.596	ug/l #	79
8) Diethyl Ether	2.17	74	124	1.108	ug/l #	3
10) Methyl Iodide	2.50	142	956	4.305	ug/l #	92
11) Tert butyl alcohol	2.99	59	6593	10.540	ug/l #	78
12) 1,1-Dichloroethene	2.34	96	347	0.842	ug/l #	1
13) Acrolein	2.28	56	680	1.307	ug/l #	24
14) Allyl chloride	2.68	41	1479970	328.219	ug/l #	39
15) Acrylonitrile	3.11	53	743	0.560	ug/l #	68
16) Acetone	2.42	43	2289	Below Cal	#	86
17) Carbon Disulfide	2.55	76	1732	0.238	ug/l #	63
18) Methyl Acetate	2.75	43	501338	151.846	ug/l	97
20) Methylene Chloride	2.82	84	870	0.808	ug/l #	73
28) Bromochloromethane	4.98	49	142	1.579	ug/l #	24
31) Cyclohexane	5.63	56	6181	1.666	ug/l #	7
36) 1,1-Dichloropropene	5.64	75	21857	4.856	ug/l #	51
38) Carbon Tetrachloride	5.62	117	26900	4.822	ug/l #	19
49) 1,4-Dioxane	7.73	88	186	3.619	ug/l #	36
56) Ethyl methacrylate	9.19	69	40	2.942	ug/l #	1
64) Tetrachloroethene	9.32	164	146	Below Cal	#	66
76) 1,2,3-Trichloropropane	11.12	75	94517	20.753	ug/l #	37
81) trans-1,4-Dichloro-2-buten	11.12	75	94517	58.813	ug/l #	7
93) 1,2,4-Trichlorobenzene	13.63	180	878	0.206	ug/l	90
94) Hexachlorobutadiene	13.77	225	583	0.308	ug/l	83
95) Naphthalene	13.82	128	1564	3.180	ug/l #	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX101220\
Data File : VX018901.D
Acq On : 12 Oct 2020 14:28
Operator : JC/SP
Sample : L4344-02DL 100X
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WASTE-ROOM-SAMPLEDL

Quant Time: Oct 13 04:07:32 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X100920W.M
Quant Title : SW846 8260
QLast Update : Sat Oct 10 06:09:09 2020
Response via : Initial Calibration

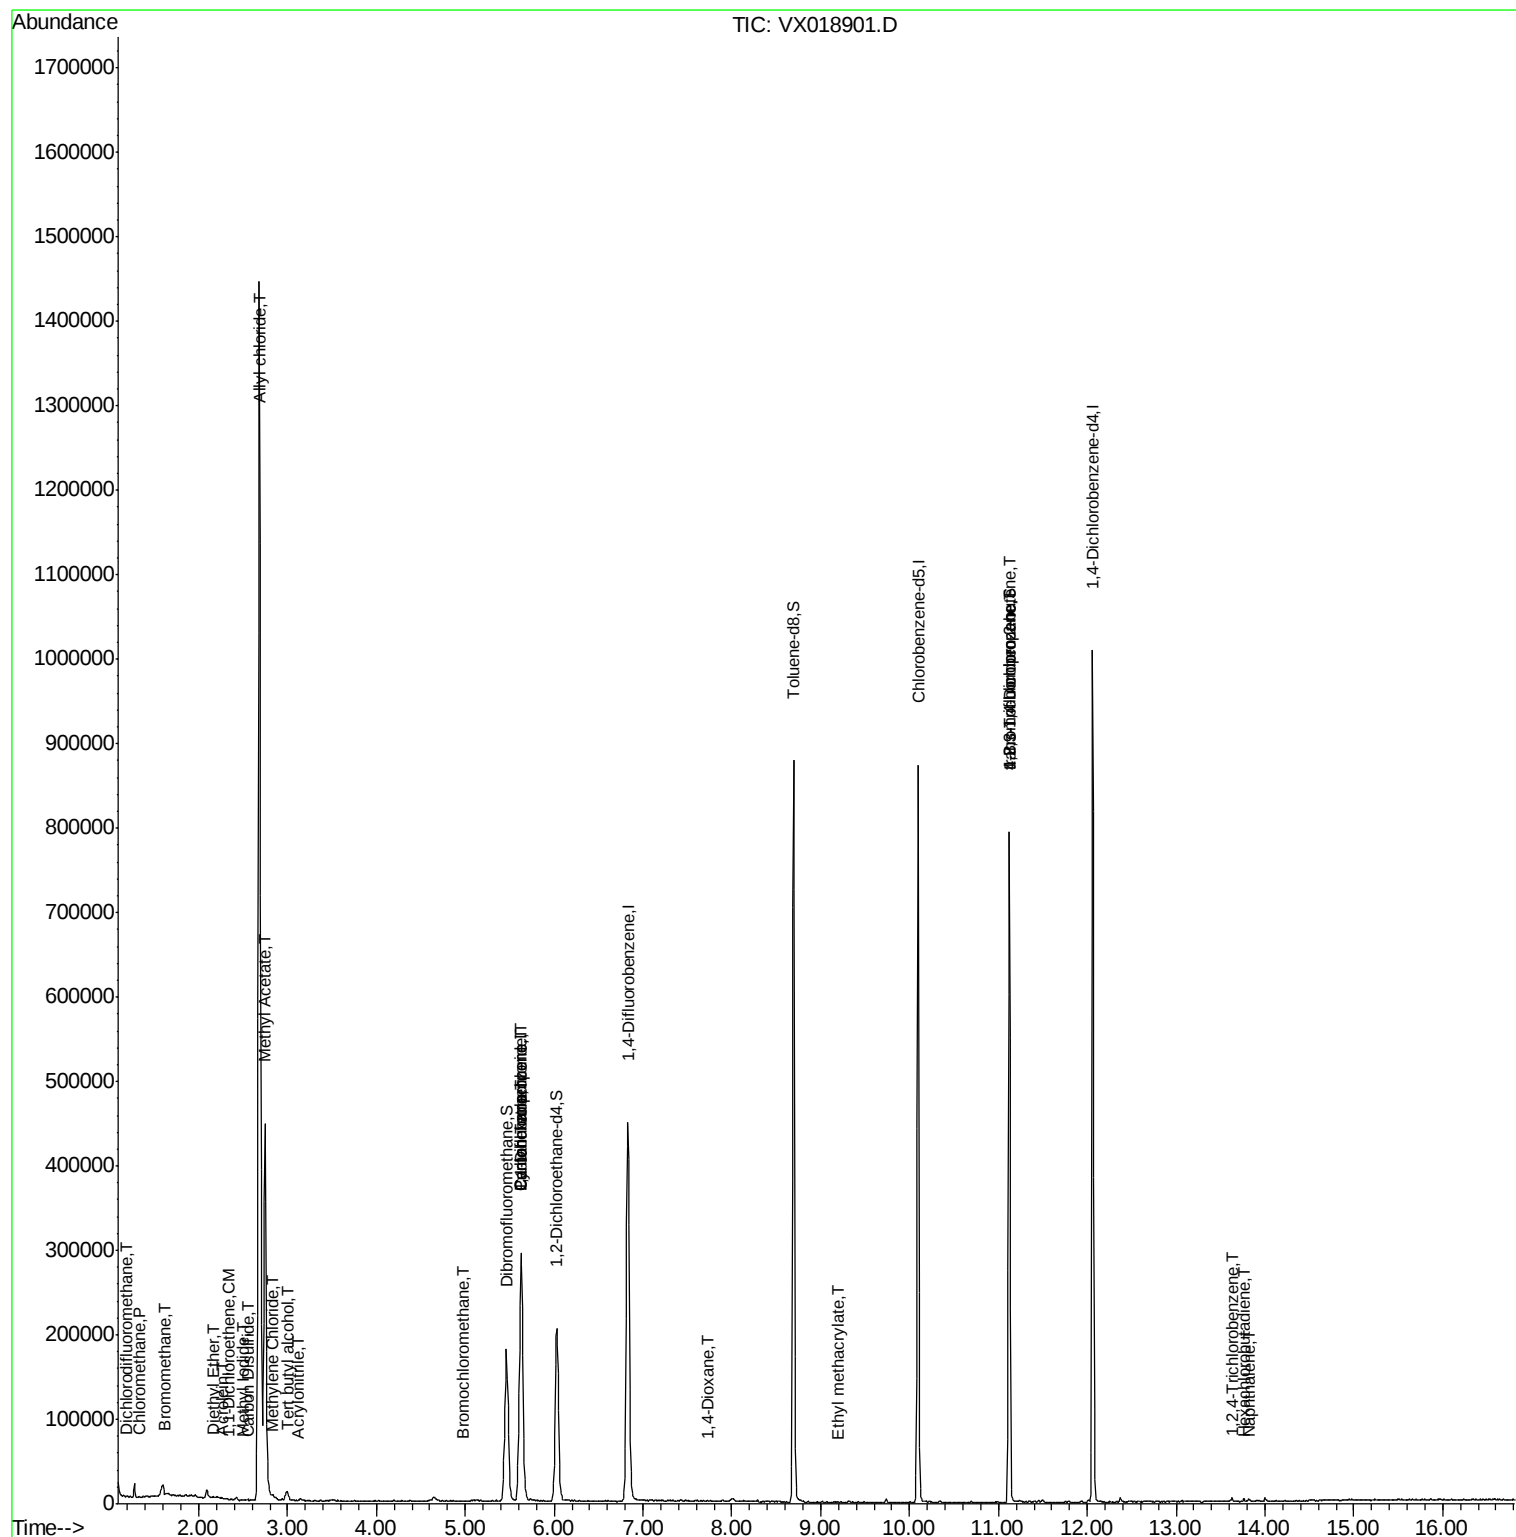







#1

Pentafluorobenzene
 Concen: 50.000 ug/l
 RT: 5.63 min Scan# 745
 Delta R.T. -0.01 min
 Lab File: VX018901.D
 Acq: 12 Oct 2020 14:28

Instrument :
 MSVOA_X
 ClientSampleId :
 WASTE-ROOM-SAMPLEDL




Tot Ion:168 Resp: 269290
 Ion Ratio Lower Upper
 168 100
 99 55.4 46.1 69.1

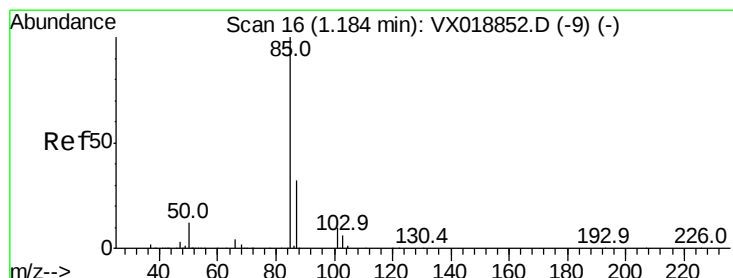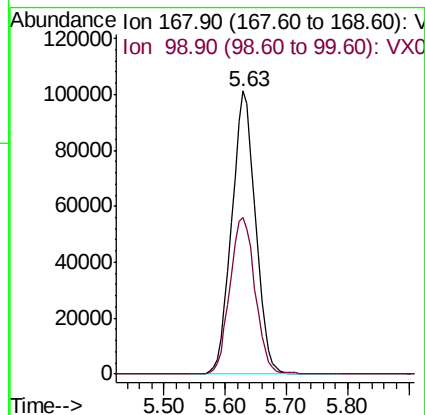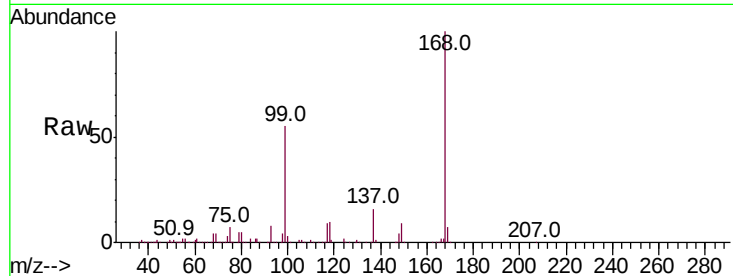


#2

Dichlorodifluoromethane
 Concen: 1.653 ug/l
 RT: 1.18 min Scan# 16
 Delta R.T. 0.00 min
 Lab File: VX018901.D
 Acq: 12 Oct 2020 14:28

Tgt Ion: 85 Resp: 112
 Ion Ratio Lower Upper
 85 100
 87 38.0 15.9 47.7

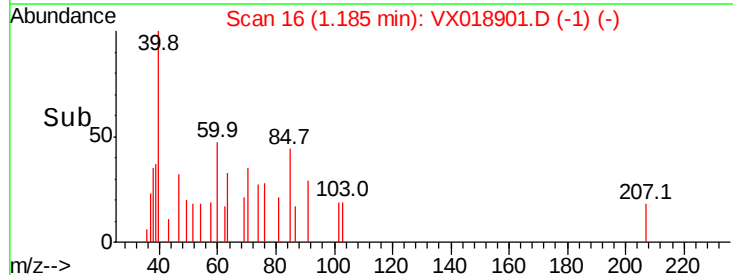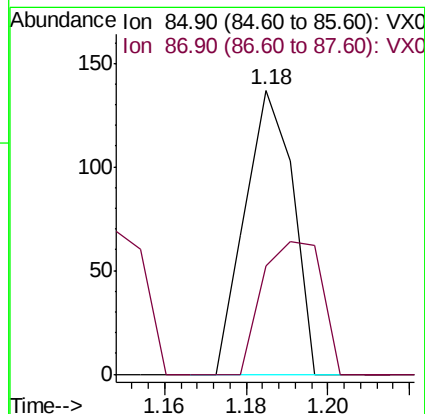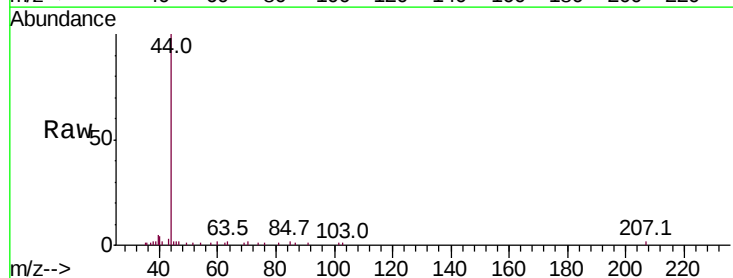

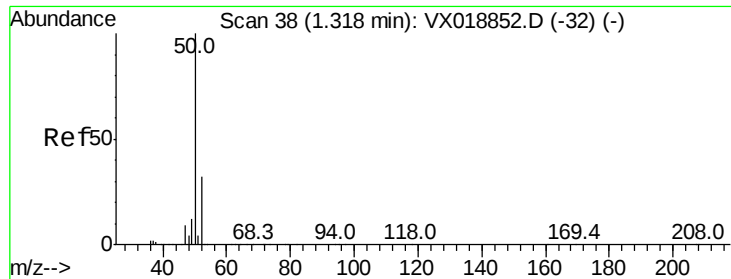

#3

Chloromethane

Concen: 0.282 ug/l

RT: 1.32 min Scan# 38

Delta R.T. 0.00 min

Lab File: VX018901.D

Acq: 12 Oct 2020 14:28

Instrument :

MSVOA_X

ClientSampleId :





WASTE-ROOM-SAMPLEDL

Tot Ion: 50 Resp: 713

Ion Ratio Lower Upper

50 100

52 50.8 25.2 37.8#

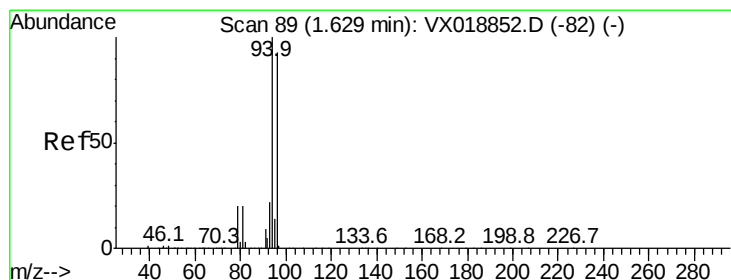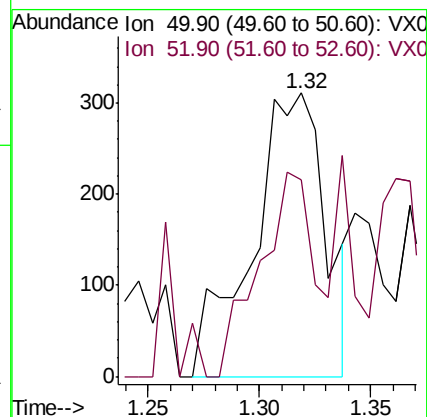

#5

Bromomethane

Concen: 0.596 ug/l

RT: 1.63 min Scan# 89

Delta R.T. 0.00 min

Lab File: VX018901.D




Acq: 12 Oct 2020 14:28


Tgt Ion: 94 Resp: 936

Ion Ratio Lower Upper

94 100

96 73.4 74.5 111.7#

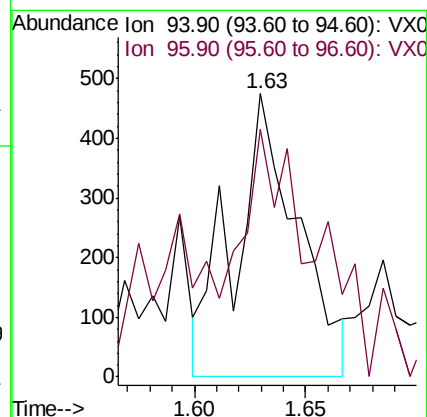

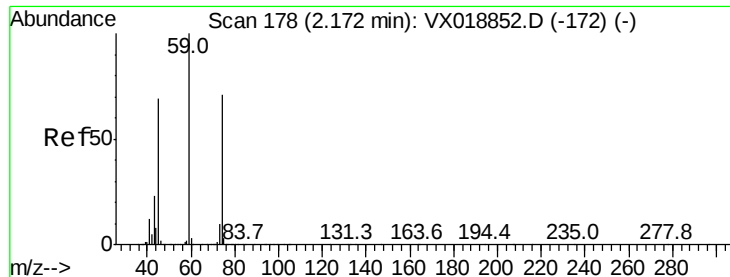

#8

Diethyl Ether

Concen: 1.108 ug/l

RT: 2.17 min Scan# 177

Delta R.T. -0.00 min

Lab File: VX018901.D

Acq: 12 Oct 2020 14:28


Instrument :
MSVOA_X
ClientSampleId :
WASTE-ROOM-SAMPLEDL

Tot Ion: 74 Resp: 124




Ion Ratio Lower Upper

74 100

45 0.0 47.0 141.2#

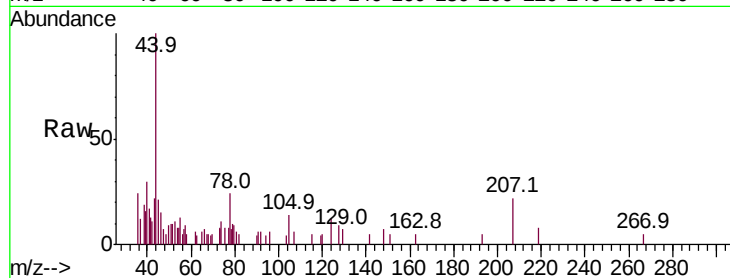

Abundance Ion 74.00 (73.70 to 74.70): VX0

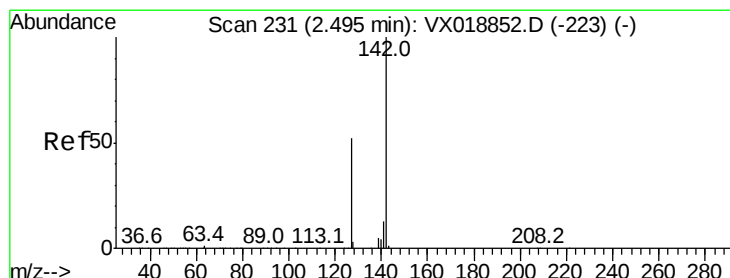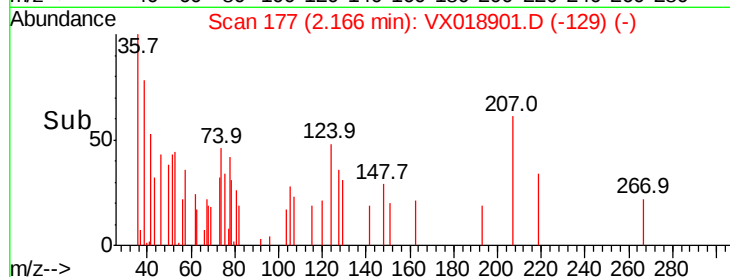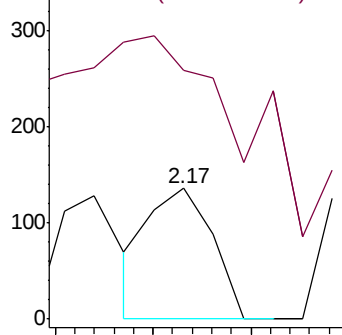

#10

Methyl Iodide

Concen: 4.305 ug/l

RT: 2.50 min Scan# 232

Delta R.T. 0.01 min

Lab File: VX018901.D

Acq: 12 Oct 2020 14:28


Tgt Ion: 142 Resp: 956

Ion Ratio Lower Upper



142 100


127 49.2 42.0 63.0

141 6.5 11.8 17.6#

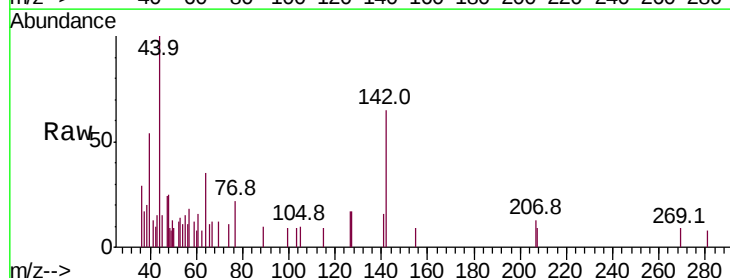

Abundance Ion 141.80 (141.50 to 142.50): V

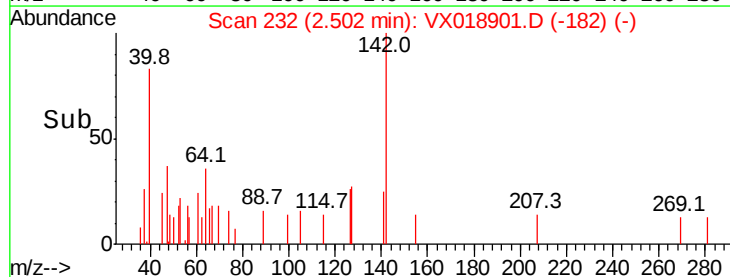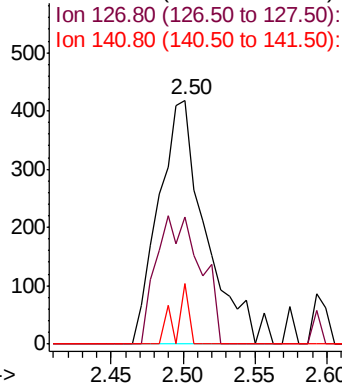







#11

Tert butyl alcohol
 Concen: 10.540 ug/l
 RT: 2.99 min Scan# 312
 Delta R.T. -0.02 min
 Lab File: VX018901.D
 Acq: 12 Oct 2020 14:28

Instrument :
 MSVOA_X
 ClientSampleId :
 WASTE-ROOM-SAMPLEDL




Tot Ion: 59 Resp: 6593
 Ion Ratio Lower Upper
 59 100
 57 2.9 9.0 13.6#

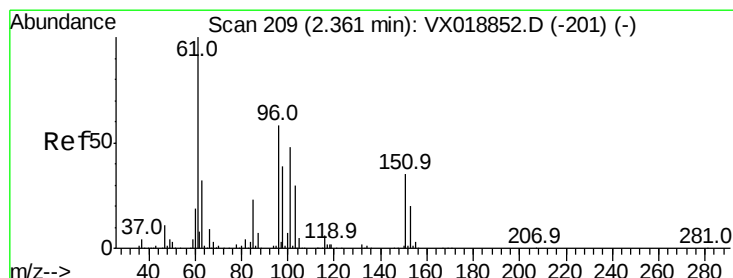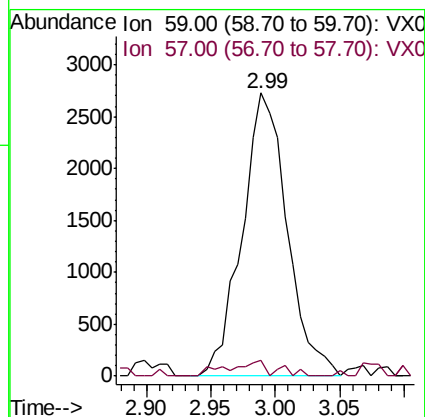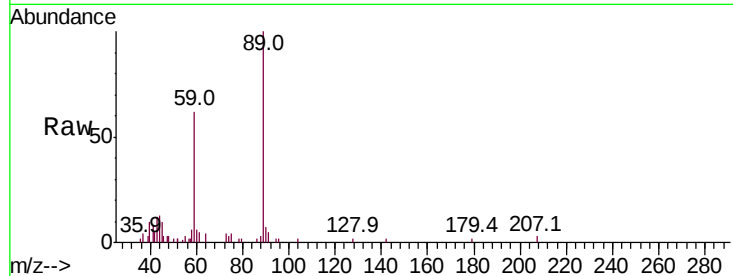


#12

1,1-Dichloroethene
 Concen: 0.842 ug/l
 RT: 2.34 min Scan# 206
 Delta R.T. -0.02 min
 Lab File: VX018901.D
 Acq: 12 Oct 2020 14:28

Tgt Ion: 96 Resp: 347
 Ion Ratio Lower Upper
 96 100
 61 14.0 137.0 205.6#
 98 0.0 53.9 80.9#



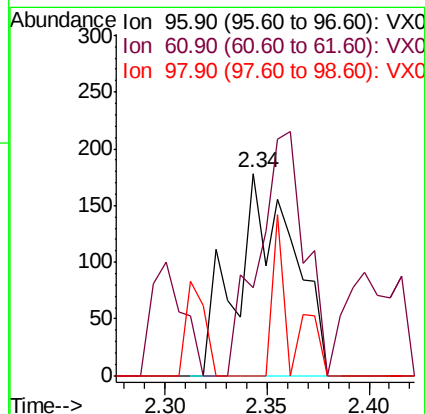
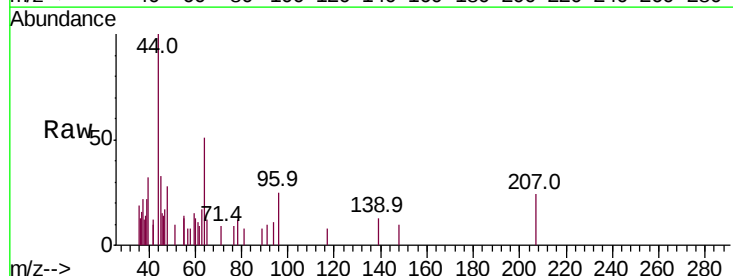




#13
Acrolein
Concen: 1.307 ug/l
RT: 2.28 min Scan# 195
Delta R.T. 0.00 min
Lab File: VX018901.D
Acq: 12 Oct 2020 14:28




Instrument :
MSVOA_X
ClientSampleId :
WASTE-ROOM-SAMPLEDL


Tot Ion: 56 Resp: 680
Ion Ratio Lower Upper
56 100
55 9.7 58.6 87.8#

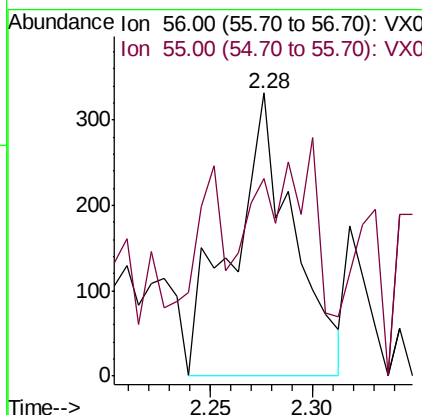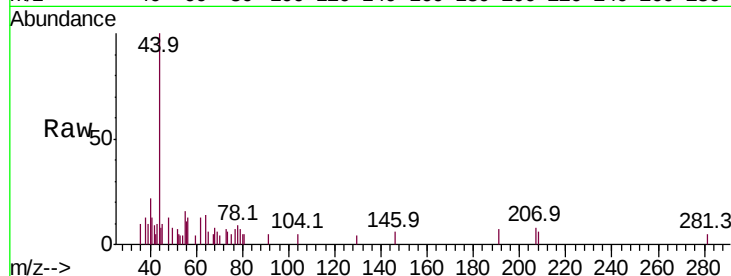

#14
Allyl chloride
Concen: 328.219 ug/l
RT: 2.68 min Scan# 262
Delta R.T. -0.02 min
Lab File: VX018901.D
Acq: 12 Oct 2020 14:28

Tgt Ion: 41 Resp: 1479970
Ion Ratio Lower Upper
41 100
39 20.1 57.8 86.8#
76 0.0 26.8 40.2#

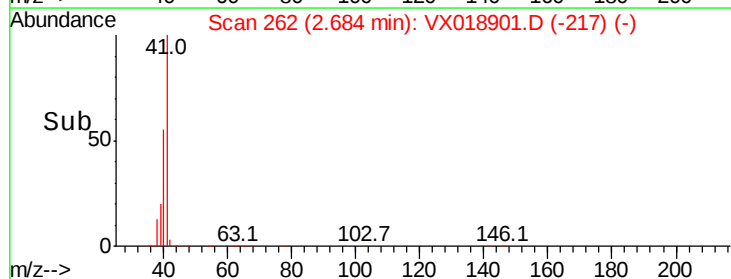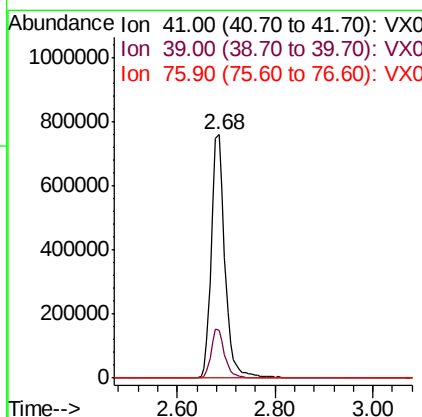



#15

Acrylonitrile

Concen: 0.560 ug/l

RT: 3.11 min Scan# 332

Delta R.T. -0.01 min

Lab File: VX018901.D

Acq: 12 Oct 2020 14:28

Instrument :

MSVOA_X

ClientSampleId :

WASTE-ROOM-SAMPLEDL


Tot Ion: 53 Resp: 743

Ion Ratio Lower Upper

53 100

52 49.4 66.7 100.1#




51 49.1 30.3 45.5#



Abundance Ion 53.00 (52.70 to 53.70): VX0

Ion 52.00 (51.70 to 52.70): VX0

Ion 51.00 (50.70 to 51.70): VX0

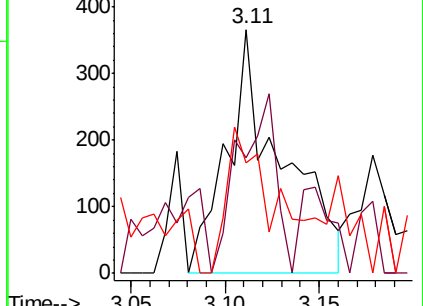

#16

Acetone

Concen: Below Cal

RT: 2.42 min Scan# 219

Delta R.T. 0.00 min

Lab File: VX018901.D


Acq: 12 Oct 2020 14:28

Tgt Ion: 43 Resp: 2289

Ion Ratio Lower Upper



43 100


58 21.0 23.0 34.4#



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

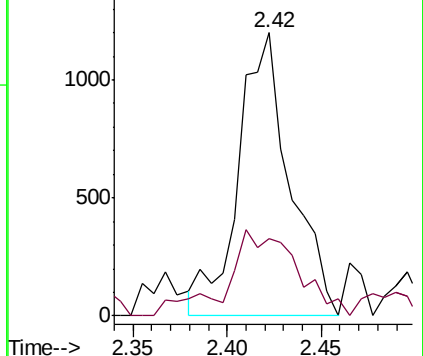



#17

Carbon Disulfide

Concen: 0.238 ug/l

RT: 2.55 min Scan# 240

Delta R.T. 0.00 min

Lab File: VX018901.D

Acq: 12 Oct 2020 14:28

Instrument :

MSVOA_X

ClientSampleId :





WASTE-ROOM-SAMPLEDL

Tot Ion: 76 Resp: 1732

Ion Ratio Lower Upper

76 100

78 22.6 7.3 10.9#

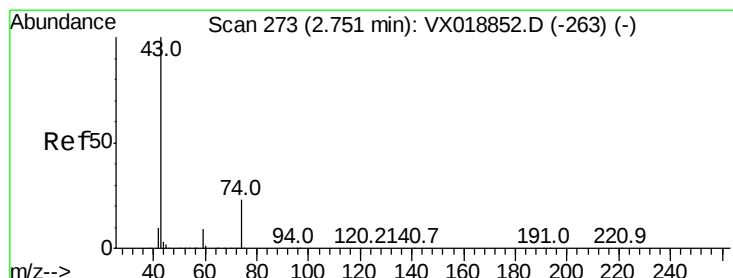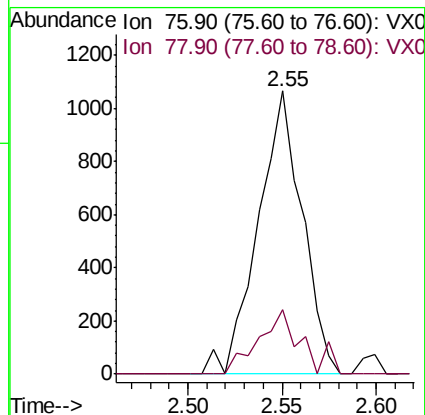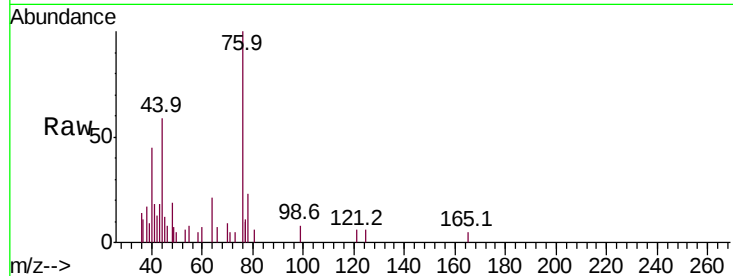

#18

Methyl Acetate

Concen: 151.846 ug/l

RT: 2.75 min Scan# 272

Delta R.T. -0.01 min

Lab File: VX018901.D




Acq: 12 Oct 2020 14:28


Tgt Ion: 43 Resp: 501338

Ion Ratio Lower Upper

43 100

74 22.0 18.9 28.3



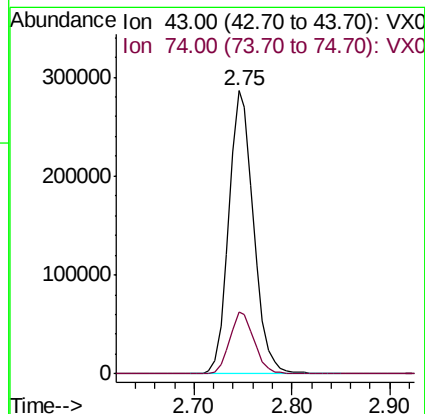
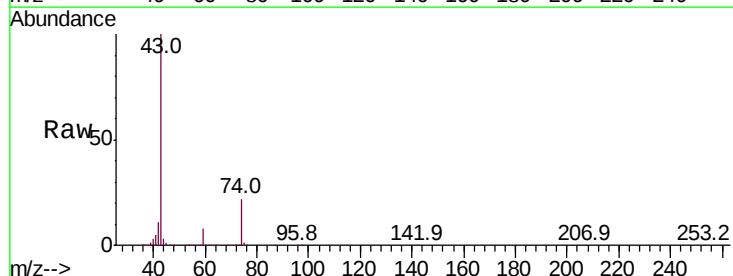




#20
Methvlene Chloride
Concen: 0.808 ug/l
RT: 2.82 min Scan# 285
Delta R.T. -0.01 min
Lab File: VX018901.D
Acq: 12 Oct 2020 14:28




Instrument :
MSVOA_X
ClientSampleId :
WASTE-ROOM-SAMPLEDL


Tot Ion: 84 Resp: 870
Ion Ratio Lower Upper
84 100
49 87.7 104.8 157.2#
51 42.5 30.6 46.0
86 78.7 50.8 76.2#

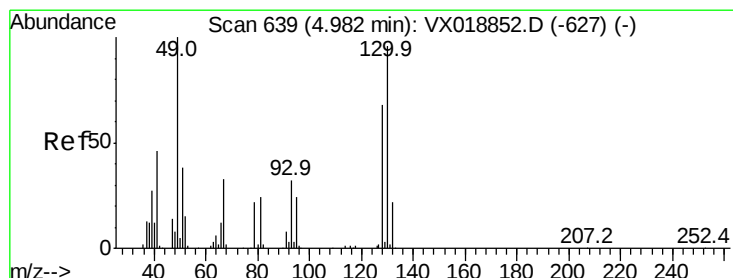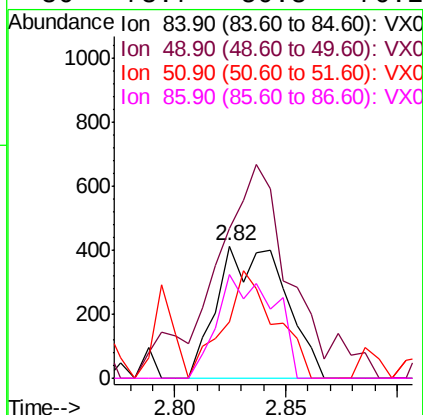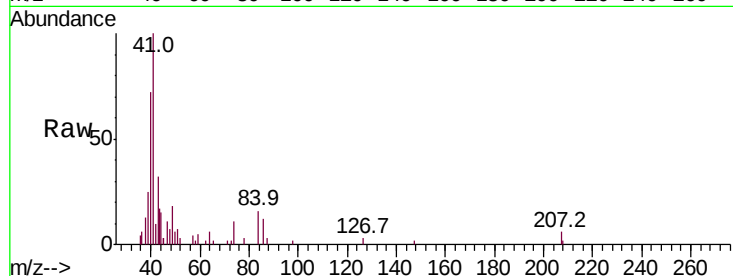

#28
Bromochloromethane
Concen: 1.579 ug/l
RT: 4.98 min Scan# 638
Delta R.T. -0.01 min
Lab File: VX018901.D
Acq: 12 Oct 2020 14:28

Tgt Ion: 49 Resp: 142
Ion Ratio Lower Upper
49 100
129 32.4 0.0 5.4#
130 18.3 71.2 106.8#


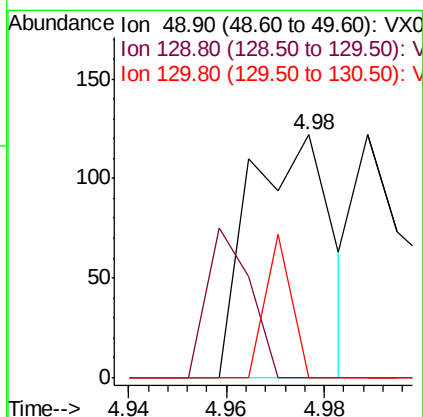

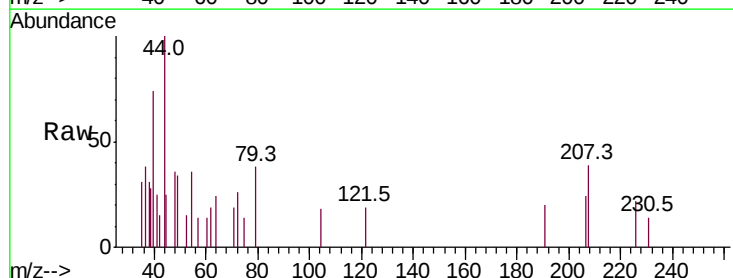




#31
Cyclohexane
Concen: 1.666 ug/l
RT: 5.63 min Scan# 745
Delta R.T. 0.07 min
Lab File: VX018901.D
Acq: 12 Oct 2020 14:28




Instrument :
MSVOA_X
ClientSampleId :
WASTE-ROOM-SAMPLEDL


Tot Ion: 56 Resp: 6181
Ion Ratio Lower Upper
56 100
69 179.8 27.1 40.7#
84 119.9 71.7 107.5#

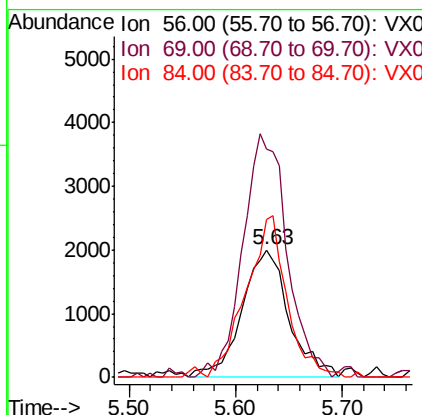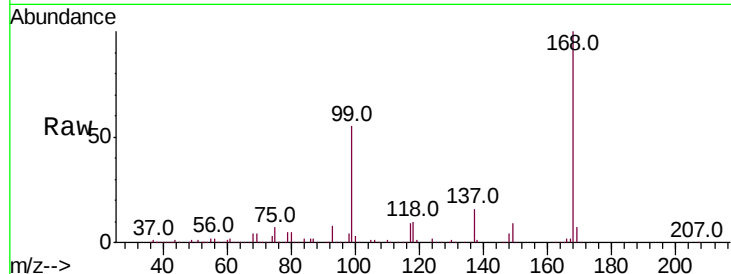

#33
1,2-Dichloroethane-d4
Concen: 51.250 ug/l
RT: 6.03 min Scan# 811
Delta R.T. 0.00 min
Lab File: VX018901.D
Acq: 12 Oct 2020 14:28

Tgt Ion: 65 Resp: 203554
Ion Ratio Lower Upper
65 100
67 49.8 0.0 97.0

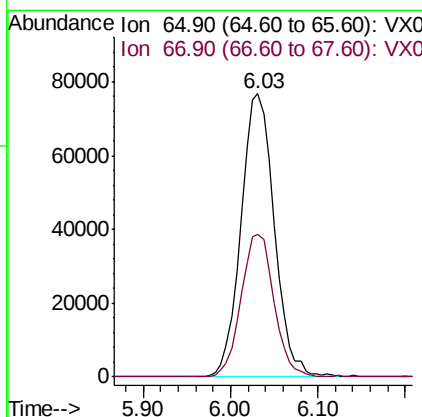



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.83 min Scan# 942

Delta R.T. -0.01 min

Lab File: VX018901.D

Acq: 12 Oct 2020 14:28

Instrument :

MSVOA_X

ClientSampleId :

WASTE-ROOM-SAMPLEDL


Tot Ion:114 Resp: 428074

Ion Ratio Lower Upper

114 100

63 22.7 0.0 42.4




88 16.9 0.0 32.6



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

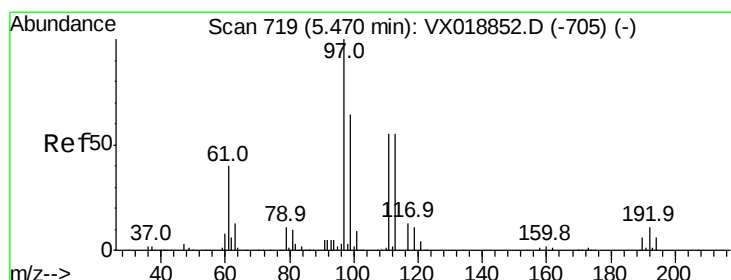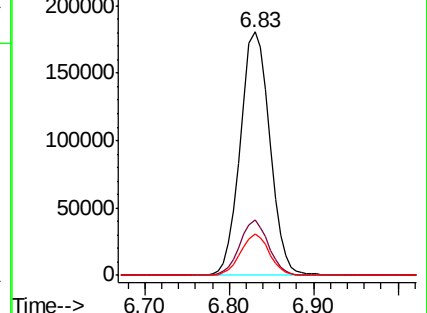

#35

Dibromofluoromethane

Concen: 48.708 ug/l

RT: 5.46 min Scan# 718

Delta R.T. -0.01 min

Lab File: VX018901.D

Acq: 12 Oct 2020 14:28


Tgt Ion:113 Resp: 148596

Ion Ratio Lower Upper

113 100

111 104.6 80.1 120.1



192 21.5 16.0 24.0




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

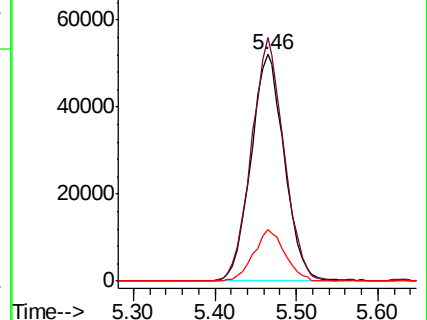

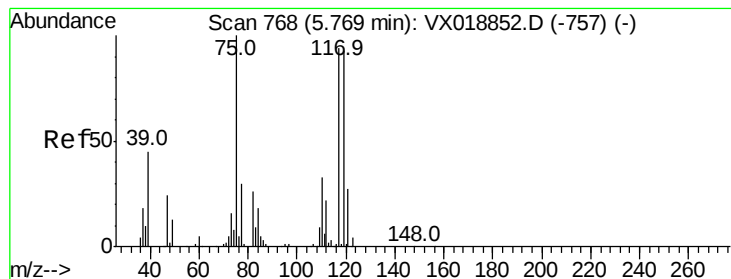

#36

1,1-Dichloropropene

Concen: 4.856 ug/l

RT: 5.64 min Scan# 746

Delta R.T. -0.13 min

Lab File: VX018901.D

Acq: 12 Oct 2020 14:28

Instrument :

MSVOA_X

ClientSampleId :

WASTE-ROOM-SAMPLEDL


Tot Ion: 75 Resp: 21857

Ion Ratio Lower Upper

75 100

110 9.5 17.8 53.5#




77 0.5 24.2 36.4#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VX0

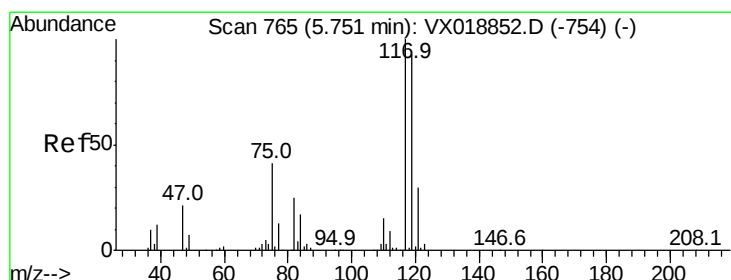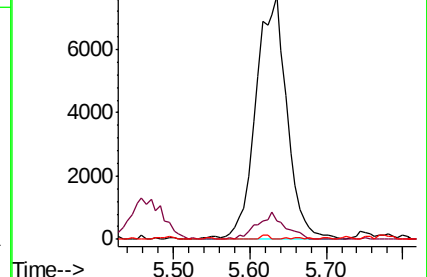

#38

Carbon Tetrachloride

Concen: 4.822 ug/l

RT: 5.62 min Scan# 744

Delta R.T. -0.13 min

Lab File: VX018901.D

Acq: 12 Oct 2020 14:28


Tgt Ion: 117 Resp: 26900

Ion Ratio Lower Upper

117 100

119 6.9 73.9 110.9#



121 0.0 23.6 35.4#




Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

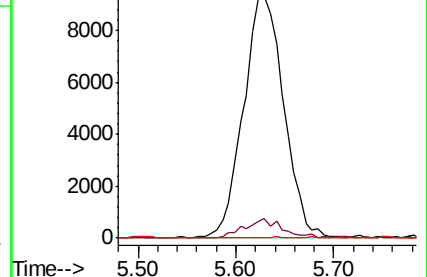



#49

1,4-Dioxane

Concen: 3.619 ug/l

RT: 7.73 min Scan# 1089

Delta R.T. 0.01 min

Lab File: VX018901.D

Acq: 12 Oct 2020 14:28

Instrument :

MSVOA_X

ClientSampleID :

WASTE-ROOM-SAMPLEDL


Tot Ion: 88 Resp: 186

Ion Ratio Lower Upper

88 100

43 116.7 31.0 46.6#




58 99.5 59.3 88.9#

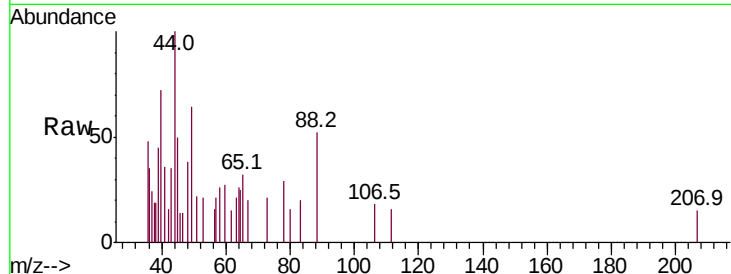

Abundance Ion 88.00 (87.70 to 88.70): VX0

Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

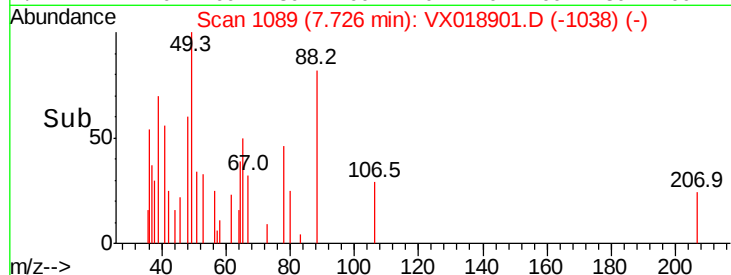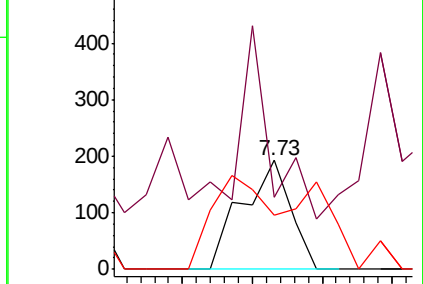

#50

Toluene-d8

Concen: 46.846 ug/l

RT: 8.70 min Scan# 1248

Delta R.T. 0.00 min

Lab File: VX018901.D


Acq: 12 Oct 2020 14:28

Tgt Ion: 98 Resp: 495730

Ion Ratio Lower Upper



98 100


100 64.9 53.1 79.7

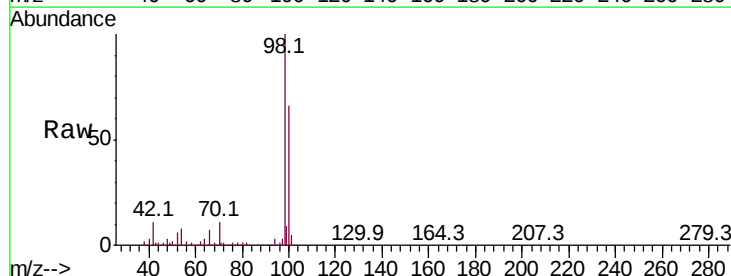

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V

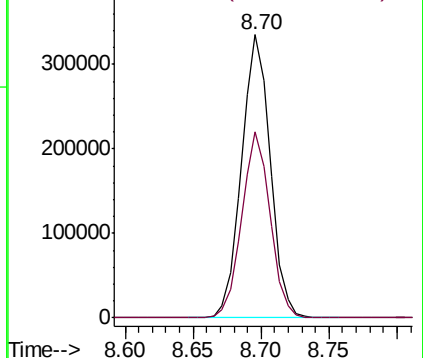



#56

Ethyl methacrylate

Concen: 2.942 ug/l

RT: 9.19 min Scan# 1329

Delta R.T. 0.03 min

Lab File: VX018901.D

Acq: 12 Oct 2020 14:28

Instrument :
MSVOA_X
ClientSampleId :
WASTE-ROOM-SAMPLEDL


Tot Ion: 69 Resp: 40

Ion Ratio Lower Upper

69 100

41 192.5 54.6 81.8#


39 112.5 31.5 47.3#

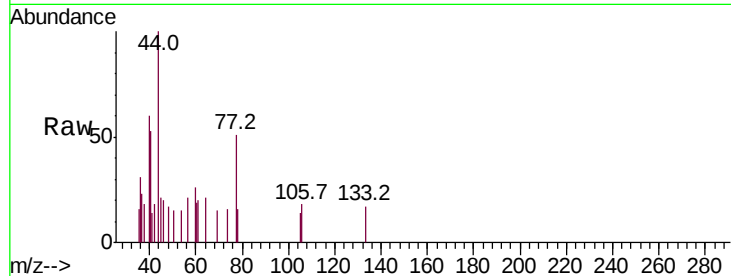



Abundance Ion 69.00 (68.70 to 69.70): VX0

Ion 41.00 (40.70 to 41.70): VX0

Ion 39.00 (38.70 to 39.70): VX0

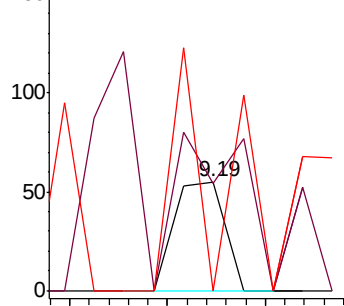

Time-->

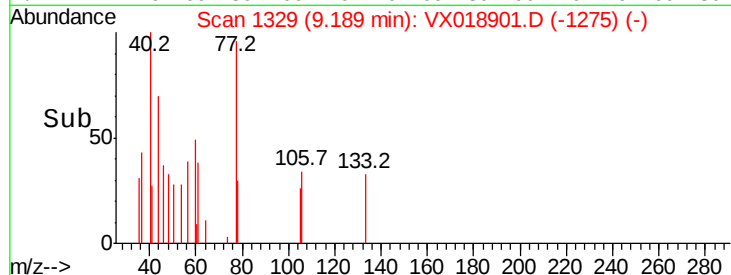

#62

4-Bromofluorobenzene

Concen: 44.286 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. 0.00 min

Lab File: VX018901.D

Acq: 12 Oct 2020 14:28


Tgt Ion: 95 Resp: 186780

Ion Ratio Lower Upper

95 100

174 92.1 0.0 160.0


176 86.6 0.0 161.2




Abundance Ion 94.90 (94.60 to 95.60): VX0


Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

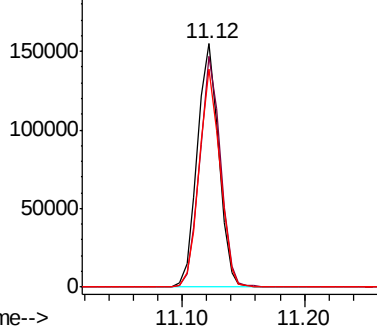

Time-->









#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1478
Delta R.T. 0.00 min
Lab File: VX018901.D
Acq: 12 Oct 2020 14:28




Instrument :
MSVOA_X
ClientSampleId :
WASTE-ROOM-SAMPLEDL


Tot Ion:117 Resp: 395432
Ion Ratio Lower Upper
117 100
82 54.9 43.4 65.2
119 31.7 28.3 42.5

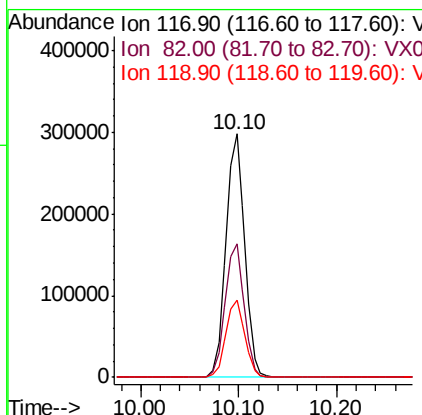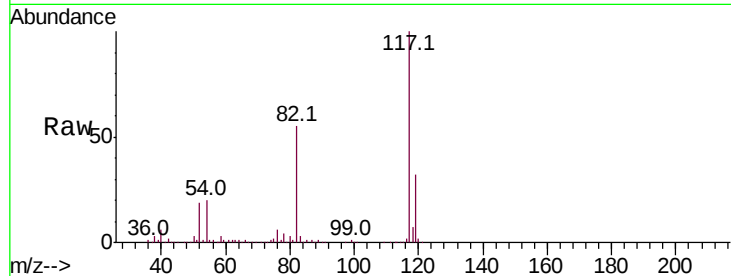

#64
Tetrachloroethene
Concen: Below Cal
RT: 9.32 min Scan# 1350
Delta R.T. 0.00 min
Lab File: VX018901.D
Acq: 12 Oct 2020 14:28

Tgt Ion:164 Resp: 146
Ion Ratio Lower Upper
164 100
166 109.2 105.4 158.0
129 127.0 79.0 118.6#
131 37.4 75.7 113.5#

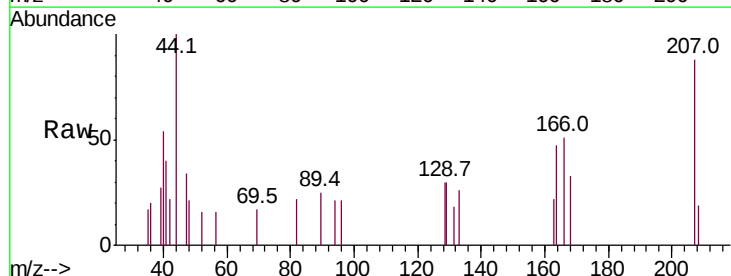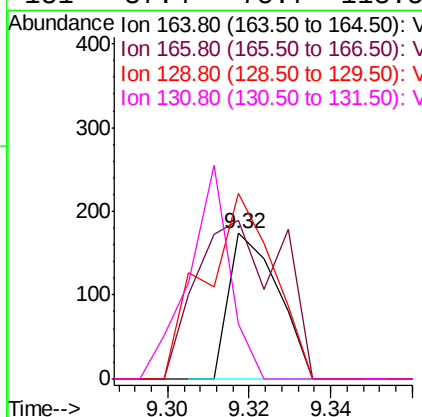

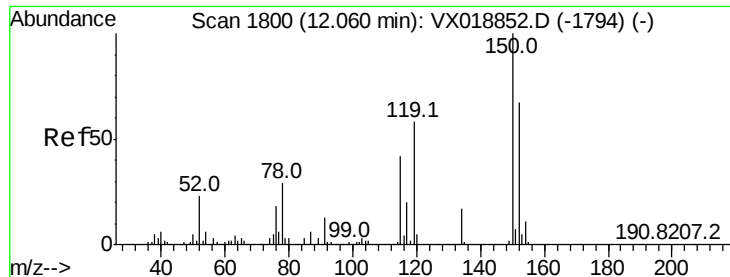

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.06 min Scan# 1800

Delta R.T. 0.00 min

Lab File: VX018901.D

Acq: 12 Oct 2020 14:28

Instrument :

MSVOA_X

ClientSampleId :

WASTE-ROOM-SAMPLEDL


Tot Ion:152 Resp: 211370

Ion Ratio Lower Upper

152 100

115 56.9 41.8 125.4




150 154.9 0.0 347.6

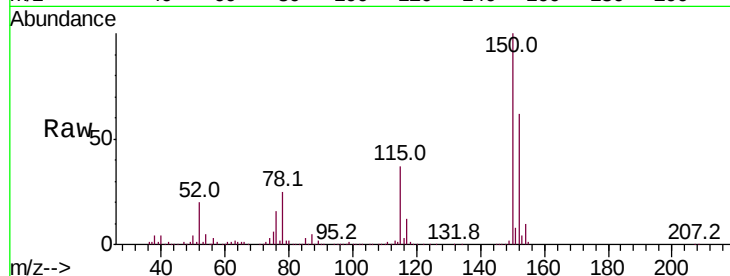

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

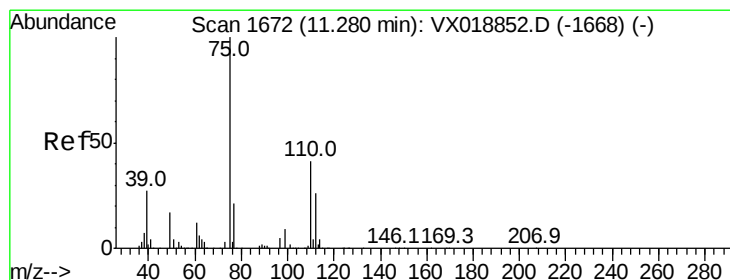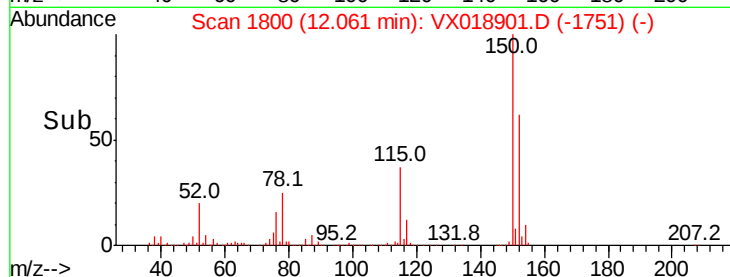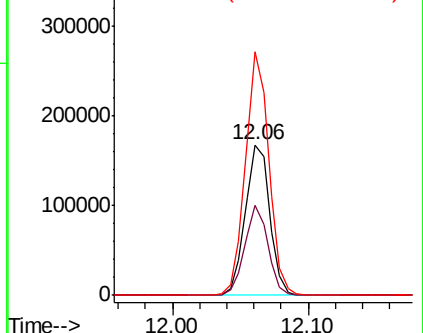

#76

1,2,3-Trichloropropane

Concen: 20.753 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.16 min

Lab File: VX018901.D


Acq: 12 Oct 2020 14:28

Tgt Ion: 75 Resp: 94517

Ion Ratio Lower Upper



75 100


77 1.5 20.2 60.6#

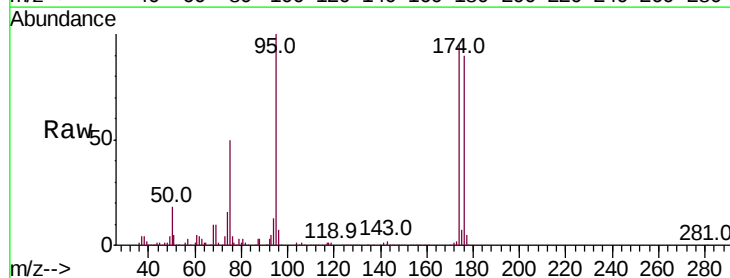

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

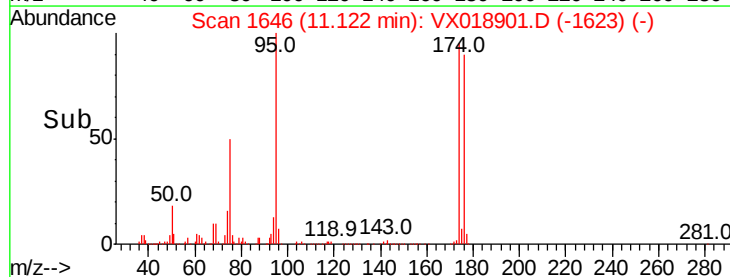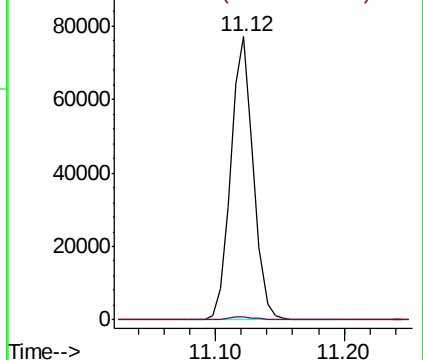



#81

trans-1,4-Dichloro-2-butene

Concen: 58.813 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. 0.06 min

Lab File: VX018901.D

Acq: 12 Oct 2020 14:28

Instrument :

MSVOA_X

ClientSampleID :

WASTE-ROOM-SAMPLEDL


Tot Ion: 75 Resp: 94517

Ion Ratio Lower Upper

75 100

53 0.5 85.0 127.4#




89 0.0 39.0 58.4#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0

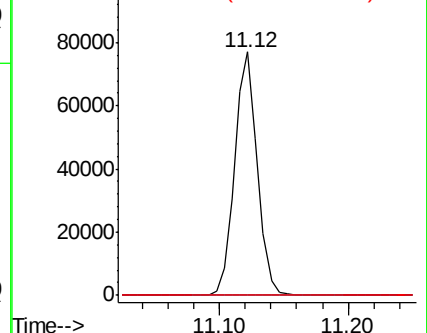

#93

1,2,4-Trichlorobenzene

Concen: 0.206 ug/l

RT: 13.63 min Scan# 2058

Delta R.T. 0.01 min

Lab File: VX018901.D

Acq: 12 Oct 2020 14:28


Tgt Ion: 180 Resp: 878

Ion Ratio Lower Upper

180 100

182 108.8 49.1 147.3



145 36.8 16.0 48.0




Abundance Ion 179.80 (179.50 to 180.50): V

Ion 181.80 (181.50 to 182.50): V

Ion 144.80 (144.50 to 145.50): V

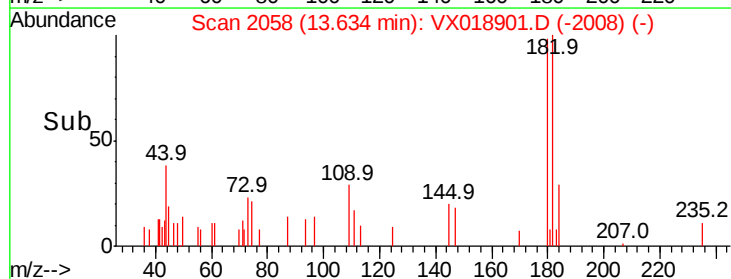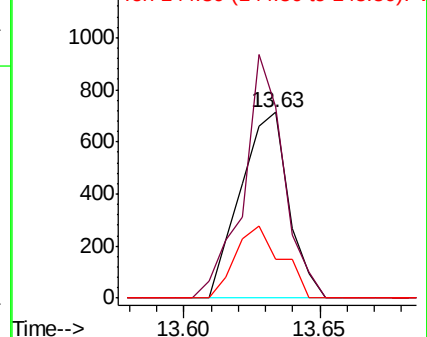

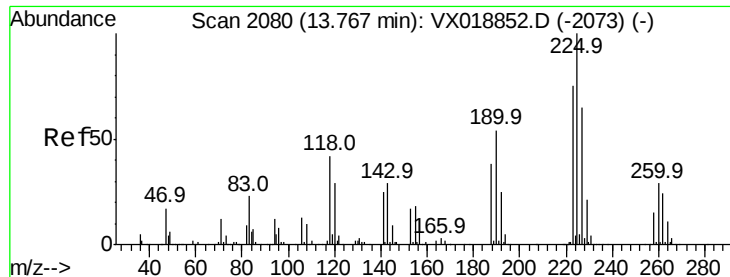

#94

Hexachlorobutadiene

Concen: 0.308 ug/l

RT: 13.77 min Scan# 2080

Delta R.T. 0.00 min

Lab File: VX018901.D

Acq: 12 Oct 2020 14:28

Instrument :

MSVOA_X

ClientSampleId :

WASTE-ROOM-SAMPLEDL


Tot Ion:225 Resp: 583

Ion Ratio Lower Upper

225 100


223 44.6 32.1 96.3

227 73.4 33.0 98.9

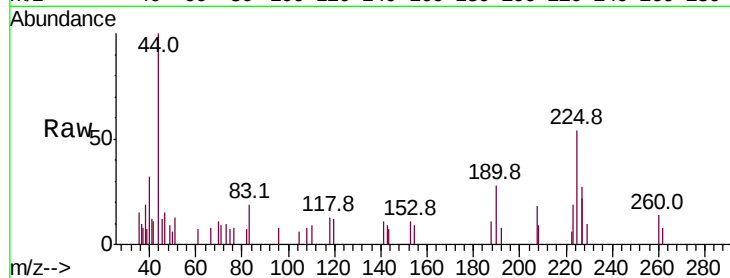


Abundance Ion 224.70 (224.40 to 225.40): V
Ion 222.70 (222.40 to 223.40): V
Ion 226.70 (226.40 to 227.40): V

13.77

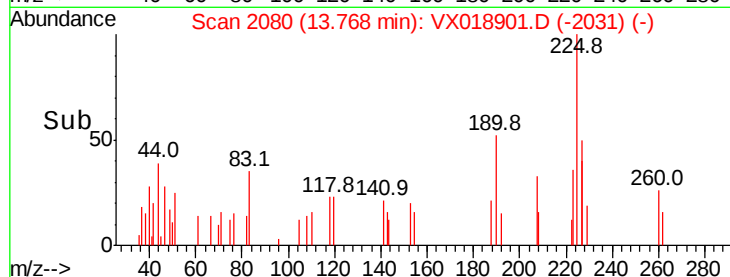

Time--> 13.70 13.75 13.80

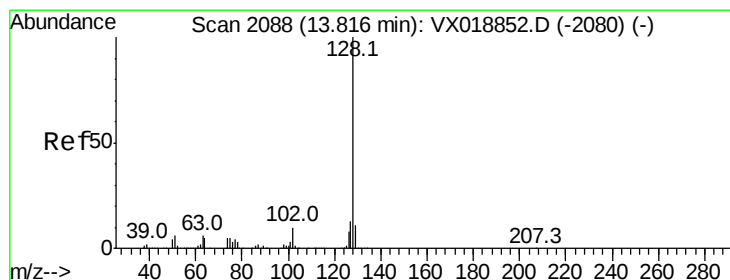

#95

Naphthalene

Concen: 3.180 ug/l

RT: 13.82 min Scan# 2088

Delta R.T. 0.00 min

Lab File: VX018901.D

Acq: 12 Oct 2020 14:28


Tgt Ion:128 Resp: 1564

Ion Ratio Lower Upper

128 100


127 21.8 10.1 15.1#

129 11.4 8.6 13.0

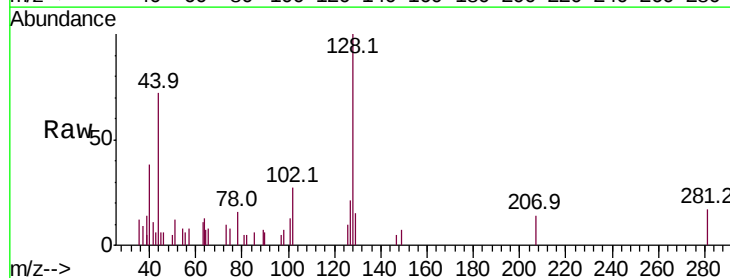

Abundance Ion 128.00 (127.70 to 128.70): V
Ion 127.00 (126.70 to 127.70): V
Ion 129.00 (128.70 to 129.70): V

13.82

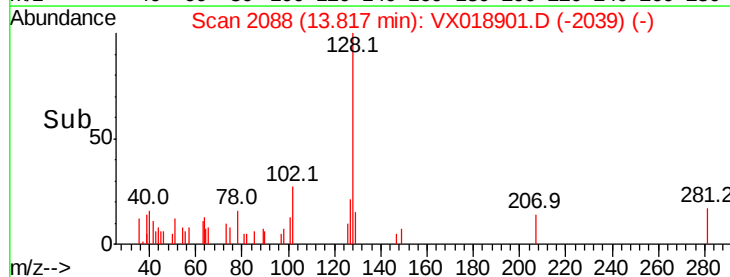

Time--> 13.75 13.80 13.85