

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101221\
 Data File : VX024767.D
 Acq On : 12 Oct 2021 16:47
 Operator : JC/MD
 Sample : M4170-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SW-RR-03-(SA)

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
 Title : SW846 8260

Signal : TIC: VX024767.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	32	rBV	11172	17373	2.34%	0.429%
2	1.569	70	79	83	rBV4	3818	8037	1.08%	0.198%
3	2.550	230	240	246	rBV2	4078	7885	1.06%	0.195%
4	5.397	694	707	722	rBV2	90120	259066	34.92%	6.397%
5	5.562	722	734	752	rVB	138619	390690	52.67%	9.647%
6	5.964	789	800	814	rBV	96490	256459	34.57%	6.332%
7	6.769	923	932	949	rBV	228243	536468	72.32%	13.246%
8	8.653	1234	1241	1249	rBV	483748	741799	100.00%	18.316%
9	8.726	1249	1253	1260	rVB	6641	10027	1.35%	0.248%
10	10.055	1466	1471	1484	rBV	493678	671670	90.55%	16.585%
11	11.085	1634	1640	1654	rBV	429100	550093	74.16%	13.583%
12	12.024	1789	1794	1804	rBV	482359	600386	80.94%	14.825%




Sum of corrected areas: 4049953

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101221\
Data File : VX024767.D
Acq On : 12 Oct 2021 16:47
Operator : JC/MD
Sample : M4170-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-RR-03-(SA)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

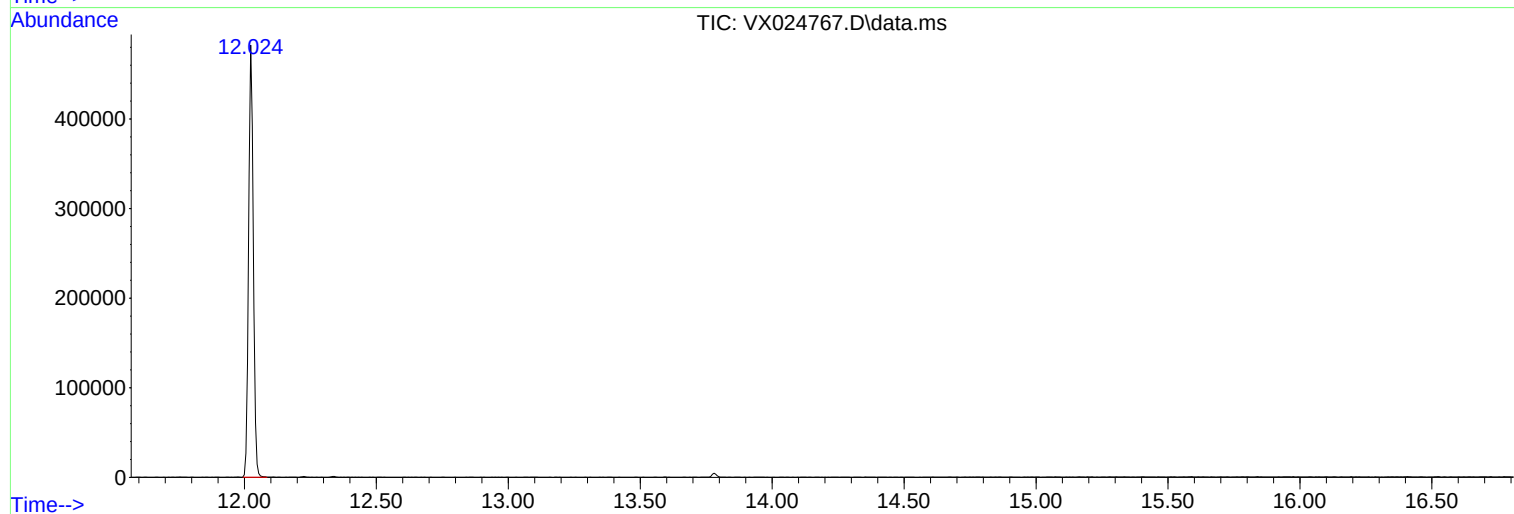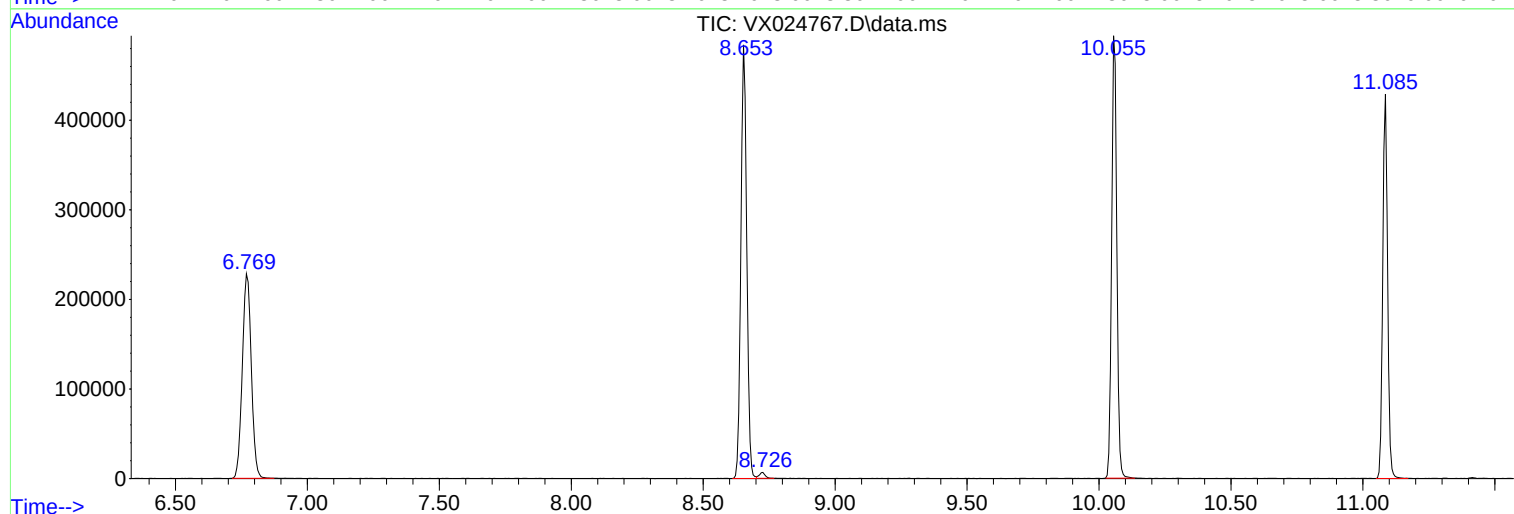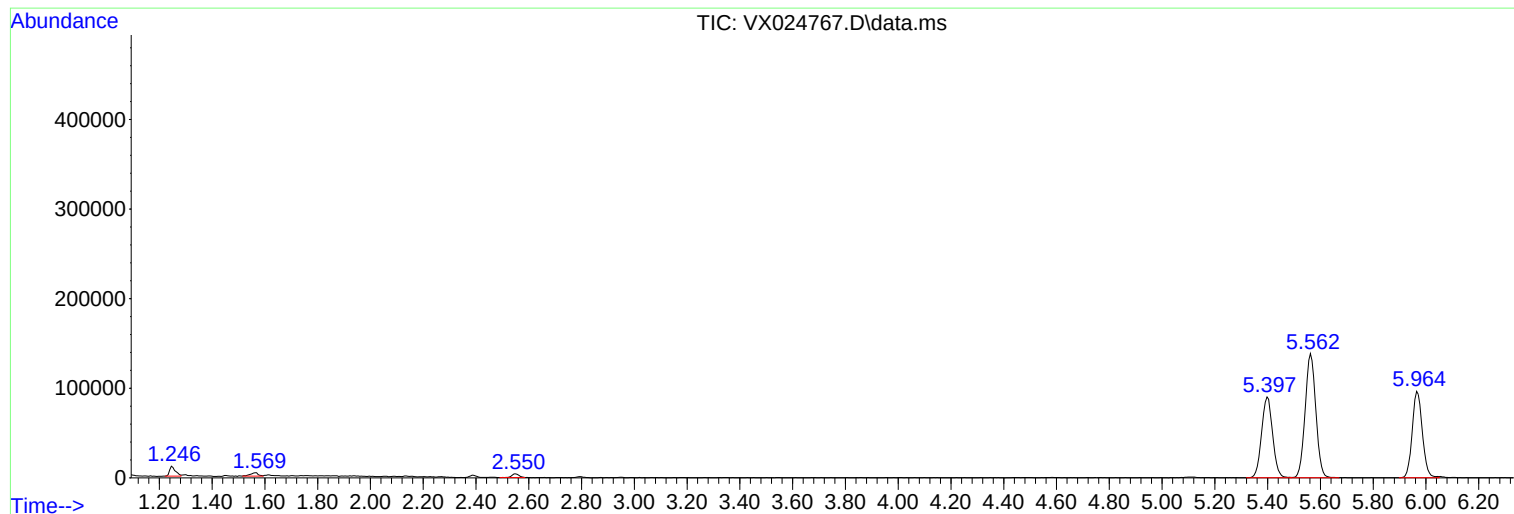

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101221\
Data File : VX024767.D
Acq On : 12 Oct 2021 16:47
Operator : JC/MD
Sample : M4170-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-RR-03-(SA)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101221\
Data File : VX024767.D
Acq On : 12 Oct 2021 16:47
Operator : JC/MD
Sample : M4170-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-RR-03-(SA)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
