

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101221\
 Data File : VX024770.D
 Acq On : 12 Oct 2021 17:57
 Operator : JC/MD
 Sample : M4169-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P287-DITCH

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
 Title : SW846 8260

Signal : TIC: VX024770.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	36	rBV	10013	17729	2.48%	0.461%
2	2.544	230	239	249	rBV	12998	24249	3.39%	0.630%
3	2.959	299	307	317	rBV	4241	10278	1.44%	0.267%
4	5.391	692	706	722	rBV	86277	250023	34.98%	6.498%
5	5.562	722	734	751	rVB	132903	373075	52.19%	9.696%
6	5.964	788	800	812	rBV2	94308	250342	35.02%	6.506%
7	6.769	922	932	944	rBV	219284	515646	72.13%	13.402%
8	8.653	1234	1241	1249	rBV	466618	714845	100.00%	18.579%
9	10.055	1465	1471	1487	rBV	458919	638983	89.39%	16.607%
10	11.085	1634	1640	1655	rVB	402489	511208	71.51%	13.286%
11	12.024	1789	1794	1803	rBV	434071	541223	75.71%	14.067%




Sum of corrected areas: 3847601

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101221\
Data File : VX024770.D
Acq On : 12 Oct 2021 17:57
Operator : JC/MD
Sample : M4169-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P287-DITCH

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

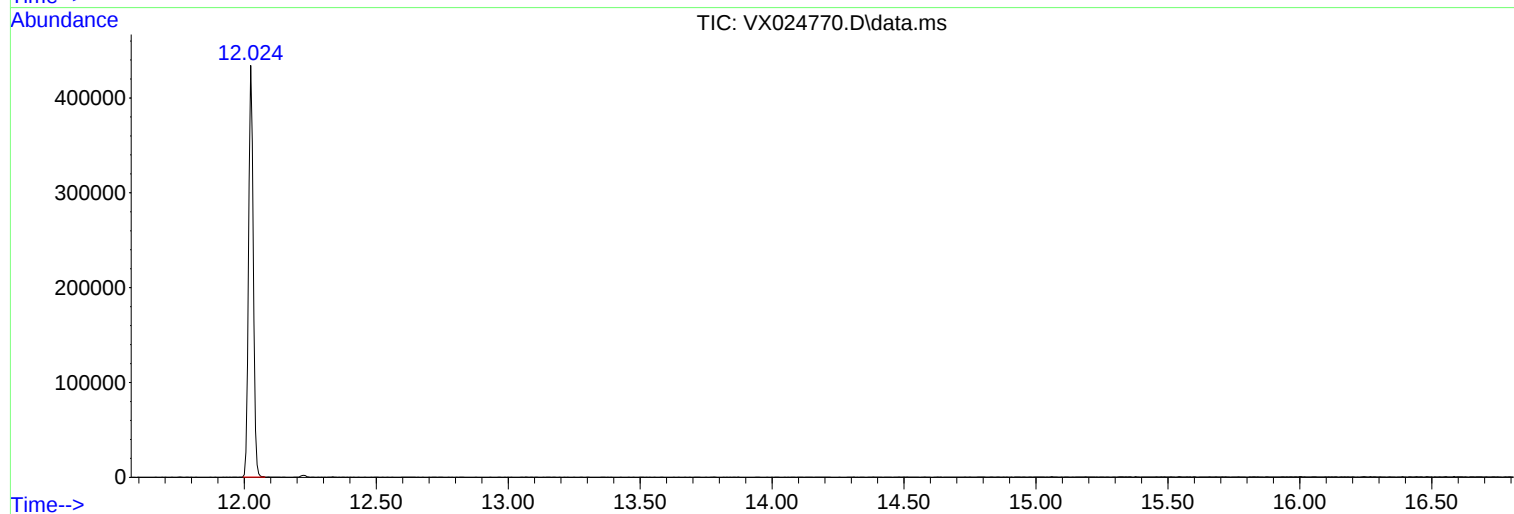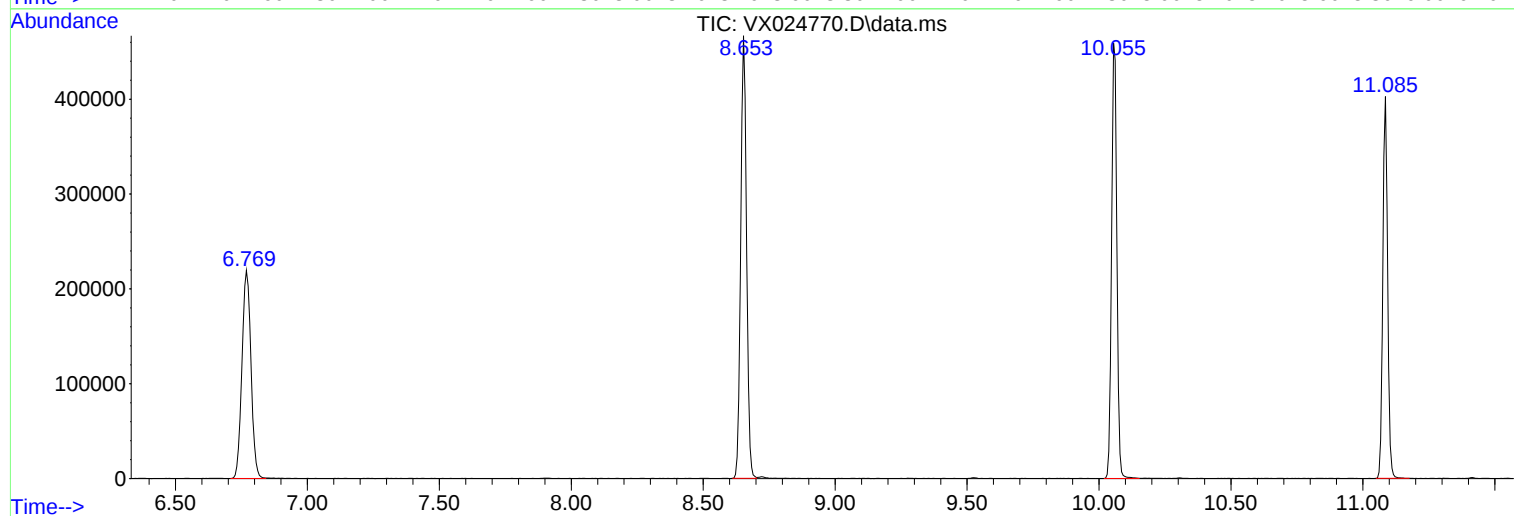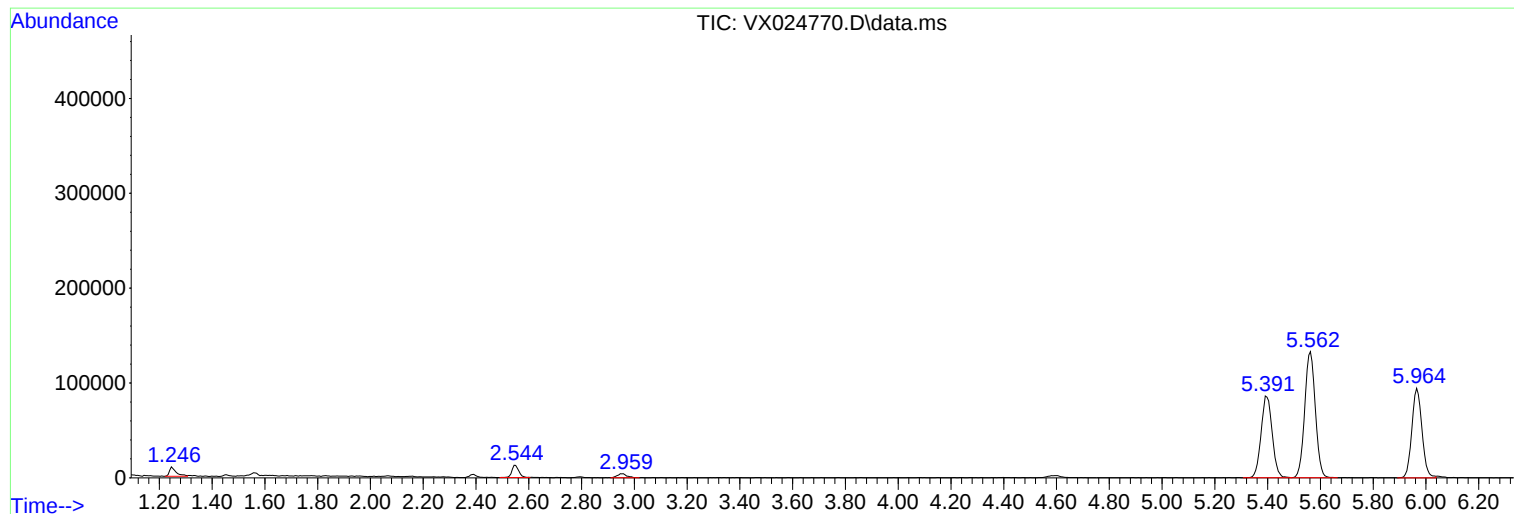

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101221\
Data File : VX024770.D
Acq On : 12 Oct 2021 17:57
Operator : JC/MD
Sample : M4169-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P287-DITCH

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101221\
Data File : VX024770.D
Acq On : 12 Oct 2021 17:57
Operator : JC/MD
Sample : M4169-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P287-DITCH

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
