

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101222\
 Data File : VX032095.D
 Acq On : 12 Oct 2022 19:24
 Operator : JC/MD
 Sample : N5130-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 557-E-1

Quant Time: Oct 13 09:23:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 06 14:28:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	83401	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	123944	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	128084	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	80014	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	90644	52.626	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	105.260%
35) Dibromofluoromethane	5.391	113	67346	48.002	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	96.000%
50) Toluene-d8	8.647	98	250130	49.546	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	99.100%
62) 4-Bromofluorobenzene	11.079	95	87349	48.942	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	97.880%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101222\
Data File : VX032095.D
Acq On : 12 Oct 2022 19:24
Operator : JC/MD
Sample : N5130-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
557-E-1

Quant Time: Oct 13 09:23:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 06 14:28:46 2022
Response via : Initial Calibration




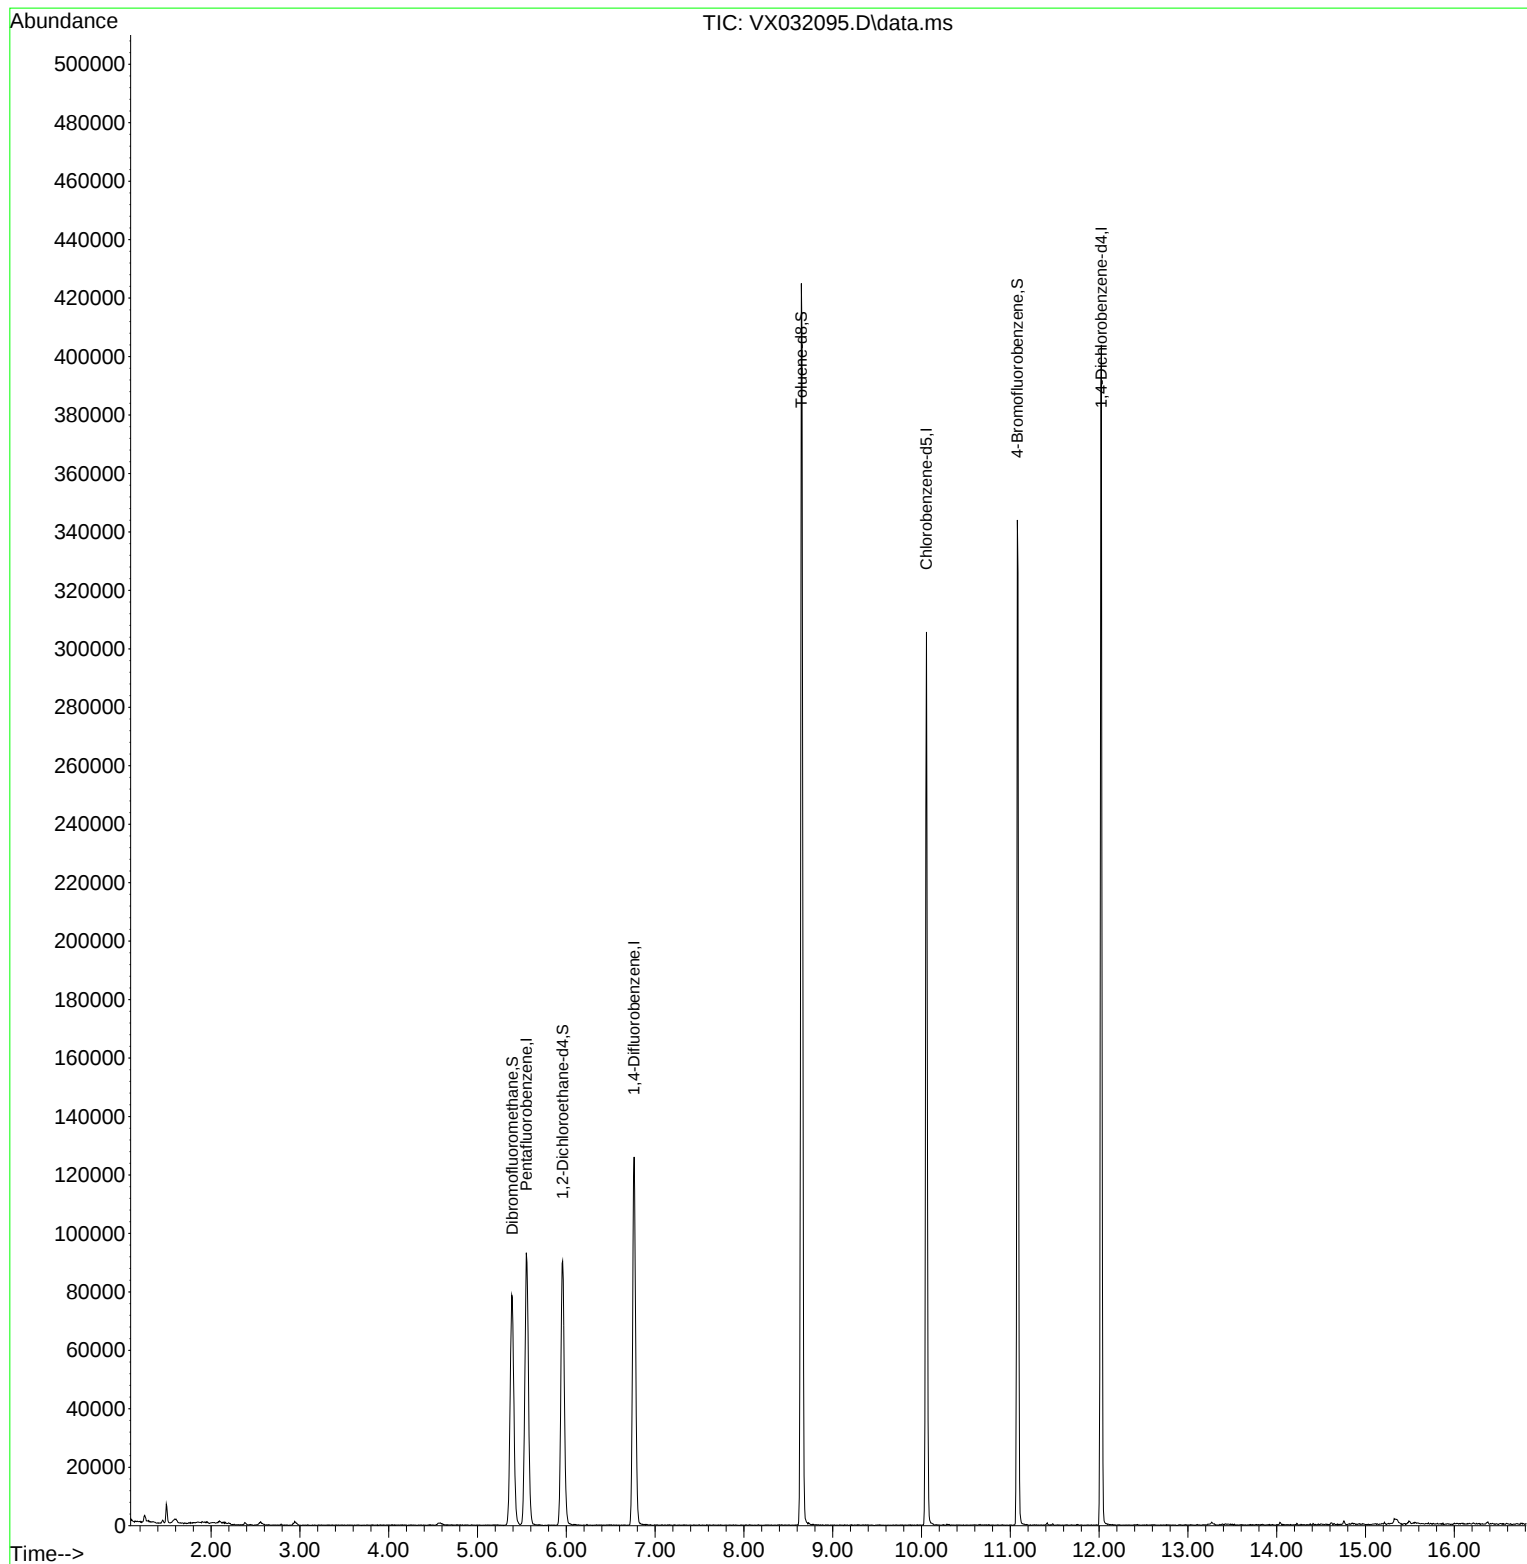


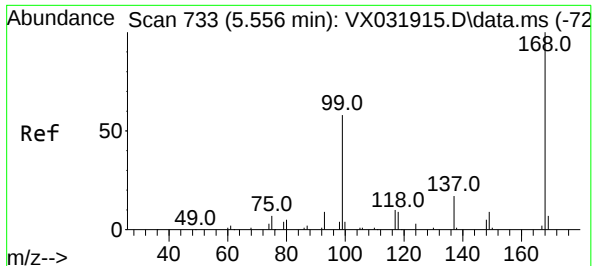

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 713
Delta R.T. -0.006 min
Lab File: VX032095.D
Acq: 12 Oct 2022 19:24




Instrument :
MSVOA_X
ClientSampleId :
557-E-1


Tgt Ion:168 Resp: 83401
Ion Ratio Lower Upper
168 100
99 63.4 48.8 73.2

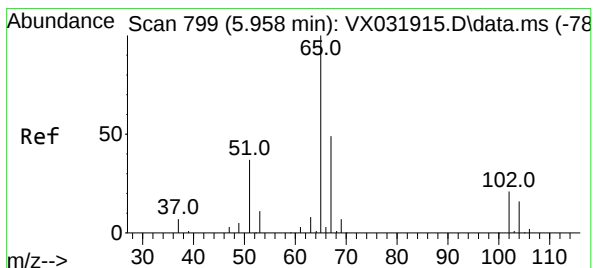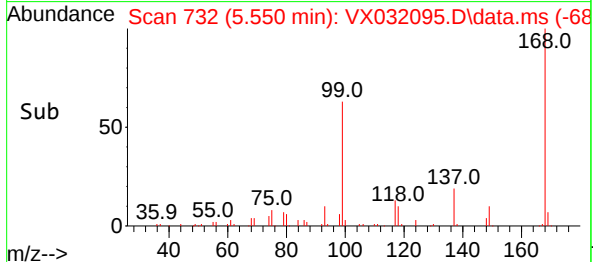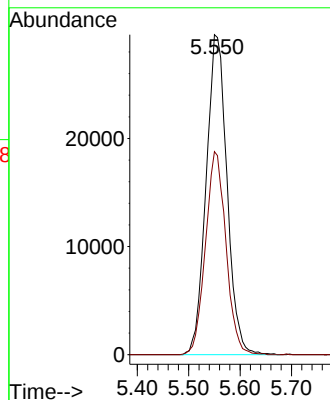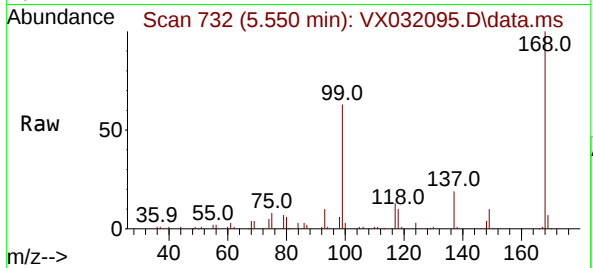

#33
1,2-Dichloroethane-d4
Concen: 52.626 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX032095.D
Acq: 12 Oct 2022 19:24

Tgt Ion: 65 Resp: 90644
Ion Ratio Lower Upper
65 100
67 49.2 0.0 102.4


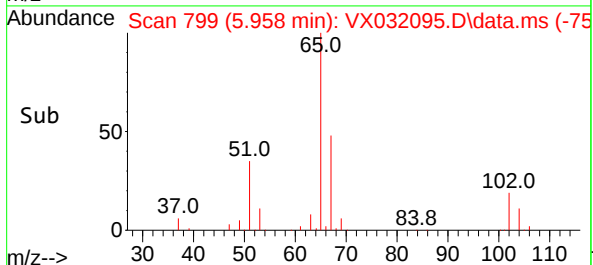
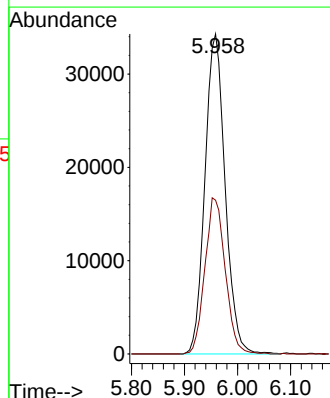
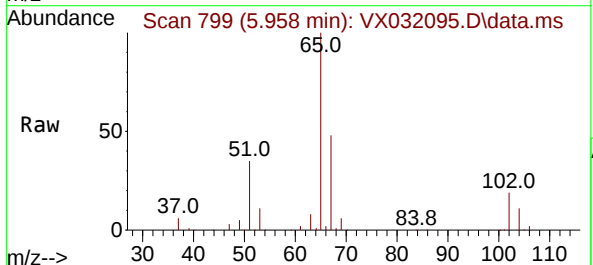


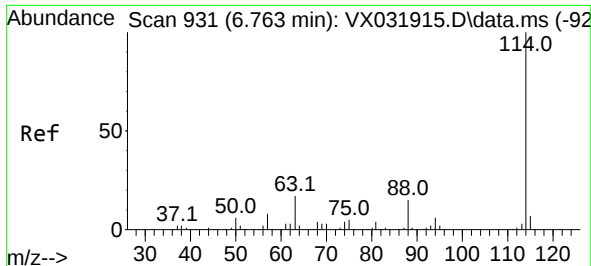

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX032095.D
Acq: 12 Oct 2022 19:24




Instrument :
MSVOA_X
ClientSampleId :
557-E-1


Tgt Ion:114 Resp: 123944
Ion Ratio Lower Upper
114 100
63 20.1 0.0 42.6
88 16.3 0.0 33.0

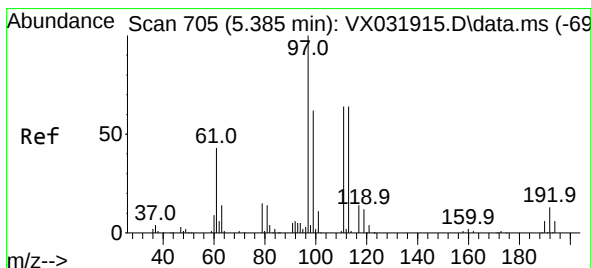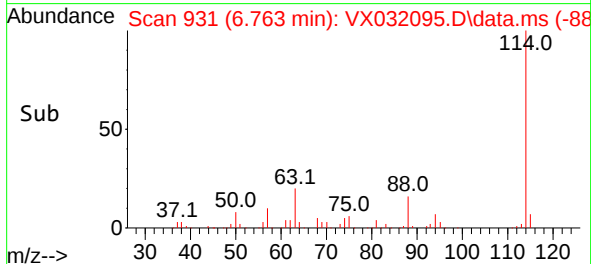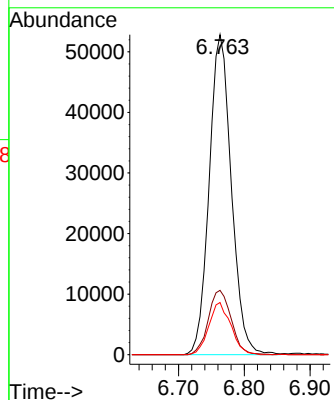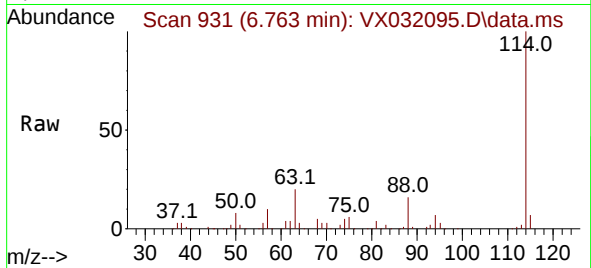

#35
Dibromofluoromethane
Concen: 48.002 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.006 min
Lab File: VX032095.D
Acq: 12 Oct 2022 19:24

Tgt Ion:113 Resp: 67346
Ion Ratio Lower Upper
113 100
111 100.7 82.4 123.6
192 17.8 14.1 21.1


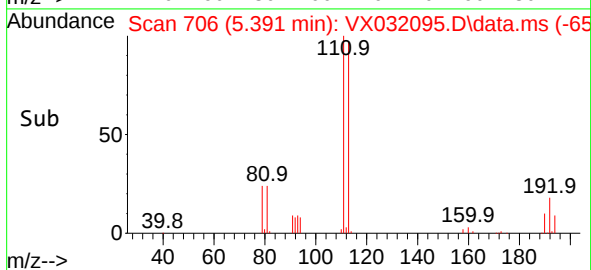
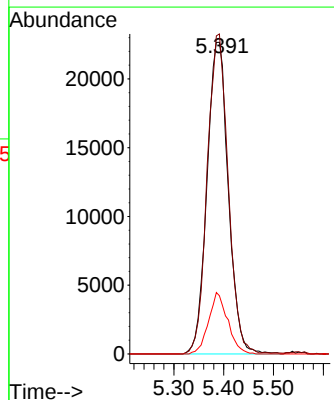
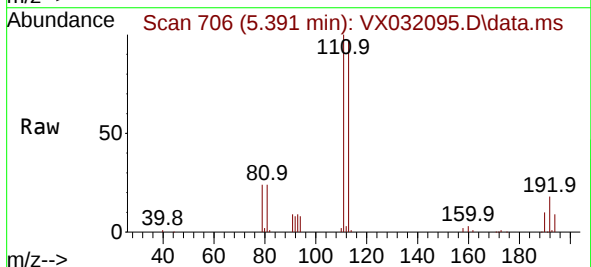


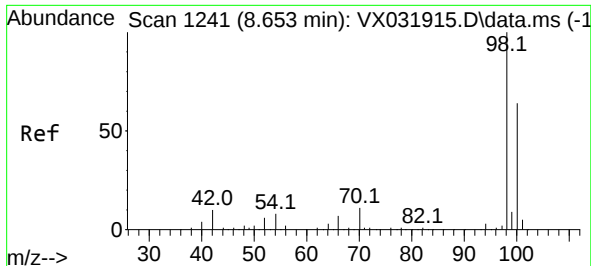

#50
Toluene-d8
Concen: 49.546 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX032095.D
Acq: 12 Oct 2022 19:24




Instrument :
MSVOA_X
ClientSampleId :
557-E-1


Tgt Ion: 98 Resp: 250130
Ion Ratio Lower Upper
98 100
100 65.8 52.5 78.7

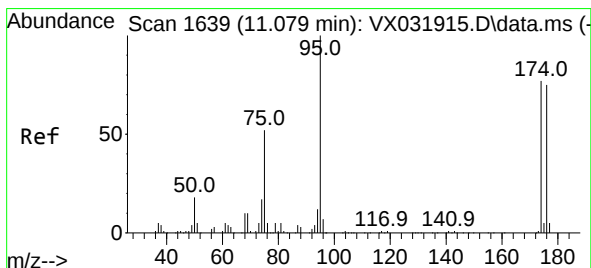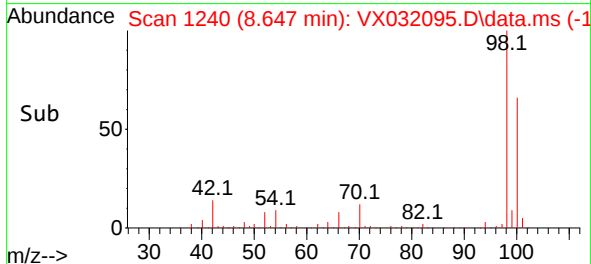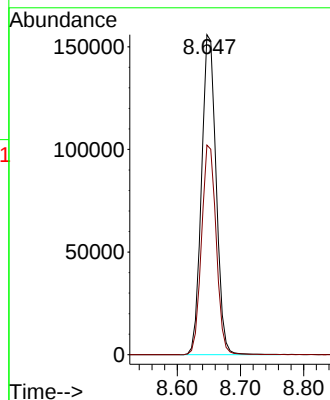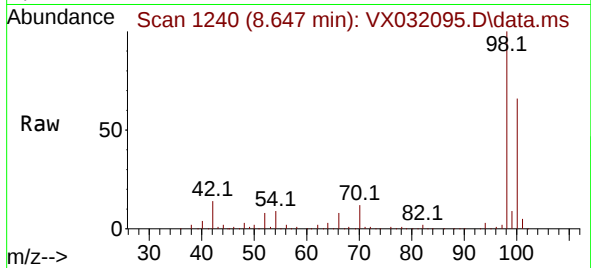

#62
4-Bromofluorobenzene
Concen: 48.942 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX032095.D
Acq: 12 Oct 2022 19:24

Tgt Ion: 95 Resp: 87349
Ion Ratio Lower Upper
95 100
174 76.1 0.0 153.2
176 73.9 0.0 144.0


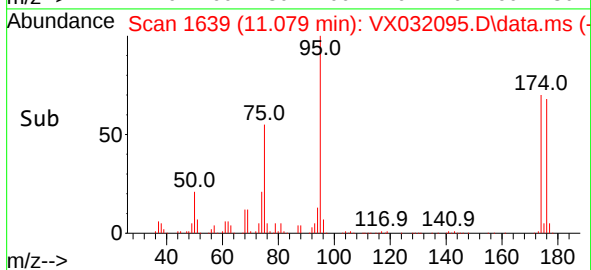
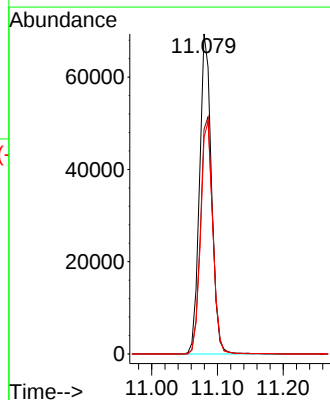
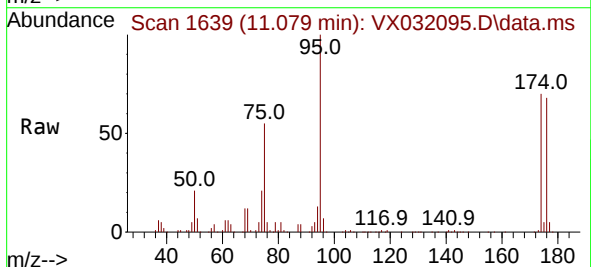


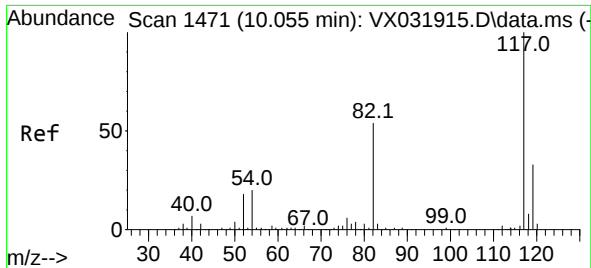

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX032095.D
Acq: 12 Oct 2022 19:24

Instrument :
MSVOA_X
ClientSampleId :
557-E-1

Tgt Ion:117 Resp: 128084
Ion Ratio Lower Upper
117 100
82 56.9 46.8 70.2
119 31.6 26.4 39.6

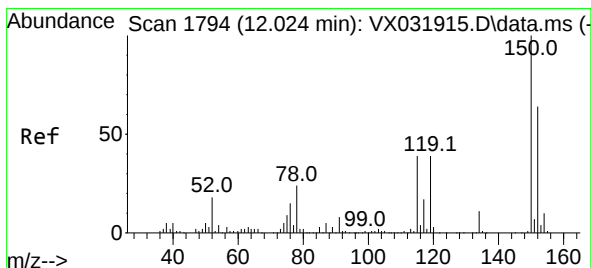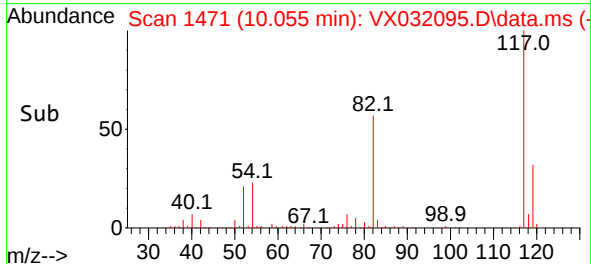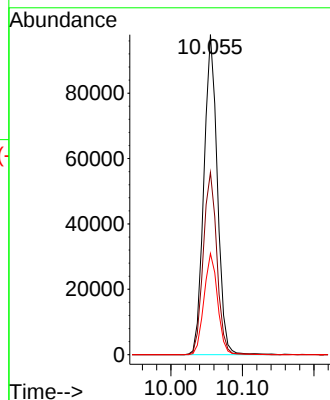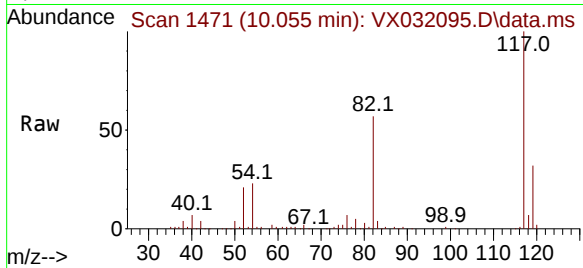

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX032095.D
Acq: 12 Oct 2022 19:24

Tgt Ion:152 Resp: 80014
Ion Ratio Lower Upper
152 100
115 61.2 43.4 130.1
150 155.7 0.0 346.8

