

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101222\
 Data File : VX032084.D
 Acq On : 12 Oct 2022 15:09
 Operator : JC/MD
 Sample : N5042-03 500X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EOR-0615

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M

Title : SW846 8260

Signal : TIC: VX032084.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.142	160	173	184	rVB4	3550	14929	2.24%	0.380%
2	2.294	191	198	207	rBV	50723	81832	12.28%	2.084%
3	2.386	207	213	228	rVB	129458	228529	34.28%	5.820%
4	2.581	233	245	261	rBV	26832	107818	16.17%	2.746%
5	3.910	449	463	490	rBV4	106731	523305	78.50%	13.328%
6	5.385	695	705	721	rBV2	76514	222247	33.34%	5.660%
7	5.550	722	732	748	rVB2	88460	249767	37.47%	6.361%
8	5.958	789	799	816	rBV	90607	240590	36.09%	6.128%
9	6.763	922	931	944	rBV	120062	287100	43.07%	7.312%
10	8.647	1234	1240	1250	rBV	420954	666651	100.00%	16.979%
11	9.488	1372	1378	1384	rBV2	6888	10077	1.51%	0.257%
12	10.055	1465	1471	1484	rBV	297383	395264	59.29%	10.067%
13	11.079	1634	1639	1653	rBV	324348	422332	63.35%	10.756%
14	12.024	1788	1794	1802	rBV	385892	475946	71.39%	12.122%




Sum of corrected areas: 3926387

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101222\
Data File : VX032084.D
Acq On : 12 Oct 2022 15:09
Operator : JC/MD
Sample : N5042-03 500X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EOR-0615

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

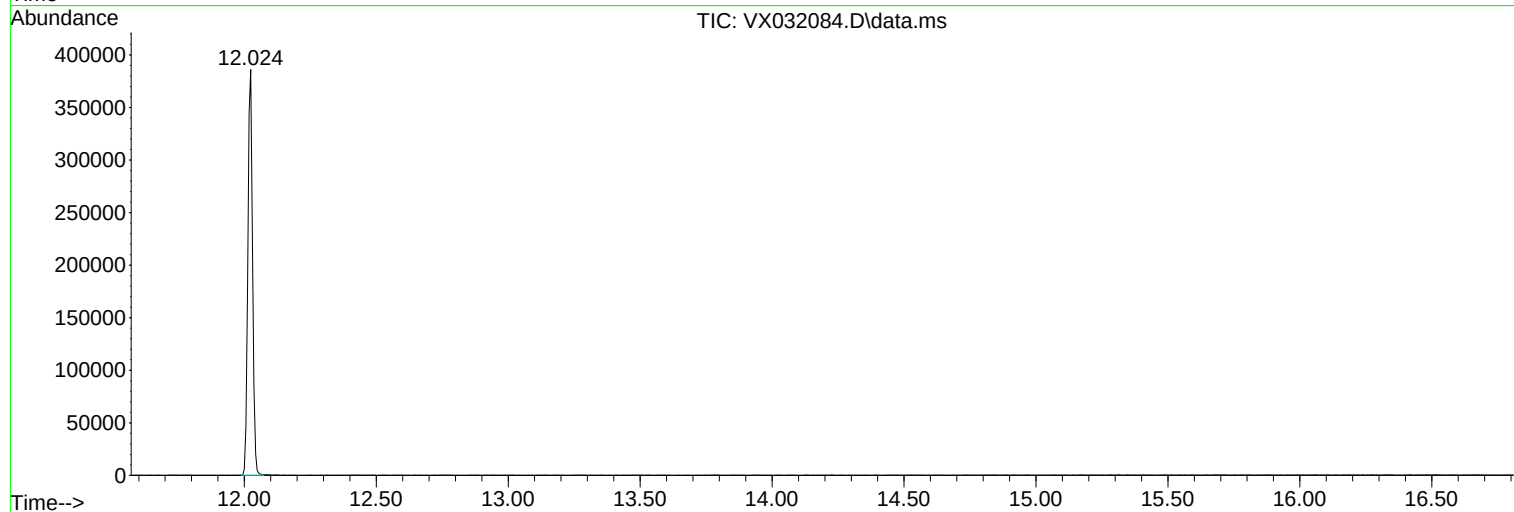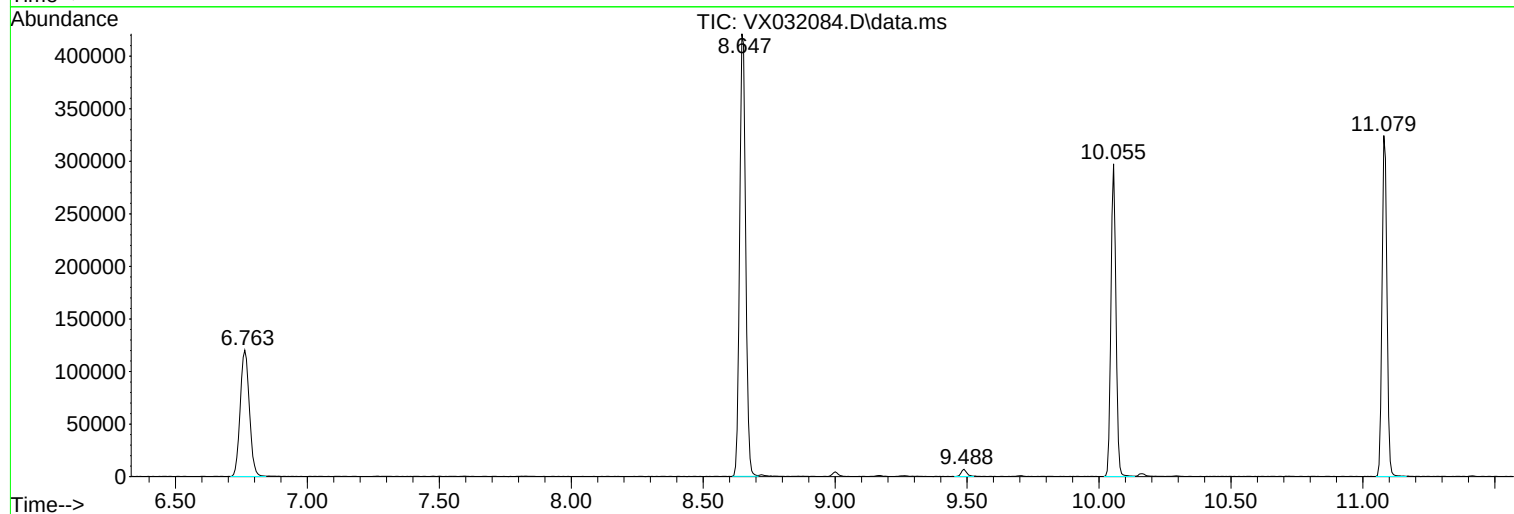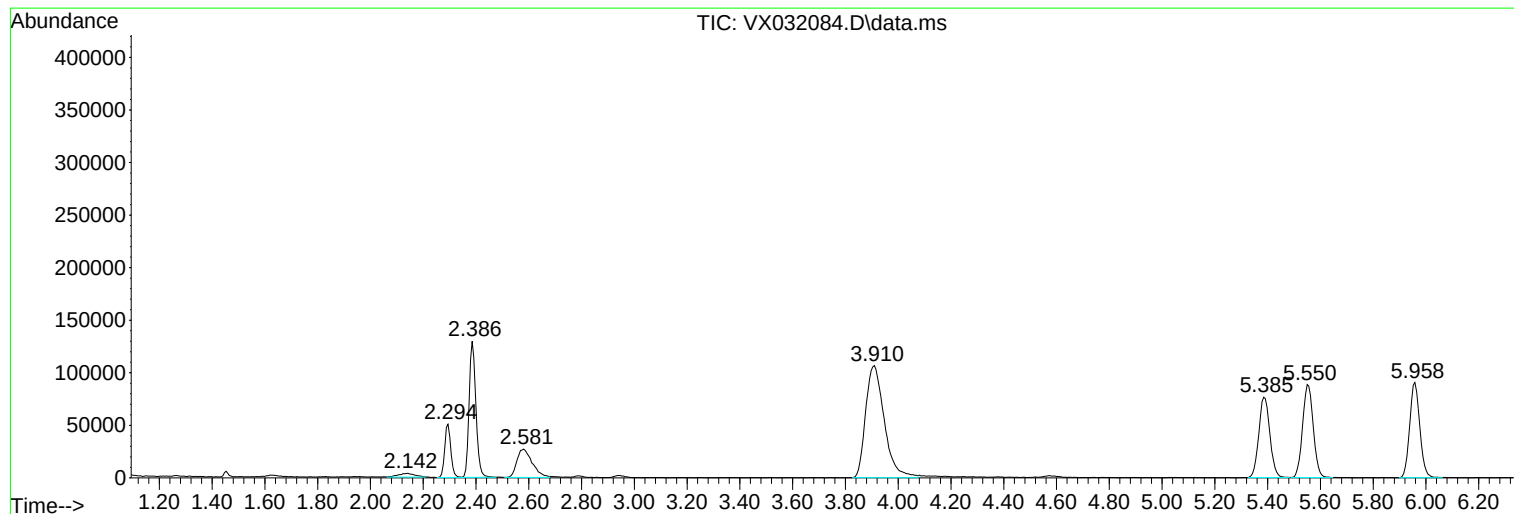

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101222\
Data File : VX032084.D
Acq On : 12 Oct 2022 15:09
Operator : JC/MD
Sample : N5042-03 500X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EOR-0615

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101222\
Data File : VX032084.D
Acq On : 12 Oct 2022 15:09
Operator : JC/MD
Sample : N5042-03 500X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EOR-0615

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc