

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101222\
 Data File : VX032088.D
 Acq On : 12 Oct 2022 16:42
 Operator : JC/MD
 Sample : N5042-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EOR-0631

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
 Title : SW846 8260

Signal : TIC: VX032088.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.129	154	171	202	rBV	2180489	8330445	100.00%	41.360%
2	5.385	693	705	721	rBV	86488	248029	2.98%	1.231%
3	5.549	721	732	747	rVB	101012	288897	3.47%	1.434%
4	5.958	788	799	809	rBV2	100513	272188	3.27%	1.351%
5	6.763	922	931	945	rVB	134499	321155	3.86%	1.595%
6	8.653	1234	1241	1247	rBV	467051	739851	8.88%	3.673%
7	10.055	1465	1471	1478	rBV	340543	448165	5.38%	2.225%
8	11.079	1634	1639	1651	rVB	395069	535806	6.43%	2.660%
9	12.024	1788	1794	1800	rBV	496361	643135	7.72%	3.193%
10	12.091	1800	1805	1811	rVB2	90007	156439	1.88%	0.777%
11	12.317	1838	1842	1849	rVB4	102838	156418	1.88%	0.777%
12	12.426	1849	1860	1863	rBV	163099	227936	2.74%	1.132%
13	12.463	1863	1866	1873	rVB	68534	90869	1.09%	0.451%
14	12.615	1887	1891	1894	rVB	94761	100576	1.21%	0.499%
15	12.701	1899	1905	1908	rBV	75082	135529	1.63%	0.673%
16	12.920	1938	1941	1944	rVV	91069	111756	1.34%	0.555%
17	12.963	1944	1948	1954	rVB	149853	220638	2.65%	1.095%
18	13.042	1954	1961	1964	rBV4	58324	104982	1.26%	0.521%
19	13.170	1974	1982	1986	rBV2	131270	209542	2.52%	1.040%
20	13.292	1992	2002	2007	rBV3	516777	927439	11.13%	4.605%
21	13.420	2019	2023	2032	rVB	381138	526406	6.32%	2.614%
22	13.505	2032	2037	2040	rBV3	58828	89512	1.07%	0.444%
23	13.542	2040	2043	2046	rBV	88731	108013	1.30%	0.536%
24	13.585	2046	2050	2055	rVV3	128130	204708	2.46%	1.016%
25	13.664	2060	2063	2068	rVB2	132619	181622	2.18%	0.902%
26	13.853	2088	2094	2099	rVB	199115	289644	3.48%	1.438%
27	13.926	2099	2106	2111	rBV2	242270	349387	4.19%	1.735%
28	14.036	2121	2124	2127	rVB2	85679	88589	1.06%	0.440%
29	14.078	2127	2131	2135	rBV	162685	196388	2.36%	0.975%
30	14.231	2149	2156	2163	rBV	529808	867436	10.41%	4.307%
31	14.322	2167	2171	2175	rBV	72924	92624	1.11%	0.460%
32	14.371	2175	2179	2183	rVB	184206	216071	2.59%	1.073%
33	14.481	2192	2197	2203	rBV2	461901	611683	7.34%	3.037%
34	14.615	2215	2219	2222	rBV	202790	301598	3.62%	1.497%
35	14.670	2226	2228	2233	rVB	126145	161605	1.94%	0.802%
36	14.822	2249	2253	2255	rVV	78948	116368	1.40%	0.578%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101222\
Data File : VX032088.D
Acq On : 12 Oct 2022 16:42
Operator : JC/MD
Sample : N5042-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EOR-0631

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M

Title : SW846 8260

37	14.847	2255	2257	2262	rVV3	75650	85338	1.02%	0.424%
38	14.901	2262	2266	2273	rVB2	78596	137104	1.65%	0.681%
39	15.182	2307	2312	2320	rBV2	190790	387904	4.66%	1.926%
40	15.377	2339	2344	2348	rBV3	58949	99221	1.19%	0.493%
41	15.481	2356	2361	2366	rBV2	125488	226348	2.72%	1.124%
42	15.615	2378	2383	2386	rVV2	129168	216625	2.60%	1.076%
43	15.651	2386	2389	2397	rVB	76576	128225	1.54%	0.637%
44	16.090	2456	2461	2469	rBV2	41536	90030	1.08%	0.447%
45	16.377	2502	2508	2513	rVB2	55310	98975	1.19%	0.491%




Sum of corrected areas: 20141219

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101222\
Data File : VX032088.D
Acq On : 12 Oct 2022 16:42
Operator : JC/MD
Sample : N5042-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EOR-0631

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

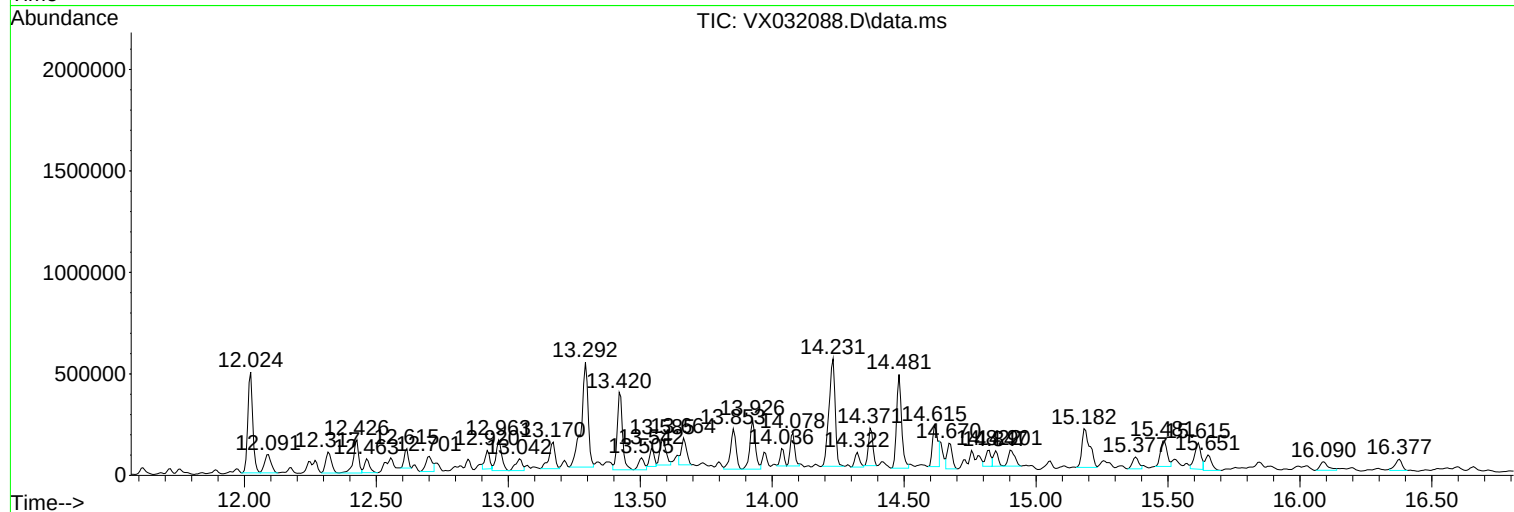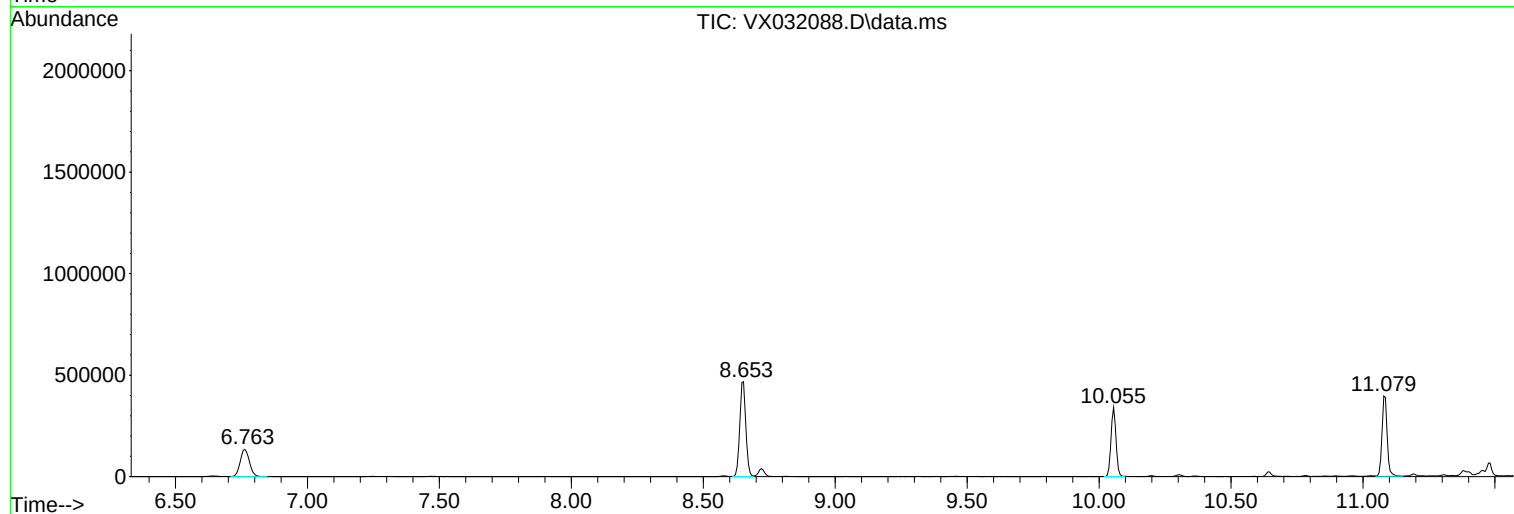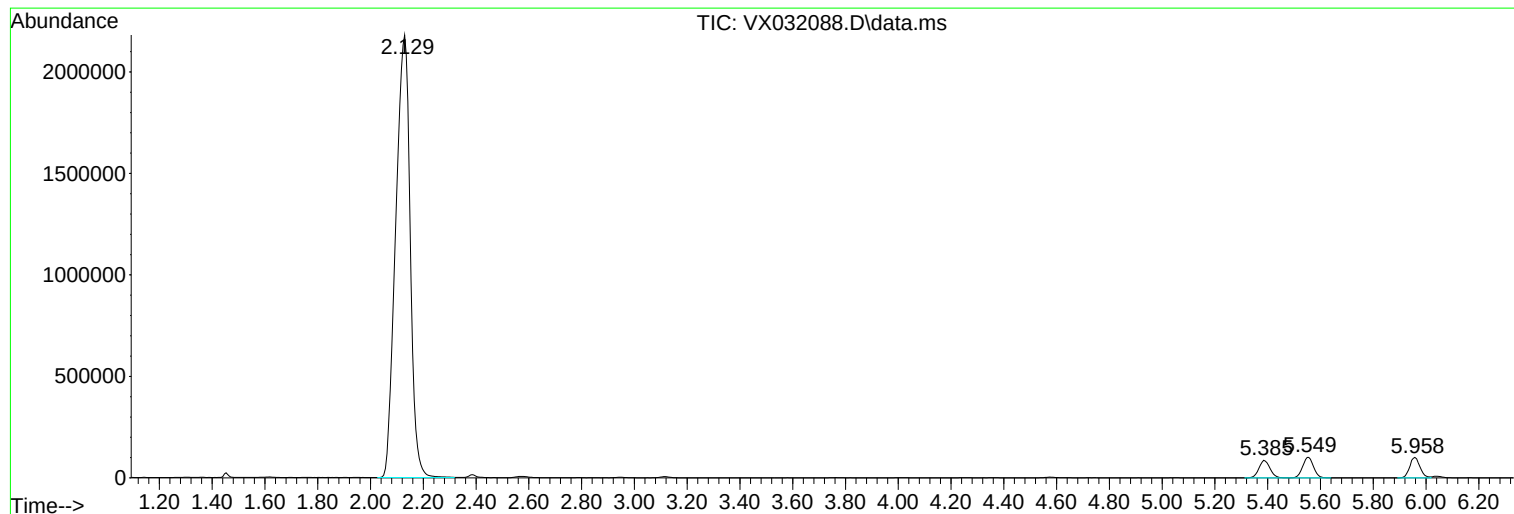

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101222\
Data File : VX032088.D
Acq On : 12 Oct 2022 16:42
Operator : JC/MD
Sample : N5042-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EOR-0631

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101222\
Data File : VX032088.D
Acq On : 12 Oct 2022 16:42
Operator : JC/MD
Sample : N5042-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EOR-0631

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc