

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101222\
 Data File : VX032089.D
 Acq On : 12 Oct 2022 17:05
 Operator : JC/MD
 Sample : N5042-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EOR-0617

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
 Title : SW846 8260

Signal : TIC: VX032089.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.130	167	171	187	rVB8	3515	12707	1.71%	0.297%
2	2.386	207	213	227	rBV	17689	31792	4.27%	0.742%
3	3.111	325	332	341	rBV	6866	15337	2.06%	0.358%
4	5.385	692	705	722	rBV	86907	252174	33.84%	5.885%
5	5.556	722	733	748	rVV	103694	289454	38.84%	6.755%
6	5.958	787	799	812	rBV	103228	271014	36.36%	6.325%
7	6.763	920	931	944	rBV	139599	327162	43.90%	7.636%
8	8.647	1234	1240	1248	rBV	479672	745270	100.00%	17.394%
9	8.720	1248	1252	1260	rVB	9237	14381	1.93%	0.336%
10	10.055	1465	1471	1478	rBV	336329	450266	60.42%	10.509%
11	10.305	1504	1512	1518	rBV7	3147	7643	1.03%	0.178%
12	11.079	1634	1639	1650	rBV	431214	550536	73.87%	12.849%
13	11.476	1701	1704	1710	rVB	10356	13893	1.86%	0.324%
14	11.713	1740	1743	1747	rBV2	5962	7785	1.04%	0.182%
15	12.024	1788	1794	1800	rBV	488144	616629	82.74%	14.391%
16	12.104	1804	1807	1810	rVB3	7362	8319	1.12%	0.194%
17	12.171	1816	1818	1823	rVB3	8764	9861	1.32%	0.230%
18	12.427	1855	1860	1864	rBV	43030	54834	7.36%	1.280%
19	12.469	1864	1867	1873	rVB7	5650	9945	1.33%	0.232%
20	12.585	1883	1886	1890	rVB4	6354	7742	1.04%	0.181%
21	12.683	1899	1902	1907	rVB6	6972	9021	1.21%	0.211%
22	12.896	1931	1937	1942	rBV5	9580	23991	3.22%	0.560%
23	12.945	1942	1945	1947	rVV3	6890	8018	1.08%	0.187%
24	12.975	1947	1950	1955	rVB3	12144	14622	1.96%	0.341%
25	13.042	1957	1961	1964	rBV	11090	12229	1.64%	0.285%
26	13.268	1986	1998	2001	rBV	64507	107090	14.37%	2.499%
27	13.384	2014	2017	2020	rBV	10850	11875	1.59%	0.277%
28	13.420	2020	2023	2027	rBV5	6229	10321	1.38%	0.241%
29	13.682	2061	2066	2067	rBV5	6387	9747	1.31%	0.227%
30	13.737	2072	2075	2078	rVV2	8953	11316	1.52%	0.264%
31	13.841	2088	2092	2098	rVB6	12111	23567	3.16%	0.550%
32	13.920	2100	2105	2111	rVB9	7519	17005	2.28%	0.397%
33	14.036	2120	2124	2128	rBV	37851	43495	5.84%	1.015%
34	14.073	2128	2130	2133	rBV4	5655	8018	1.08%	0.187%
35	14.225	2151	2155	2160	rVB4	12683	23030	3.09%	0.537%
36	14.481	2193	2197	2198	rBV4	9585	14449	1.94%	0.337%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101222\
Data File : VX032089.D
Acq On : 12 Oct 2022 17:05
Operator : JC/MD
Sample : N5042-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EOR-0617

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Title : SW846 8260

37	14.615	2216	2219	2226	rBV8	18659	38160	5.12%	0.891%
38	14.755	2238	2242	2246	rBV	34188	34799	4.67%	0.812%
39	15.182	2308	2312	2314	rBV3	14419	19506	2.62%	0.455%
40	15.213	2314	2317	2320	rVB3	13538	16459	2.21%	0.384%
41	15.377	2340	2344	2351	rVB9	9644	18577	2.49%	0.434%
42	15.487	2358	2362	2367	rBV2	30137	44231	5.93%	1.032%
43	15.615	2381	2383	2386	rVB4	9754	9466	1.27%	0.221%
44	15.847	2417	2421	2424	rBV6	5531	8719	1.17%	0.203%
45	16.085	2456	2460	2463	rBV4	6350	11491	1.54%	0.268%
46	16.377	2502	2508	2515	rVB	21929	38781	5.20%	0.905%




Sum of corrected areas: 4284727

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101222\
Data File : VX032089.D
Acq On : 12 Oct 2022 17:05
Operator : JC/MD
Sample : N5042-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EOR-0617

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

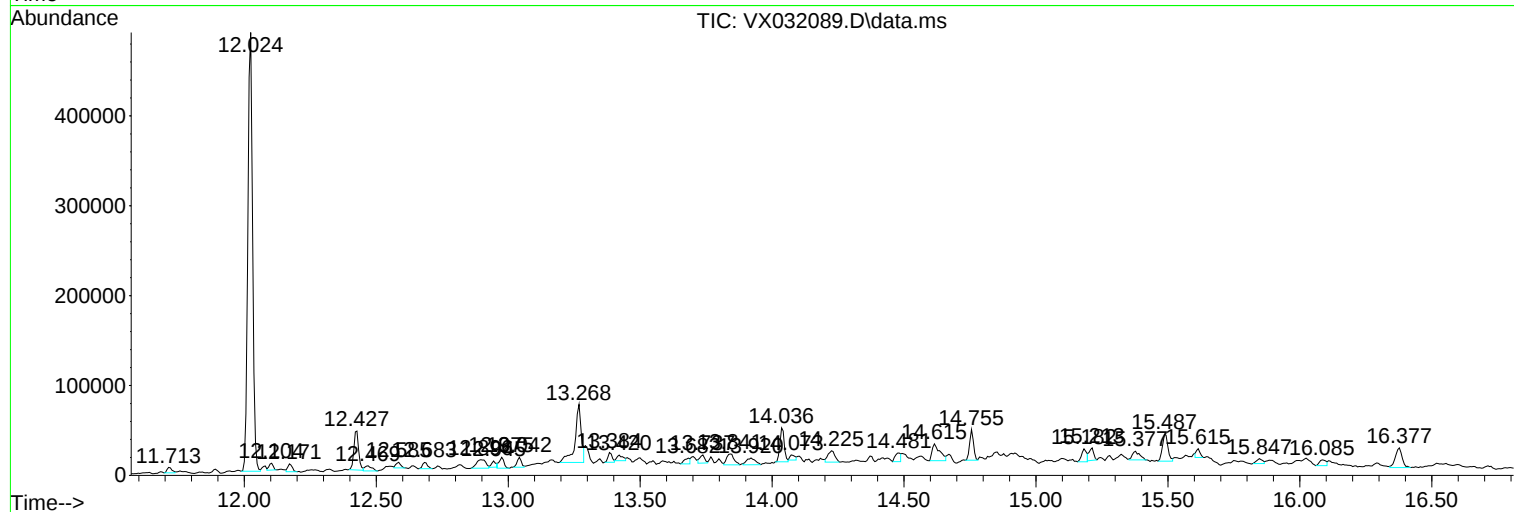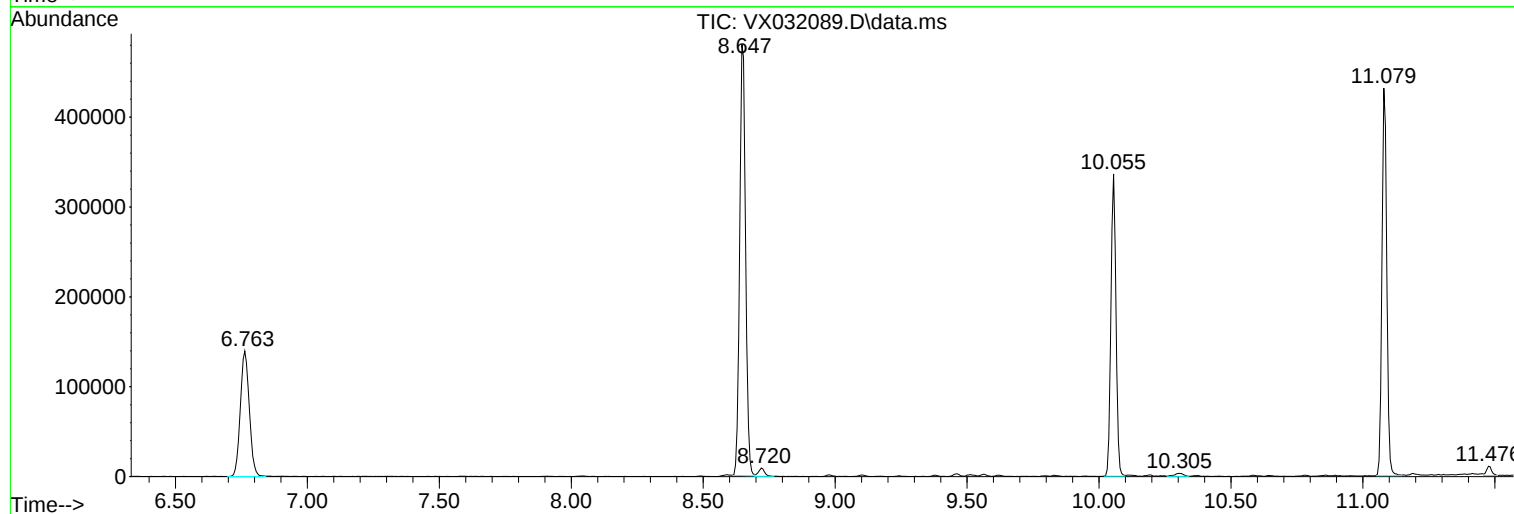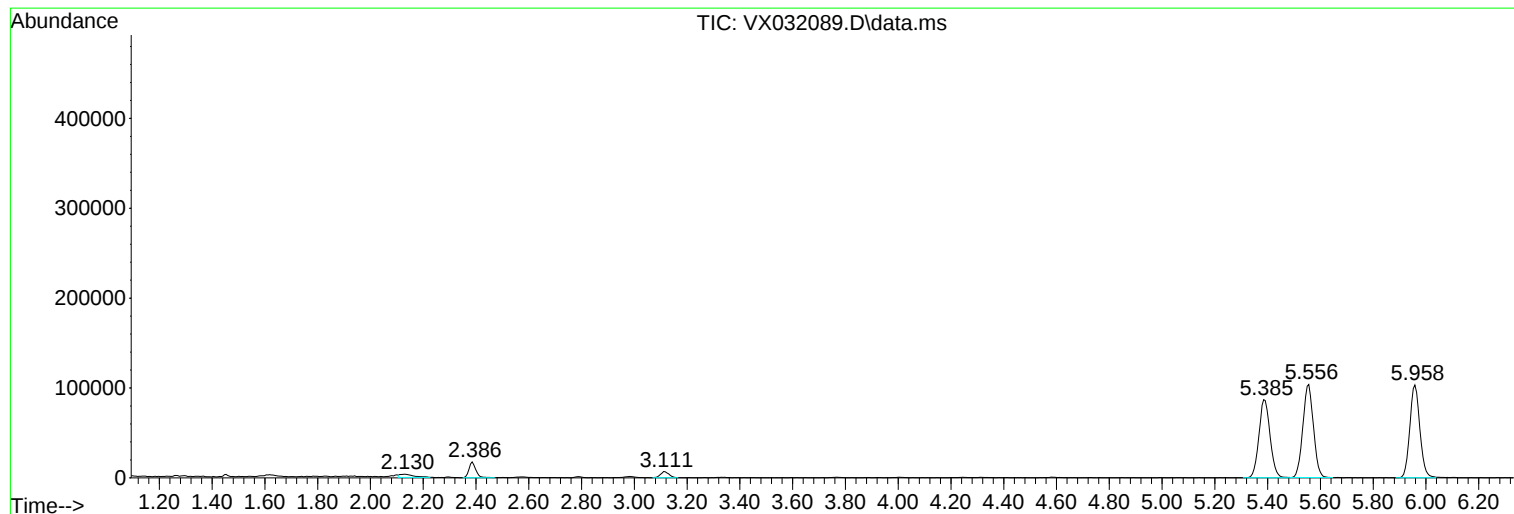

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101222\
Data File : VX032089.D
Acq On : 12 Oct 2022 17:05
Operator : JC/MD
Sample : N5042-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EOR-0617










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Dodecane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.268	8.68 ug/l	107090	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dodecane	170	C12H26	000112-40-3	96
2			Hexadecane	226	C16H34	000544-76-3	87
3			Undecane	156	C11H24	001120-21-4	86
4			Heptadecane, 2,6,10,14-tetramethyl-	296	C21H44	018344-37-1	86
5			Tetradecane	198	C14H30	000629-59-4	80

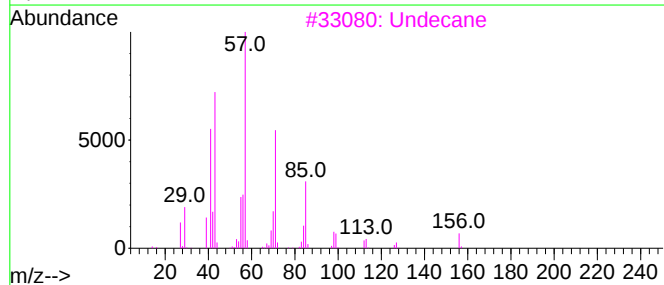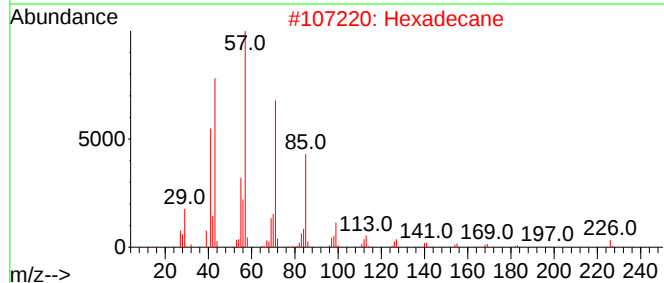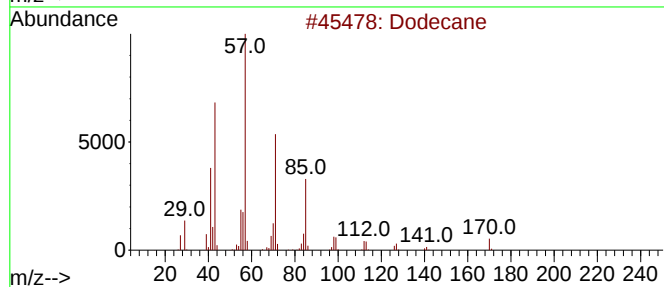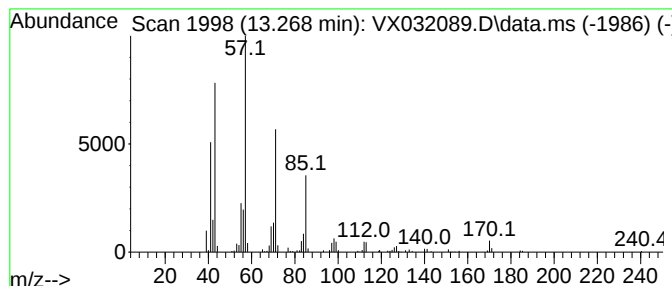

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101222\
Data File : VX032089.D
Acq On : 12 Oct 2022 17:05
Operator : JC/MD
Sample : N5042-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EOR-0617

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Decane	13.268	8.7	ug/l	107090	4	12.024	616629	50.0