

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101222\
 Data File : VX032090.D
 Acq On : 12 Oct 2022 17:28
 Operator : JC/MD
 Sample : N5042-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EOR-0126

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
 Title : SW846 8260

Signal : TIC: VX032090.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.117	324	333	340	rVB2	4909	10536	1.44%	0.292%
2	5.385	690	705	718	rBV	84441	244242	33.35%	6.761%
3	5.556	721	733	747	rVB	99048	279356	38.14%	7.733%
4	5.952	788	798	815	rBV	98844	264307	36.09%	7.317%
5	6.763	922	931	945	rBV	134025	316961	43.28%	8.774%
6	8.647	1234	1240	1250	rBV	468437	732422	100.00%	20.276%
7	10.055	1465	1471	1485	rBV	333212	443022	60.49%	12.264%
8	11.079	1634	1639	1648	rBV	414335	527814	72.06%	14.611%
9	12.024	1788	1794	1800	rBV	467814	583528	79.67%	16.154%
10	12.427	1855	1860	1864	rBV	11254	14460	1.97%	0.400%
11	12.908	1929	1939	1942	rBV6	3836	8429	1.15%	0.233%
12	13.268	1985	1998	2008	rBV	27037	63159	8.62%	1.748%
13	13.701	2060	2069	2071	rBV8	4321	10546	1.44%	0.292%
14	13.841	2088	2092	2099	rVB6	6348	10858	1.48%	0.301%
15	14.042	2120	2125	2128	rBV	19001	23967	3.27%	0.663%
16	14.231	2153	2156	2160	rVB6	5839	8431	1.15%	0.233%
17	14.615	2216	2219	2222	rBV5	6975	10700	1.46%	0.296%
18	14.755	2238	2242	2246	rBV	17121	19581	2.67%	0.542%
19	15.335	2331	2337	2340	rBV7	5188	12335	1.68%	0.341%
20	15.493	2358	2363	2367	rBV3	10793	15811	2.16%	0.438%
21	16.377	2503	2508	2512	rVB4	7898	11860	1.62%	0.328%




Sum of corrected areas: 3612325

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101222\
Data File : VX032090.D
Acq On : 12 Oct 2022 17:28
Operator : JC/MD
Sample : N5042-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EOR-0126

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

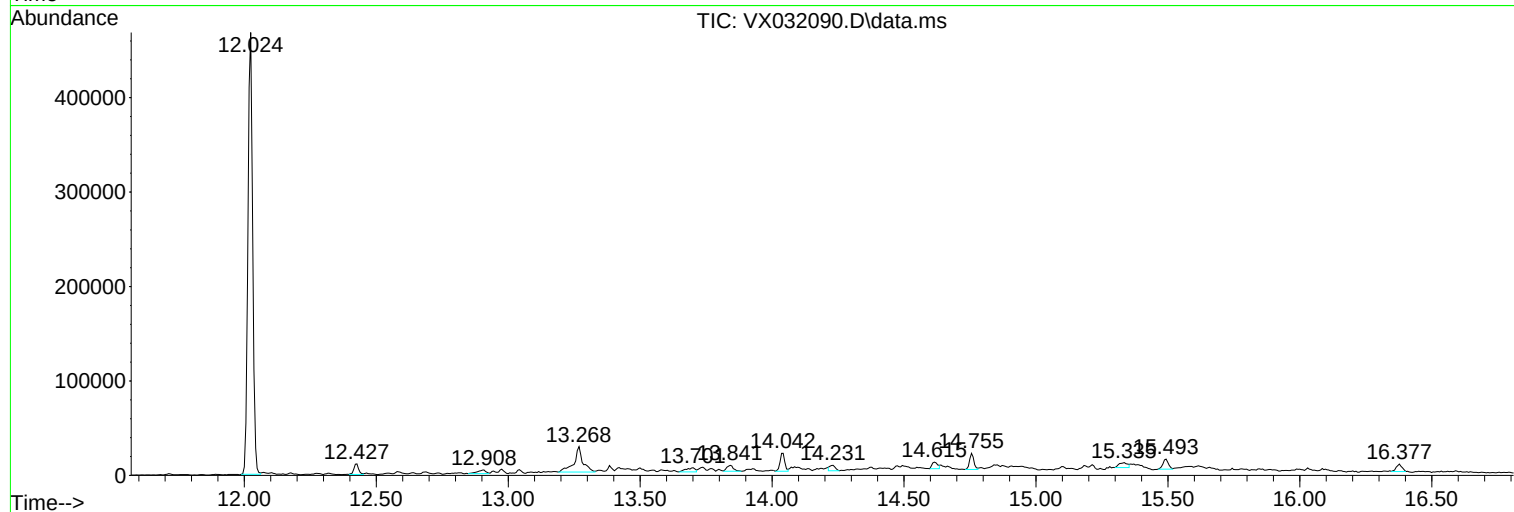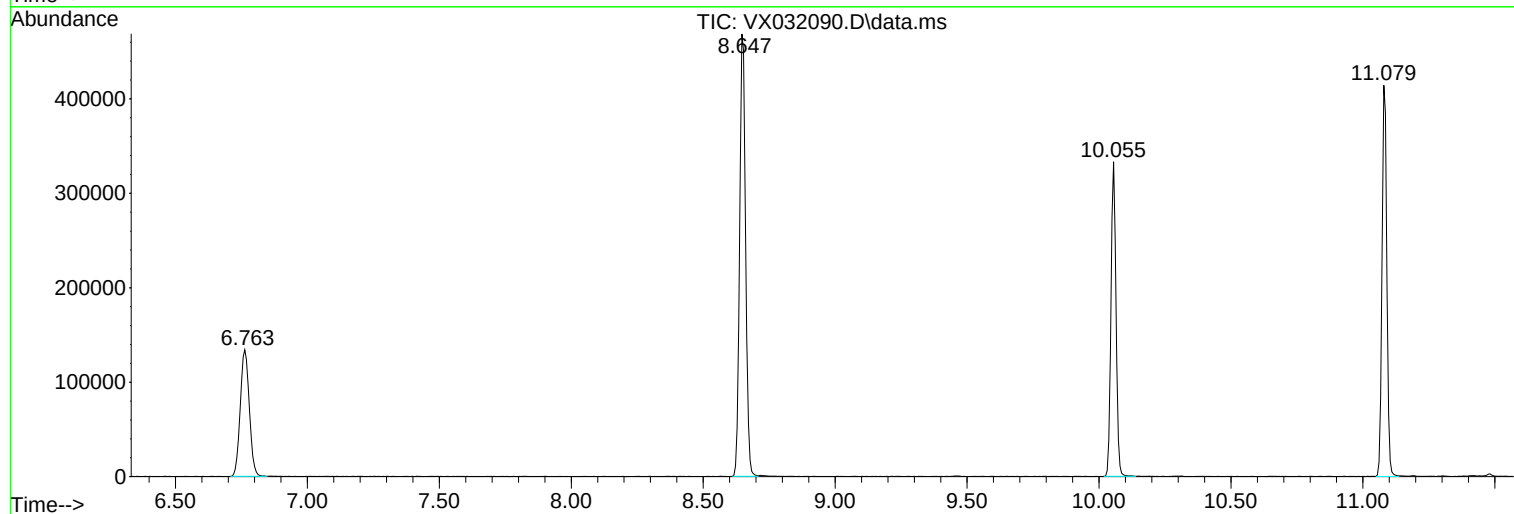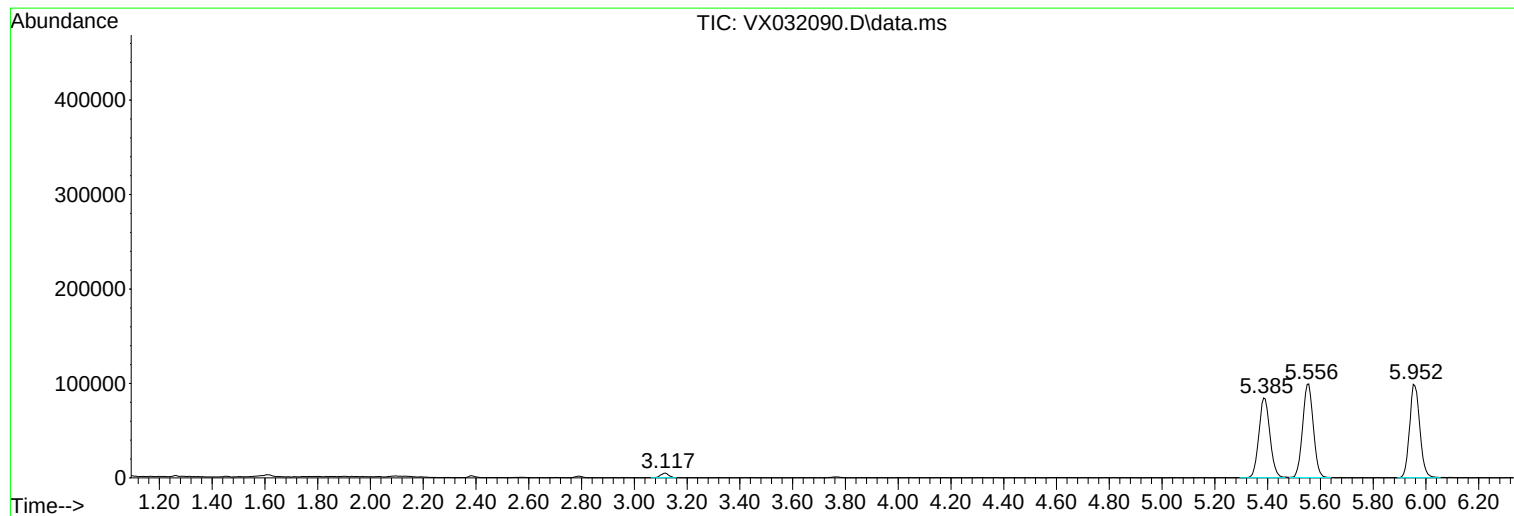

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101222\
Data File : VX032090.D
Acq On : 12 Oct 2022 17:28
Operator : JC/MD
Sample : N5042-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EOR-0126










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Dodecane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.268	5.41 ug/l	63159	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dodecane	170	C12H26	000112-40-3	95
2			Undecane	156	C11H24	001120-21-4	90
3			Tetradecane	198	C14H30	000629-59-4	87
4			Tridecane	184	C13H28	000629-50-5	80
5			Carbonic acid, prop-1-en-2-yl tr...	284	C17H32O3	1000382-90-8	80

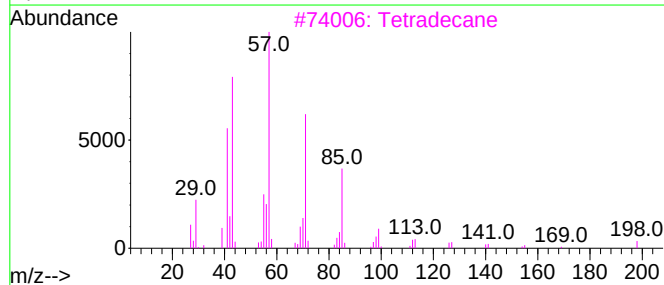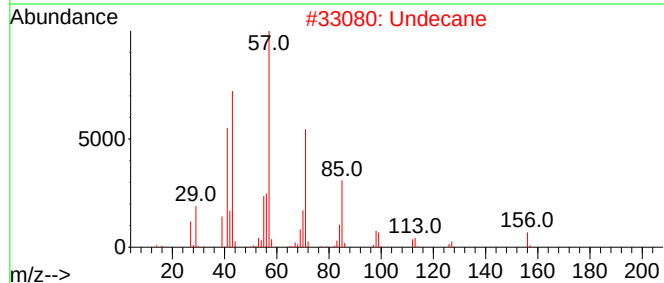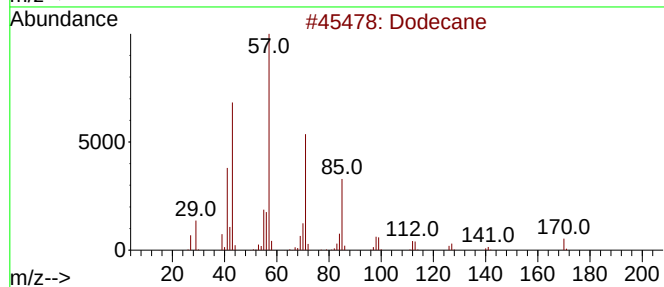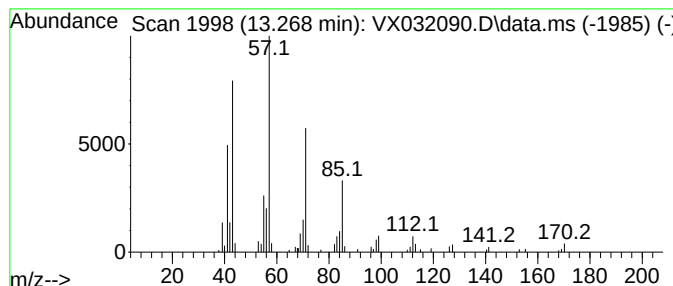

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101222\
Data File : VX032090.D
Acq On : 12 Oct 2022 17:28
Operator : JC/MD
Sample : N5042-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EOR-0126

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Dodecane	13.268	5.4	ug/l	63159	4	12.024	583528	50.0