

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101222\
 Data File : VX032091.D
 Acq On : 12 Oct 2022 17:51
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M

Title : SW846 8260

Signal : TIC: VX032091.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.947	298	305	312	rVB2	3576	8199	1.17%	0.251%
2	5.385	692	705	721	rBV2	79194	232845	33.12%	7.126%
3	5.550	721	732	745	rVV	95726	267659	38.07%	8.191%
4	5.958	789	799	816	rBV2	92302	248352	35.32%	7.601%
5	6.763	922	931	943	rBV	129289	306266	43.56%	9.373%
6	8.647	1232	1240	1251	rBV	441676	703109	100.00%	21.518%
7	10.055	1465	1471	1483	rBV	312976	423455	60.23%	12.959%
8	11.079	1634	1639	1654	rBV	369827	472671	67.23%	14.466%
9	12.024	1788	1794	1805	rBV	451452	554411	78.85%	16.967%
10	14.036	2116	2124	2129	rBV	7052	9854	1.40%	0.302%
11	14.621	2215	2220	2227	rBV9	3365	8420	1.20%	0.258%
12	14.756	2238	2242	2245	rBV2	7787	8214	1.17%	0.251%
13	15.335	2330	2337	2343	rBV8	5257	15792	2.25%	0.483%
14	15.493	2357	2363	2368	rBV3	5281	8319	1.18%	0.255%




Sum of corrected areas: 3267566

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101222\
Data File : VX032091.D
Acq On : 12 Oct 2022 17:51
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

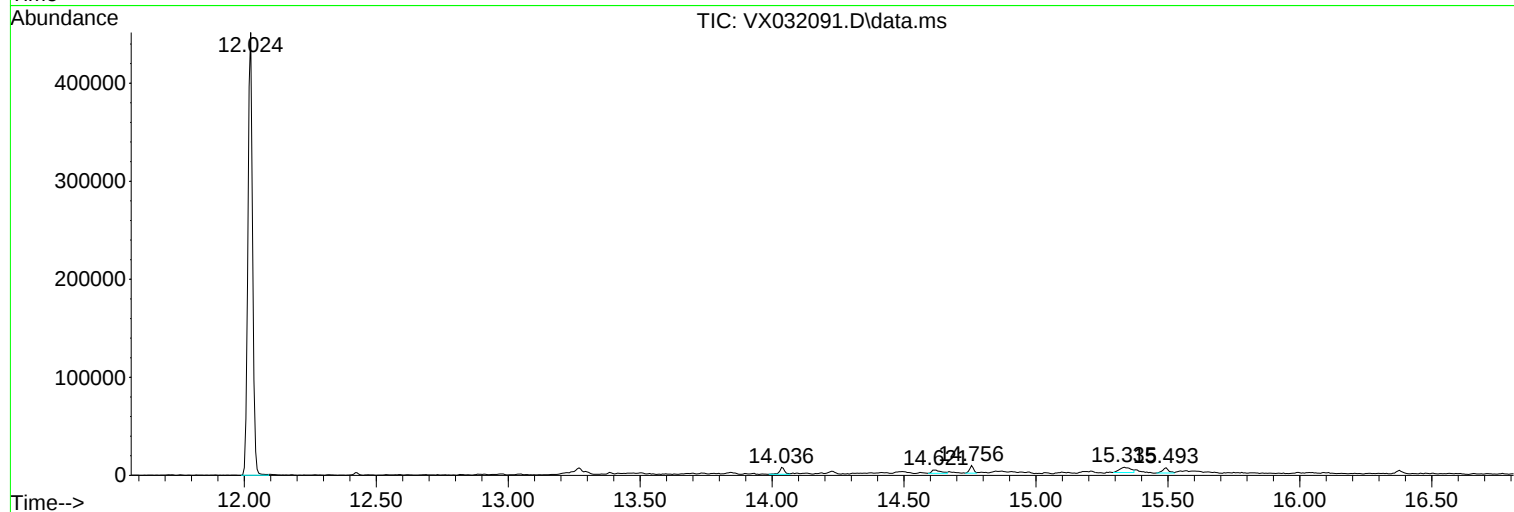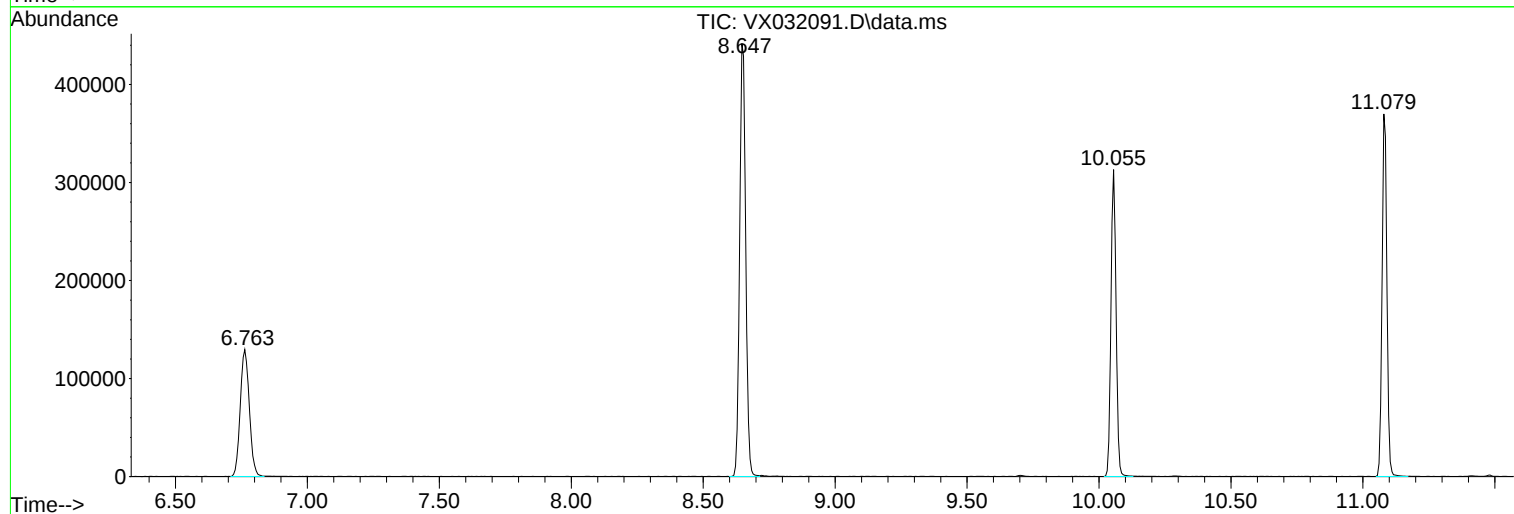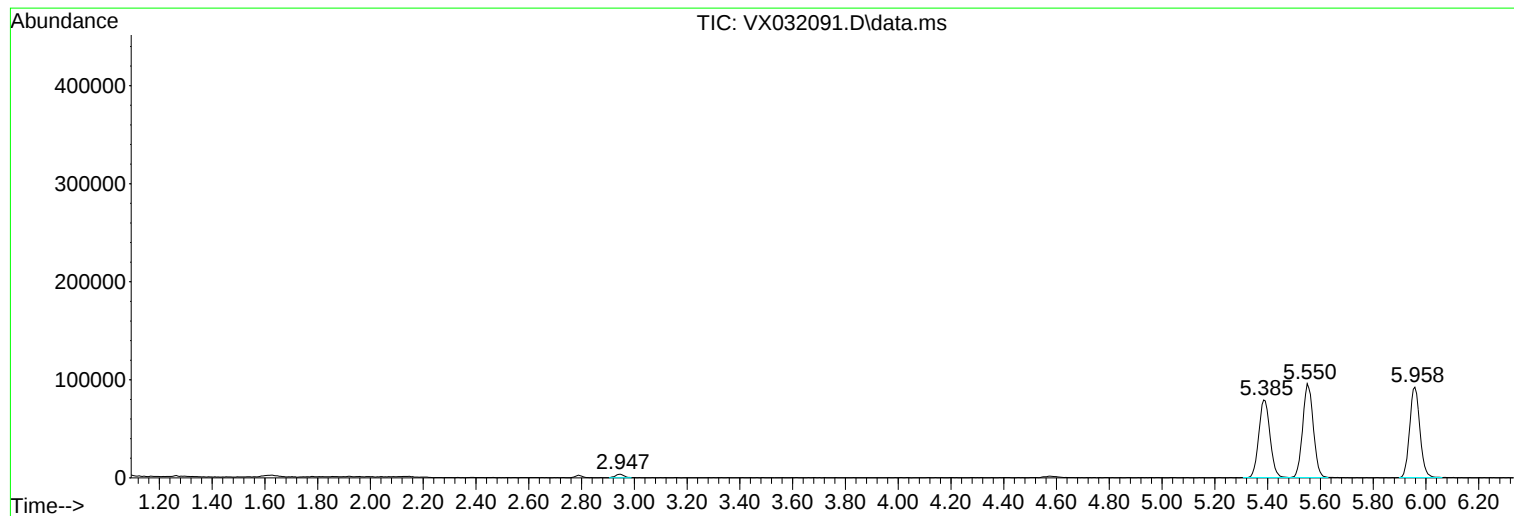

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101222\
Data File : VX032091.D
Acq On : 12 Oct 2022 17:51
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101222\
Data File : VX032091.D
Acq On : 12 Oct 2022 17:51
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------