



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101222\
Data File : VX032072.D
Acq On : 12 Oct 2022 09:39
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Title : SW846 8260
Last Update : Thu Oct 06 14:28:46 2022

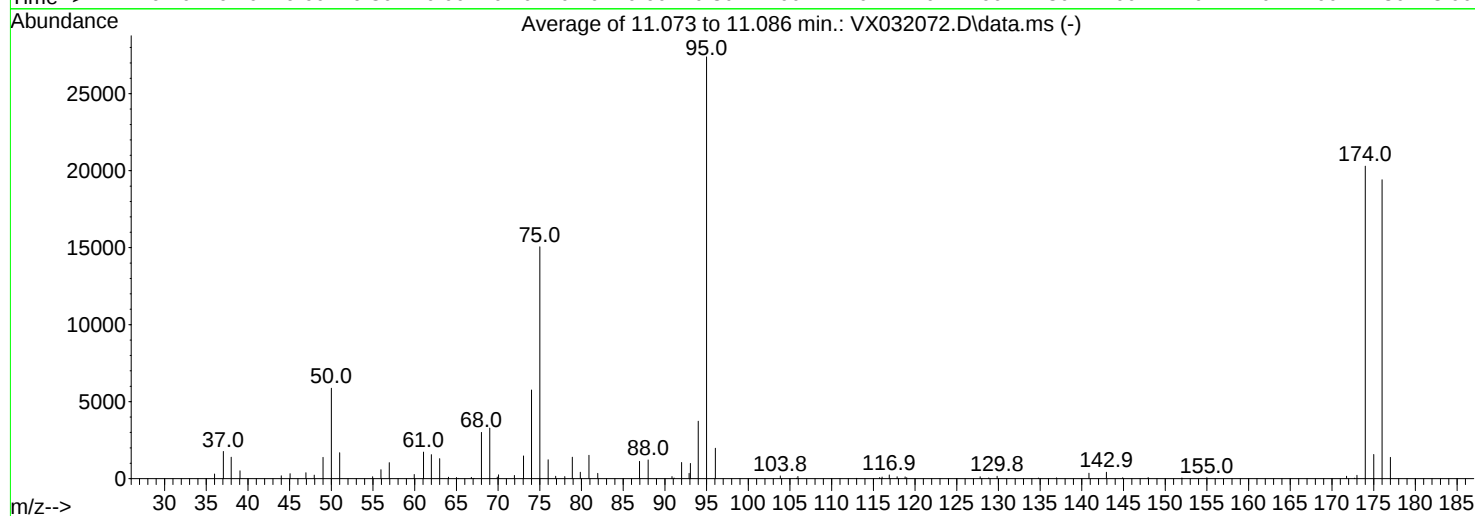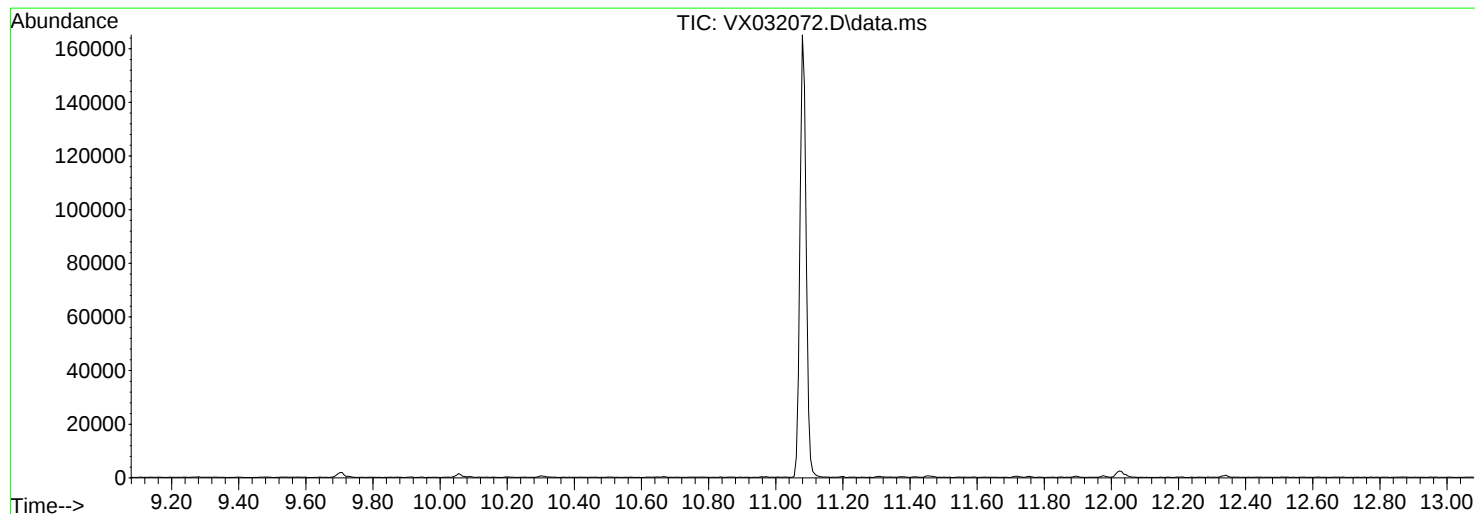

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.4	5866	PASS
75	95	30	60	55.0	15056	PASS
95	95	100	100	100.0	27392	PASS
96	95	5	9	7.2	1974	PASS
173	174	0.00	2	1.1	221	PASS
174	95	50	100	74.1	20296	PASS
175	174	5	9	7.7	1568	PASS
176	174	95	101	95.7	19415	PASS
177	176	5	9	7.1	1379	PASS