

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101223\
 Data File : VX038249.D
 Acq On : 12 Oct 2023 12:15
 Operator : JC/MD
 Sample : 04859-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SVS-GROUNDWATER

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M

Title : SW846 8260

Signal : TIC: VX038249.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.380	207	212	218	rVB	4175	6674	1.03%	0.177%
2	2.532	229	237	243	rBV2	6001	12848	1.99%	0.340%
3	5.385	694	705	720	rBV	74466	221491	34.33%	5.869%
4	5.550	723	732	747	rVV	115147	334324	51.81%	8.859%
5	5.958	787	799	813	rBV2	81185	223145	34.58%	5.913%
6	6.763	921	931	946	rBV	193729	462291	71.64%	12.250%
7	8.647	1234	1240	1250	rBV	399080	645269	100.00%	17.098%
8	10.055	1465	1471	1486	rBV	449870	605107	93.78%	16.034%
9	11.079	1634	1639	1654	rBV	352021	462357	71.65%	12.251%
10	12.024	1788	1794	1803	rBV	480455	619320	95.98%	16.411%
11	12.244	1825	1830	1837	rBV	27095	35768	5.54%	0.948%
12	12.414	1853	1858	1868	rBV	14300	18036	2.80%	0.478%
13	13.774	2077	2081	2090	rBV	58231	74584	11.56%	1.976%
14	14.640	2219	2223	2231	rVB	17819	22290	3.45%	0.591%
15	14.780	2241	2246	2253	rBV	11873	14856	2.30%	0.394%
16	16.328	2494	2500	2506	rBV2	9039	15523	2.41%	0.411%




Sum of corrected areas: 3773883

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101223\
Data File : VX038249.D
Acq On : 12 Oct 2023 12:15
Operator : JC/MD
Sample : 04859-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SVS-GROUNDWATER

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

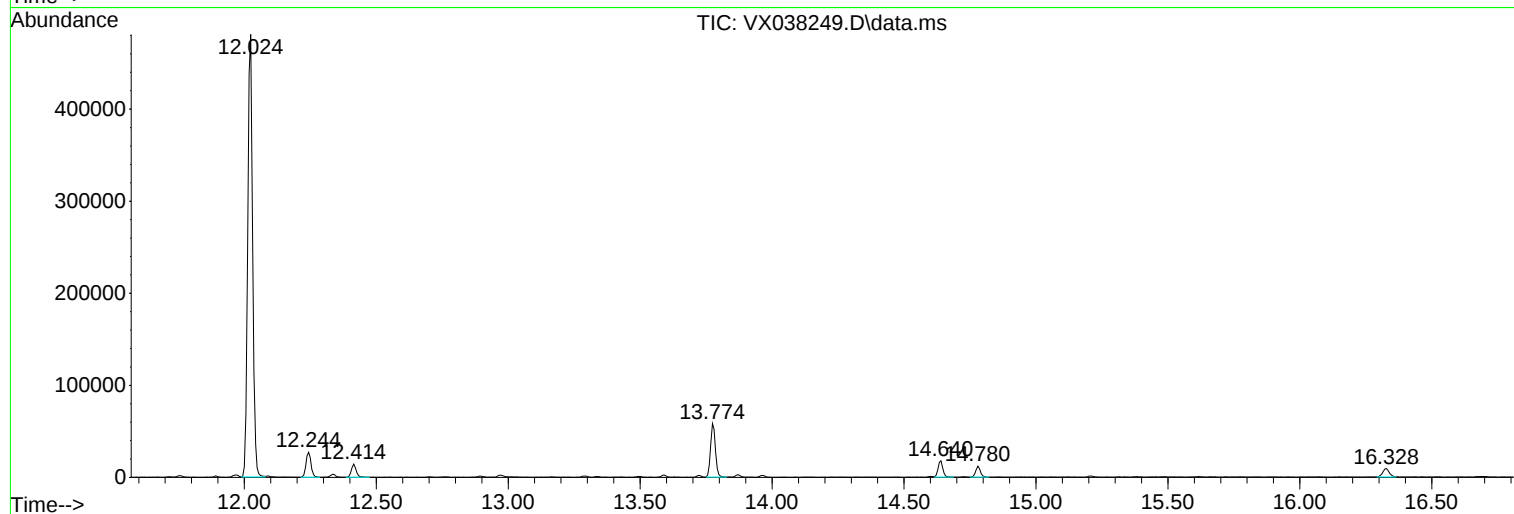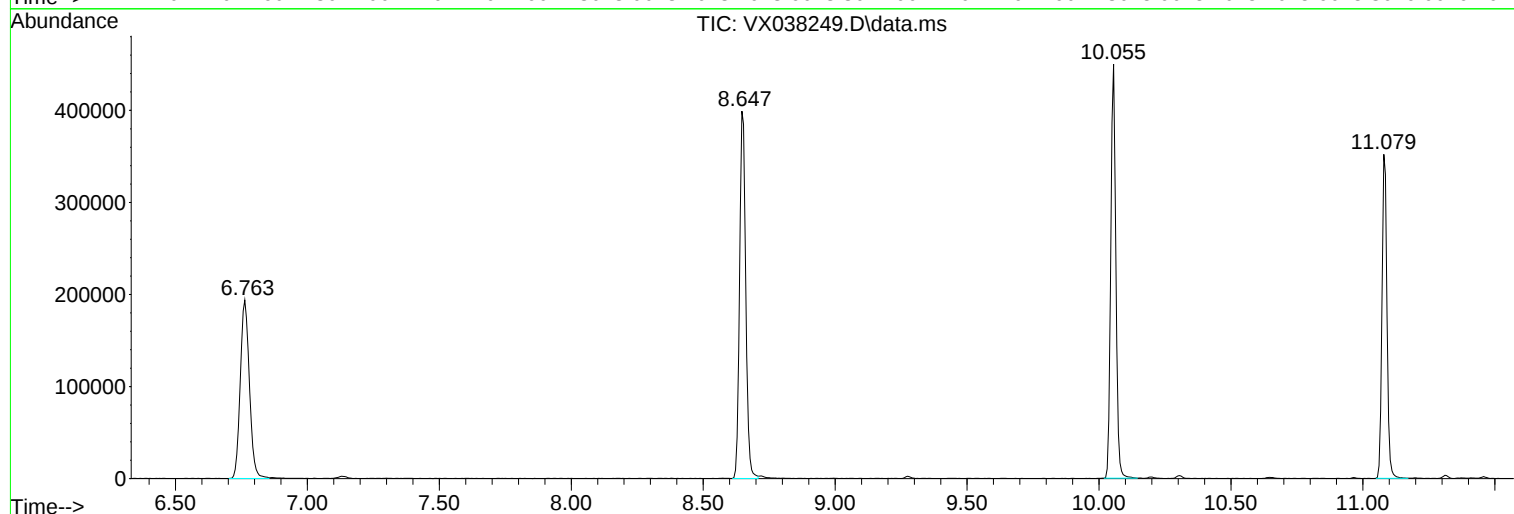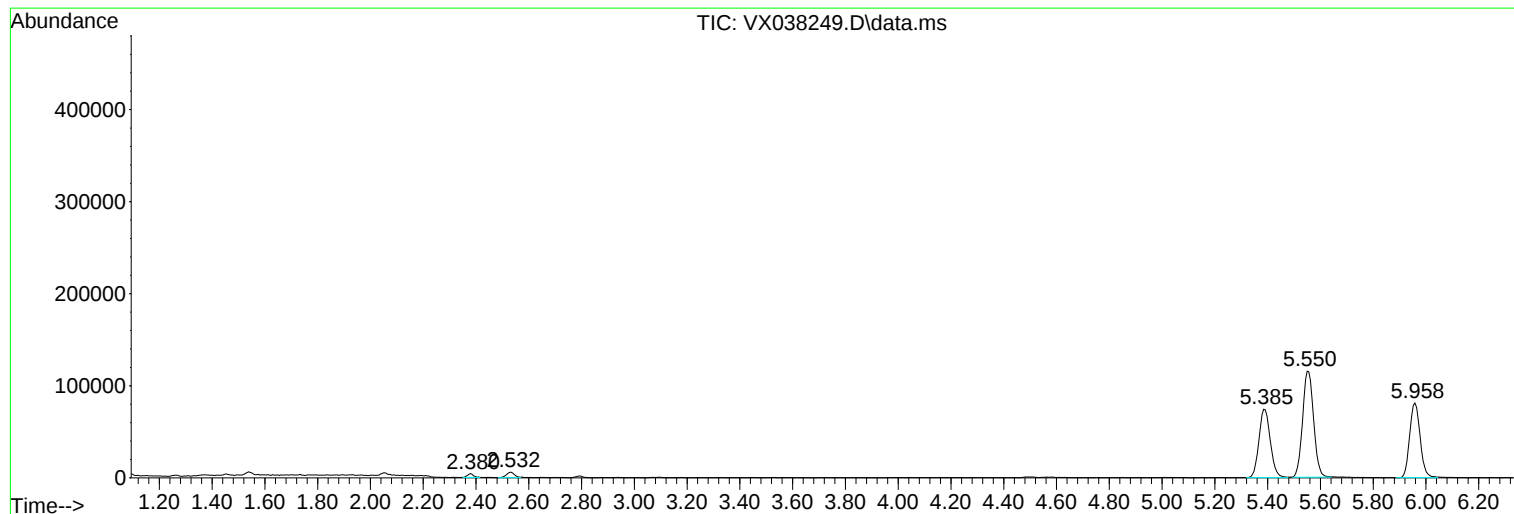

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101223\
Data File : VX038249.D
Acq On : 12 Oct 2023 12:15
Operator : JC/MD
Sample : 04859-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SVS-GROUNDWATER

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101223\
Data File : VX038249.D
Acq On : 12 Oct 2023 12:15
Operator : JC/MD
Sample : 04859-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SVS-GROUNDWATER

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------